

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031420\
 Data File : PS009286.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2020 08:55
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 04:47:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.492	0.000	44957774	0	59.563	N.D.	#
5) T	DICAMBA	0.000	7.168	0	42333749	N.D.	18.441	
6) T	MCP	0.000	7.168	0	42333749	N.D.	23.275	
9) T	2,4-D	8.427	0.000	63895776	0	121.193	N.D.	#
12) T	2,4,5-T	0.000	9.253	0	6757273	N.D.	2.289	
15) T	Picloram	11.037	11.023	14995569	27529915	4.941	6.760	#
16) T	DCPA	0.000	11.023	0	27529915	N.D.	7.108	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031420\
Data File : PS009286.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2020 08:55
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 04:47:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

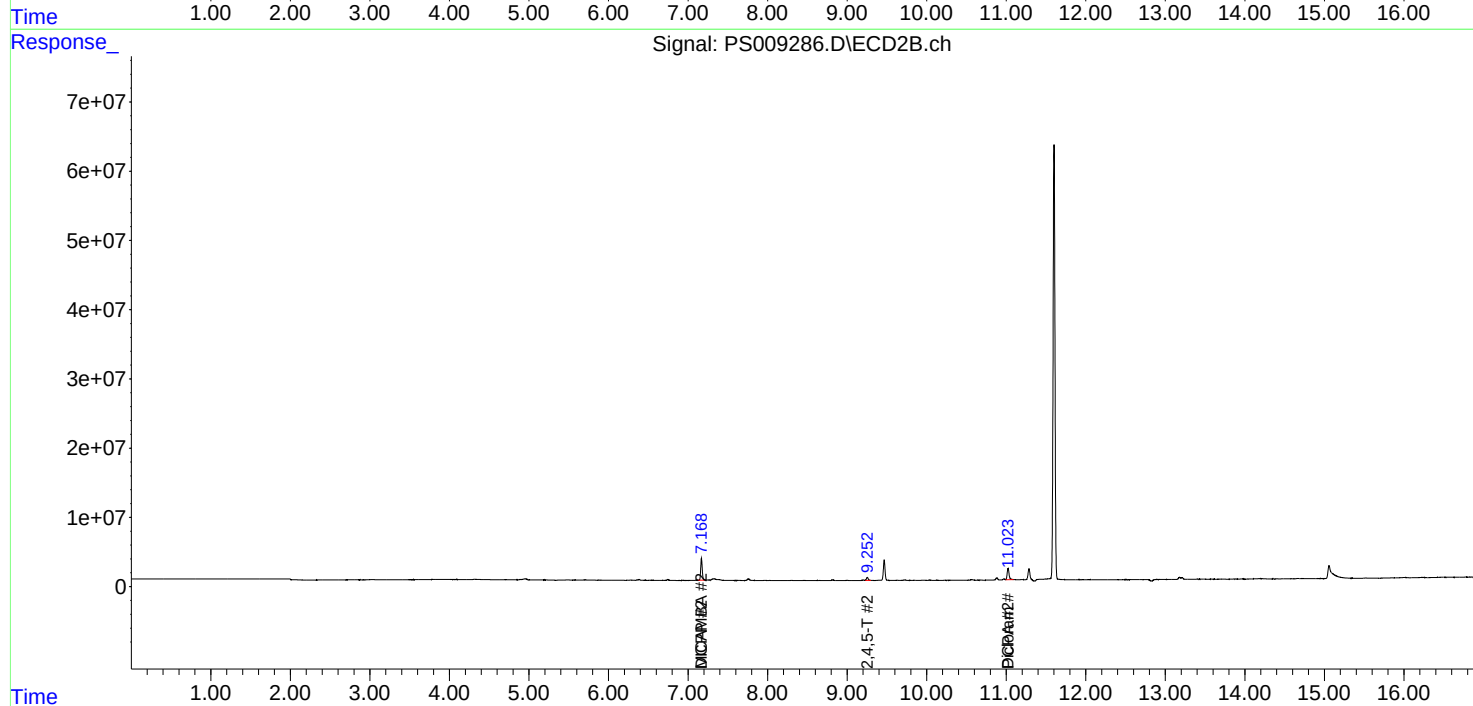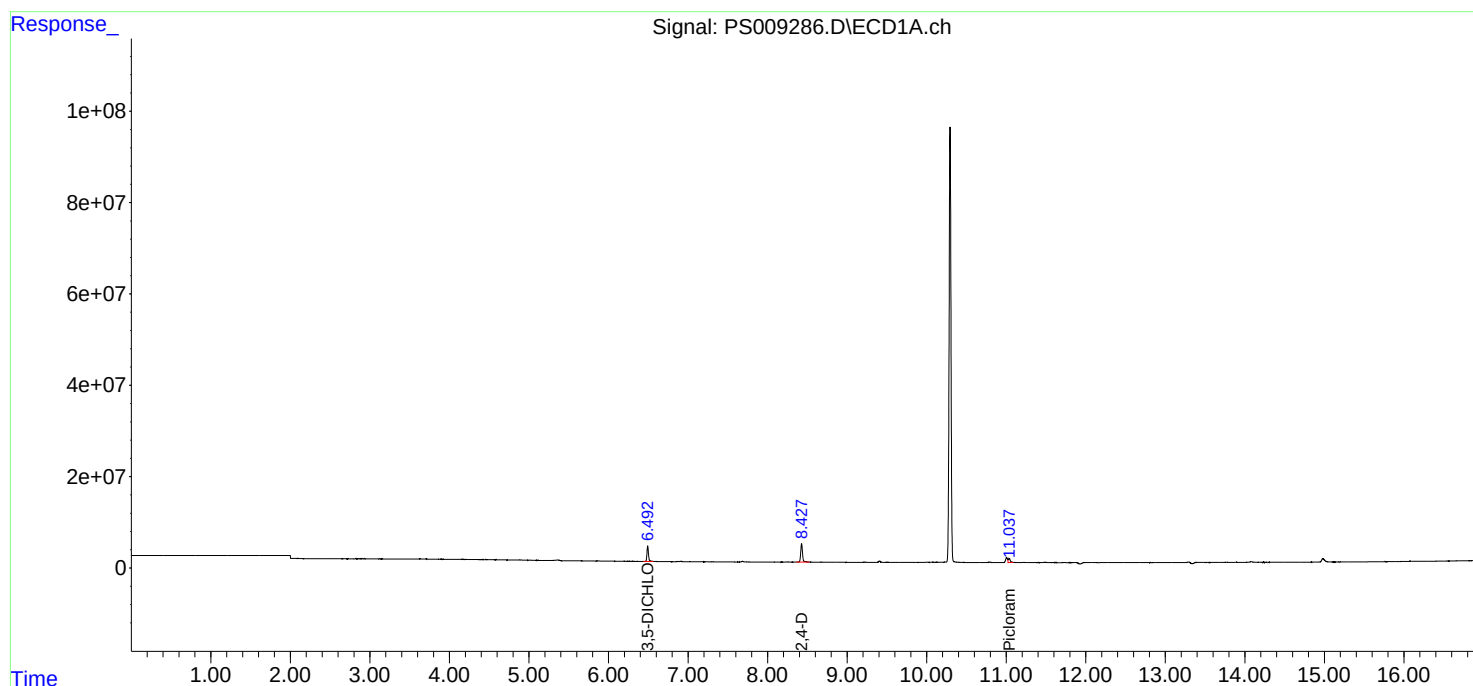


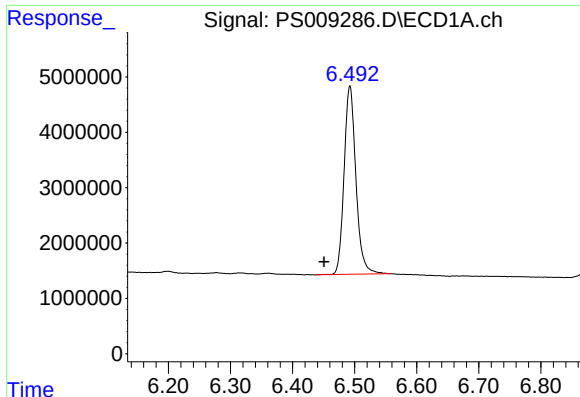

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.492 min
Delta R.T.: 0.042 min
Response: 44957774
Conc: 59.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

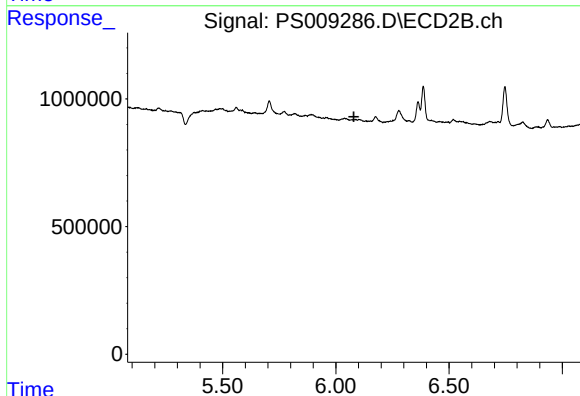


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.080 min
Response: 0
Conc: N.D.

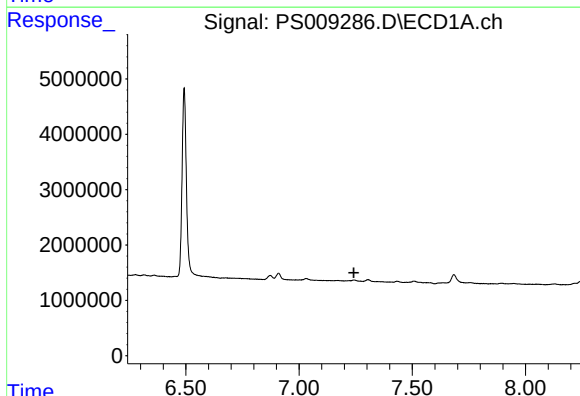


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.242 min
Response: 0
Conc: N.D.

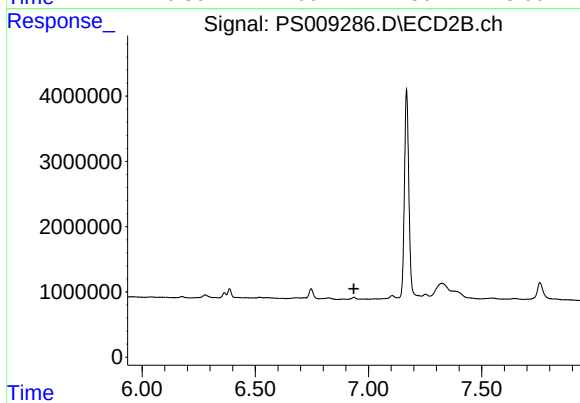

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

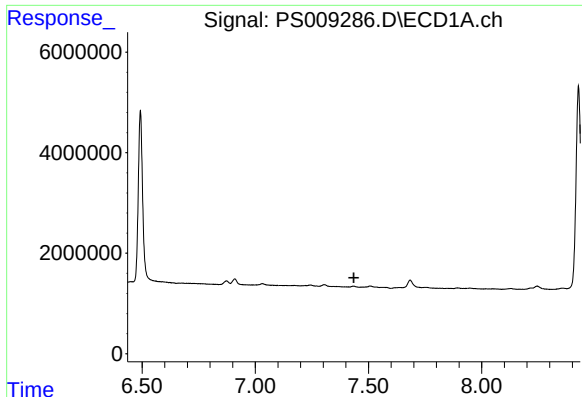

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

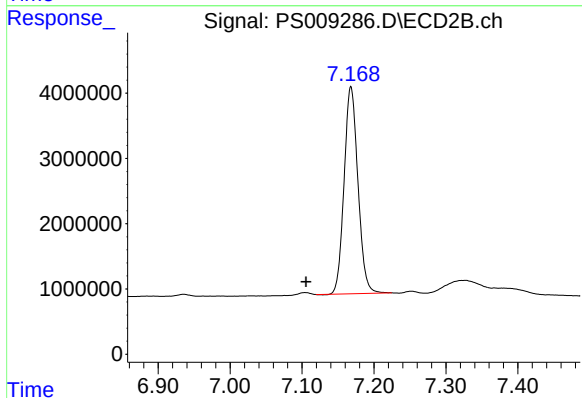


#5 DICAMBA

R.T.: 7.168 min
Delta R.T.: 0.062 min
Response: 42333749
Conc: 18.44 ng/ml

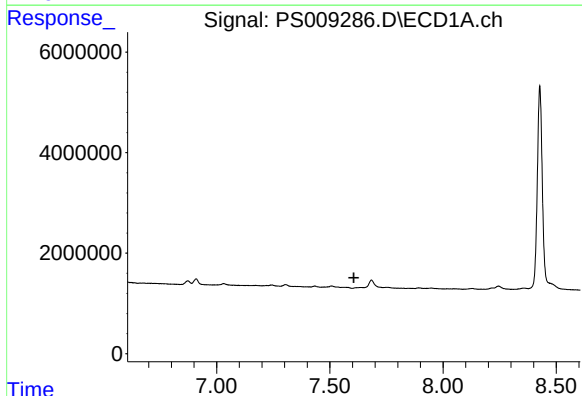


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.606 min
Response: 0
Conc: N.D.

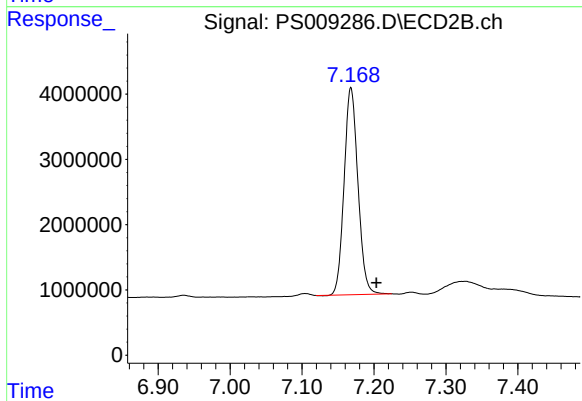

#6 MCP


R.T.: 7.168 min
Delta R.T.: -0.036 min
Response: 42333749
Conc: 23.28 ug/ml

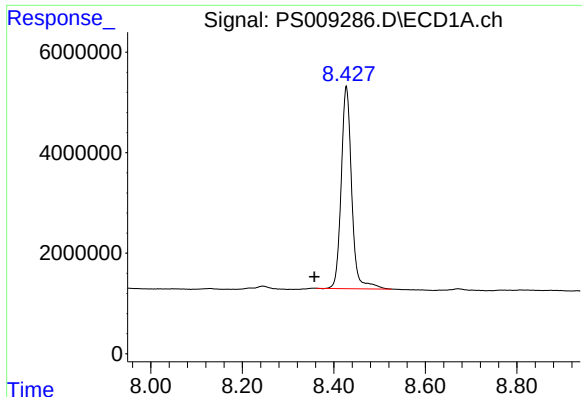

#9 2,4-D


R.T.: 8.427 min
Delta R.T.: 0.069 min
Response: 63895776
Conc: 121.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

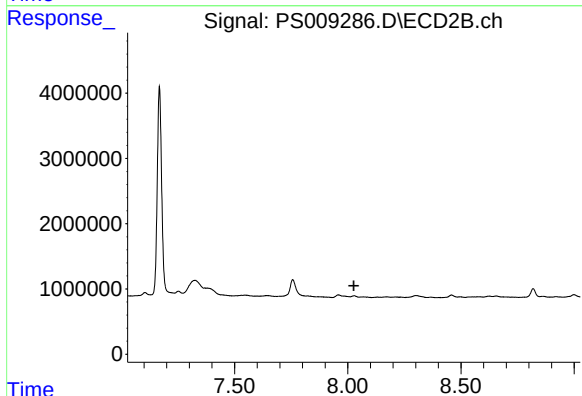


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.027 min
Response: 0
Conc: N.D.

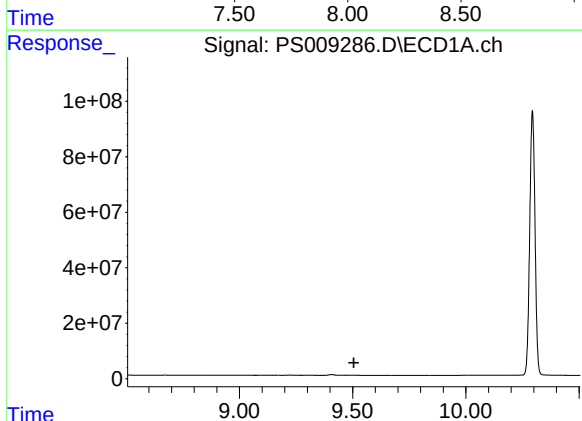


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.505 min
Response: 0
Conc: N.D.

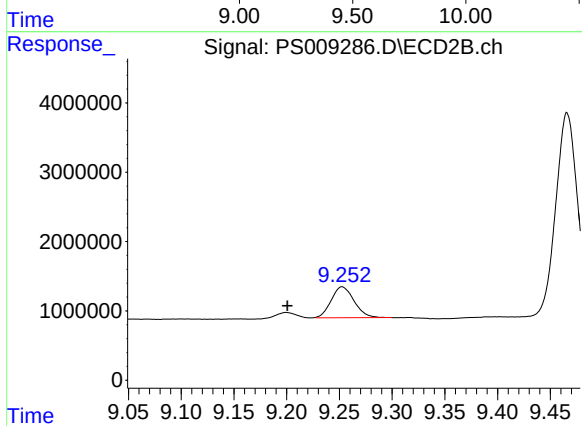

#12 2,4,5-T


R.T.: 9.253 min
Delta R.T.: 0.052 min
Response: 6757273
Conc: 2.29 ng/ml

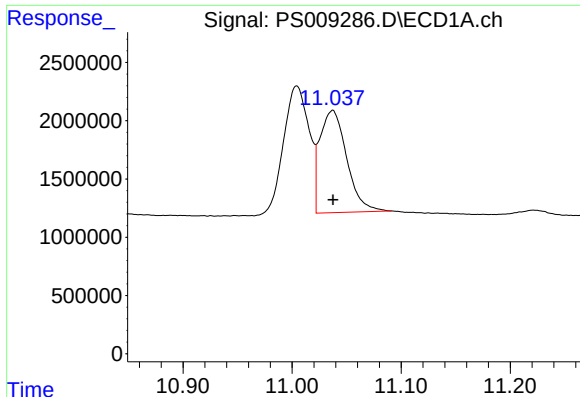

#15 Picloram


R.T.: 11.037 min
Delta R.T.: 0.000 min
Response: 14995569
Conc: 4.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

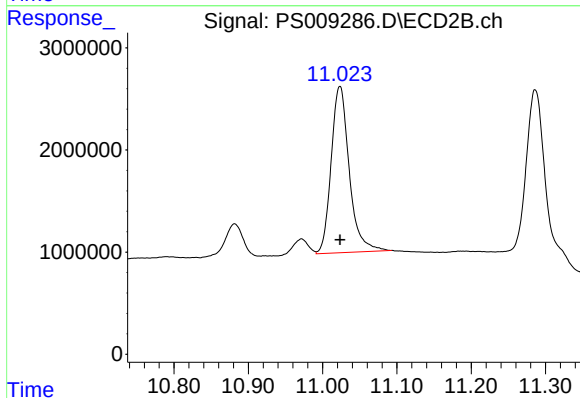


#15 Picloram

R.T.: 11.023 min
Delta R.T.: 0.000 min
Response: 27529915
Conc: 6.76 ng/ml

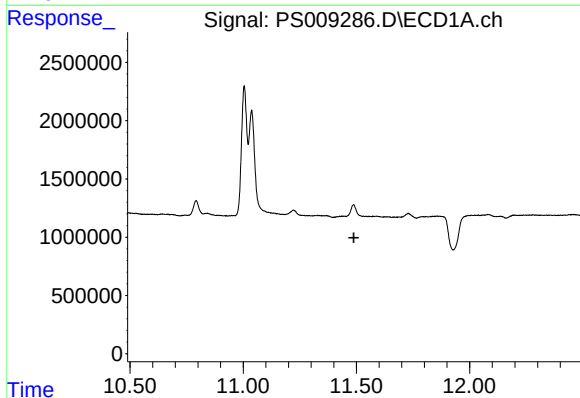

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

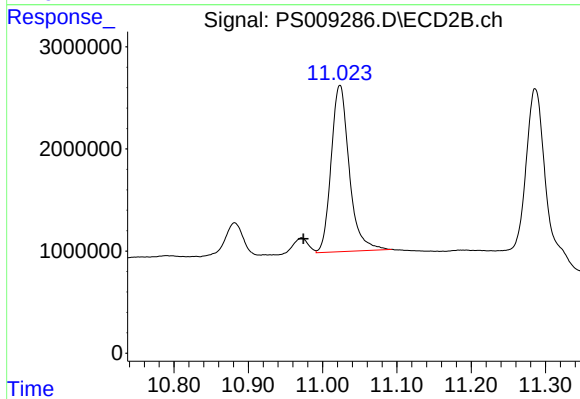

#16 DCPA

R.T.: 11.023 min
Delta R.T.: 0.049 min
Response: 27529915
Conc: 7.11 ng/ml