

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031420\
 Data File : PS009289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2020 10:36
 Operator : DD\AJ
 Sample : PB127537BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 04:48:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	260.6E6	278.1E6	471.154	506.345
Target Compounds							
1) T	Dalapon	3.007	2.587	15099540	90814394	19.363	115.340 #
2) T	3,5-DICHL...	0.000	6.110	0	44391995	N.D.	54.582
3) T	4-Nitroph...	0.000	6.591	0	24653252	N.D.	77.478
7) T	MCPA	7.735	7.400	12470060	62436746	4.094	23.137 #
8) T	DICHLORPROP	0.000	7.753	0	29967569	N.D.	54.013
12) T	2,4,5-T	9.445	9.252	18980854	47833026	7.461	16.203 #
14) T	DINOSEB	0.000	10.045	0	12891641	N.D.	5.869
15) T	Picloram	11.037	11.022	96370339	171.6E6	31.754	42.149 #
16) T	DCPA	0.000	11.022	0	171.6E6	N.D.	44.316



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031420\
Data File : PS009289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2020 10:36
Operator : DD\AJ
Sample : PB127537BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 04:48:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

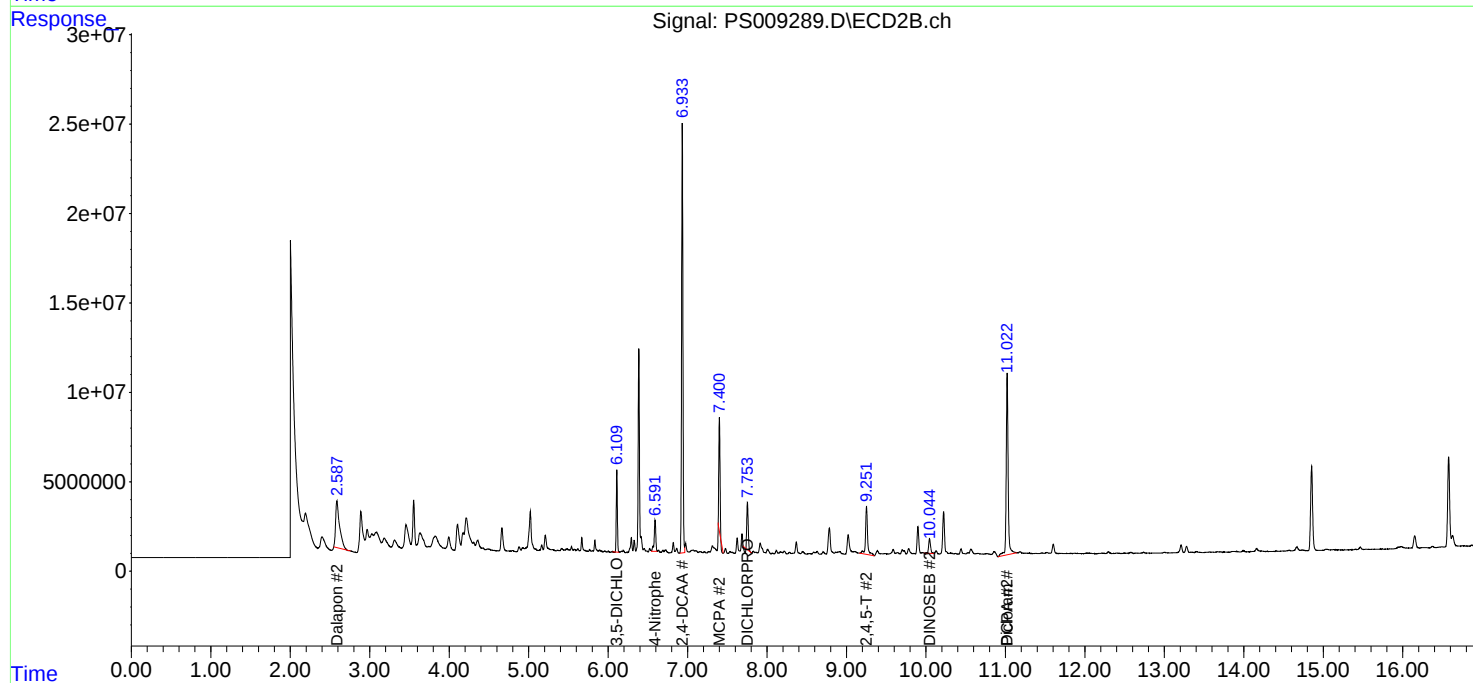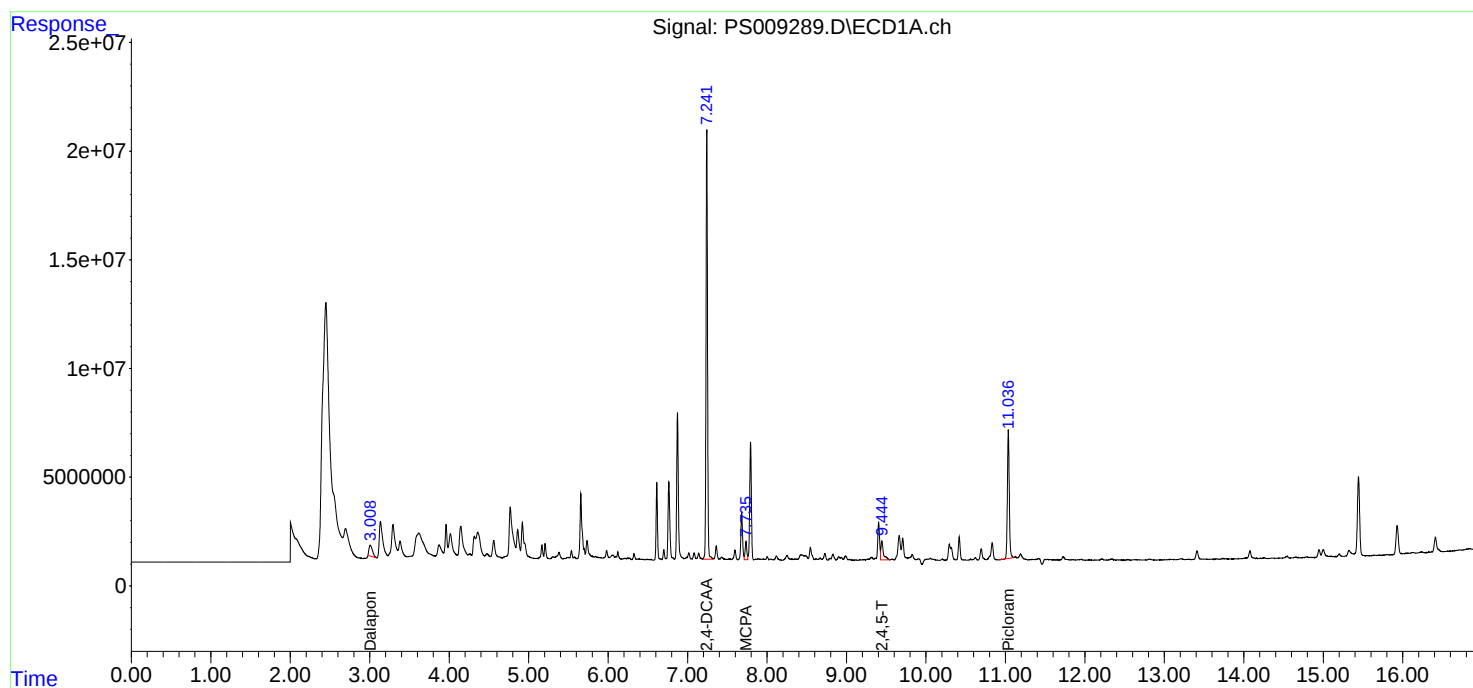


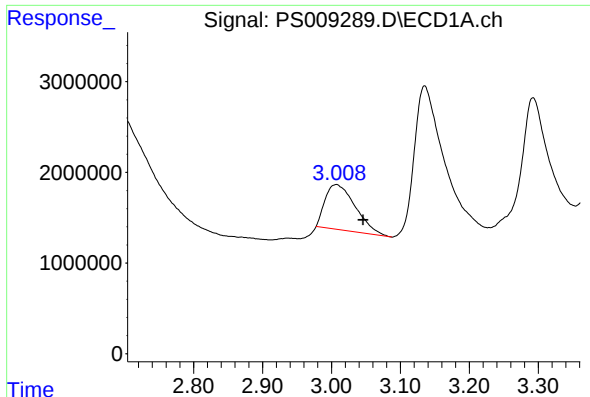

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 15099540
Conc: 19.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

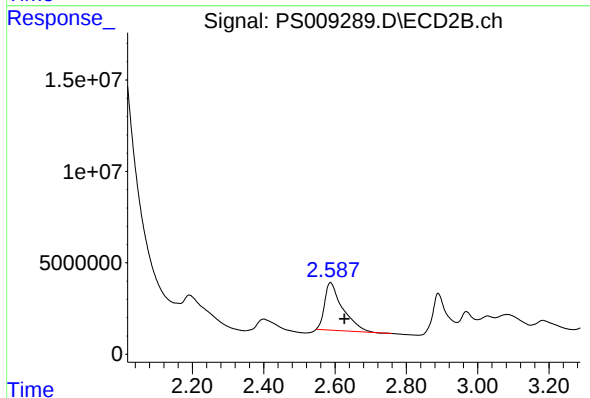


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.039 min
Response: 90814394
Conc: 115.34 ng/ml

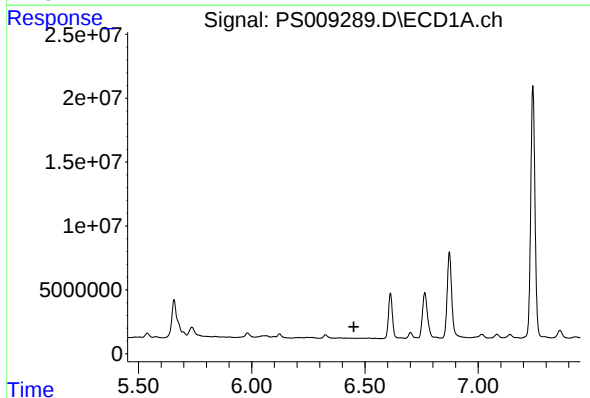


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

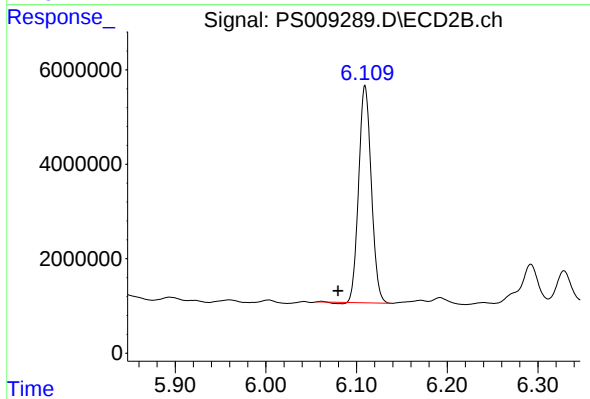

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 44391995
Conc: 54.58 ng/ml

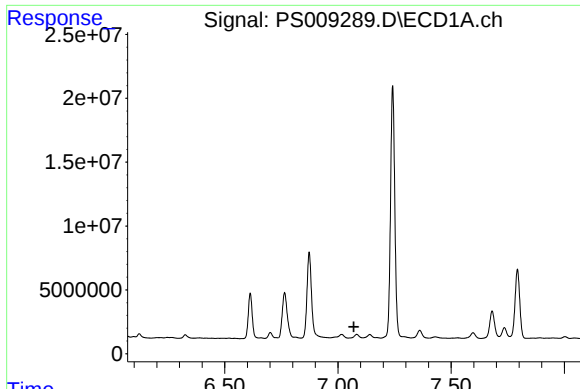

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

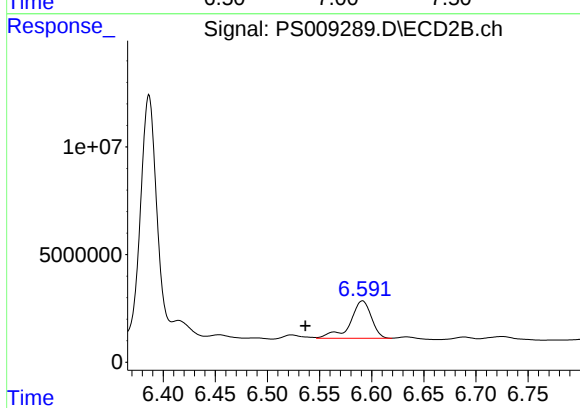


#3 4-Nitrophenol

R.T.: 6.591 min
Delta R.T.: 0.055 min
Response: 24653252
Conc: 77.48 ng/ml

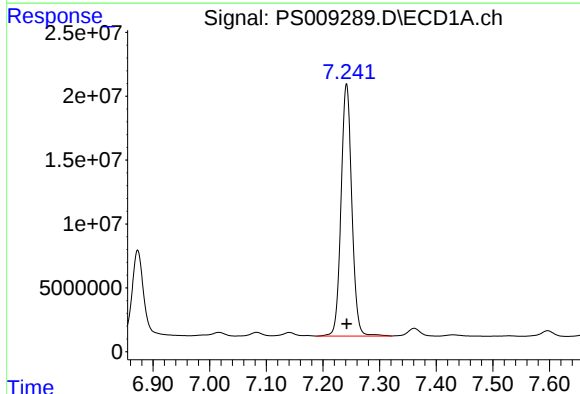


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 260628552
Conc: 471.15 ng/ml

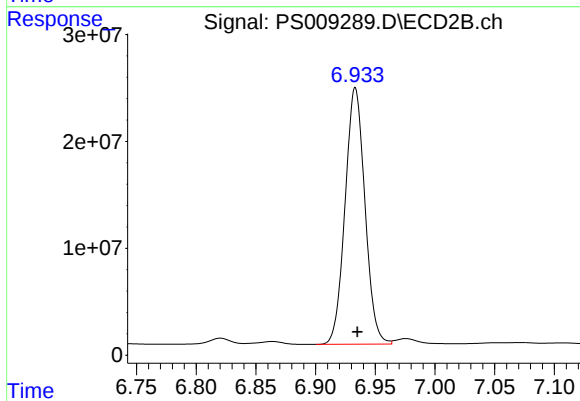

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 278083610
Conc: 506.35 ng/ml

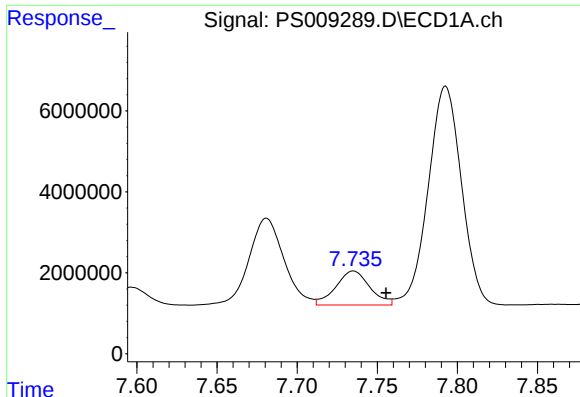

#7 MCPA


R.T.: 7.735 min
Delta R.T.: -0.021 min
Response: 12470060
Conc: 4.09 ug/ml

Instrument :
ECD_S
ClientSampleId :

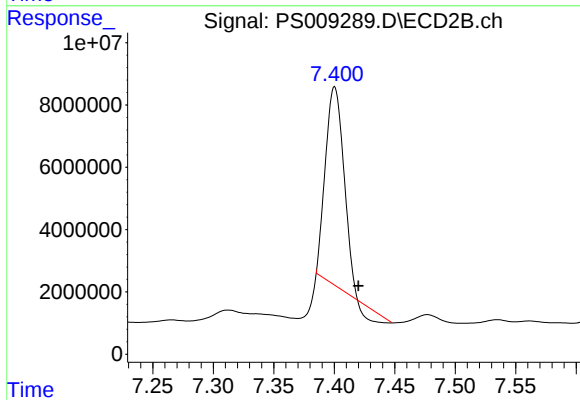


#7 MCPA

R.T.: 7.400 min
Delta R.T.: -0.020 min
Response: 62436746
Conc: 23.14 ug/ml

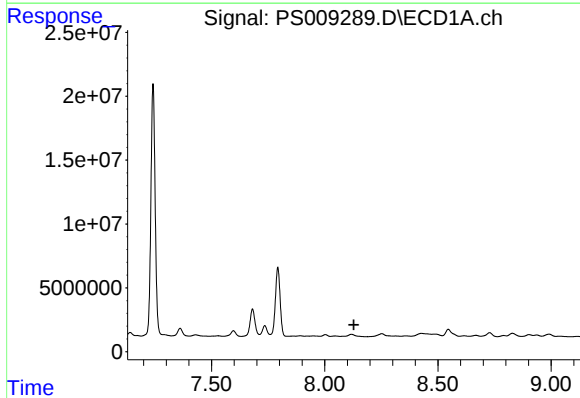


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

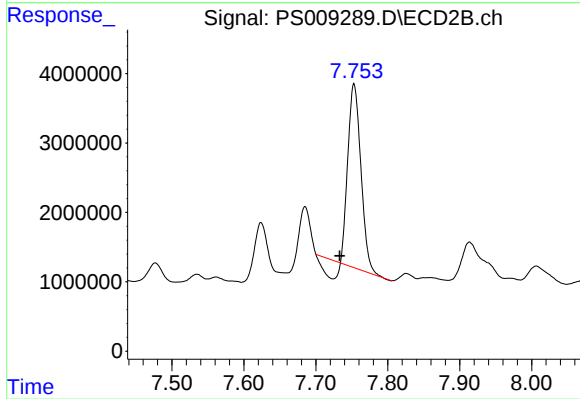

#8 DICHLORPROP


R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 29967569
Conc: 54.01 ng/ml

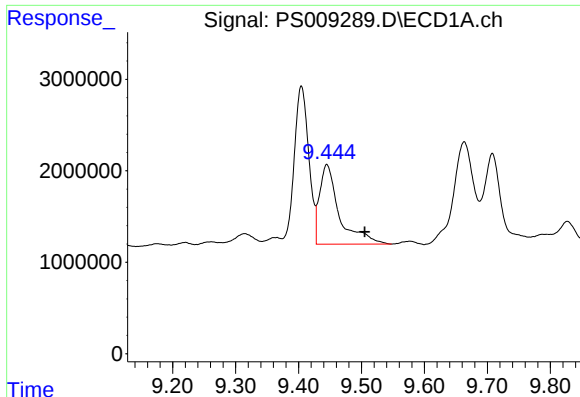

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 18980854
Conc: 7.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

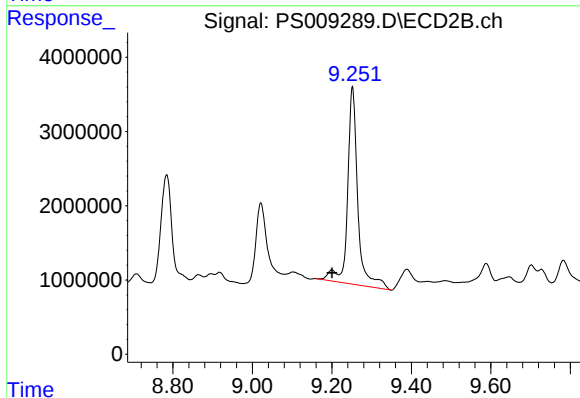


#12 2,4,5-T

R.T.: 9.252 min
Delta R.T.: 0.051 min
Response: 47833026
Conc: 16.20 ng/ml

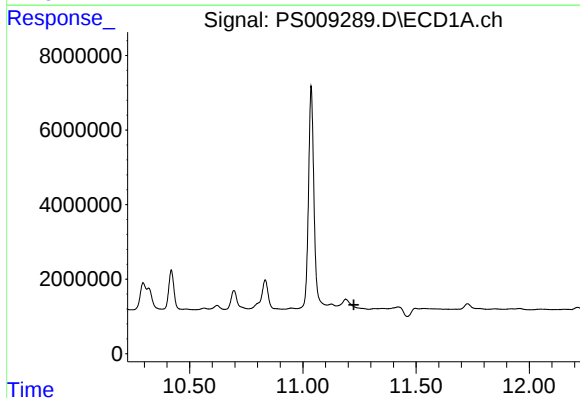


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.225 min
Response: 0
Conc: N.D.

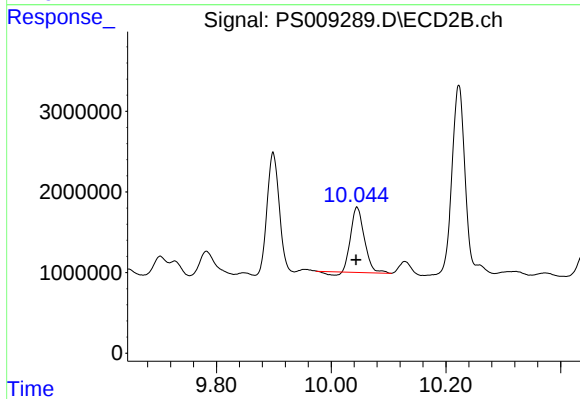

#14 DINOSEB


R.T.: 10.045 min
Delta R.T.: 0.001 min
Response: 12891641
Conc: 5.87 ng/ml

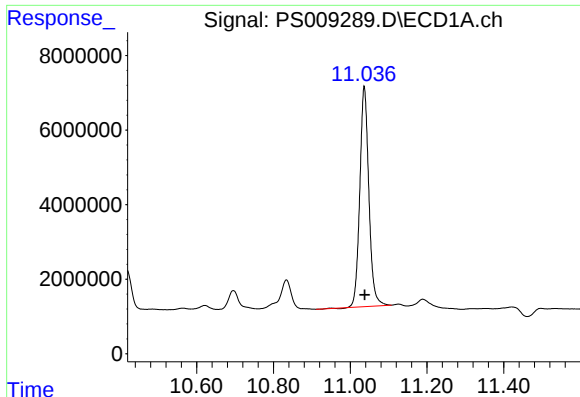

#15 Picloram


R.T.: 11.037 min
Delta R.T.: 0.000 min
Response: 96370339
Conc: 31.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

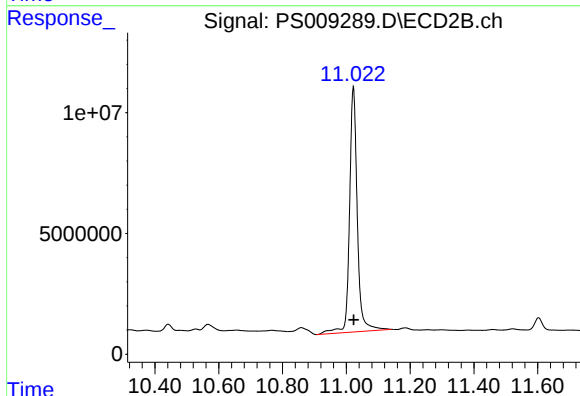


#15 Picloram

R.T.: 11.022 min
Delta R.T.: -0.001 min
Response: 171638381
Conc: 42.15 ng/ml

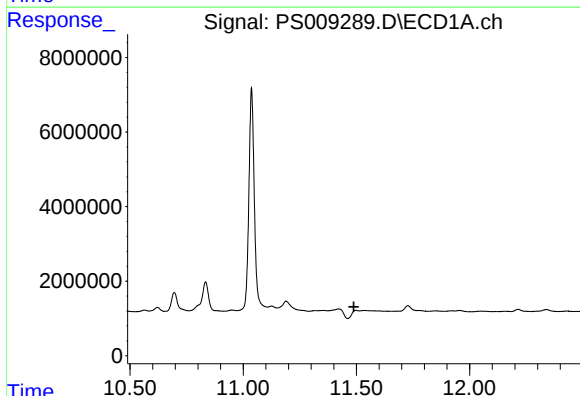

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

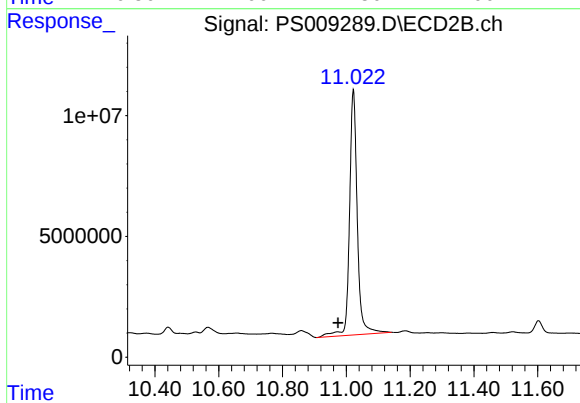

#16 DCPA

R.T.: 11.022 min
Delta R.T.: 0.048 min
Response: 171638381
Conc: 44.32 ng/ml