

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031420\
 Data File : PS009291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2020 11:22
 Operator : DD\AJ
 Sample : PB127537TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 04:49:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.933	208.9E6	211.0E6	377.668	384.184
Target Compounds							
1) T	Dalapon	3.006	2.591	19904667	103.6E6	25.524	131.616 #
2) T	3,5-DICHL...	0.000	6.110	0	62859757	N.D.	77.289
3) T	4-Nitroph...	0.000	6.591	0	18172002	N.D.	57.109
8) T	DICHLORPROP	0.000	7.753	0	42051555	N.D.	75.793
12) T	2,4,5-T	9.445	0.000	53392521	0	20.989	N.D. #
15) T	Picloram	11.035	11.021	10750018	18867051	3.542	4.633 #
16) T	DCPA	0.000	11.021	0	18867051	N.D.	4.871



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031420\
Data File : PS009291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2020 11:22
Operator : DD\AJ
Sample : PB127537TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 04:49:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

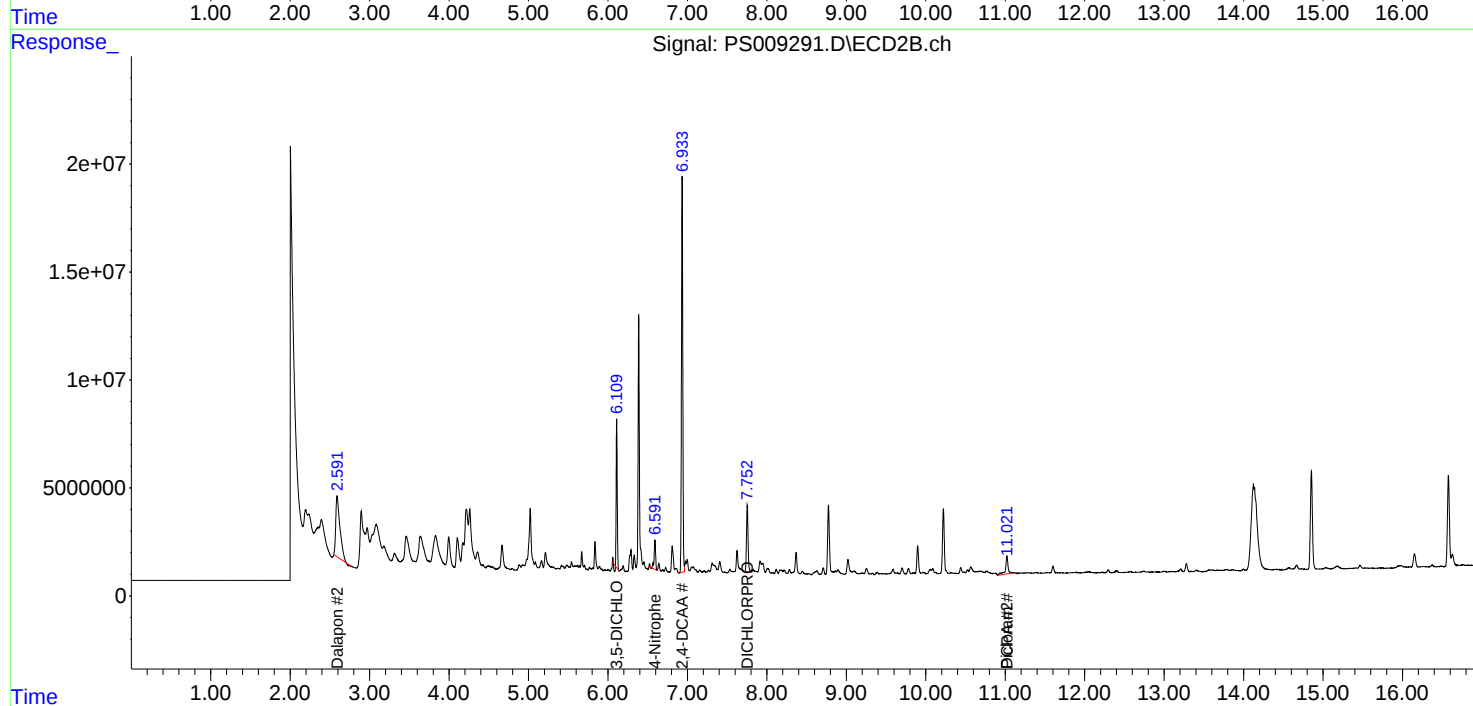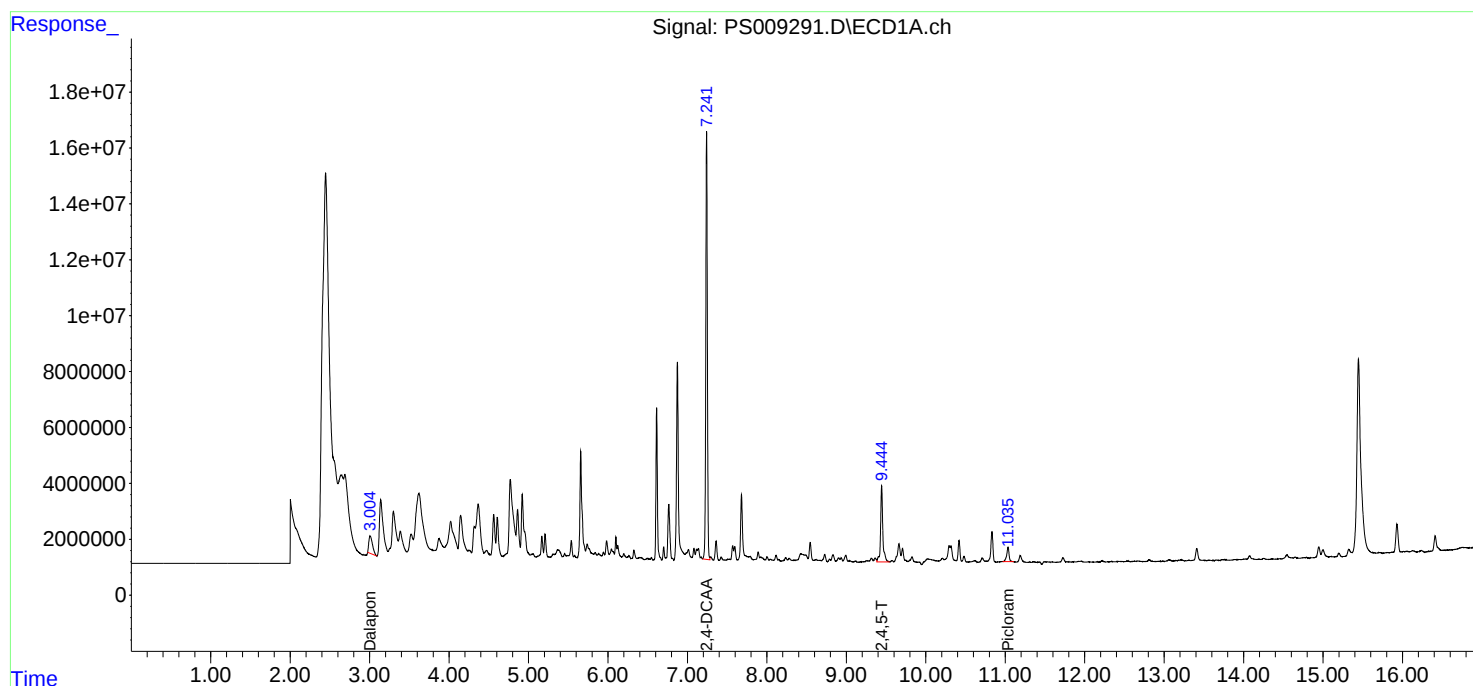


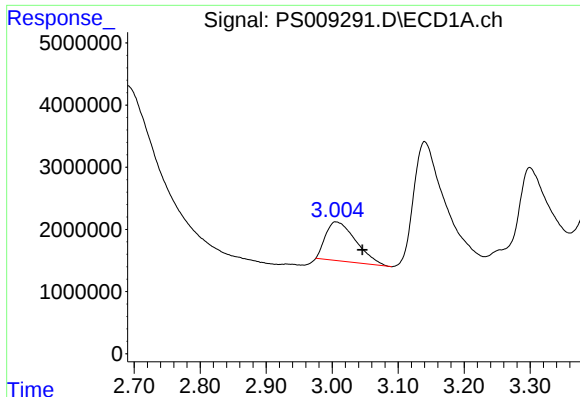

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 19904667
Conc: 25.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

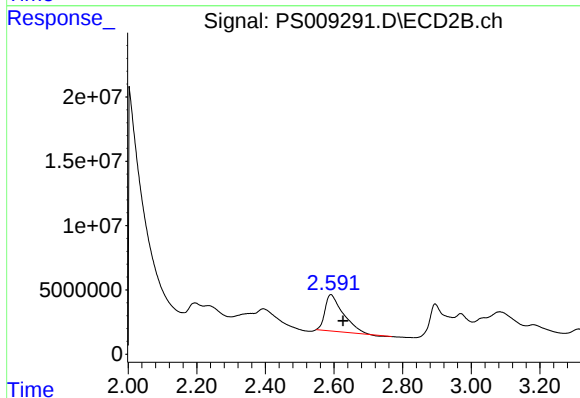


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.036 min
Response: 103629407
Conc: 131.62 ng/ml

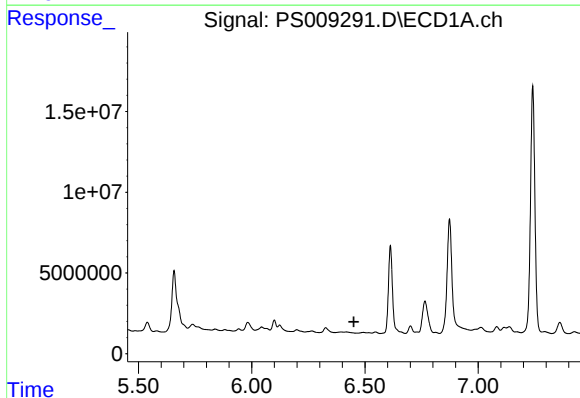


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

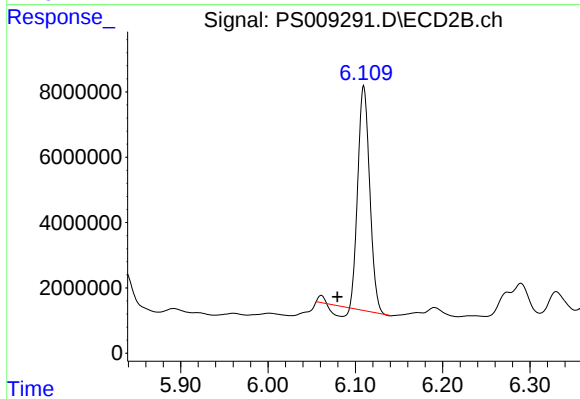

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 62859757
Conc: 77.29 ng/ml

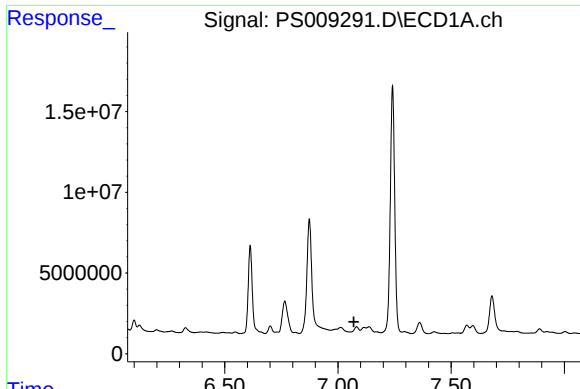

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.071 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

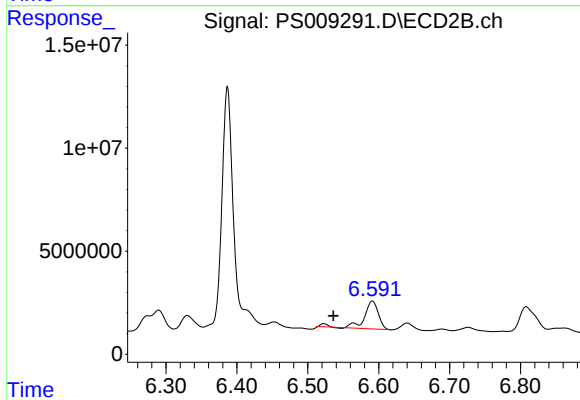


#3 4-Nitrophenol

R.T.: 6.591 min
Delta R.T.: 0.055 min
Response: 18172002
Conc: 57.11 ng/ml

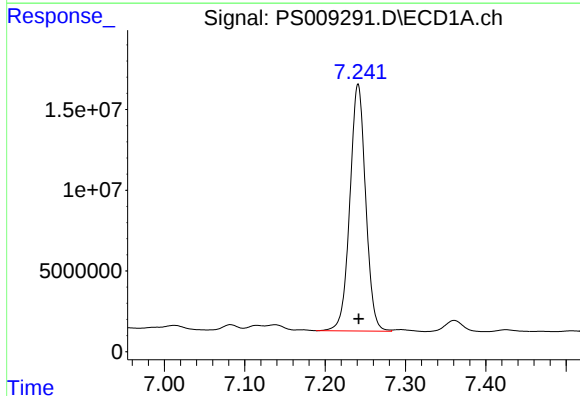


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 208914596
Conc: 377.67 ng/ml

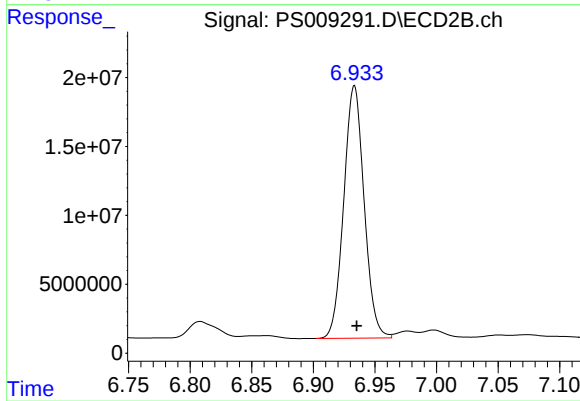

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 210992926
Conc: 384.18 ng/ml

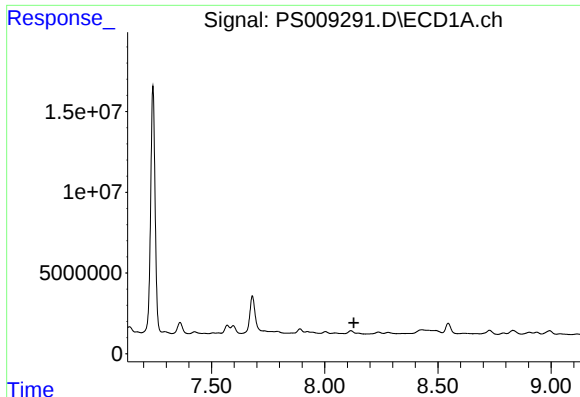

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

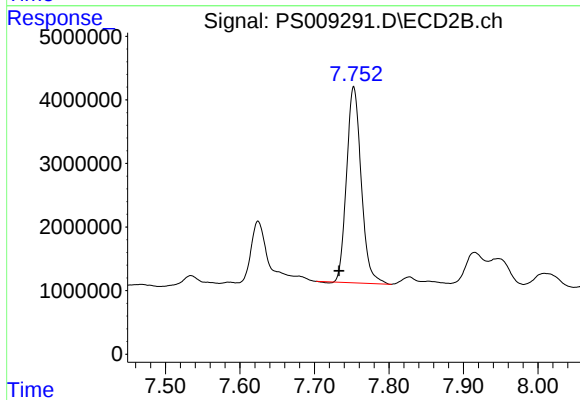


#8 DICHLORPROP

R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 42051555
Conc: 75.79 ng/ml

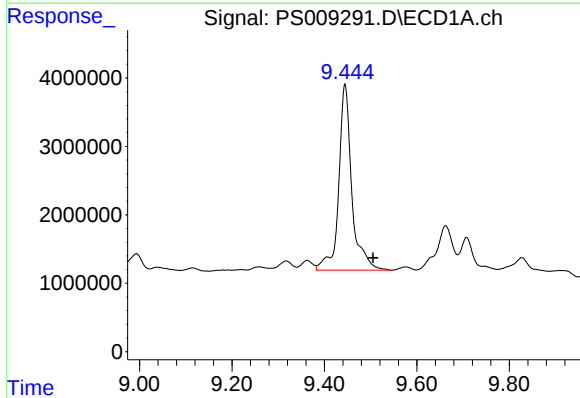


#12 2,4,5-T

R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 53392521
Conc: 20.99 ng/ml

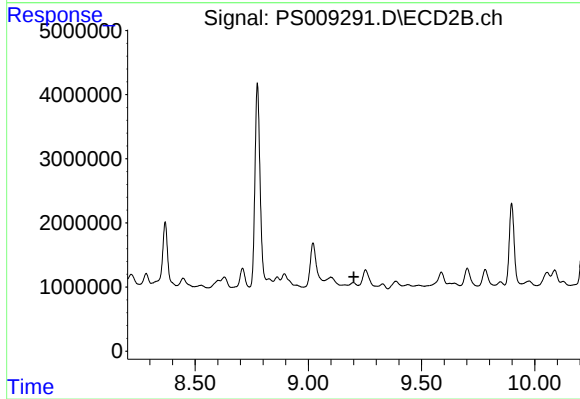

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

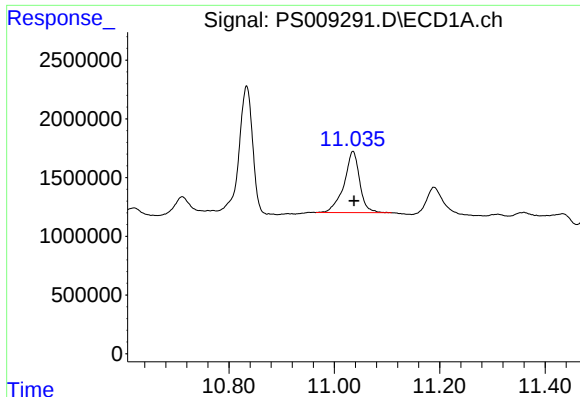

#15 Picloram


R.T.: 11.035 min
Delta R.T.: -0.002 min
Response: 10750018
Conc: 3.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

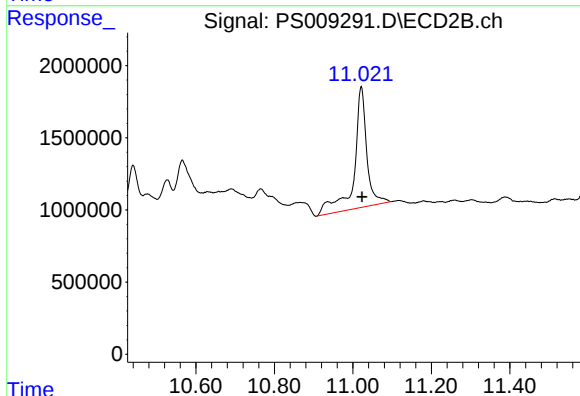


#15 Picloram

R.T.: 11.021 min
Delta R.T.: -0.002 min
Response: 18867051
Conc: 4.63 ng/ml

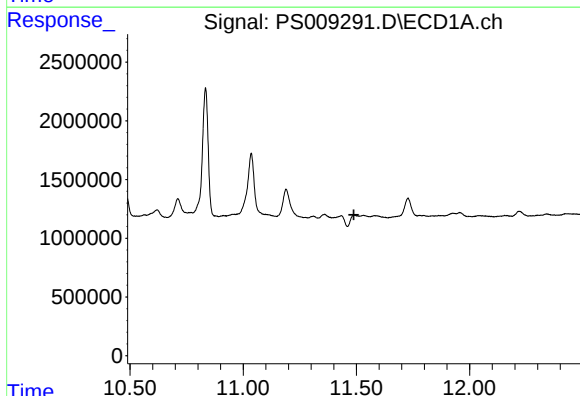

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

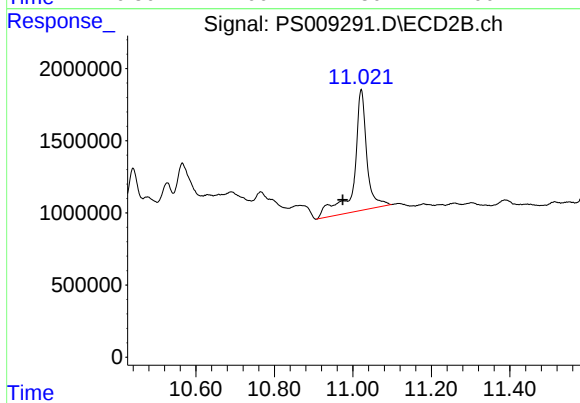

#16 DCPA

R.T.: 11.021 min
Delta R.T.: 0.047 min
Response: 18867051
Conc: 4.87 ng/ml