

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031422\
 Data File : PS018553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 08:55
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 13:33:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
9) T	2,4-D	8.421f	0.000	9585113	0	2.861	N.D. #
11) T	2,4,5-TP ...	0.000	8.643f	0	4323531	N.D.	<MDL
12) T	2,4,5-T	9.499	9.062	9403923	3390521	<MDL	<MDL #
14) T	DINOSEB	11.221	0.000	10200310	0	<MDL	N.D. #
15) T	Picloram	11.033	10.875	64787577	15993612	3.152	3.009
16) T	DCPA	11.486	10.831	6635814	3674672	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031422\
Data File : PS018553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 08:55
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 13:33:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

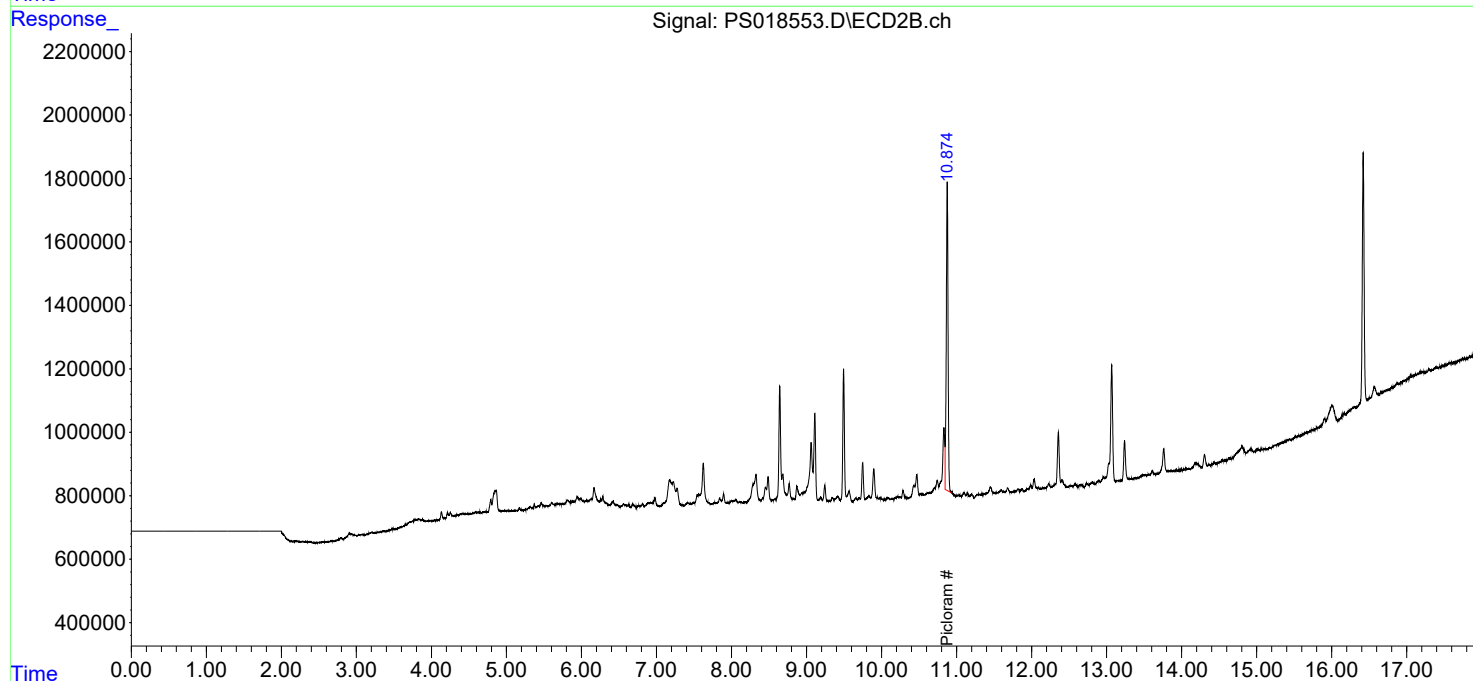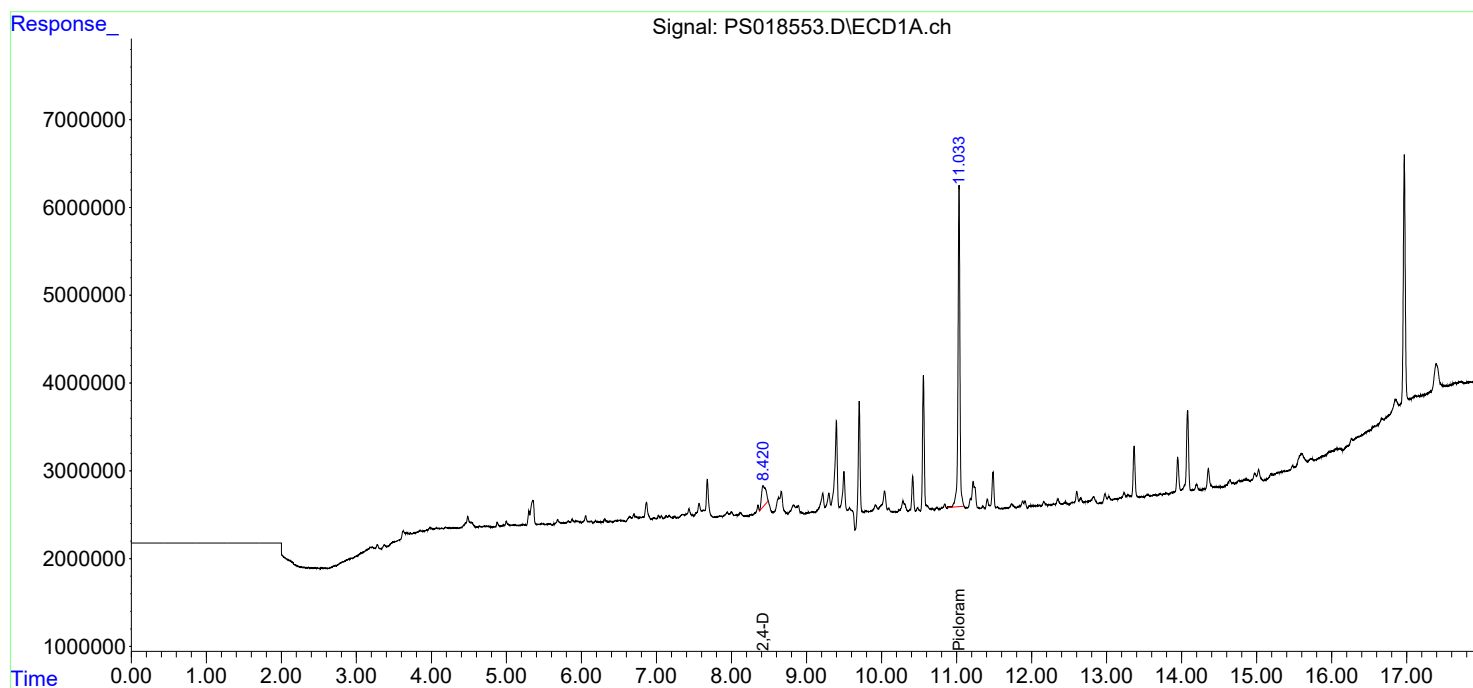


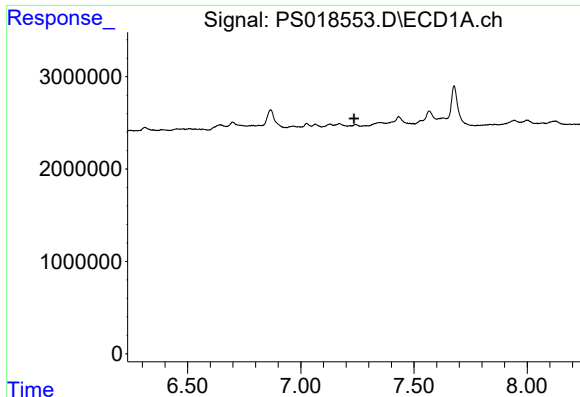

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.235 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

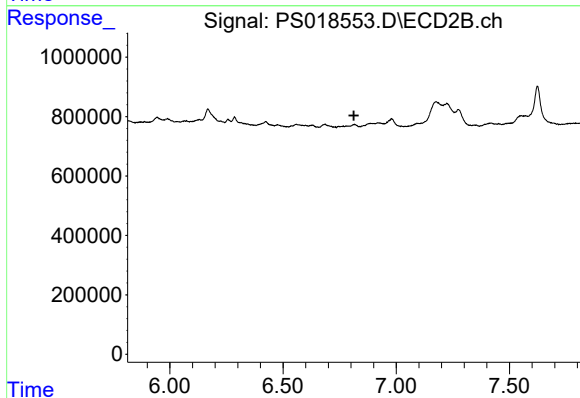


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.813 min
Response: 0
Conc: N.D.

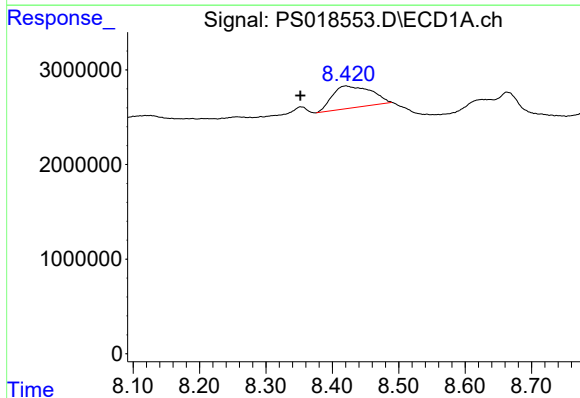


#9 2,4-D

R.T.: 8.421 min
Delta R.T.: 0.069 min
Response: 9585113
Conc: 2.86 ng/ml

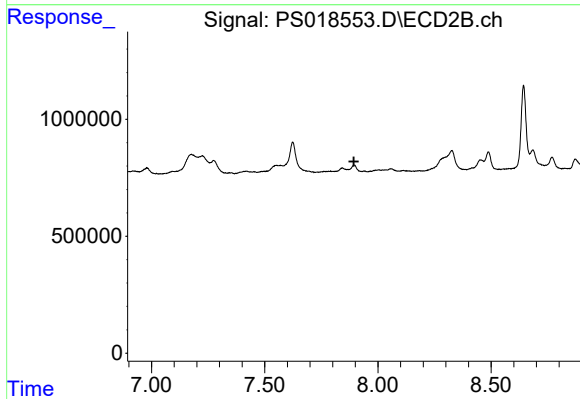

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

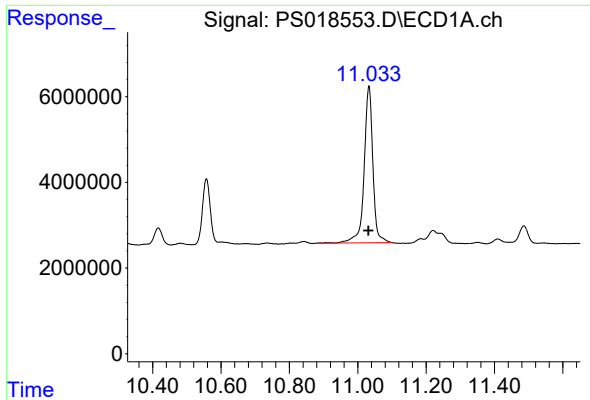

#15 Picloram

R.T.: 11.033 min
Delta R.T.: 0.002 min
Response: 64787577
Conc: 3.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

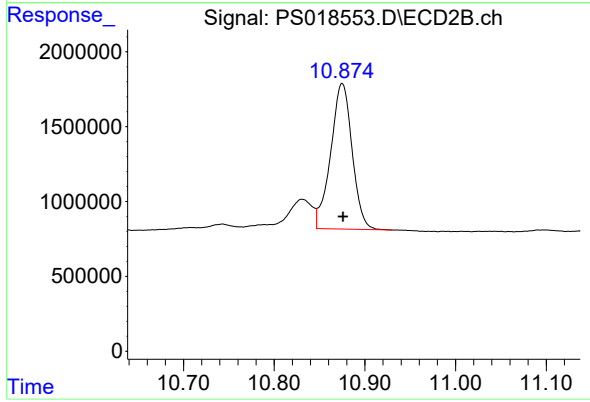

#15 Picloram

R.T.: 10.875 min
Delta R.T.: 0.000 min
Response: 15993612
Conc: 3.01 ng/ml