

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031422\
 Data File : PS018574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 18:12
 Operator : AJ\MA
 Sample : PB143168BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB143168BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:06:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.234	6.812	1227.4E6	342.5E6	431.272	486.688
Target Compounds							
3) T	4-Nitroph...	7.125f	6.477f	10883838	10961729	6.316	26.981 #
8) T	DICHLORPROP	0.000	7.626	0	15383850	N.D.	19.434
9) T	2,4-D	8.421f	0.000	7086170	0	2.115	N.D. #
11) T	2,4,5-TP ...	9.280f	8.641f	16698559	5347813	1.098	1.226
12) T	2,4,5-T	9.497	9.109f	5234682	3447511	<MDL	<MDL #
14) T	DINOSEB	11.243	0.000	6200719	0	<MDL	N.D. #
15) T	Picloram	11.028	10.874	58304413	17823113	2.836	3.353
16) T	DCPA	0.000	10.874f	0	17823113	N.D.	3.389



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031422\
Data File : PS018574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 18:12
Operator : AJ\MA
Sample : PB143168BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB143168BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:06:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

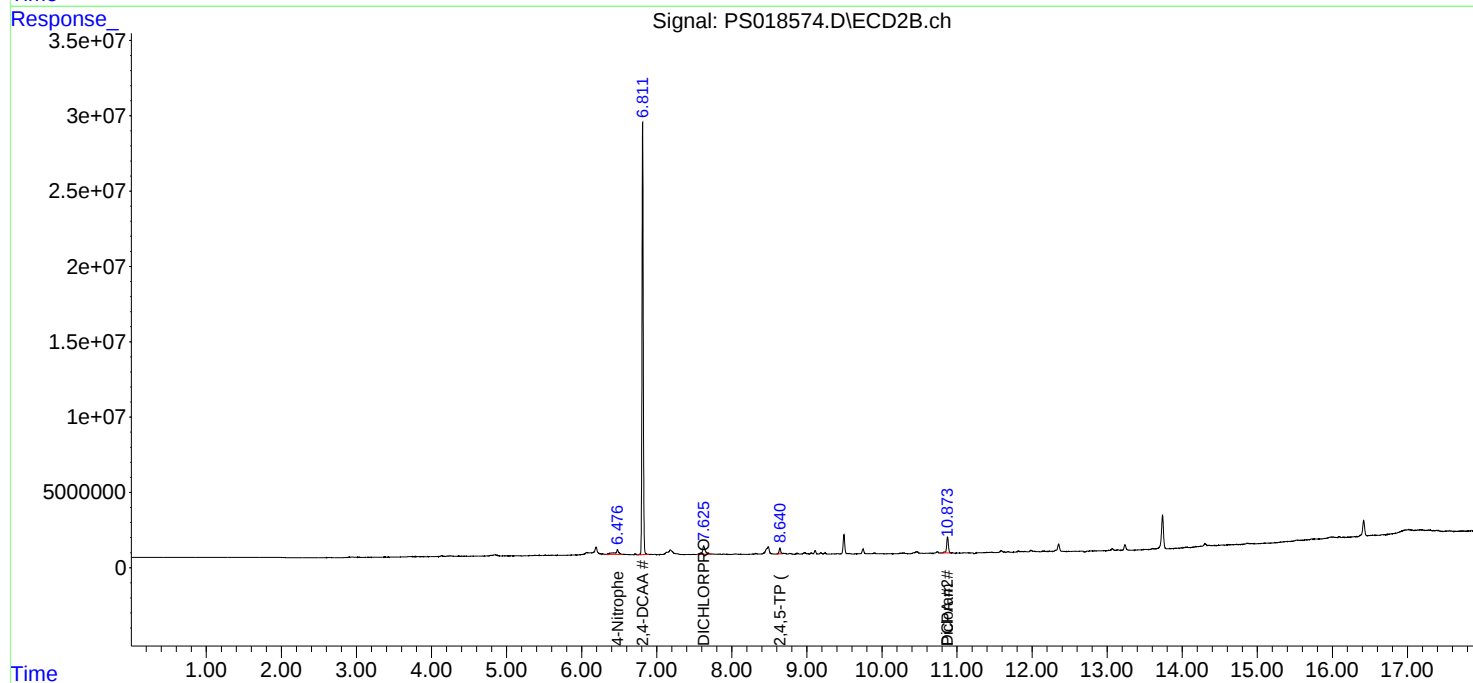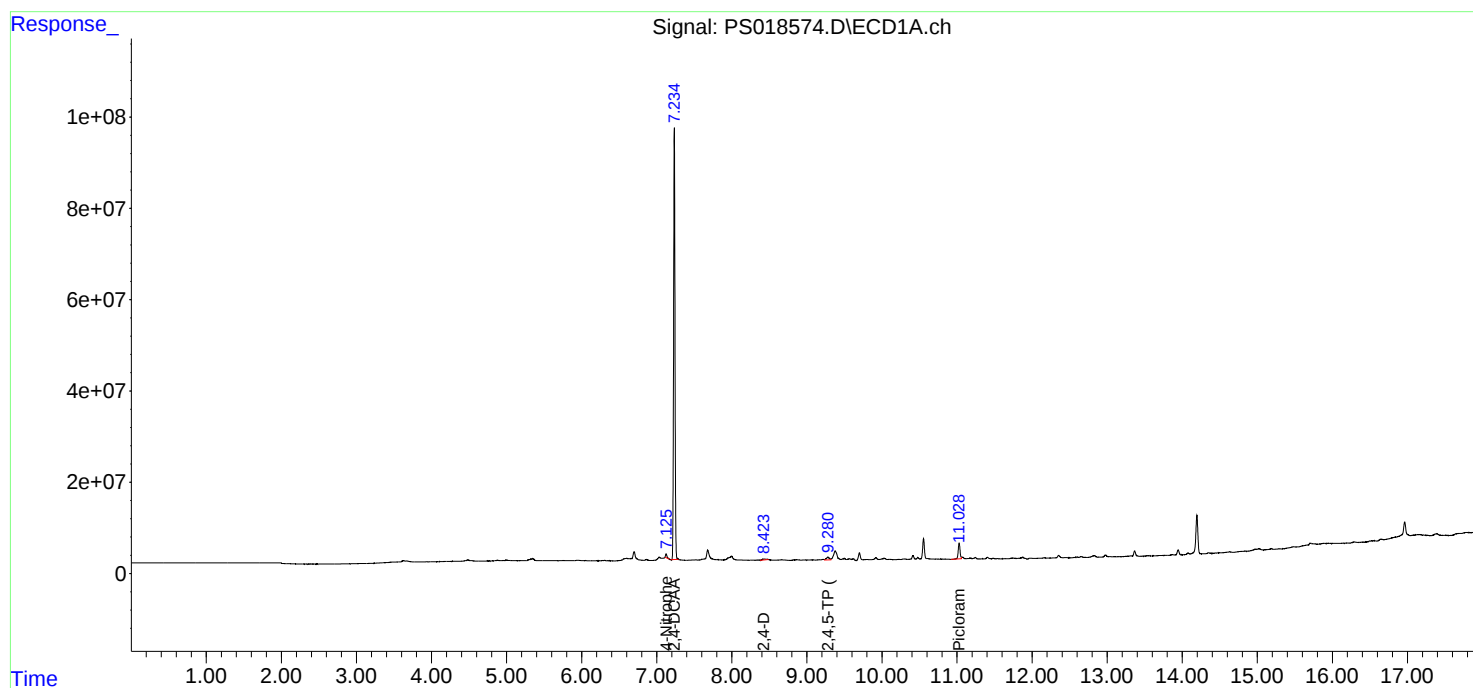


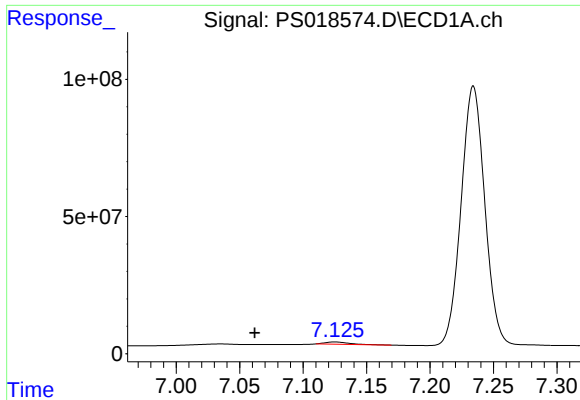

#3 4-Nitrophenol


R.T.: 7.125 min
Delta R.T.: 0.063 min
Response: 10883838
Conc: 6.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB143168BL

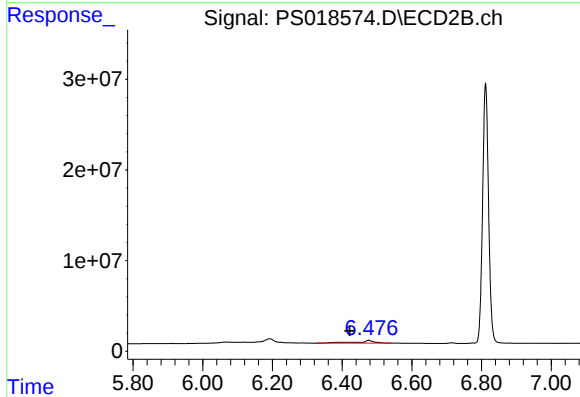


#3 4-Nitrophenol

R.T.: 6.477 min
Delta R.T.: 0.055 min
Response: 10961729
Conc: 26.98 ng/ml

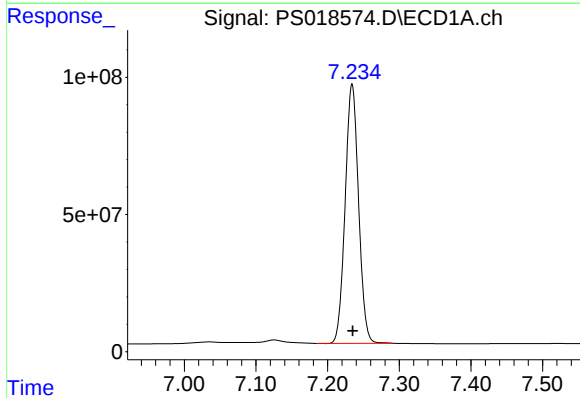


#4 2,4-DCAA

R.T.: 7.234 min
Delta R.T.: 0.000 min
Response: 1227362734
Conc: 431.27 ng/ml

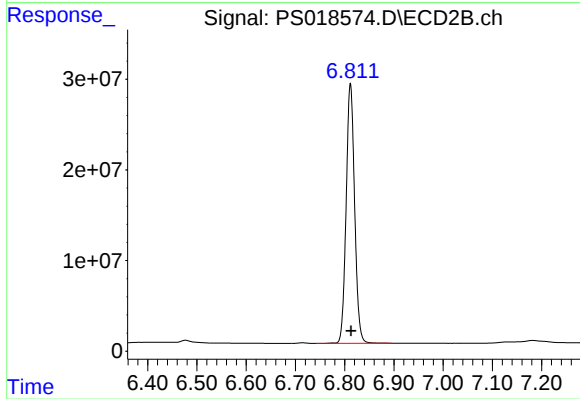

#4 2,4-DCAA


R.T.: 6.812 min
Delta R.T.: -0.001 min
Response: 342460238
Conc: 486.69 ng/ml

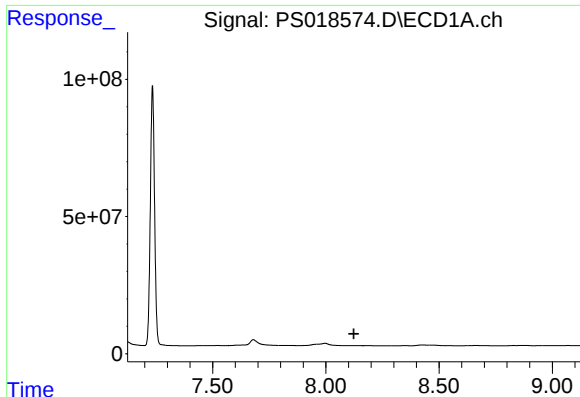

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB143168BL

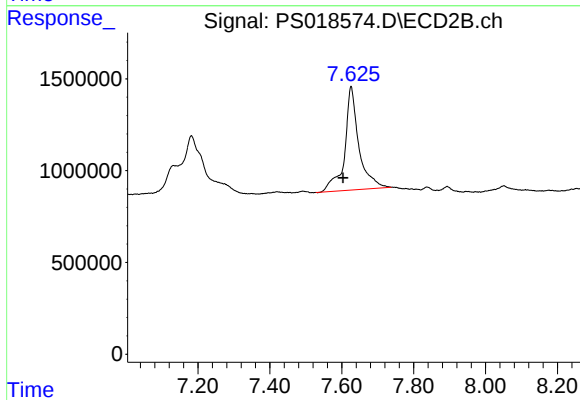


#8 DICHLORPROP

R.T.: 7.626 min
Delta R.T.: 0.022 min
Response: 15383850
Conc: 19.43 ng/ml

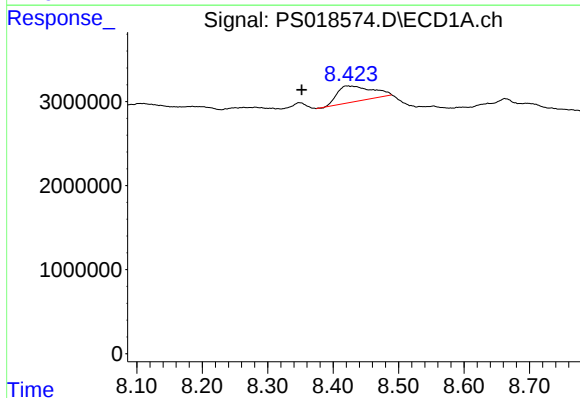


#9 2,4-D

R.T.: 8.421 min
Delta R.T.: 0.069 min
Response: 7086170
Conc: 2.11 ng/ml

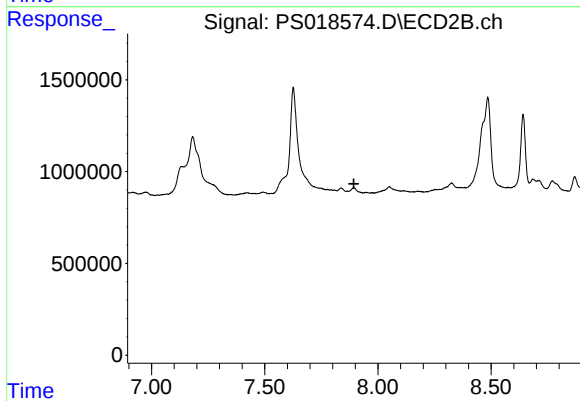

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

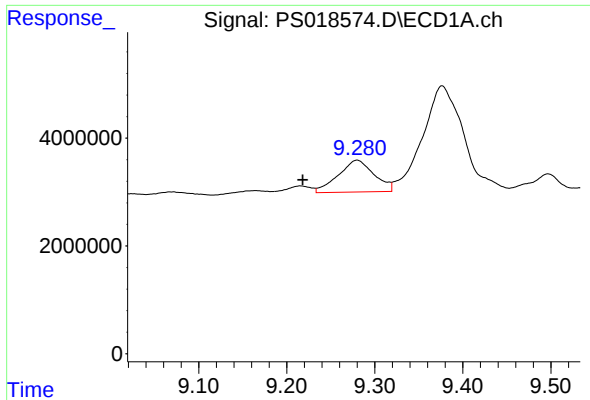

#11 2,4,5-TP (SILVEX)


R.T.: 9.280 min
Delta R.T.: 0.062 min
Response: 16698559
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB143168BL

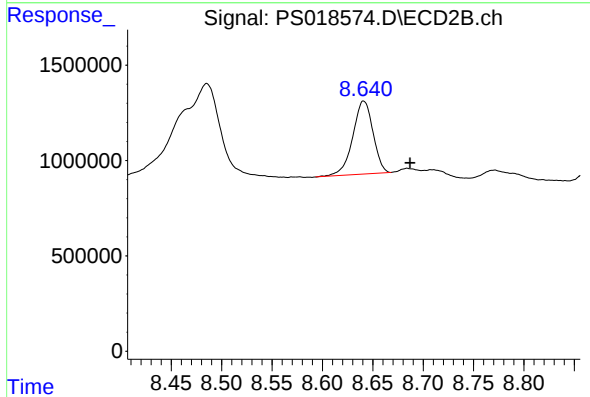


#11 2,4,5-TP (SILVEX)

R.T.: 8.641 min
Delta R.T.: -0.046 min
Response: 5347813
Conc: 1.23 ng/ml

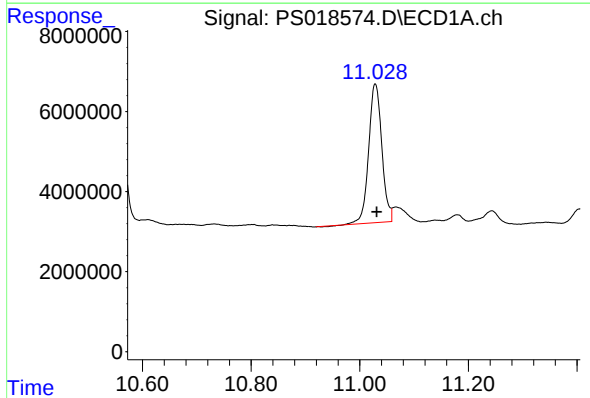


#15 Picloram

R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 58304413
Conc: 2.84 ng/ml

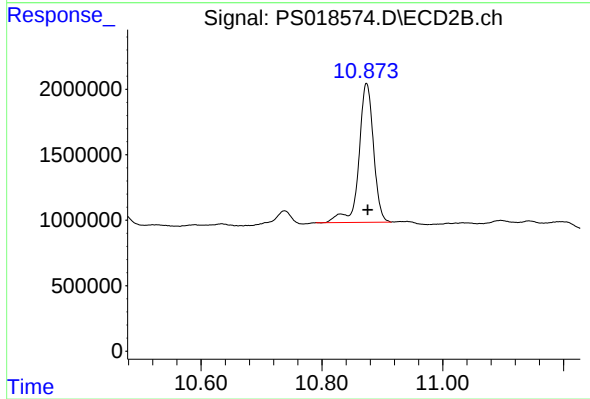

#15 Picloram


R.T.: 10.874 min
Delta R.T.: -0.002 min
Response: 17823113
Conc: 3.35 ng/ml

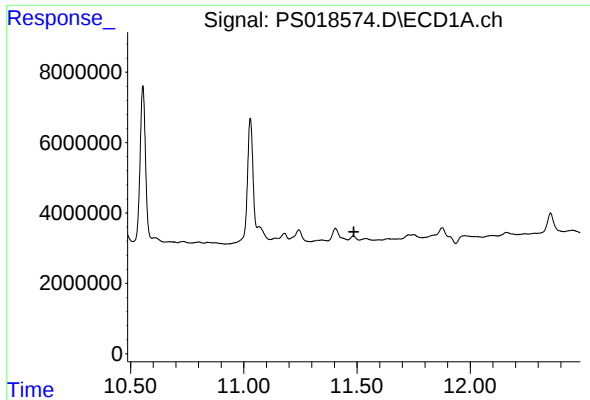

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB143168BL

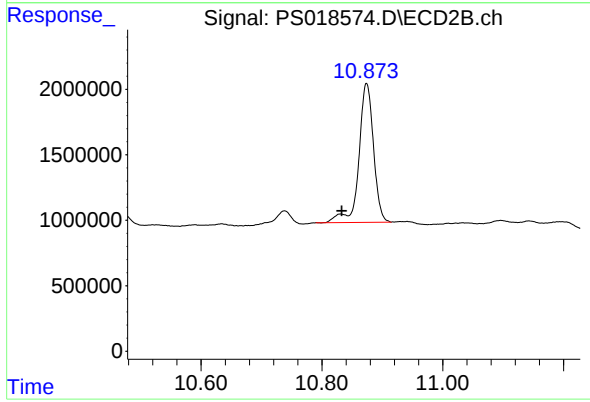

#16 DCPA

R.T.: 10.874 min
Delta R.T.: 0.041 min
Response: 17823113
Conc: 3.39 ng/ml