

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031422\
 Data File : PS018578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 19:47
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:07:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.234	6.811	1244.0E6	346.4E6	437.105	492.234
Target Compounds							
3) T	4-Nitroph...	7.124f	6.423	8470576	2042662	4.916	5.028
5) T	DICAMBA	7.427	0.000	3199417	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.622	0	11169954	N.D.	14.110
9) T	2,4-D	8.349	0.000	3571719	0	1.066	N.D. #
10) T	Pentachlo...	8.662	8.323	10424747	2537835	<MDL	<MDL #
11) T	2,4,5-TP ...	9.216	8.685	8527739	2519103	<MDL	<MDL #
12) T	2,4,5-T	9.498	9.061	13827913	3548907	<MDL	<MDL #
13) T	2,4-DB	10.037	0.000	5059867	0	1.850	N.D. #
14) T	DINOSEB	11.219	9.898	1288318	2074162	<MDL	<MDL #
15) T	Picloram	11.030	10.874	135.3E6	36370229	6.584	6.842
16) T	DCPA	11.484	10.830	6189048	2883700	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031422\
Data File : PS018578.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 19:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:07:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

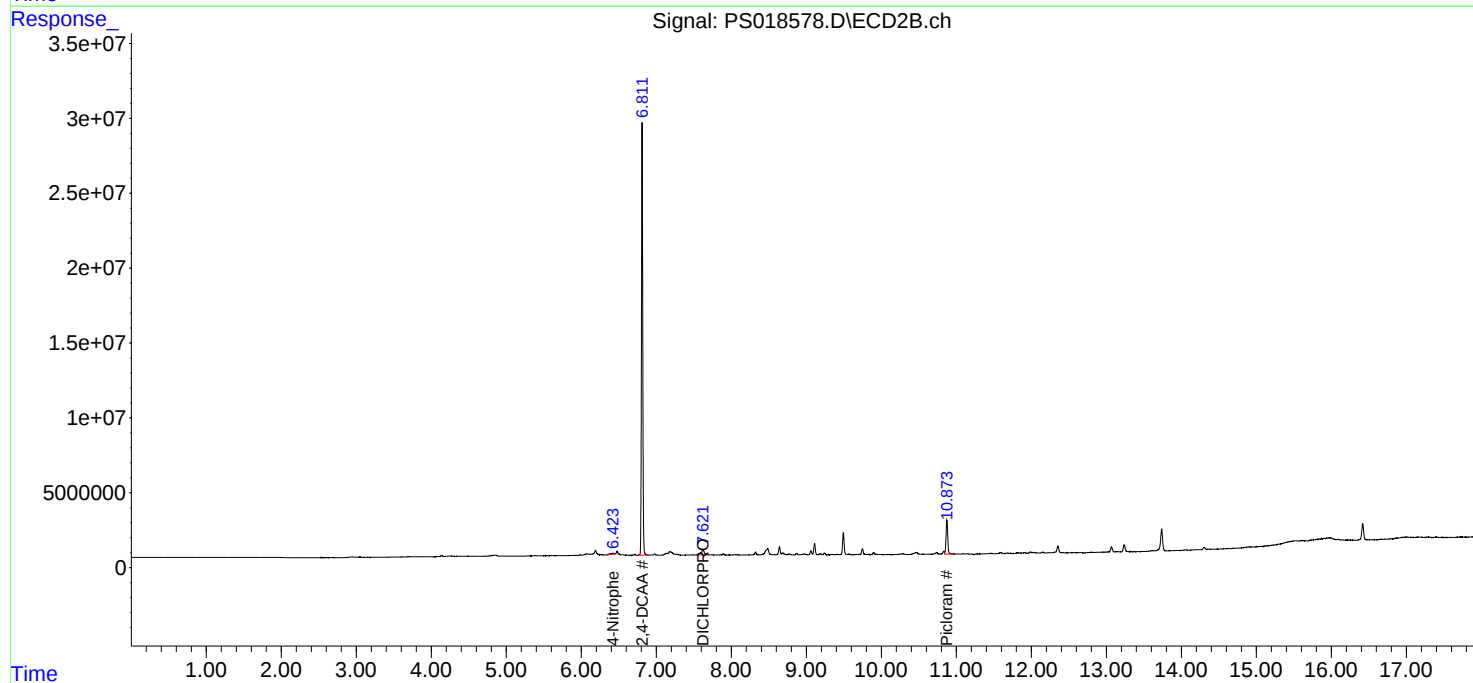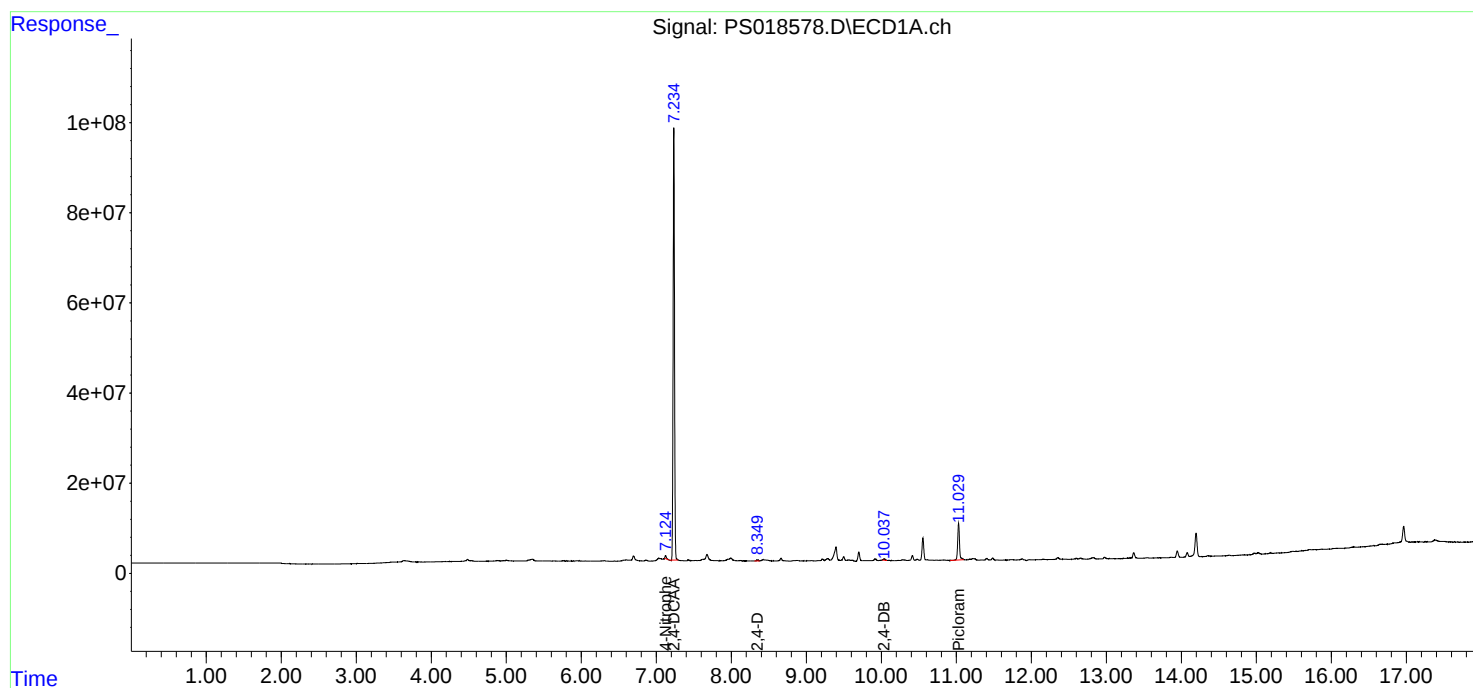


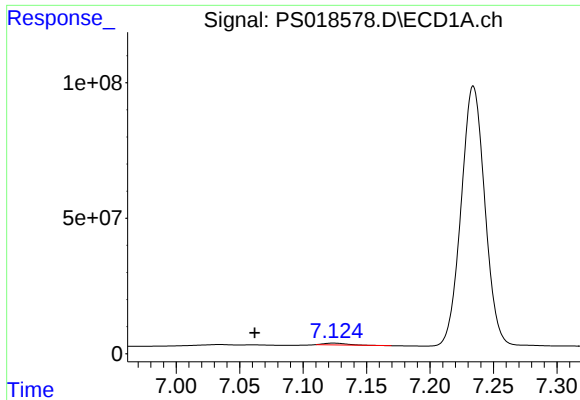

#3 4-Nitrophenol


R.T.: 7.124 min
Delta R.T.: 0.062 min
Response: 8470576
Conc: 4.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

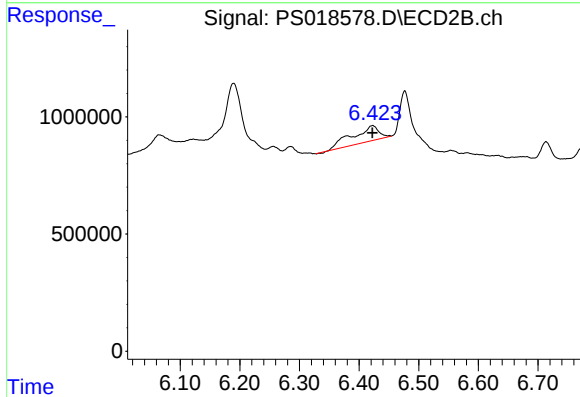


#3 4-Nitrophenol

R.T.: 6.423 min
Delta R.T.: 0.000 min
Response: 2042662
Conc: 5.03 ng/ml

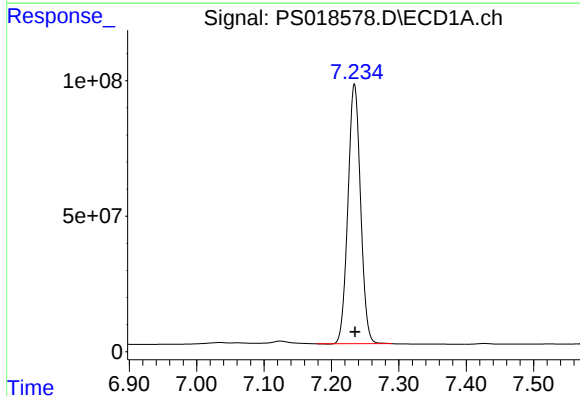


#4 2,4-DCAA

R.T.: 7.234 min
Delta R.T.: 0.000 min
Response: 1243963585
Conc: 437.10 ng/ml

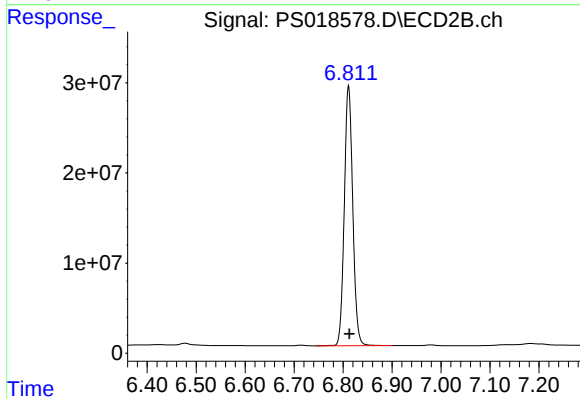

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: -0.002 min
Response: 346363040
Conc: 492.23 ng/ml

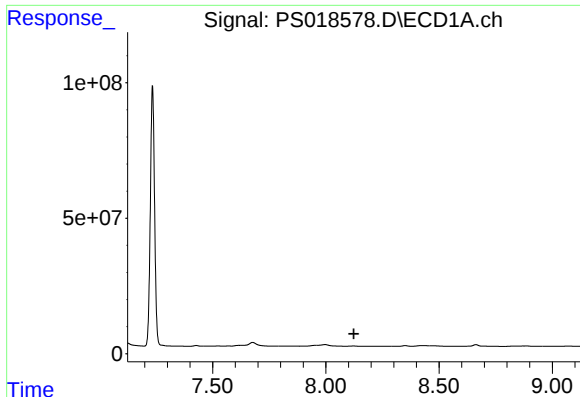

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

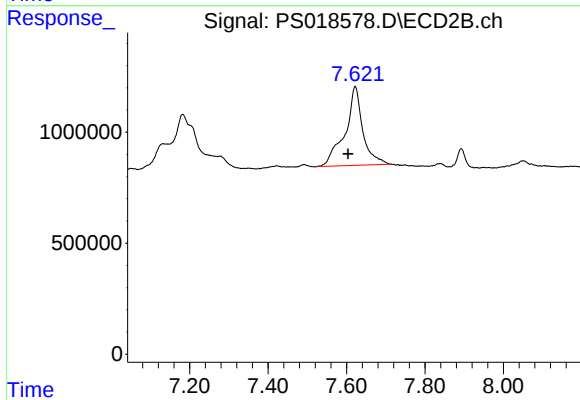


#8 DICHLORPROP

R.T.: 7.622 min
Delta R.T.: 0.018 min
Response: 11169954
Conc: 14.11 ng/ml

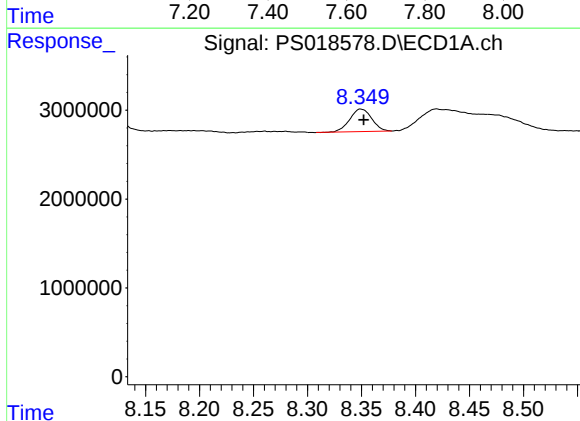


#9 2,4-D

R.T.: 8.349 min
Delta R.T.: -0.003 min
Response: 3571719
Conc: 1.07 ng/ml

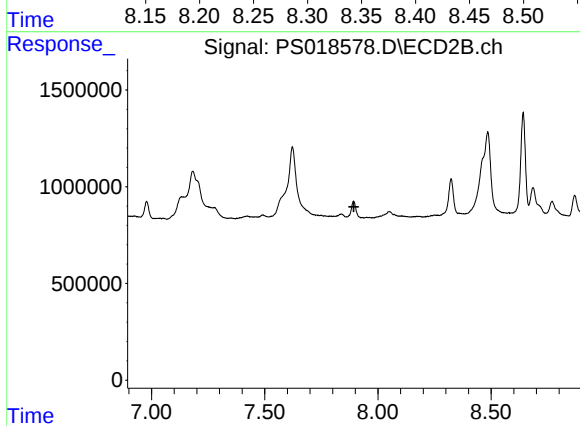

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

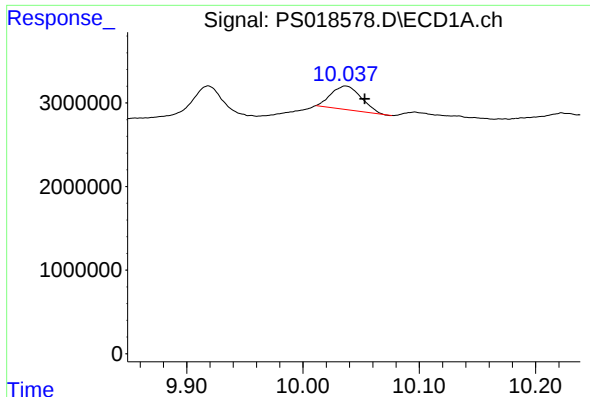

#13 2,4-DB


R.T.: 10.037 min
Delta R.T.: -0.016 min
Response: 5059867
Conc: 1.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

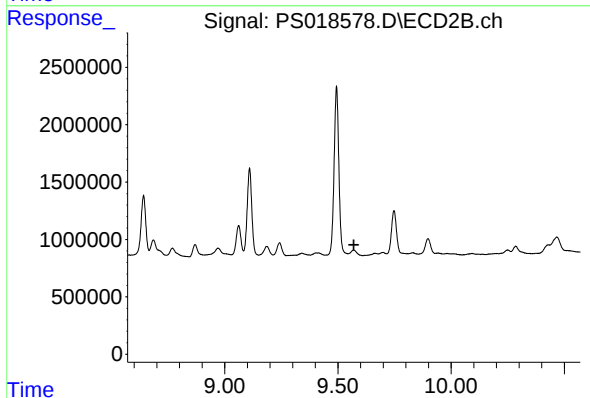


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.570 min
Response: 0
Conc: N.D.

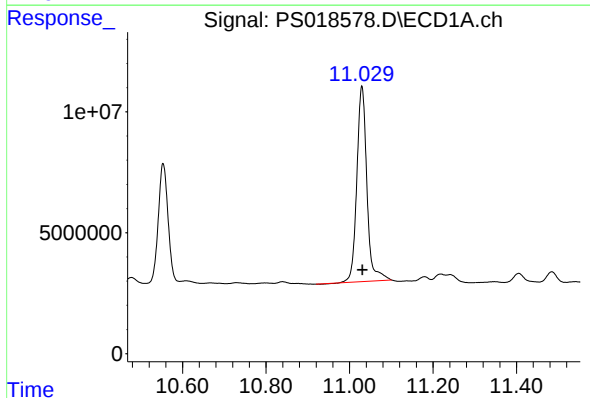

#15 Picloram

R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 135345383
Conc: 6.58 ng/ml

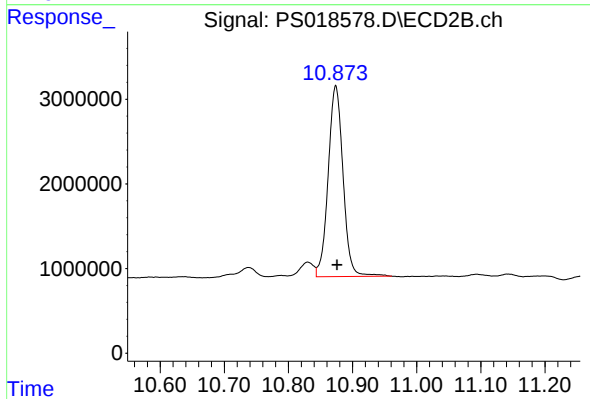

#15 Picloram

R.T.: 10.874 min
Delta R.T.: -0.002 min
Response: 36370229
Conc: 6.84 ng/ml