

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031422\
Data File : PS018567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 14:56
Operator : AJ\MA
Sample : N1831-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
AU-06-03072022

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/15/2022
Supervised By :Ankita Jodhani 03/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 15:20:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.235	6.812	907.5E6	274.4E6	318.895m	389.925

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031422\
Data File : PS018567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 14:56
Operator : AJ\MA
Sample : N1831-01
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_S
ClientSampleId :
AU-06-03072022


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/15/2022
Supervised By : Ankita Jodhani 03/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 15:20:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

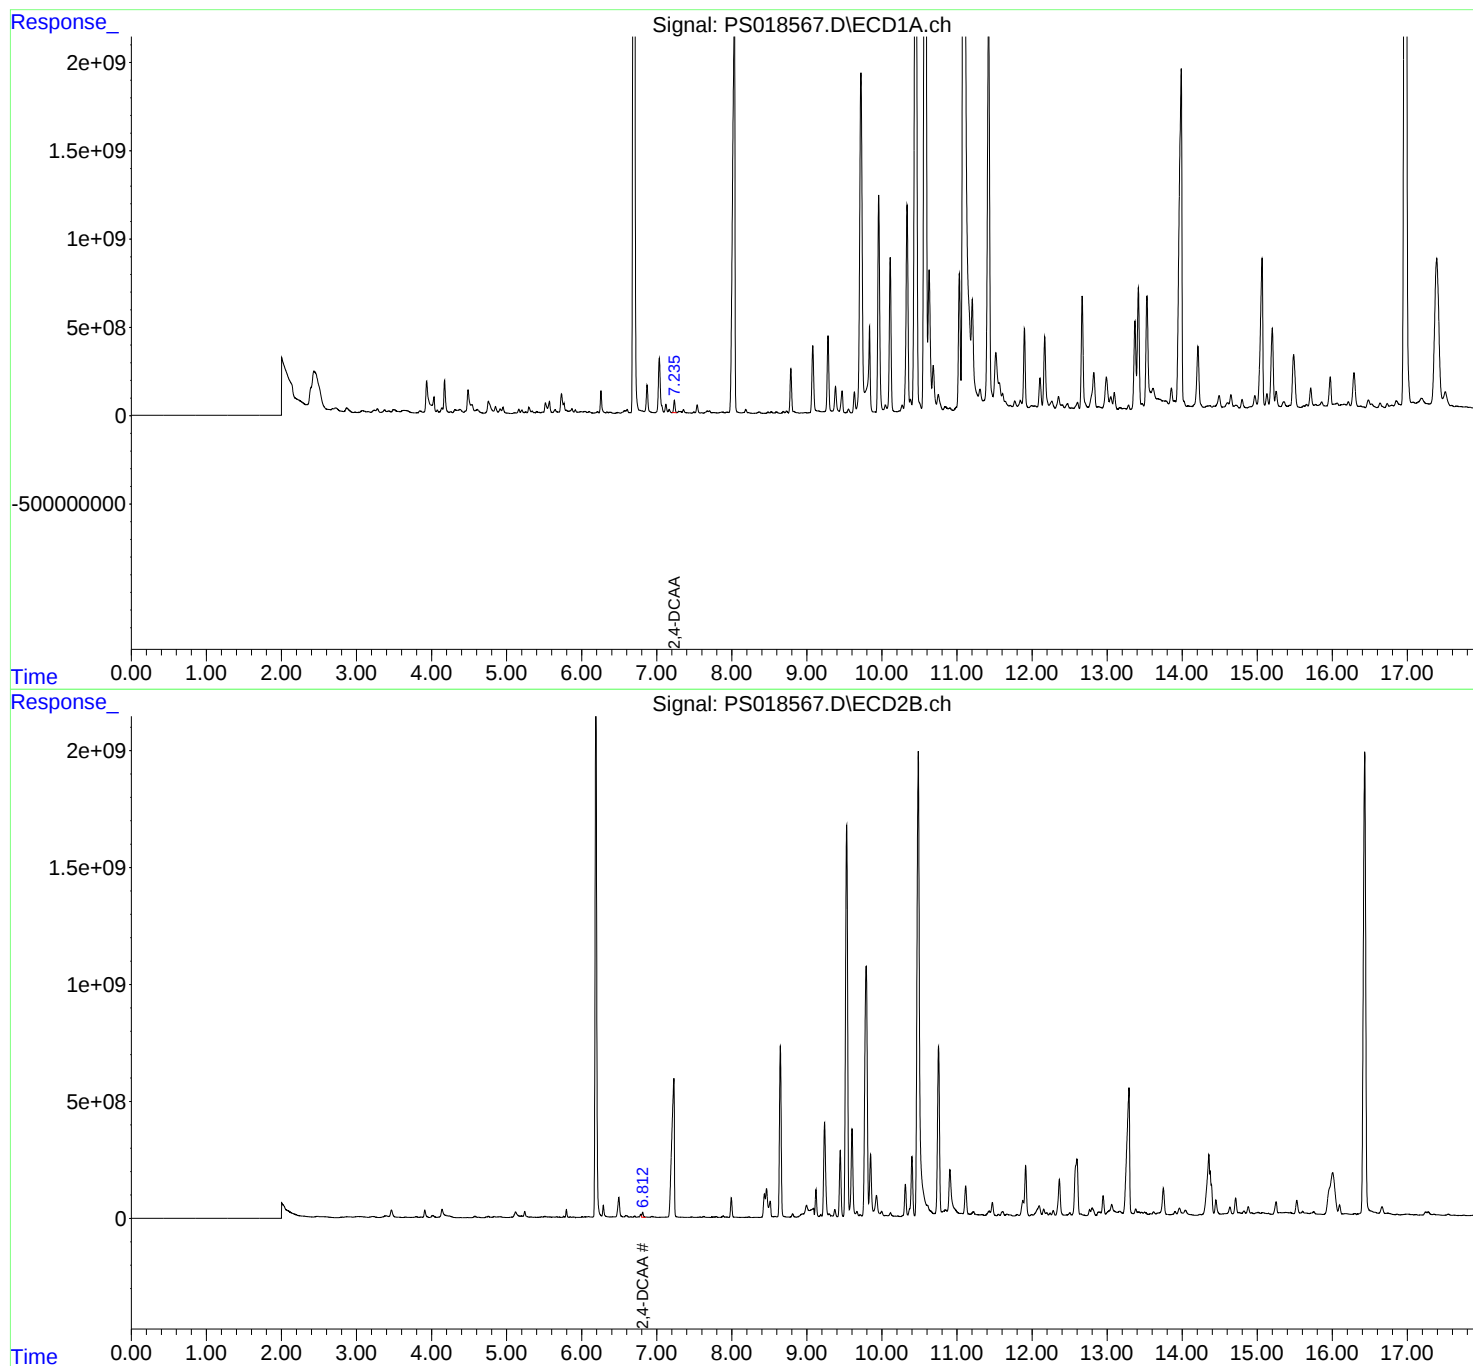

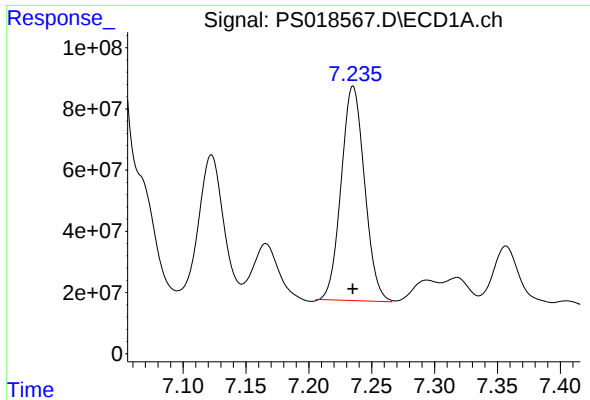


#4 2,4-DCAA

R.T.: 7.235 min
Delta R.T.: 0.000 min
Response: 907548128
Conc: 318.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-03072022

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/15/2022
Supervised By :Ankita Jodhani 03/15/2022

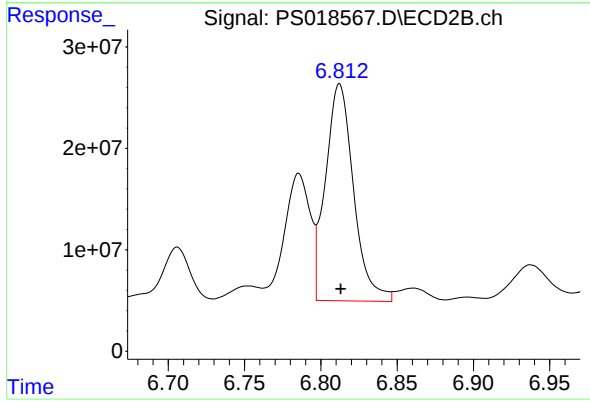

#4 2,4-DCAA

R.T.: 6.812 min
Delta R.T.: 0.000 min
Response: 274372742
Conc: 389.93 ng/ml