

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031521\
 Data File : PL065302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 14:31
 Operator : AR\AJ
 Sample : PB135160BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 02:05:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 01:11:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.884	45263522	55240116	19.212	20.054
28)	SA Decachlor...	7.940	8.894	44039095	36736545	20.437	19.996
Target Compounds							
6)	B beta-BHC	0.000	4.745	0	7821167	N.D.	4.481 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031521\
Data File : PL065302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 14:31
Operator : AR\AJ
Sample : PB135160BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 02:05:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 01:11:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

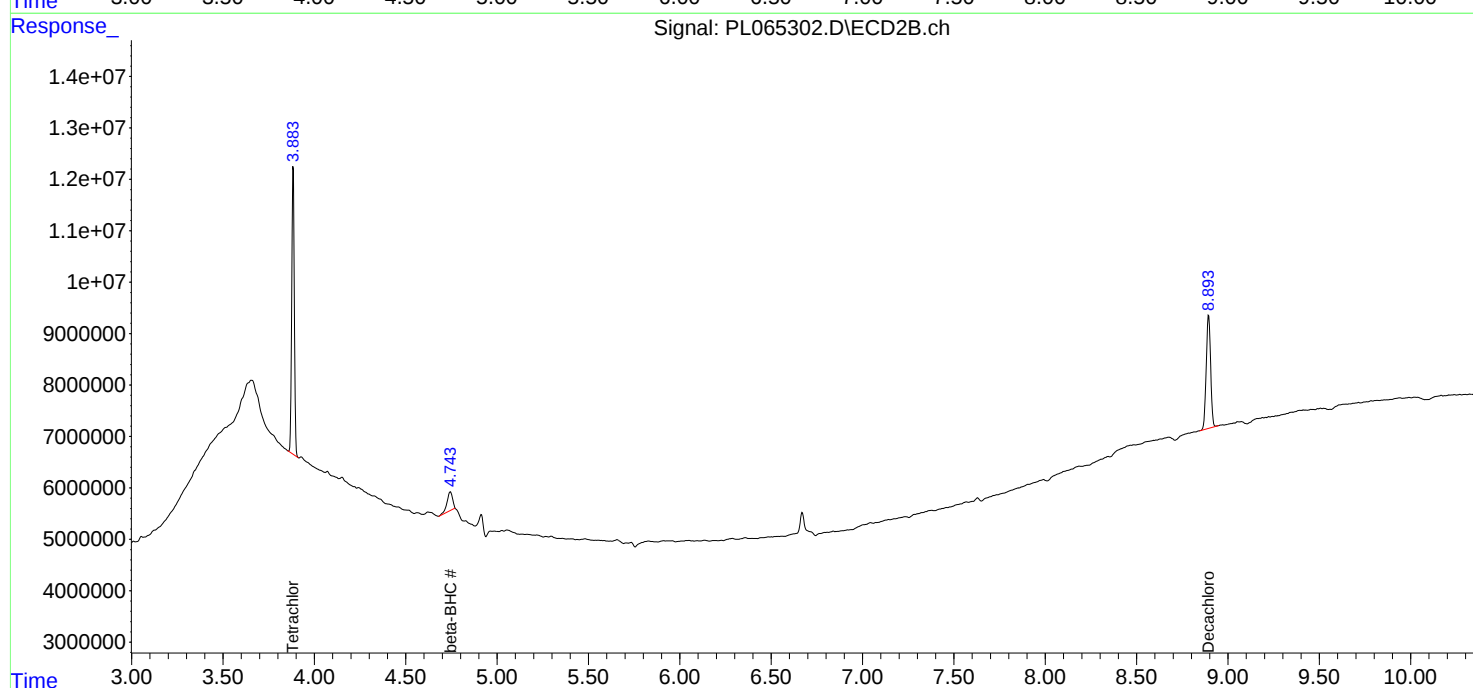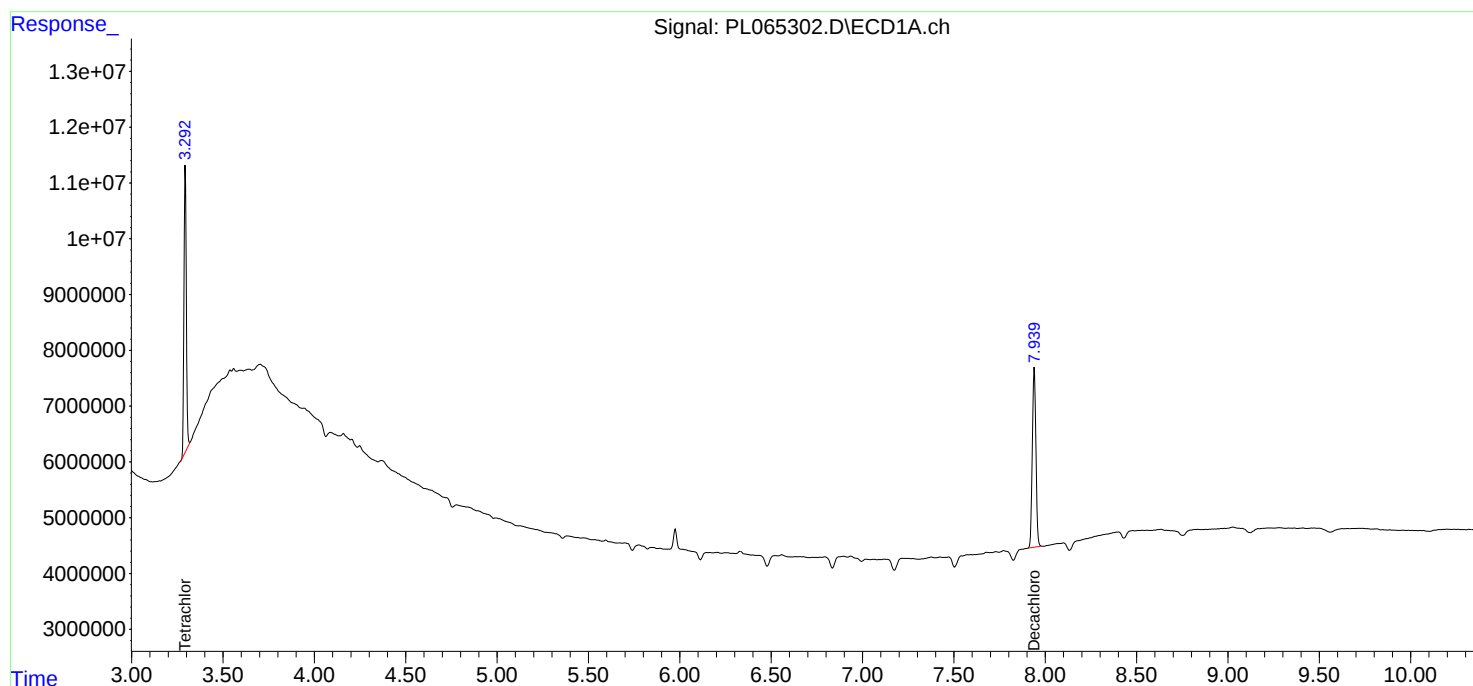


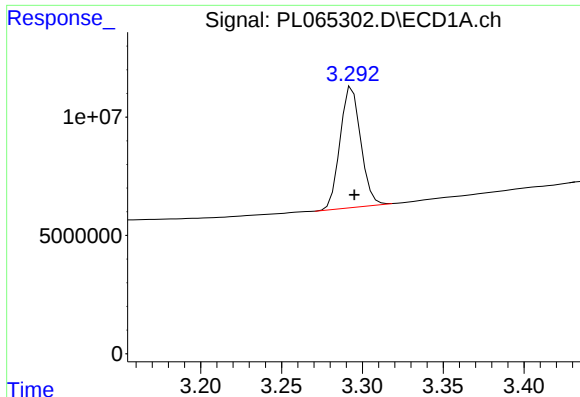

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: -0.001 min
Response: 45263522
Conc: 19.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

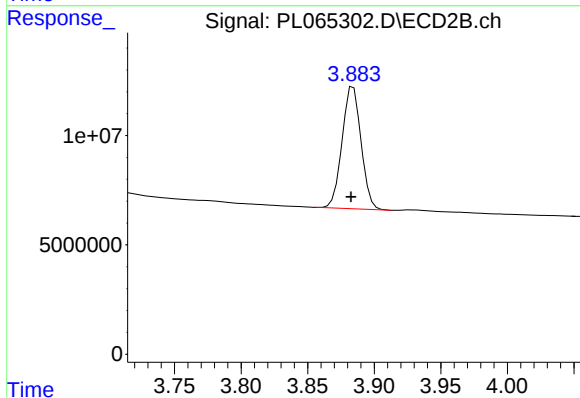


#1 Tetrachloro-m-xylene

R.T.: 3.884 min
Delta R.T.: 0.002 min
Response: 55240116
Conc: 20.05 ng/ml

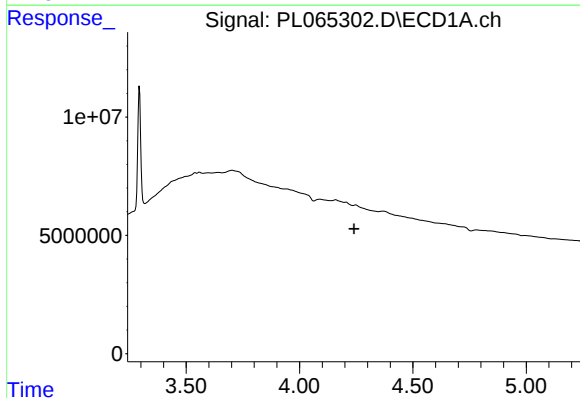


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.241 min
Response: 0
Conc: N.D.

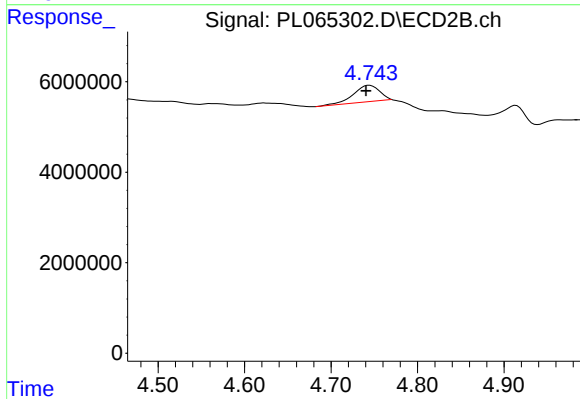

#6 beta-BHC


R.T.: 4.745 min
Delta R.T.: 0.004 min
Response: 7821167
Conc: 4.48 ng/ml

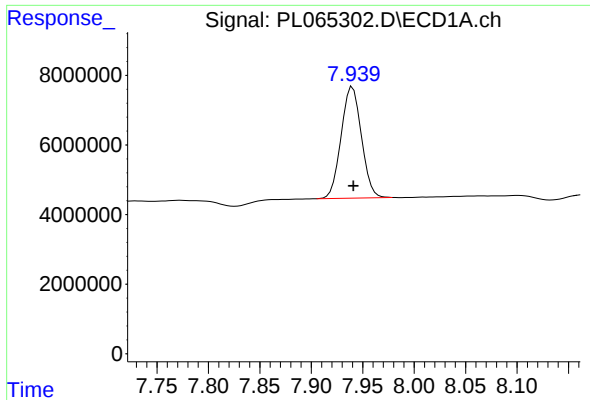

#28 Decachlorobiphenyl

R.T.: 7.940 min
Delta R.T.: 0.000 min
Response: 44039095
Conc: 20.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

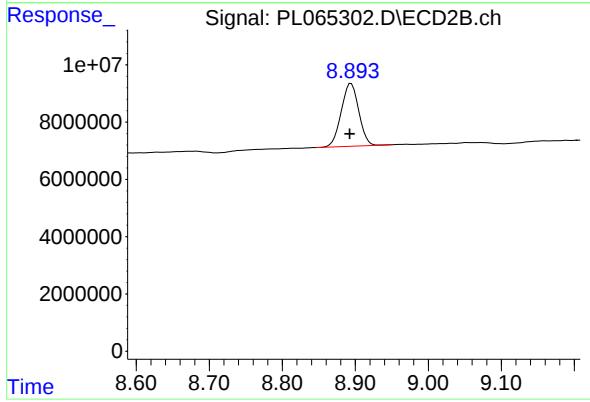

#28 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: 0.002 min
Response: 36736545
Conc: 20.00 ng/ml