

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031521\
 Data File : PS014241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 09:02
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 11:15:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Sat Mar 06 03:17:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) T	DICAMBA	7.392	7.062	3503091	11176151	<MDL	6.913 #
6) T	MCP	7.585	7.185	-2520677	2914255	N.D.	2.199
7) T	MCPA	7.672	0.000	6815997	0	1.572	N.D. #
10) T	Pentachlo...	8.624	8.409	7942259	2043397	<MDL	<MDL #
11) T	2,4,5-TP ...	9.174	8.772	8222492	2897967	1.440	1.306
12) T	2,4,5-T	9.472	9.163	7720203	3389836	1.288	1.566
14) T	DINOSEB	11.163	9.986	7920172	4723095	1.712	3.001 #
15) T	Picloram	11.014	10.997	51315441	32113659	6.429	9.728 #
16) T	DCPA	11.432	10.911	12858104	6578692	1.503	1.960 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031521\
Data File : PS014241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 09:02
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 11:15:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Sat Mar 06 03:17:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

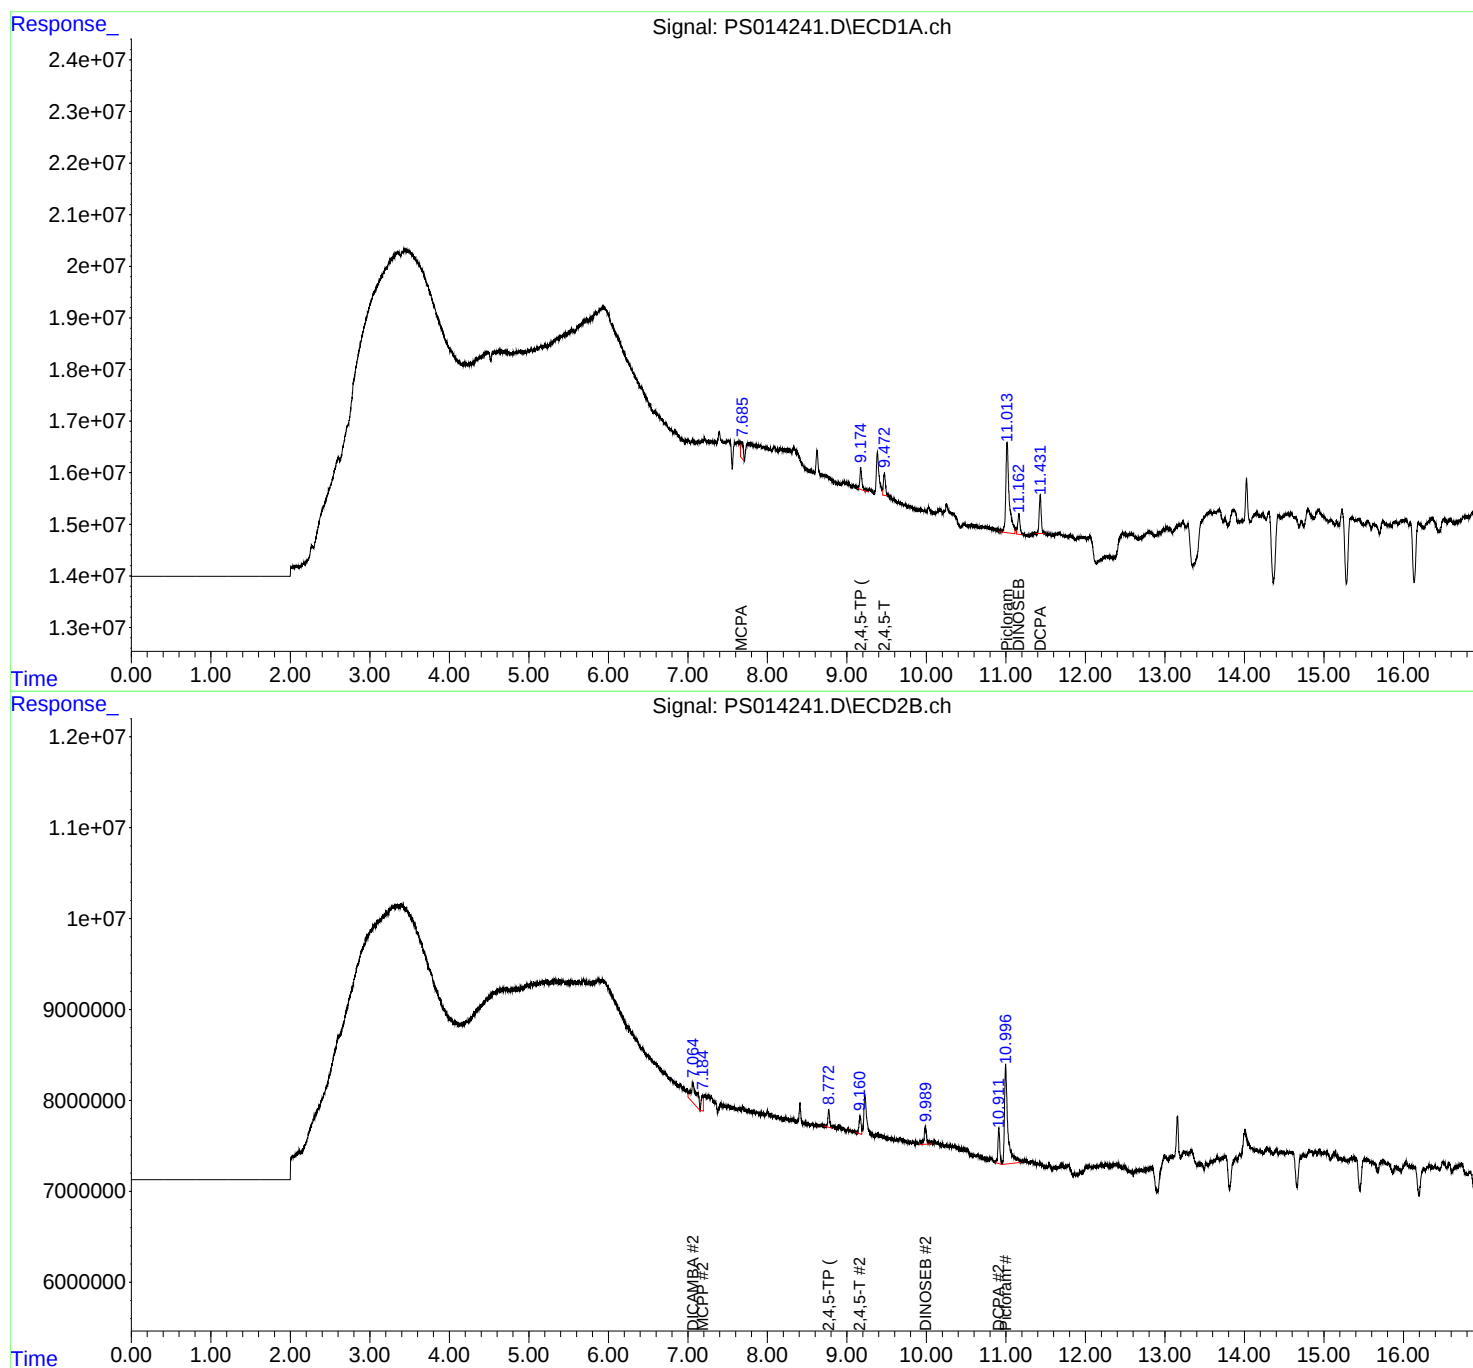


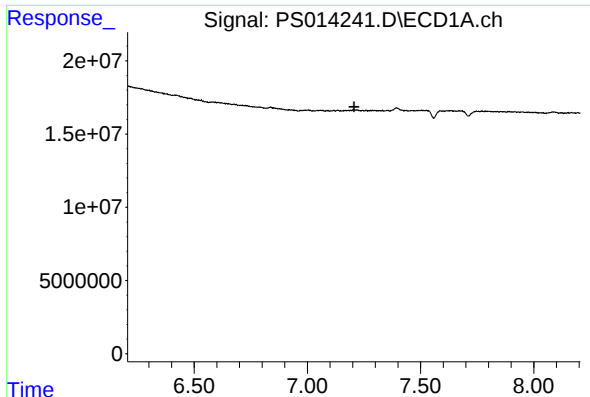

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

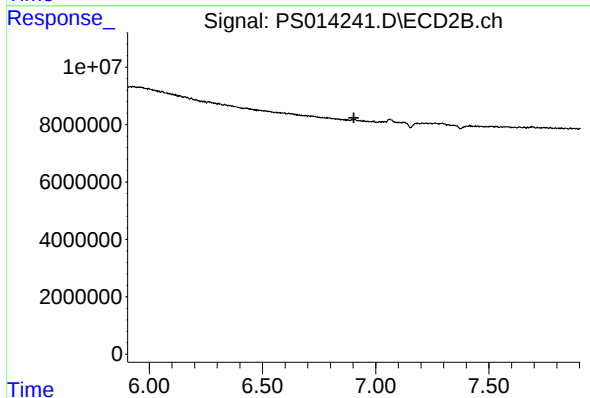


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.904 min
Response: 0
Conc: N.D.

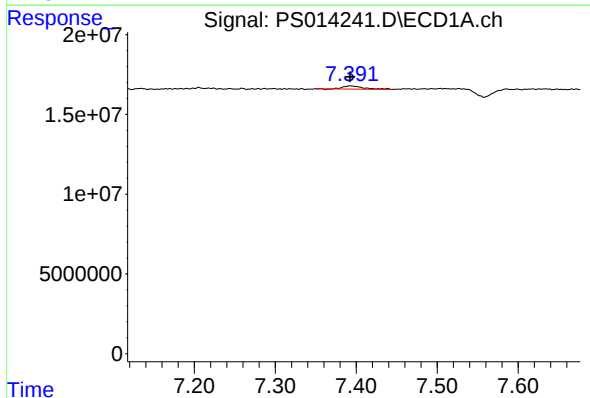


#5 DICAMBA

R.T.: 7.392 min
Delta R.T.: 0.000 min
Response: 3503091
Conc: N.D.

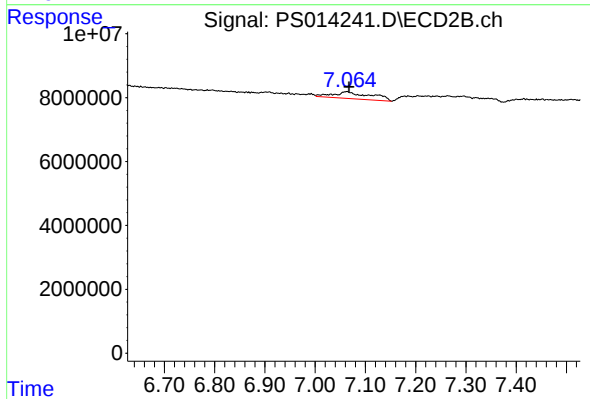

#5 DICAMBA


R.T.: 7.062 min
Delta R.T.: -0.006 min
Response: 11176151
Conc: 6.91 ng/ml

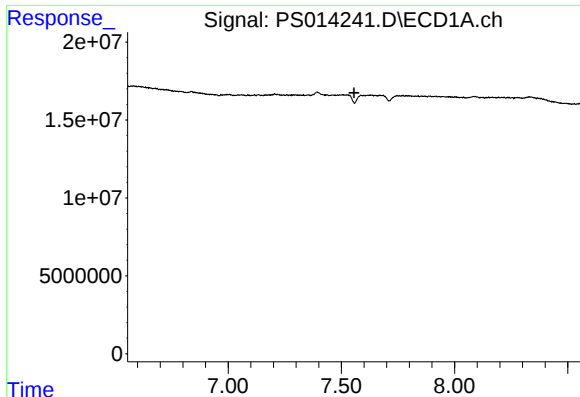

#6 MCPP


R.T.: 7.585 min
Delta R.T.: 0.030 min
Response: -2520677
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

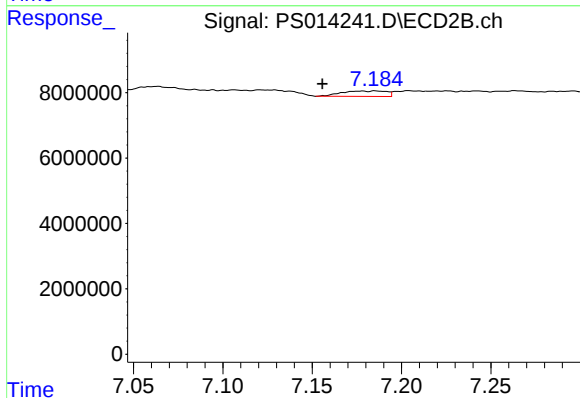


#6 MCPP

R.T.: 7.185 min
Delta R.T.: 0.030 min
Response: 2914255
Conc: 2.20 ug/ml

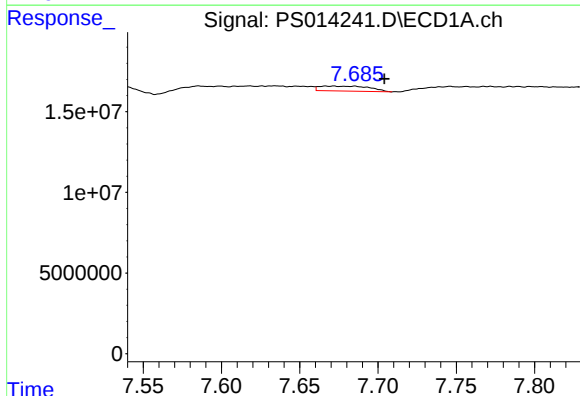


#7 MCPA

R.T.: 7.672 min
Delta R.T.: -0.032 min
Response: 6815997
Conc: 1.57 ug/ml

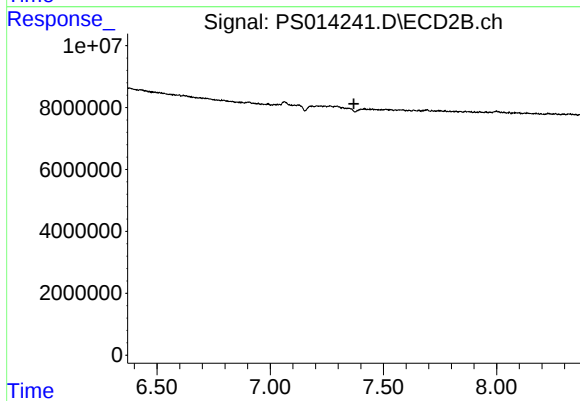

#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

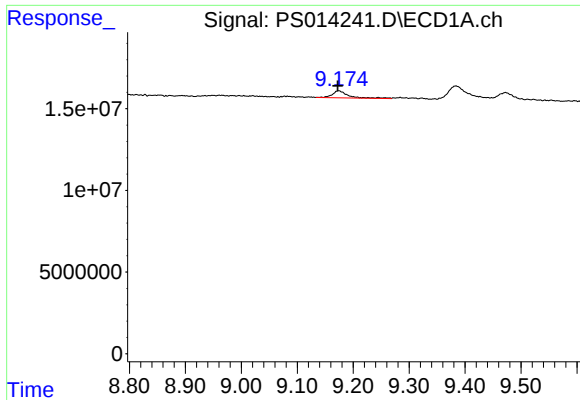

#11 2,4,5-TP (SILVEX)


R.T.: 9.174 min

Delta R.T.: 0.002 min

Response: 8222492

Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

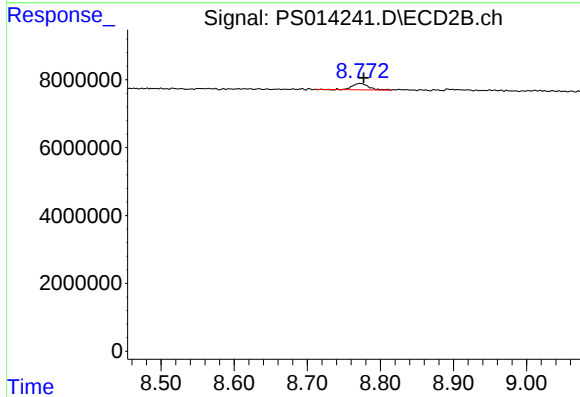


#11 2,4,5-TP (SILVEX)

R.T.: 8.772 min

Delta R.T.: -0.005 min

Response: 2897967

Conc: 1.31 ng/ml

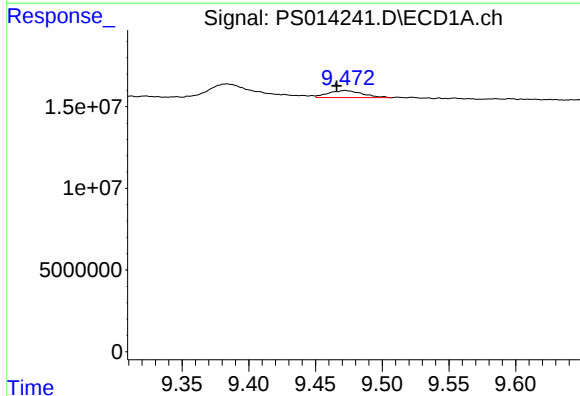


#12 2,4,5-T

R.T.: 9.472 min

Delta R.T.: 0.006 min

Response: 7720203

Conc: 1.29 ng/ml

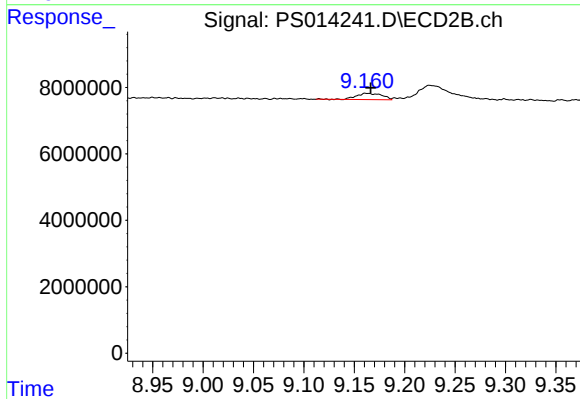


#12 2,4,5-T

R.T.: 9.163 min

Delta R.T.: -0.003 min

Response: 3389836


Conc: 1.57 ng/ml

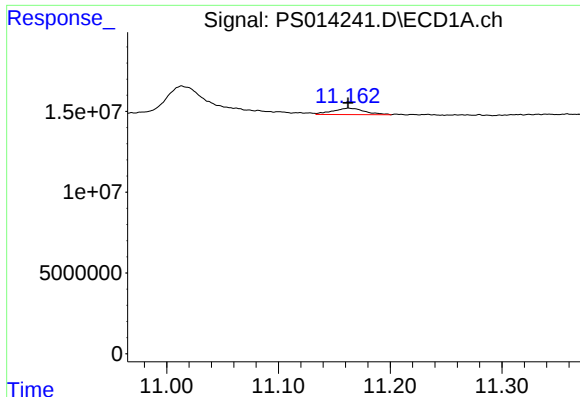

#14 DINOSEB


R.T.: 11.163 min
Delta R.T.: 0.000 min
Response: 7920172
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

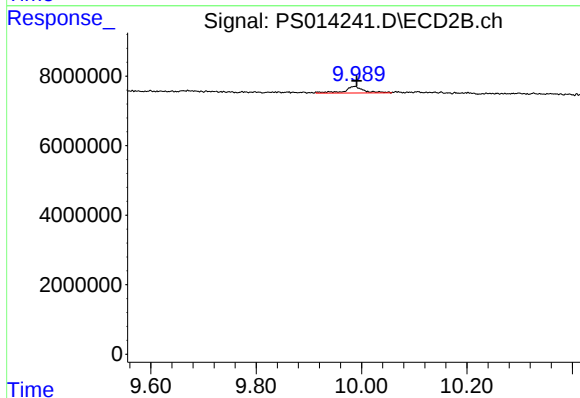


#14 DINOSEB

R.T.: 9.986 min
Delta R.T.: -0.005 min
Response: 4723095
Conc: 3.00 ng/ml

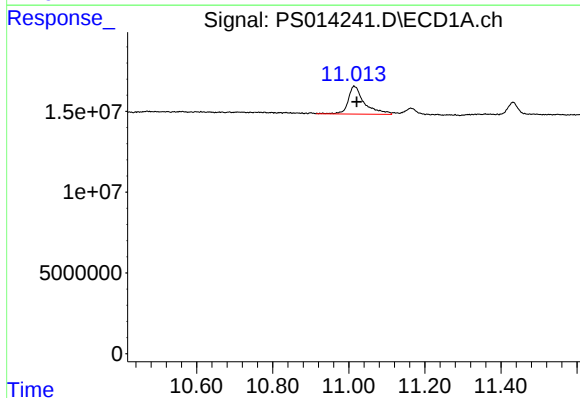


#15 Picloram

R.T.: 11.014 min
Delta R.T.: -0.007 min
Response: 51315441
Conc: 6.43 ng/ml

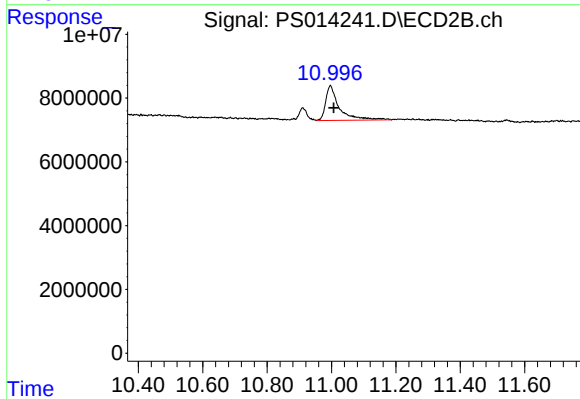

#15 Picloram


R.T.: 10.997 min
Delta R.T.: -0.011 min
Response: 32113659
Conc: 9.73 ng/ml

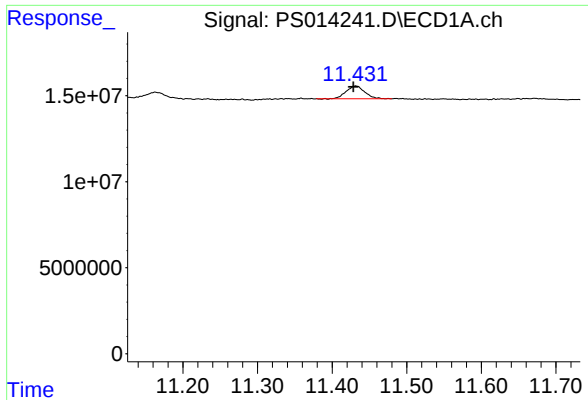

#16 DCPA

R.T.: 11.432 min
Delta R.T.: 0.003 min
Response: 12858104
Conc: 1.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

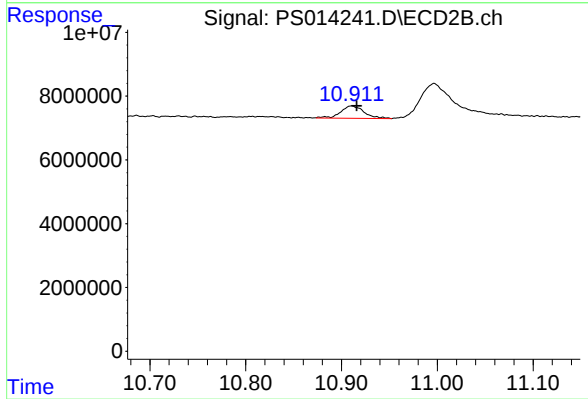

#16 DCPA

R.T.: 10.911 min
Delta R.T.: -0.005 min
Response: 6578692
Conc: 1.96 ng/ml