

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031521\
 Data File : PS014249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 14:22
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 15:27:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Sat Mar 06 03:17:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.207	6.905	458.4E6	198.2E6	455.210	520.960
Target Compounds							
2) T	3,5-DICHL...	6.468f	0.000	4148045	0	3.000	N.D. #
5) T	DICAMBA	0.000	7.071	0	3197133	N.D.	1.977
6) T	MCP	0.000	7.140	0	4270028	N.D.	3.222
10) T	Pentachlo...	0.000	8.423	0	1088200	N.D.	<MDL
15) T	Picloram	0.000	11.005	0	429051	N.D.	<MDL
16) T	DCPA	11.433	10.918	4228820	1930223	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031521\
Data File : PS014249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 14:22
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 15:27:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Sat Mar 06 03:17:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

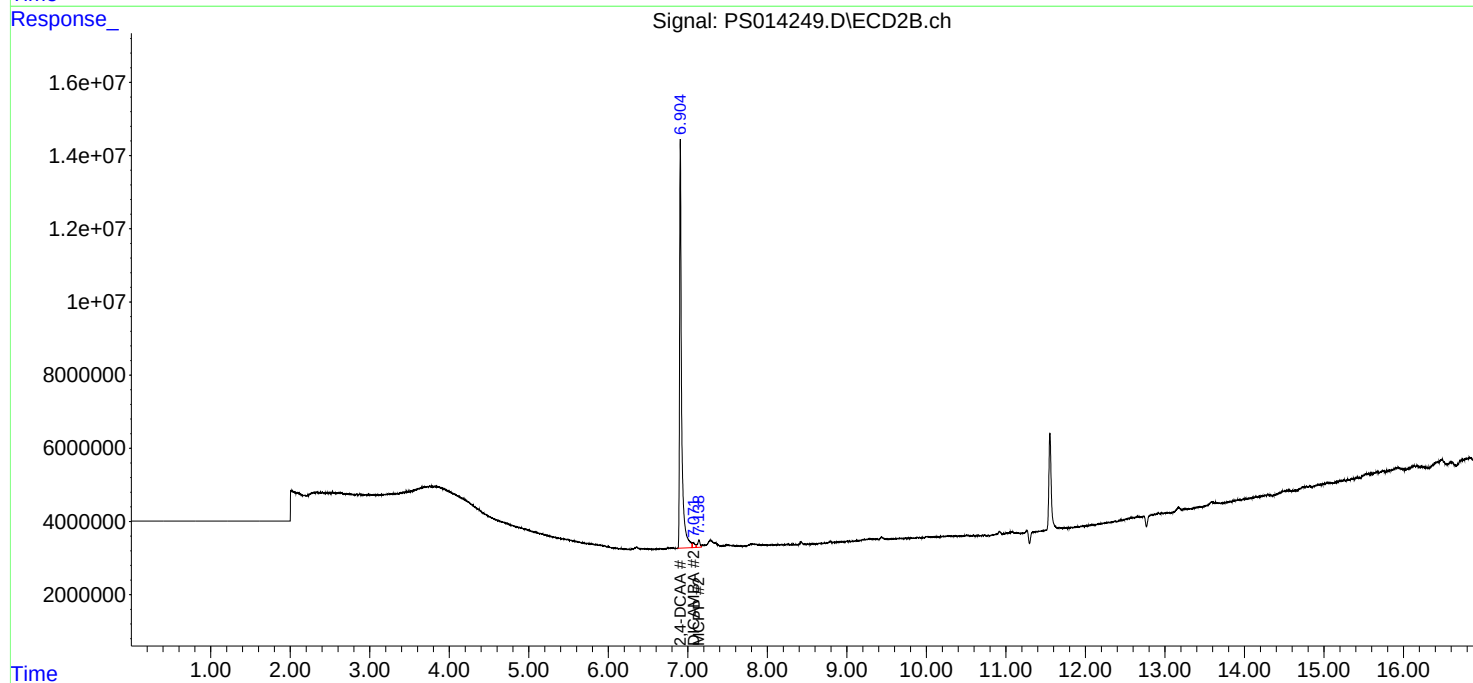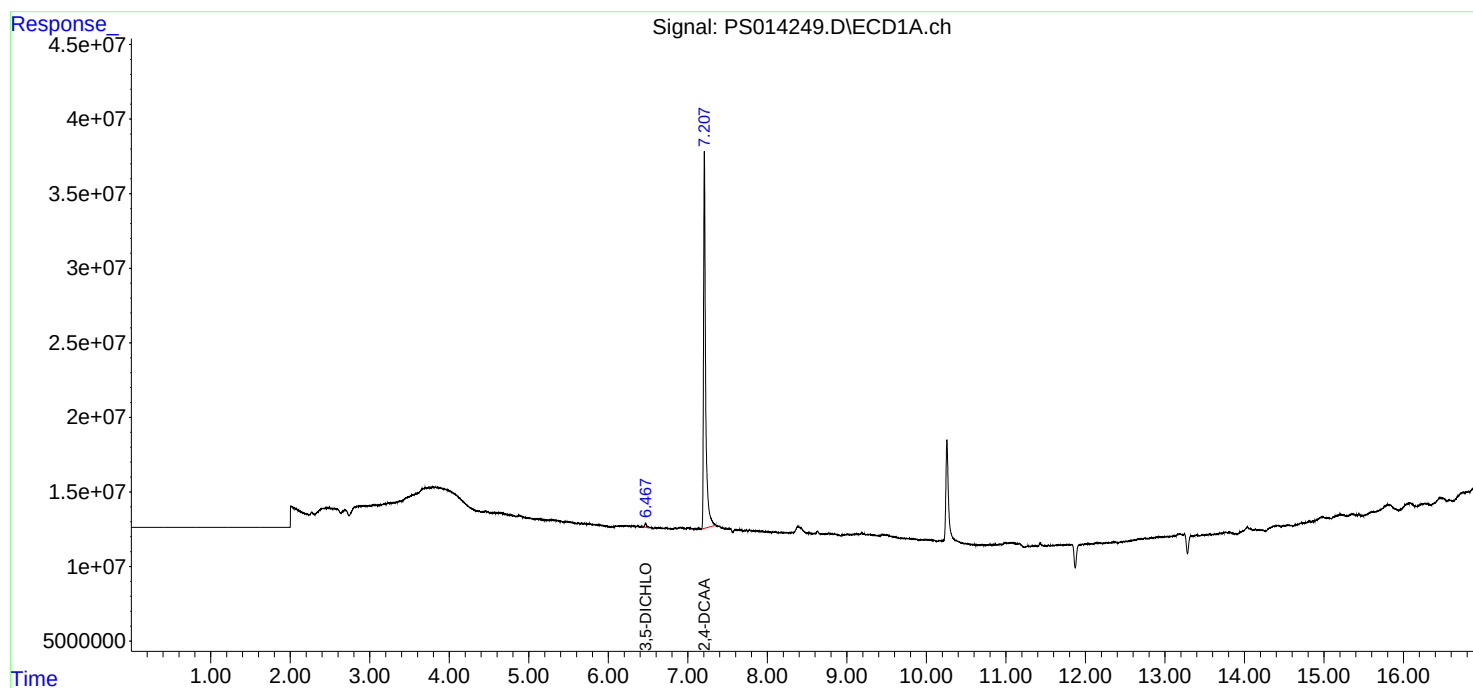


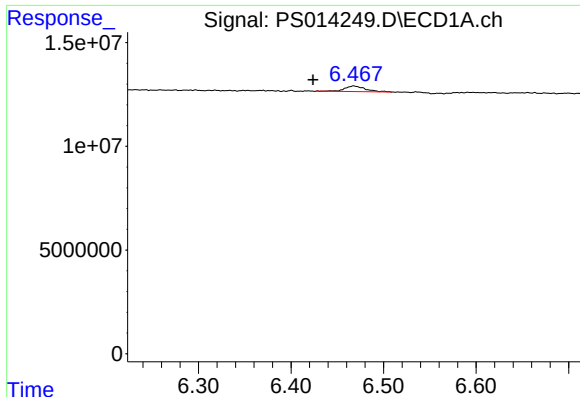

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.468 min
Delta R.T.: 0.044 min
Response: 4148045
Conc: 3.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

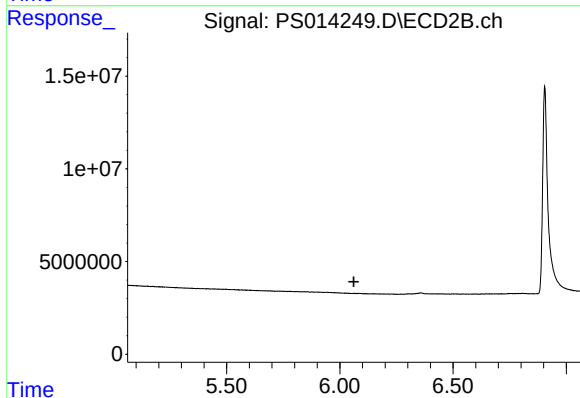


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.062 min
Response: 0
Conc: N.D.

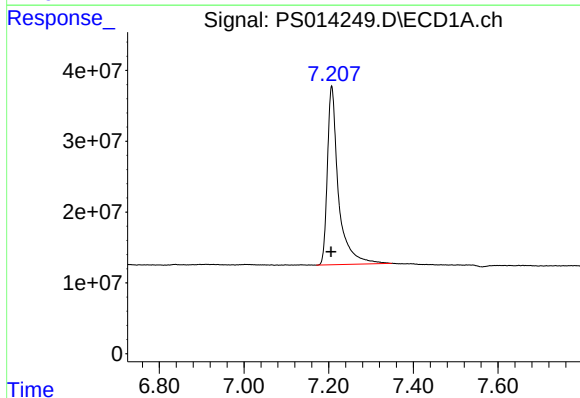


#4 2,4-DCAA

R.T.: 7.207 min
Delta R.T.: 0.002 min
Response: 458384678
Conc: 455.21 ng/ml

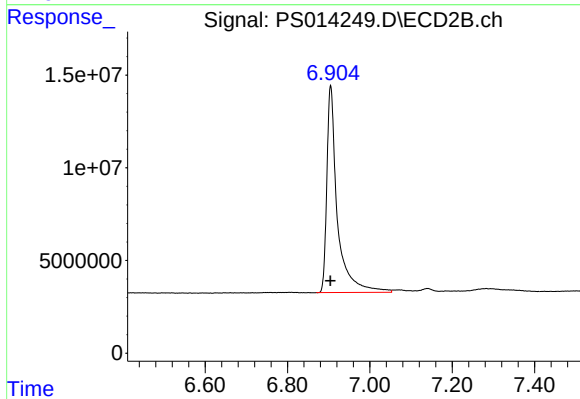

#4 2,4-DCAA


R.T.: 6.905 min
Delta R.T.: 0.000 min
Response: 198197724
Conc: 520.96 ng/ml

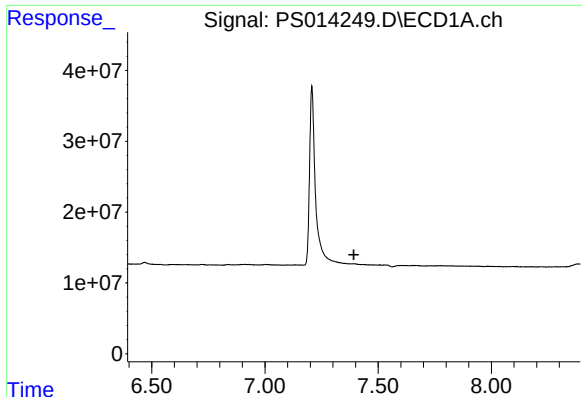

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

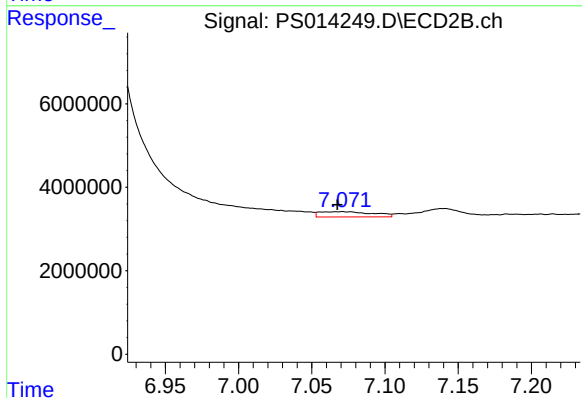


#5 DICAMBA

R.T.: 7.071 min
Delta R.T.: 0.003 min
Response: 3197133
Conc: 1.98 ng/ml

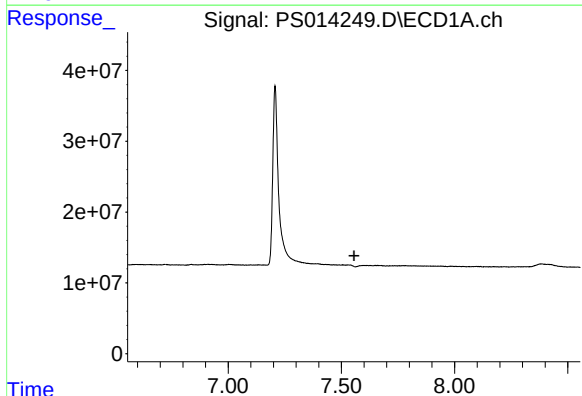

#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.556 min
Response: 0
Conc: N.D.

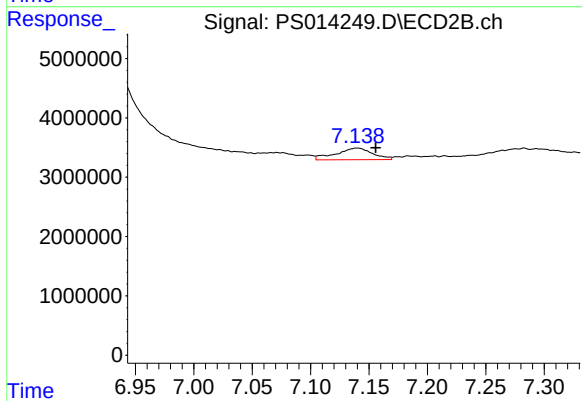

#6 MCP

R.T.: 7.140 min
Delta R.T.: -0.016 min
Response: 4270028
Conc: 3.22 ug/ml