

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031522\
 Data File : PS018586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 09:15
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 12:46:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) T	4-Nitroph...	7.025	6.476f	-3659743	2889289	N.D. 7.112
8) T	DICHLORPROP	0.000	7.623	0	4843359	N.D. 6.118
9) T	2,4-D	8.415f	0.000	6294736	0	1.879 N.D. #
10) T	Pentachlo...	8.664	0.000	3225809	0	<MDL N.D. #
11) T	2,4,5-TP ...	9.216	8.641f	7972018	7388200	<MDL 1.694 #
12) T	2,4,5-T	9.498	9.110f	6774007	6280451	<MDL 1.516 #
13) T	2,4-DB	10.030	0.000	5757489	0	2.105 N.D. #
14) T	DINOSEB	11.245	9.900	11379454	1669102	1.064 <MDL #
15) T	Picloram	11.031	10.875	124.9E6	46871679	6.075 8.817 #
16) T	DCPA	11.487	10.875f	8894722	46871679	<MDL 8.912 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031522\
Data File : PS018586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 09:15
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 12:46:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

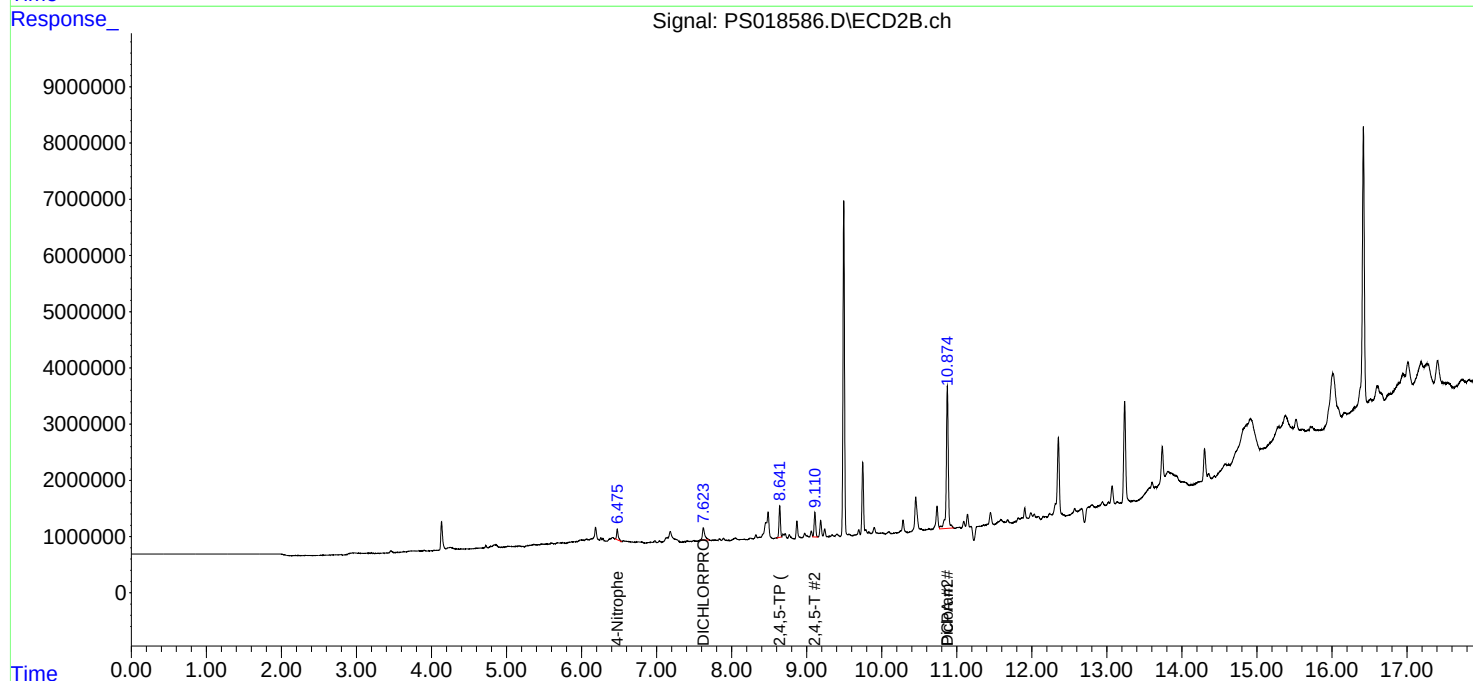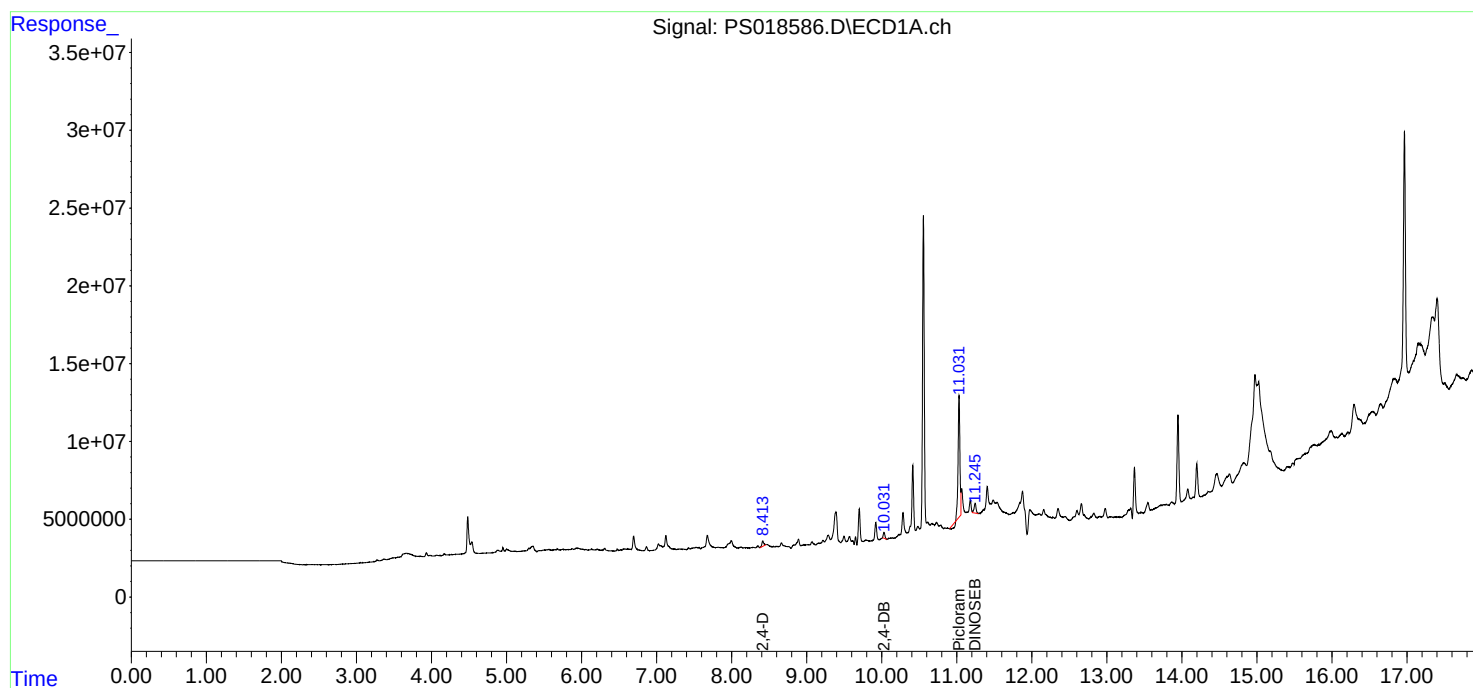


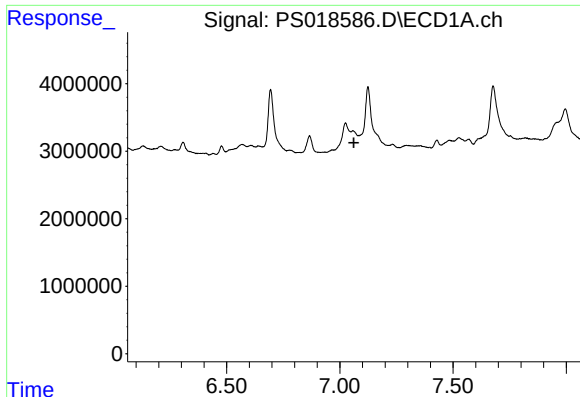

#3 4-Nitrophenol


R.T.: 7.025 min
Delta R.T.: -0.037 min
Response: -3659743
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

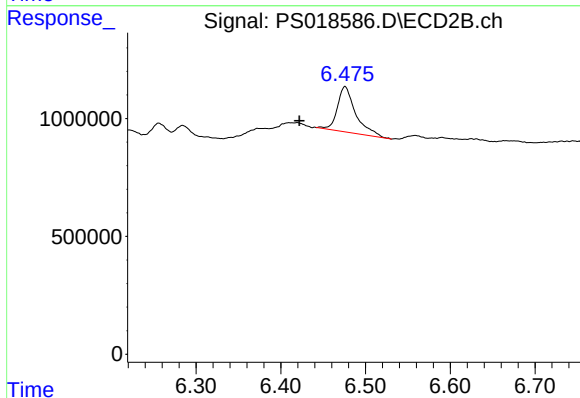


#3 4-Nitrophenol

R.T.: 6.476 min
Delta R.T.: 0.054 min
Response: 2889289
Conc: 7.11 ng/ml

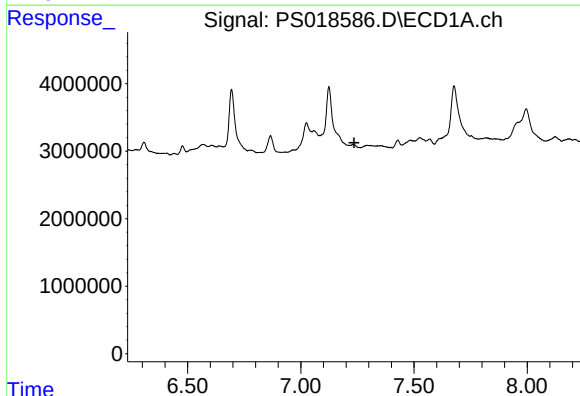


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.235 min
Response: 0
Conc: N.D.

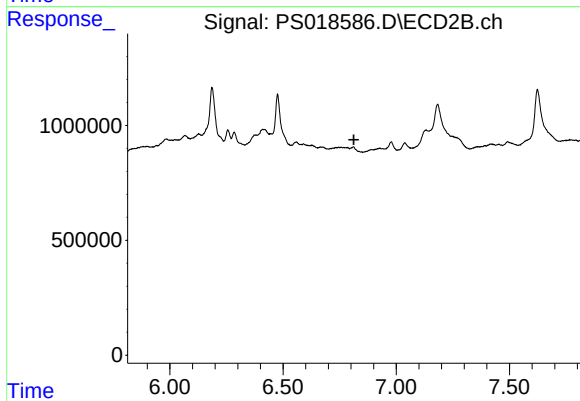

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.813 min
Response: 0
Conc: N.D.

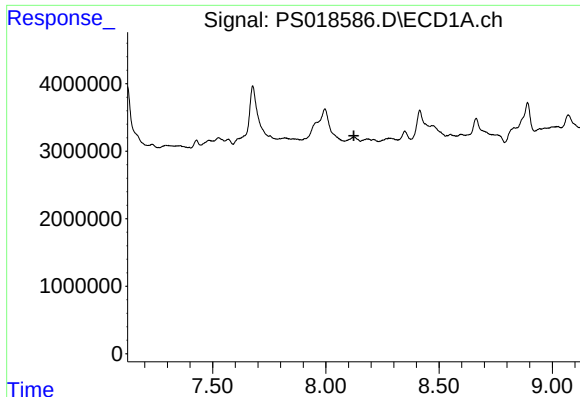

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

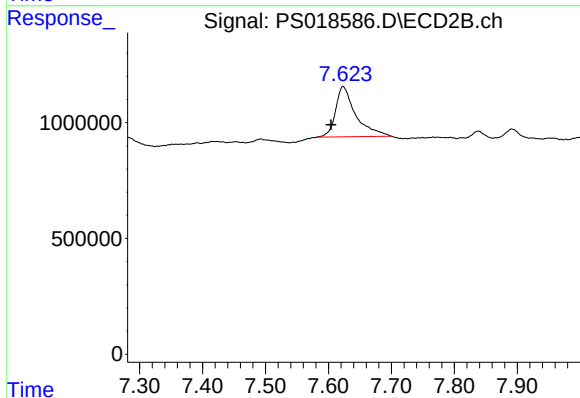


#8 DICHLORPROP

R.T.: 7.623 min
Delta R.T.: 0.019 min
Response: 4843359
Conc: 6.12 ng/ml

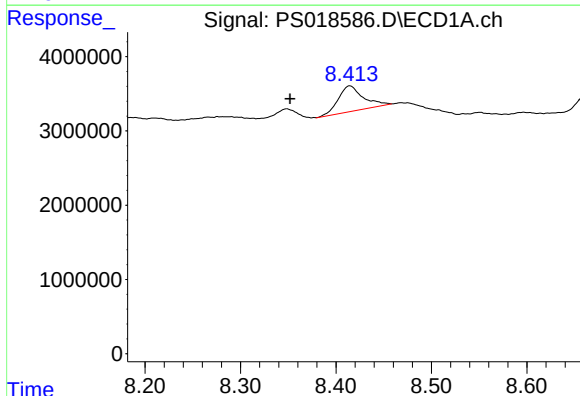


#9 2,4-D

R.T.: 8.415 min
Delta R.T.: 0.063 min
Response: 6294736
Conc: 1.88 ng/ml

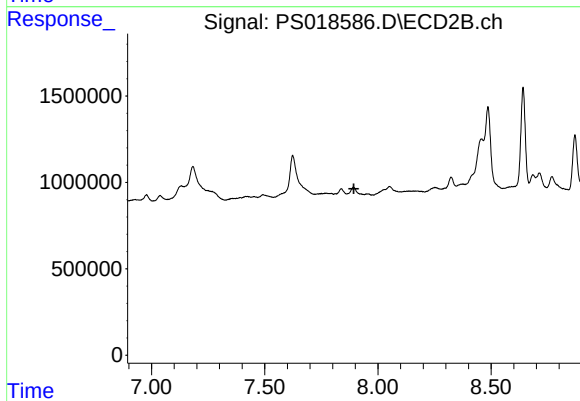

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

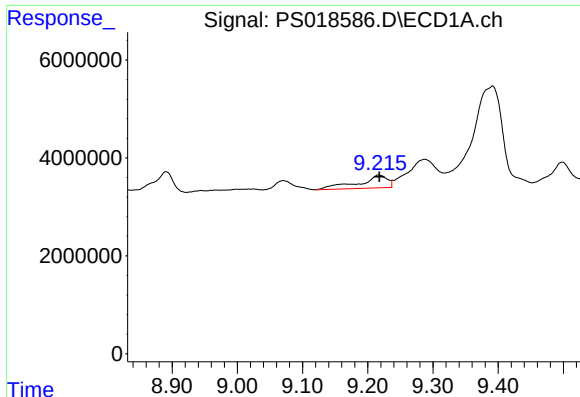

#11 2,4,5-TP (SILVEX)


R.T.: 9.216 min
Delta R.T.: -0.002 min
Response: 7972018
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

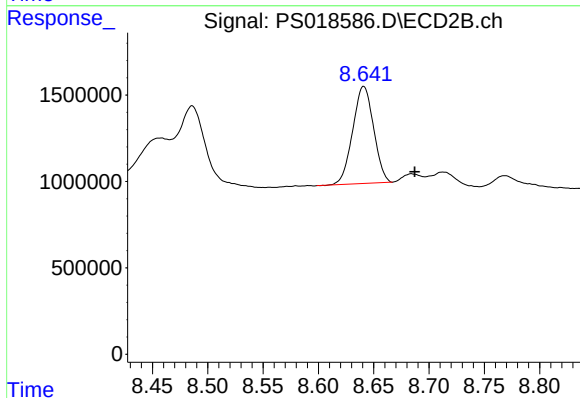


#11 2,4,5-TP (SILVEX)

R.T.: 8.641 min
Delta R.T.: -0.046 min
Response: 7388200
Conc: 1.69 ng/ml

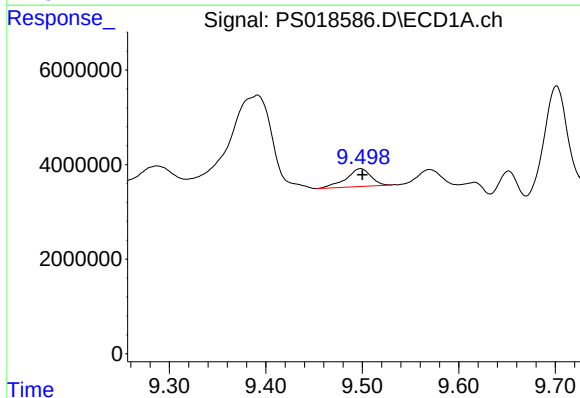


#12 2,4,5-T

R.T.: 9.498 min
Delta R.T.: -0.002 min
Response: 6774007
Conc: N.D.

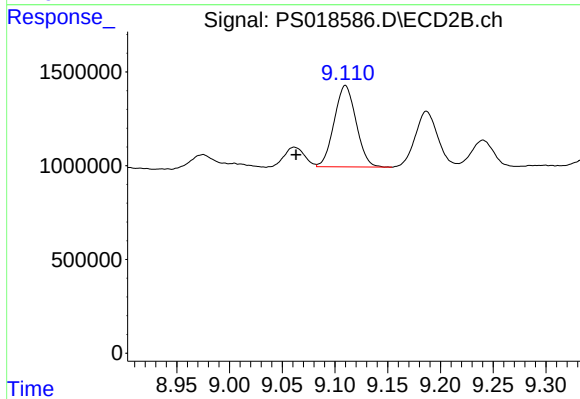

#12 2,4,5-T


R.T.: 9.110 min
Delta R.T.: 0.047 min
Response: 6280451
Conc: 1.52 ng/ml

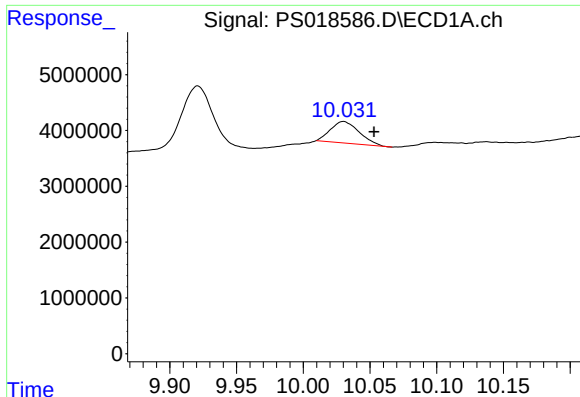

#13 2,4-DB


R.T.: 10.030 min
Delta R.T.: -0.023 min
Response: 5757489
Conc: 2.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

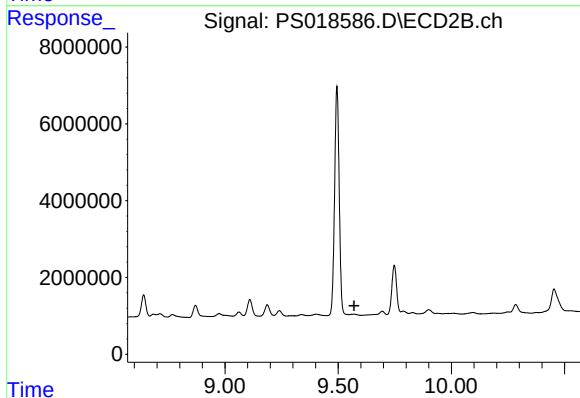


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.570 min
Response: 0
Conc: N.D.

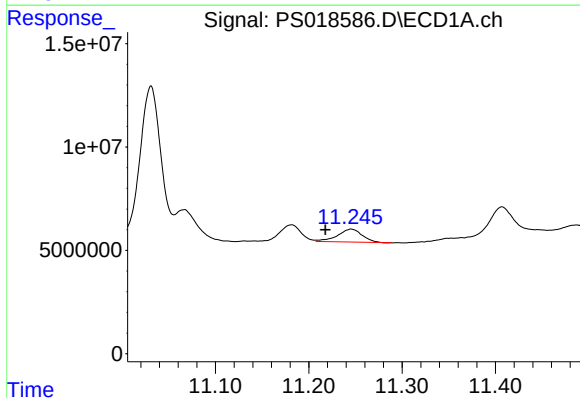


#14 DINOSEB

R.T.: 11.245 min
Delta R.T.: 0.027 min
Response: 11379454
Conc: 1.06 ng/ml

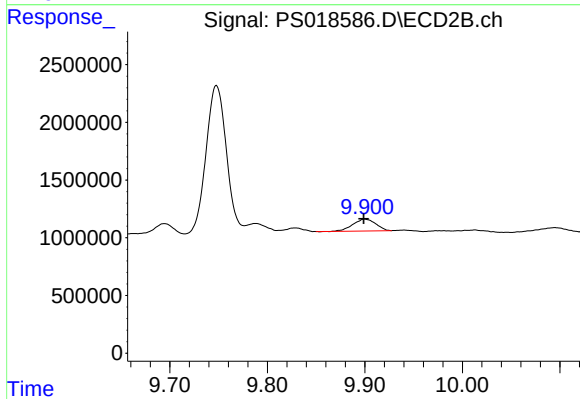

#14 DINOSEB


R.T.: 9.900 min
Delta R.T.: 0.000 min
Response: 1669102
Conc: N.D.

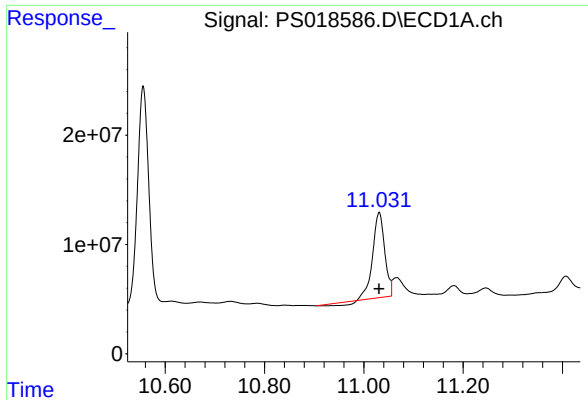

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 124870221
Conc: 6.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

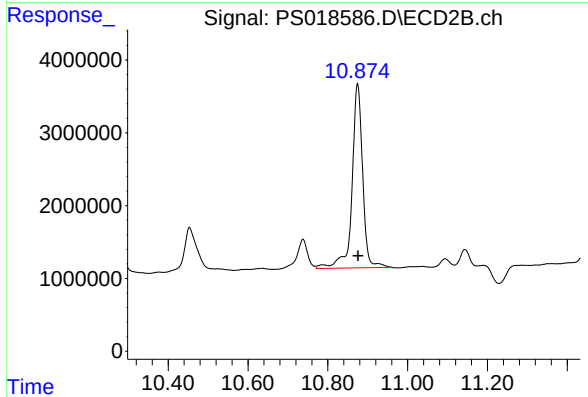


#15 Picloram

R.T.: 10.875 min
Delta R.T.: -0.001 min
Response: 46871679
Conc: 8.82 ng/ml

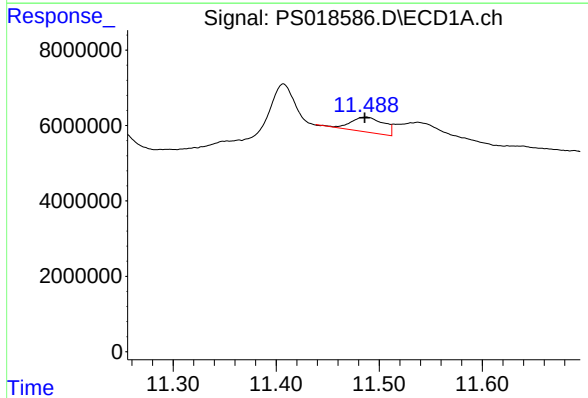

#16 DCPA

R.T.: 11.487 min
Delta R.T.: 0.001 min
Response: 8894722
Conc: N.D.

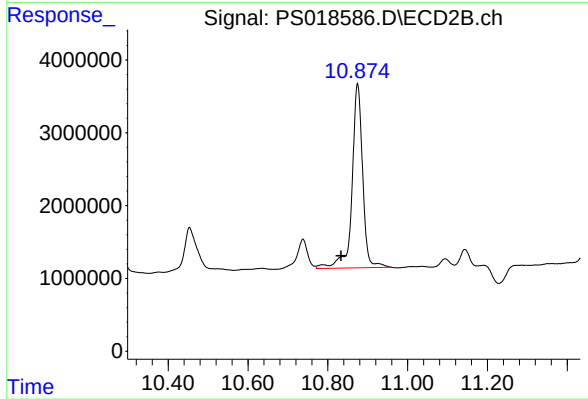

#16 DCPA

R.T.: 10.875 min
Delta R.T.: 0.042 min
Response: 46871679
Conc: 8.91 ng/ml