

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031522\
 Data File : PS018591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 11:15
 Operator : AJ\MA
 Sample : PB143207BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 12:47:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.811	1241.5E6	351.6E6	436.240	499.744
Target Compounds							
3) T	4-Nitroph...	7.124f	6.476f	5222988	3135360	3.031	7.717 #
8) T	DICHLORPROP	0.000	7.625	0	16675525	N.D.	21.065
9) T	2,4-D	8.421f	0.000	8207330	0	2.449	N.D. #
10) T	Pentachlo...	8.661	8.323	9258408	2136398	<MDL	<MDL #
11) T	2,4,5-TP ...	9.214	8.641f	5573412	4982234	<MDL	1.142 #
12) T	2,4,5-T	9.496	9.060	10855430	2164090	<MDL	<MDL #
13) T	2,4-DB	10.030	0.000	4681038	0	1.711	N.D. #
14) T	DINOSEB	11.245	9.898	10619483	1774718	<MDL	<MDL #
15) T	Picloram	11.029	10.873	111.6E6	34407451	5.430	6.472
16) T	DCPA	11.484	10.830	4213913	2473215	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031522\
Data File : PS018591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 11:15
Operator : AJ\MA
Sample : PB143207BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 12:47:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

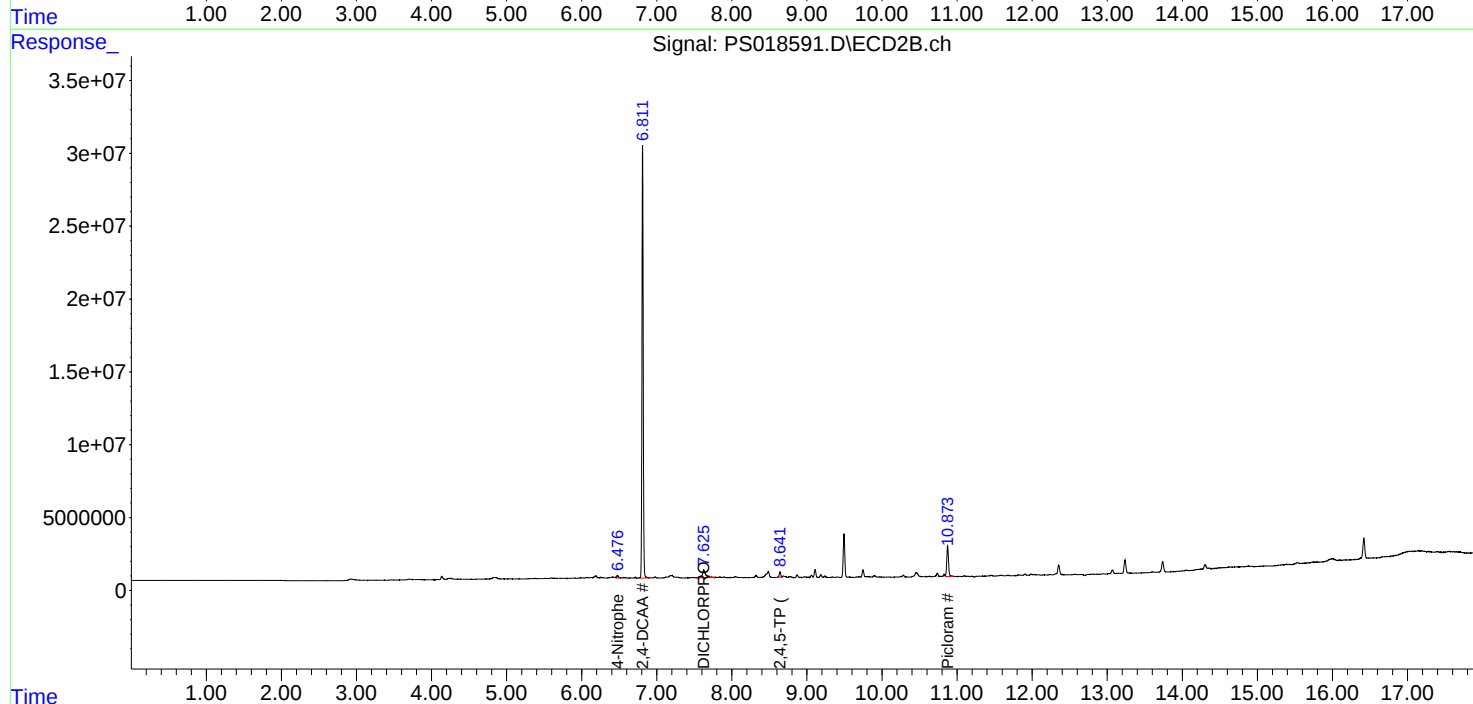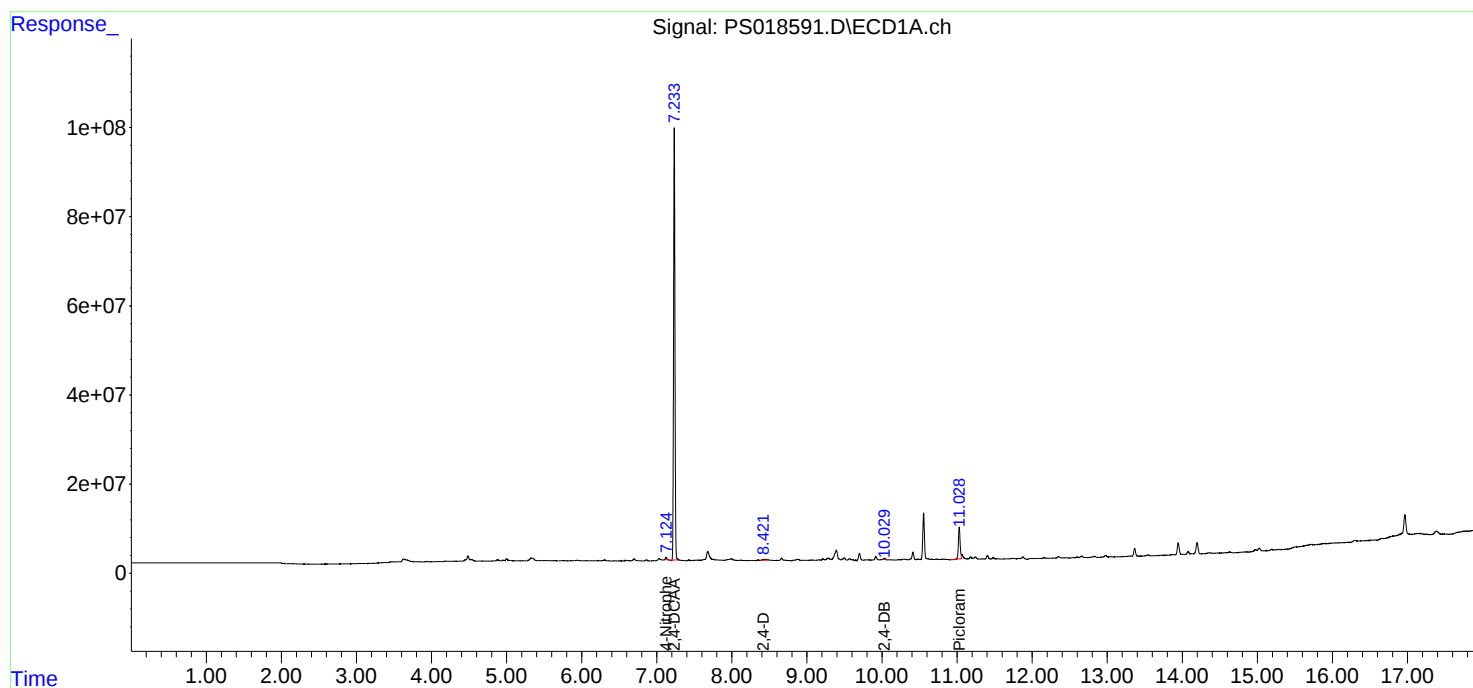


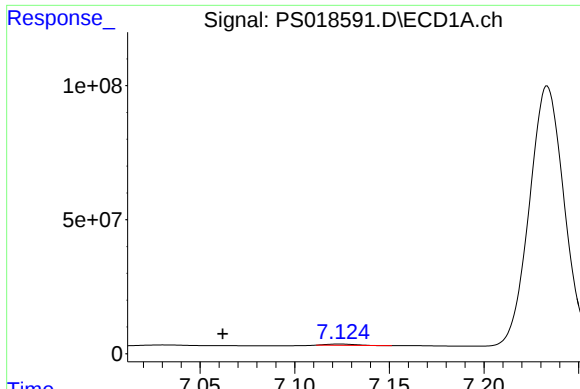

#3 4-Nitrophenol


R.T.: 7.124 min
Delta R.T.: 0.062 min
Response: 5222988
Conc: 3.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

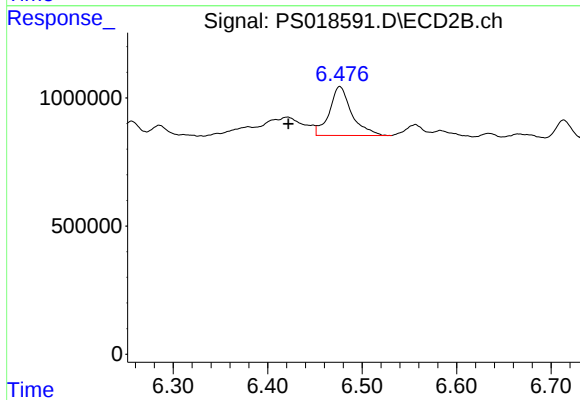


#3 4-Nitrophenol

R.T.: 6.476 min
Delta R.T.: 0.054 min
Response: 3135360
Conc: 7.72 ng/ml

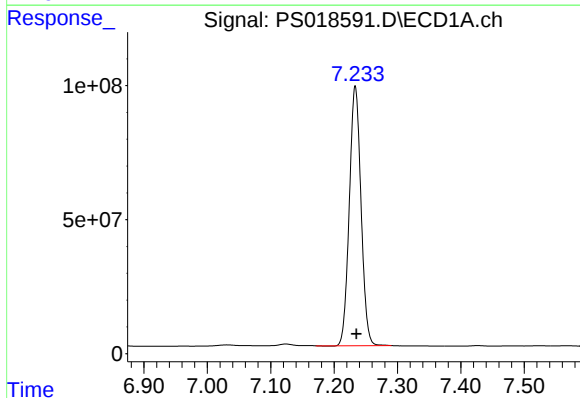


#4 2,4-DCAA

R.T.: 7.233 min
Delta R.T.: -0.002 min
Response: 1241503320
Conc: 436.24 ng/ml

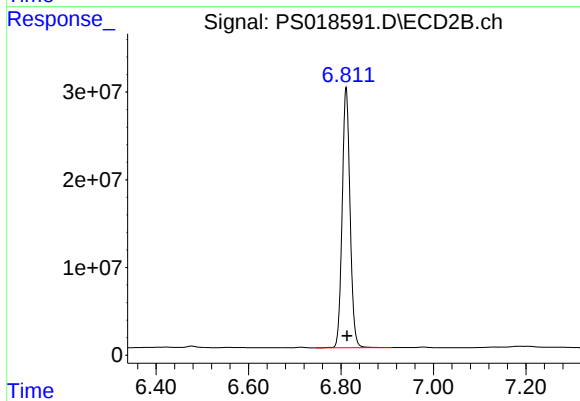

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: -0.002 min
Response: 351647642
Conc: 499.74 ng/ml

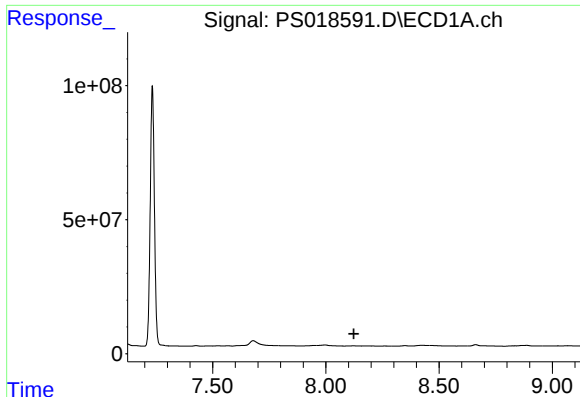

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

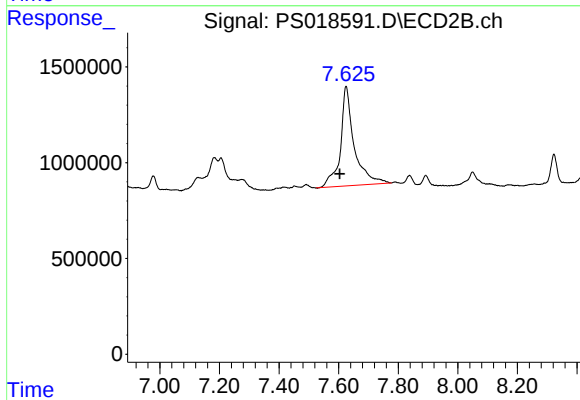


#8 DICHLORPROP

R.T.: 7.625 min
Delta R.T.: 0.021 min
Response: 16675525
Conc: 21.07 ng/ml

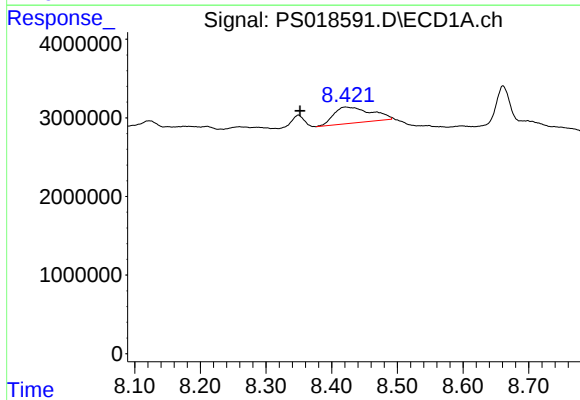


#9 2,4-D

R.T.: 8.421 min
Delta R.T.: 0.069 min
Response: 8207330
Conc: 2.45 ng/ml

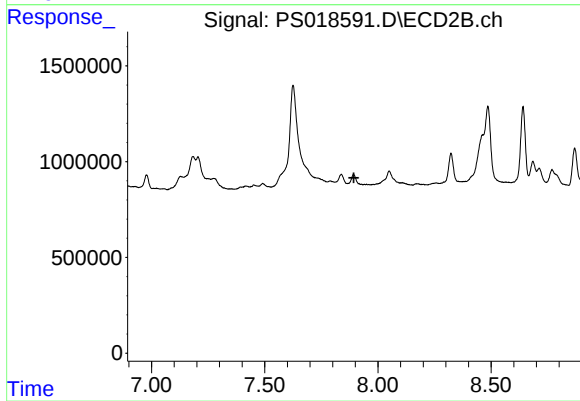

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

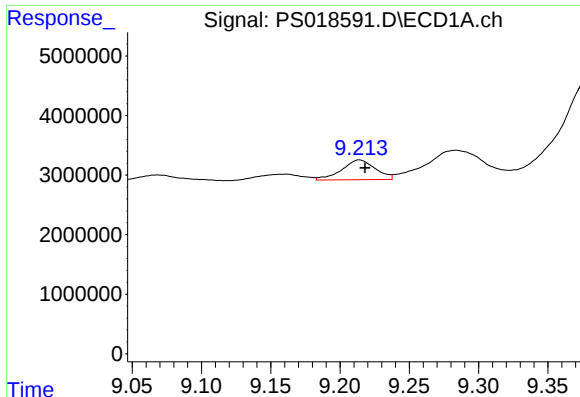

#11 2,4,5-TP (SILVEX)


R.T.: 9.214 min
Delta R.T.: -0.004 min
Response: 5573412
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

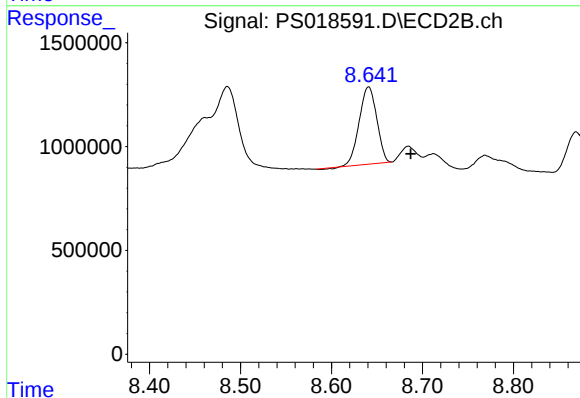


#11 2,4,5-TP (SILVEX)

R.T.: 8.641 min
Delta R.T.: -0.046 min
Response: 4982234
Conc: 1.14 ng/ml

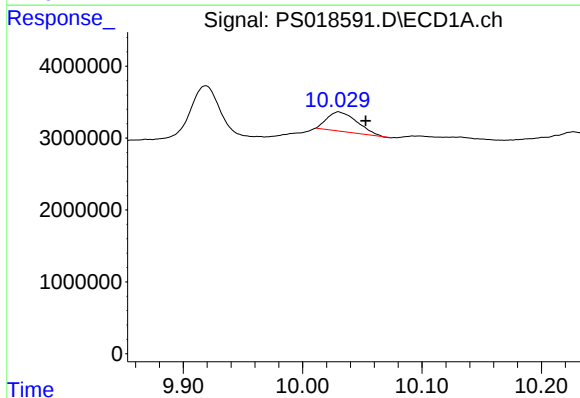


#13 2,4-DB

R.T.: 10.030 min
Delta R.T.: -0.023 min
Response: 4681038
Conc: 1.71 ng/ml

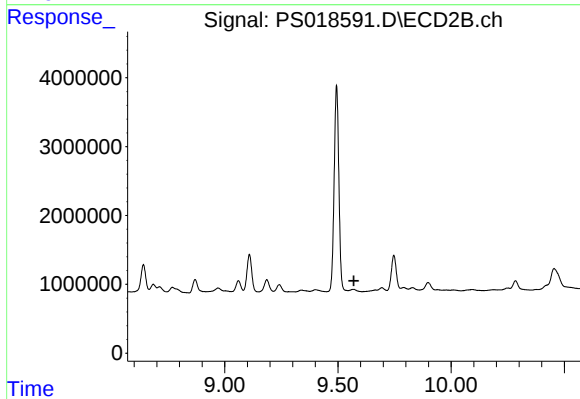

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.570 min
Response: 0
Conc: N.D.

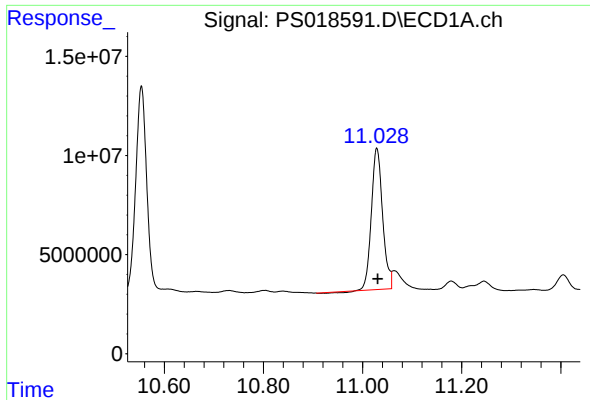

#15 Picloram

R.T.: 11.029 min
Delta R.T.: -0.002 min
Response: 111608688
Conc: 5.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

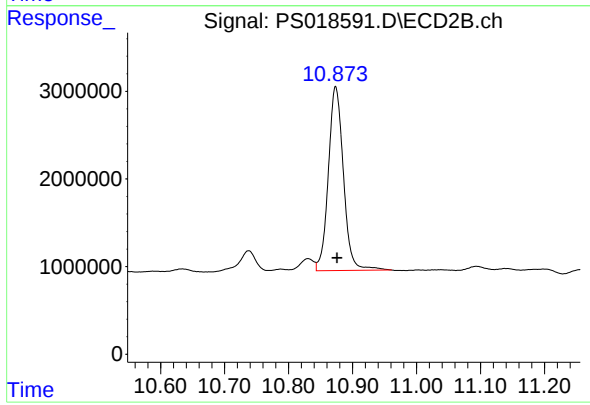

#15 Picloram

R.T.: 10.873 min
Delta R.T.: -0.003 min
Response: 34407451
Conc: 6.47 ng/ml