

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031522\
 Data File : PS018599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 14:26
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 21:41:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.811	1277.8E6	359.9E6	448.984	511.465
Target Compounds							
3) T	4-Nitroph...	7.123f	6.476f	12775722	13472547	7.414	33.161 #
5) T	DICAMBA	7.487f	0.000	2418923	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.624	0	22373087	N.D.	28.263
9) T	2,4-D	8.410f	0.000	3439163	0	1.026	N.D. #
10) T	Pentachlo...	8.665	0.000	6256663	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.217	8.709	74404709	8285939	4.892	1.900 #
12) T	2,4,5-T	9.498	9.062	7441819	1087125	<MDL	<MDL #
13) T	2,4-DB	10.026	9.577	7287364	2630257	2.664	4.633 #
14) T	DINOSEB	11.246	9.899	5807645	3766724	<MDL	1.229 #
15) T	Picloram	11.006	10.881	42837569	32735519	2.084	6.158 #
16) T	DCPA	0.000	10.846	0	11193202	N.D.	2.128



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031522\
Data File : PS018599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 14:26
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 21:41:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

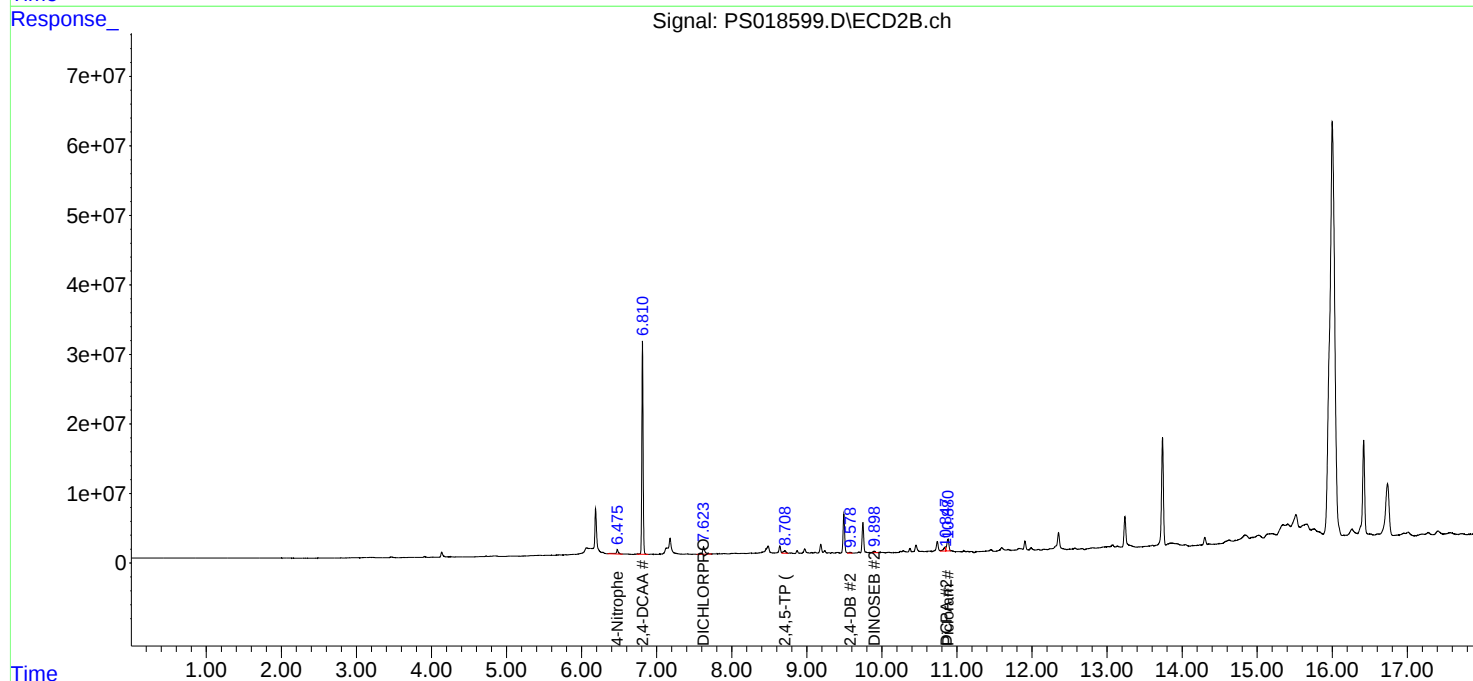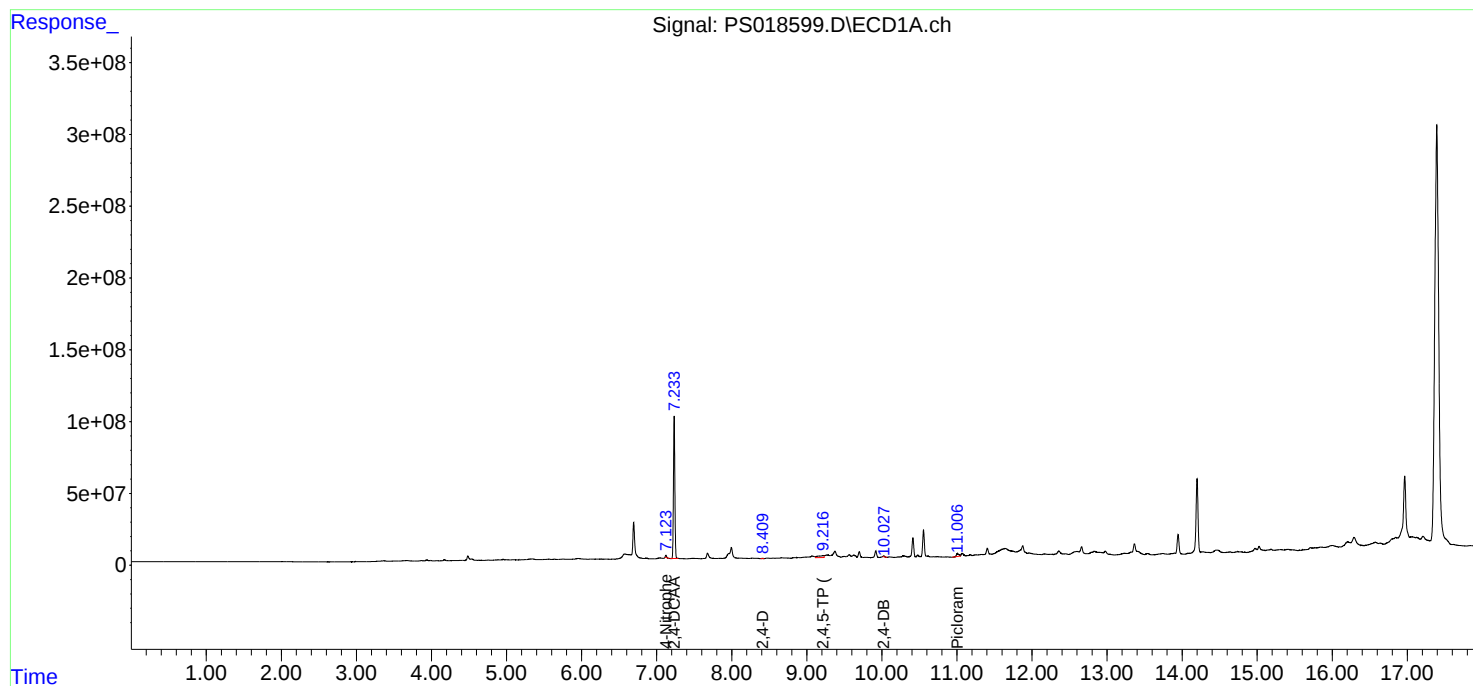


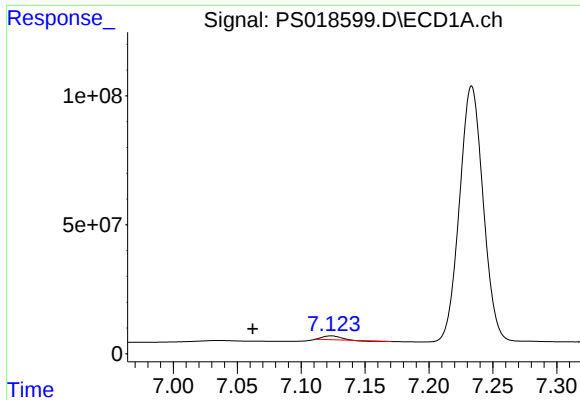

#3 4-Nitrophenol


R.T.: 7.123 min
Delta R.T.: 0.061 min
Response: 12775722
Conc: 7.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

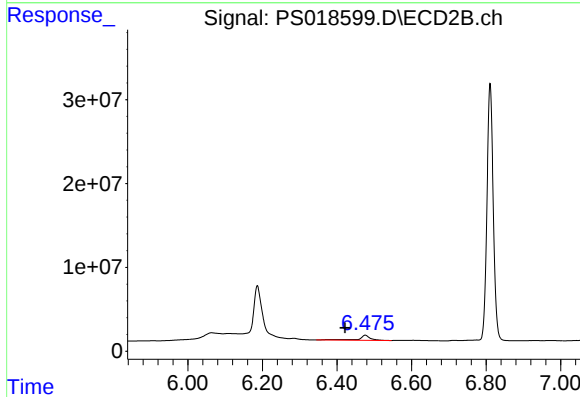


#3 4-Nitrophenol

R.T.: 6.476 min
Delta R.T.: 0.054 min
Response: 13472547
Conc: 33.16 ng/ml

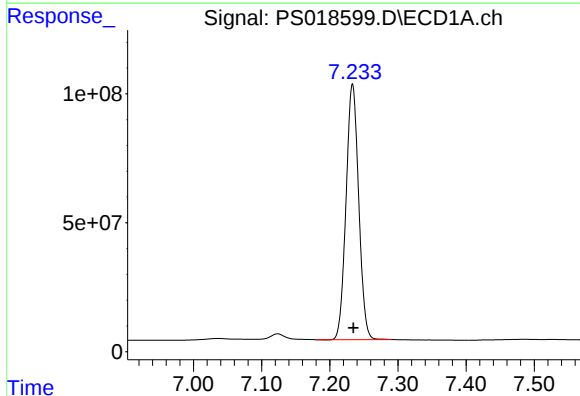


#4 2,4-DCAA

R.T.: 7.233 min
Delta R.T.: -0.002 min
Response: 1277771990
Conc: 448.98 ng/ml

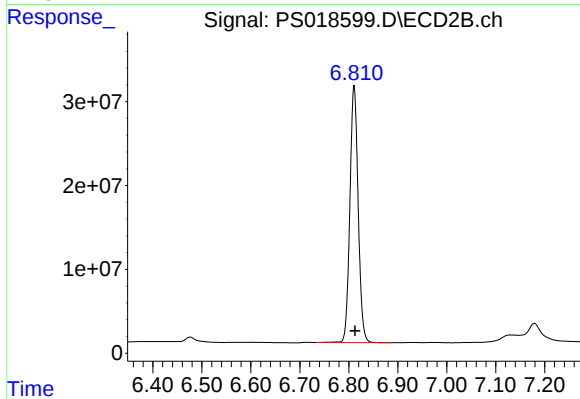

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: -0.002 min
Response: 359895225
Conc: 511.47 ng/ml

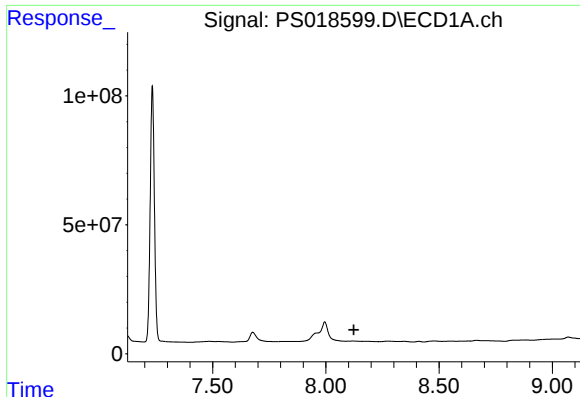

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

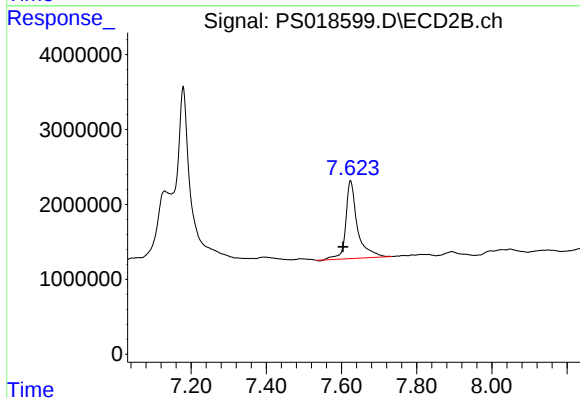


#8 DICHLORPROP

R.T.: 7.624 min
Delta R.T.: 0.020 min
Response: 22373087
Conc: 28.26 ng/ml

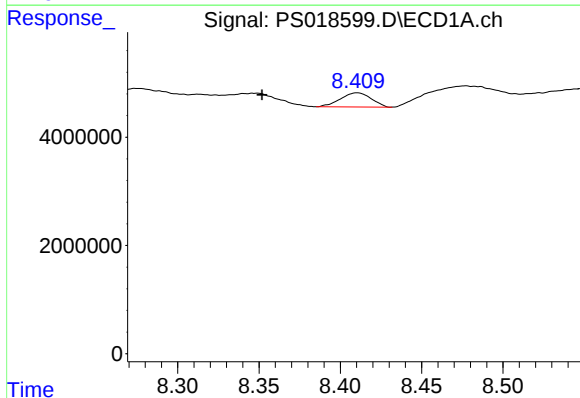


#9 2,4-D

R.T.: 8.410 min
Delta R.T.: 0.058 min
Response: 3439163
Conc: 1.03 ng/ml

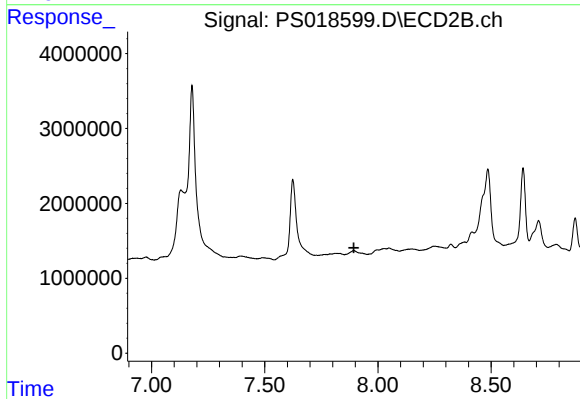

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

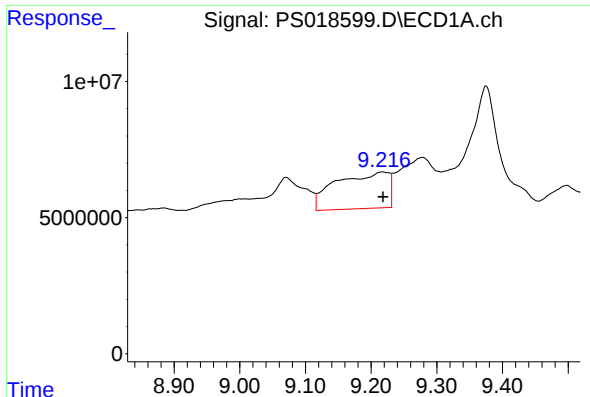

#11 2,4,5-TP (SILVEX)


R.T.: 9.217 min
Delta R.T.: 0.000 min
Response: 74404709
Conc: 4.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

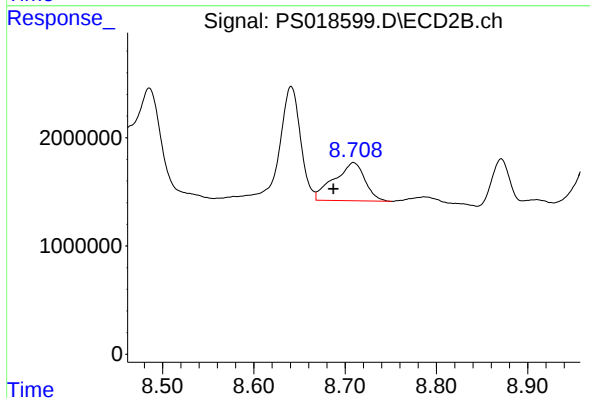


#11 2,4,5-TP (SILVEX)

R.T.: 8.709 min
Delta R.T.: 0.022 min
Response: 8285939
Conc: 1.90 ng/ml

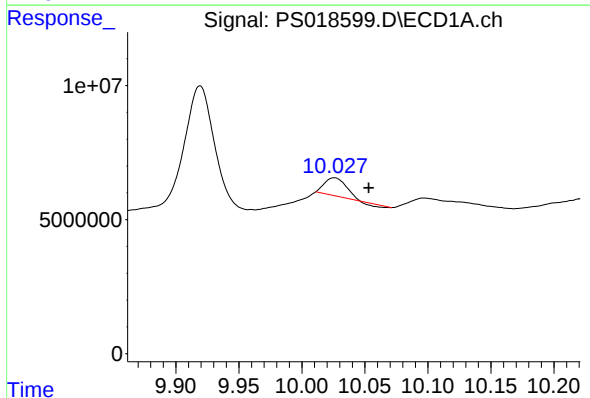


#13 2,4-DB

R.T.: 10.026 min
Delta R.T.: -0.027 min
Response: 7287364
Conc: 2.66 ng/ml

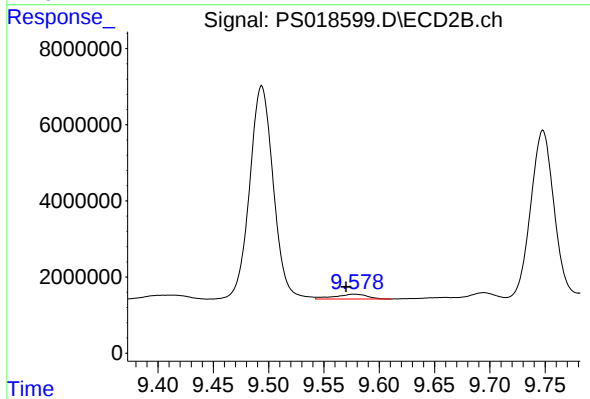

#13 2,4-DB


R.T.: 9.577 min
Delta R.T.: 0.007 min
Response: 2630257
Conc: 4.63 ng/ml

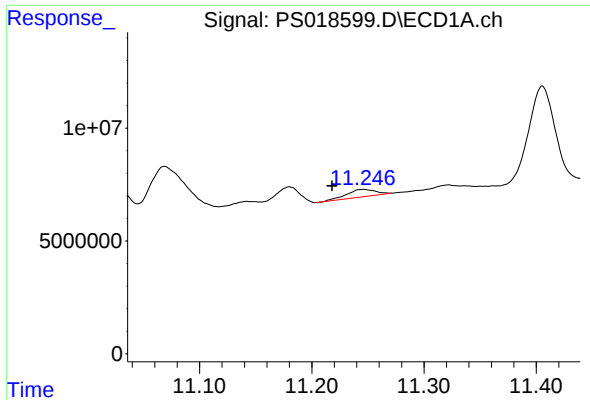

#14 DINOSEB


R.T.: 11.246 min
Delta R.T.: 0.028 min
Response: 5807645
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

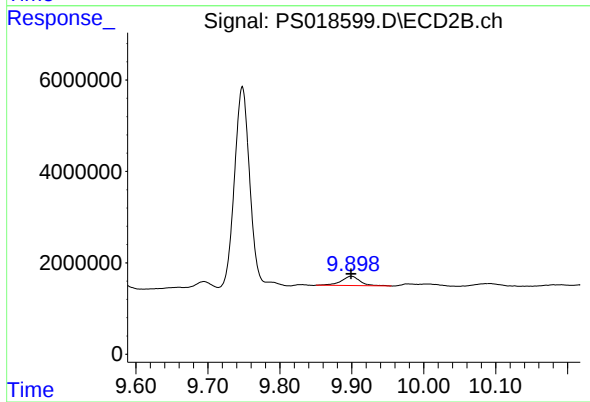


#14 DINOSEB

R.T.: 9.899 min
Delta R.T.: 0.000 min
Response: 3766724
Conc: 1.23 ng/ml

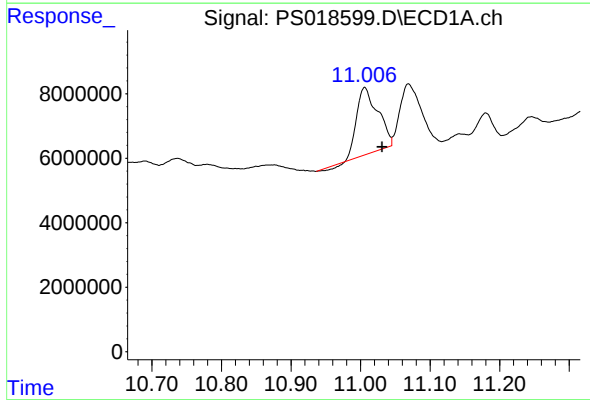


#15 Picloram

R.T.: 11.006 min
Delta R.T.: -0.025 min
Response: 42837569
Conc: 2.08 ng/ml

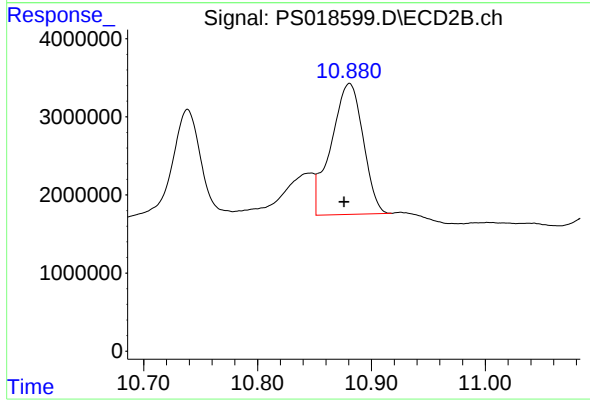

#15 Picloram


R.T.: 10.881 min
Delta R.T.: 0.005 min
Response: 32735519
Conc: 6.16 ng/ml

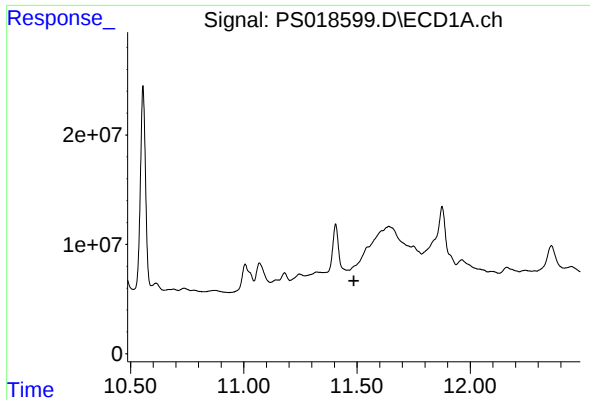

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

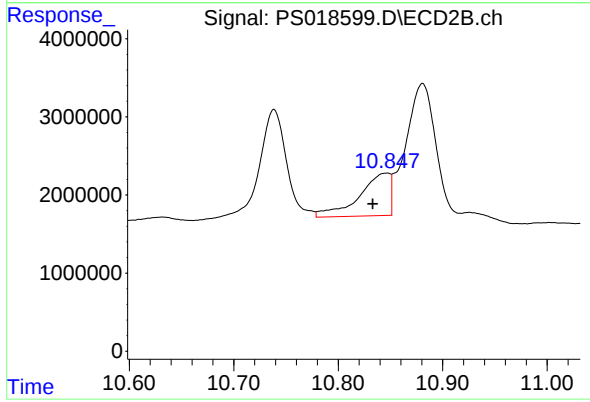

#16 DCPA

R.T.: 10.846 min
Delta R.T.: 0.013 min
Response: 11193202
Conc: 2.13 ng/ml