

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031620\
 Data File : PS009307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2020 12:55
 Operator : DD\AJ
 Sample : L1912-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 13:42:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.933	167.0E6	154.8E6	301.920	281.905
Target Compounds							
2) T	3,5-DICHL...	0.000	6.109	0	31358670	N.D.	38.557
5) T	DICAMBA	7.368	0.000	16623041	0	7.811	N.D. #
7) T	MCPA	7.792	7.400	28271080	33244697	9.282	12.319 #
8) T	DICHLORPROP	0.000	7.752	0	31078690	N.D.	56.016
10) T	Pentachlo...	8.727	0.000	14162416	0	2.014	N.D. #
11) T	2,4,5-TP ...	0.000	8.786	0	58006367	N.D.	19.458
12) T	2,4,5-T	9.450	0.000	13100726	0	5.150	N.D. #
13) T	2,4-DB	0.000	9.722	0	16640505	N.D.	43.835
14) T	DINOSEB	11.187	10.053	12840621	40002850	6.282	18.212 #
15) T	Picloram	11.011	11.021	14985505	10581089	4.938	2.598 #
16) T	DCPA	0.000	11.021	0	10581089	N.D.	2.732



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031620\
Data File : PS009307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2020 12:55
Operator : DD\AJ
Sample : L1912-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 13:42:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

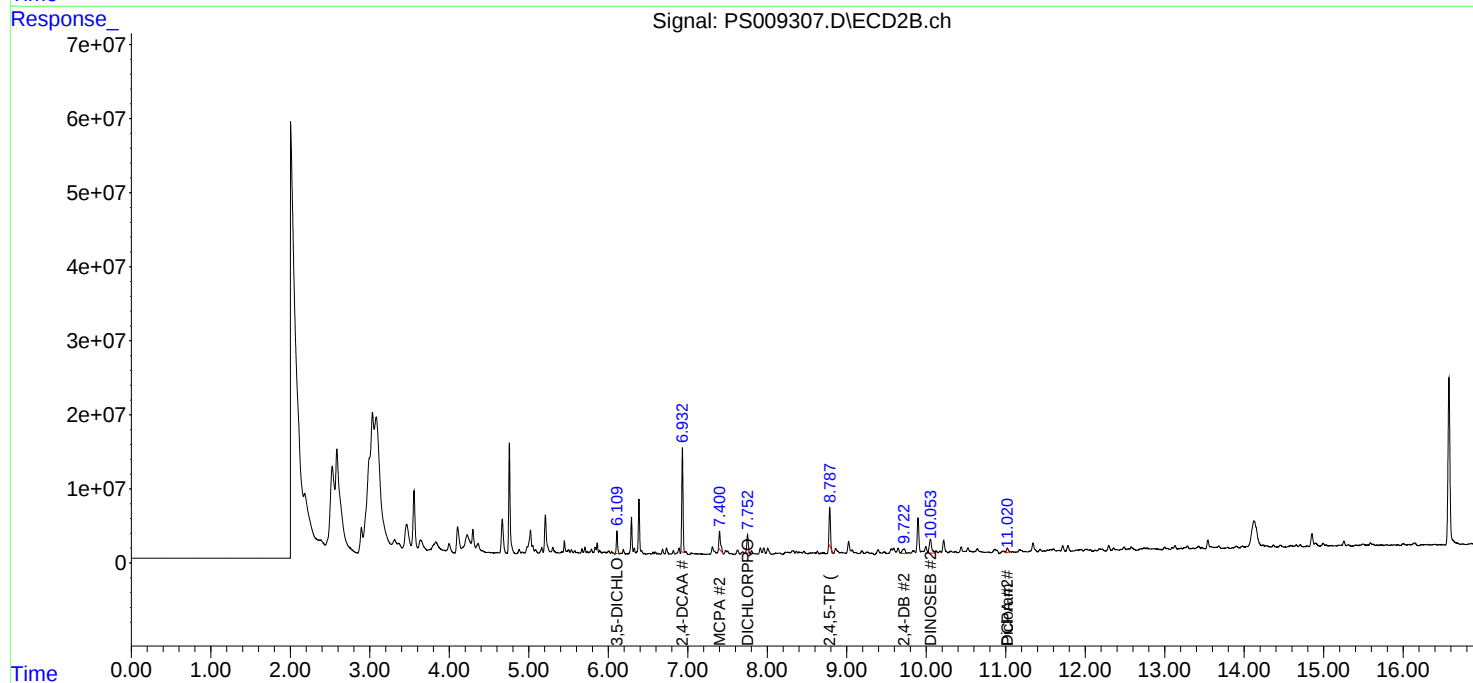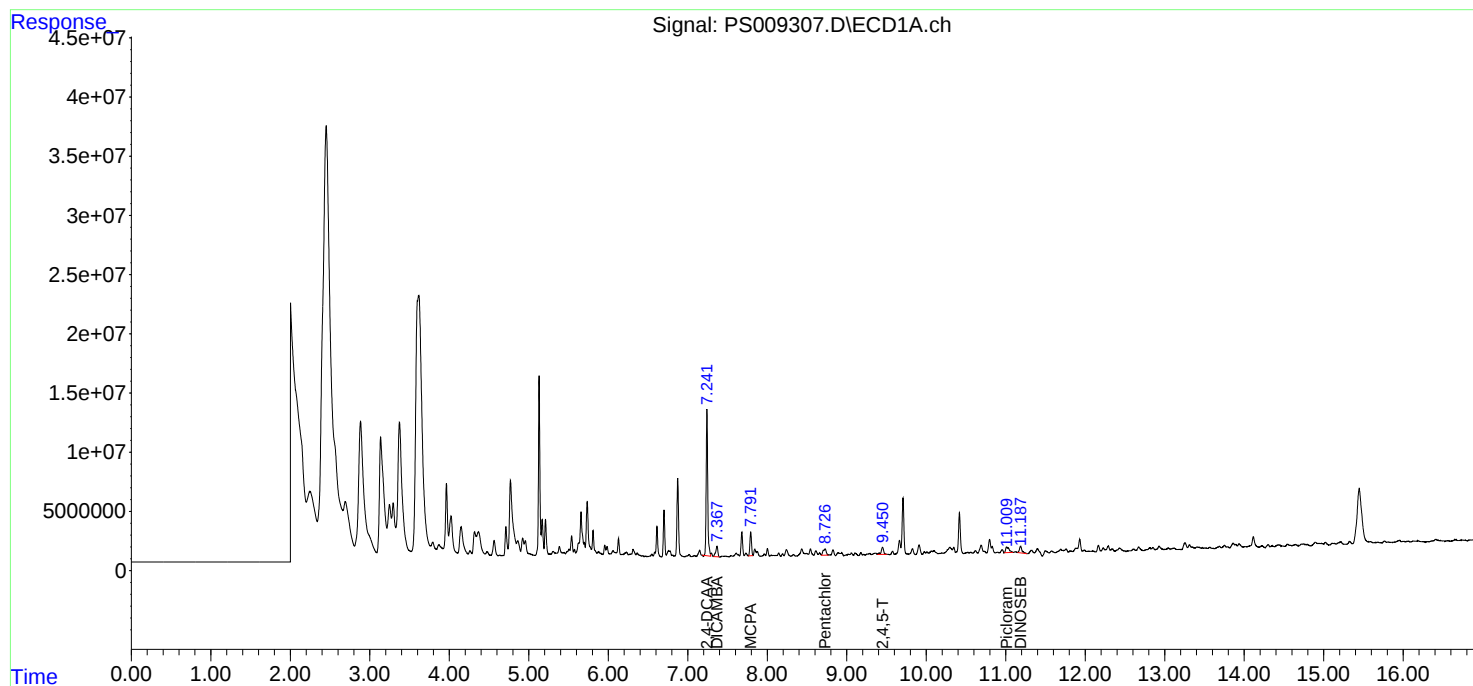


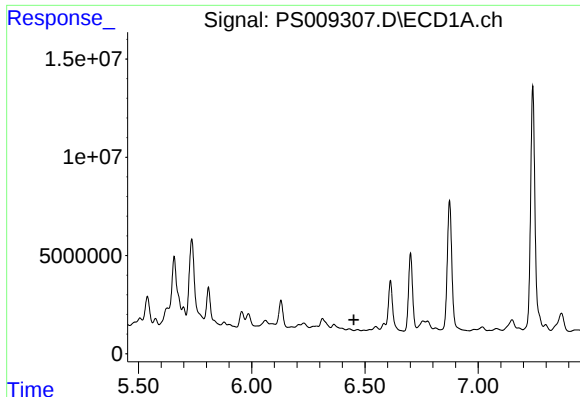

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

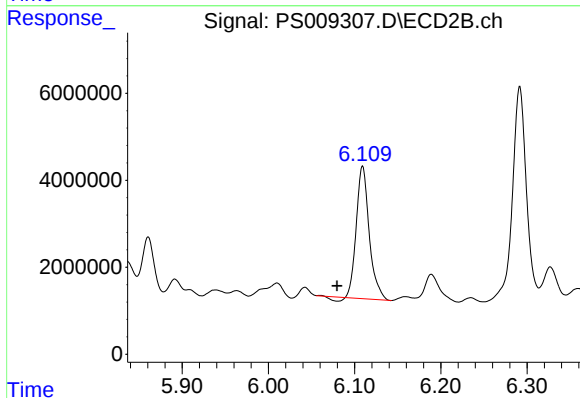


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.109 min
Delta R.T.: 0.030 min
Response: 31358670
Conc: 38.56 ng/ml

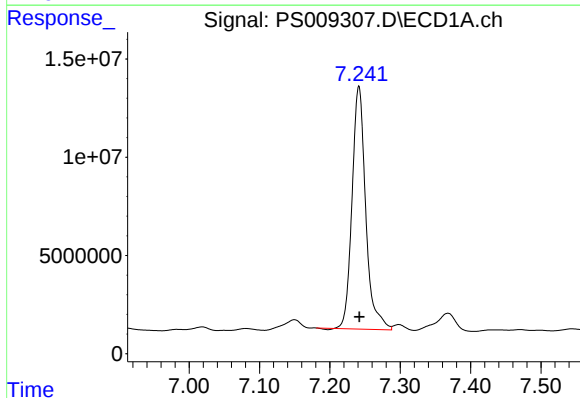


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 167012869
Conc: 301.92 ng/ml

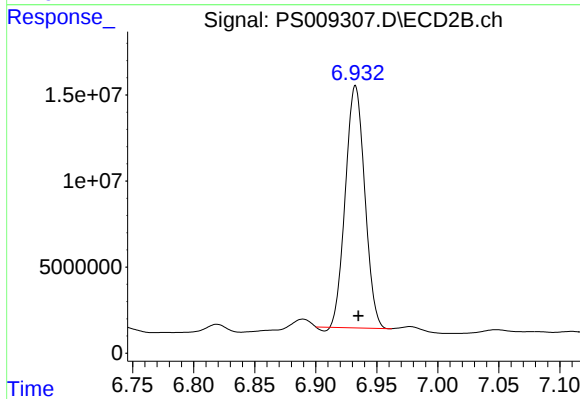

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.003 min
Response: 154821828
Conc: 281.91 ng/ml

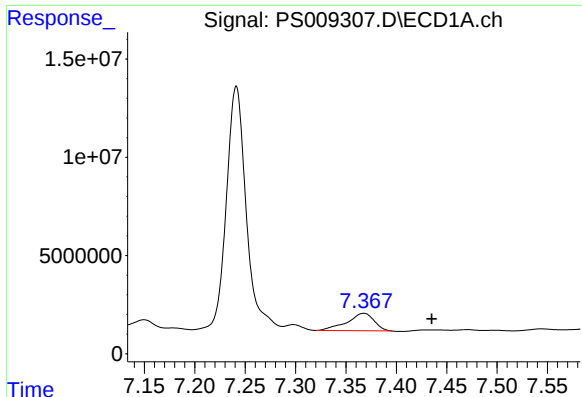

#5 DICAMBA


R.T.: 7.368 min
Delta R.T.: -0.068 min
Response: 16623041
Conc: 7.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

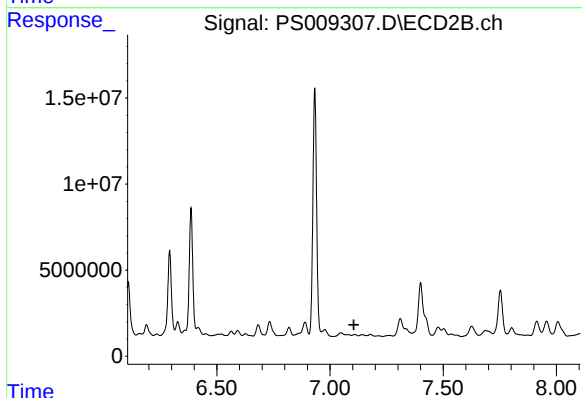


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.106 min
Response: 0
Conc: N.D.

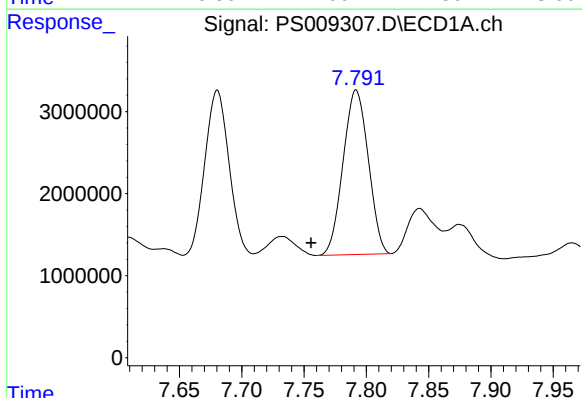


#7 MCPA

R.T.: 7.792 min
Delta R.T.: 0.036 min
Response: 28271080
Conc: 9.28 ug/ml

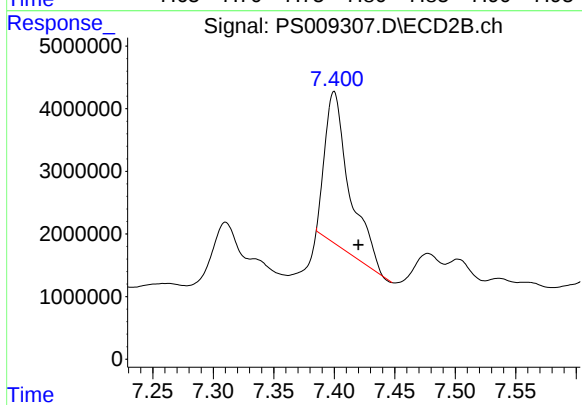

#7 MCPA


R.T.: 7.400 min
Delta R.T.: -0.020 min
Response: 33244697
Conc: 12.32 ug/ml

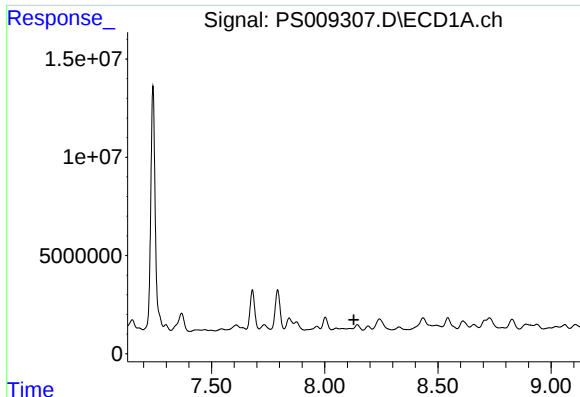

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

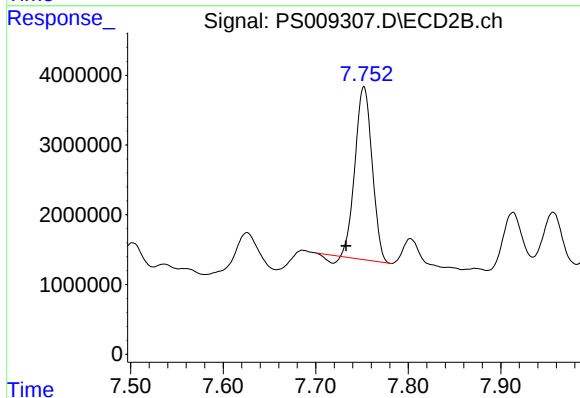


#8 DICHLORPROP

R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 31078690
Conc: 56.02 ng/ml

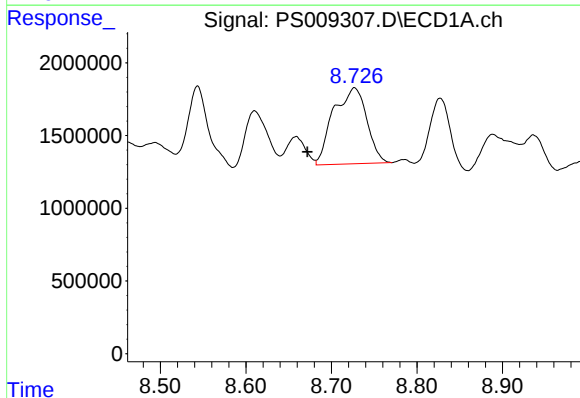


#10 Pentachlorophenol

R.T.: 8.727 min
Delta R.T.: 0.055 min
Response: 14162416
Conc: 2.01 ng/ml

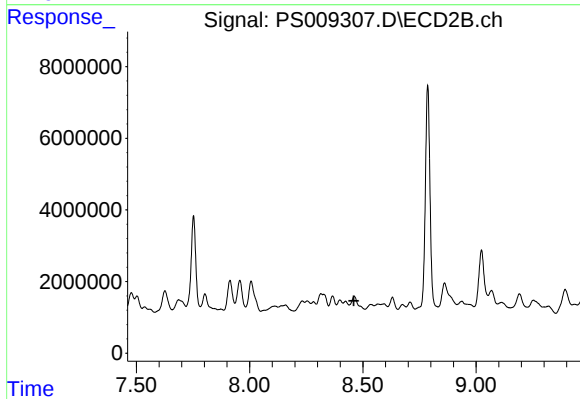

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.461 min
Response: 0
Conc: N.D.

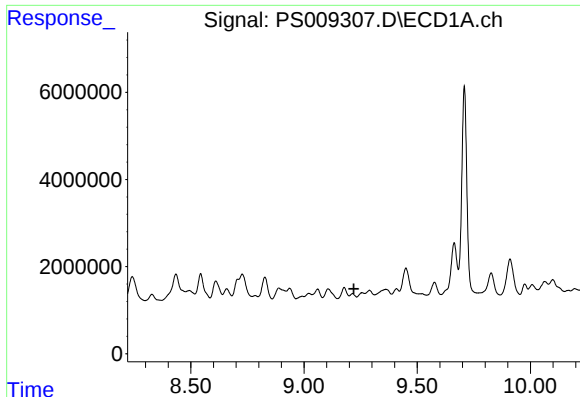

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

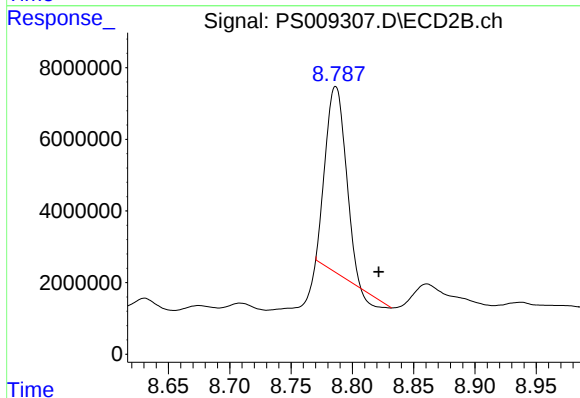


#11 2,4,5-TP (SILVEX)

R.T.: 8.786 min
Delta R.T.: -0.035 min
Response: 58006367
Conc: 19.46 ng/ml

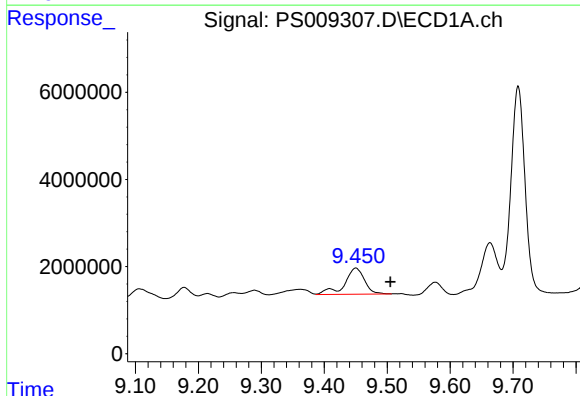


#12 2,4,5-T

R.T.: 9.450 min
Delta R.T.: -0.055 min
Response: 13100726
Conc: 5.15 ng/ml

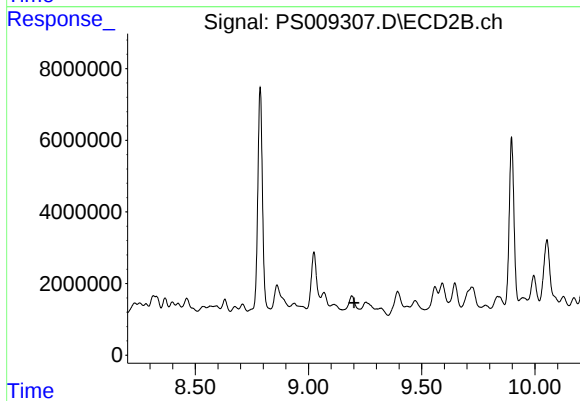

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

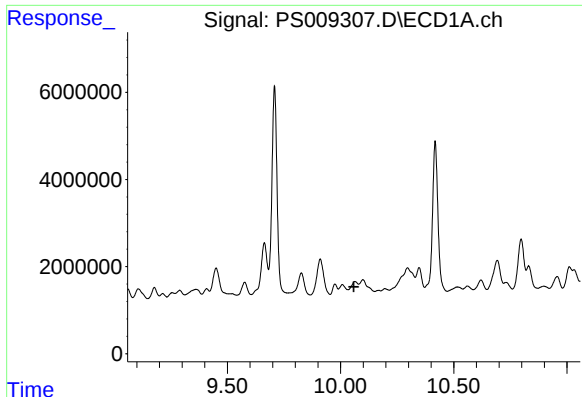

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

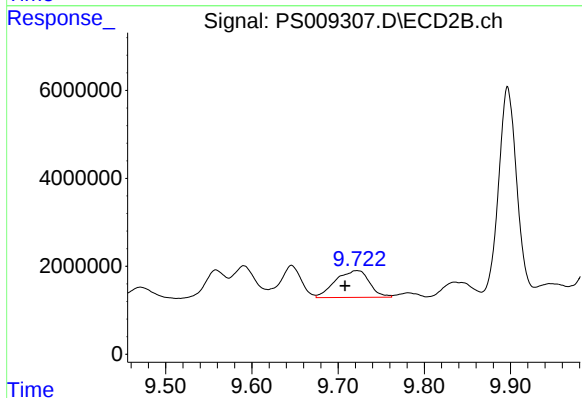


#13 2,4-DB

R.T.: 9.722 min
Delta R.T.: 0.014 min
Response: 16640505
Conc: 43.84 ng/ml

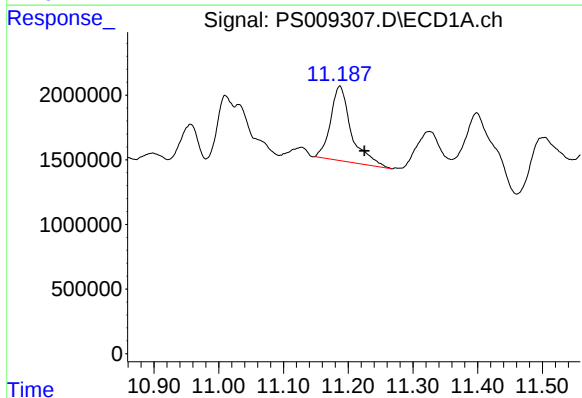


#14 DINOSEB

R.T.: 11.187 min
Delta R.T.: -0.038 min
Response: 12840621
Conc: 6.28 ng/ml

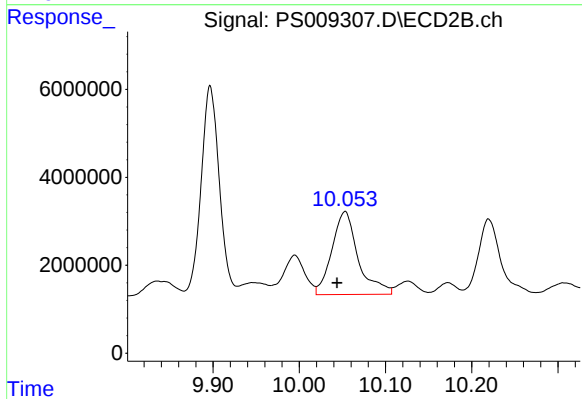

#14 DINOSEB


R.T.: 10.053 min
Delta R.T.: 0.009 min
Response: 40002850
Conc: 18.21 ng/ml

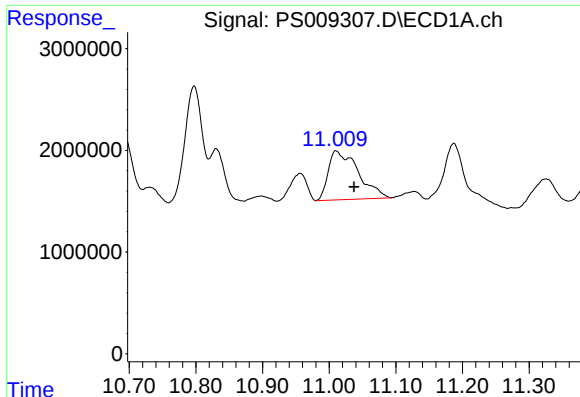

#15 Picloram


R.T.: 11.011 min
Delta R.T.: -0.027 min
Response: 14985505
Conc: 4.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

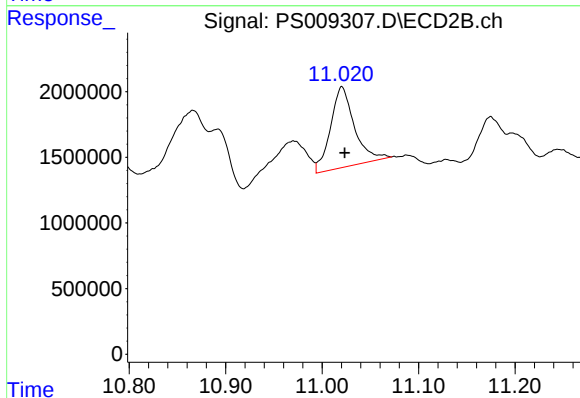


#15 Picloram

R.T.: 11.021 min
Delta R.T.: -0.003 min
Response: 10581089
Conc: 2.60 ng/ml

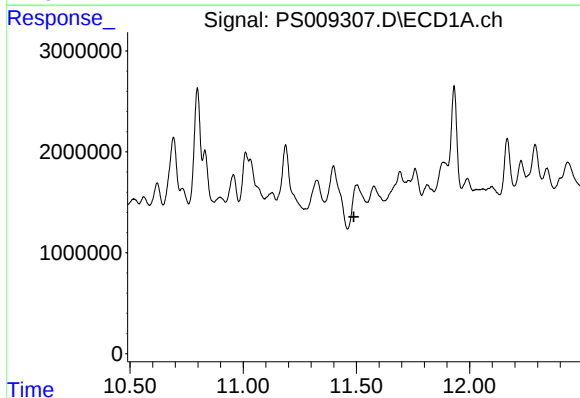

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

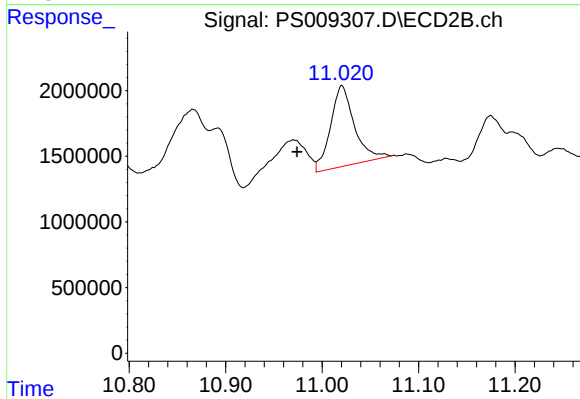

#16 DCPA

R.T.: 11.021 min
Delta R.T.: 0.046 min
Response: 10581089
Conc: 2.73 ng/ml