

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031620\
 Data File : PS009308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2020 13:18
 Operator : DD\AJ
 Sample : L1912-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 13:42:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.269	0.000	24410733	0	44.129	N.D. #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.109	0	62878924	N.D.	77.313
3) T	4-Nitroph...	7.140	6.563	13284304	11045595	55.650	34.713 #
5) T	DICAMBA	7.376	0.000	21321408	0	10.019	N.D. #
7) T	MCPA	7.792	7.400	62052425	47928352	20.374	17.760
8) T	DICHLORPROP	0.000	7.752	0	33655246	N.D.	60.660
10) T	Pentachlo...	8.727	0.000	9275772	0	1.319	N.D. #
11) T	2,4,5-TP ...	0.000	8.785	0	26892927	N.D.	9.021
12) T	2,4,5-T	9.447	0.000	27098733	0	10.653	N.D. #
14) T	DINOSEB	11.186	10.044	13401846	27708508	6.556	12.615 #
15) T	Picloram	0.000	11.021	0	16032538	N.D.	3.937
16) T	DCPA	0.000	11.021	0	16032538	N.D.	4.140



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031620\
Data File : PS009308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2020 13:18
Operator : DD\AJ
Sample : L1912-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 13:42:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

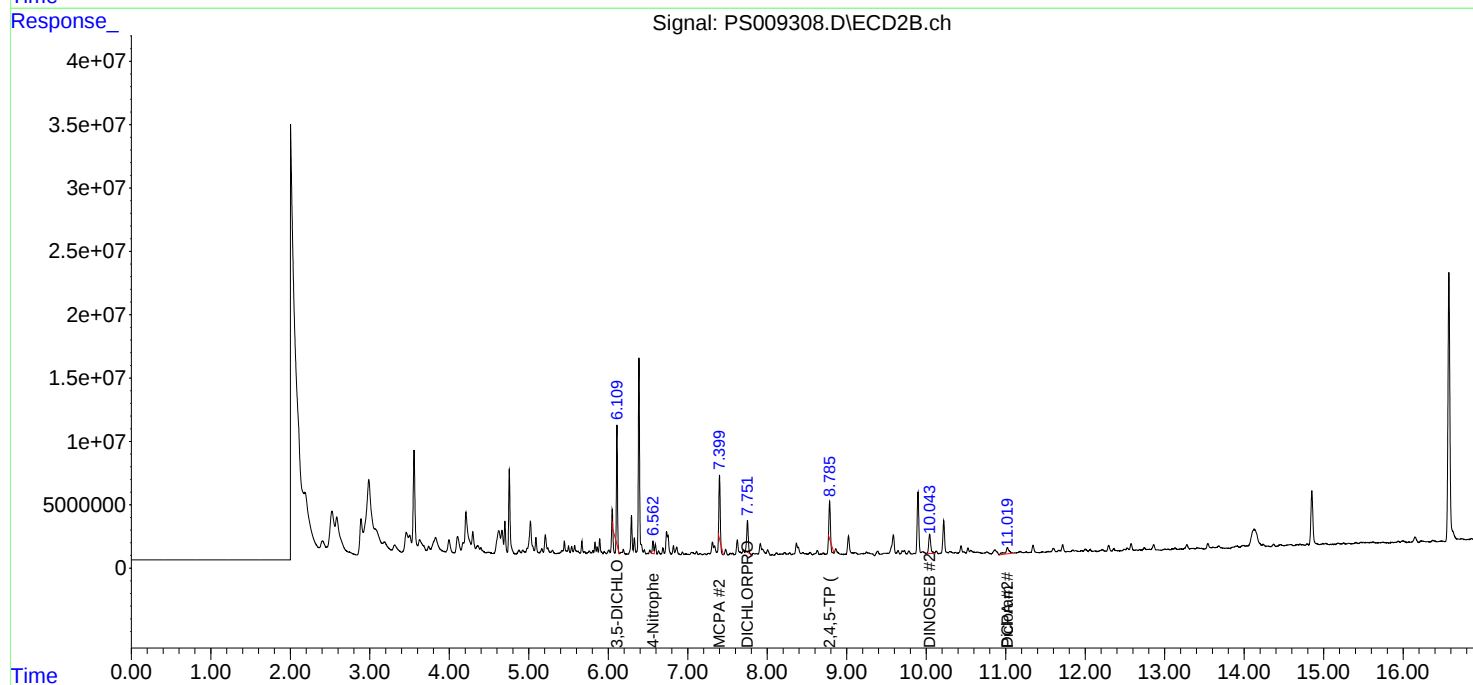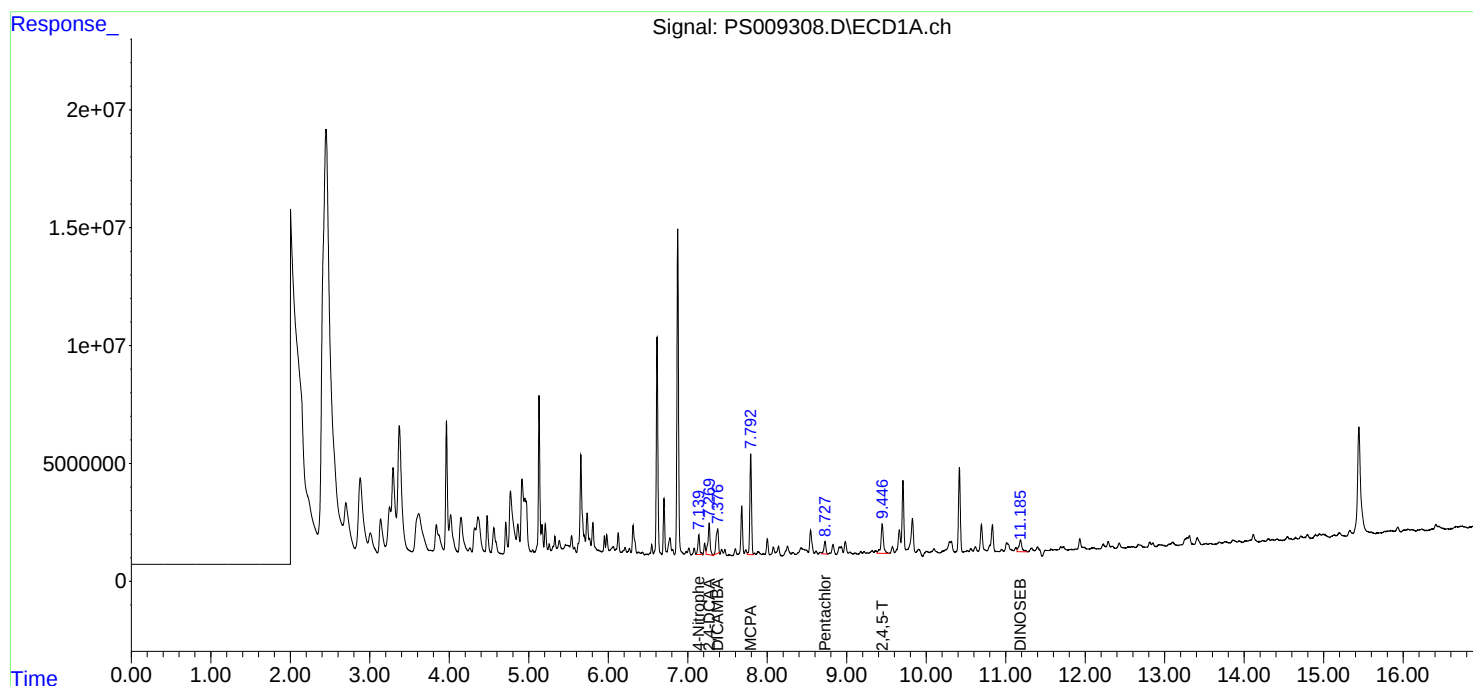


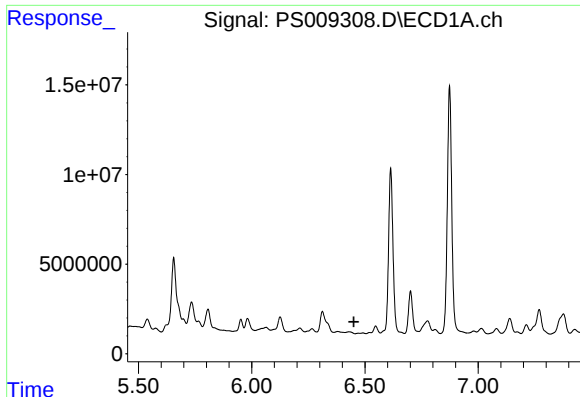

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

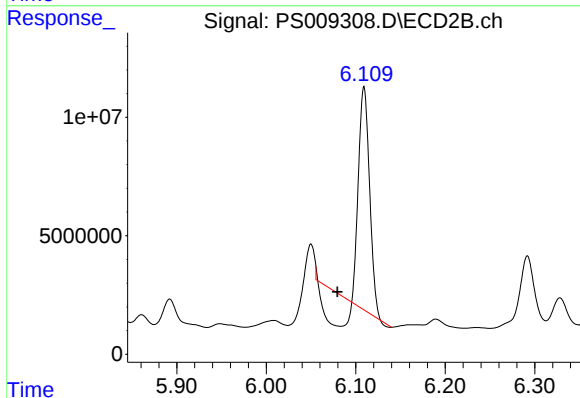


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.109 min
Delta R.T.: 0.030 min
Response: 62878924
Conc: 77.31 ng/ml

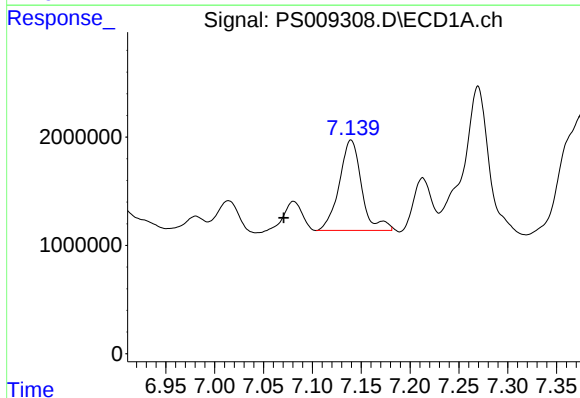


#3 4-Nitrophenol

R.T.: 7.140 min
Delta R.T.: 0.069 min
Response: 13284304
Conc: 55.65 ng/ml

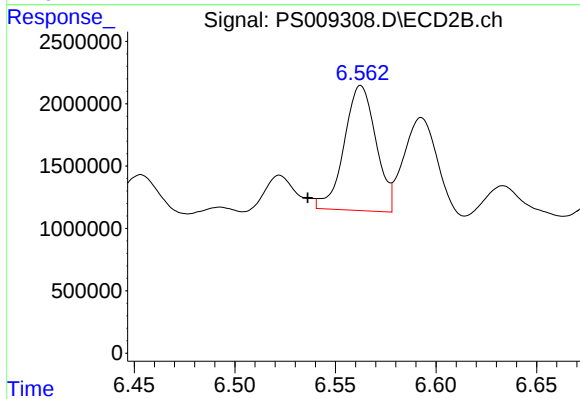

#3 4-Nitrophenol


R.T.: 6.563 min
Delta R.T.: 0.026 min
Response: 11045595
Conc: 34.71 ng/ml

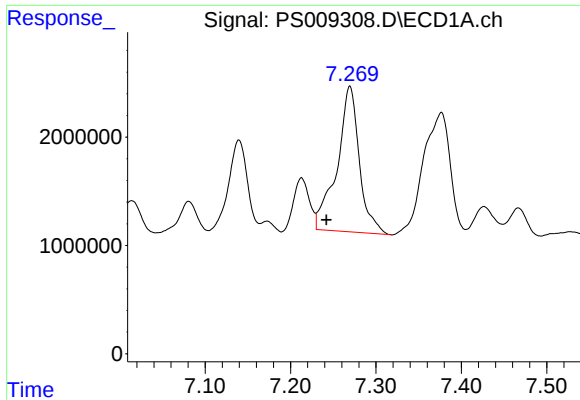

#4 2,4-DCAA


R.T.: 7.269 min
Delta R.T.: 0.028 min
Response: 24410733
Conc: 44.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

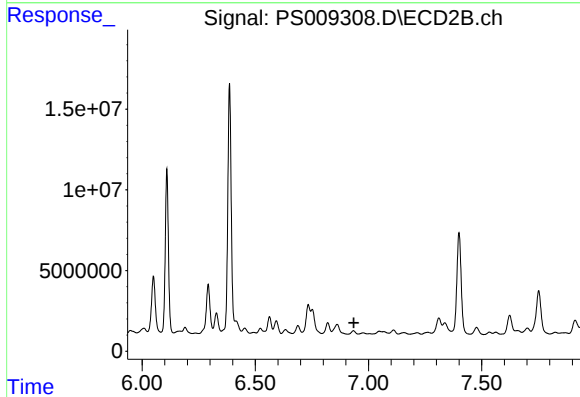


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

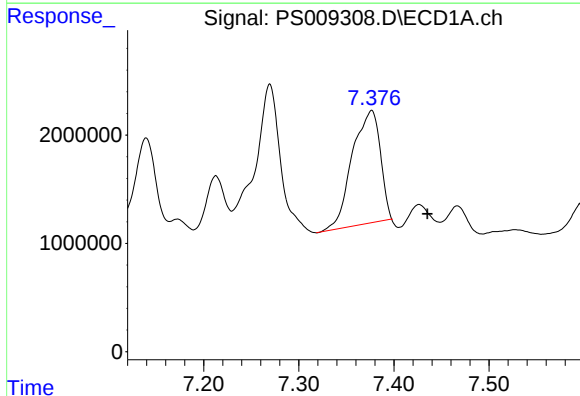


#5 DICAMBA

R.T.: 7.376 min
Delta R.T.: -0.059 min
Response: 21321408
Conc: 10.02 ng/ml

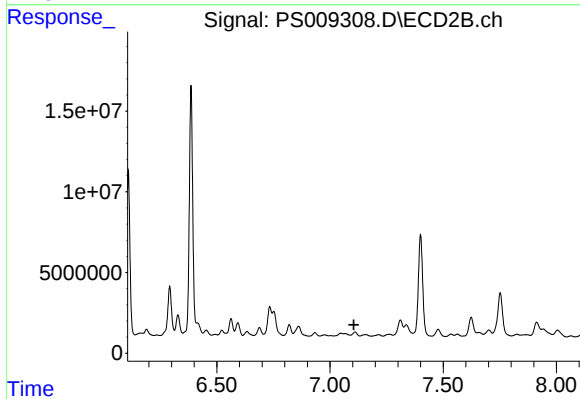

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.106 min
Response: 0
Conc: N.D.

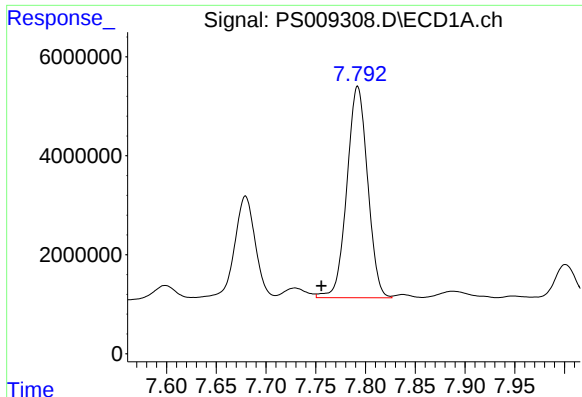

#7 MCPA


R.T.: 7.792 min
Delta R.T.: 0.037 min
Response: 62052425
Conc: 20.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

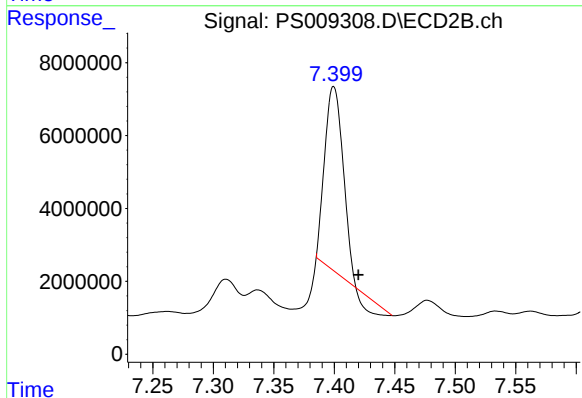


#7 MCPA

R.T.: 7.400 min
Delta R.T.: -0.020 min
Response: 47928352
Conc: 17.76 ug/ml

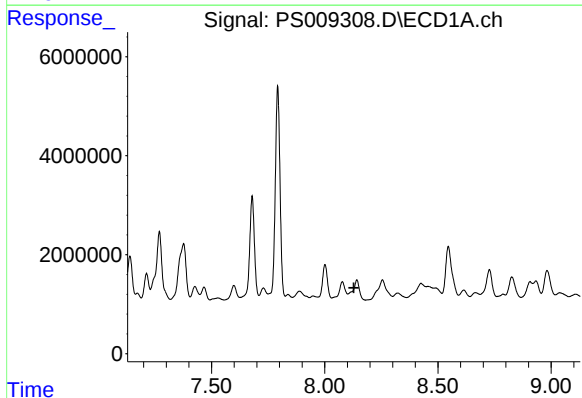


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

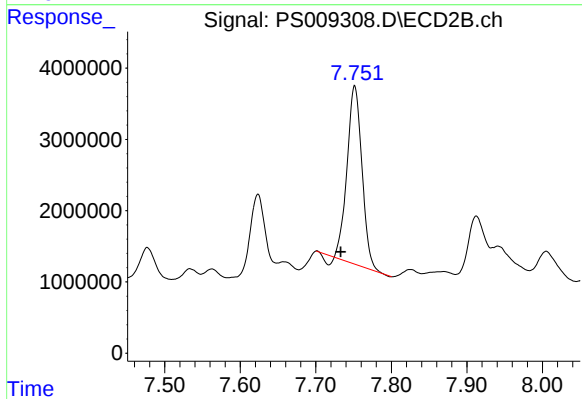

#8 DICHLORPROP


R.T.: 7.752 min
Delta R.T.: 0.018 min
Response: 33655246
Conc: 60.66 ng/ml

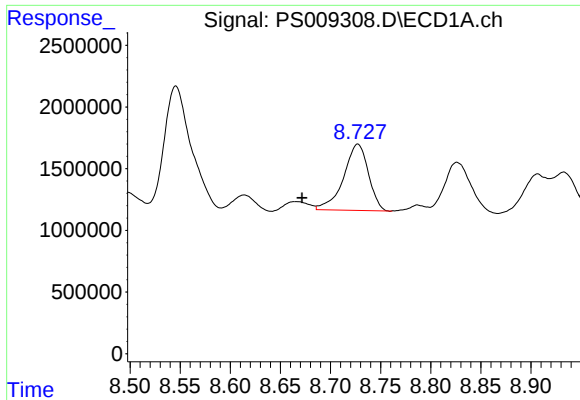

#10 Pentachlorophenol


R.T.: 8.727 min
Delta R.T.: 0.055 min
Response: 9275772
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

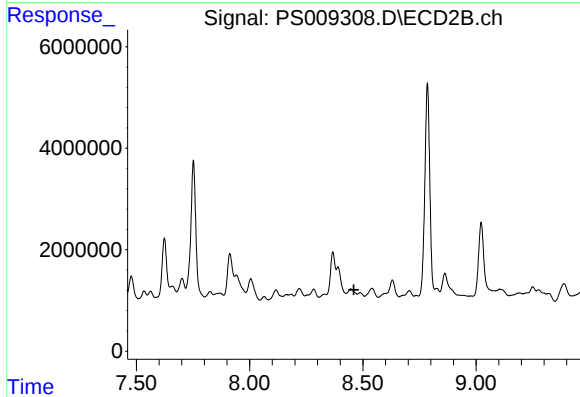


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.461 min
Response: 0
Conc: N.D.

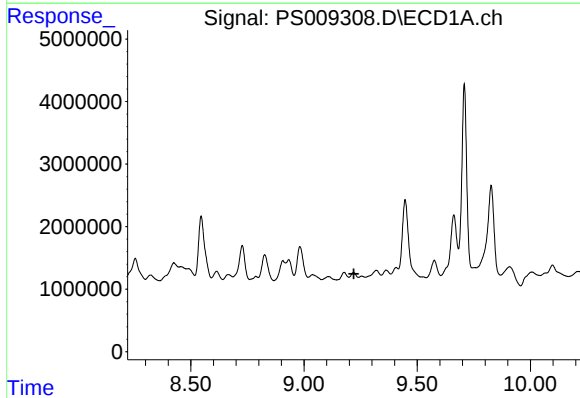


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.221 min
Response: 0
Conc: N.D.

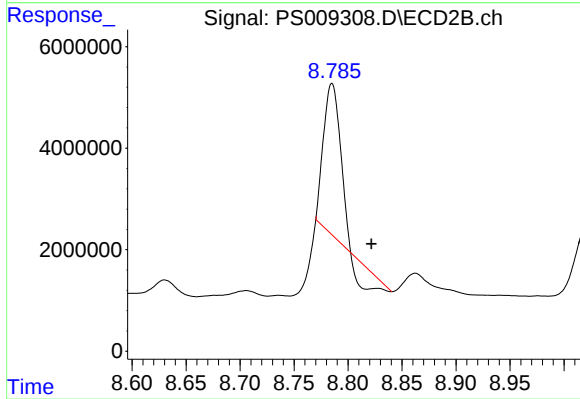

#11 2,4,5-TP (SILVEX)


R.T.: 8.785 min
Delta R.T.: -0.036 min
Response: 26892927
Conc: 9.02 ng/ml

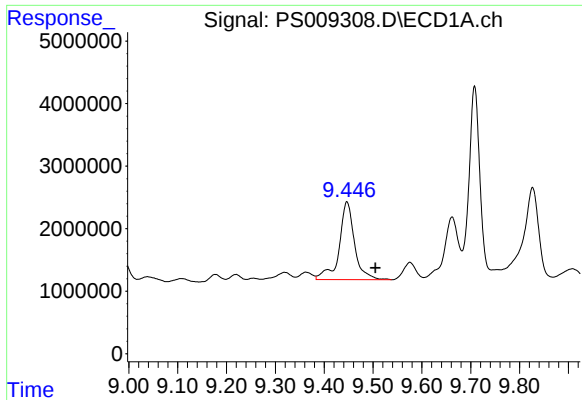

#12 2,4,5-T


R.T.: 9.447 min
Delta R.T.: -0.058 min
Response: 27098733
Conc: 10.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

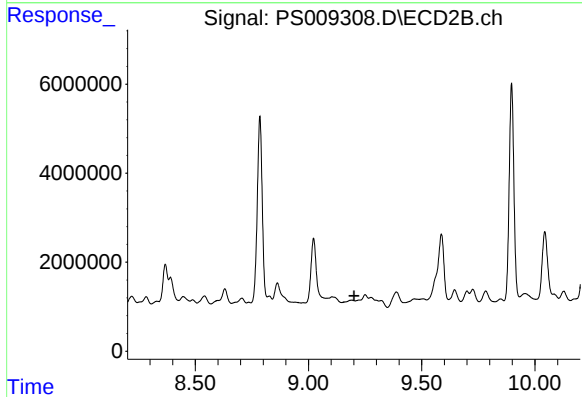


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

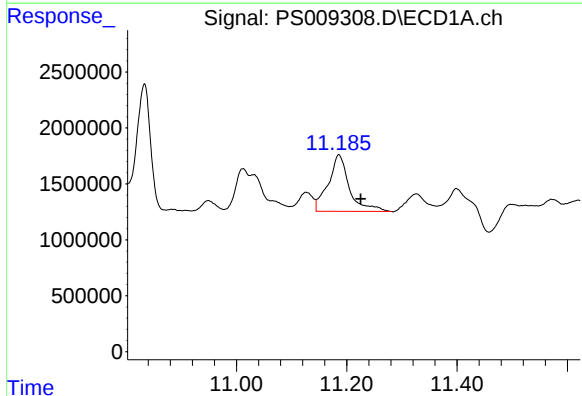


#14 DINOSEB

R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 13401846
Conc: 6.56 ng/ml

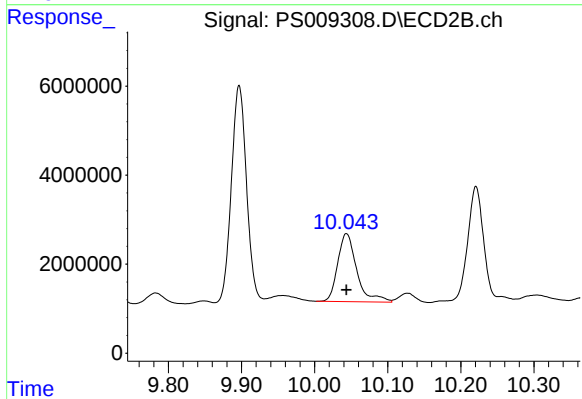

#14 DINOSEB


R.T.: 10.044 min
Delta R.T.: 0.000 min
Response: 27708508
Conc: 12.61 ng/ml

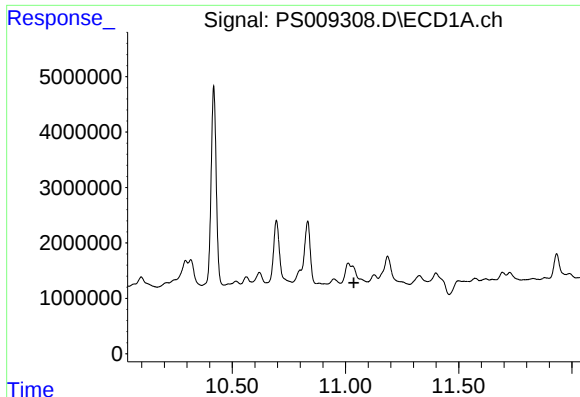

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

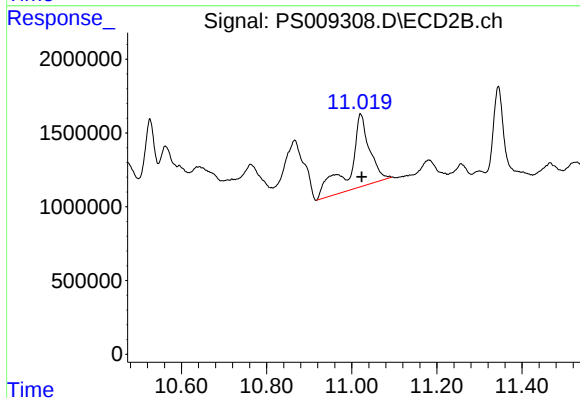


#15 Picloram

R.T.: 11.021 min
Delta R.T.: -0.002 min
Response: 16032538
Conc: 3.94 ng/ml

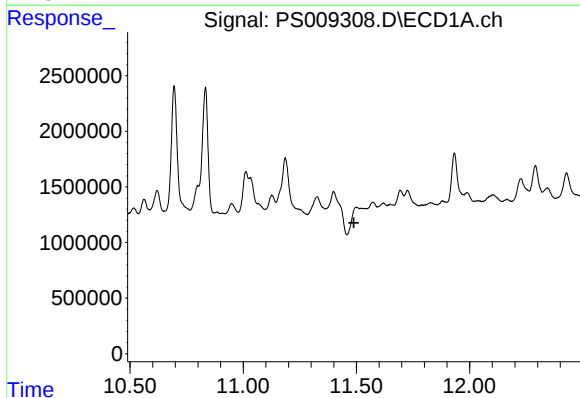

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

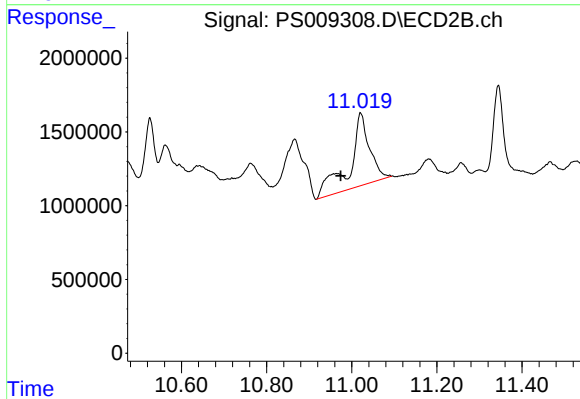

#16 DCPA

R.T.: 11.021 min
Delta R.T.: 0.047 min
Response: 16032538
Conc: 4.14 ng/ml