

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031620\
 Data File : PS009312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2020 14:49
 Operator : DD\AJ
 Sample : L1912-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 16:35:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.933	160.7E6	155.2E6	290.551	282.519
Target Compounds							
2) T	3,5-DICHL...	0.000	6.109	0	89194524	N.D.	109.669
3) T	4-Nitroph...	7.140	6.563	11149856	3686717	46.708	11.586 #
7) T	MCPA	7.734	7.400	20959632	54379840	6.882	20.151 #
8) T	DICHLORPROP	0.000	7.752	0	20729826	N.D.	37.363
10) T	Pentachlo...	8.726	0.000	11183427	0	1.591	N.D. #
11) T	2,4,5-TP ...	0.000	8.785	0	15168934	N.D.	5.088
12) T	2,4,5-T	9.446	0.000	28565963	0	11.229	N.D. #
14) T	DINOSEB	0.000	10.047	0	32714068	N.D.	14.894
15) T	Picloram	0.000	11.022	0	4464251	N.D.	1.096
16) T	DCPA	0.000	11.022	0	4464251	N.D.	1.153



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031620\
Data File : PS009312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2020 14:49
Operator : DD\AJ
Sample : L1912-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 16:35:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

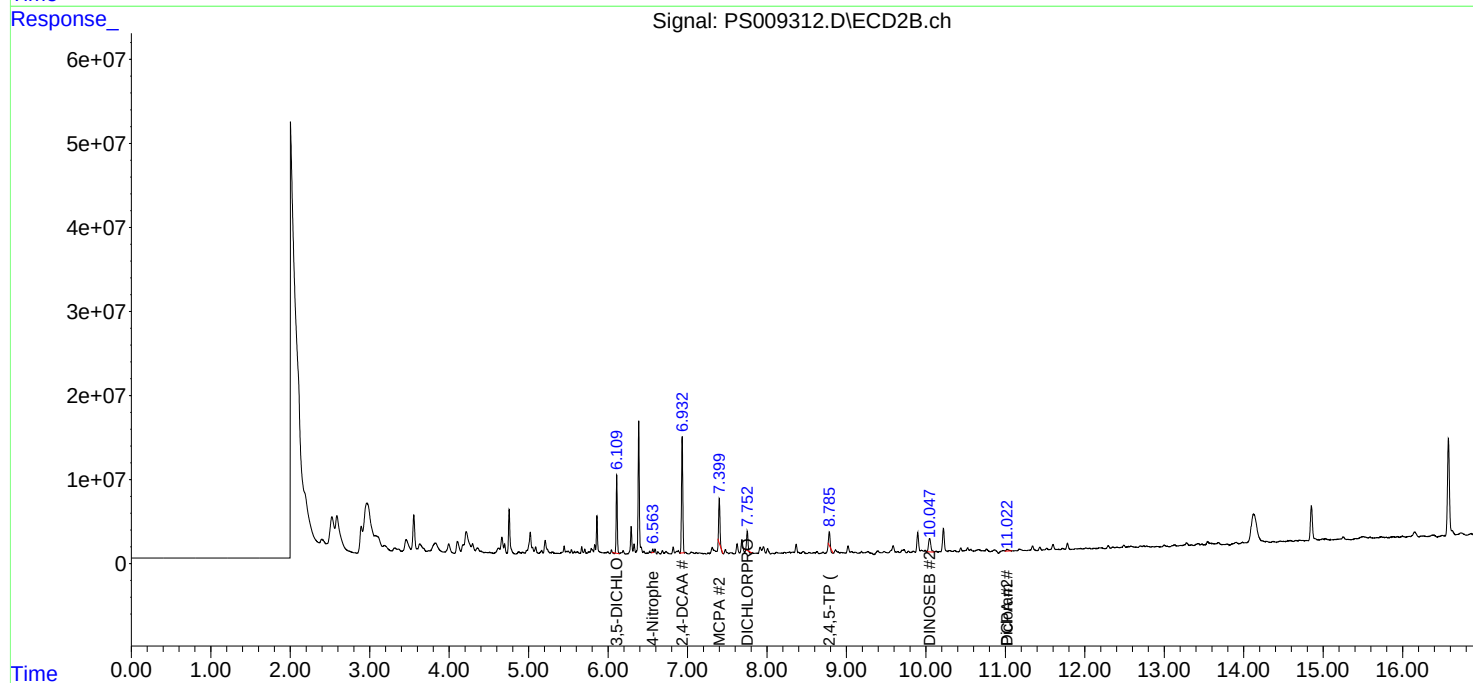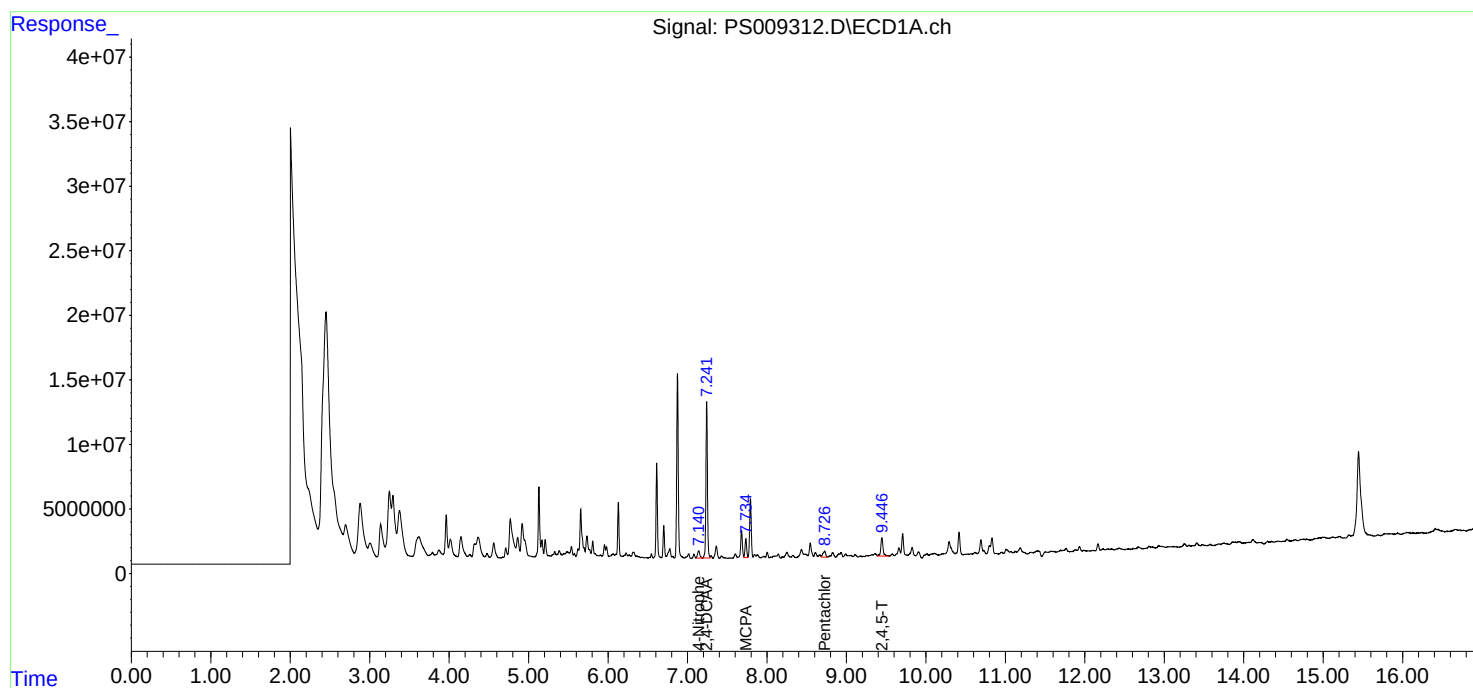


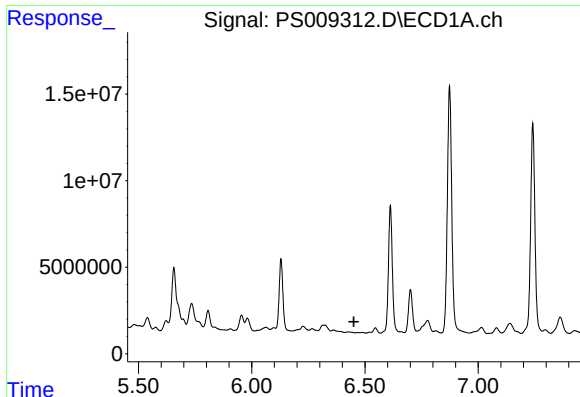

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

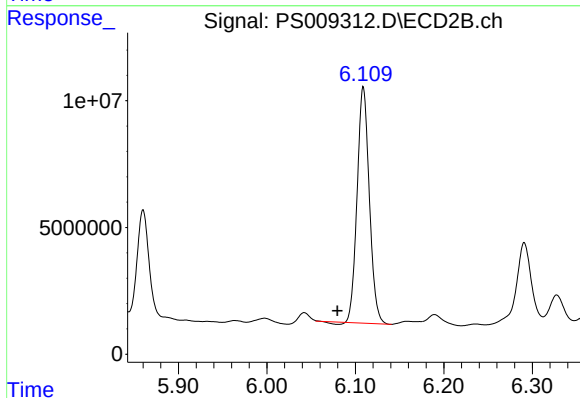


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.109 min
Delta R.T.: 0.029 min
Response: 89194524
Conc: 109.67 ng/ml

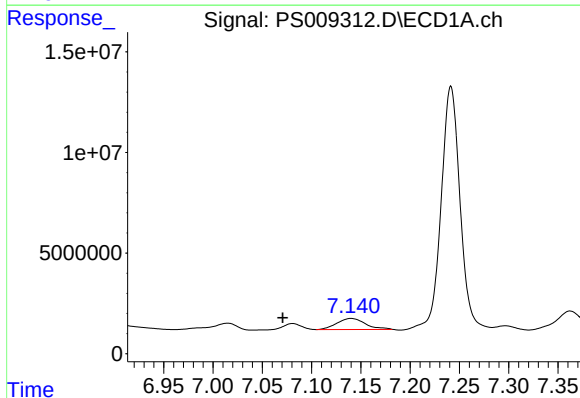


#3 4-Nitrophenol

R.T.: 7.140 min
Delta R.T.: 0.069 min
Response: 11149856
Conc: 46.71 ng/ml

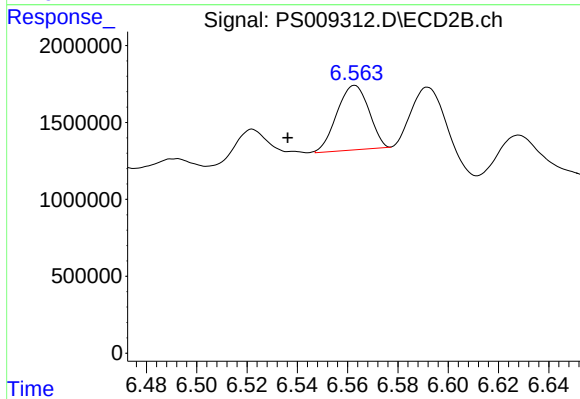

#3 4-Nitrophenol


R.T.: 6.563 min
Delta R.T.: 0.027 min
Response: 3686717
Conc: 11.59 ng/ml

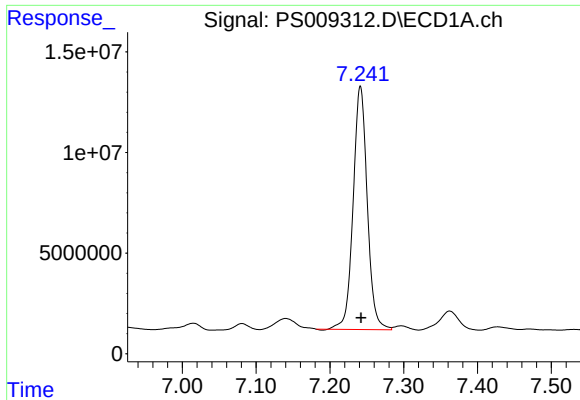

#4 2,4-DCAA


R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 160724351
Conc: 290.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

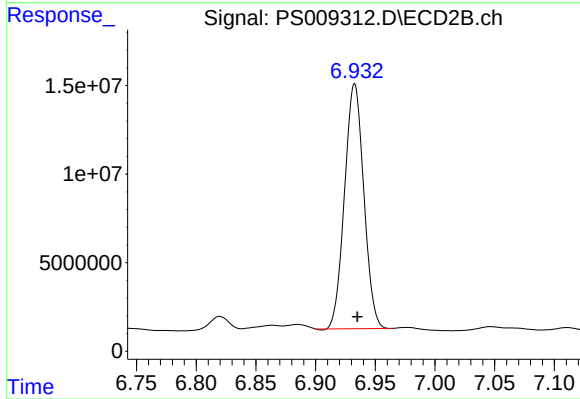


#4 2,4-DCAA

R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 155158579
Conc: 282.52 ng/ml

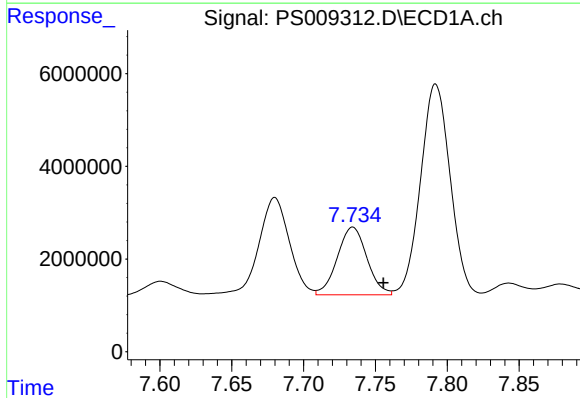


#7 MCPA

R.T.: 7.734 min
Delta R.T.: -0.021 min
Response: 20959632
Conc: 6.88 ug/ml

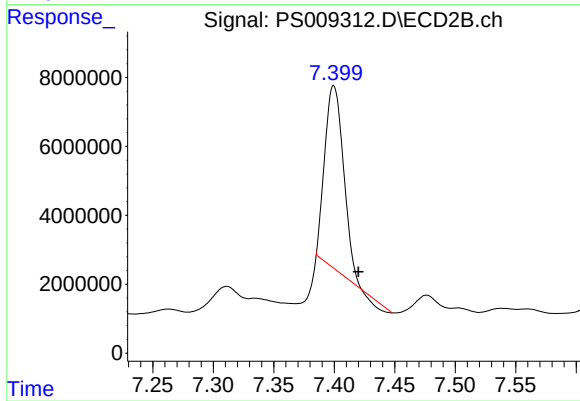

#7 MCPA


R.T.: 7.400 min
Delta R.T.: -0.020 min
Response: 54379840
Conc: 20.15 ug/ml

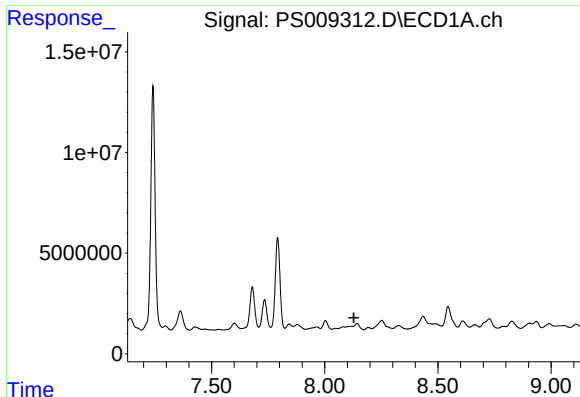

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

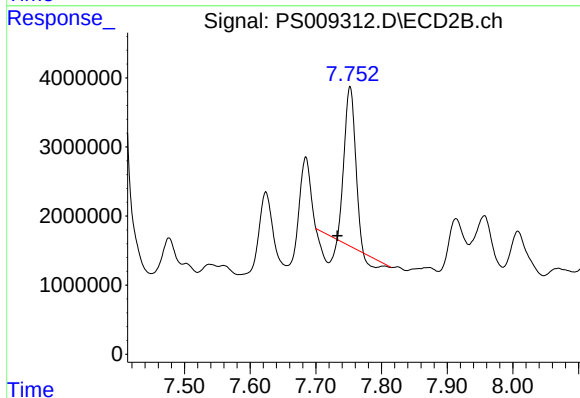


#8 DICHLORPROP

R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 20729826
Conc: 37.36 ng/ml

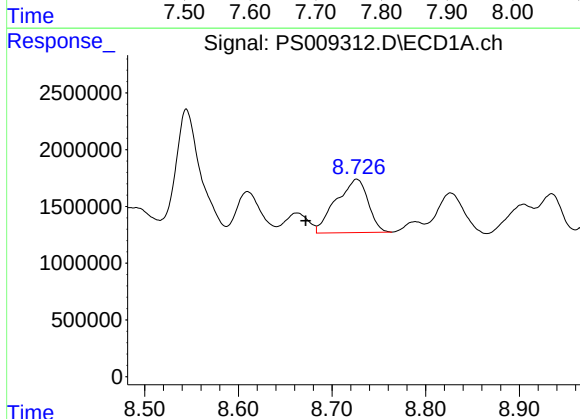


#10 Pentachlorophenol

R.T.: 8.726 min
Delta R.T.: 0.055 min
Response: 11183427
Conc: 1.59 ng/ml

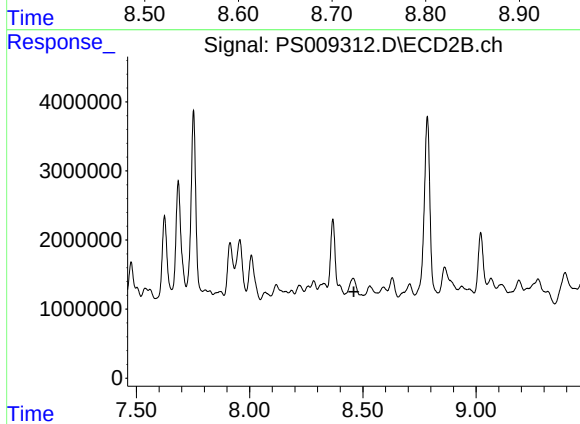

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.461 min
Response: 0
Conc: N.D.

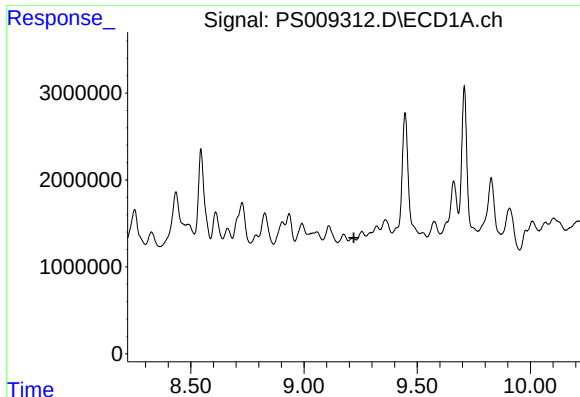

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

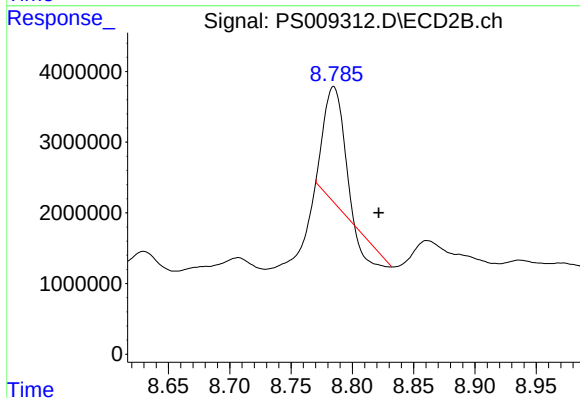


#11 2,4,5-TP (SILVEX)

R.T.: 8.785 min
Delta R.T.: -0.037 min
Response: 15168934
Conc: 5.09 ng/ml

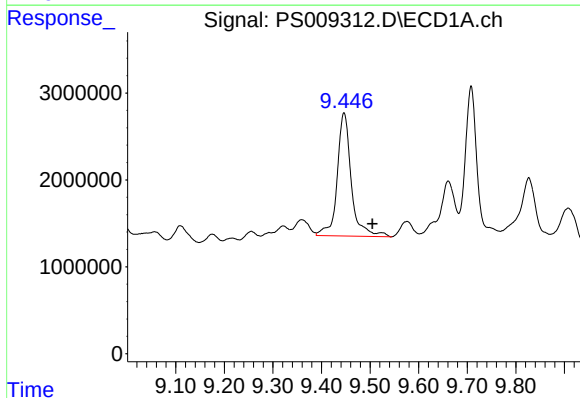


#12 2,4,5-T

R.T.: 9.446 min
Delta R.T.: -0.059 min
Response: 28565963
Conc: 11.23 ng/ml

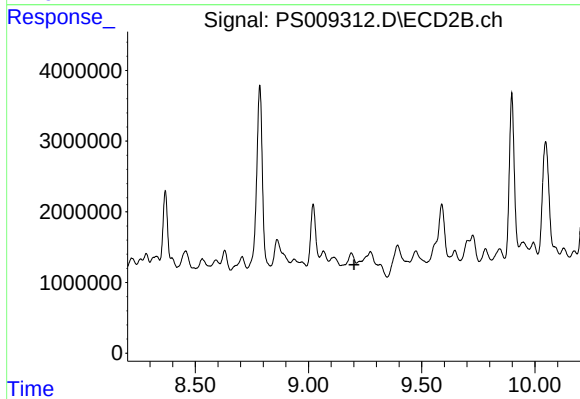

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

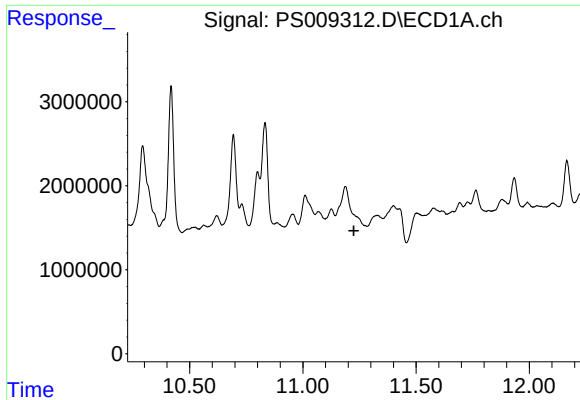

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.225 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

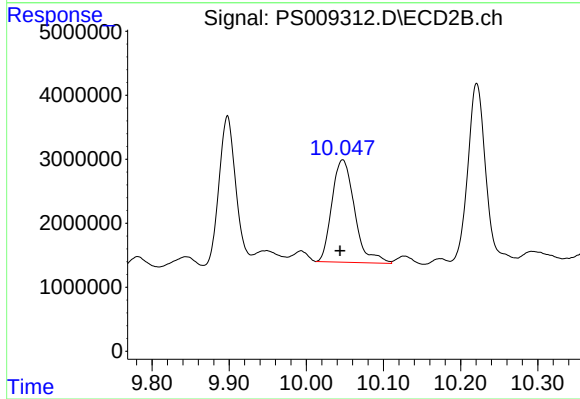


#14 DINOSEB

R.T.: 10.047 min
Delta R.T.: 0.004 min
Response: 32714068
Conc: 14.89 ng/ml

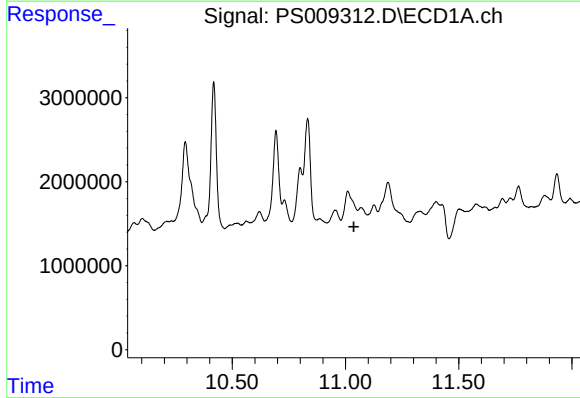


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

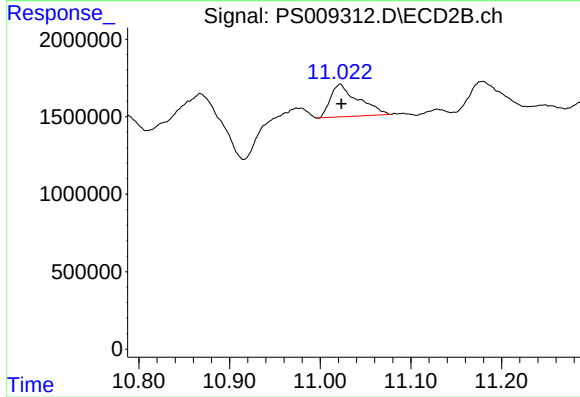

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.002 min
Response: 4464251
Conc: 1.10 ng/ml

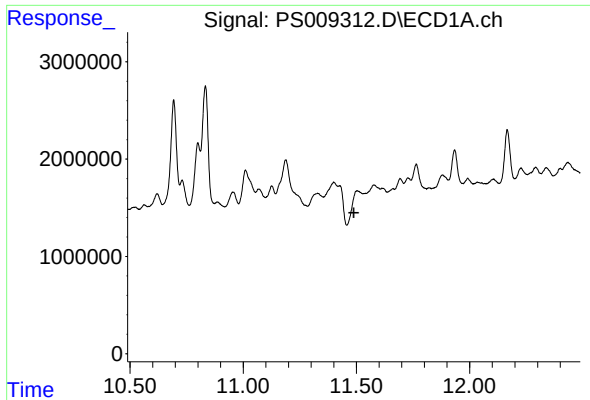

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

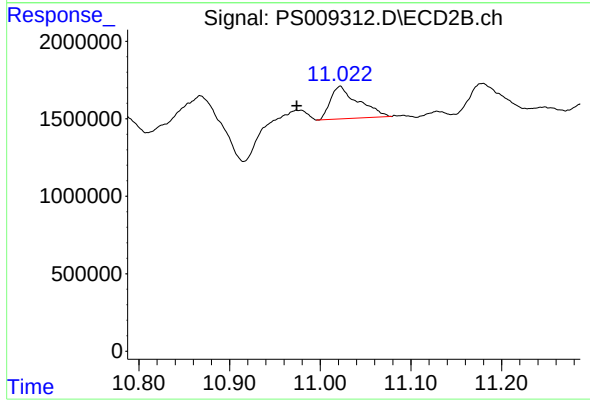

#16 DCPA

R.T.: 11.022 min
Delta R.T.: 0.048 min
Response: 4464251
Conc: 1.15 ng/ml