

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031622\
 Data File : PS018613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 09:31
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 00:14:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.811	1369.2E6	370.2E6	481.120	526.149
Target Compounds							
3) T	4-Nitroph...	7.124f	0.000	2830898	0	1.643	N.D. #
5) T	DICAMBA	7.426	0.000	2383162	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.623	0	8608451	N.D.	10.875
9) T	2,4-D	8.411f	0.000	2435514	0	<MDL	N.D. #
10) T	Pentachlo...	8.661	0.000	7915783	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.214	8.713	8854161	2513563	<MDL	<MDL #
12) T	2,4,5-T	9.496	9.062	11231419	2369585	<MDL	<MDL #
13) T	2,4-DB	10.029	0.000	13603898	0	4.973	N.D. #
14) T	DINOSEB	11.247	9.902	19571850	4727315	1.830	1.543
15) T	Picloram	11.029	10.876	273.6E6	86174722	13.309	16.210
16) T	DCPA	11.483	10.832	3853589	1718230	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031622\
Data File : PS018613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 09:31
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 00:14:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

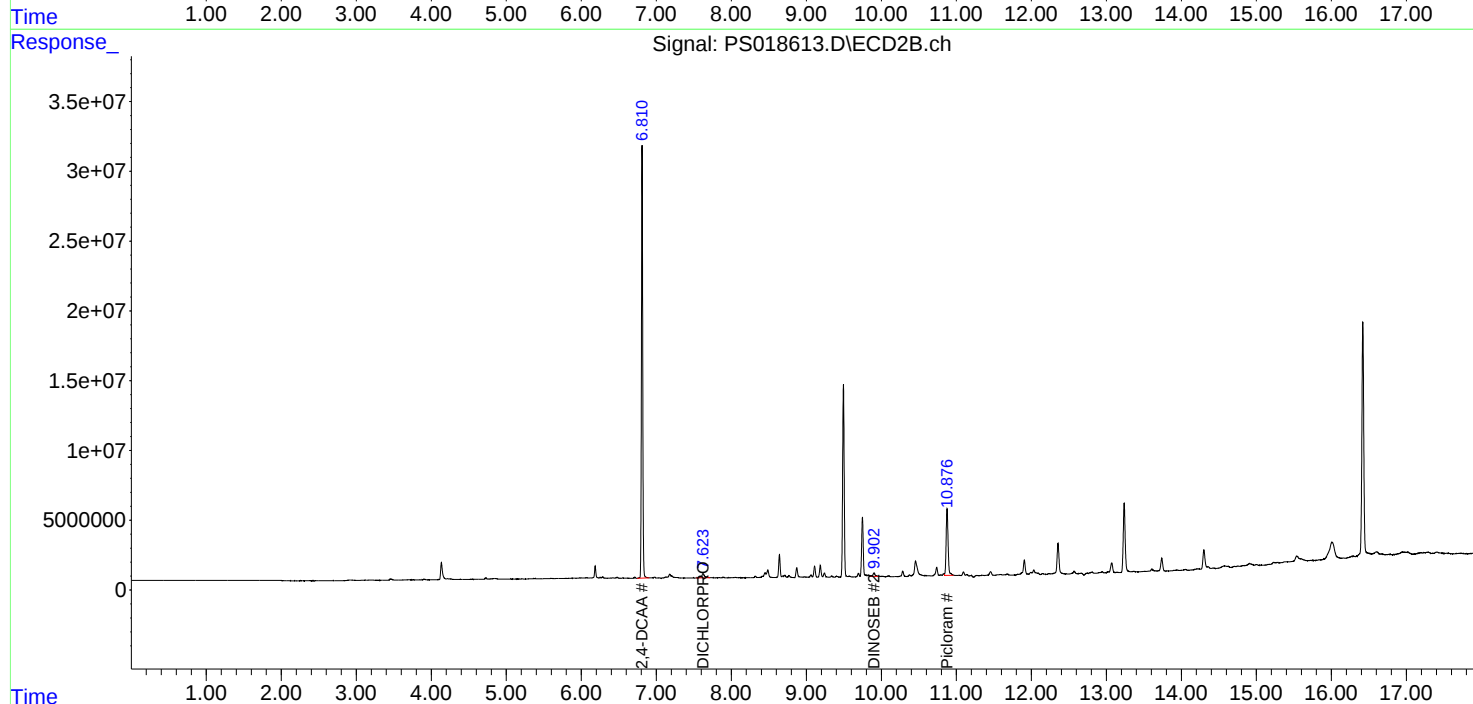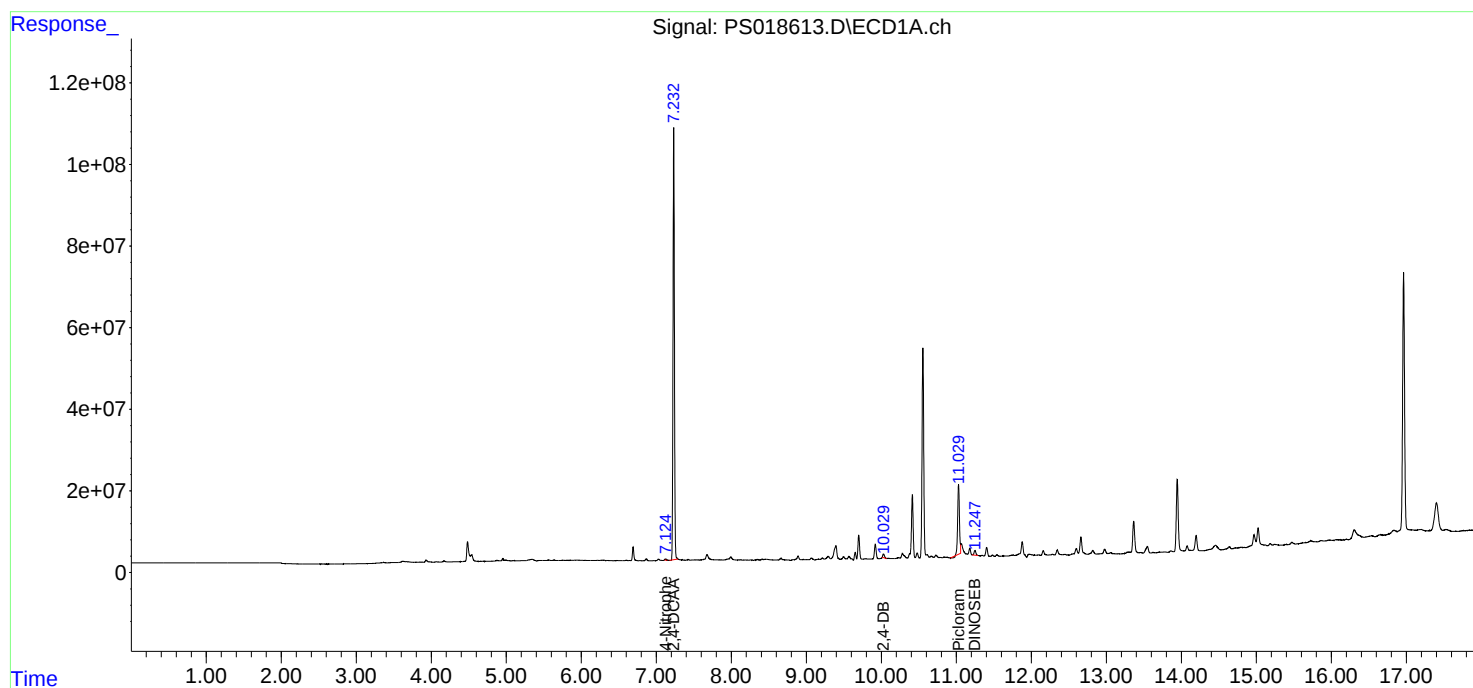


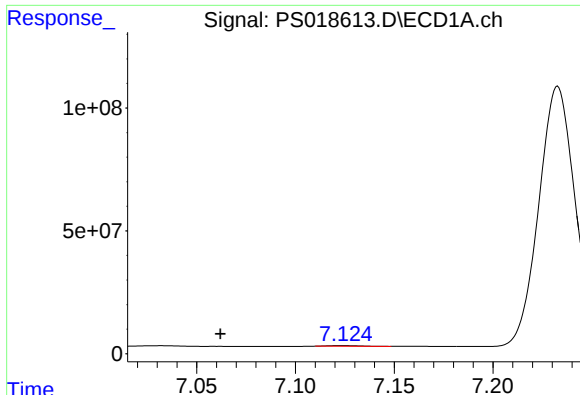

#3 4-Nitrophenol


R.T.: 7.124 min
Delta R.T.: 0.062 min
Response: 2830898
Conc: 1.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

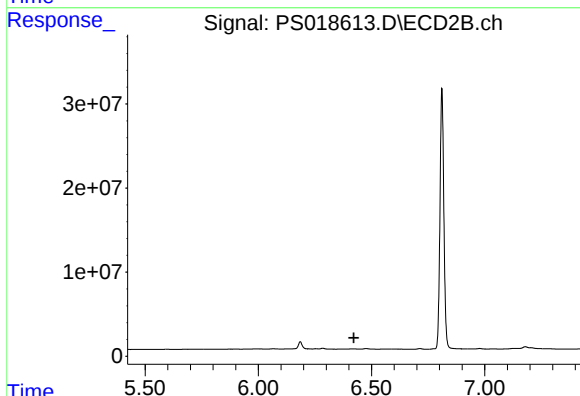


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

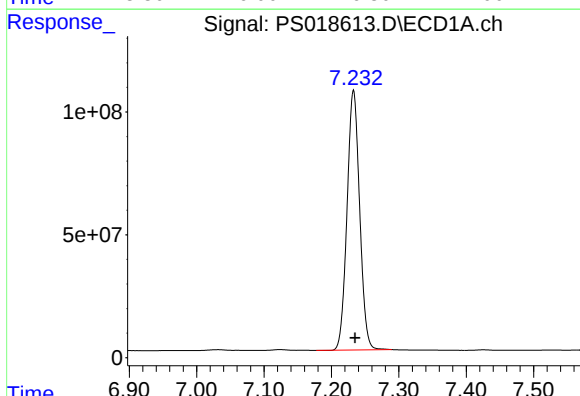


#4 2,4-DCAA

R.T.: 7.233 min
Delta R.T.: -0.002 min
Response: 1369226995
Conc: 481.12 ng/ml

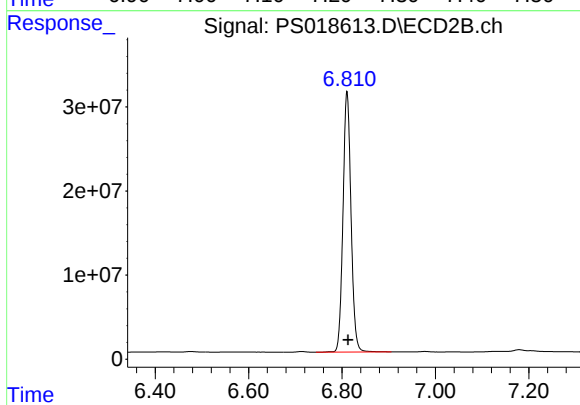

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: -0.002 min
Response: 370227543
Conc: 526.15 ng/ml

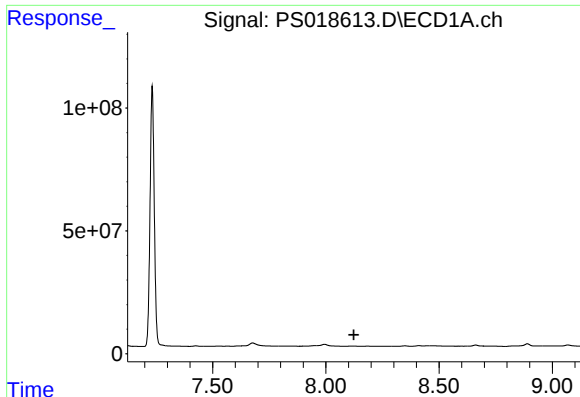

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

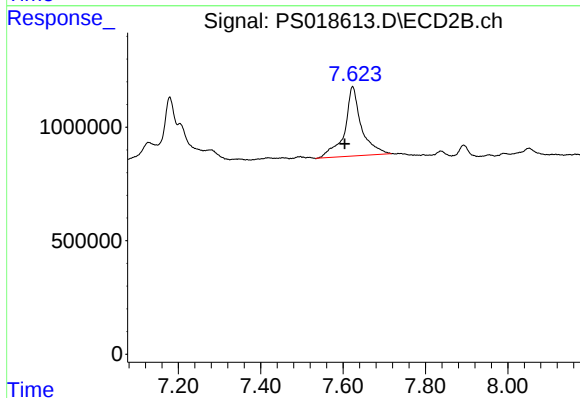


#8 DICHLORPROP

R.T.: 7.623 min
Delta R.T.: 0.019 min
Response: 8608451
Conc: 10.87 ng/ml

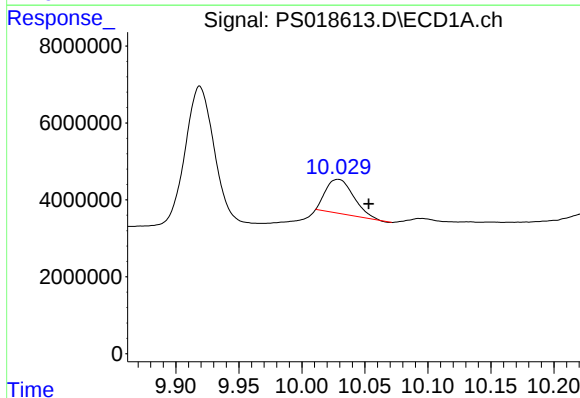


#13 2,4-DB

R.T.: 10.029 min
Delta R.T.: -0.024 min
Response: 13603898
Conc: 4.97 ng/ml

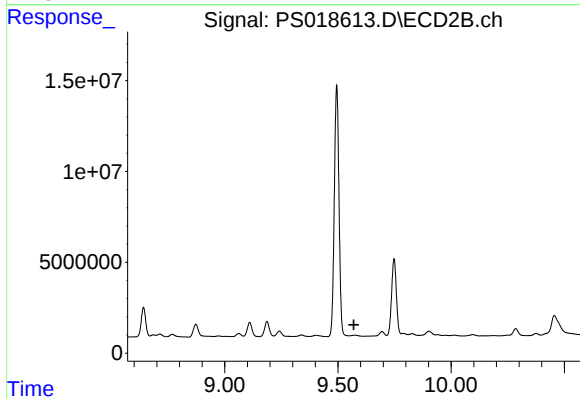

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.570 min
Response: 0
Conc: N.D.

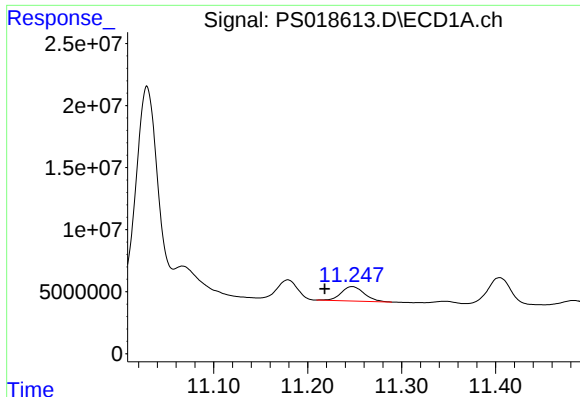

#14 DINOSEB


R.T.: 11.247 min
Delta R.T.: 0.029 min
Response: 19571850
Conc: 1.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

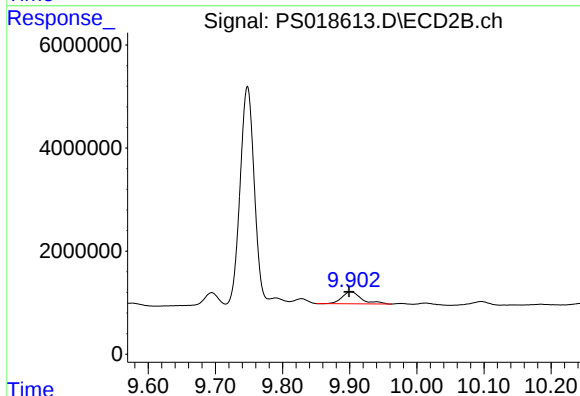


#14 DINOSEB

R.T.: 9.902 min
Delta R.T.: 0.003 min
Response: 4727315
Conc: 1.54 ng/ml

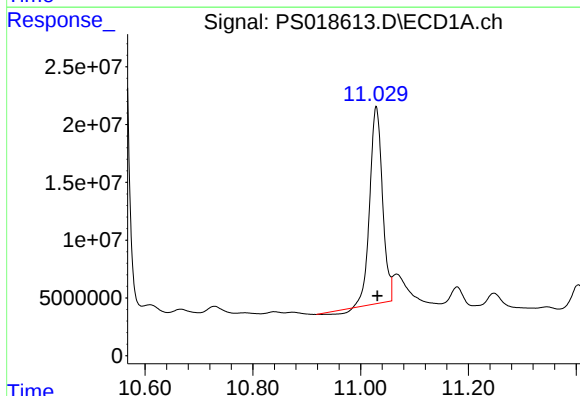

#15 Picloram

R.T.: 11.029 min
Delta R.T.: -0.002 min
Response: 273574087
Conc: 13.31 ng/ml

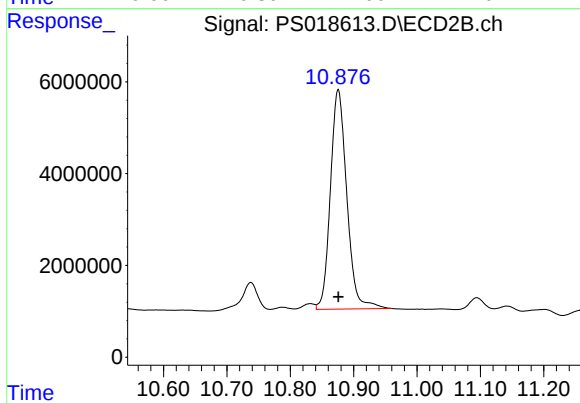

#15 Picloram

R.T.: 10.876 min
Delta R.T.: 0.000 min
Response: 86174722
Conc: 16.21 ng/ml