

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031622\
 Data File : PS018617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 17:30
 Operator : AJ\MA
 Sample : N1890-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 00:15:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.234	6.813	933.5E6	305.3E6	327.997	433.898 #
Target Compounds							
1) T	Dalapon	2.973f	0.000	153.6E6	0	39.497	N.D. #
2) T	3,5-DICHL...	6.478	6.010	88746456	53840989	23.030	51.468 #
3) T	4-Nitroph...	7.045	6.416	979.9E6	6465524	568.679	15.914 #
5) T	DICAMBA	7.439	6.942	112.0E6	177.6E6	10.272	59.622 #
6) T	MCP	7.597	7.077	17519895	9977404	2.064	4.076 #
8) T	DICHLORPROP	8.152	7.580	-13622868	68826770	N.D.	86.945
9) T	2,4-D	8.372	7.883	303.8E6	153.8E6	90.677	164.347 #
10) T	Pentachlo...	8.686	8.326	457.8E6	7465053	12.646	<MDL #
11) T	2,4,5-TP ...	9.280f	8.646f	9747.3E6	14360.4E6	640.923	3292.154 #
12) T	2,4,5-T	9.500	9.055	67965574	715.6E6	4.550	172.769 #
13) T	2,4-DB	10.068	9.595	895.0E6	2129.7E6	327.180	3751.217 #
15) T	Picloram	11.027	10.900	44854.5E6	4779.2E6	2182.092	899.004 #
16) T	DCPA	0.000	10.839	0	129.1E6	N.D.	24.542



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031622\
Data File : PS018617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 17:30
Operator : AJ\MA
Sample : N1890-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 00:15:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

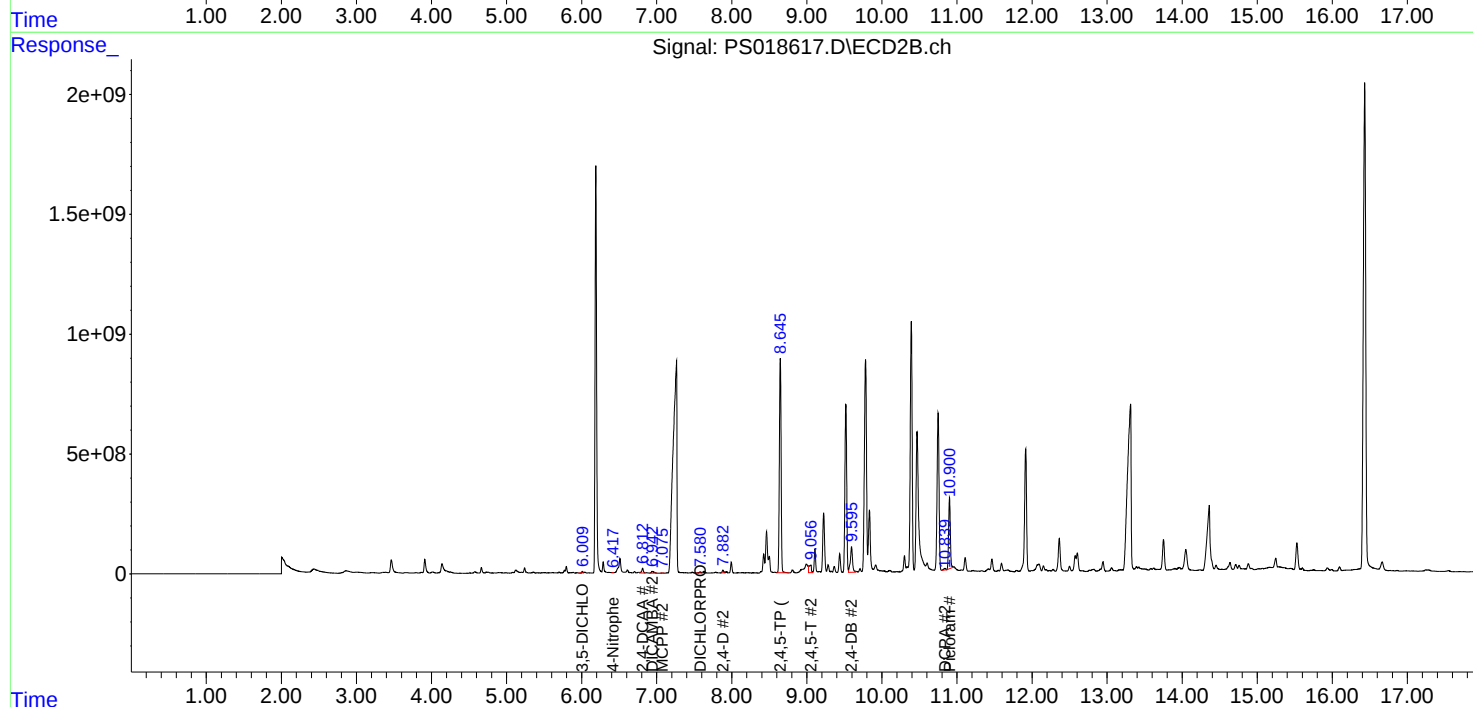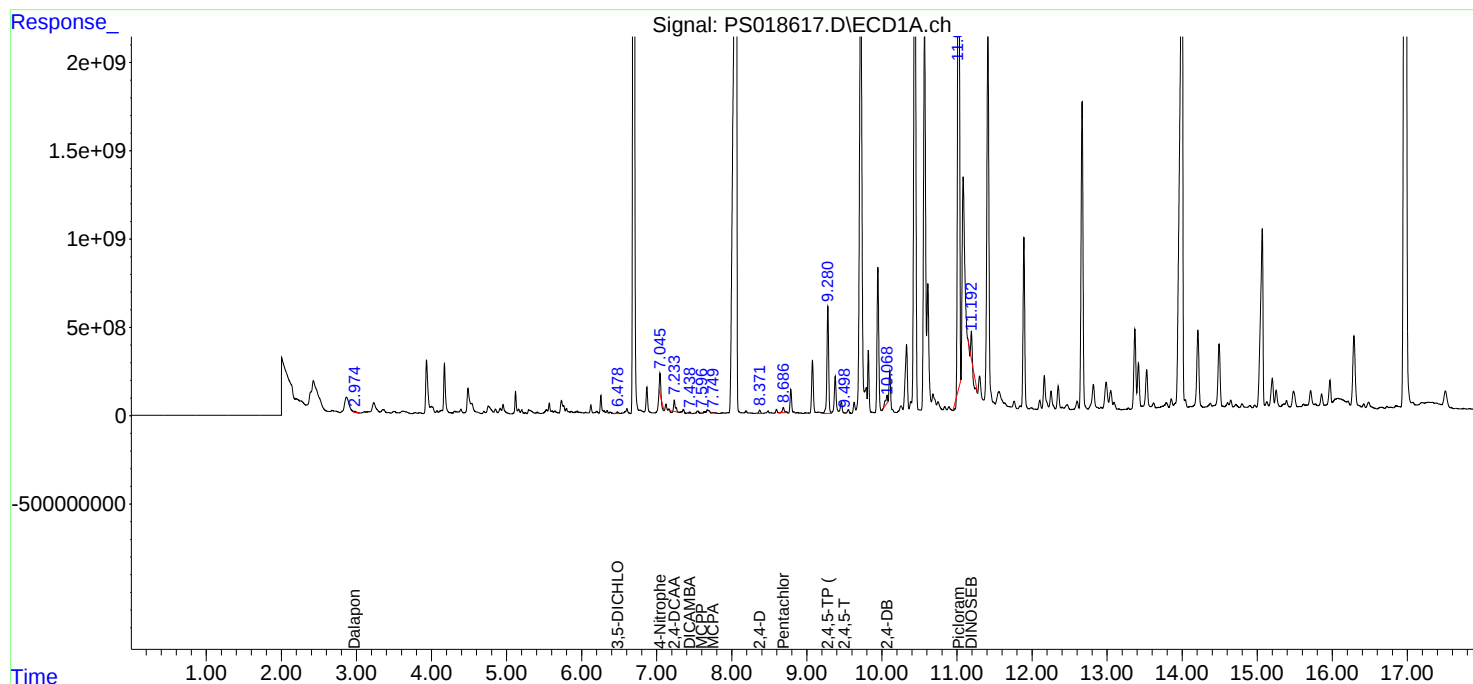


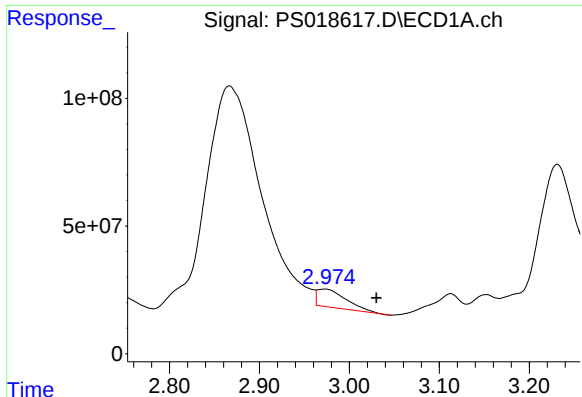

#1 Dalapon


R.T.: 2.973 min
Delta R.T.: -0.057 min
Response: 153584226
Conc: 39.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

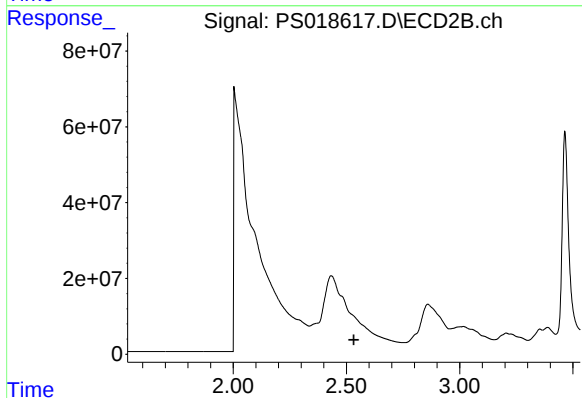


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.533 min
Response: 0
Conc: N.D.

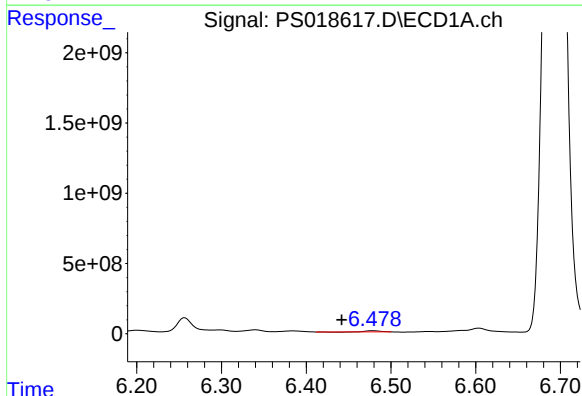


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.478 min
Delta R.T.: 0.036 min
Response: 88746456
Conc: 23.03 ng/ml

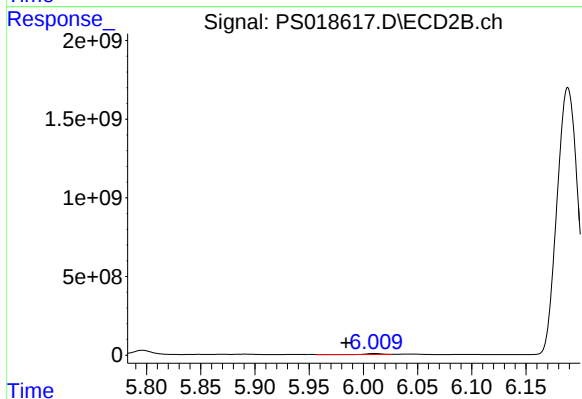

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.010 min
Delta R.T.: 0.026 min
Response: 53840989
Conc: 51.47 ng/ml

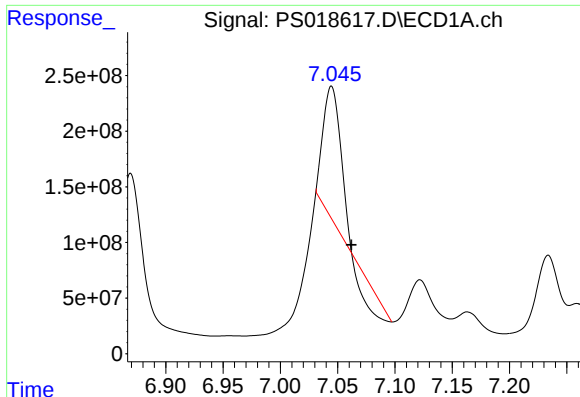

#3 4-Nitrophenol


R.T.: 7.045 min
Delta R.T.: -0.017 min
Response: 979898143
Conc: 568.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

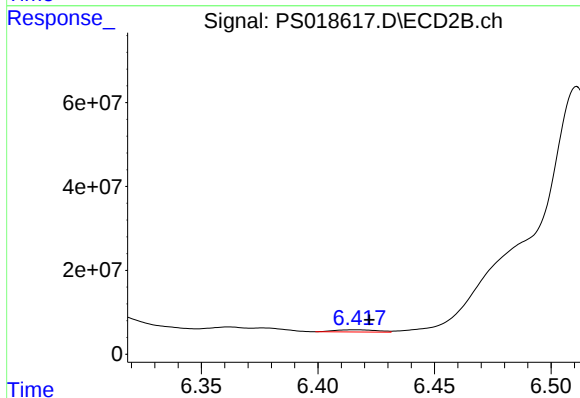


#3 4-Nitrophenol

R.T.: 6.416 min
Delta R.T.: -0.006 min
Response: 6465524
Conc: 15.91 ng/ml

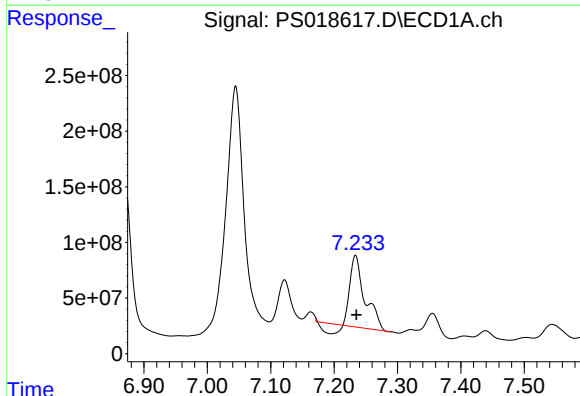


#4 2,4-DCAA

R.T.: 7.234 min
Delta R.T.: -0.001 min
Response: 933452052
Conc: 328.00 ng/ml

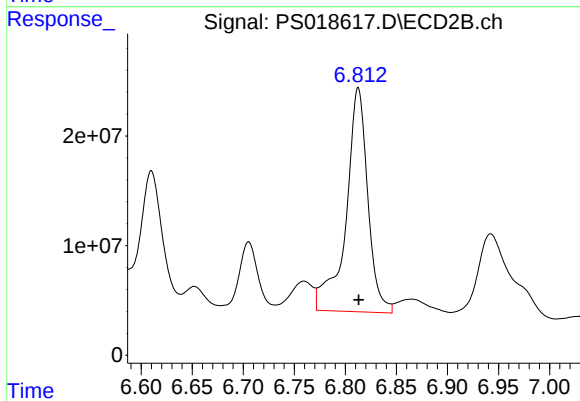

#4 2,4-DCAA


R.T.: 6.813 min
Delta R.T.: 0.000 min
Response: 305314404
Conc: 433.90 ng/ml

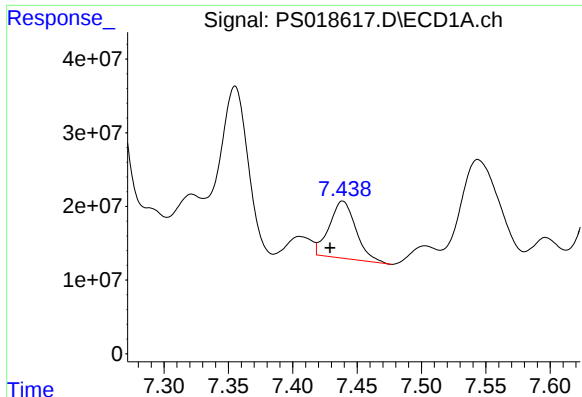

#5 DICAMBA


R.T.: 7.439 min
Delta R.T.: 0.010 min
Response: 112031557
Conc: 10.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

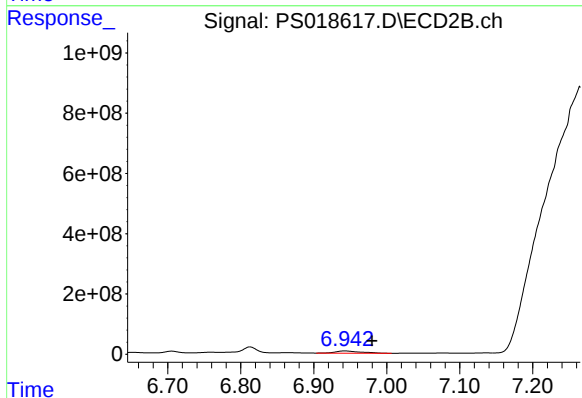


#5 DICAMBA

R.T.: 6.942 min
Delta R.T.: -0.038 min
Response: 177588679
Conc: 59.62 ng/ml

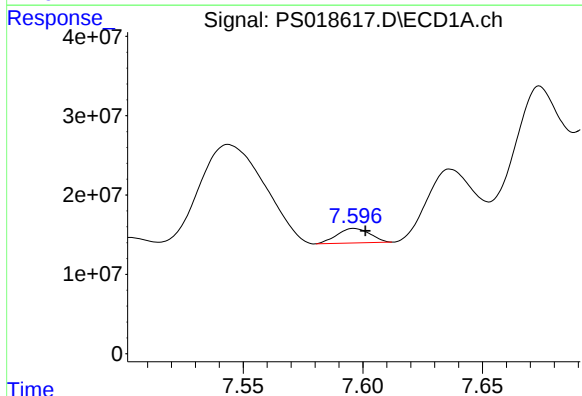


#6 MCP

R.T.: 7.597 min
Delta R.T.: -0.004 min
Response: 17519895
Conc: 2.06 ug/ml

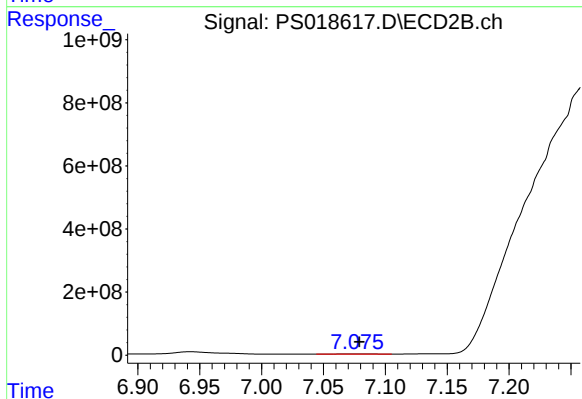

#6 MCP


R.T.: 7.077 min
Delta R.T.: -0.002 min
Response: 9977404
Conc: 4.08 ug/ml

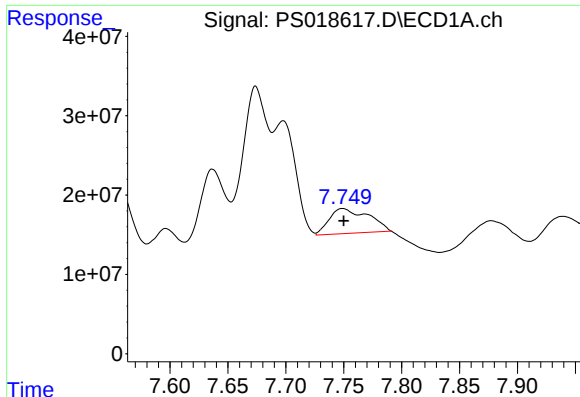

#7 MCPA


R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 74375337
Conc: 6.15 ug/ml

Instrument :
ECD_S
ClientSampleId :

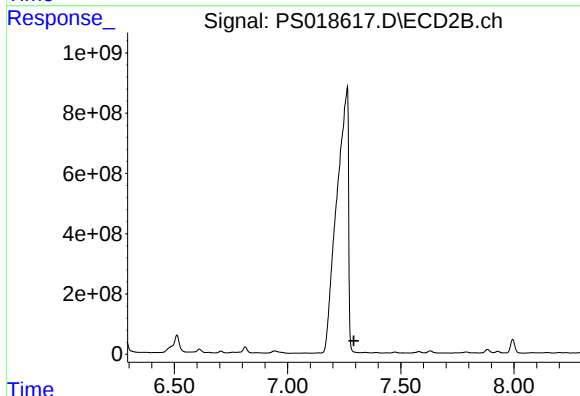


#7 MCPA

R.T.: 7.264 min
Delta R.T.: -0.029 min
Response: -6988955663
Conc: N.D.

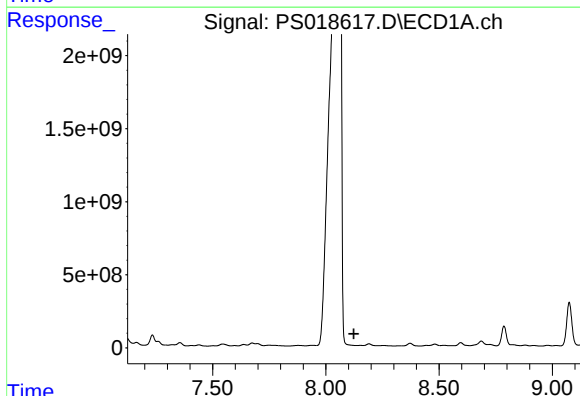


#8 DICHLORPROP

R.T.: 8.152 min
Delta R.T.: 0.028 min
Response: -13622868
Conc: N.D.

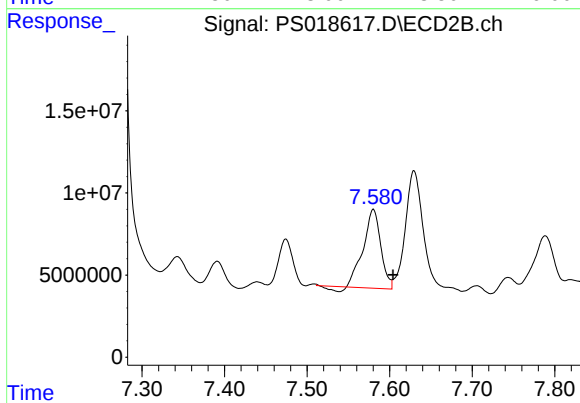

#8 DICHLORPROP


R.T.: 7.580 min
Delta R.T.: -0.024 min
Response: 68826770
Conc: 86.94 ng/ml

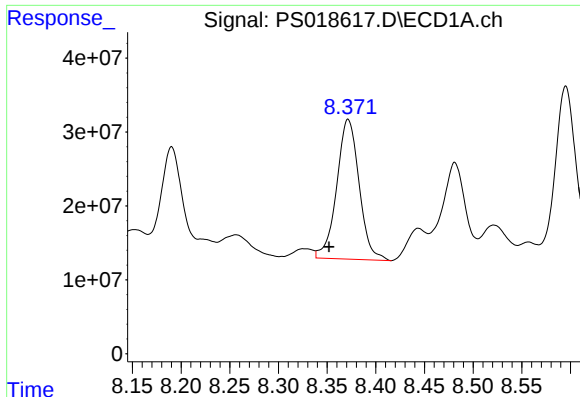

#9 2,4-D


R.T.: 8.372 min
Delta R.T.: 0.020 min
Response: 303826161
Conc: 90.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

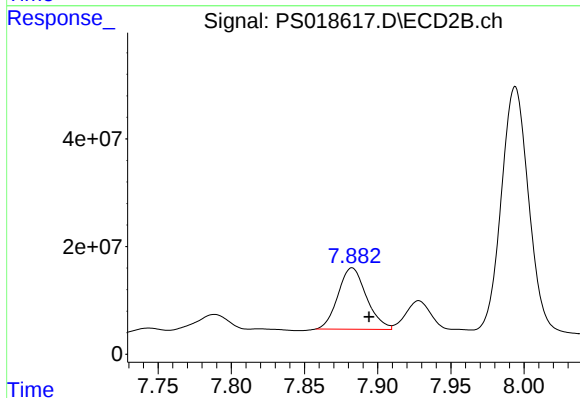


#9 2,4-D

R.T.: 7.883 min
Delta R.T.: -0.011 min
Response: 153831195
Conc: 164.35 ng/ml

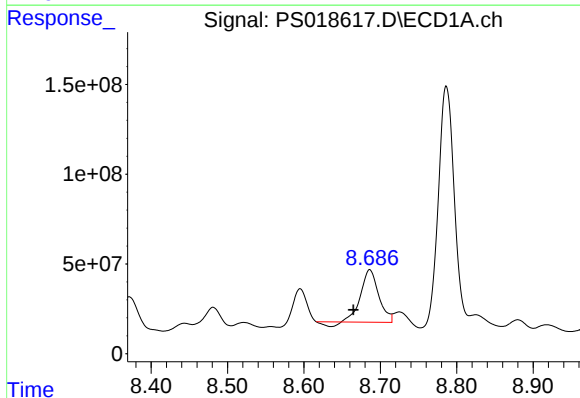


#10 Pentachlorophenol

R.T.: 8.686 min
Delta R.T.: 0.021 min
Response: 457805895
Conc: 12.65 ng/ml

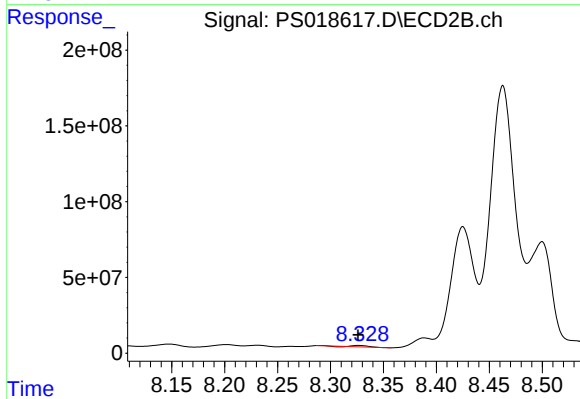

#10 Pentachlorophenol


R.T.: 8.326 min
Delta R.T.: 0.000 min
Response: 7465053
Conc: N.D.

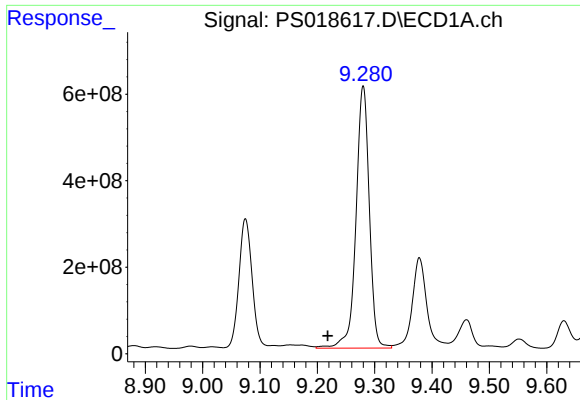

#11 2,4,5-TP (SILVEX)


R.T.: 9.280 min
Delta R.T.: 0.062 min
Response: 9747277592
Conc: 640.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

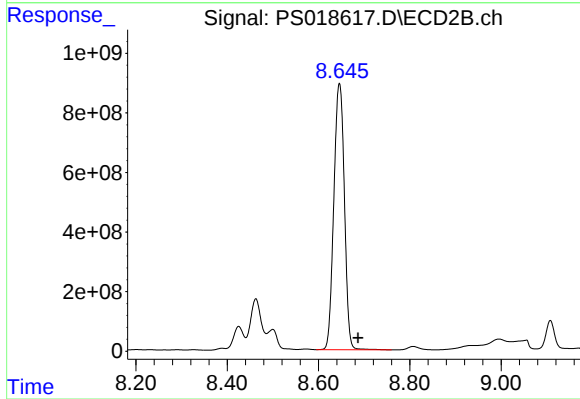


#11 2,4,5-TP (SILVEX)

R.T.: 8.646 min
Delta R.T.: -0.041 min
Response: 14360367182
Conc: 3292.15 ng/ml

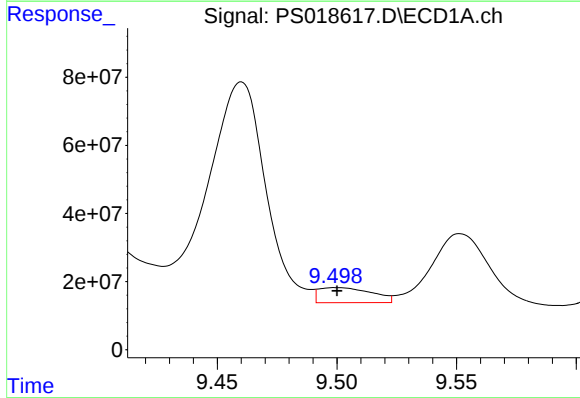


#12 2,4,5-T

R.T.: 9.500 min
Delta R.T.: 0.000 min
Response: 67965574
Conc: 4.55 ng/ml

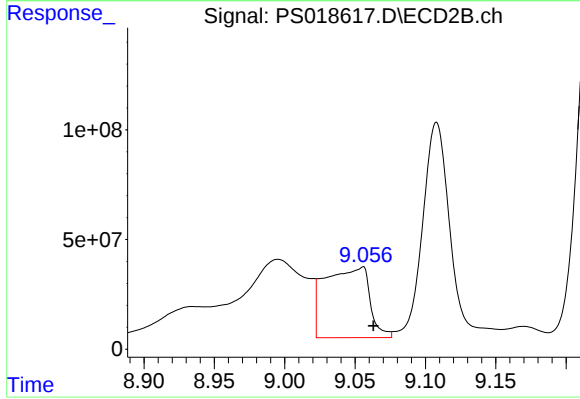

#12 2,4,5-T


R.T.: 9.055 min
Delta R.T.: -0.008 min
Response: 715639796
Conc: 172.77 ng/ml

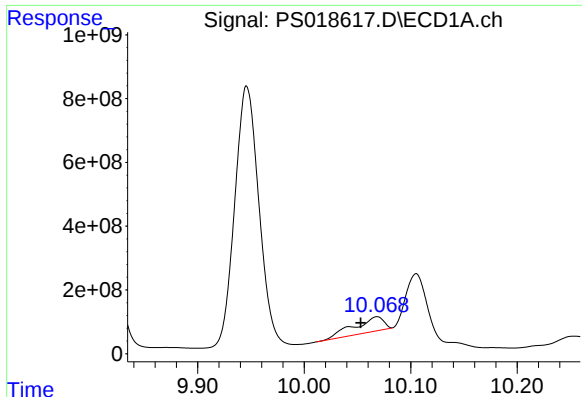

#13 2,4-DB


R.T.: 10.068 min
Delta R.T.: 0.015 min
Response: 894972351
Conc: 327.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

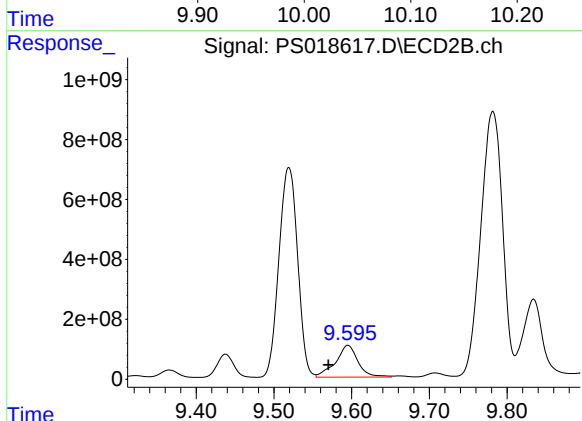


#13 2,4-DB

R.T.: 9.595 min
Delta R.T.: 0.025 min
Response: 2129747151
Conc: 3751.22 ng/ml

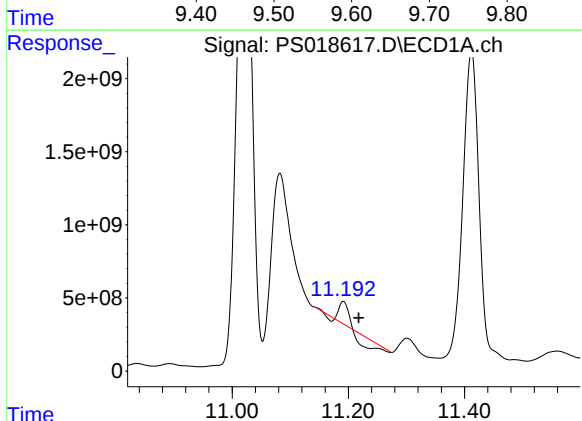


#14 DINOSEB

R.T.: 11.191 min
Delta R.T.: -0.027 min
Response: 59471650
Conc: 5.56 ng/ml

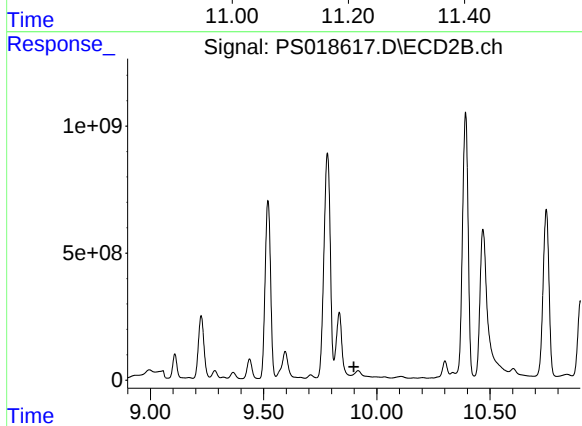

#14 DINOSEB


R.T.: 9.917 min
Delta R.T.: 0.018 min
Response: -156550856
Conc: N.D.

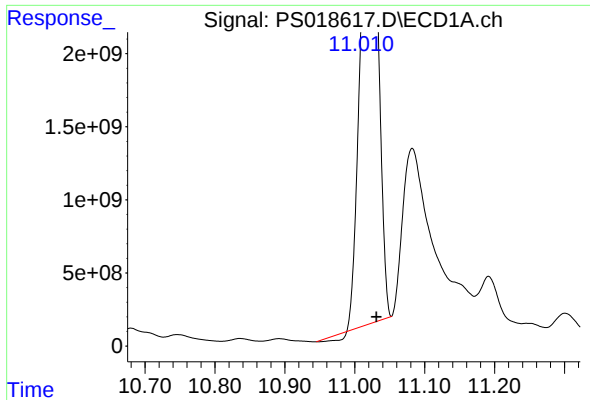

#15 Picloram


R.T.: 11.027 min
Delta R.T.: -0.004 min
Response: 44854500681
Conc: 2182.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

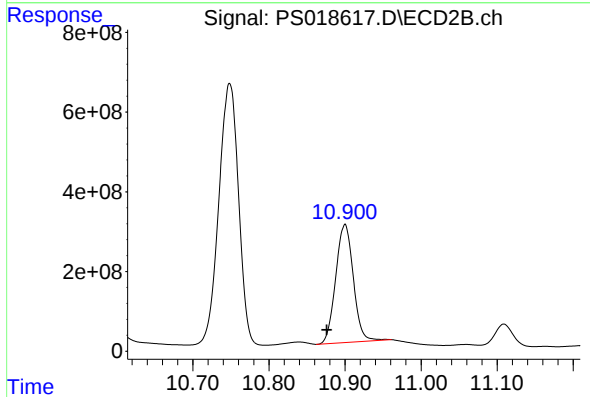


#15 Picloram

R.T.: 10.900 min
Delta R.T.: 0.024 min
Response: 4779194000
Conc: 899.00 ng/ml

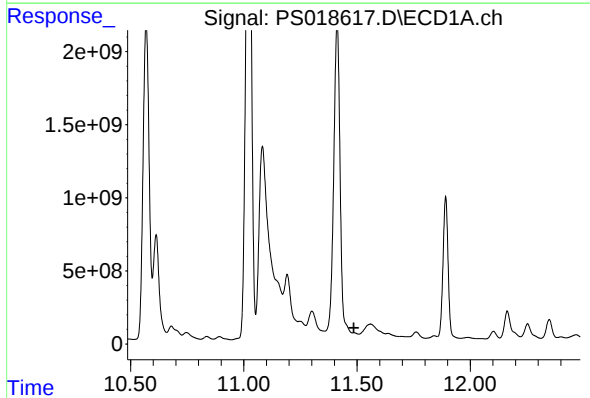

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.486 min
Response: 0
Conc: N.D.

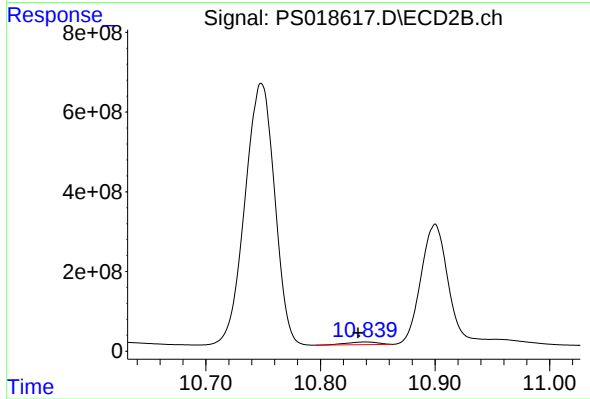

#16 DCPA

R.T.: 10.839 min
Delta R.T.: 0.006 min
Response: 129071463
Conc: 24.54 ng/ml