

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031622\
 Data File : PS018620.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 18:42
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 00:16:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	6.811	1390.6E6	386.8E6	488.646	549.737
Target Compounds							
3) T	4-Nitroph...	7.123f	6.476f	11885477	6112976	6.898	15.046 #
5) T	DICAMBA	7.492f	0.000	8148302	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.623	0	21498210	N.D.	27.157
9) T	2,4-D	8.411f	0.000	3879078	0	1.158	N.D. #
10) T	Pentachlo...	8.687	0.000	5367323	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.218	8.707	35117110	8325295	2.309	1.909
12) T	2,4,5-T	9.494	9.061	7006736	1346084	<MDL	<MDL #
13) T	2,4-DB	10.023	0.000	3489854	0	1.276	N.D. #
14) T	DINOSEB	11.250	0.000	6276700	0	<MDL	N.D. #
15) T	Picloram	11.026	10.878	55183877	63387826	2.685	11.924 #
16) T	DCPA	11.484	10.791f	2876054	4742937	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031622\
Data File : PS018620.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 18:42
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 00:16:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

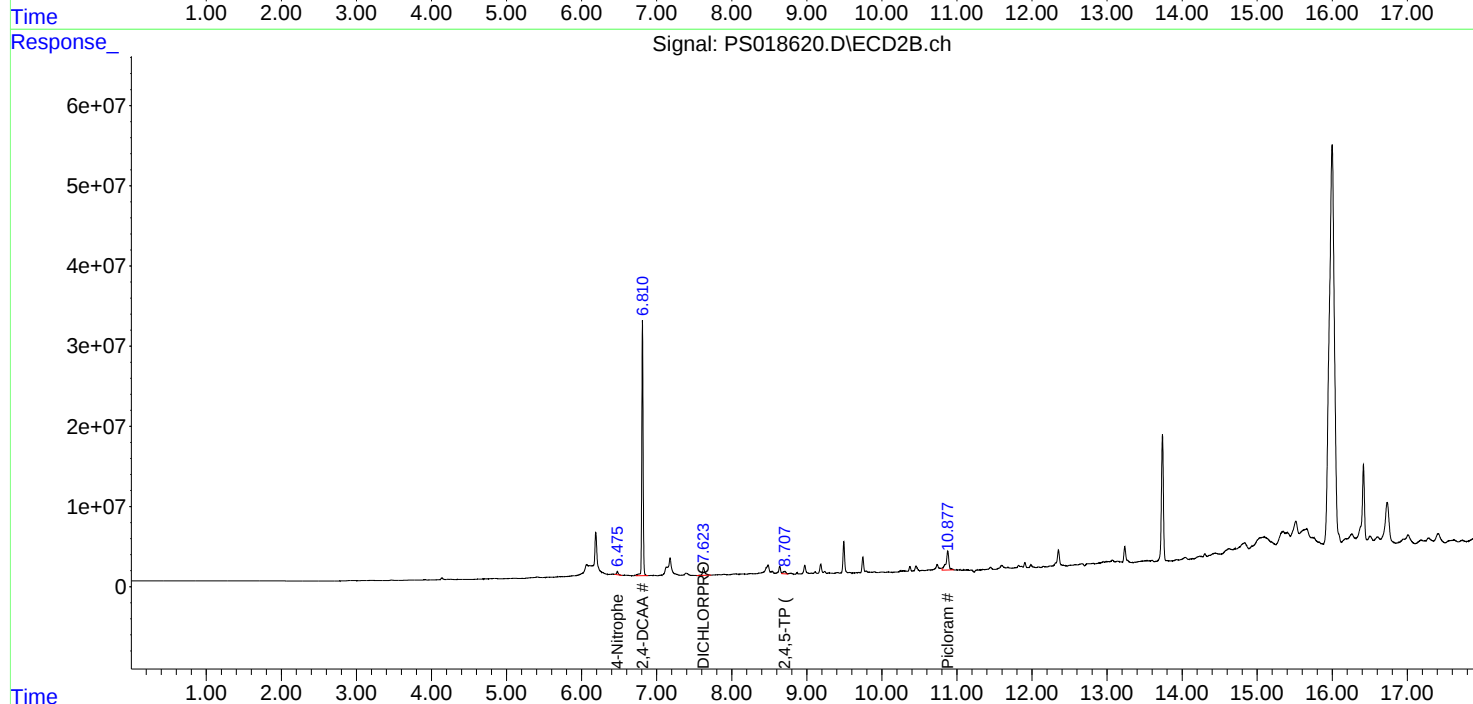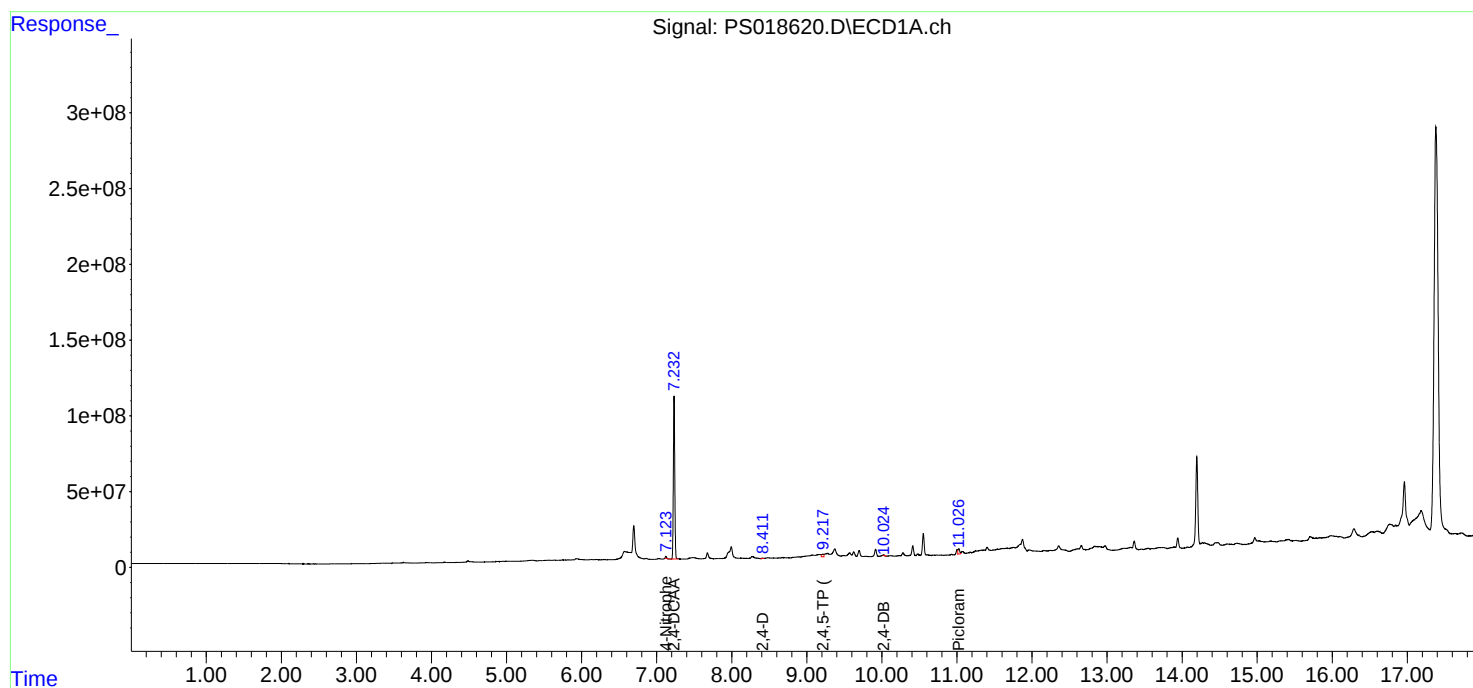


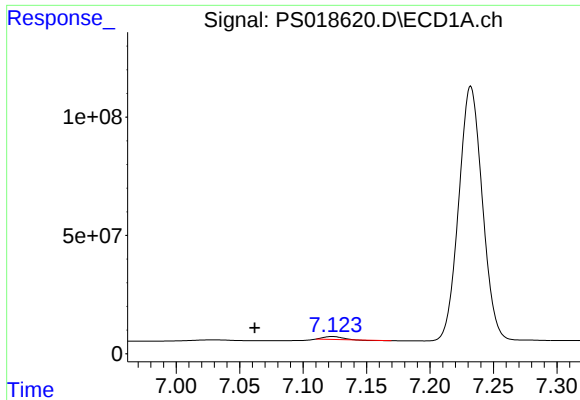

#3 4-Nitrophenol


R.T.: 7.123 min
Delta R.T.: 0.061 min
Response: 11885477
Conc: 6.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

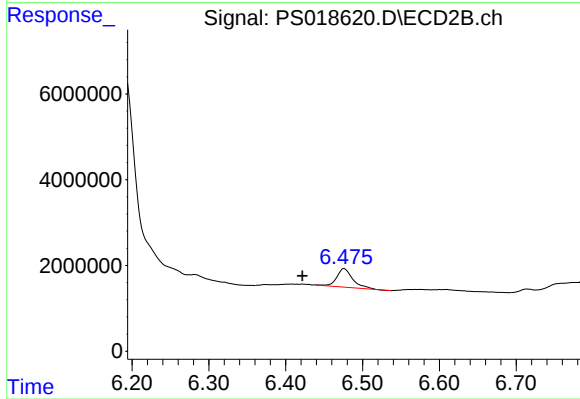


#3 4-Nitrophenol

R.T.: 6.476 min
Delta R.T.: 0.054 min
Response: 6112976
Conc: 15.05 ng/ml

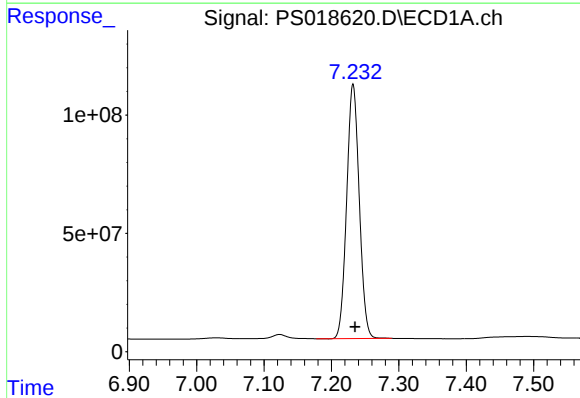


#4 2,4-DCAA

R.T.: 7.232 min
Delta R.T.: -0.003 min
Response: 1390646052
Conc: 488.65 ng/ml

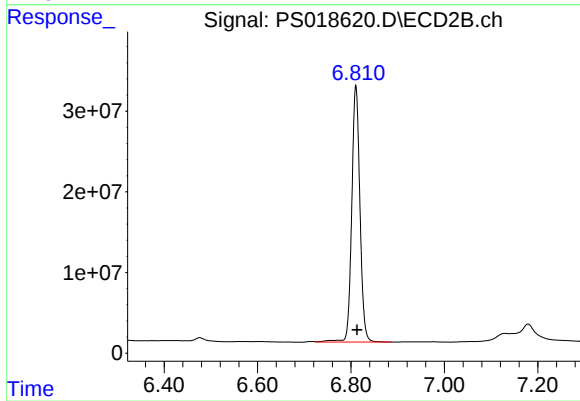

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: -0.002 min
Response: 386825545
Conc: 549.74 ng/ml

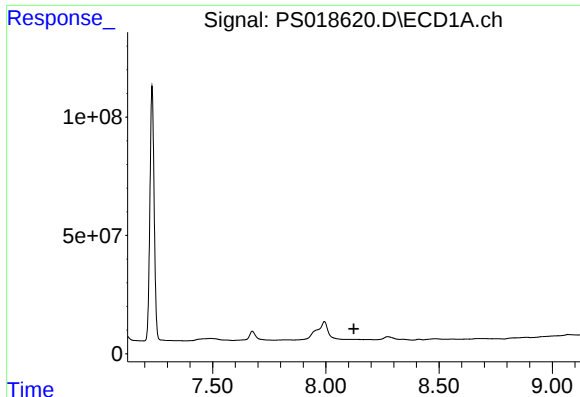

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

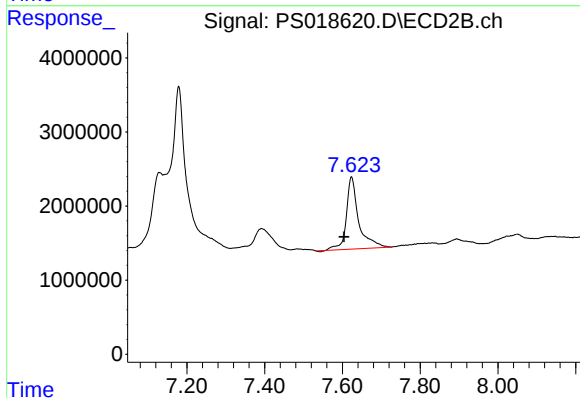


#8 DICHLORPROP

R.T.: 7.623 min
Delta R.T.: 0.019 min
Response: 21498210
Conc: 27.16 ng/ml

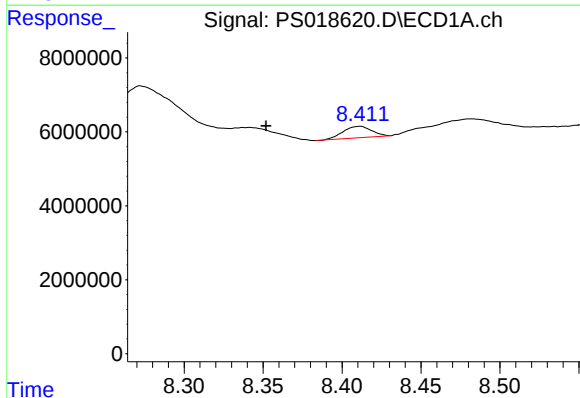


#9 2,4-D

R.T.: 8.411 min
Delta R.T.: 0.059 min
Response: 3879078
Conc: 1.16 ng/ml

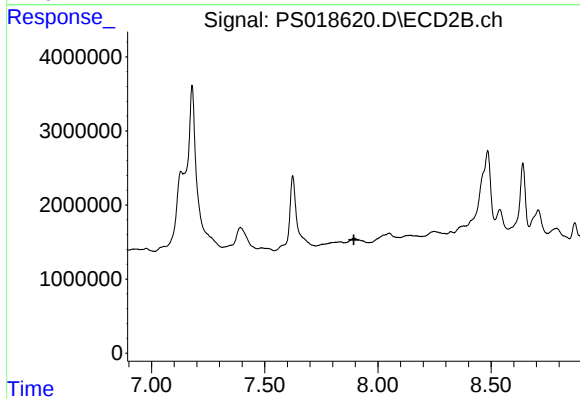

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.894 min
Response: 0
Conc: N.D.

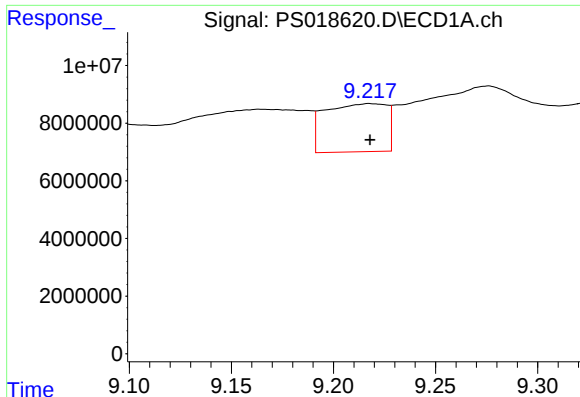

#11 2,4,5-TP (SILVEX)


R.T.: 9.218 min
Delta R.T.: 0.000 min
Response: 35117110
Conc: 2.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

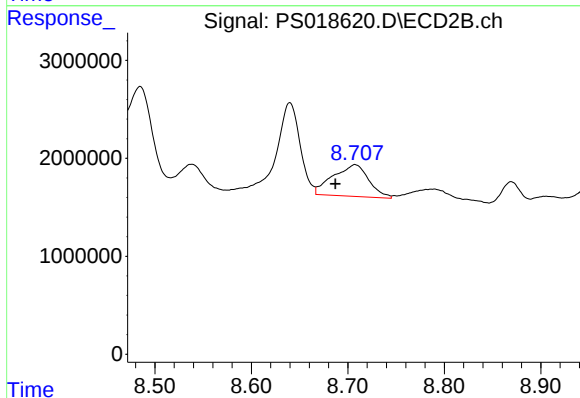


#11 2,4,5-TP (SILVEX)

R.T.: 8.707 min
Delta R.T.: 0.020 min
Response: 8325295
Conc: 1.91 ng/ml

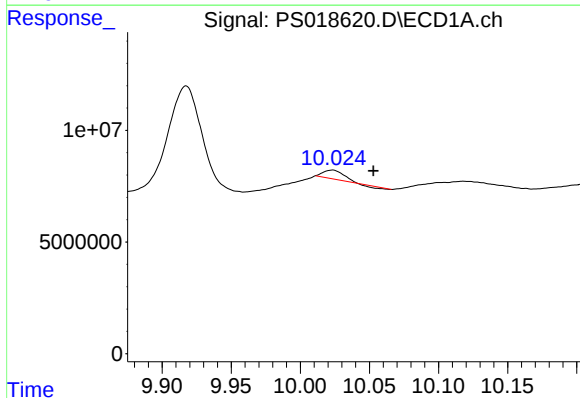


#13 2,4-DB

R.T.: 10.023 min
Delta R.T.: -0.030 min
Response: 3489854
Conc: 1.28 ng/ml

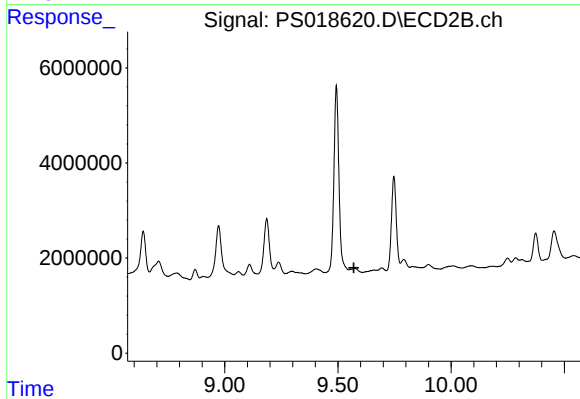

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.570 min
Response: 0
Conc: N.D.

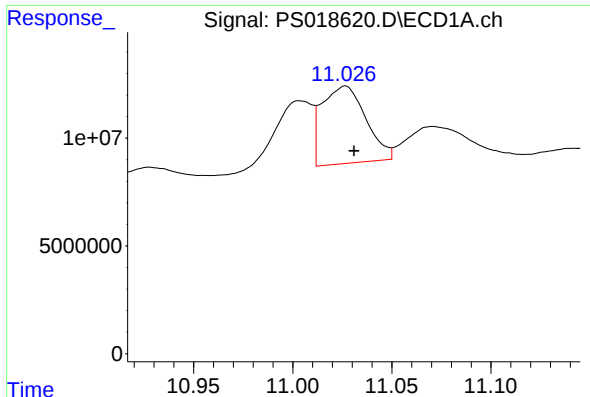

#15 Picloram

R.T.: 11.026 min
Delta R.T.: -0.005 min
Response: 55183877
Conc: 2.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

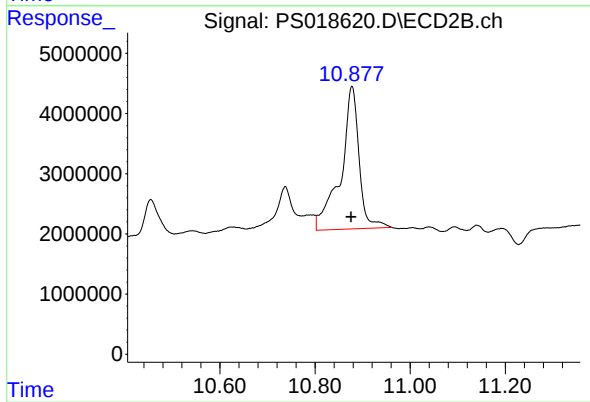

#15 Picloram

R.T.: 10.878 min
Delta R.T.: 0.002 min
Response: 63387826
Conc: 11.92 ng/ml