

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031623\
 Data File : PS022397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 08:36
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 21:41:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.310	0.000	620634	0	<MDL	N.D.	#
Target Compounds								
1) T	Dalapon	2.447	2.508	1396679	76159	<MDL	<MDL	#
3) T	4-Nitroph...	6.139	0.000	4798721	0	3.771	N.D.	#
5) T	DICAMBA	6.444	6.928f	574836	5068179	<MDL	<MDL	#
6) T	MCP	0.000	7.021	0	825917	N.D.	<MDL	
8) T	DICHLORPROP	0.000	7.537	0	2860956	N.D.	1.164	
9) T	2,4-D	7.197	0.000	72511480	0	22.116	N.D.	#
10) T	Pentachlo...	7.448	8.209	2460269	1191534	<MDL	<MDL	#
11) T	2,4,5-TP ...	7.984	8.576	7232995	1729639	<MDL	<MDL	#
12) T	2,4,5-T	8.261	8.970	7162466	1902417	<MDL	<MDL	#
13) T	2,4-DB	8.737	9.524f	1223584	2976461	<MDL	1.793	#
15) T	Picloram	9.604	10.753	110.2E6	28624639	4.472	1.460	#
16) T	DCPA	10.044	10.699	3577964	43344094	<MDL	2.771	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031623\
Data File : PS022397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 08:36
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 21:41:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

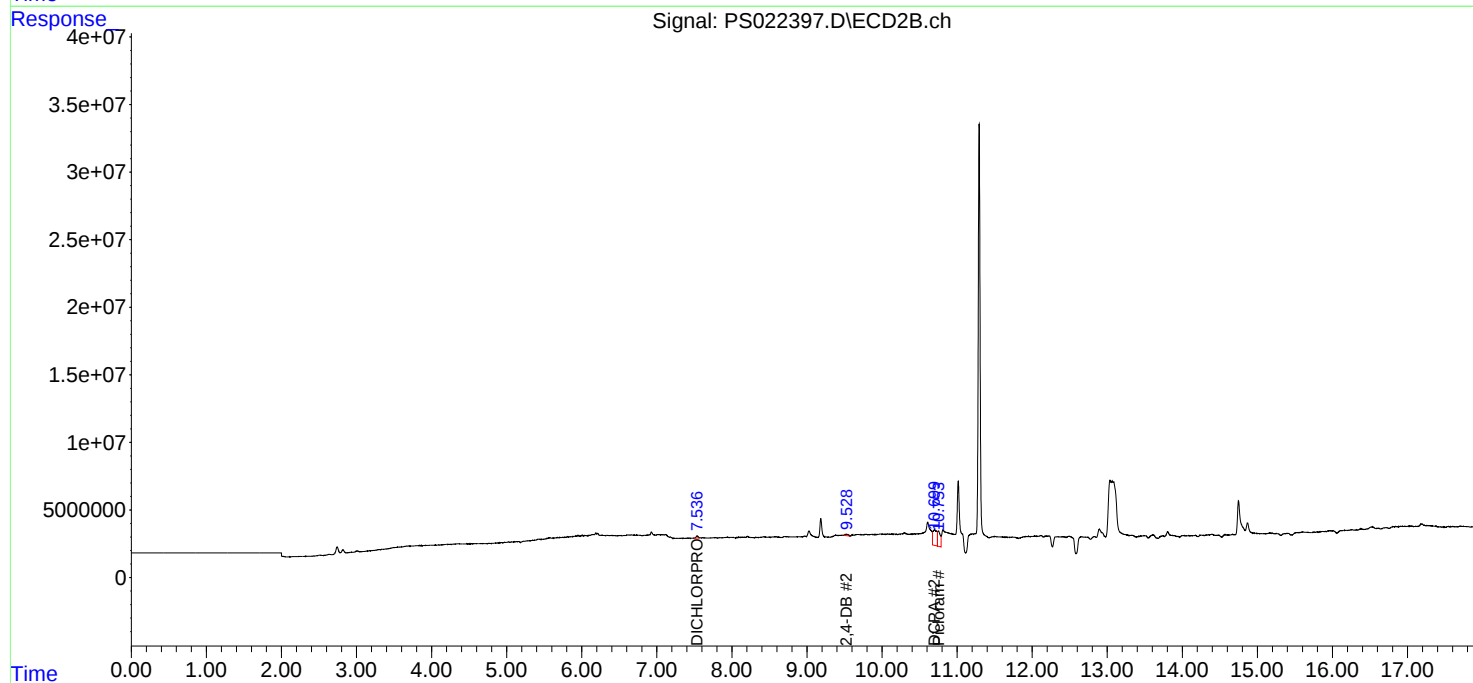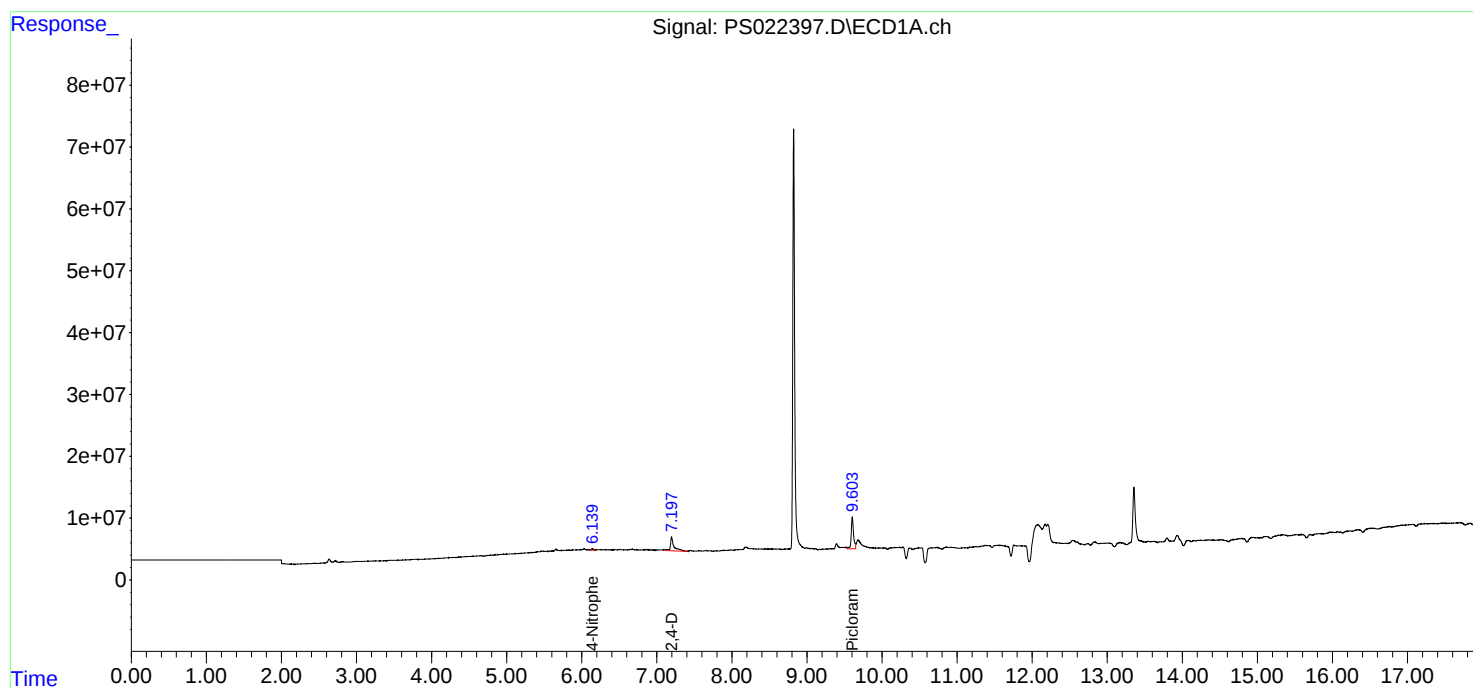


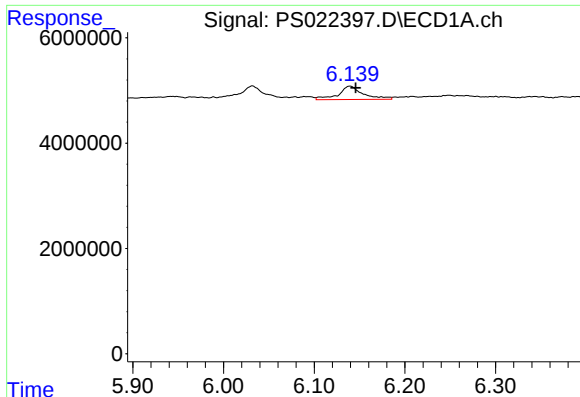

#3 4-Nitrophenol


R.T.: 6.139 min
Delta R.T.: -0.006 min
Response: 4798721
Conc: 3.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

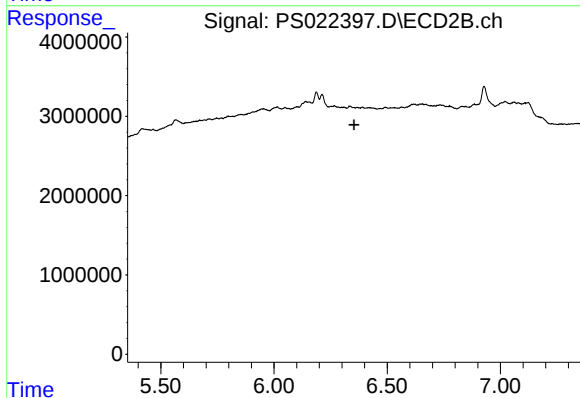


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

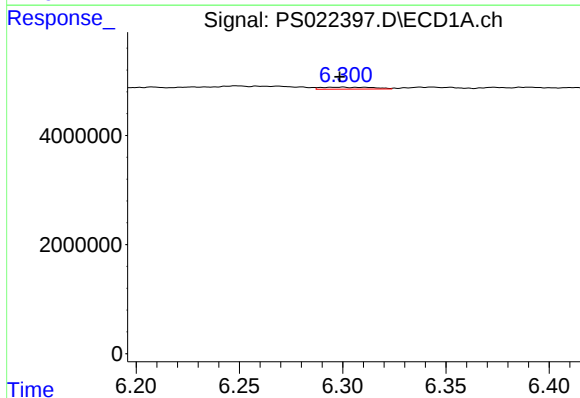


#4 2,4-DCAA

R.T.: 6.310 min
Delta R.T.: 0.011 min
Response: 620634
Conc: N.D.

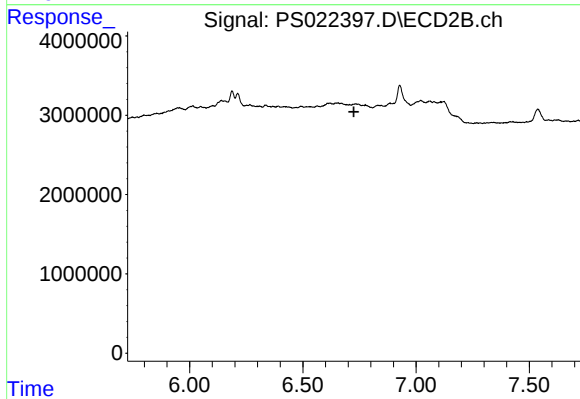

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.726 min
Response: 0
Conc: N.D.

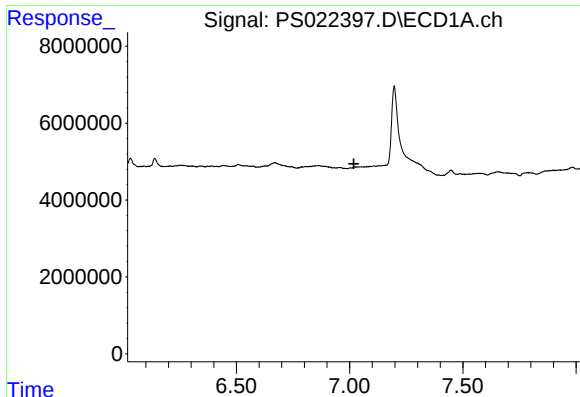

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

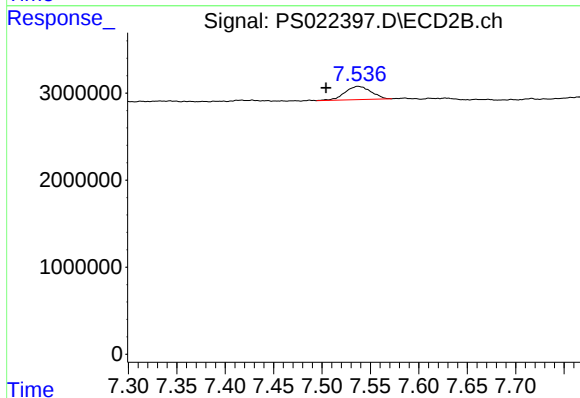


#8 DICHLORPROP

R.T.: 7.537 min
Delta R.T.: 0.033 min
Response: 2860956
Conc: 1.16 ng/ml

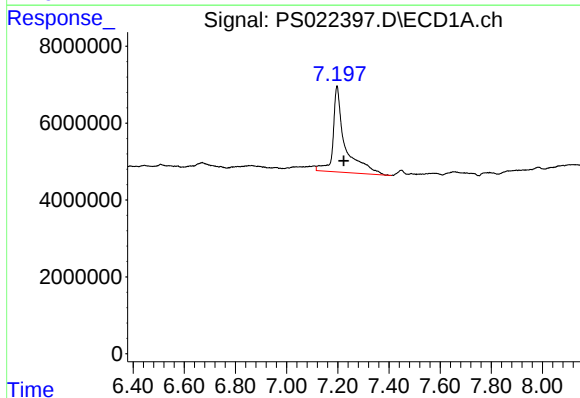


#9 2,4-D

R.T.: 7.197 min
Delta R.T.: -0.026 min
Response: 72511480
Conc: 22.12 ng/ml

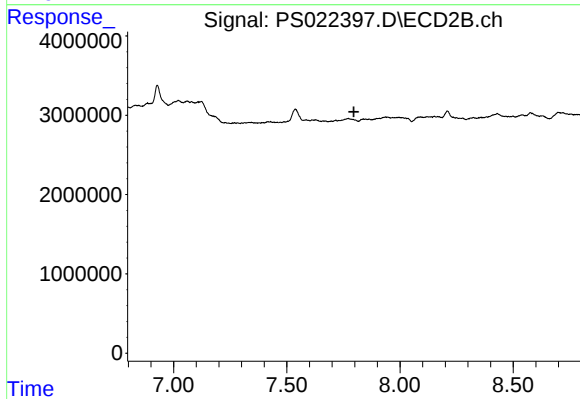

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.796 min
Response: 0
Conc: N.D.

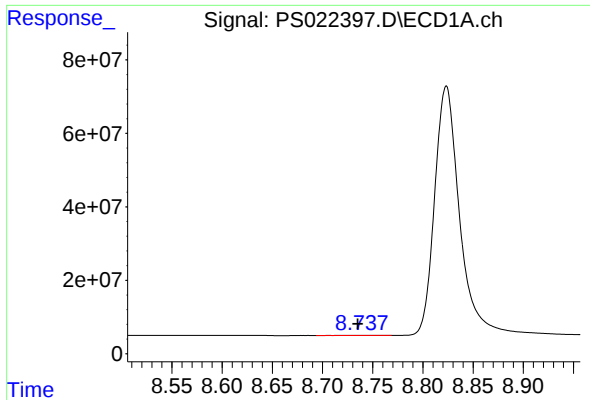

#13 2,4-DB


R.T.: 8.737 min
Delta R.T.: 0.002 min
Response: 1223584
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

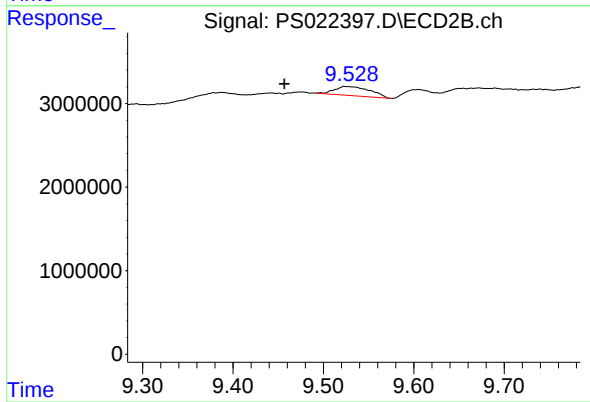


#13 2,4-DB

R.T.: 9.524 min
Delta R.T.: 0.067 min
Response: 2976461
Conc: 1.79 ng/ml

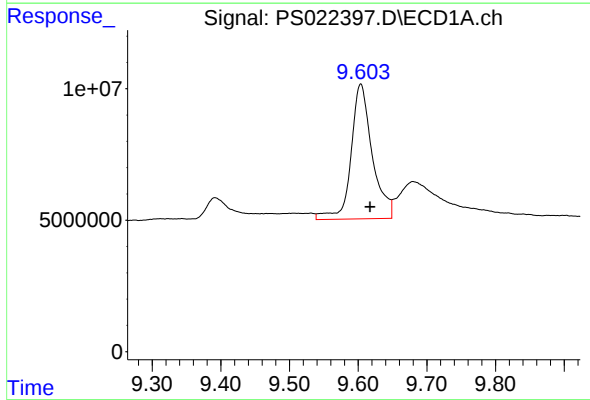


#15 Picloram

R.T.: 9.604 min
Delta R.T.: -0.014 min
Response: 110169395
Conc: 4.47 ng/ml

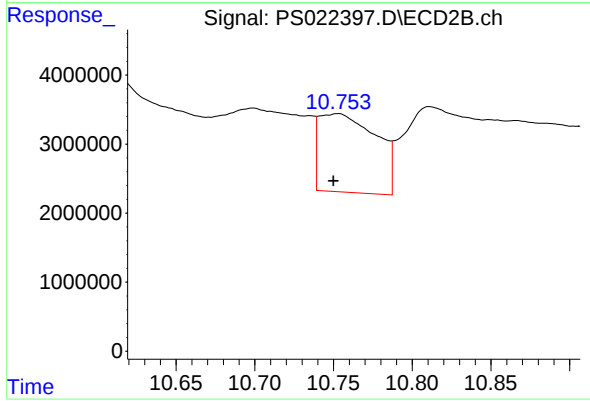

#15 Picloram


R.T.: 10.753 min
Delta R.T.: 0.003 min
Response: 28624639
Conc: 1.46 ng/ml

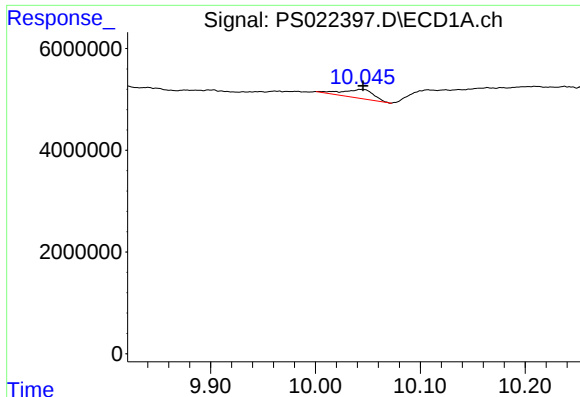

#16 DCPA

R.T.: 10.044 min
Delta R.T.: -0.001 min
Response: 3577964
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

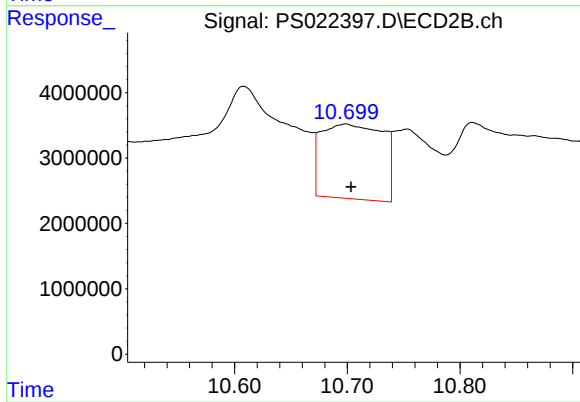

#16 DCPA

R.T.: 10.699 min
Delta R.T.: -0.005 min
Response: 43344094
Conc: 2.77 ng/ml