

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
 Data File : PS009323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2020 08:49
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 11:51:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.933	247.9E6	263.1E6	448.129	479.047
Target Compounds							
12) T	2,4,5-T	0.000	9.252	0	9127292	N.D.	3.092
15) T	Picloram	11.037	11.023	18671592	31479400	6.152	7.730 #
16) T	DCPA	0.000	11.023	0	31479400	N.D.	8.128



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
Data File : PS009323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2020 08:49
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 11:51:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

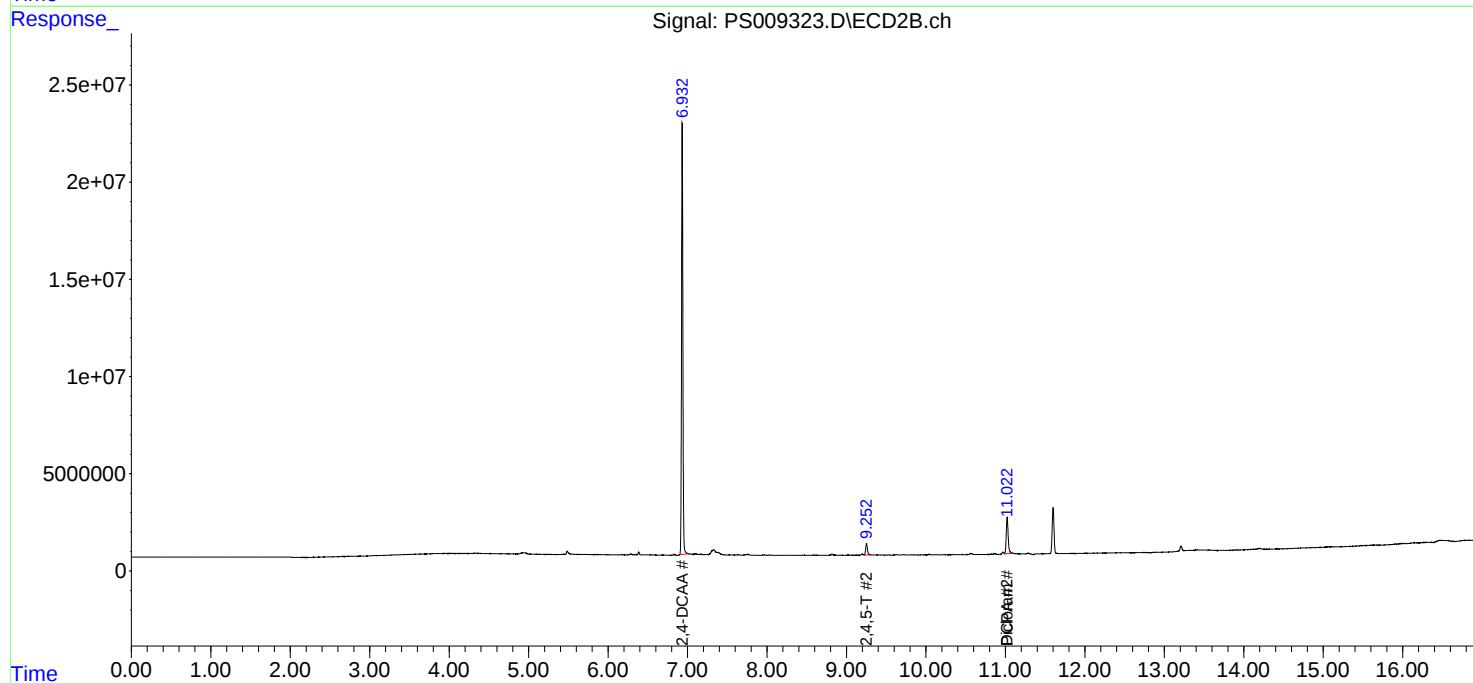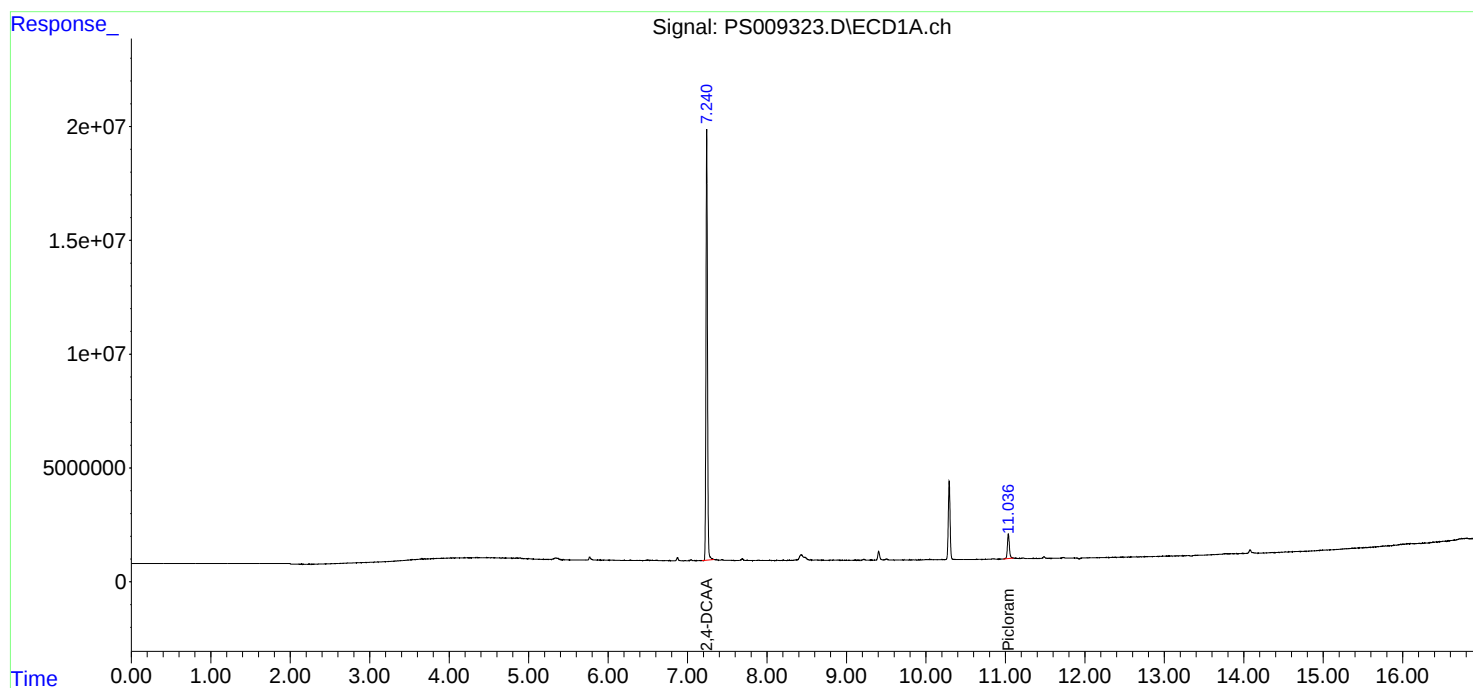


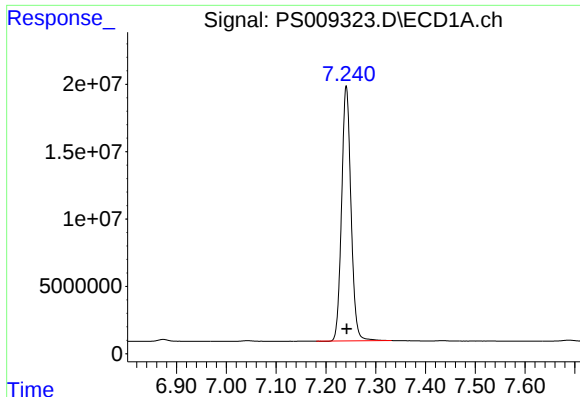

#4 2,4-DCAA


R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 247891574
Conc: 448.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

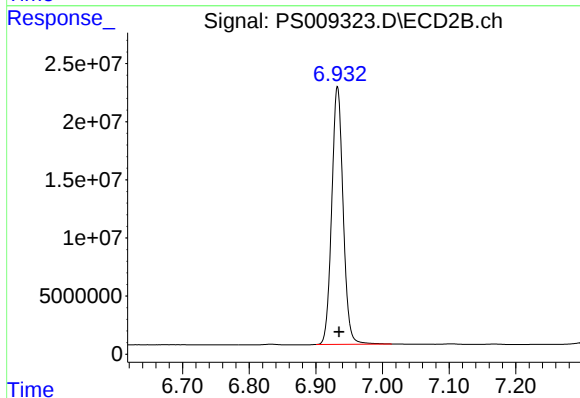


#4 2,4-DCAA

R.T.: 6.933 min
Delta R.T.: -0.003 min
Response: 263091470
Conc: 479.05 ng/ml

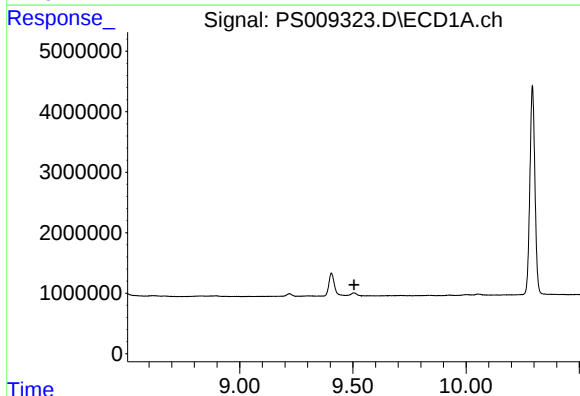


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.505 min
Response: 0
Conc: N.D.

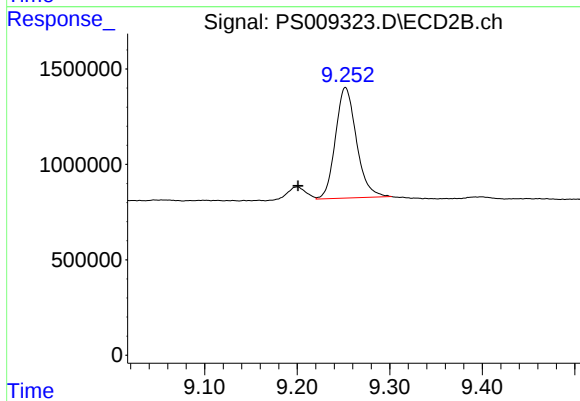

#12 2,4,5-T


R.T.: 9.252 min
Delta R.T.: 0.051 min
Response: 9127292
Conc: 3.09 ng/ml

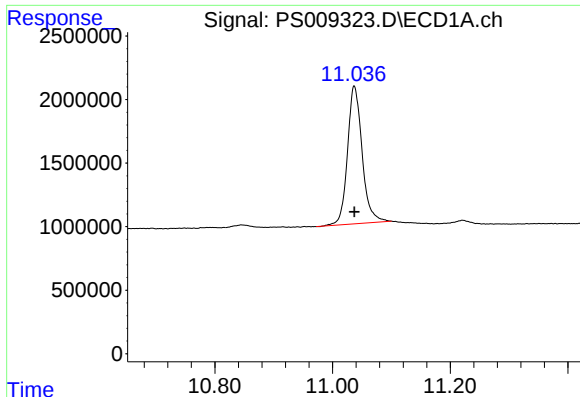

#15 Picloram


R.T.: 11.037 min
Delta R.T.: 0.000 min
Response: 18671592
Conc: 6.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

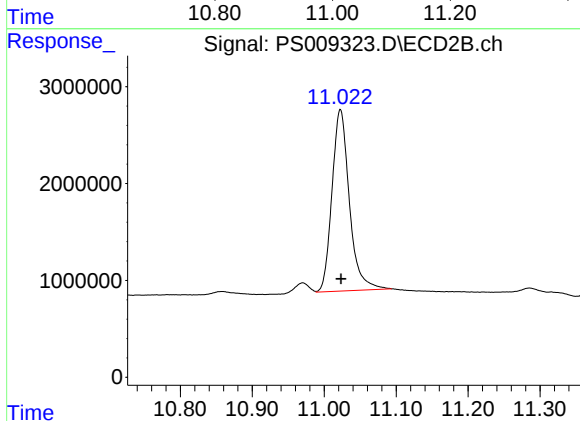


#15 Picloram

R.T.: 11.023 min
Delta R.T.: 0.000 min
Response: 31479400
Conc: 7.73 ng/ml

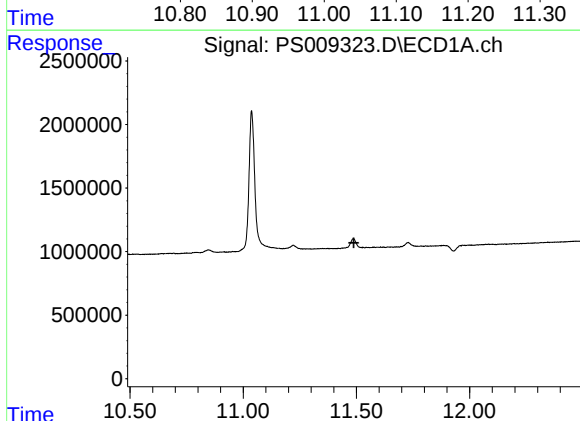

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

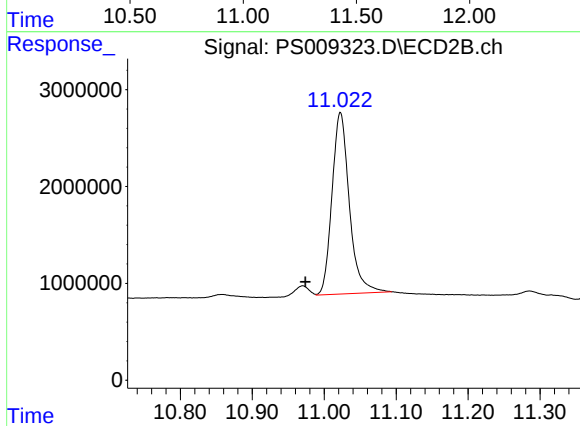

#16 DCPA

R.T.: 11.023 min
Delta R.T.: 0.048 min
Response: 31479400
Conc: 8.13 ng/ml