

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
 Data File : PS009327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2020 11:52
 Operator : DD\AJ
 Sample : PB127569BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 16:37:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.931	245.7E6	248.3E6	444.099	452.047
Target Compounds							
1) T	Dalapon	3.008	2.582	21359160	101.9E6	27.389	129.464 #
2) T	3,5-DICHL...	0.000	6.107	0	62086523	N.D.	76.338
7) T	MCPA	7.738	0.000	9286839	0	3.049	N.D. #
8) T	DICHLORPROP	8.123	7.751	11338819	26054179	21.985	46.960 #
12) T	2,4,5-T	9.450	0.000	23147797	0	9.100	N.D. #
14) T	DINOSEB	0.000	10.044	0	22684726	N.D.	10.328
15) T	Picloram	0.000	11.022	0	19428596	N.D.	4.771
16) T	DCPA	0.000	11.022	0	19428596	N.D.	5.016



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
Data File : PS009327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2020 11:52
Operator : DD\AJ
Sample : PB127569BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 16:37:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

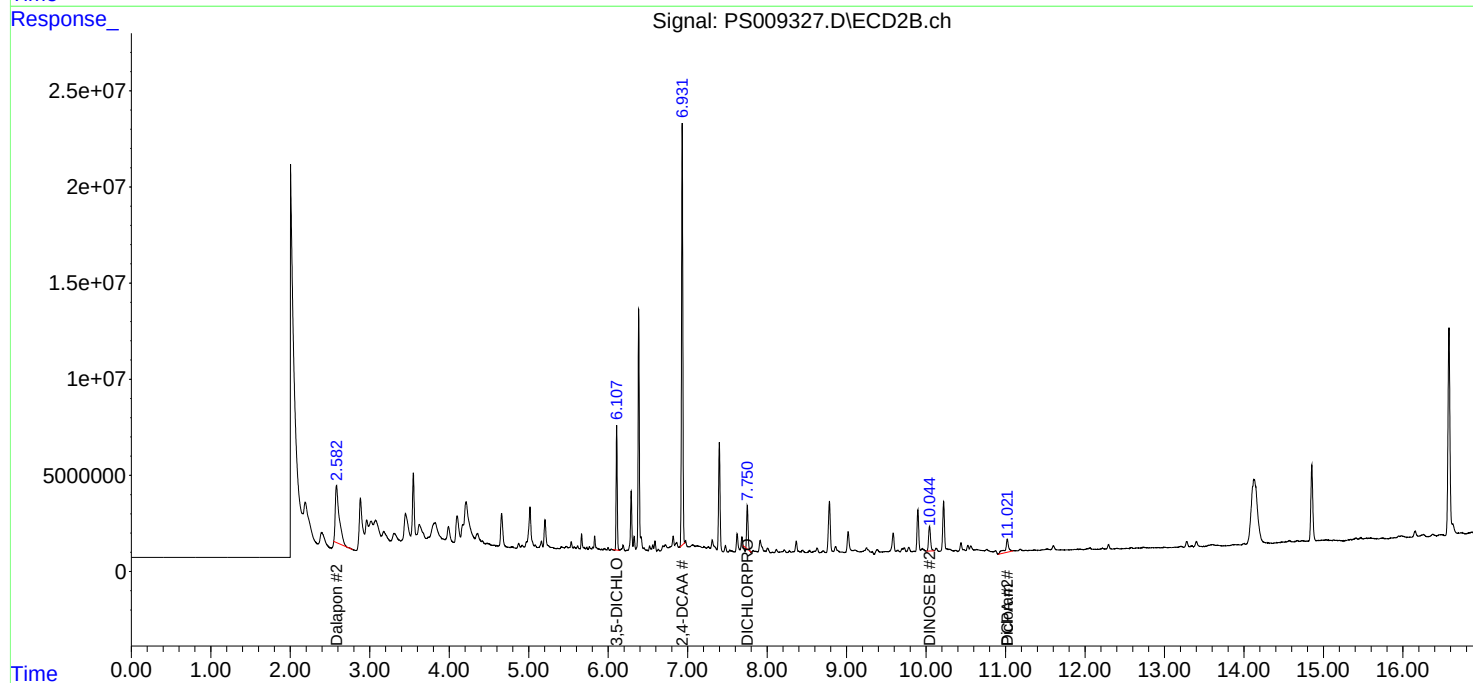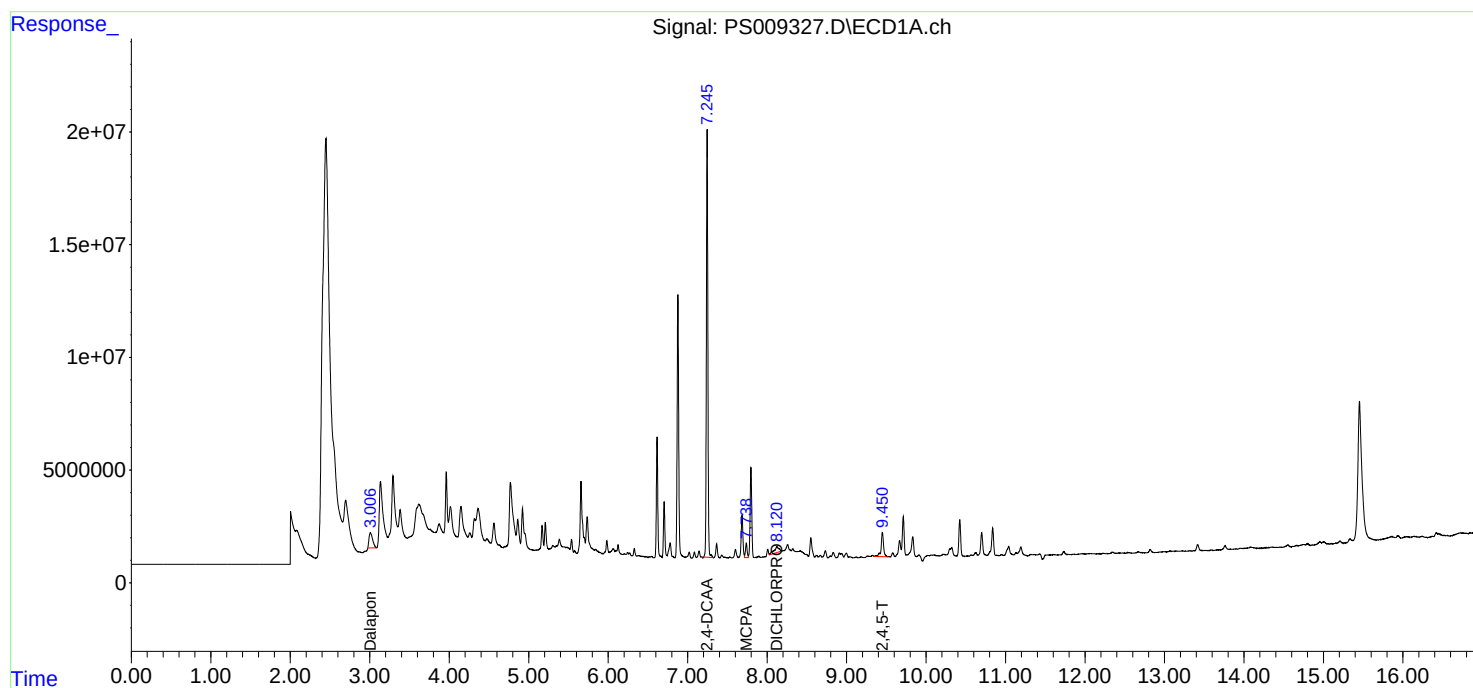


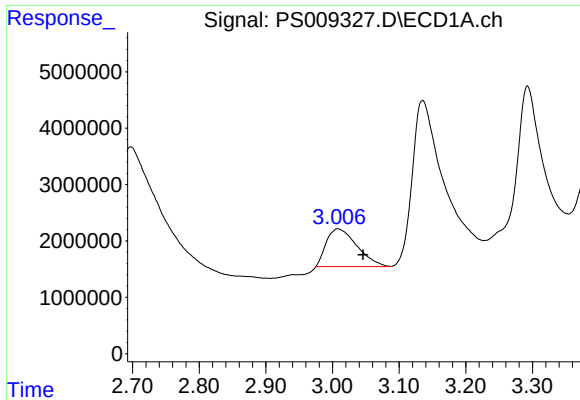

#1 Dalapon


R.T.: 3.008 min
Delta R.T.: -0.038 min
Response: 21359160
Conc: 27.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

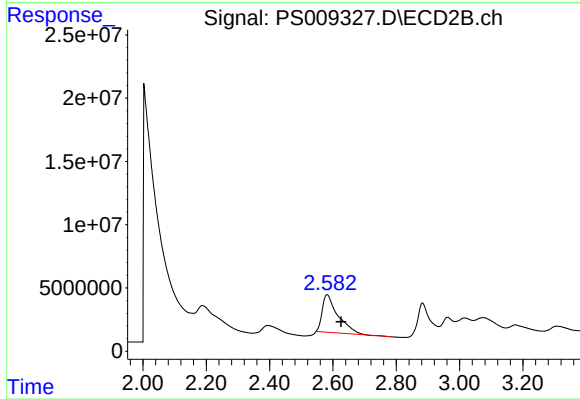


#1 Dalapon

R.T.: 2.582 min
Delta R.T.: -0.045 min
Response: 101935118
Conc: 129.46 ng/ml

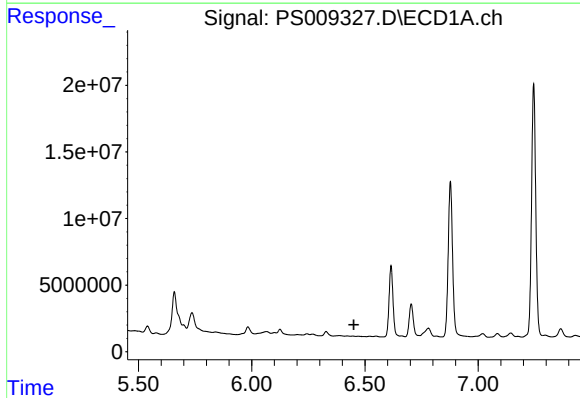


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

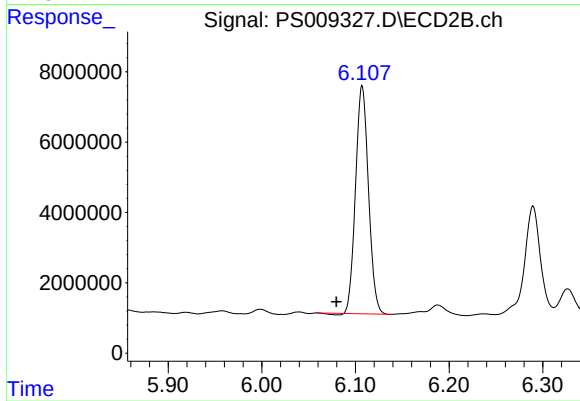

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.107 min
Delta R.T.: 0.028 min
Response: 62086523
Conc: 76.34 ng/ml

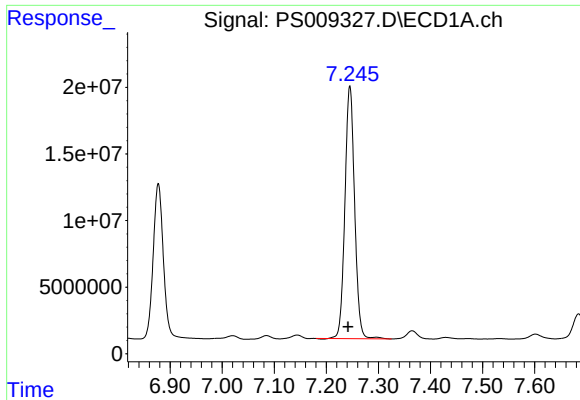

#4 2,4-DCAA


R.T.: 7.245 min
Delta R.T.: 0.003 min
Response: 245662333
Conc: 444.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

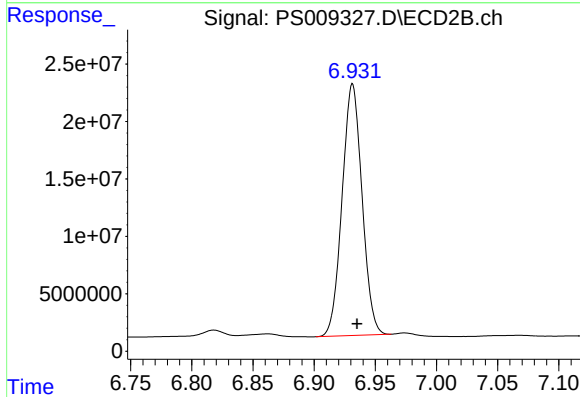


#4 2,4-DCAA

R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 248263221
Conc: 452.05 ng/ml

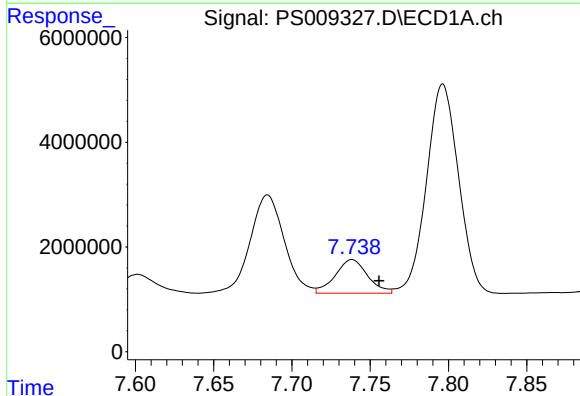


#7 MCPA

R.T.: 7.738 min
Delta R.T.: -0.017 min
Response: 9286839
Conc: 3.05 ug/ml

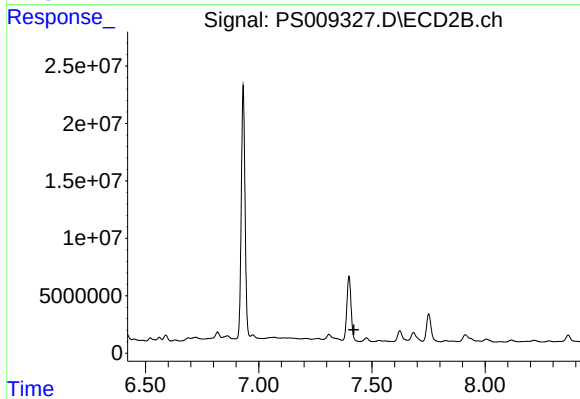

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

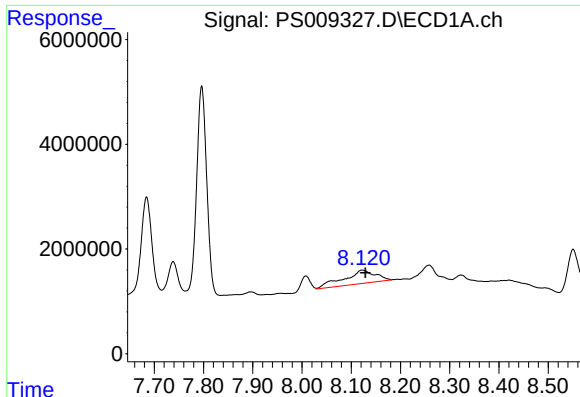

#8 DICHLORPROP


R.T.: 8.123 min
Delta R.T.: -0.006 min
Response: 11338819
Conc: 21.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

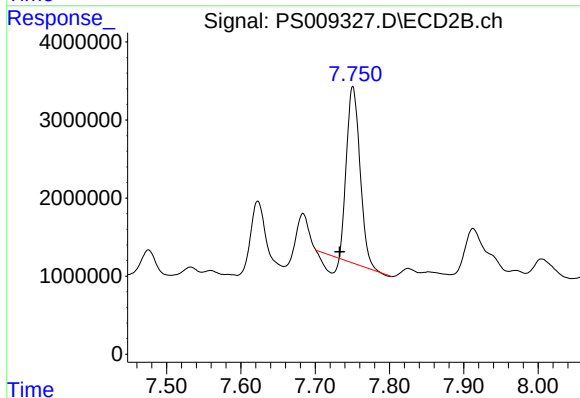


#8 DICHLORPROP

R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 26054179
Conc: 46.96 ng/ml

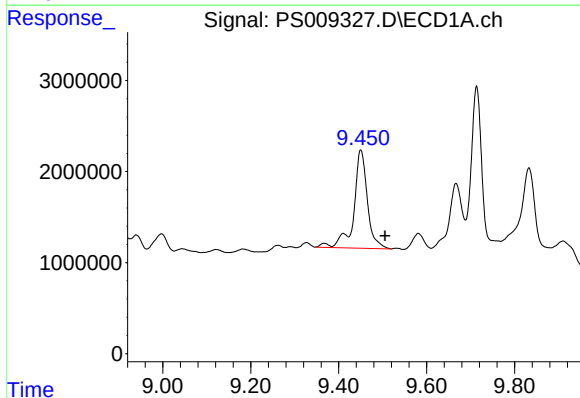


#12 2,4,5-T

R.T.: 9.450 min
Delta R.T.: -0.055 min
Response: 23147797
Conc: 9.10 ng/ml

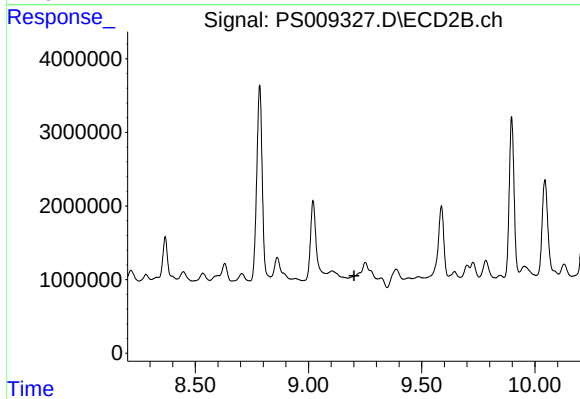

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

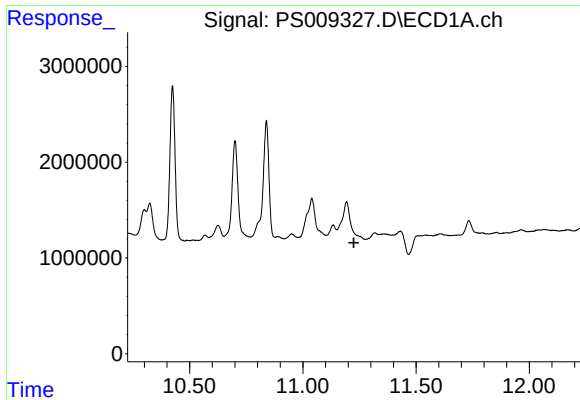

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.225 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

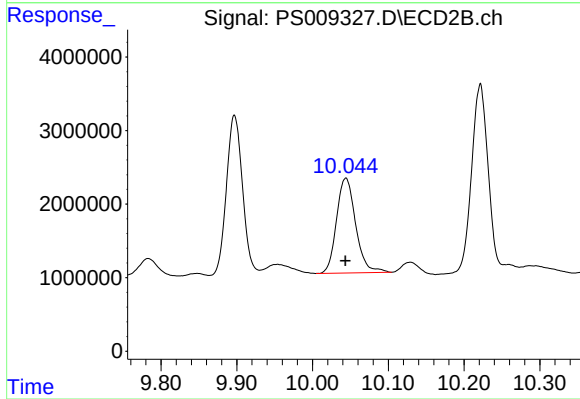


#14 DINOSEB

R.T.: 10.044 min
Delta R.T.: 0.000 min
Response: 22684726
Conc: 10.33 ng/ml

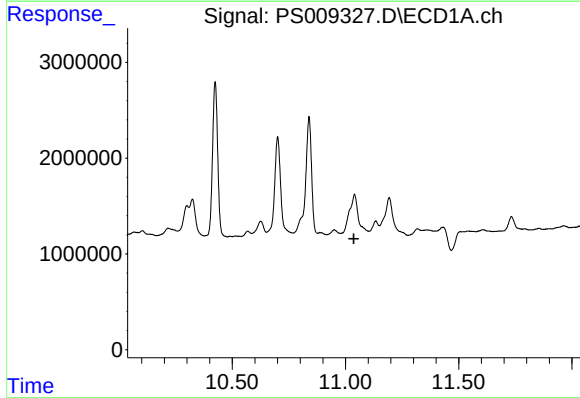


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

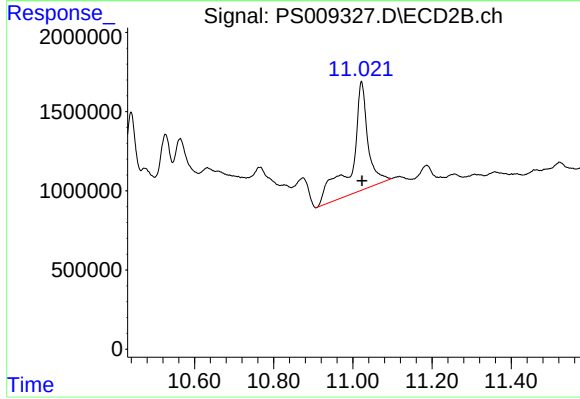

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.001 min
Response: 19428596
Conc: 4.77 ng/ml

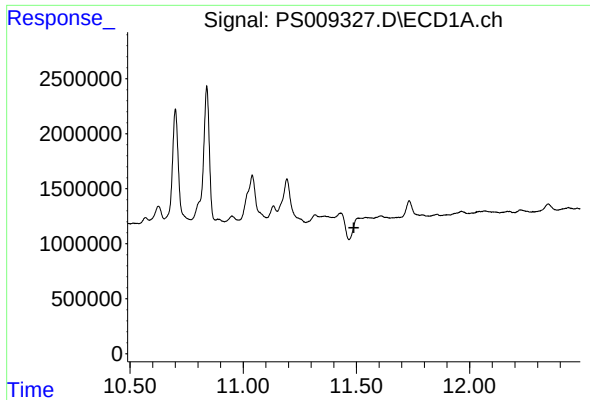

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

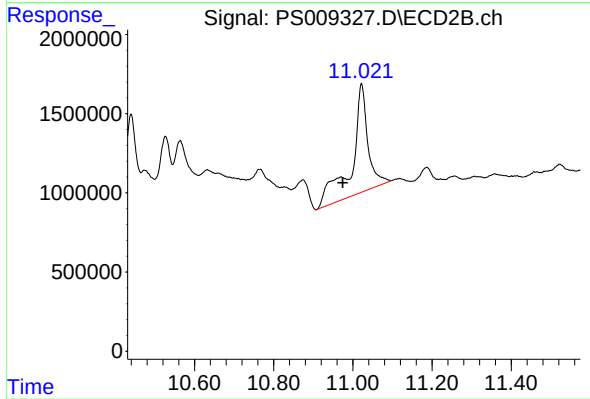

#16 DCPA

R.T.: 11.022 min
Delta R.T.: 0.048 min
Response: 19428596
Conc: 5.02 ng/ml