

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
 Data File : PS009333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2020 14:09
 Operator : DD\AJ
 Sample : L1933-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 16:38:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	240.2E6	245.3E6	434.202	446.742
Target Compounds							
1) T	Dalapon	3.008	2.588	22879148	104.2E6	29.338	132.379 #
2) T	3,5-DICHL...	0.000	6.110	0	64945151	N.D.	79.853
8) T	DICHLORPROP	0.000	7.752	0	38028811	N.D.	68.542
9) T	2,4-D	8.295	0.000	6795861	0	12.890	N.D. #
10) T	Pentachlo...	8.670	8.457	8878794	9068537	1.263	1.195
12) T	2,4,5-T	9.445	0.000	34679975	0	13.633	N.D. #
14) T	DINOSEB	0.000	10.088	0	17919194	N.D.	8.158
15) T	Picloram	11.014	0.000	14168427	0	4.668	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
Data File : PS009333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2020 14:09
Operator : DD\AJ
Sample : L1933-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 16:38:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

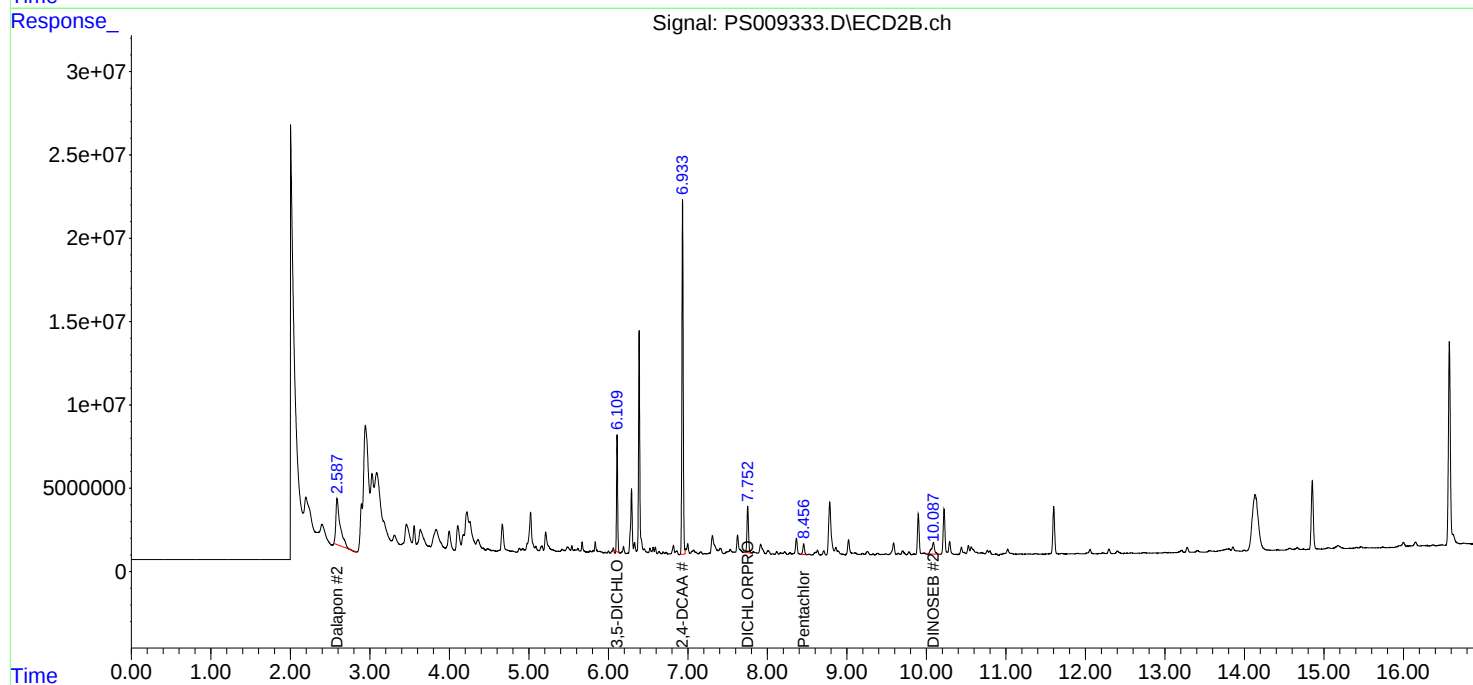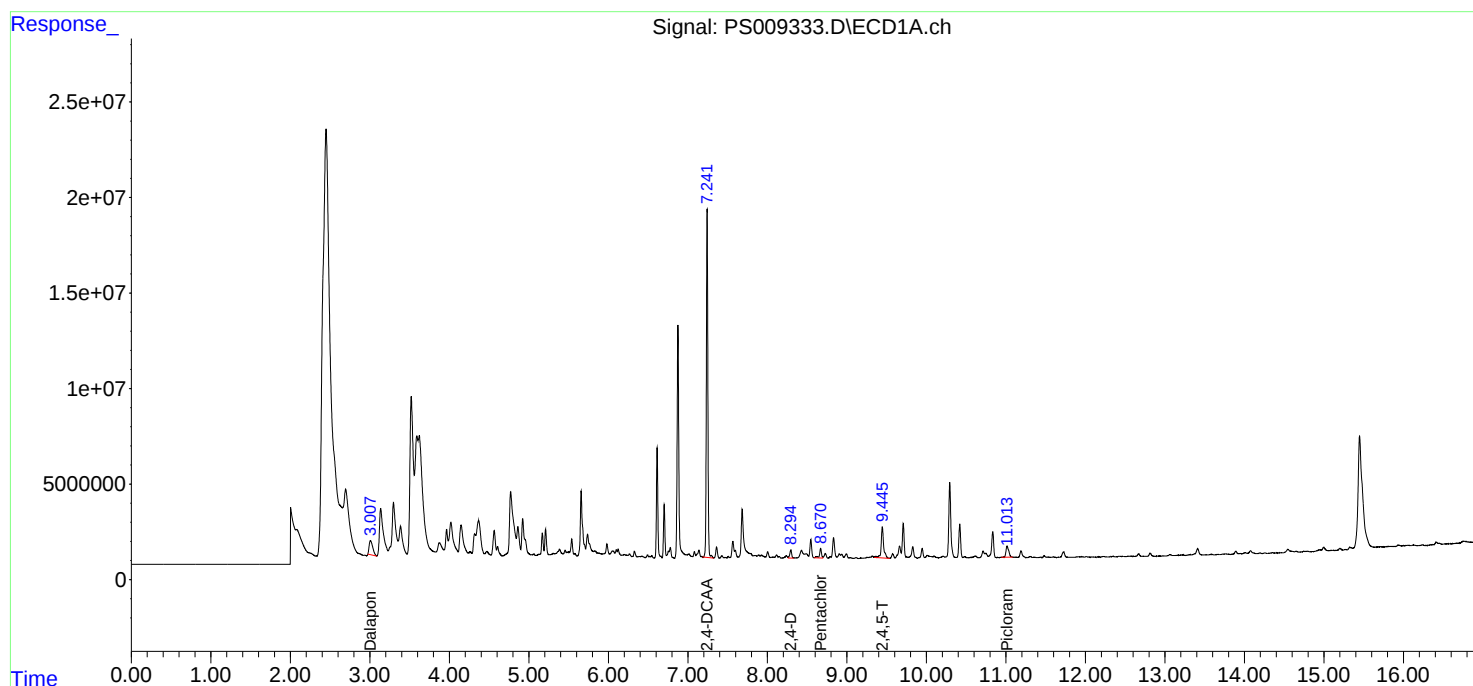


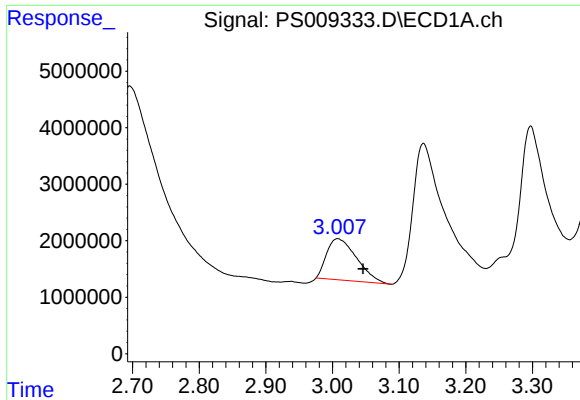

#1 Dalapon


R.T.: 3.008 min
Delta R.T.: -0.038 min
Response: 22879148
Conc: 29.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

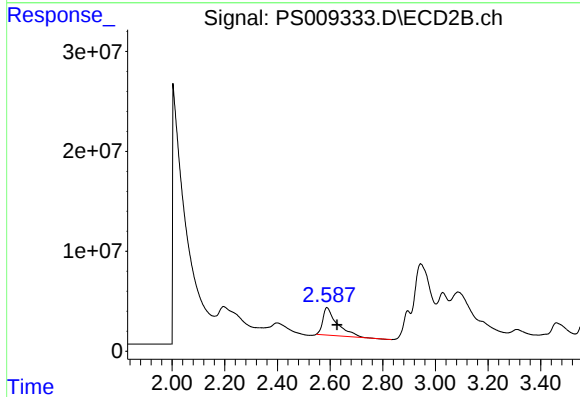


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 104230414
Conc: 132.38 ng/ml

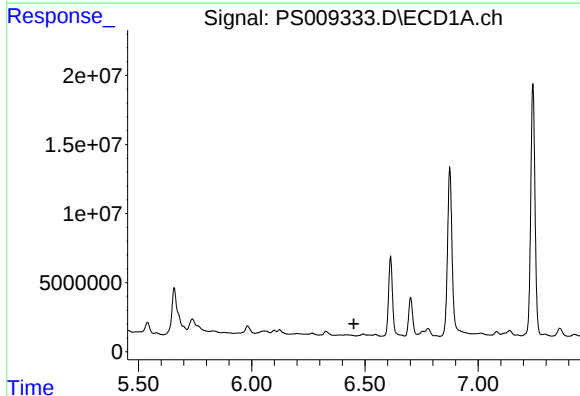


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

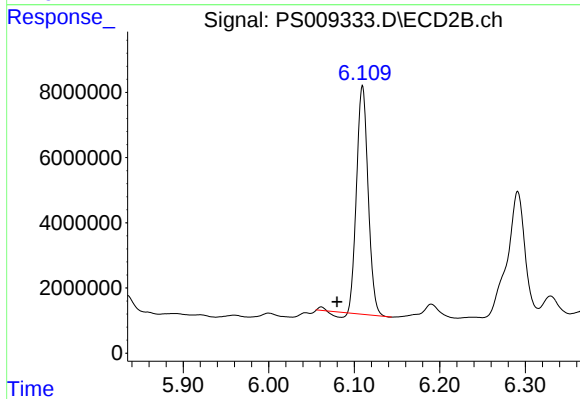

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 64945151
Conc: 79.85 ng/ml

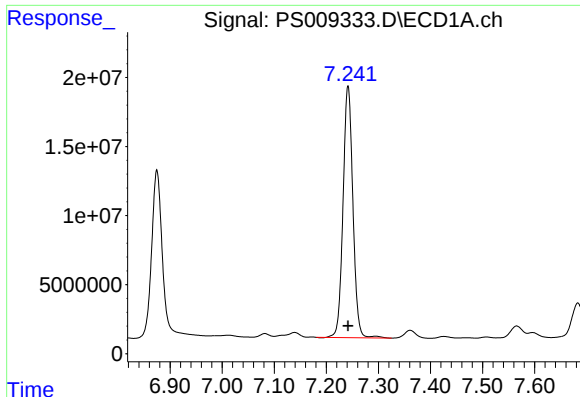

#4 2,4-DCAA


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 240187405
Conc: 434.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

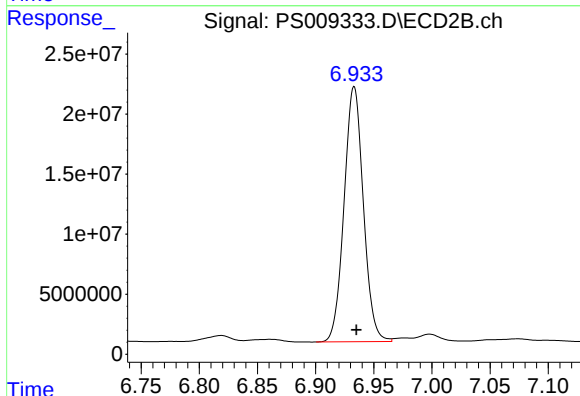


#4 2,4-DCAA

R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 245349527
Conc: 446.74 ng/ml

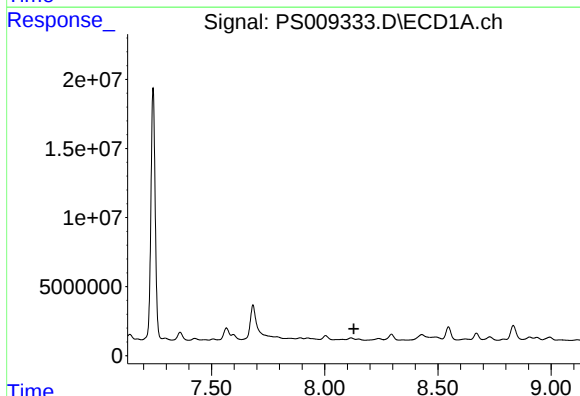


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

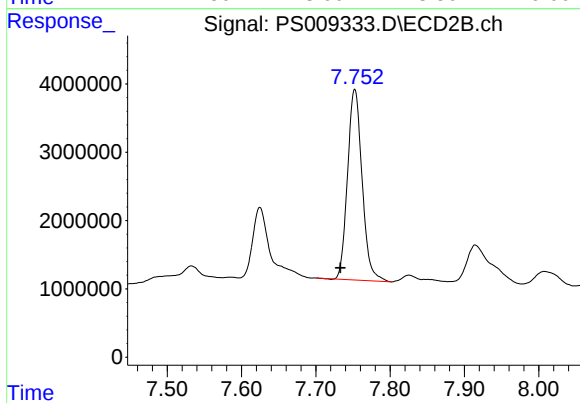

#8 DICHLORPROP


R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 38028811
Conc: 68.54 ng/ml

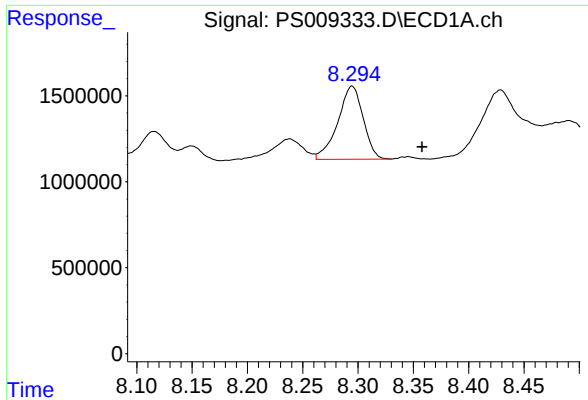

#9 2,4-D


R.T.: 8.295 min
Delta R.T.: -0.063 min
Response: 6795861
Conc: 12.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

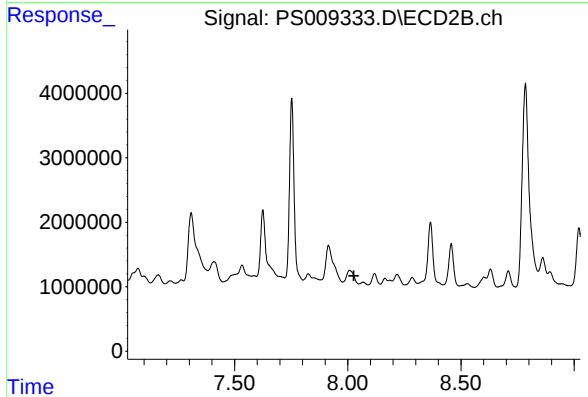


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.027 min
Response: 0
Conc: N.D.

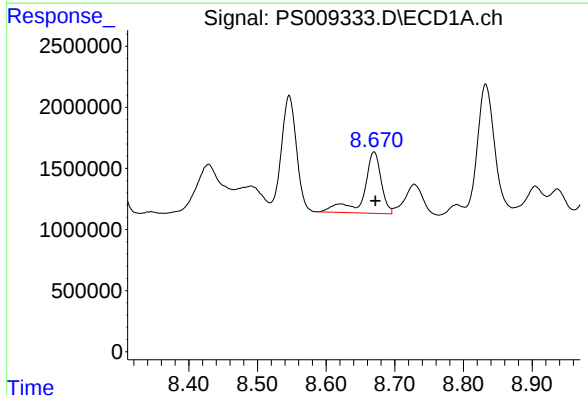


#10 Pentachlorophenol

R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 8878794
Conc: 1.26 ng/ml

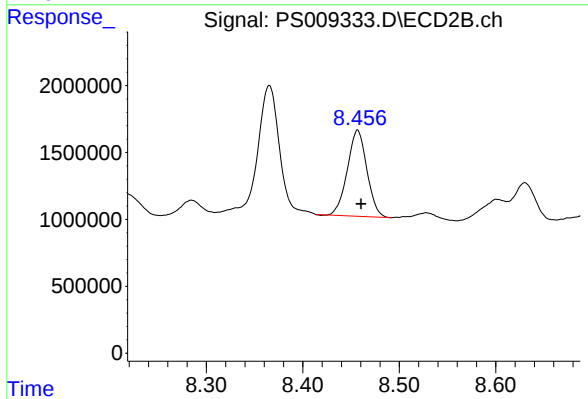

#10 Pentachlorophenol


R.T.: 8.457 min
Delta R.T.: -0.004 min
Response: 9068537
Conc: 1.19 ng/ml

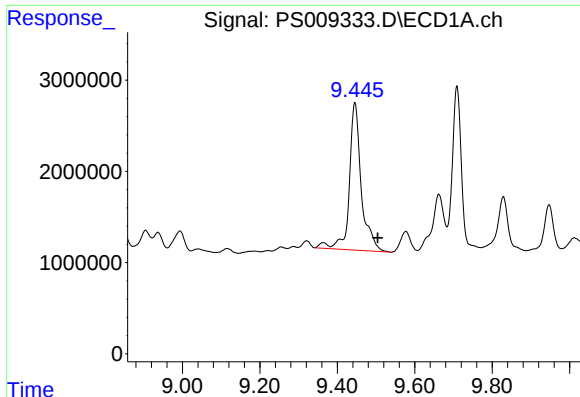

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 34679975
Conc: 13.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

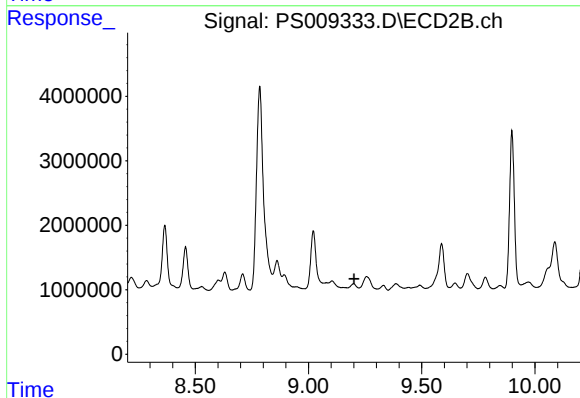


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

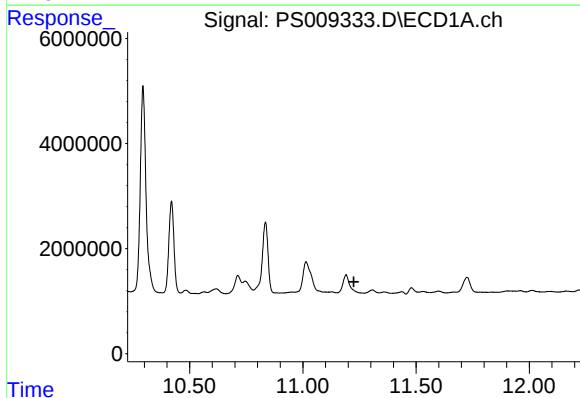


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.225 min
Response: 0
Conc: N.D.

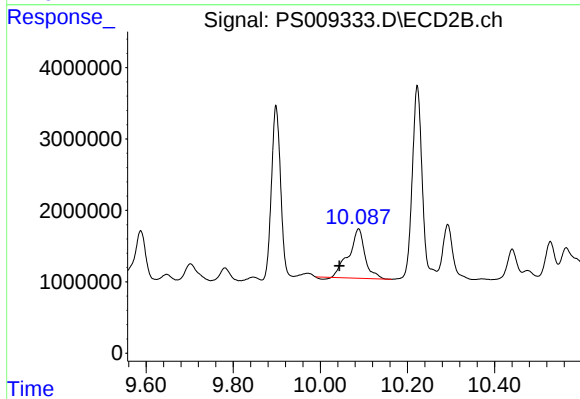

#14 DINOSEB


R.T.: 10.088 min
Delta R.T.: 0.044 min
Response: 17919194
Conc: 8.16 ng/ml

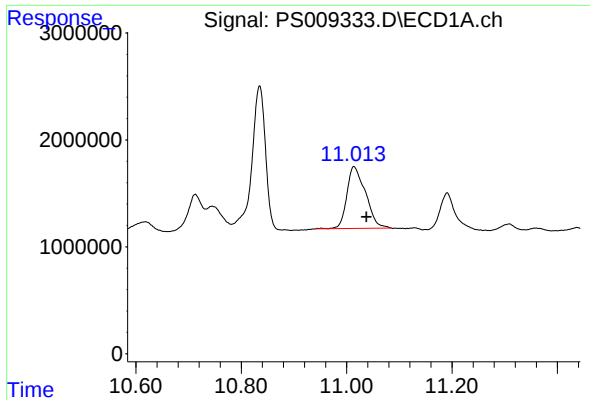

#15 Picloram

R.T.: 11.014 min
Delta R.T.: -0.023 min
Response: 14168427
Conc: 4.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

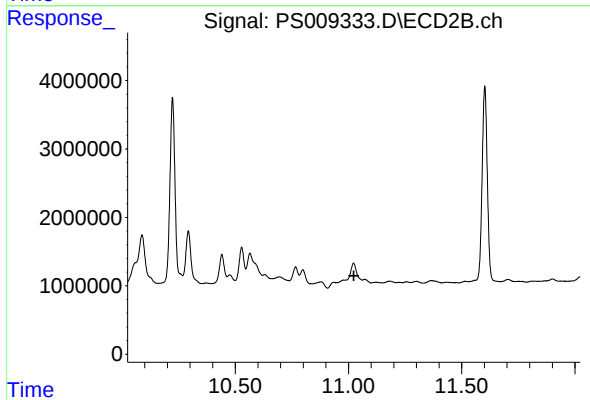

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.