

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
 Data File : PS009334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2020 14:32
 Operator : DD\AJ
 Sample : L1933-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 16:38:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	190.6E6	191.9E6	344.491	349.358
Target Compounds							
1) T	Dalapon	3.008	2.588	22574318	107.1E6	28.948	136.076 #
2) T	3,5-DICHL...	0.000	6.109	0	70453055	N.D.	86.625
8) T	DICHLORPROP	0.000	7.753	0	36421964	N.D.	65.646
9) T	2,4-D	8.296	0.000	19346449	0	36.695	N.D. #
12) T	2,4,5-T	9.445	0.000	62697458	0	24.647	N.D. #
14) T	DINOSEB	0.000	10.087	0	15652238	N.D.	7.126
15) T	Picloram	11.013	0.000	9658420	0	3.182	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
Data File : PS009334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2020 14:32
Operator : DD\AJ
Sample : L1933-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 16:38:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

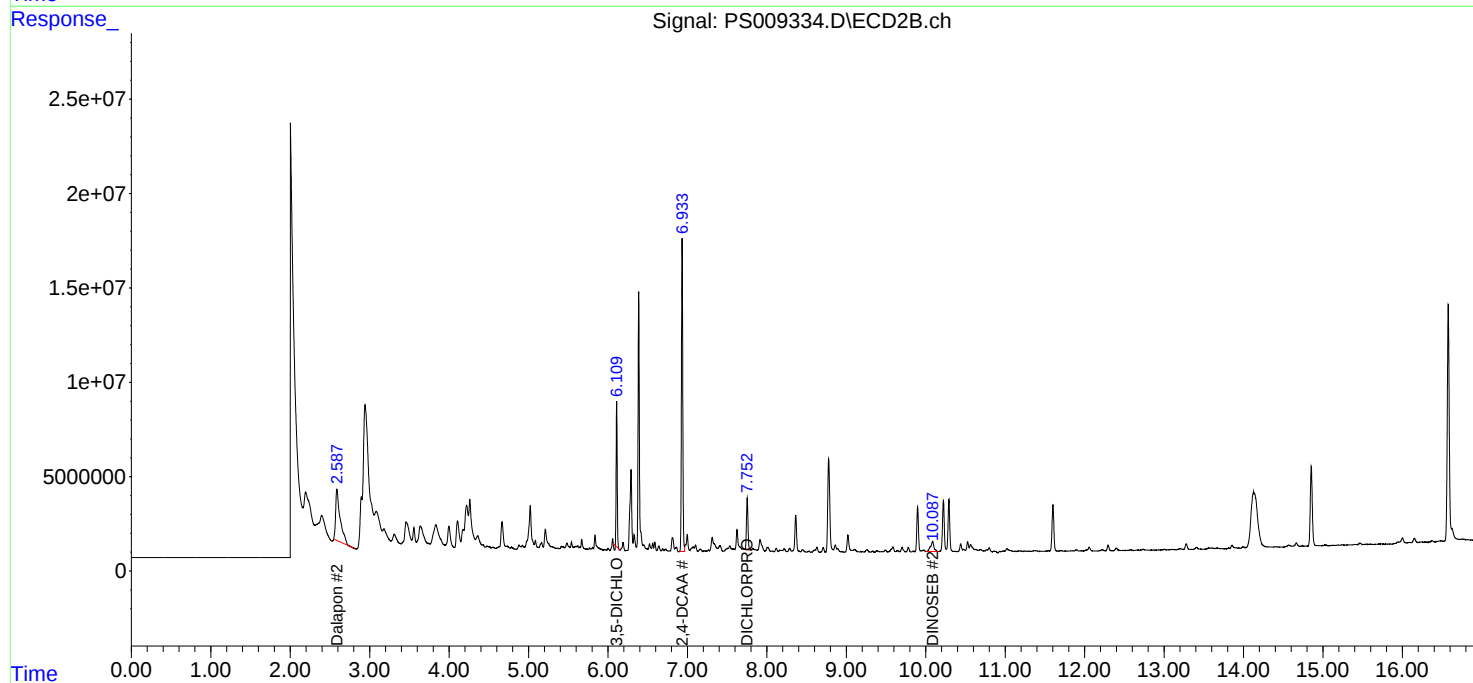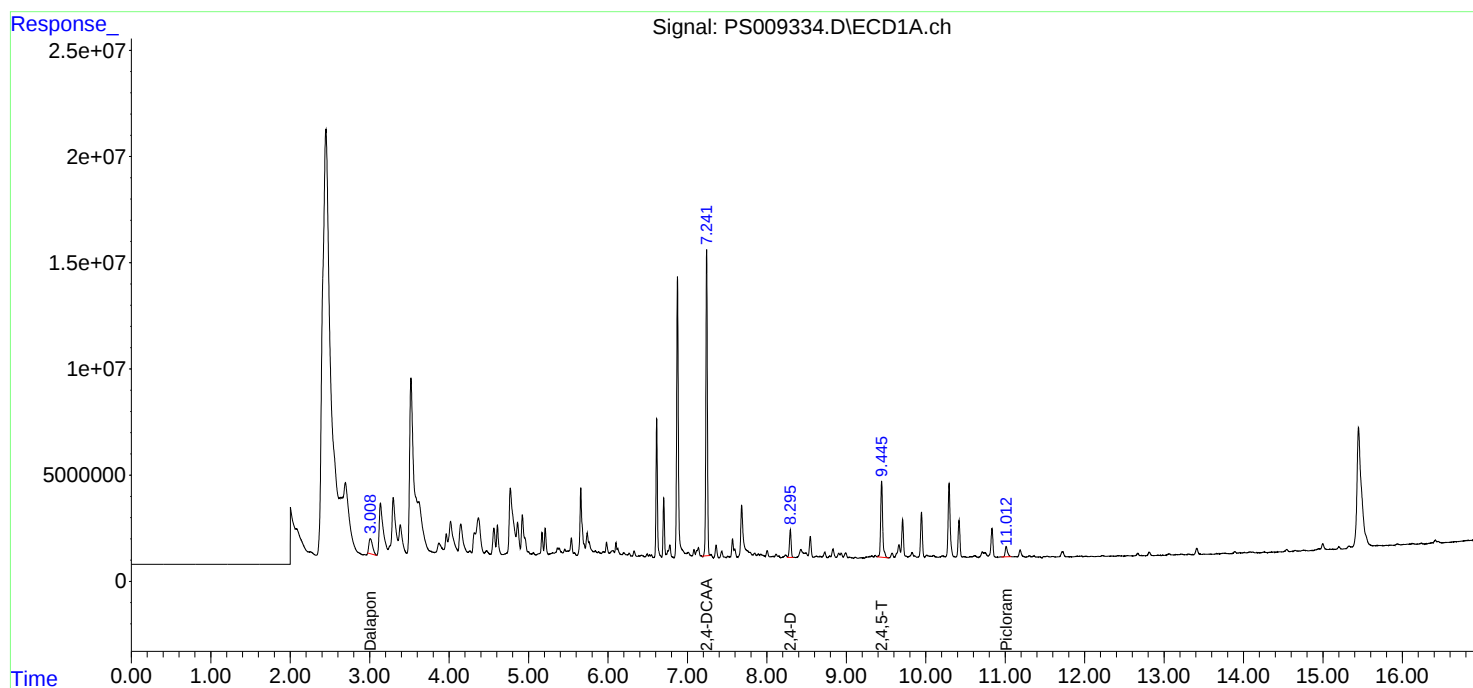


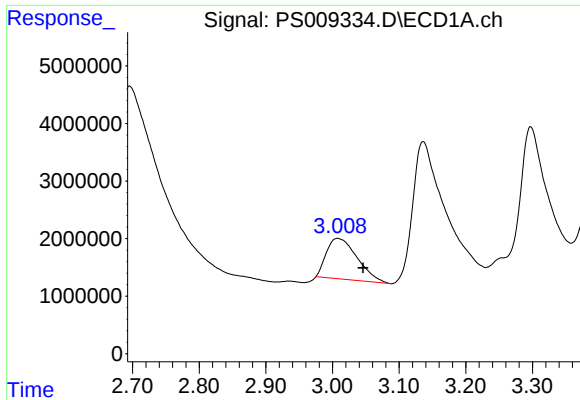

#1 Dalapon


R.T.: 3.008 min
Delta R.T.: -0.038 min
Response: 22574318
Conc: 28.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

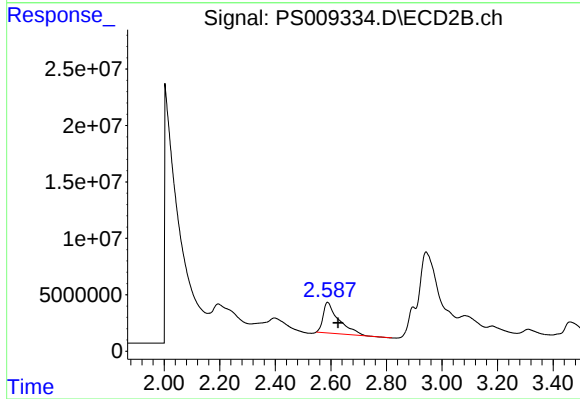


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.039 min
Response: 107141013
Conc: 136.08 ng/ml

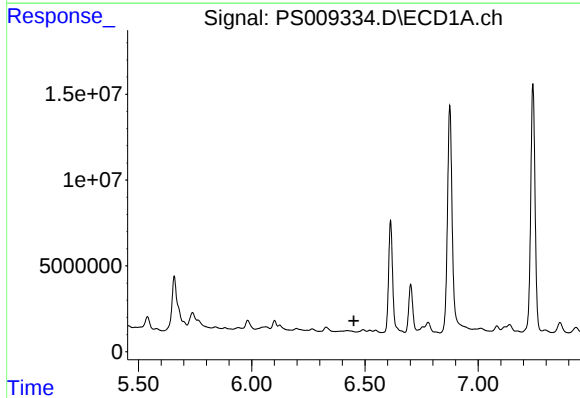


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

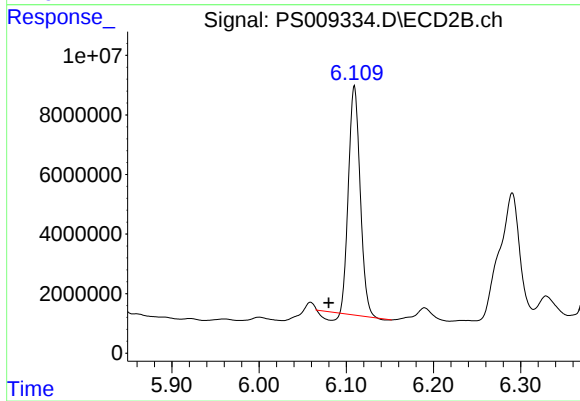

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.030 min
Response: 70453055
Conc: 86.63 ng/ml

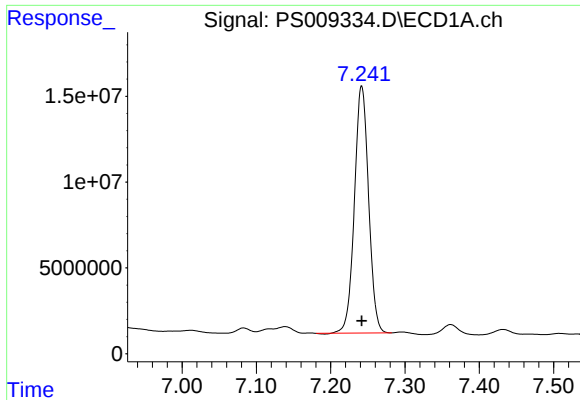

#4 2,4-DCAA


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 190562002
Conc: 344.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

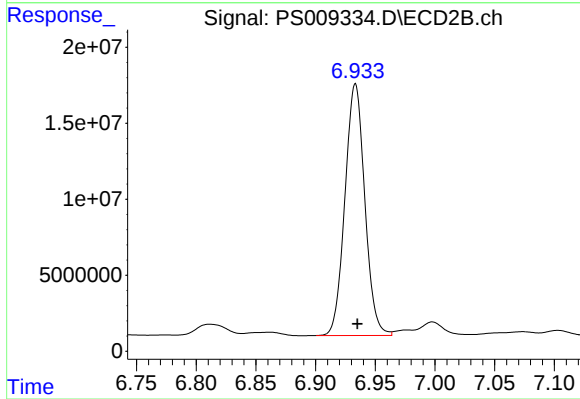


#4 2,4-DCAA

R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 191866438
Conc: 349.36 ng/ml

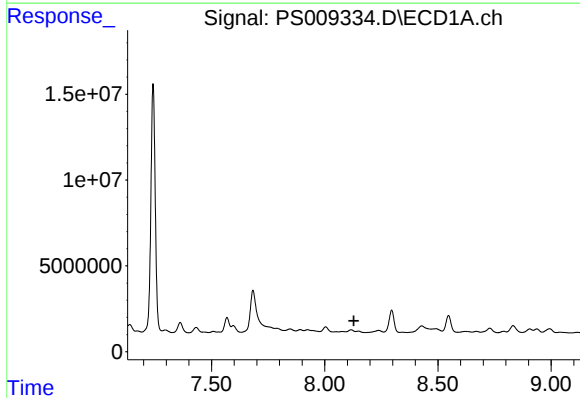


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

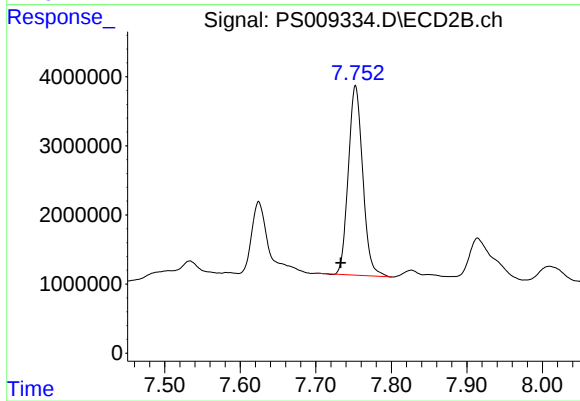

#8 DICHLORPROP


R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 36421964
Conc: 65.65 ng/ml

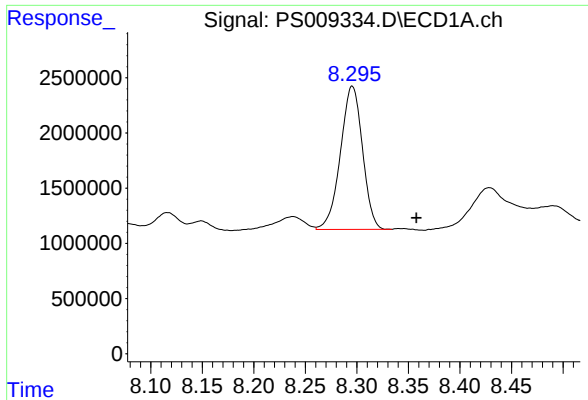

#9 2,4-D


R.T.: 8.296 min
Delta R.T.: -0.062 min
Response: 19346449
Conc: 36.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

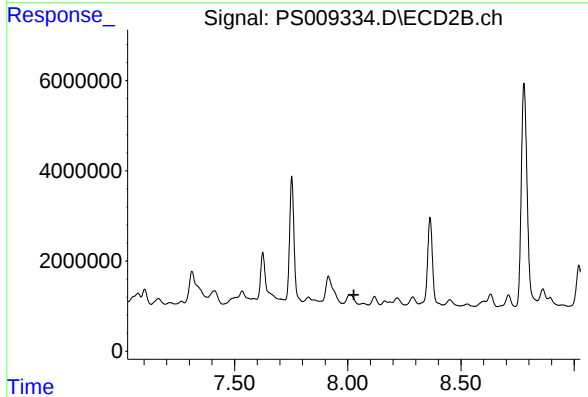


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.027 min
Response: 0
Conc: N.D.

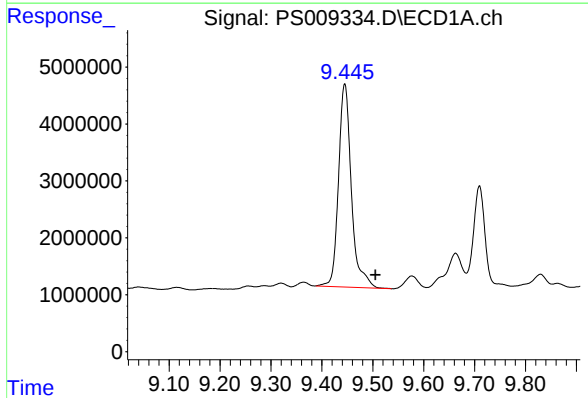


#12 2,4,5-T

R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 62697458
Conc: 24.65 ng/ml

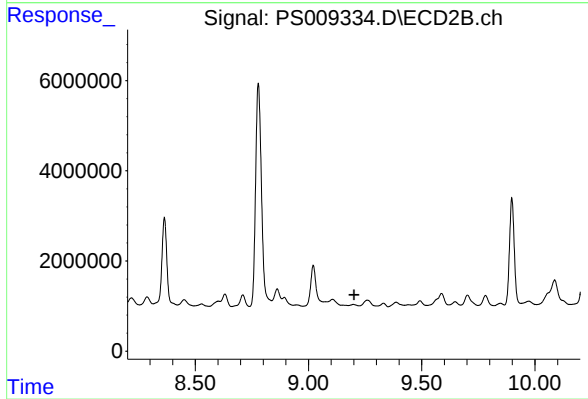

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

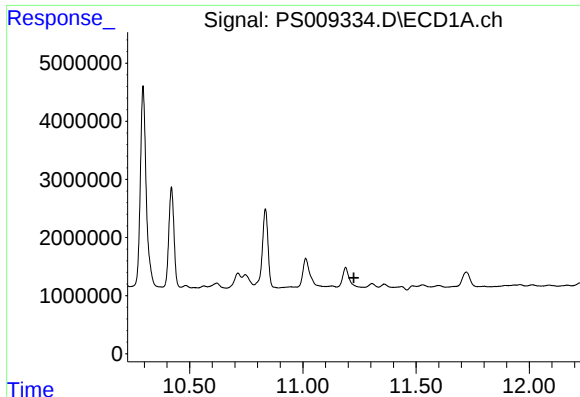

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.225 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

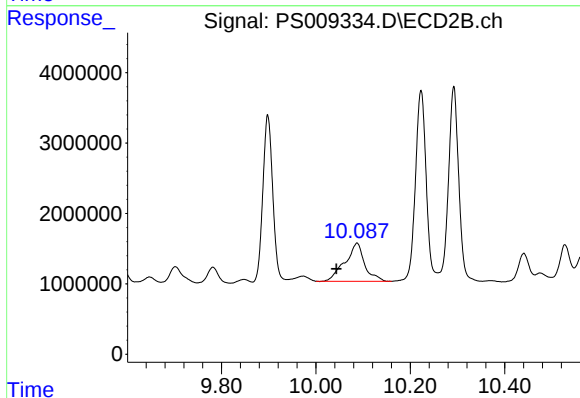


#14 DINOSEB

R.T.: 10.087 min
Delta R.T.: 0.043 min
Response: 15652238
Conc: 7.13 ng/ml

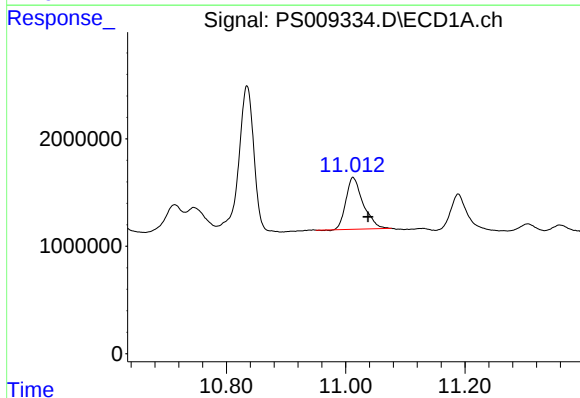

#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.025 min
Response: 9658420
Conc: 3.18 ng/ml

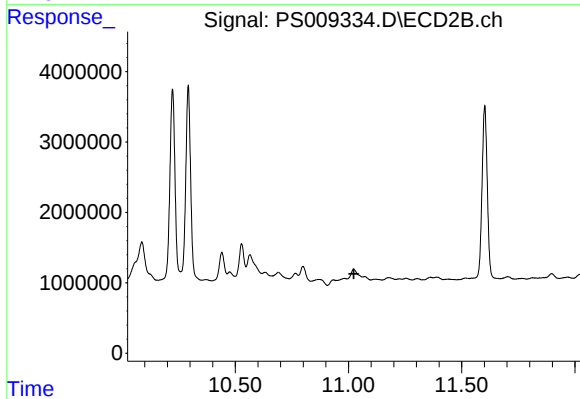

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.023 min
Response: 0
Conc: N.D.