

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
 Data File : PS009338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2020 16:04
 Operator : DD\AJ
 Sample : L1942-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 16:39:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	192.2E6	190.0E6	347.376	346.032
Target Compounds							
1) T	Dalapon	3.008	2.588	21718275	85081116	27.850	108.058 #
2) T	3,5-DICHL...	0.000	6.110	0	86857989	N.D.	106.796
3) T	4-Nitroph...	7.137	0.000	10966286	0	45.939	N.D. #
8) T	DICHLORPROP	0.000	7.752	0	36781607	N.D.	66.294
9) T	2,4-D	8.426	0.000	12464382	0	23.641	N.D. #
12) T	2,4,5-T	9.446	0.000	42908210	0	16.867	N.D. #
14) T	DINOSEB	11.188	10.086	7650038	25450338	3.742	11.587 #
15) T	Picloram	11.013	0.000	10579400	0	3.486	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
Data File : PS009338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2020 16:04
Operator : DD\AJ
Sample : L1942-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 16:39:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

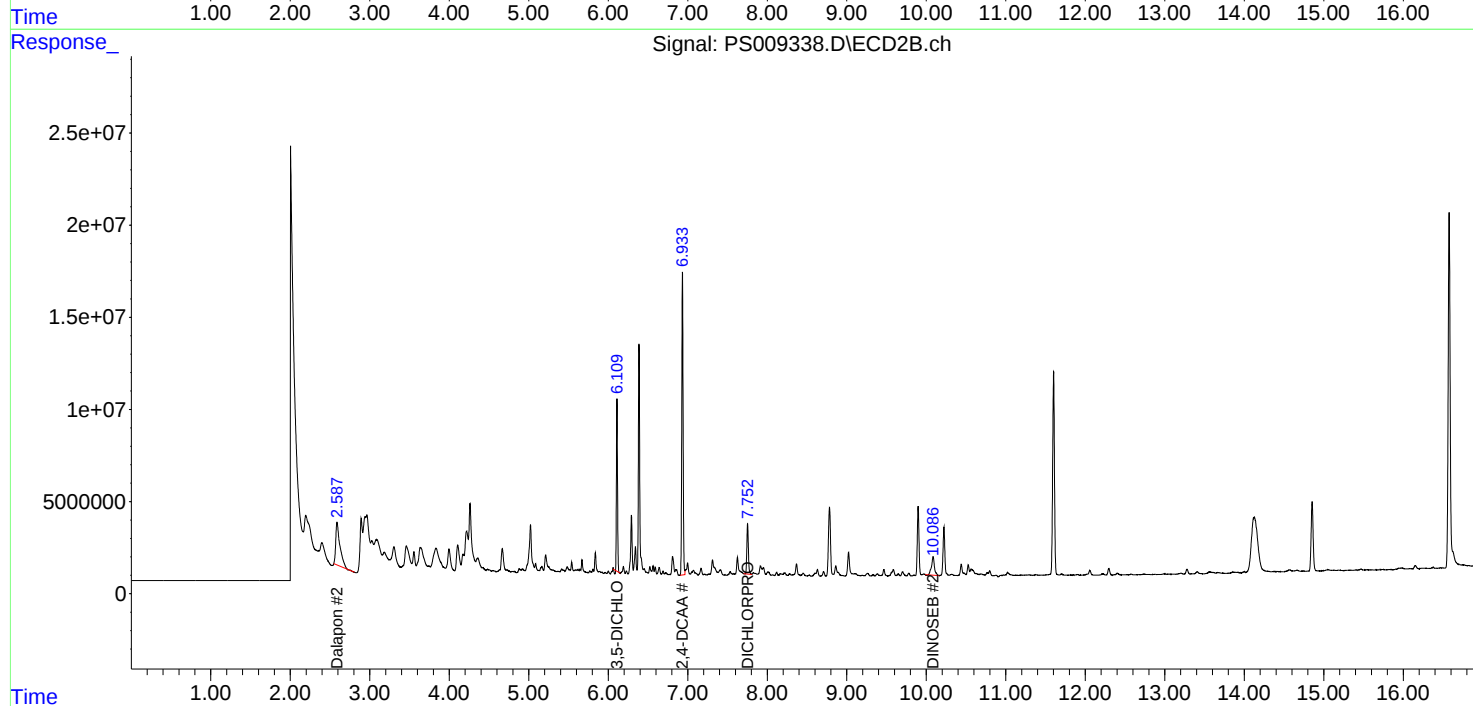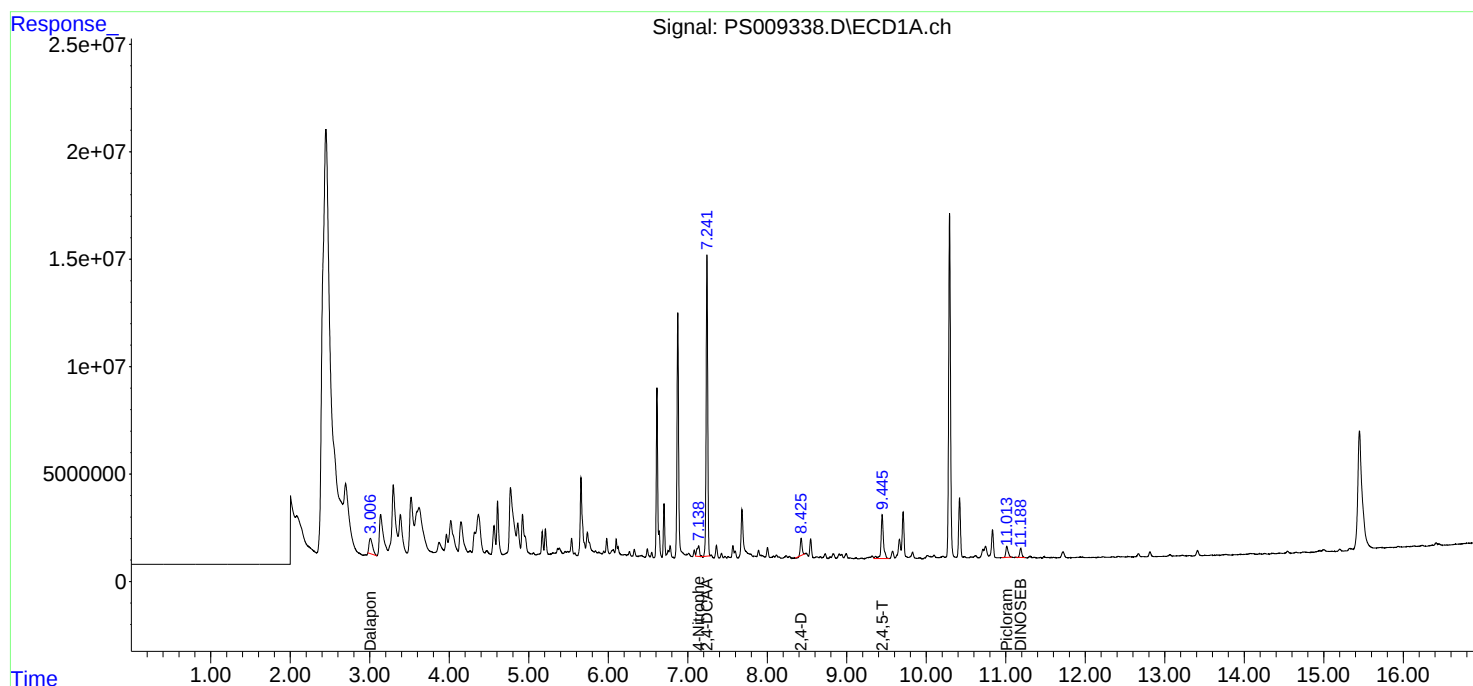


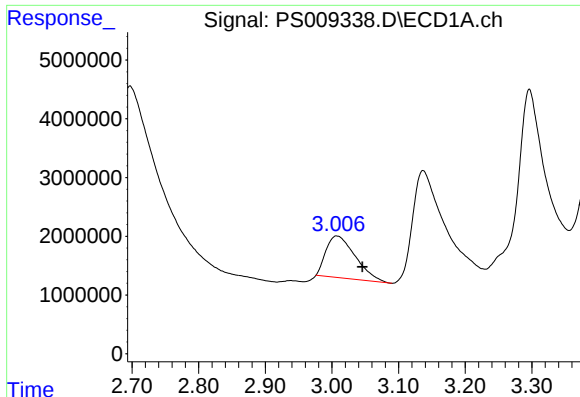

#1 Dalapon


R.T.: 3.008 min
Delta R.T.: -0.038 min
Response: 21718275
Conc: 27.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

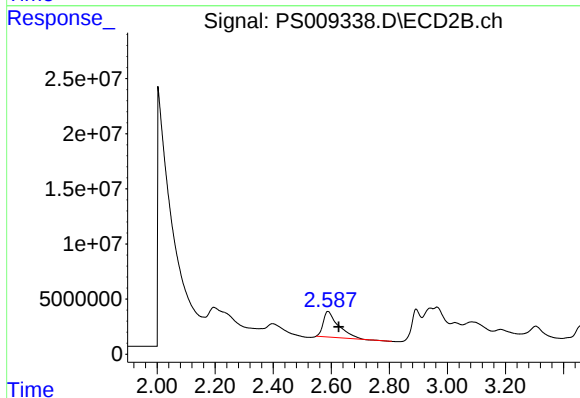


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 85081116
Conc: 108.06 ng/ml

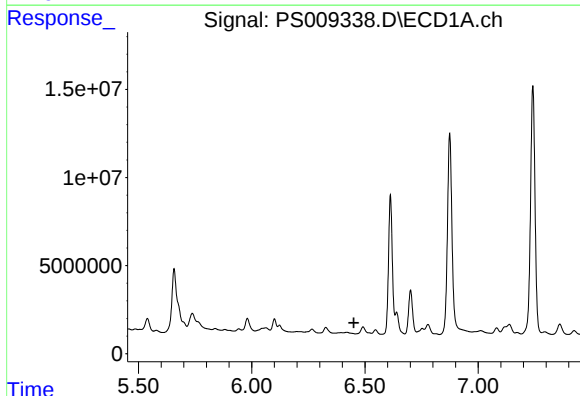


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

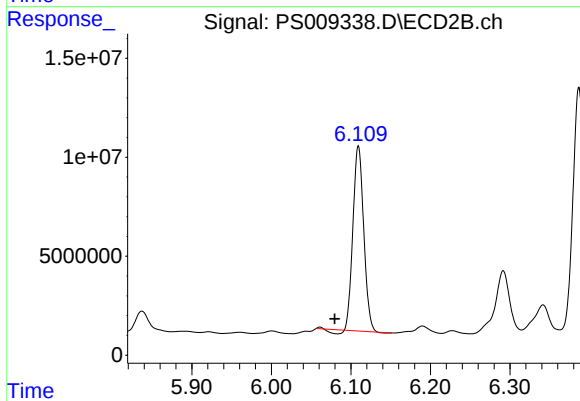

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 86857989
Conc: 106.80 ng/ml

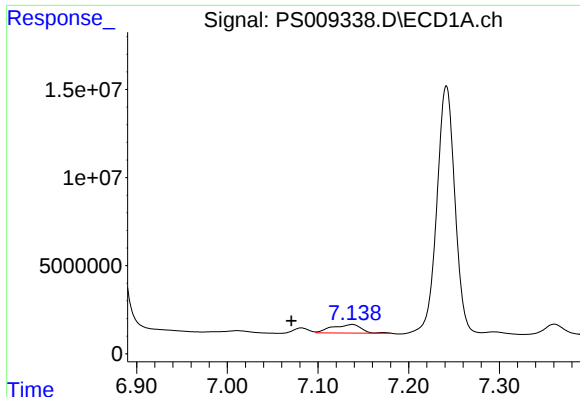

#3 4-Nitrophenol


R.T.: 7.137 min
Delta R.T.: 0.067 min
Response: 10966286
Conc: 45.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

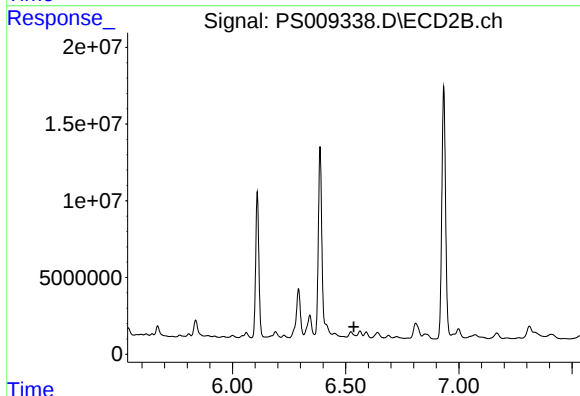


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.536 min
Response: 0
Conc: N.D.

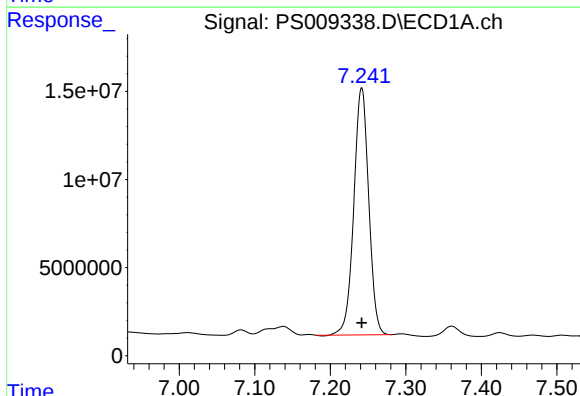


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 192157765
Conc: 347.38 ng/ml

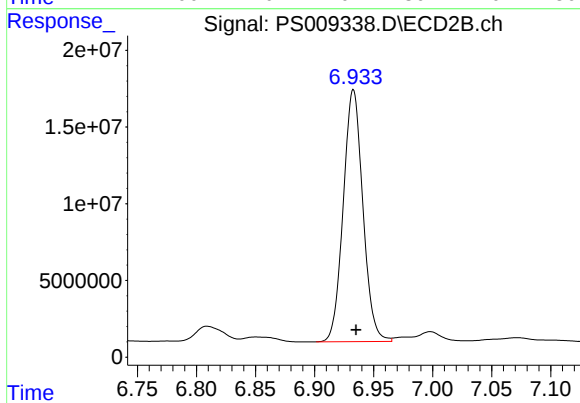

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 190039835
Conc: 346.03 ng/ml

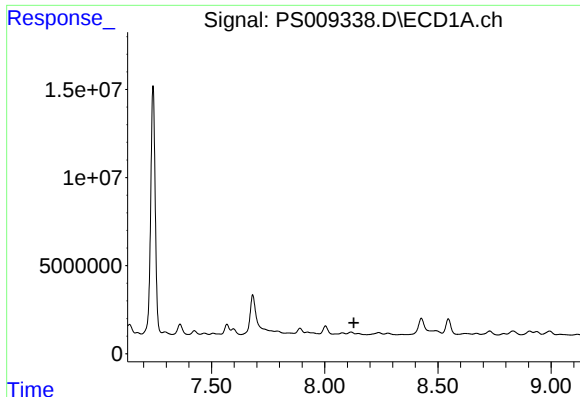

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

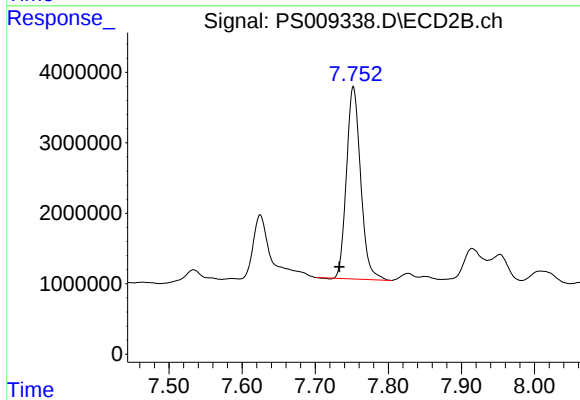


#8 DICHLORPROP

R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 36781607
Conc: 66.29 ng/ml

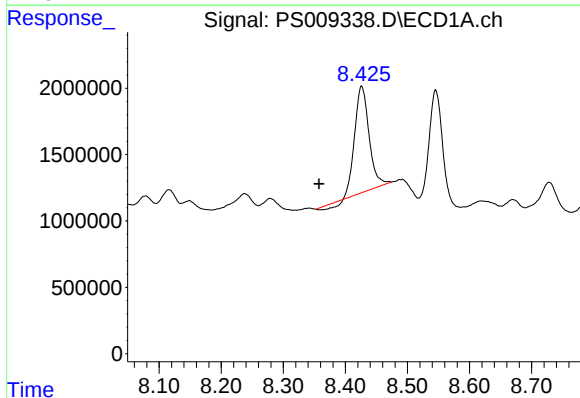


#9 2,4-D

R.T.: 8.426 min
Delta R.T.: 0.069 min
Response: 12464382
Conc: 23.64 ng/ml

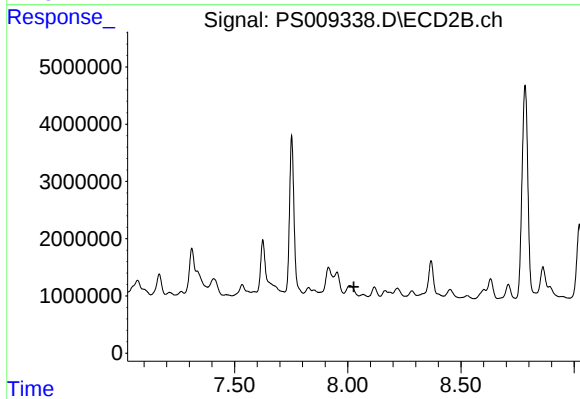

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

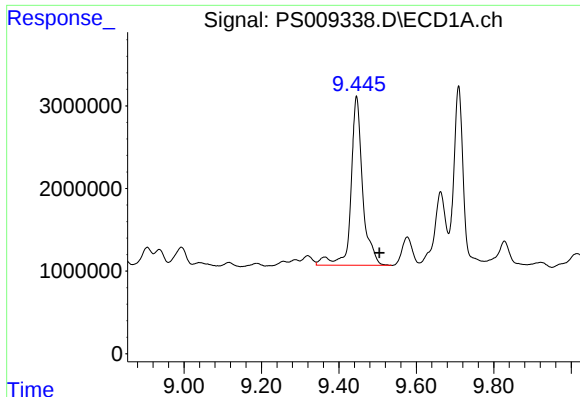

#12 2,4,5-T


R.T.: 9.446 min
Delta R.T.: -0.059 min
Response: 42908210
Conc: 16.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

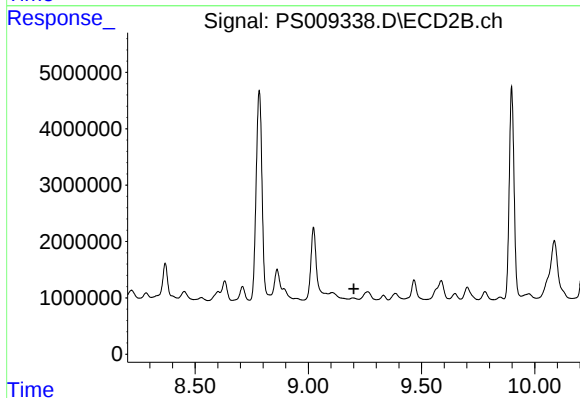


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

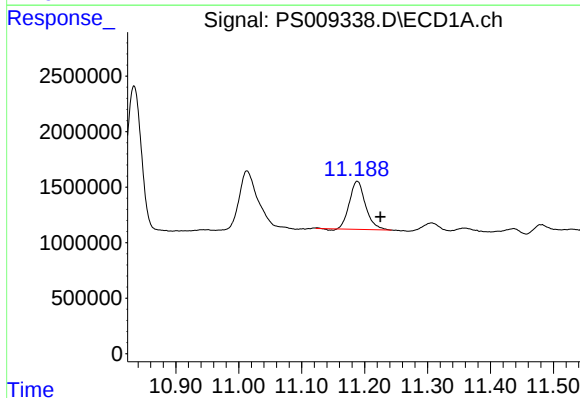


#14 DINOSEB

R.T.: 11.188 min
Delta R.T.: -0.037 min
Response: 7650038
Conc: 3.74 ng/ml

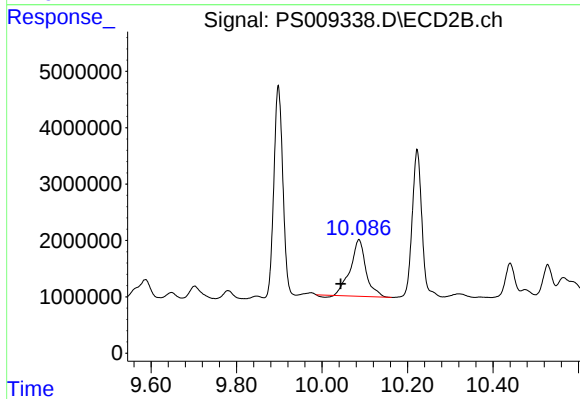

#14 DINOSEB


R.T.: 10.086 min
Delta R.T.: 0.043 min
Response: 25450338
Conc: 11.59 ng/ml

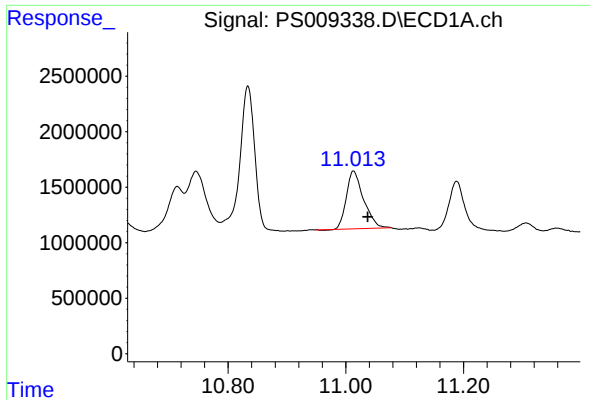

#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.024 min
Response: 10579400
Conc: 3.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

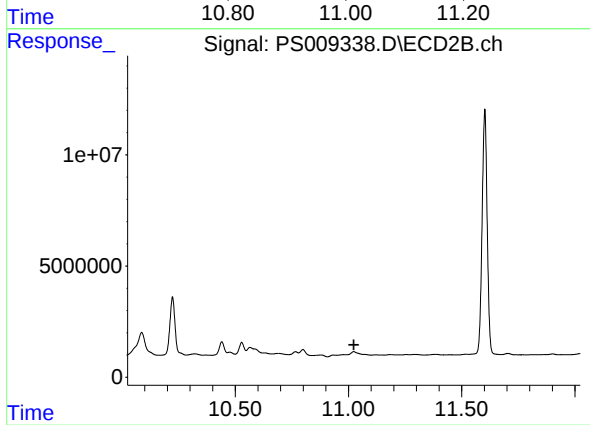

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.