

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
 Data File : PS009339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2020 16:27
 Operator : DD\AJ
 Sample : L1942-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 17:42:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.934	210.7E6	206.7E6	380.824	376.381
Target Compounds							
1) T	Dalapon	3.009	2.588	23306896	78101291	29.887	99.194 #
2) T	3,5-DICHL...	0.000	6.110	0	89181622	N.D.	109.653
3) T	4-Nitroph...	7.138	0.000	11987595	0	50.218	N.D. #
8) T	DICHLORPROP	0.000	7.753	0	37097537	N.D.	66.864
9) T	2,4-D	8.427	0.000	5359237	0	10.165	N.D. #
12) T	2,4,5-T	9.445	0.000	53710724	0	21.114	N.D. #
14) T	DINOSEB	11.189	10.086	10045570	40920837	4.914	18.630 #
15) T	Picloram	11.014	0.000	11791317	0	3.885	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
Data File : PS009339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2020 16:27
Operator : DD\AJ
Sample : L1942-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 17:42:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

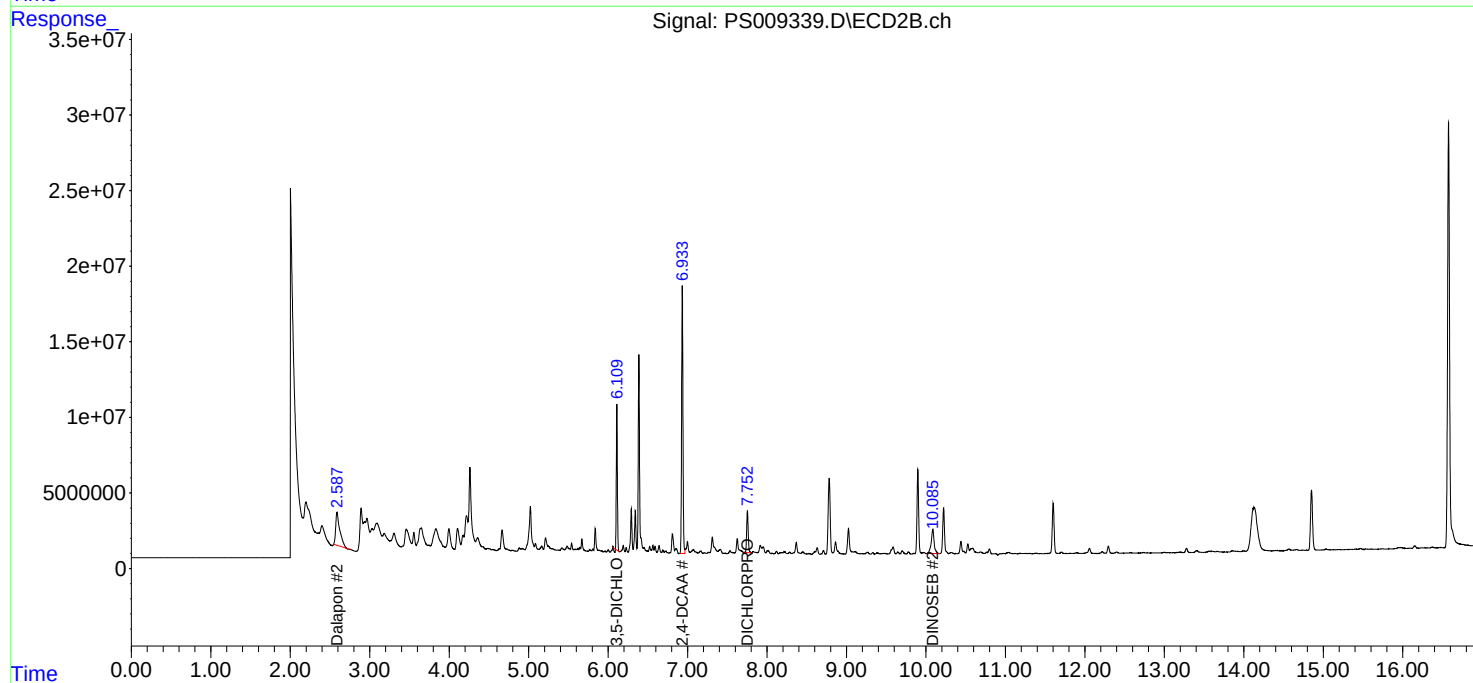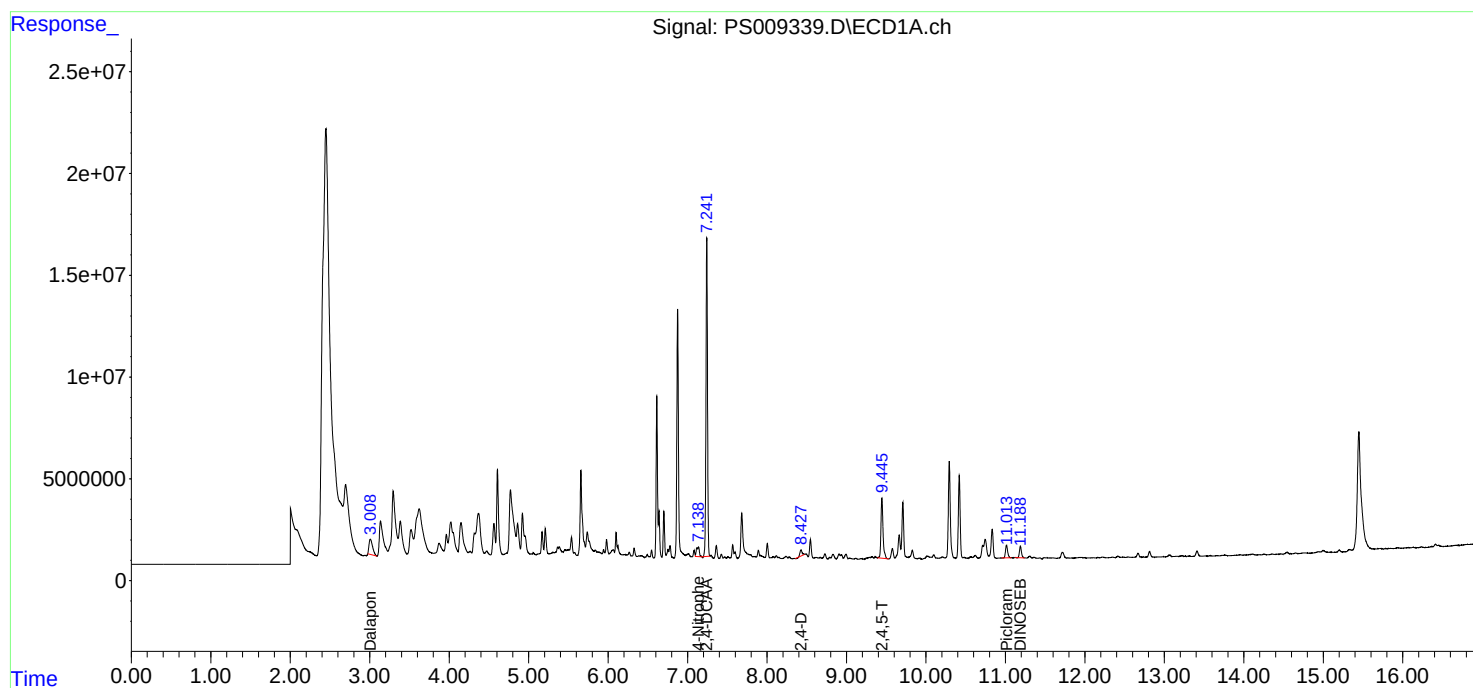


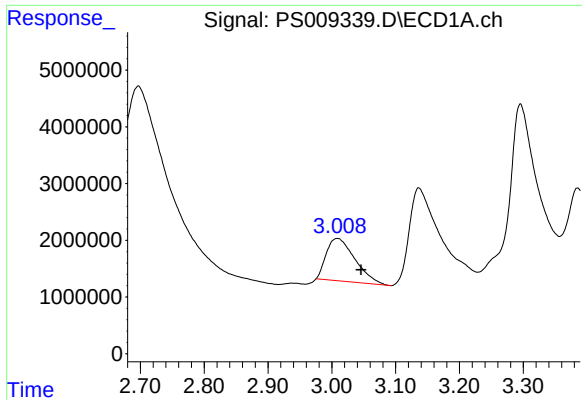

#1 Dalapon


R.T.: 3.009 min
Delta R.T.: -0.037 min
Response: 23306896
Conc: 29.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

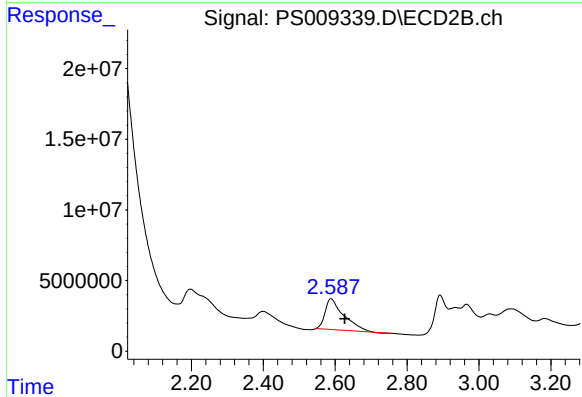


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.039 min
Response: 78101291
Conc: 99.19 ng/ml

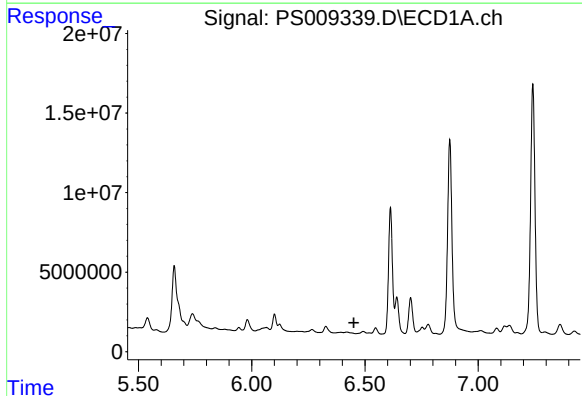


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

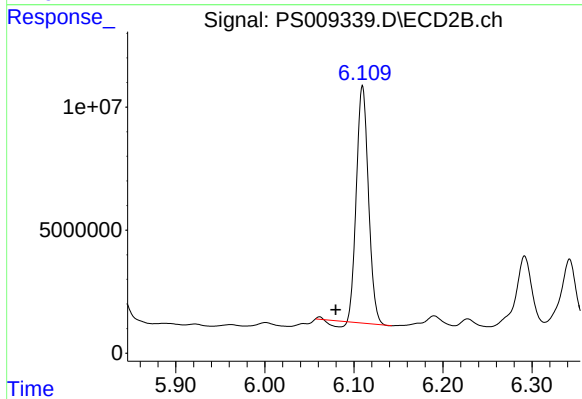

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.110 min
Delta R.T.: 0.030 min
Response: 89181622
Conc: 109.65 ng/ml

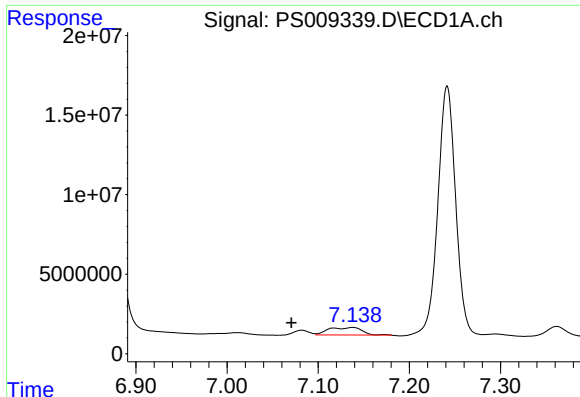

#3 4-Nitrophenol


R.T.: 7.138 min
Delta R.T.: 0.067 min
Response: 11987595
Conc: 50.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

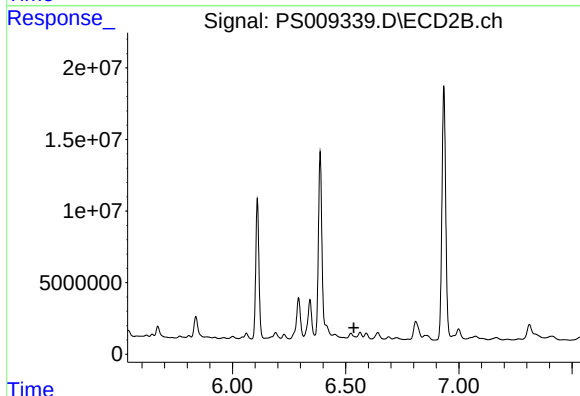


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.536 min
Response: 0
Conc: N.D.

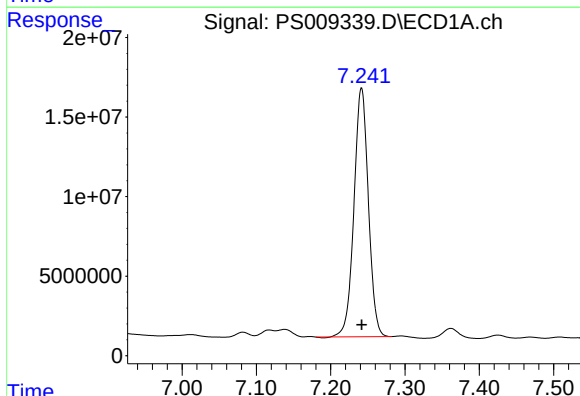


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 210660717
Conc: 380.82 ng/ml

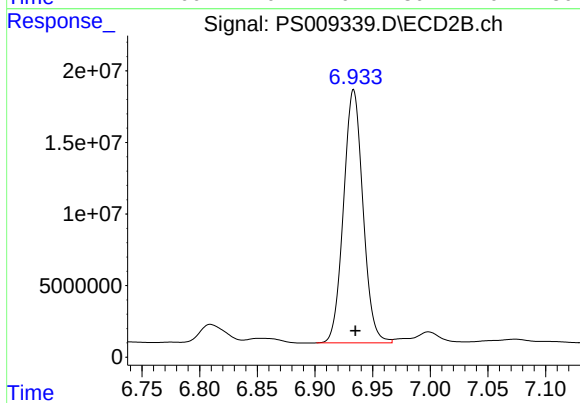

#4 2,4-DCAA


R.T.: 6.934 min
Delta R.T.: -0.002 min
Response: 206707650
Conc: 376.38 ng/ml

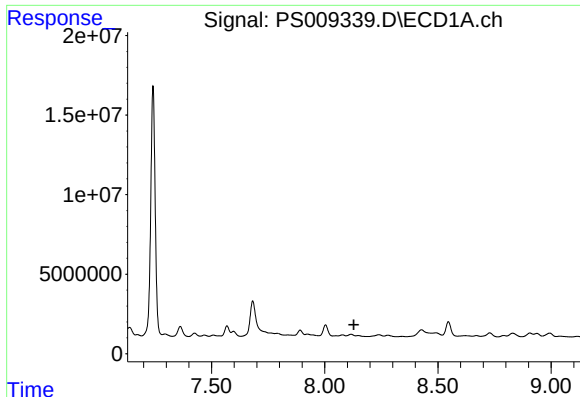

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

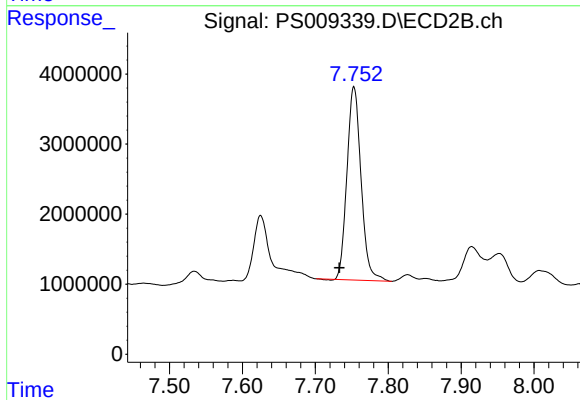


#8 DICHLORPROP

R.T.: 7.753 min
Delta R.T.: 0.020 min
Response: 37097537
Conc: 66.86 ng/ml

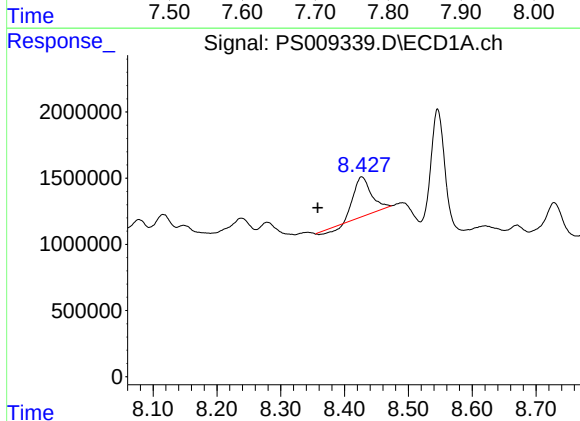


#9 2,4-D

R.T.: 8.427 min
Delta R.T.: 0.069 min
Response: 5359237
Conc: 10.16 ng/ml

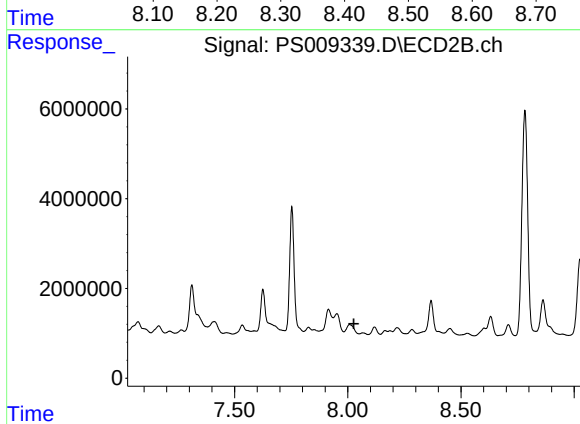

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

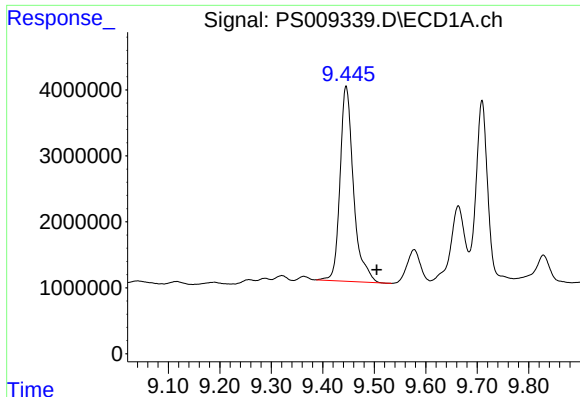

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 53710724
Conc: 21.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

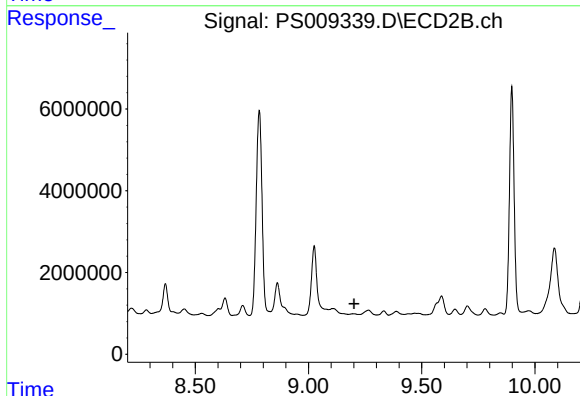


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

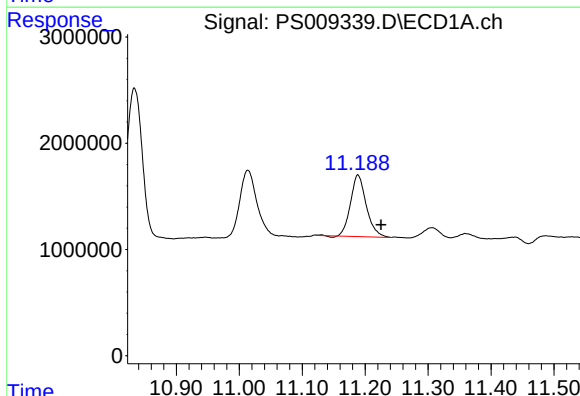


#14 DINOSEB

R.T.: 11.189 min
Delta R.T.: -0.036 min
Response: 10045570
Conc: 4.91 ng/ml

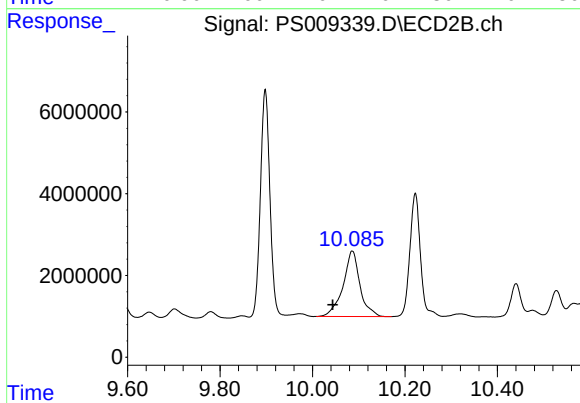

#14 DINOSEB


R.T.: 10.086 min
Delta R.T.: 0.042 min
Response: 40920837
Conc: 18.63 ng/ml

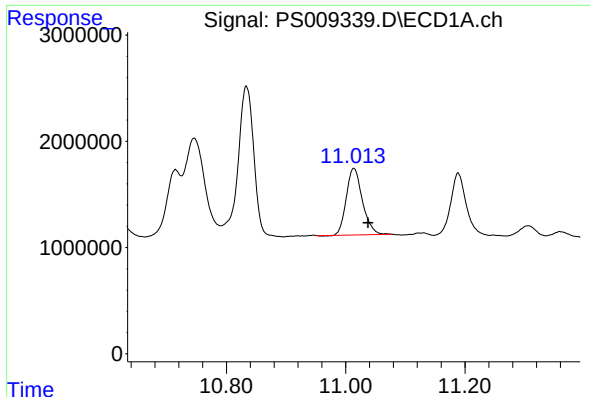

#15 Picloram

R.T.: 11.014 min
Delta R.T.: -0.024 min
Response: 11791317
Conc: 3.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

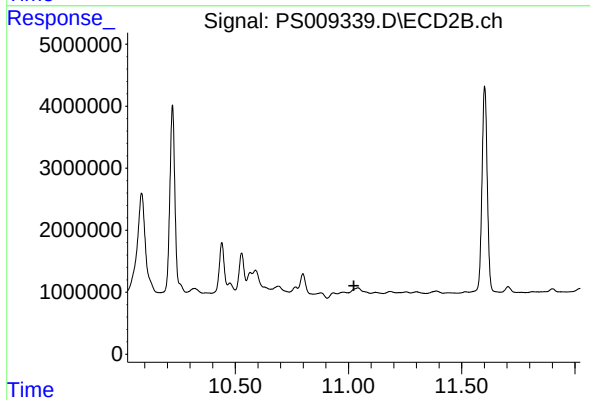

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.