

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
 Data File : PS009344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2020 18:21
 Operator : DD\AJ
 Sample : L1943-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 03:53:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	202.2E6	188.9E6	365.549	343.943
Target Compounds							
1) T	Dalapon	3.007	2.588	26208458	130.0E6	33.608	165.083 #
2) T	3,5-DICHL...	0.000	6.109	0	61063350	N.D.	75.080
3) T	4-Nitroph...	7.117	0.000	12144561	0	50.875	N.D. #
8) T	DICHLORPROP	0.000	7.752	0	39279948	N.D.	70.797
10) T	Pentachlo...	8.670	8.457	123.5E6	132.5E6	17.572	17.462
11) T	2,4,5-TP ...	0.000	8.784	0	34431893	N.D.	11.550
12) T	2,4,5-T	9.446	0.000	42346905	0	16.647	N.D. #
14) T	DINOSEB	11.189	10.086	11088990	43280588	5.425	19.705 #
15) T	Picloram	11.013	0.000	12485828	0	4.114	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031720\
Data File : PS009344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2020 18:21
Operator : DD\AJ
Sample : L1943-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 03:53:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

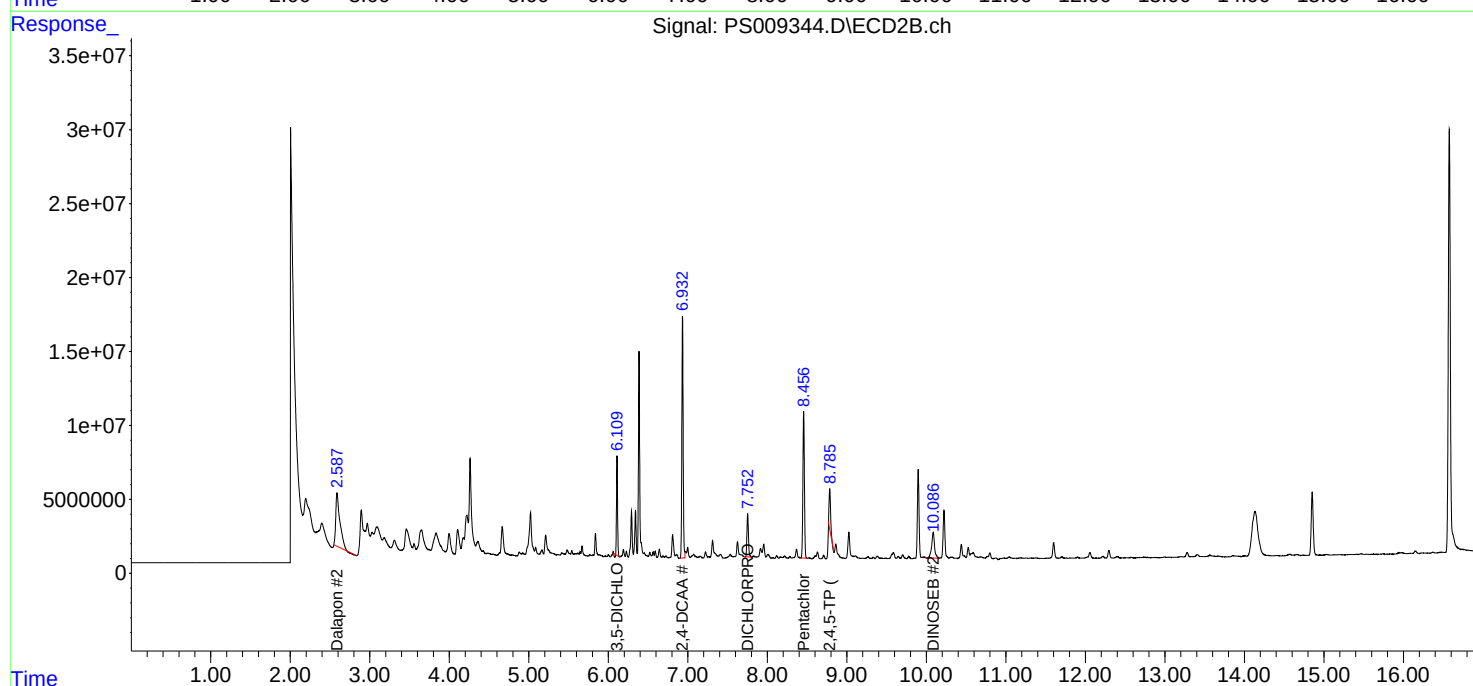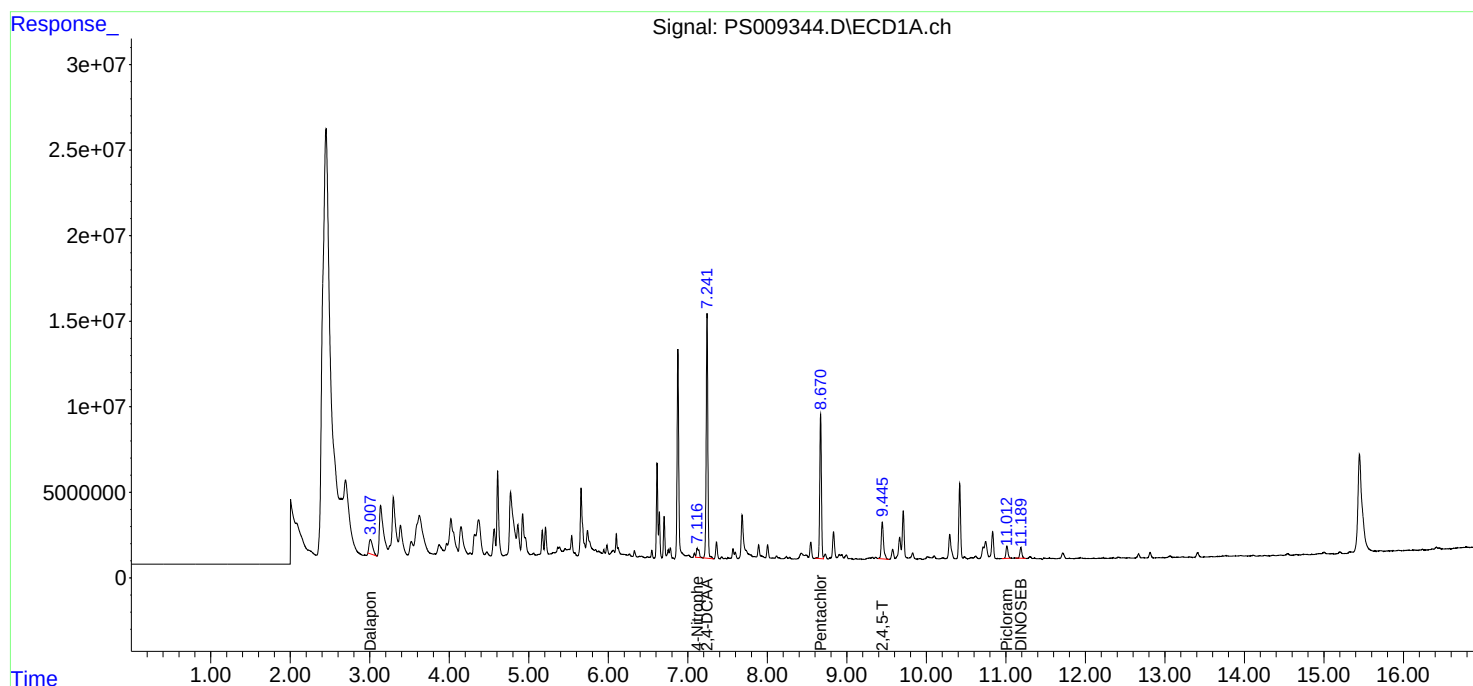


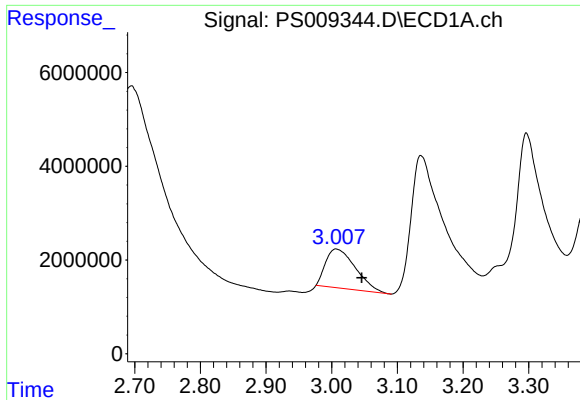

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 26208458
Conc: 33.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

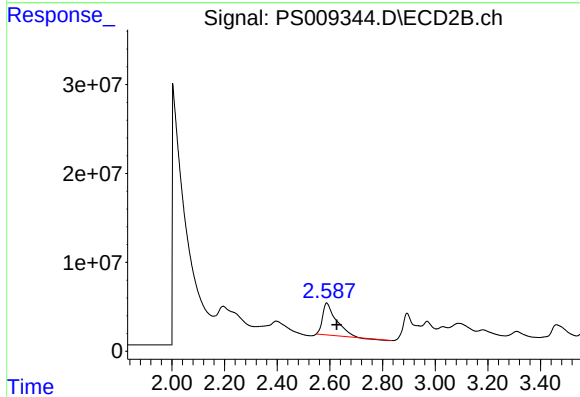


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 129980408
Conc: 165.08 ng/ml

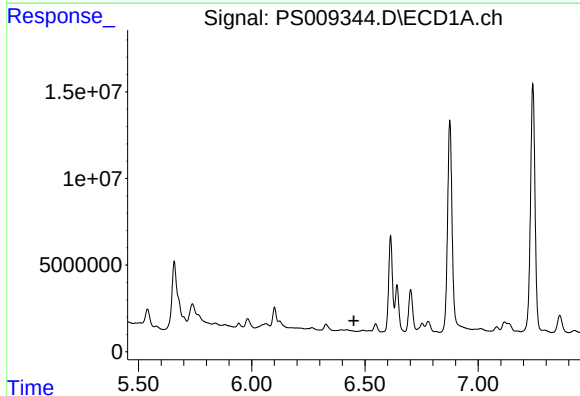


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

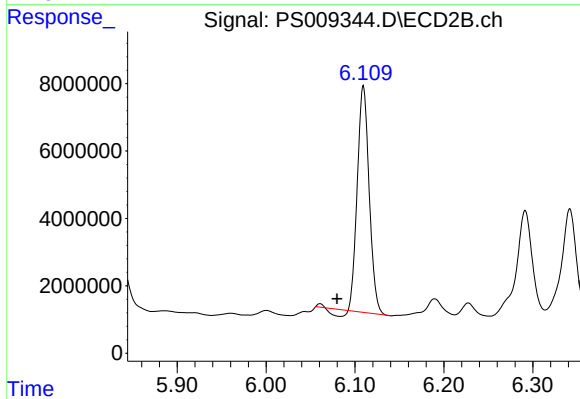

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.030 min
Response: 61063350
Conc: 75.08 ng/ml

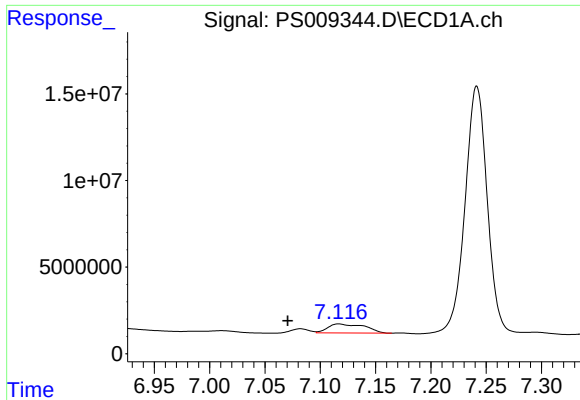

#3 4-Nitrophenol


R.T.: 7.117 min
Delta R.T.: 0.046 min
Response: 12144561
Conc: 50.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

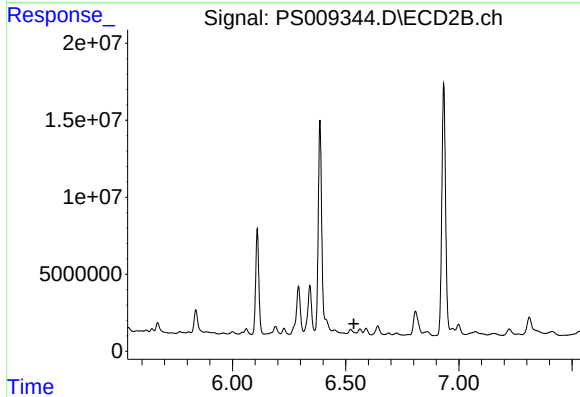


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.536 min
Response: 0
Conc: N.D.

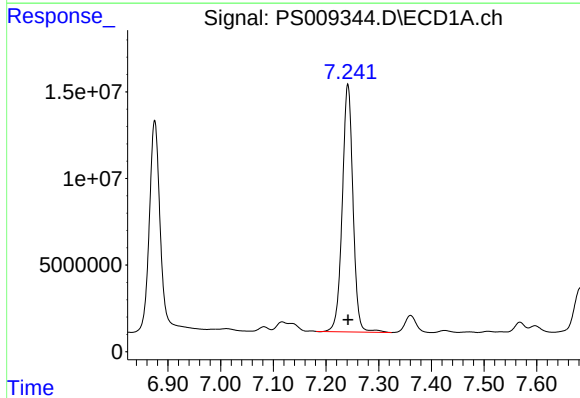


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 202211058
Conc: 365.55 ng/ml

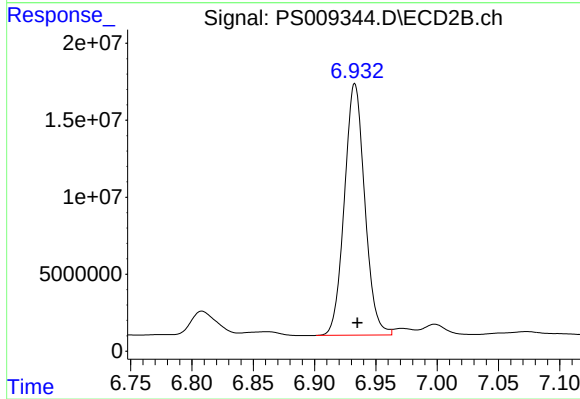

#4 2,4-DCAA


R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 188892779
Conc: 343.94 ng/ml

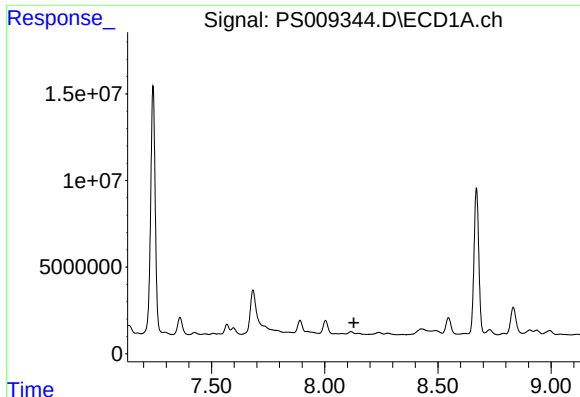

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

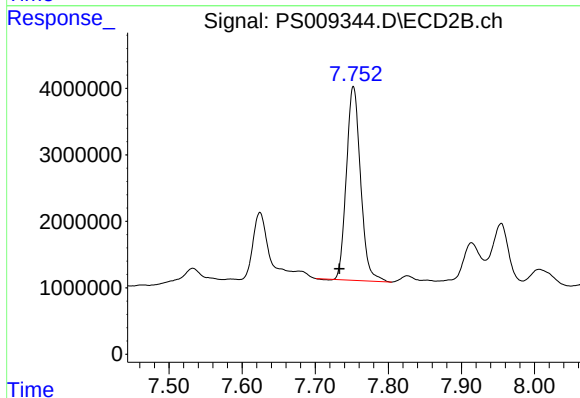


#8 DICHLORPROP

R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 39279948
Conc: 70.80 ng/ml

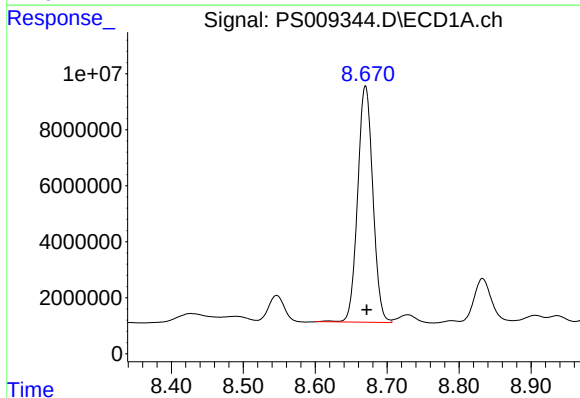


#10 Pentachlorophenol

R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 123549567
Conc: 17.57 ng/ml

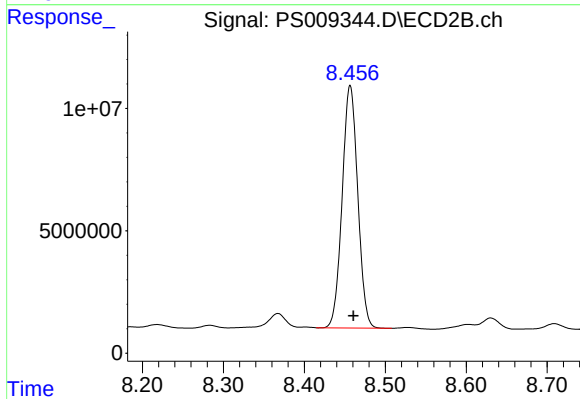

#10 Pentachlorophenol


R.T.: 8.457 min
Delta R.T.: -0.004 min
Response: 132539893
Conc: 17.46 ng/ml

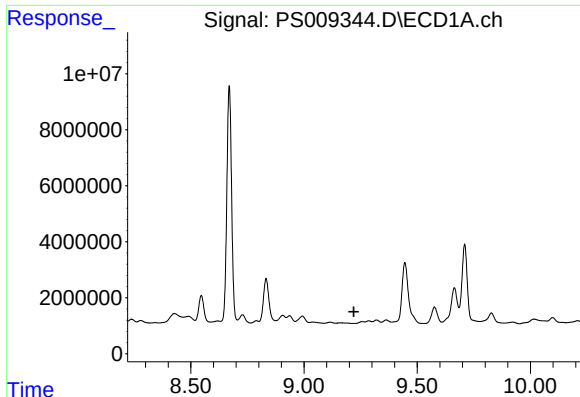

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

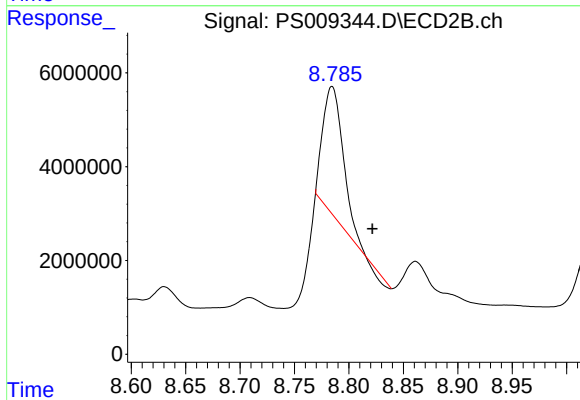


#11 2,4,5-TP (SILVEX)

R.T.: 8.784 min
Delta R.T.: -0.037 min
Response: 34431893
Conc: 11.55 ng/ml

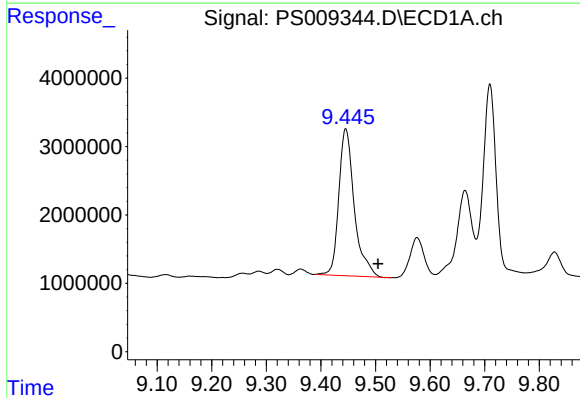


#12 2,4,5-T

R.T.: 9.446 min
Delta R.T.: -0.059 min
Response: 42346905
Conc: 16.65 ng/ml

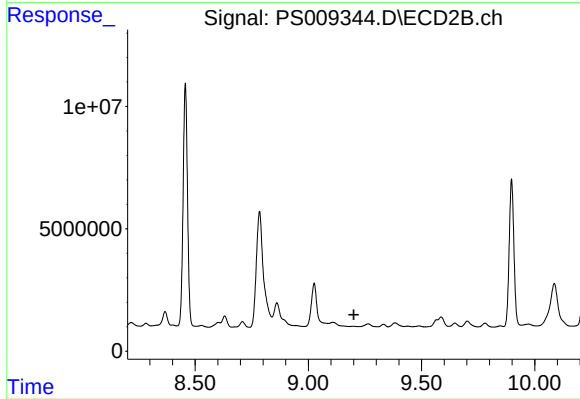

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

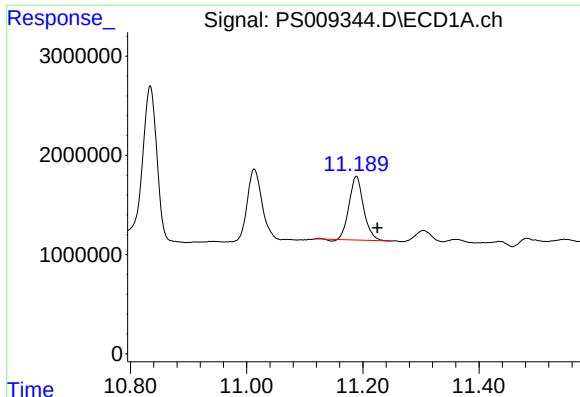

#14 DINOSEB


R.T.: 11.189 min
Delta R.T.: -0.036 min
Response: 11088990
Conc: 5.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

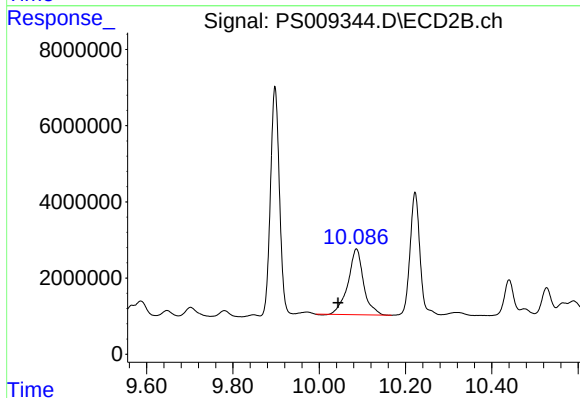


#14 DINOSEB

R.T.: 10.086 min
Delta R.T.: 0.043 min
Response: 43280588
Conc: 19.70 ng/ml

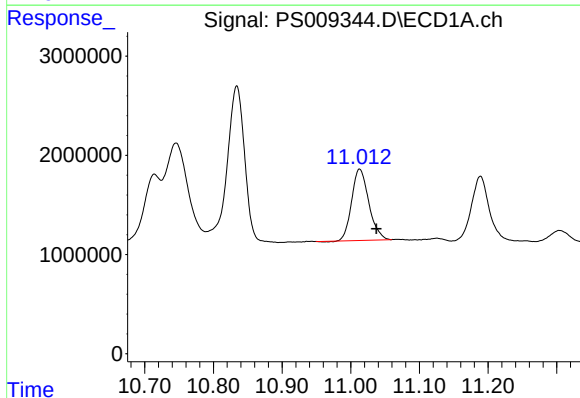

#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.024 min
Response: 12485828
Conc: 4.11 ng/ml

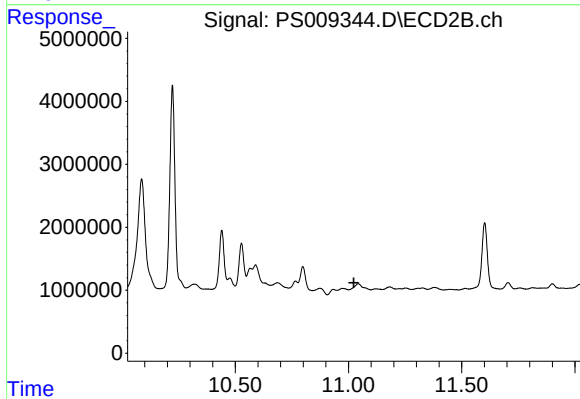

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.