

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031721\
 Data File : PS014267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2021 09:05
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 02:27:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.170	6.891	615.3E6	248.9E6	430.625	527.647
Target Compounds							
5) T	DICAMBA	0.000	7.119f	0	2864203	N.D.	1.430
6) T	MCP	0.000	7.119	0	2864203	N.D.	1.720
9) T	2,4-D	8.341f	0.000	25382857	0	17.221	N.D. #
11) T	2,4,5-TP ...	0.000	8.747	0	780921	N.D.	<MDL
12) T	2,4,5-T	9.341f	0.000	21553883	0	2.770	N.D. #
15) T	Picloram	10.960	10.984	68222666	50053966	6.533	13.194 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031721\
Data File : PS014267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2021 09:05
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 02:27:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

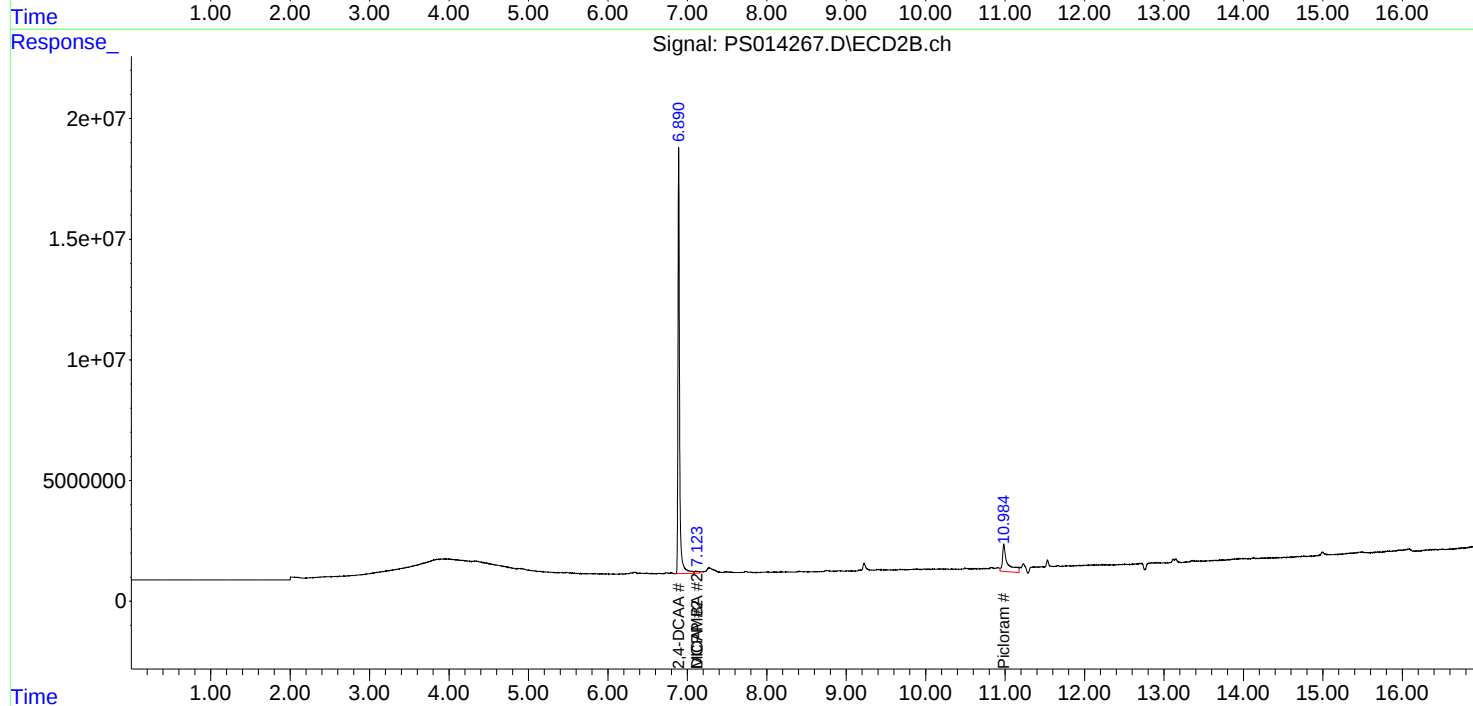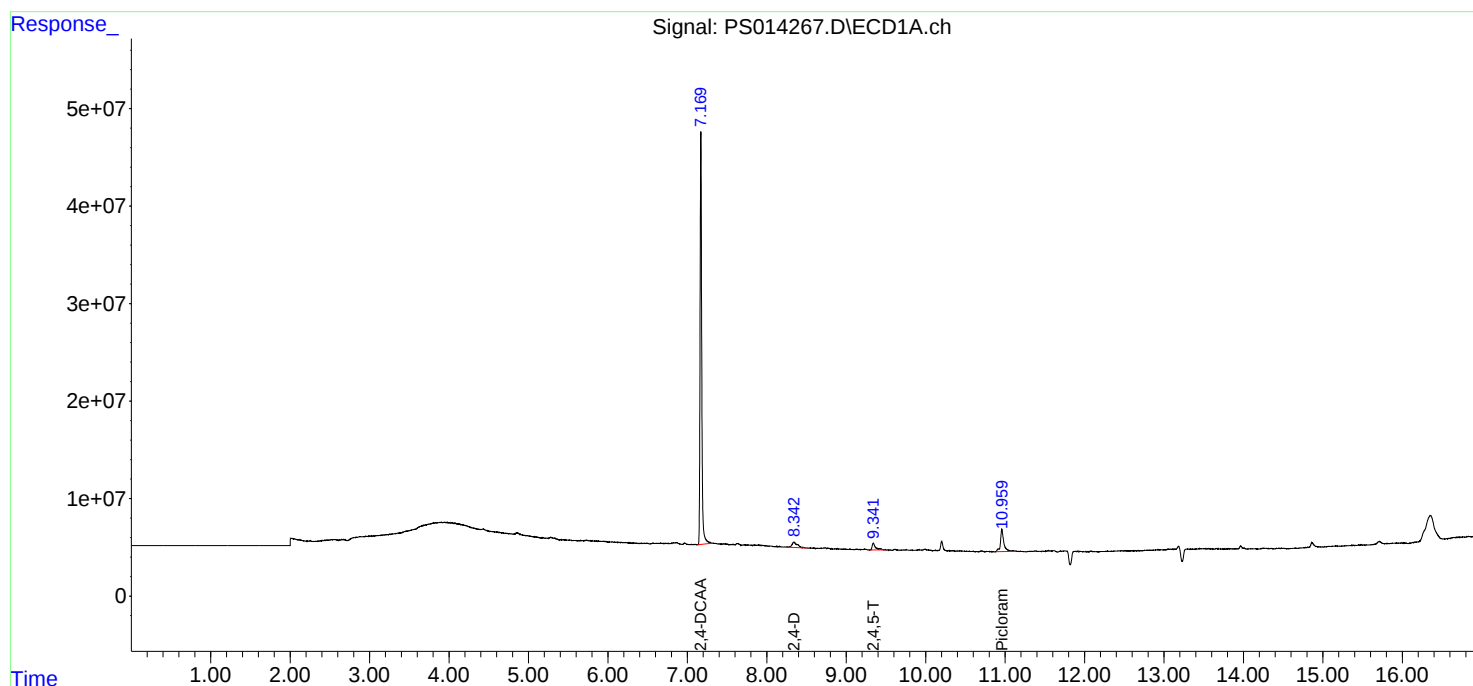


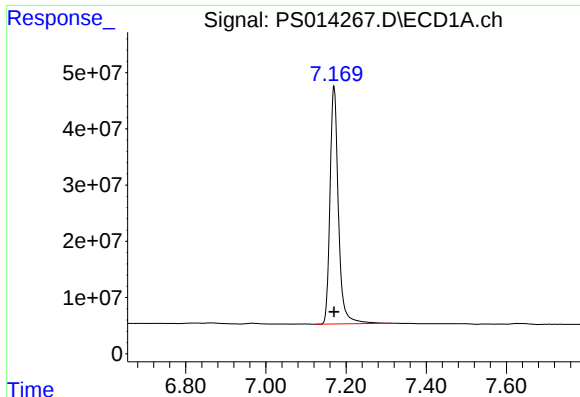

#4 2,4-DCAA


R.T.: 7.170 min
Delta R.T.: 0.000 min
Response: 615295623
Conc: 430.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

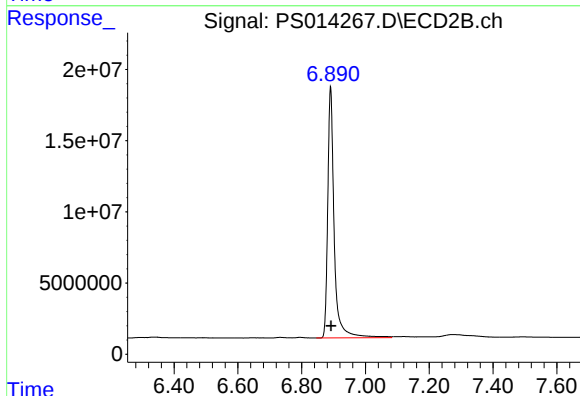


#4 2,4-DCAA

R.T.: 6.891 min
Delta R.T.: 0.000 min
Response: 248927511
Conc: 527.65 ng/ml

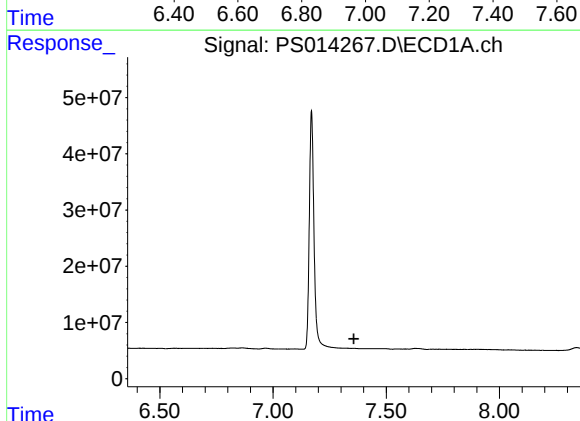


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.

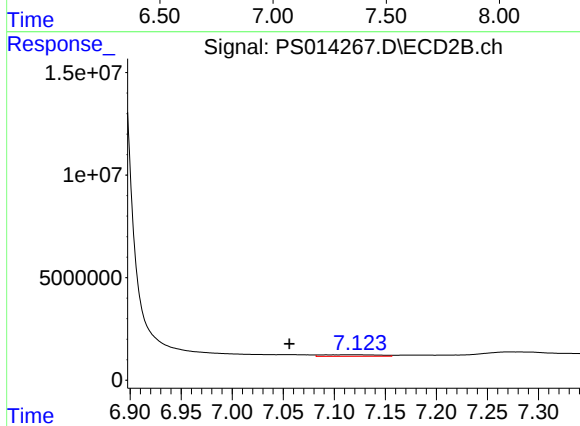

#5 DICAMBA


R.T.: 7.119 min
Delta R.T.: 0.063 min
Response: 2864203
Conc: 1.43 ng/ml

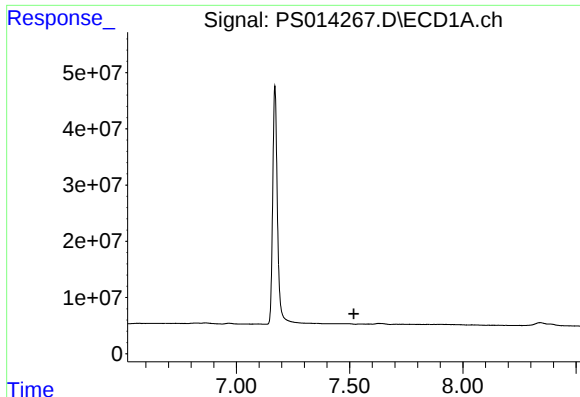

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

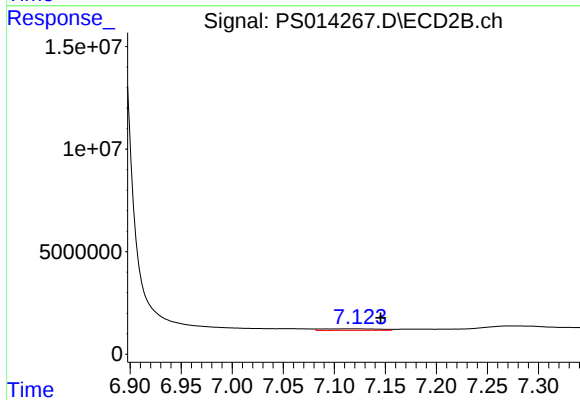


#6 MCP

R.T.: 7.119 min
Delta R.T.: -0.027 min
Response: 2864203
Conc: 1.72 ug/ml

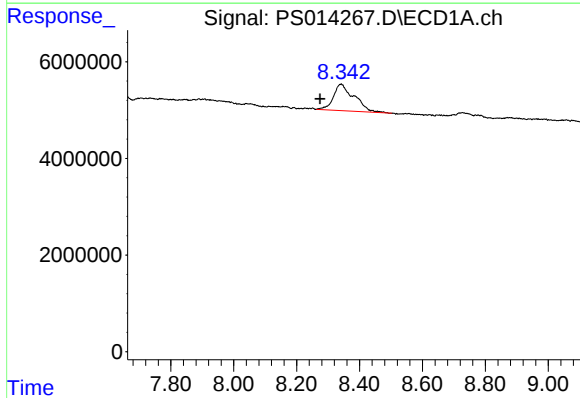


#9 2,4-D

R.T.: 8.341 min
Delta R.T.: 0.066 min
Response: 25382857
Conc: 17.22 ng/ml

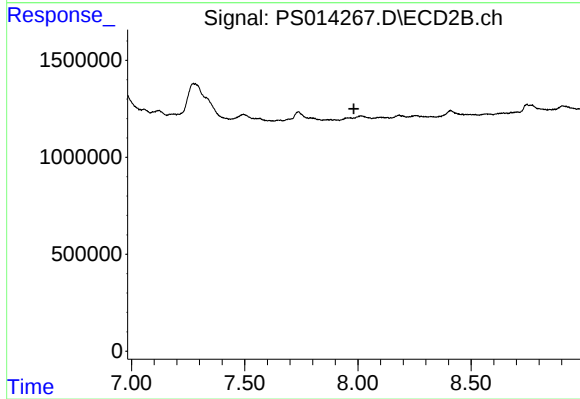

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.982 min
Response: 0
Conc: N.D.

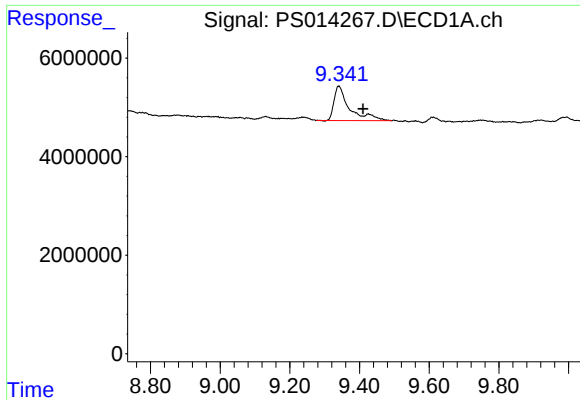

#12 2,4,5-T


R.T.: 9.341 min
Delta R.T.: -0.069 min
Response: 21553883
Conc: 2.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

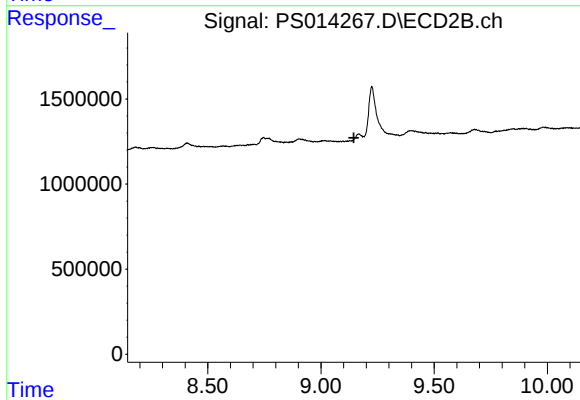


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.145 min
Response: 0
Conc: N.D.

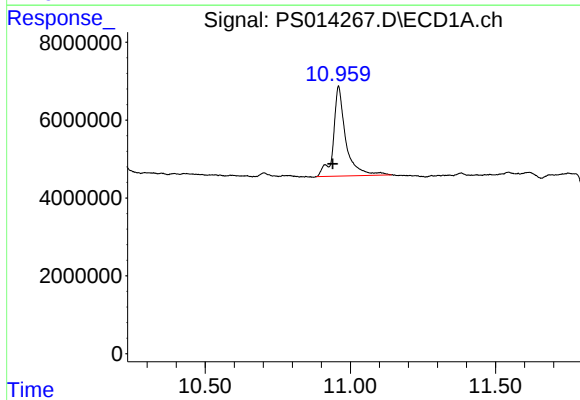

#15 Picloram

R.T.: 10.960 min
Delta R.T.: 0.020 min
Response: 68222666
Conc: 6.53 ng/ml

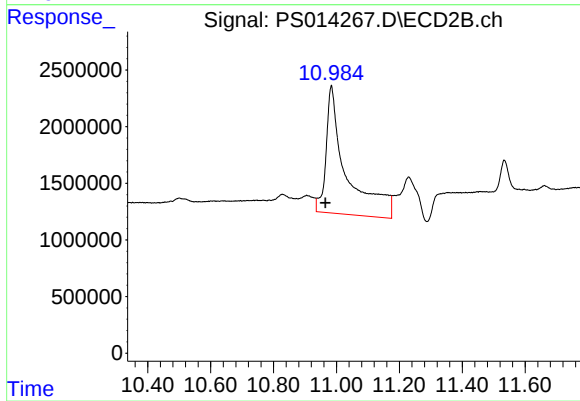

#15 Picloram

R.T.: 10.984 min
Delta R.T.: 0.020 min
Response: 50053966
Conc: 13.19 ng/ml