

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031721\
 Data File : PS014279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2021 16:42
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 02:28:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.167	6.887	621.0E6	246.0E6	434.640	521.478
Target Compounds							
5) T	DICAMBA	0.000	7.054	0	5728089	N.D.	2.859
6) T	MCPD	0.000	7.174	0	917858	N.D.	<MDL
7) T	MCPA	7.624f	0.000	1390620	0	<MDL	N.D. #
10) T	Pentachlo...	8.579	8.401	6290513	4070557	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.765	0	3112304	N.D.	1.144
12) T	2,4,5-T	0.000	9.158	0	2928955	N.D.	1.099
14) T	DINOSEB	0.000	9.977	0	1395748	N.D.	<MDL
15) T	Picloram	10.907	10.982	8033844	5288189	<MDL	1.394 #
16) T	DCPA	0.000	10.902	0	3786111	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031721\
Data File : PS014279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2021 16:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 02:28:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

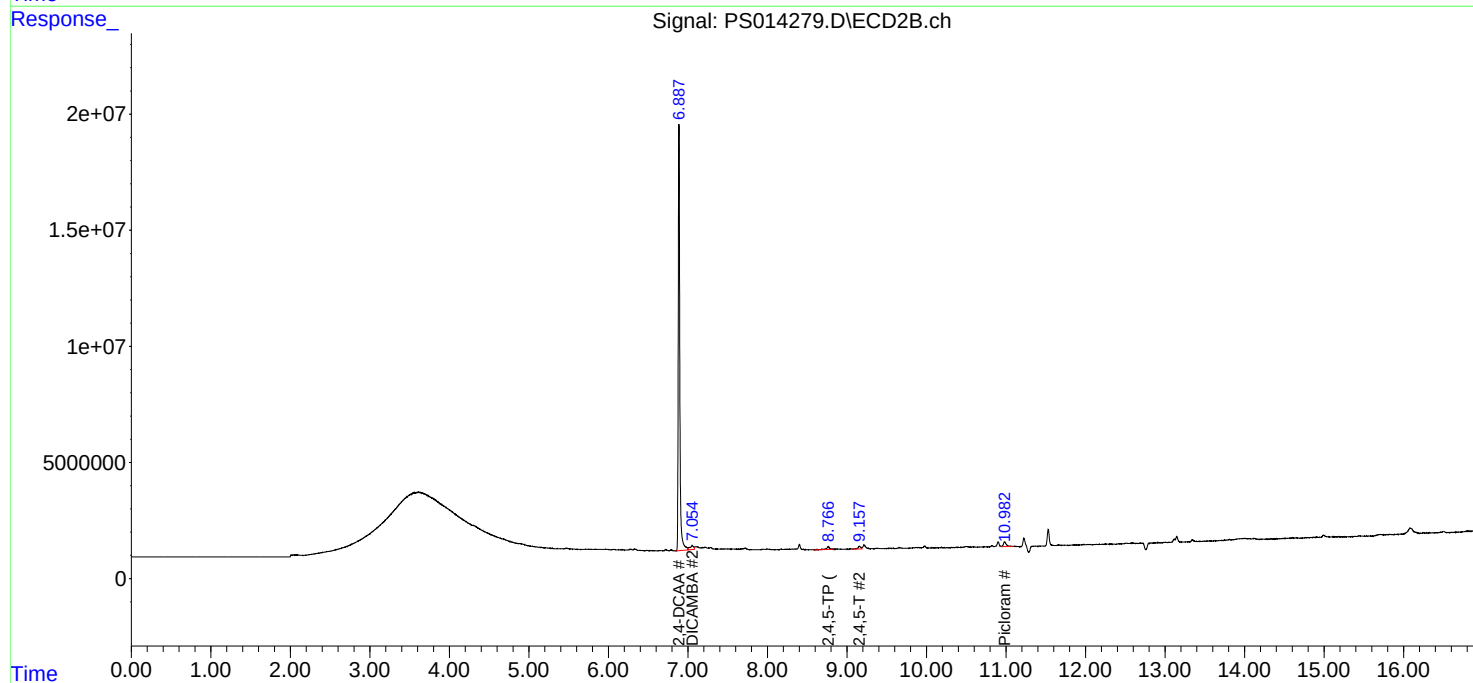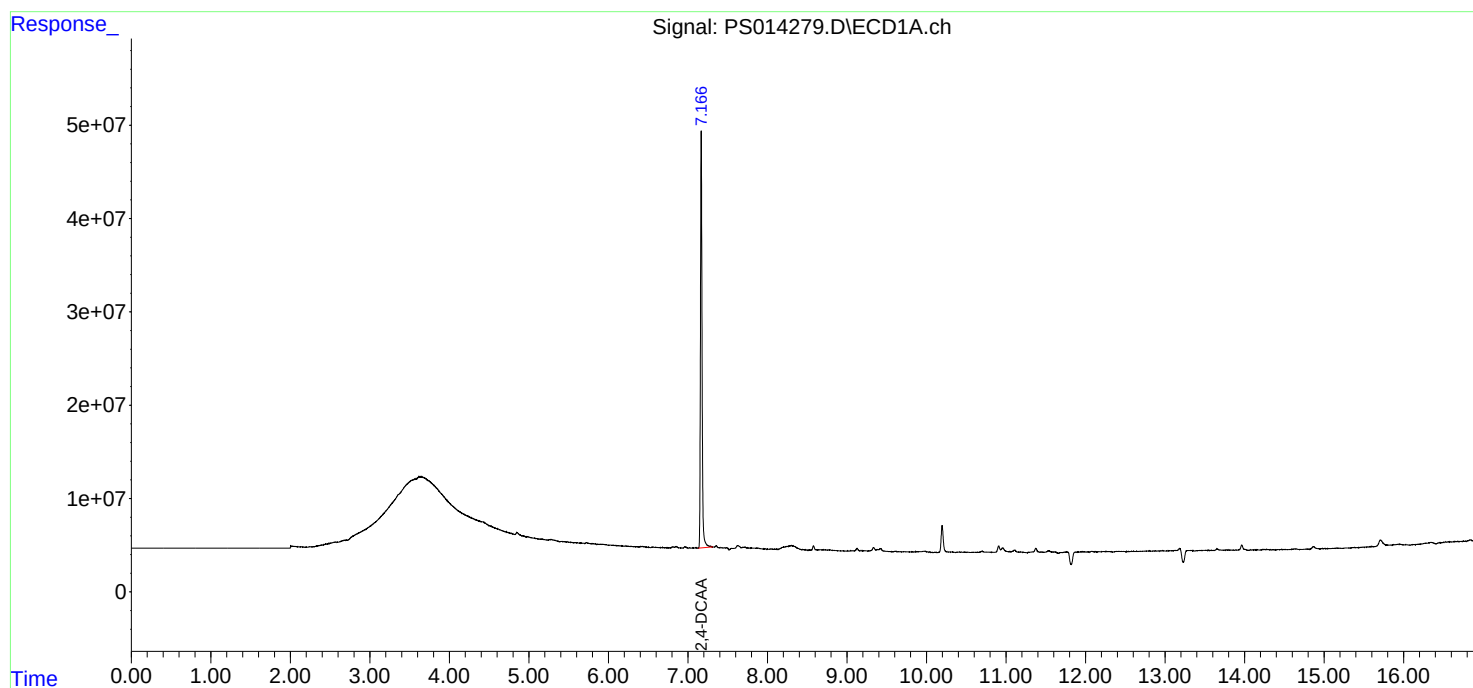


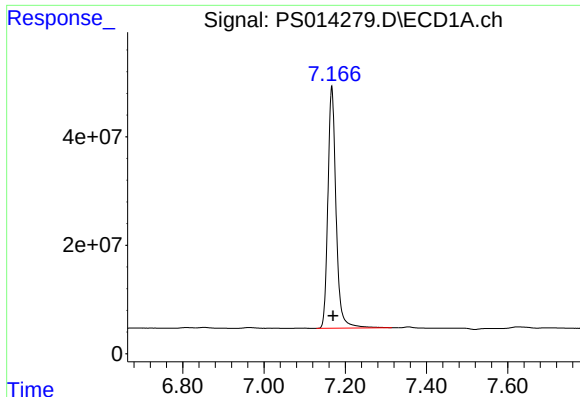

#4 2,4-DCAA


R.T.: 7.167 min
Delta R.T.: -0.003 min
Response: 621031673
Conc: 434.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

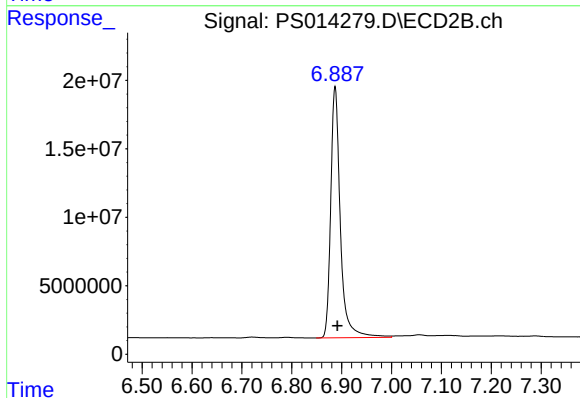


#4 2,4-DCAA

R.T.: 6.887 min
Delta R.T.: -0.005 min
Response: 246017258
Conc: 521.48 ng/ml

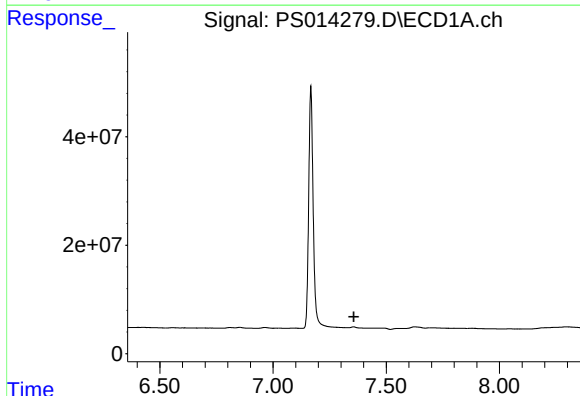


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.

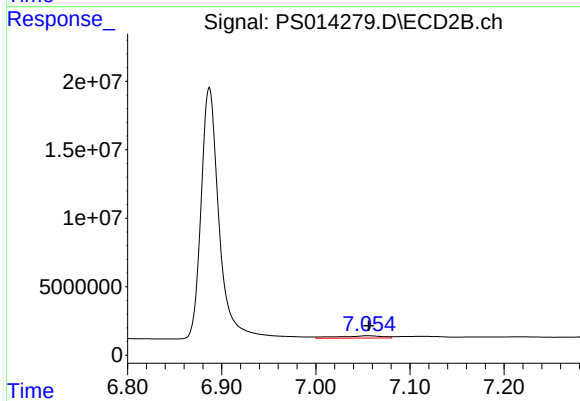

#5 DICAMBA


R.T.: 7.054 min
Delta R.T.: -0.002 min
Response: 5728089
Conc: 2.86 ng/ml

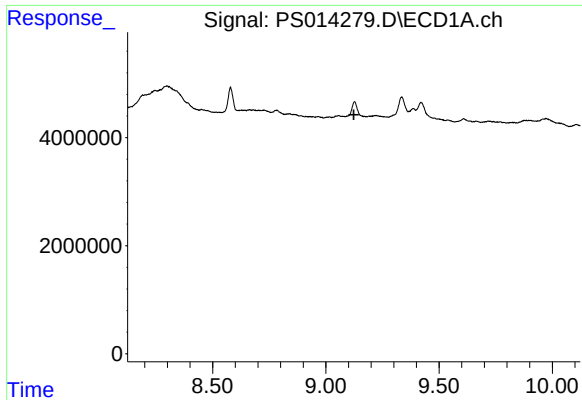

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

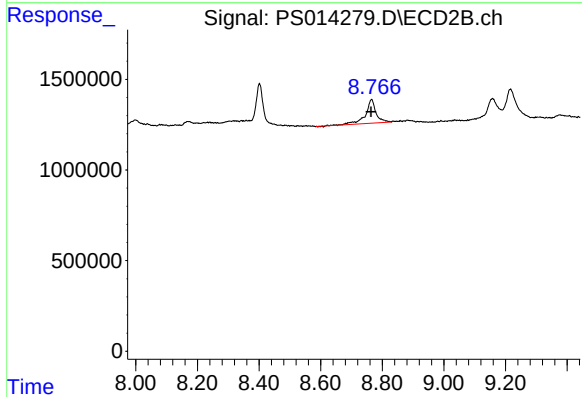


#11 2,4,5-TP (SILVEX)

R.T.: 8.765 min
Delta R.T.: 0.002 min
Response: 3112304
Conc: 1.14 ng/ml

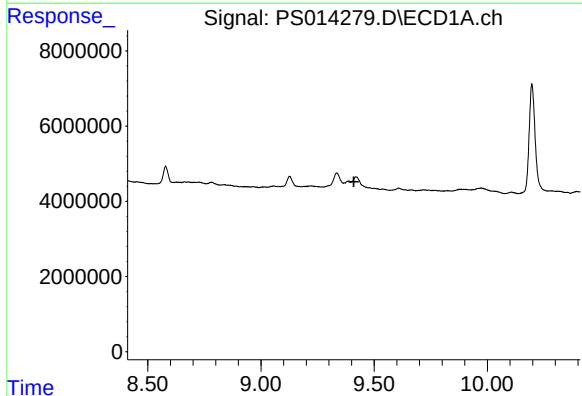


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

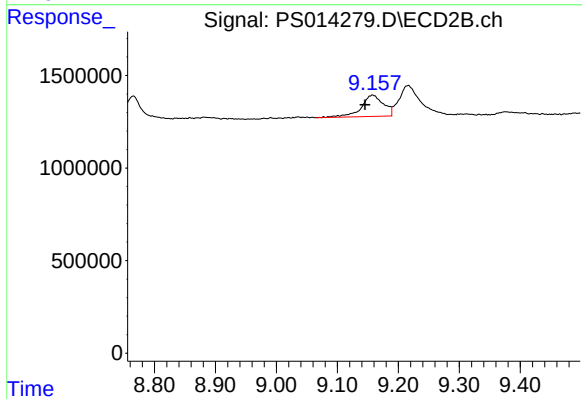

#12 2,4,5-T


R.T.: 9.158 min
Delta R.T.: 0.013 min
Response: 2928955
Conc: 1.10 ng/ml

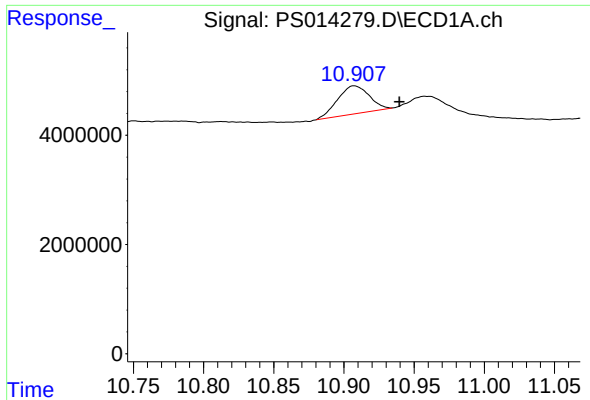

#15 Picloram

R.T.: 10.907 min
Delta R.T.: -0.032 min
Response: 8033844
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

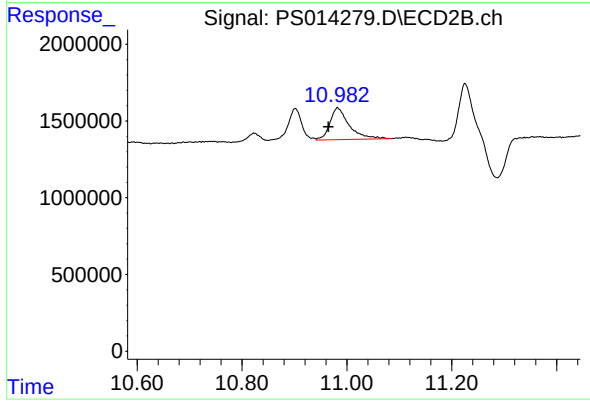

#15 Picloram

R.T.: 10.982 min
Delta R.T.: 0.017 min
Response: 5288189
Conc: 1.39 ng/ml