

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031723\
 Data File : PS022404.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2023 08:43
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 22:18:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.314	0.000	1482775	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.443	2.513	1110580	736712	<MDL	<MDL #
3) T	4-Nitroph...	6.141	0.000	5702544	0	4.481	N.D. #
5) T	DICAMBA	6.443	6.881	1492739	3520011	<MDL	<MDL #
6) T	MCP	0.000	6.929f	0	10595905	N.D.	1.388
7) T	MCPA	6.743	0.000	87064	0	<MDL	N.D. #
8) T	DICHLORPROP	6.958f	7.540	168150	3133012	<MDL	1.274 #
9) T	2,4-D	7.200	0.000	75634790	0	23.068	N.D. #
10) T	Pentachlo...	7.448	8.209	2161959	3334817	<MDL	<MDL #
11) T	2,4,5-TP ...	7.982	8.578	10875751	3225628	<MDL	<MDL #
12) T	2,4,5-T	8.267	8.973	9191796	1674618	<MDL	<MDL #
13) T	2,4-DB	8.726	0.000	526306	0	<MDL	N.D. #
15) T	Picloram	9.605	10.703f	119.3E6	61945743	4.842	3.160 #
16) T	DCPA	10.042	10.703	3625603	61945743	<MDL	3.959 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031723\
Data File : PS022404.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2023 08:43
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 22:18:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

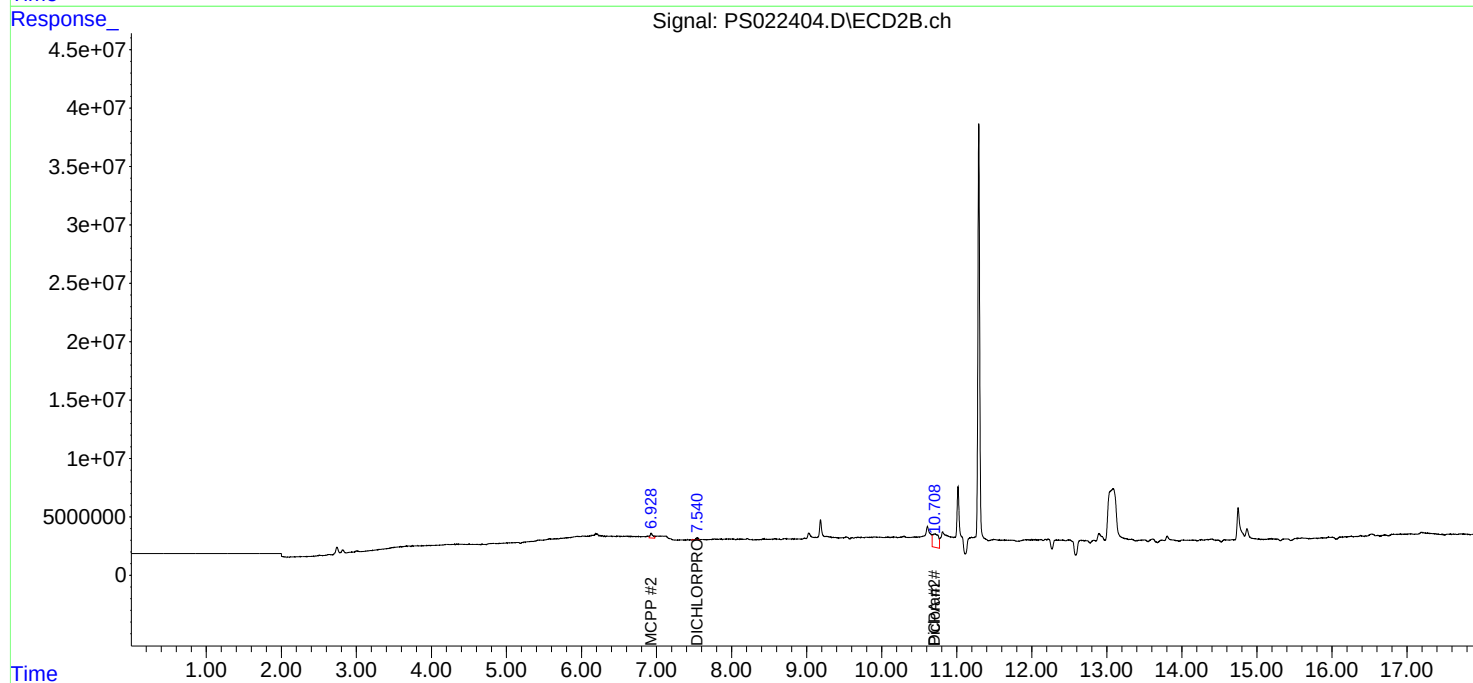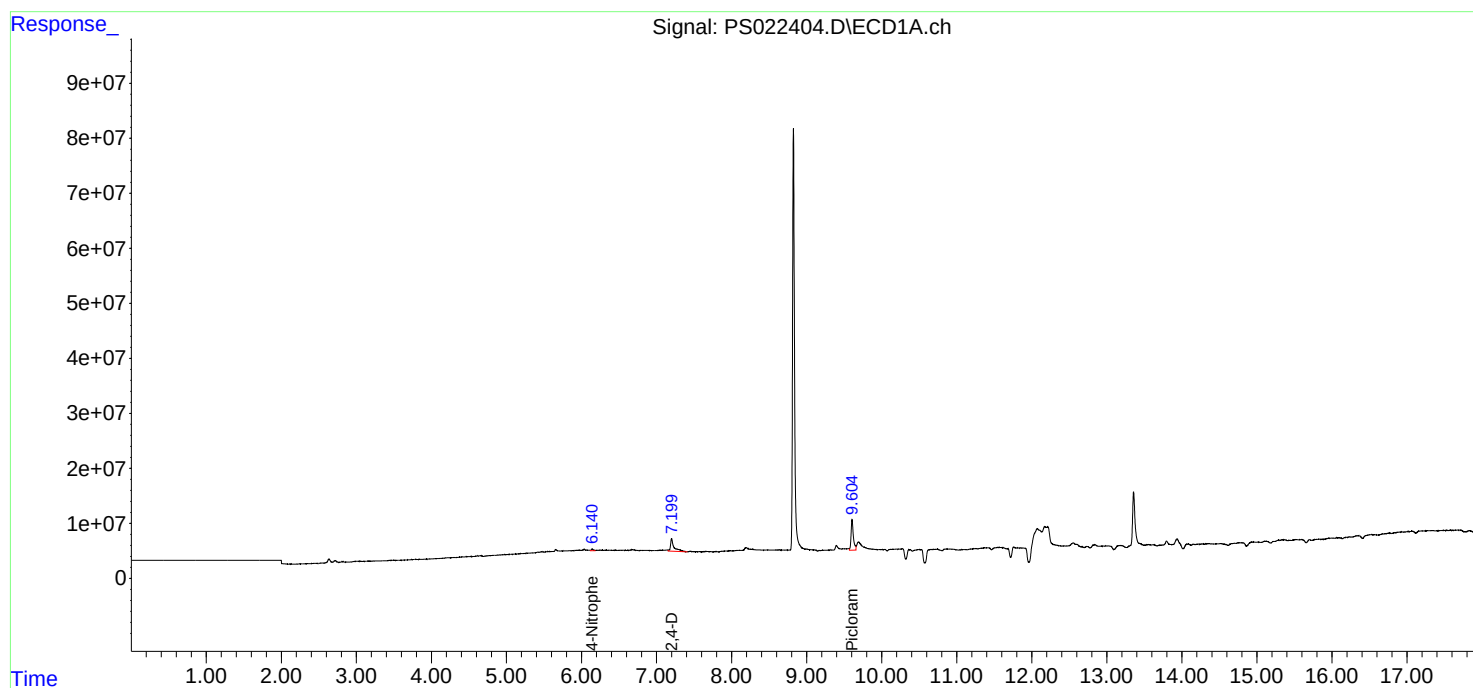


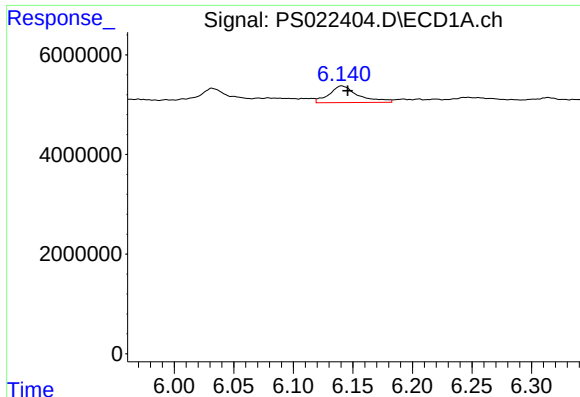

#3 4-Nitrophenol


R.T.: 6.141 min
Delta R.T.: -0.005 min
Response: 5702544
Conc: 4.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

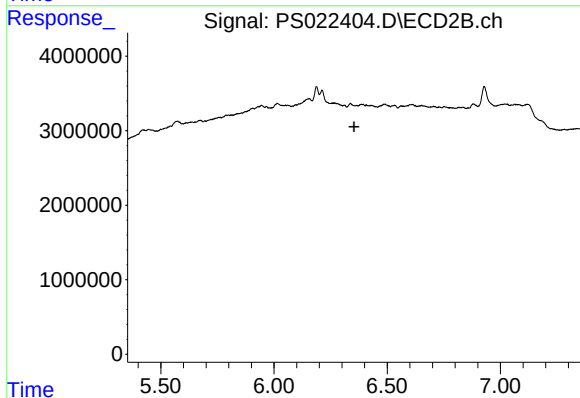


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

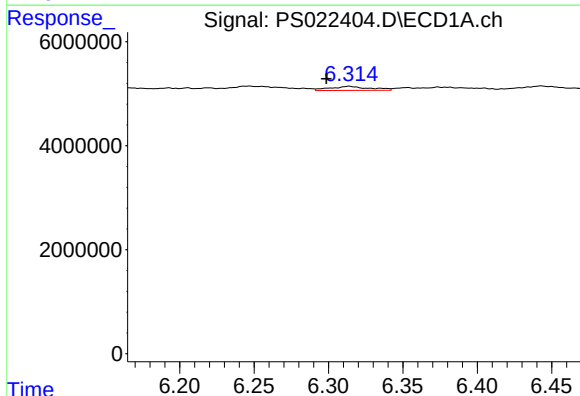


#4 2,4-DCAA

R.T.: 6.314 min
Delta R.T.: 0.015 min
Response: 1482775
Conc: N.D.

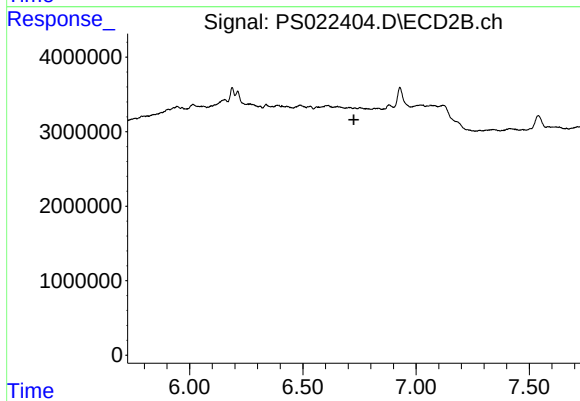

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.726 min
Response: 0
Conc: N.D.

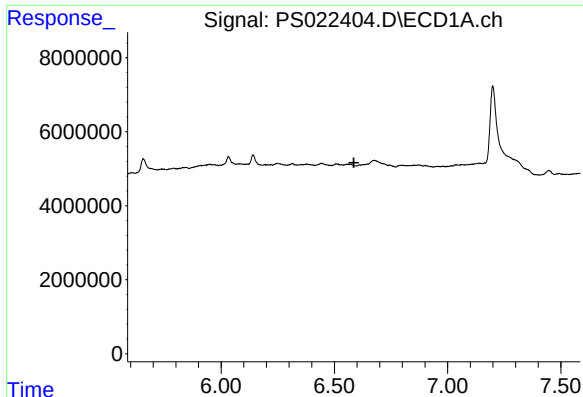

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

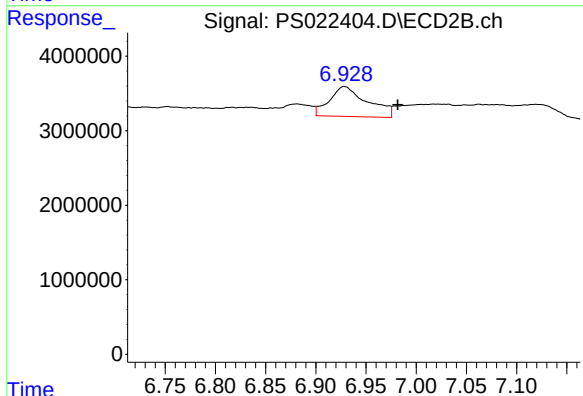


#6 MCP

R.T.: 6.929 min
Delta R.T.: -0.053 min
Response: 10595905
Conc: 1.39 ug/ml

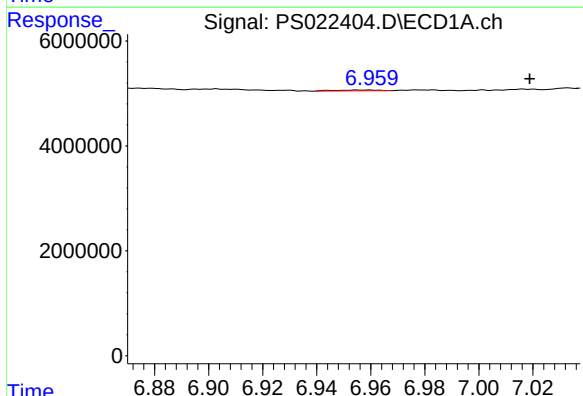


#8 DICHLORPROP

R.T.: 6.958 min
Delta R.T.: -0.061 min
Response: 168150
Conc: N.D.

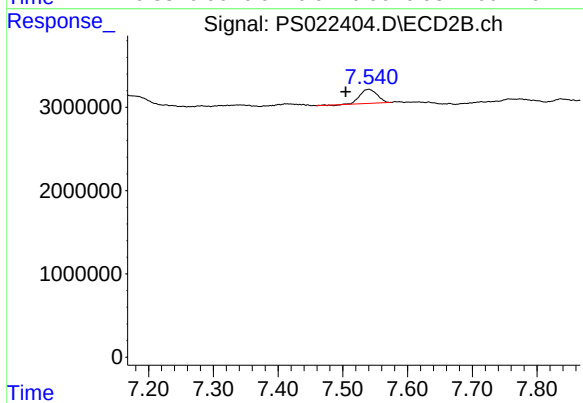

#8 DICHLORPROP


R.T.: 7.540 min
Delta R.T.: 0.035 min
Response: 3133012
Conc: 1.27 ng/ml

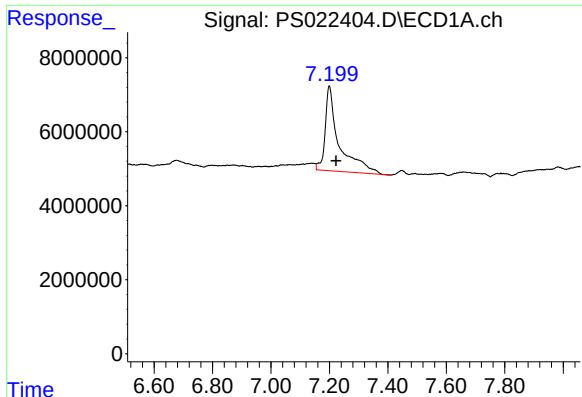

#9 2,4-D


R.T.: 7.200 min
Delta R.T.: -0.023 min
Response: 75634790
Conc: 23.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

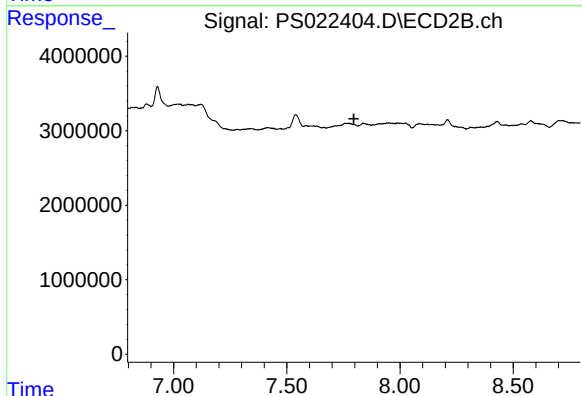


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.796 min
Response: 0
Conc: N.D.

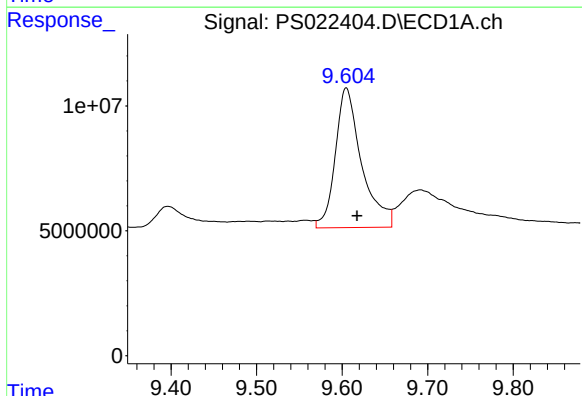


#15 Picloram

R.T.: 9.605 min
Delta R.T.: -0.013 min
Response: 119272057
Conc: 4.84 ng/ml

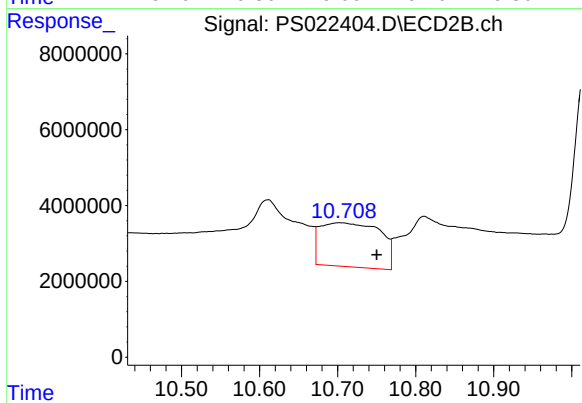

#15 Picloram


R.T.: 10.703 min
Delta R.T.: -0.047 min
Response: 61945743
Conc: 3.16 ng/ml

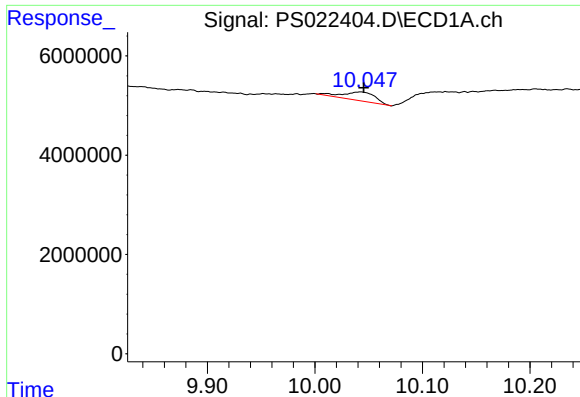

#16 DCPA

R.T.: 10.042 min
Delta R.T.: -0.003 min
Response: 3625603
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

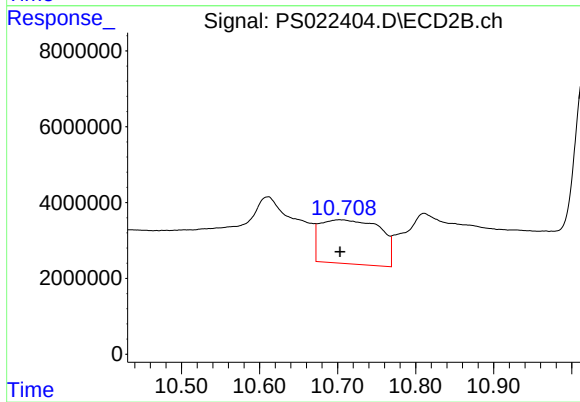

#16 DCPA

R.T.: 10.703 min
Delta R.T.: 0.000 min
Response: 61945743
Conc: 3.96 ng/ml