

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS031723\  
 Data File : PS022416.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 17 Mar 2023 22:53  
 Operator : AR\AJ  
 Sample : 01954-03  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 SV-TP2-0316

Manual Integrations  
 APPROVED

Reviewed By :Abdul Mirza 03/20/2023  
 Supervised By :Ankita Jodhani 03/20/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 18 02:06:37 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS022023.M  
 Quant Title : 8080.M  
 QLast Update : Mon Feb 20 13:26:02 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1  | Resp#2  | ng/ml    | ng/ml   |
|-----------------------------|-------|-------|---------|---------|----------|---------|
| -----                       |       |       |         |         |          |         |
| System Monitoring Compounds |       |       |         |         |          |         |
| 4) S 2,4-DCAA               | 6.296 | 6.721 | 916.0E6 | 662.3E6 | 369.538m | 315.559 |

Target Compounds

-----

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS031723\  
Data File : PS022416.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Mar 2023 22:53  
Operator : AR\AJ  
Sample : 01954-03  
Misc :  
ALS Vial : 11 Sample Multiplier: 1



Instrument :  
ECD\_S  
ClientSampleId :  
SV-TP2-0316


Manual Integrations  
APPROVED

Reviewed By : Abdul Mirza 03/20/2023  
Supervised By : Ankita Jodhani 03/20/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 18 02:06:37 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS022023.M  
Quant Title : 8080.M  
QLast Update : Mon Feb 20 13:26:02 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

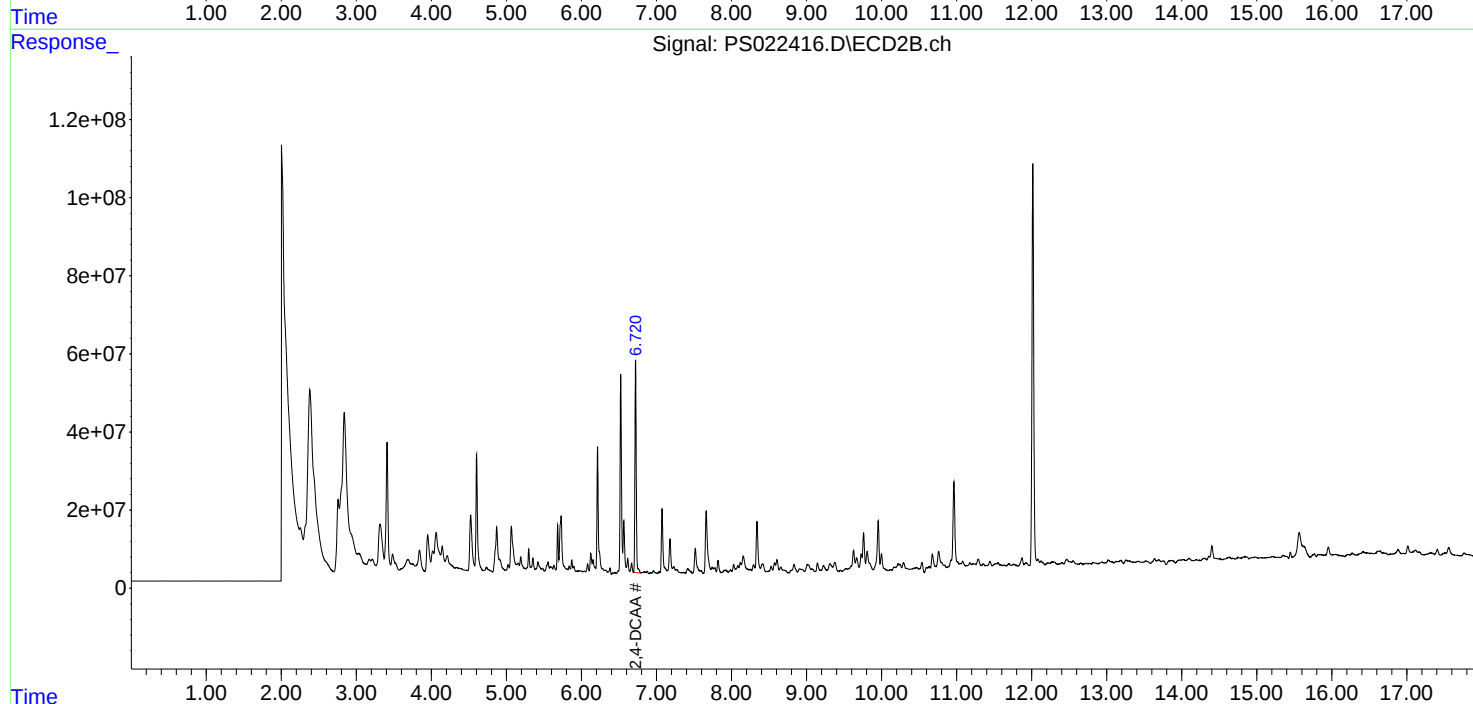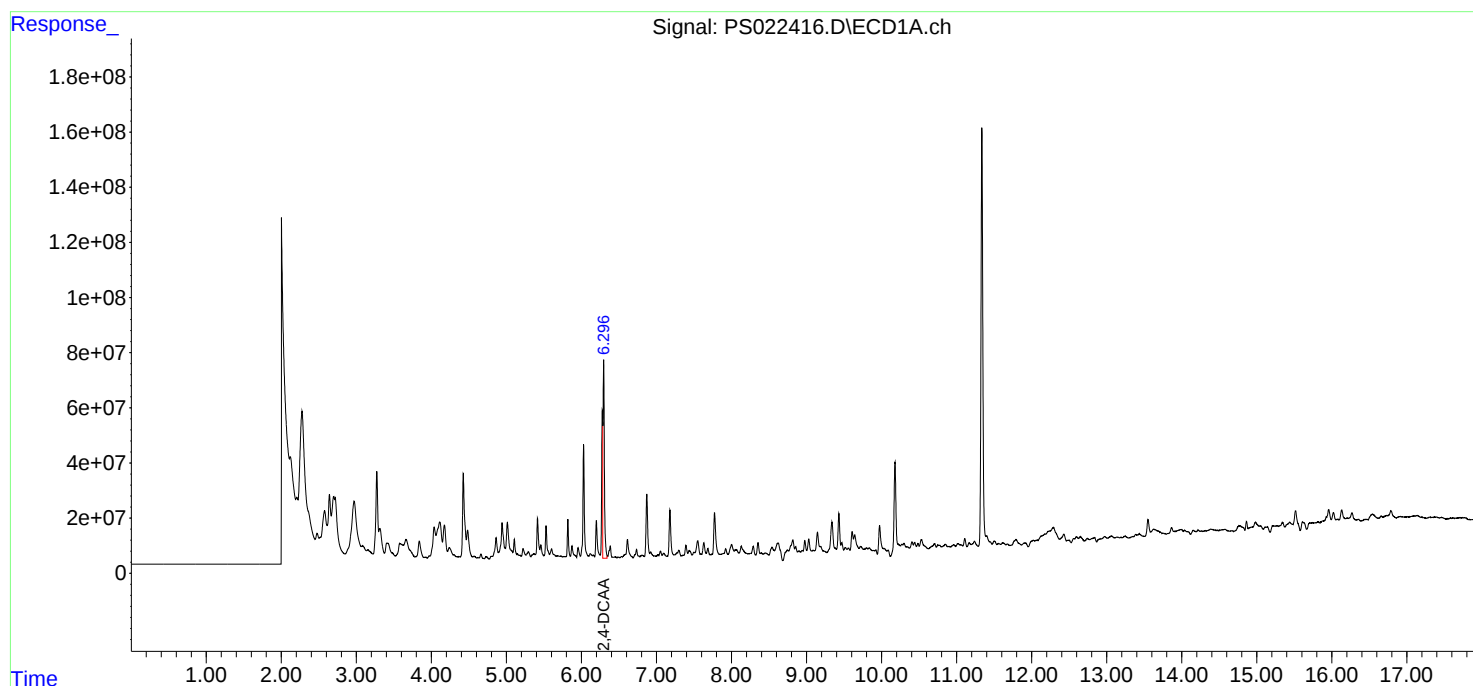

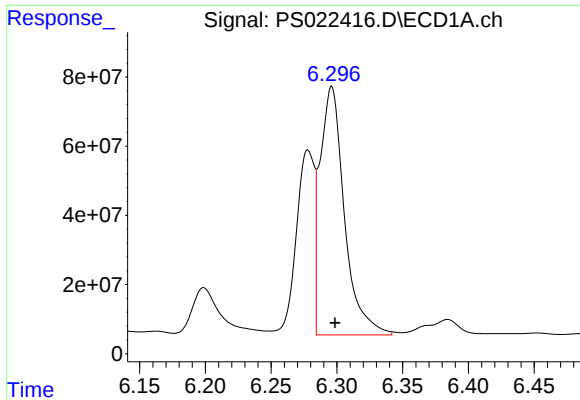


#4 2,4-DCAA

R.T.: 6.296 min  
Delta R.T.: -0.003 min  
Response: 915969476  
Conc: 369.54 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
SV-TP2-0316

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 03/20/2023  
Supervised By :Ankita Jodhani 03/20/2023

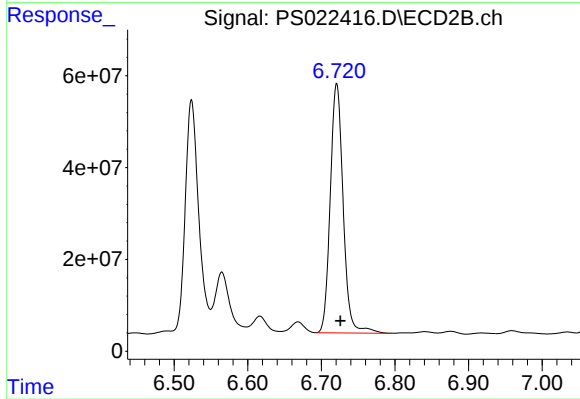

#4 2,4-DCAA

R.T.: 6.721 min  
Delta R.T.: -0.005 min  
Response: 662347056  
Conc: 315.56 ng/ml