

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031725\
 Data File : PS029441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2025 09:25
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:41:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.137	0.000	1144342	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.335	0.000	1509379	0	<MDL	N.D. #
3) T	4-Nitroph...	6.974	0.000	322429	0	<MDL	N.D. #
5) T	DICAMBA	7.331	0.000	14222	0	<MDL	N.D. #
6) T	MCP	7.563f	0.000	3885169	0	<MDL	N.D. #
7) T	MCPA	7.652	0.000	2731314	0	<MDL	N.D. #
8) T	DICHLORPROP	8.030	0.000	2407258	0	<MDL	N.D. #
9) T	2,4-D	8.285	0.000	2813927	0	<MDL	N.D. #
10) T	Pentachlo...	8.565	9.339f	3071541	10927987	<MDL	<MDL #
11) T	2,4,5-TP ...	9.125	0.000	5074559	0	<MDL	N.D. #
12) T	2,4,5-T	9.446	10.165	4273741	3434397	<MDL	<MDL #
13) T	2,4-DB	9.996	0.000	2847600	0	<MDL	N.D. #
14) T	DINOSEB	11.178	0.000	2381798	0	<MDL	N.D. #
15) T	Picloram	11.023	12.168	40653119	85087418	1.331	7.359 #
16) T	DCPA	11.489	12.123	4267017	21781795	<MDL	1.840 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031725\
Data File : PS029441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2025 09:25
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:41:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

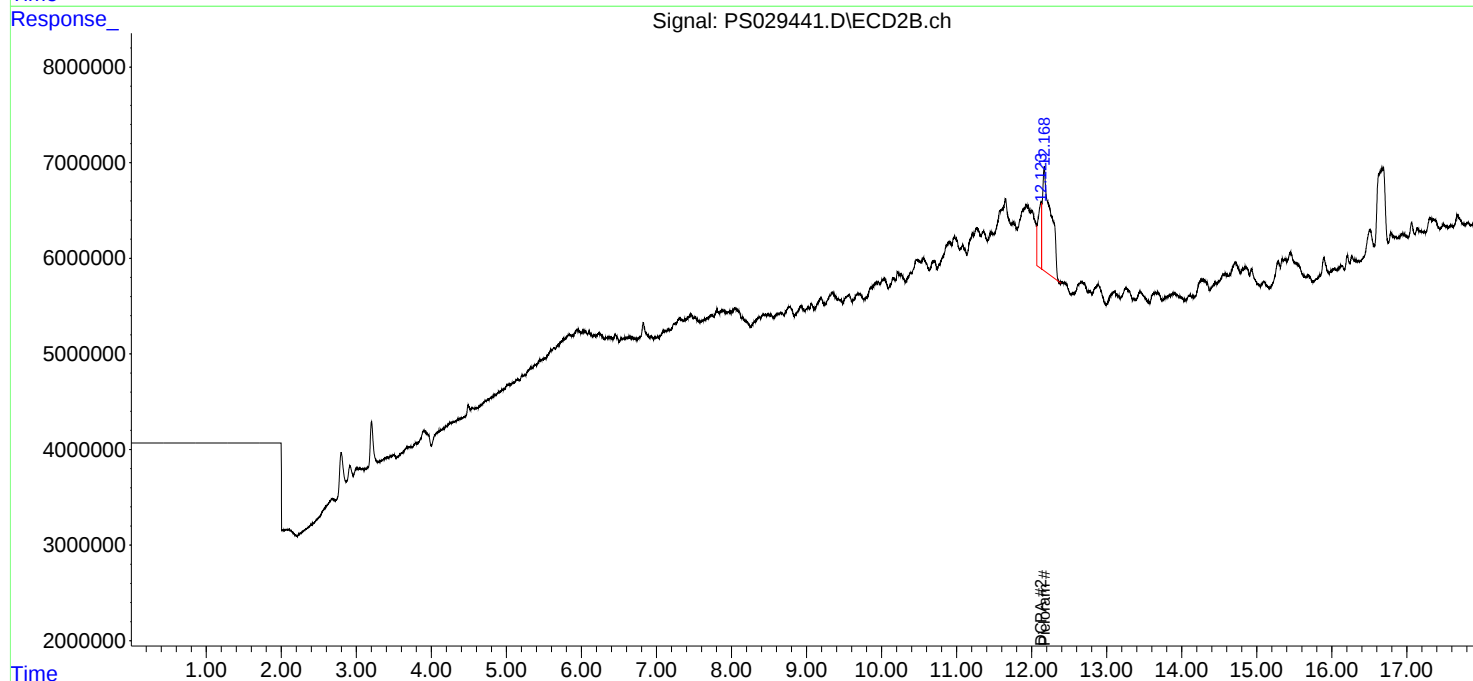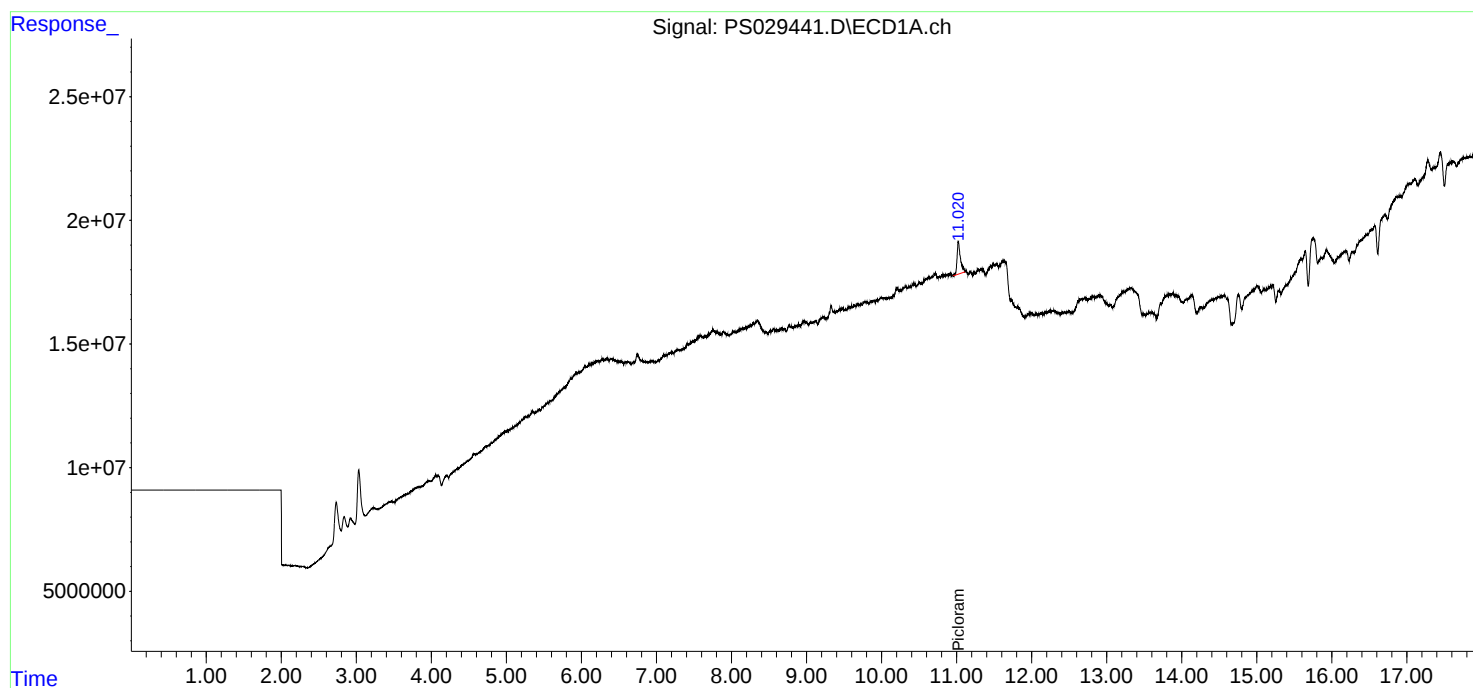


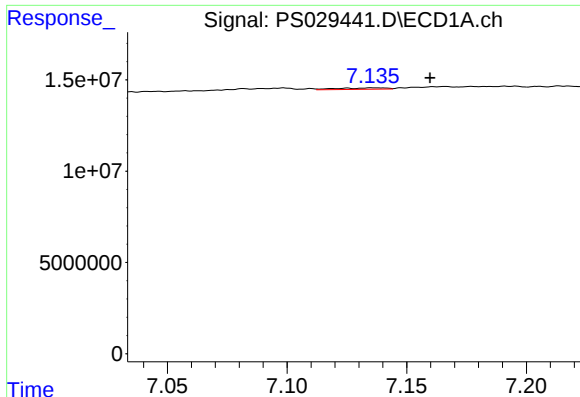

#4 2,4-DCAA


R.T.: 7.137 min
Delta R.T.: -0.023 min
Response: 1144342
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

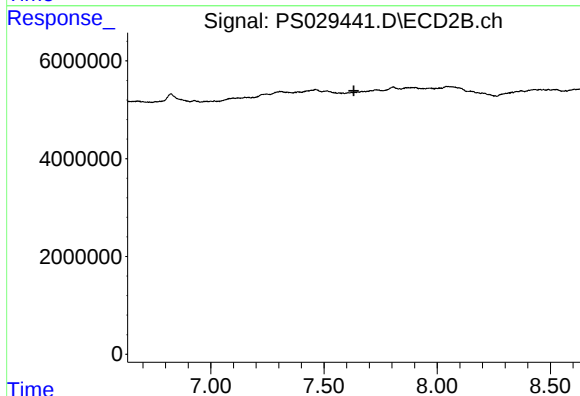


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.632 min
Response: 0
Conc: N.D.

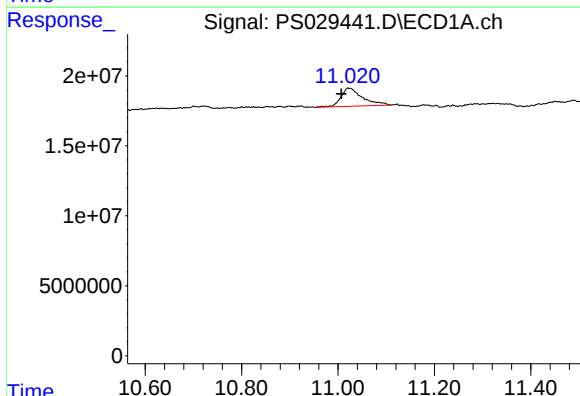


#15 Picloram

R.T.: 11.023 min
Delta R.T.: 0.016 min
Response: 40653119
Conc: 1.33 ng/ml

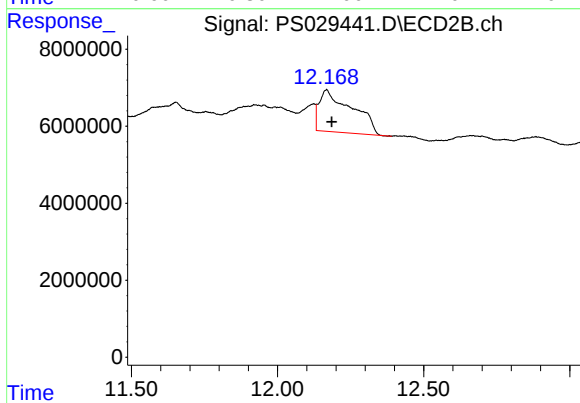

#15 Picloram


R.T.: 12.168 min
Delta R.T.: -0.017 min
Response: 85087418
Conc: 7.36 ng/ml

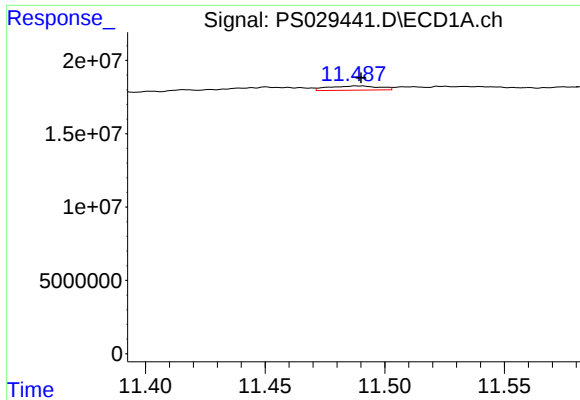

#16 DCPA

R.T.: 11.489 min
Delta R.T.: -0.001 min
Response: 4267017
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

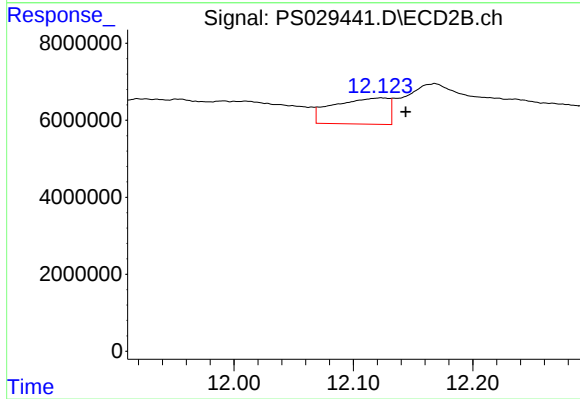

#16 DCPA

R.T.: 12.123 min
Delta R.T.: -0.021 min
Response: 21781795
Conc: 1.84 ng/ml