

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031725\
 Data File : PS029442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2025 10:32
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:42:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	7.614	1972.0E6	426.0E6	478.581	453.013
Target Compounds							
1) T	Dalapon	0.000	2.670	0	12771664	N.D.	6.033
2) T	3,5-DICHL...	6.349	0.000	2538838	0	<MDL	N.D. #
3) T	4-Nitroph...	6.957	0.000	9909492	0	4.234	N.D. #
7) T	MCPA	7.683	0.000	939884	0	<MDL	N.D. #
8) T	DICHLORPROP	8.031	0.000	30658089	0	6.670	N.D. #
9) T	2,4-D	8.279	0.000	4001240	0	<MDL	N.D. #
10) T	Pentachlo...	8.560	0.000	6681239	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.105f	0.000	8839047	0	<MDL	N.D. #
12) T	2,4,5-T	9.453	0.000	16919860	0	<MDL	N.D. #
13) T	2,4-DB	10.008	0.000	1687497	0	<MDL	N.D. #
14) T	DINOSEB	11.190	0.000	326616	0	<MDL	N.D. #
15) T	Picloram	11.001	12.191	613619	4776833	<MDL	<MDL #
16) T	DCPA	11.481	12.191f	10294996	4776833	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031725\
Data File : PS029442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2025 10:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:42:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

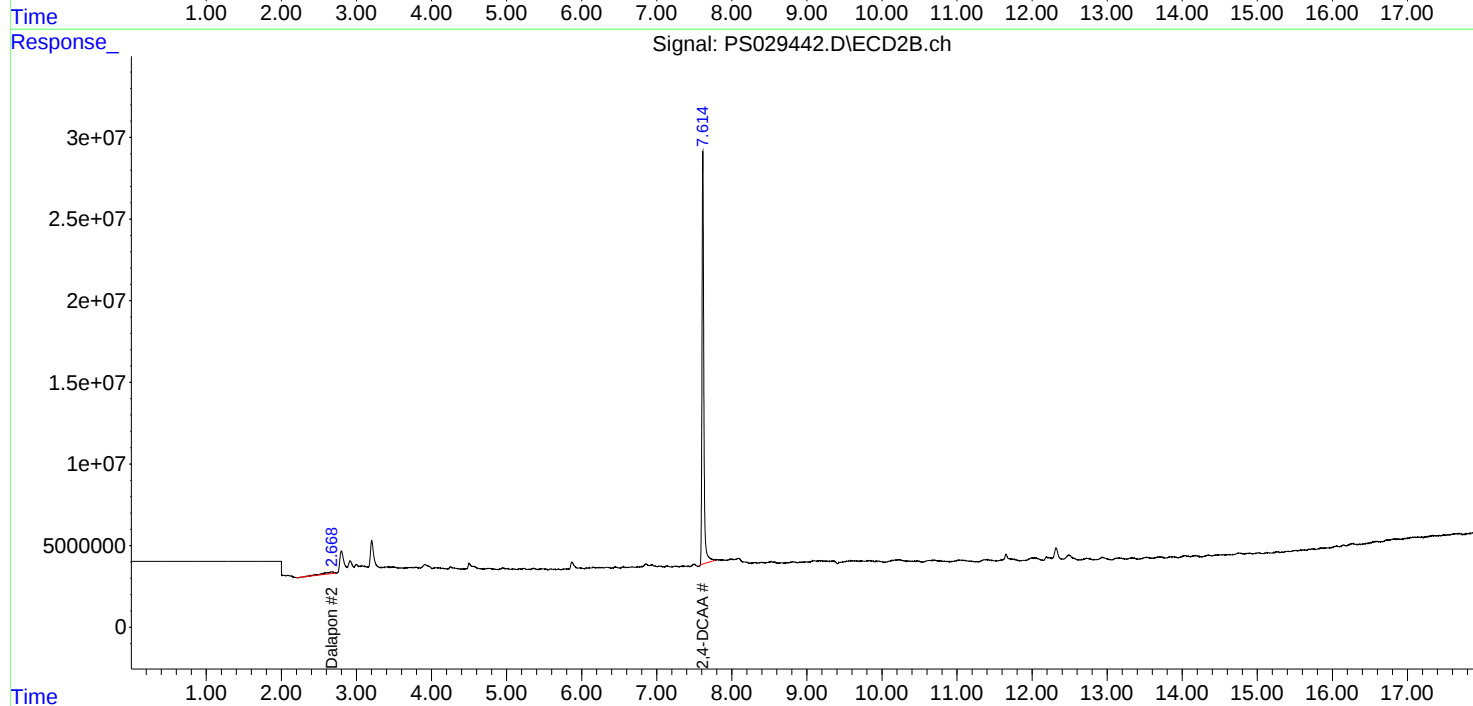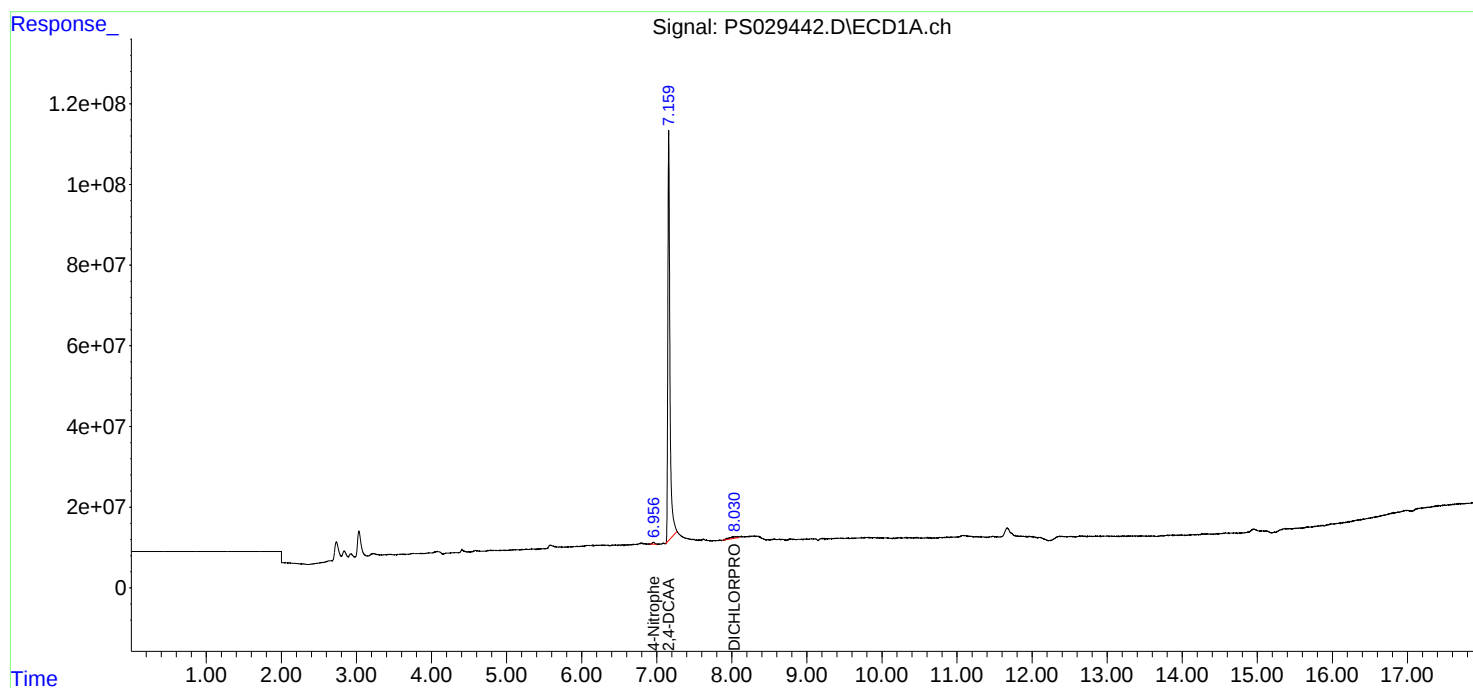


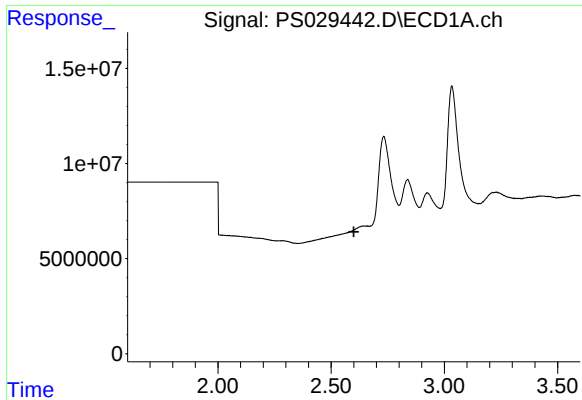

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.600 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

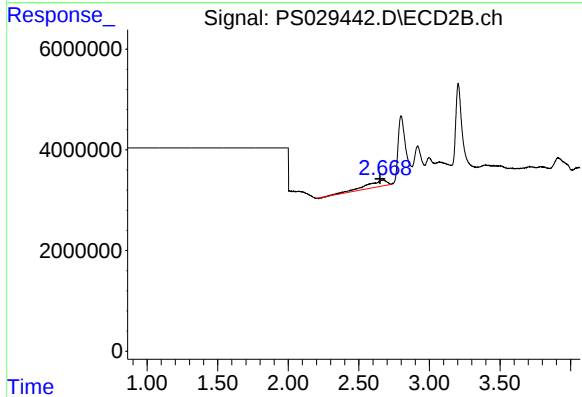


#1 Dalapon

R.T.: 2.670 min
Delta R.T.: 0.019 min
Response: 12771664
Conc: 6.03 ng/ml

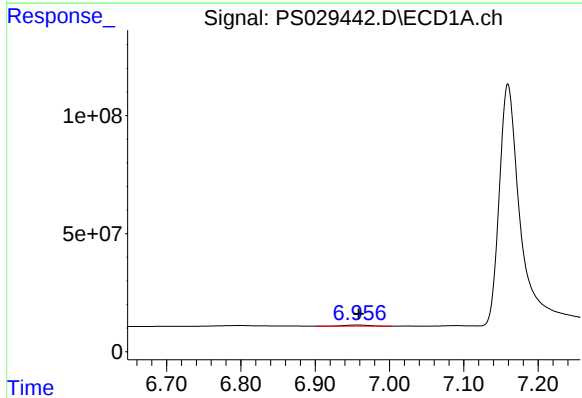


#3 4-Nitrophenol

R.T.: 6.957 min
Delta R.T.: -0.002 min
Response: 9909492
Conc: 4.23 ng/ml

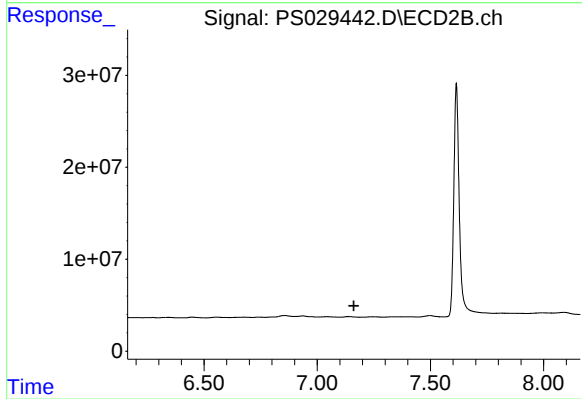

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.162 min
Response: 0
Conc: N.D.

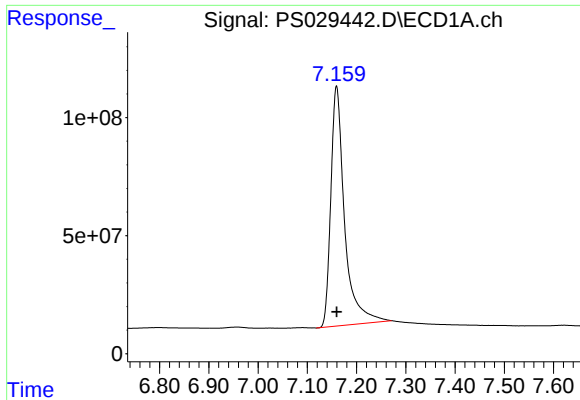

#4 2,4-DCAA


R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 1972029030
Conc: 478.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

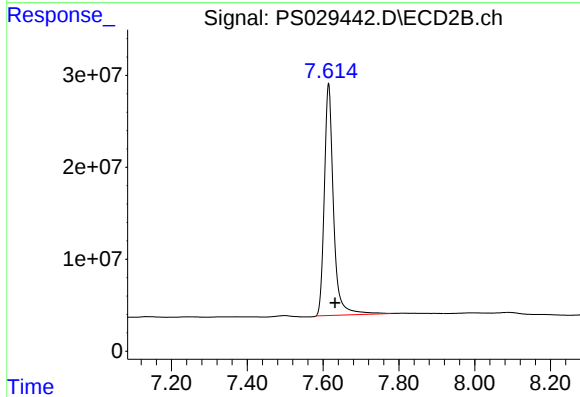


#4 2,4-DCAA

R.T.: 7.614 min
Delta R.T.: -0.017 min
Response: 425982723
Conc: 453.01 ng/ml

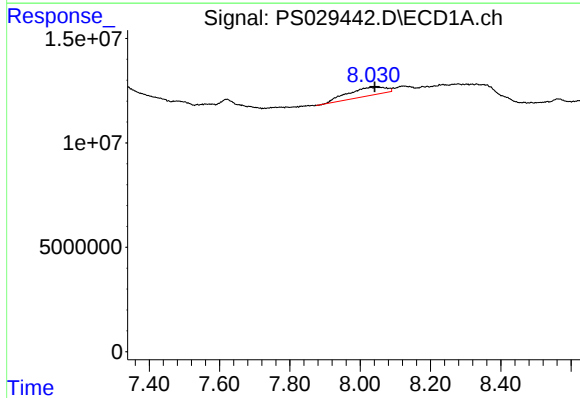

#8 DICHLORPROP

R.T.: 8.031 min
Delta R.T.: -0.011 min
Response: 30658089
Conc: 6.67 ng/ml

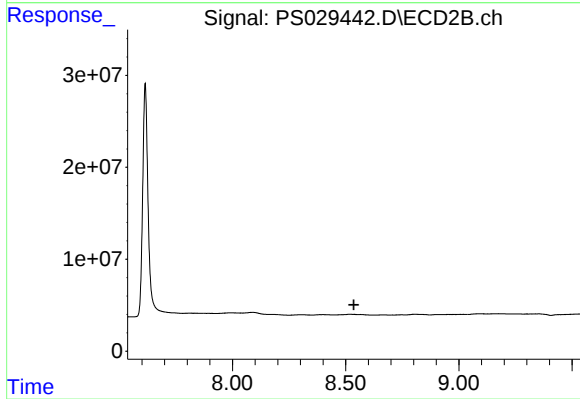

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.536 min
Response: 0
Conc: N.D.