

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
 Data File : PS003568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2019 09:45
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:34:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.803	0	2463295	N.D.	5.246 #
Target Compounds							
2) T	3,5-DICHL...	0.000	8.946	0	127911	N.D.	0.207 #
5) T	DICAMBA	0.000	11.037	0	1342711	N.D.	0.804 #
6) T	MCP	0.000	11.312	0	41003	N.D.	0.035 #
8) T	DICHLORPROP	0.000	12.208	0	216770	N.D.	0.525 #
9) T	2,4-D	0.000	12.702	0	85011	N.D.	0.162 #
10) T	Pentachlo...	0.000	13.184	0	473407	N.D.	0.072 #
11) T	2,4,5-TP ...	0.000	13.758	0	895168	N.D.	0.352 #
12) T	2,4,5-T	0.000	14.392	0	320917	N.D.	0.159 #
13) T	2,4-DB	0.000	15.012	0	167299	N.D.	0.655 #
14) T	DINOSEB	0.000	15.485	0	158559	N.D.	0.089 #
15) T	Picloram	0.000	16.690	0	715478	N.D.	0.282 #
16) T	DCPA	0.000	16.616	0	1342866	N.D.	0.432 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
Data File : PS003568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2019 09:45
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:34:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

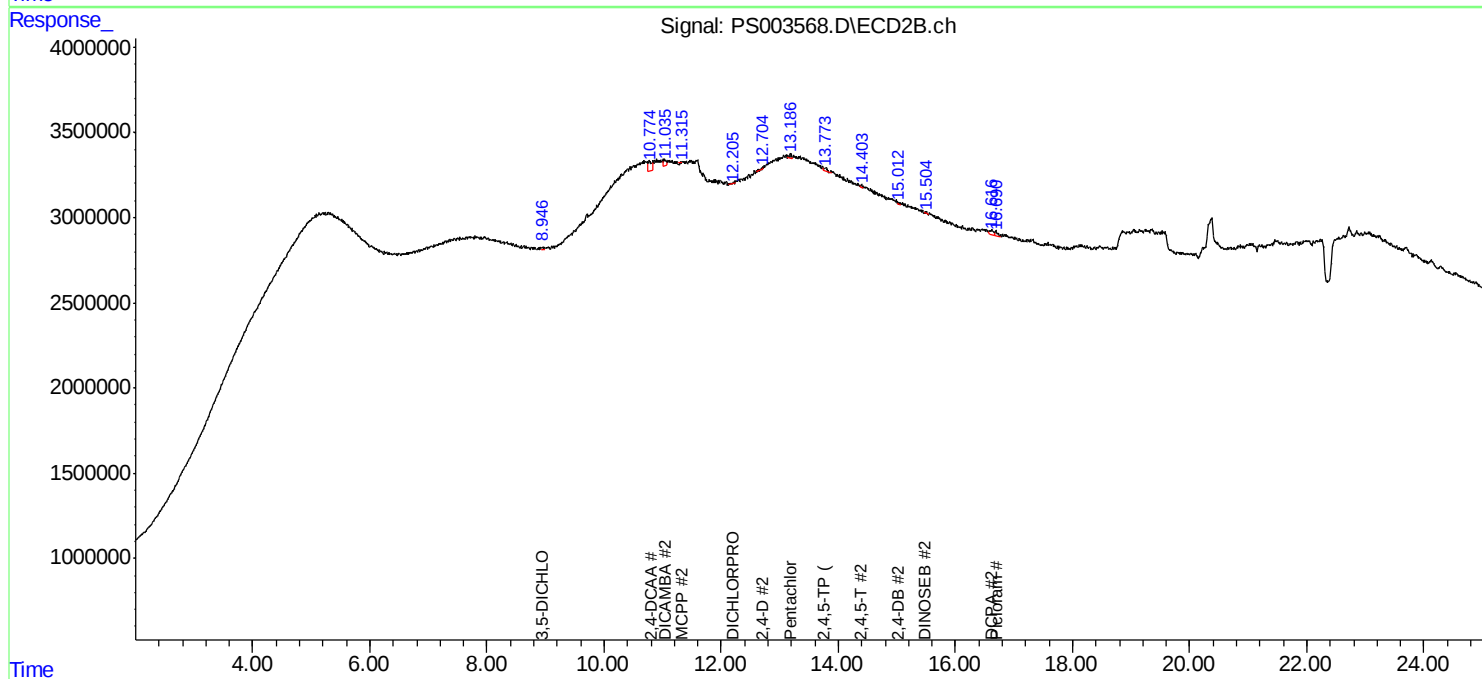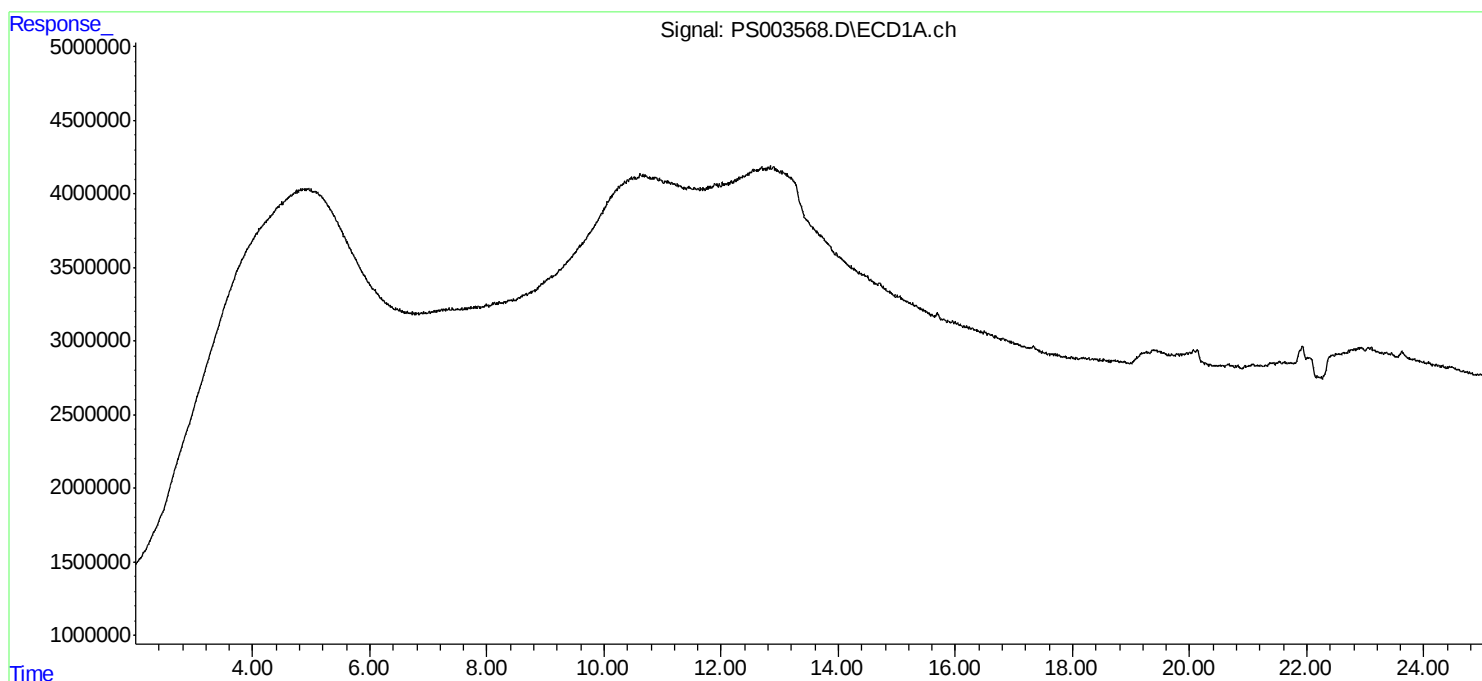


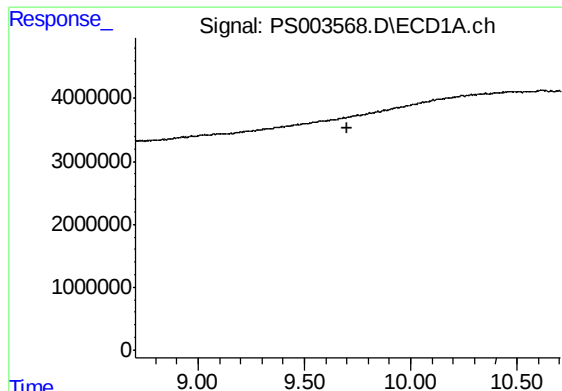

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

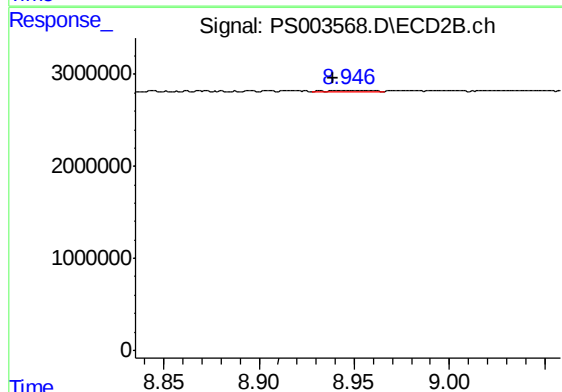


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.946 min
Delta R.T.: 0.007 min
Response: 127911
Conc: 0.21 ng/ml

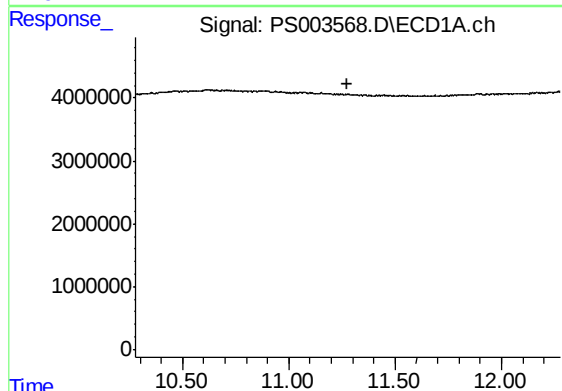


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.278 min
Response: 0
Conc: N.D.

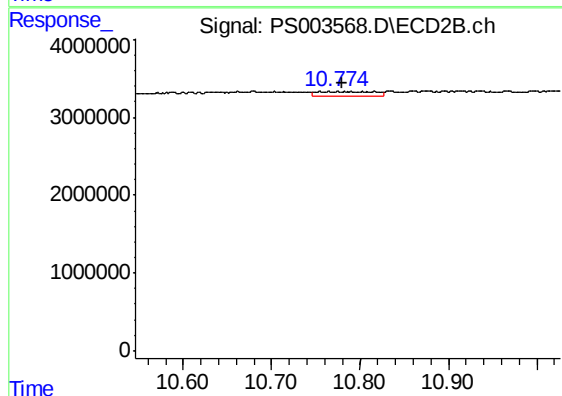

#4 2,4-DCAA


R.T.: 10.803 min
Delta R.T.: 0.023 min
Response: 2463295
Conc: 5.25 ng/ml

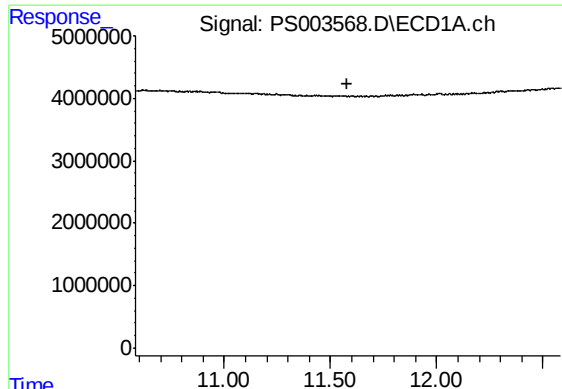

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

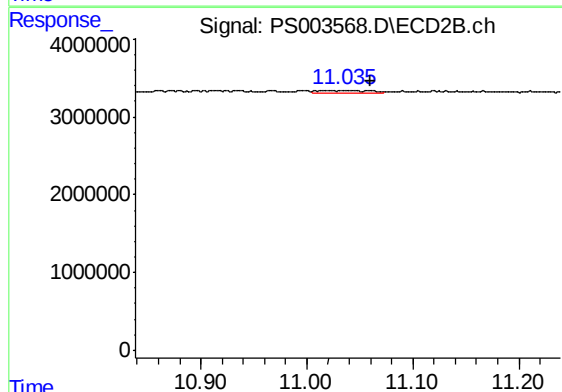


#5 DICAMBA

R.T.: 11.037 min
Delta R.T.: -0.023 min
Response: 1342711
Conc: 0.80 ng/ml

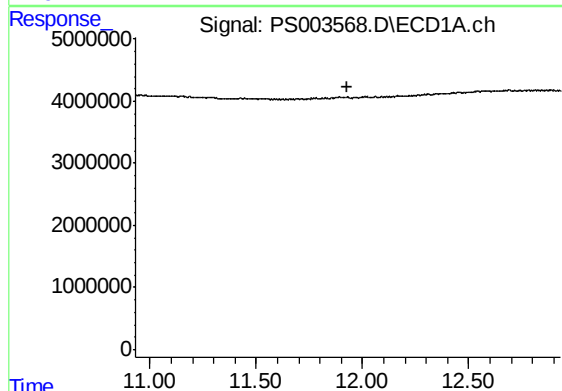


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.931 min
Response: 0
Conc: N.D.

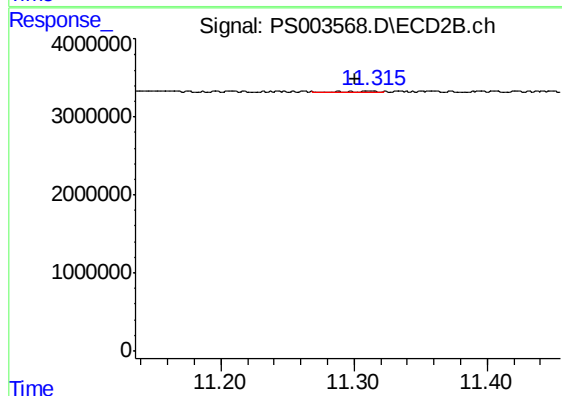

#6 MCPP


R.T.: 11.312 min
Delta R.T.: 0.012 min
Response: 41003
Conc: 0.03 ug/ml

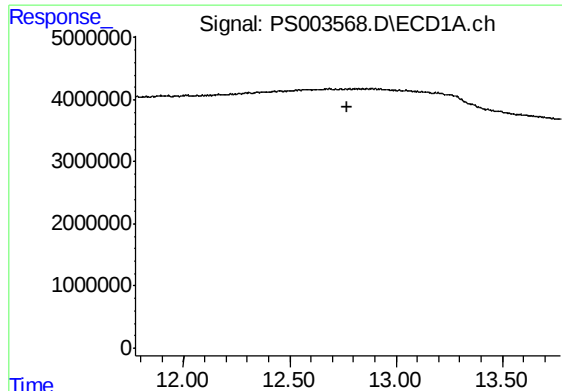

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

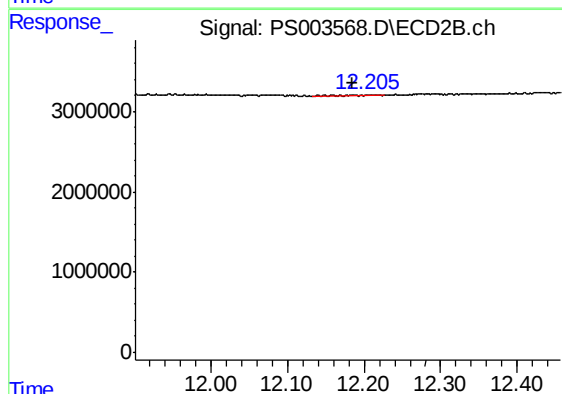


#8 DICHLORPROP

R.T.: 12.208 min
Delta R.T.: 0.023 min
Response: 216770
Conc: 0.52 ng/ml

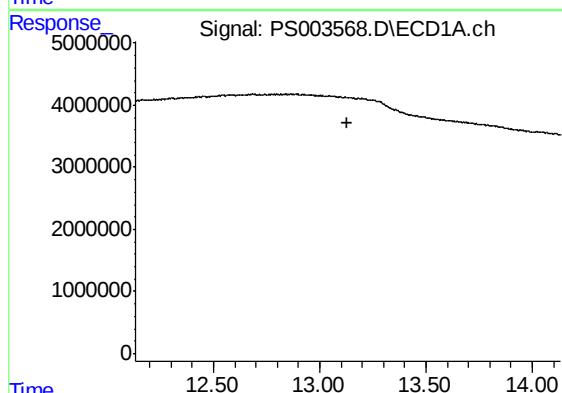


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

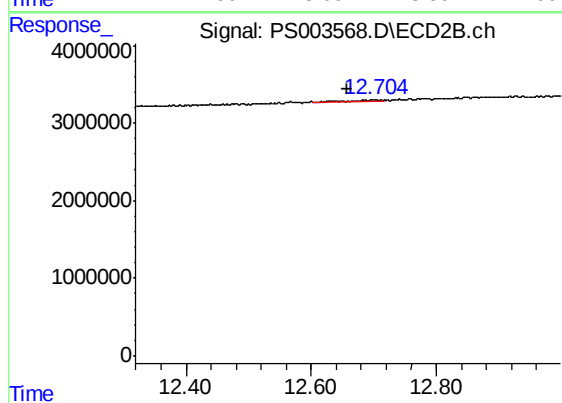

#9 2,4-D


R.T.: 12.702 min
Delta R.T.: 0.045 min
Response: 85011
Conc: 0.16 ng/ml

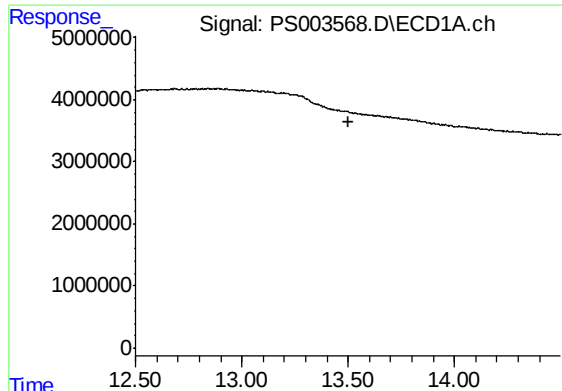

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

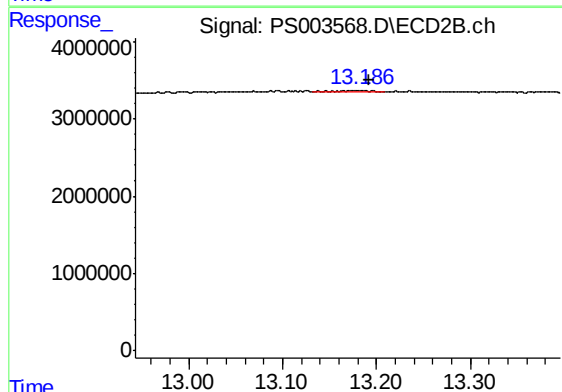


#10 Pentachlorophenol

R.T.: 13.184 min
Delta R.T.: -0.007 min
Response: 473407
Conc: 0.07 ng/ml

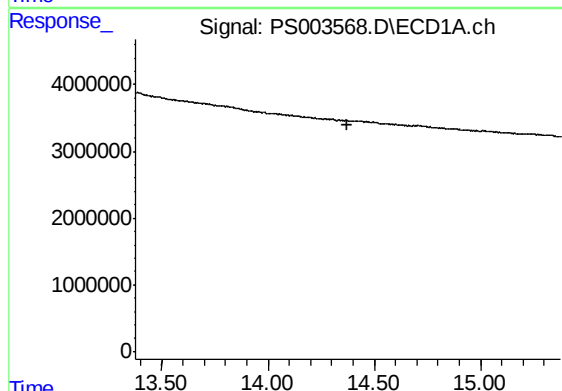


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

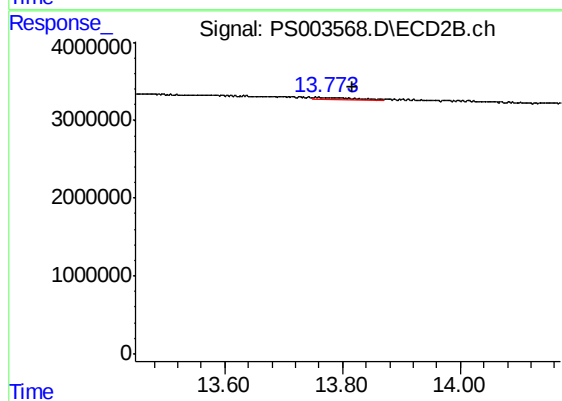

#11 2,4,5-TP (SILVEX)


R.T.: 13.758 min
Delta R.T.: -0.060 min
Response: 895168
Conc: 0.35 ng/ml

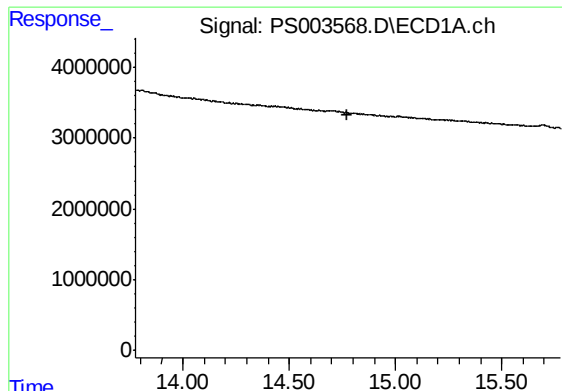

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

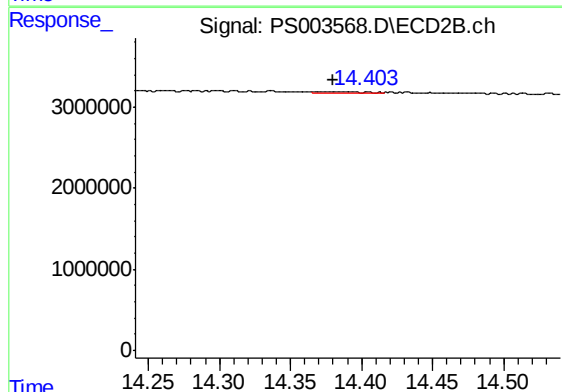


#12 2,4,5-T

R.T.: 14.392 min
Delta R.T.: 0.012 min
Response: 320917
Conc: 0.16 ng/ml

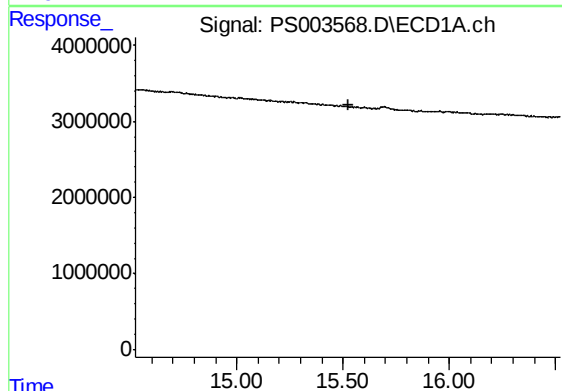


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.523 min
Response: 0
Conc: N.D.

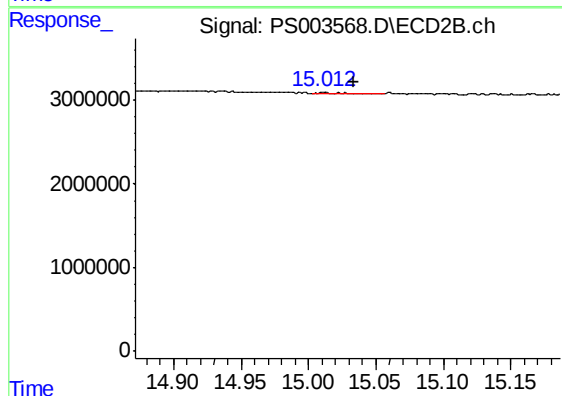

#13 2,4-DB


R.T.: 15.012 min
Delta R.T.: -0.022 min
Response: 167299
Conc: 0.66 ng/ml

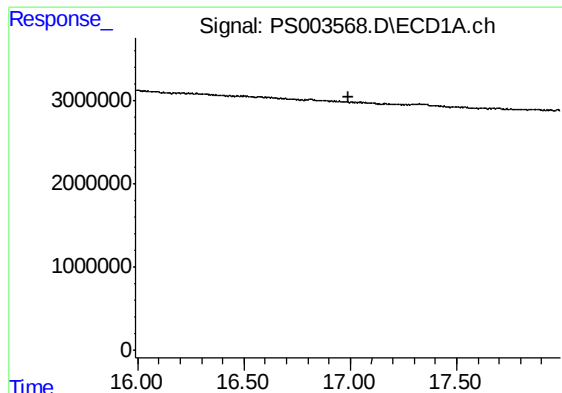

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

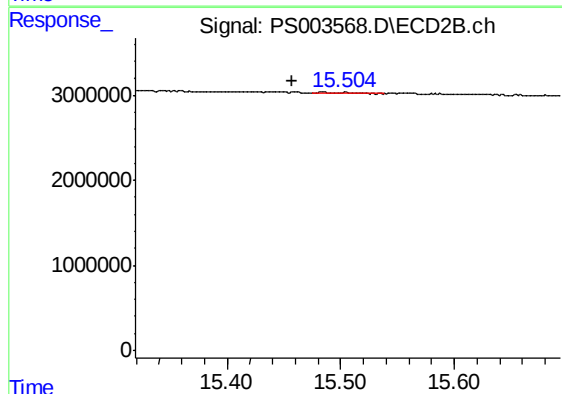


#14 DINOSEB

R.T.: 15.485 min
Delta R.T.: 0.028 min
Response: 158559
Conc: 0.09 ng/ml

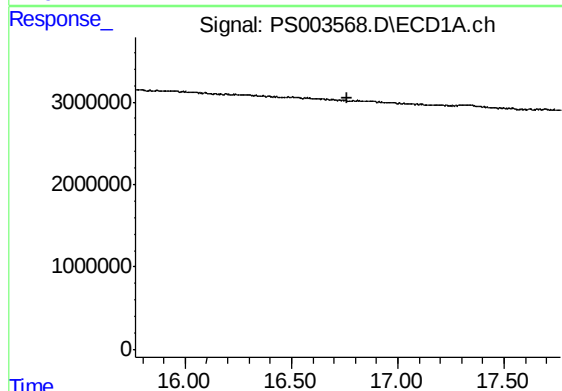


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

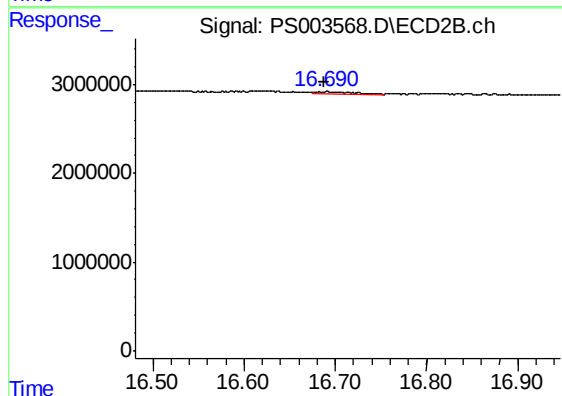

#15 Picloram


R.T.: 16.690 min
Delta R.T.: 0.001 min
Response: 715478
Conc: 0.28 ng/ml

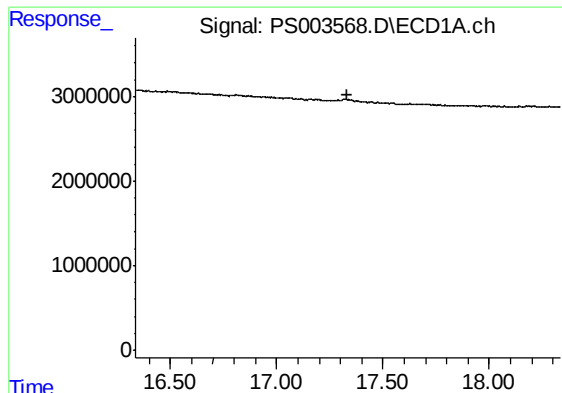

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

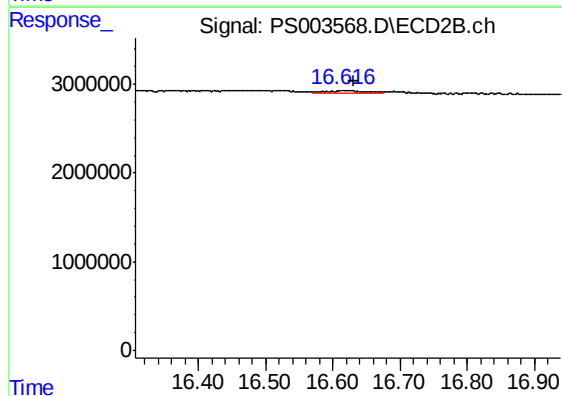

#16 DCPA

R.T.: 16.616 min
Delta R.T.: -0.016 min
Response: 1342866
Conc: 0.43 ng/ml