

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
 Data File : PS003575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2019 13:42
 Operator : EI\SJ
 Sample : K1685-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-05-031419-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:36:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.270	10.773	238.4E6	237.3E6	542.992	505.375
Target Compounds							
1) T	Dalapon	2.790	2.280	33880946	71512637	52.129	112.941 #
2) T	3,5-DICHL...	0.000	8.939	0	8236264	N.D.	13.339 #
3) T	4-Nitroph...	0.000	9.944	0	2582047	N.D.	11.485 #
5) T	DICAMBA	0.000	11.014	0	6157461	N.D.	3.686 #
6) T	MCPD	11.970	0.000	6229876	0	4.745	N.D. #
7) T	MCPA	12.165	11.685	14231186	-650862	7.175	N.D. #
9) T	2,4-D	0.000	12.634	0	1551262	N.D.	2.955 #
11) T	2,4,5-TP ...	0.000	13.845	0	308728	N.D.	0.121 #
12) T	2,4,5-T	0.000	14.437	0	15324505	N.D.	7.599 #
13) T	2,4-DB	0.000	15.001	0	3304946	N.D.	12.942 #
14) T	DINOSEB	0.000	15.438	0	1873317	N.D.	1.050 #
15) T	Picloram	16.762	16.715	7890526	11305690	3.206	4.454 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
Data File : PS003575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2019 13:42
Operator : EI\SJ
Sample : K1685-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:36:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

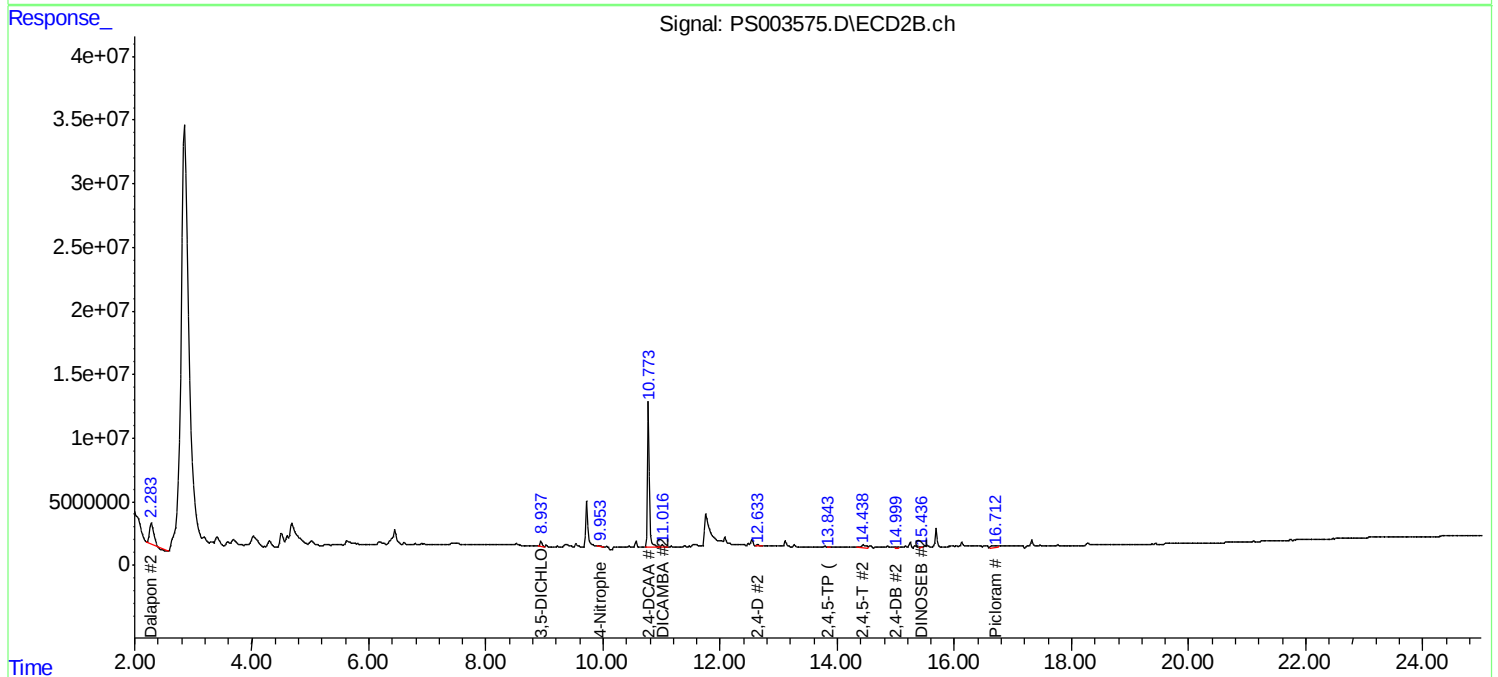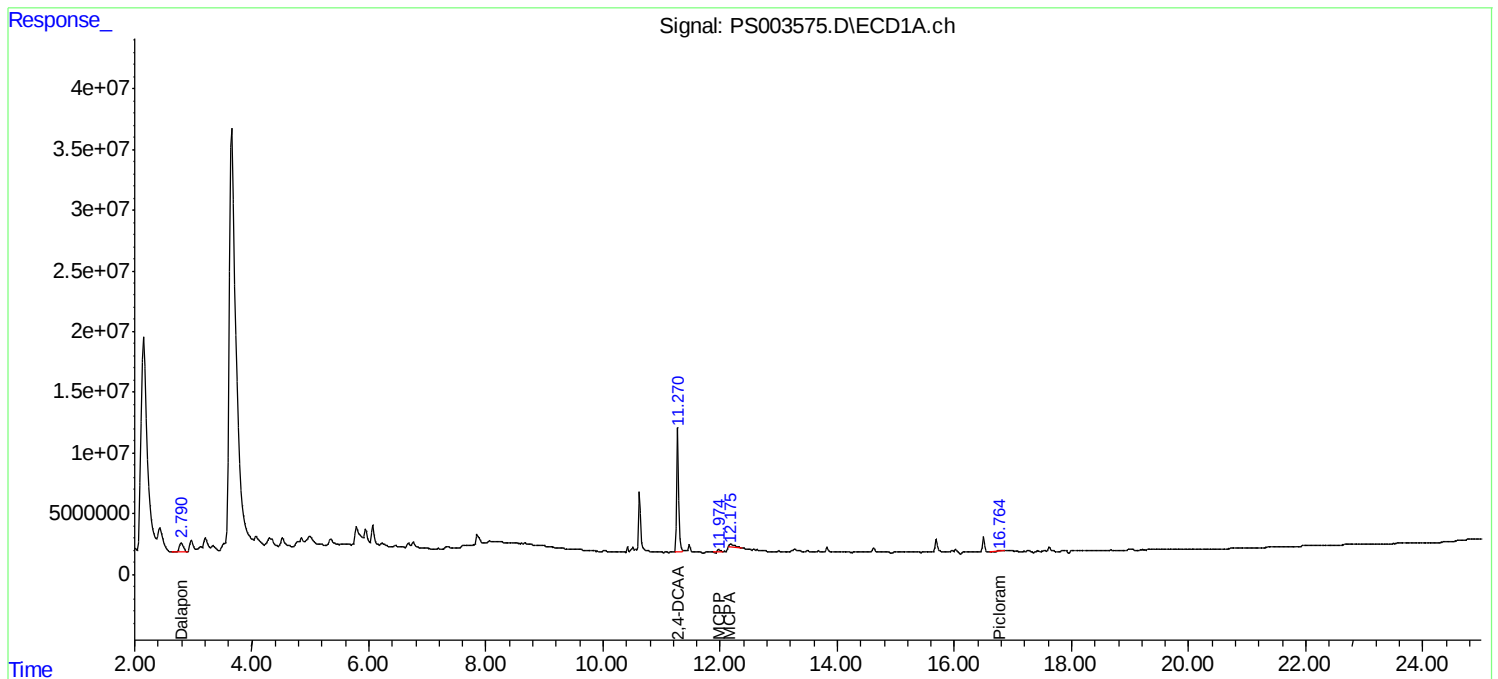


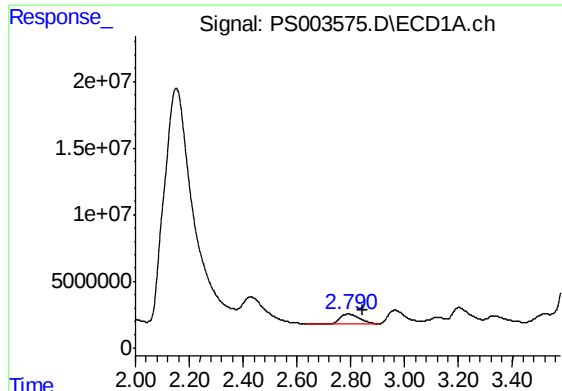

#1 Dalapon


R.T.: 2.790 min
Delta R.T.: -0.054 min
Response: 33880946
Conc: 52.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-B

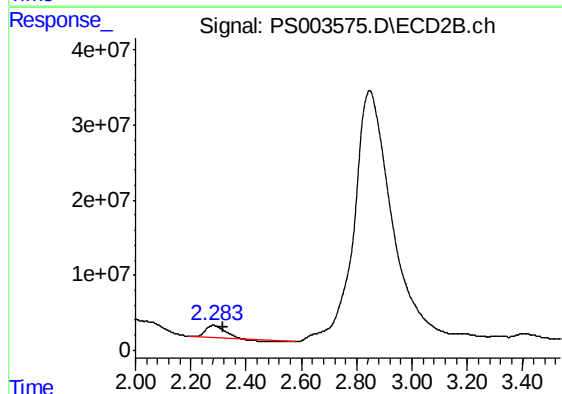


#1 Dalapon

R.T.: 2.280 min
Delta R.T.: -0.037 min
Response: 71512637
Conc: 112.94 ng/ml

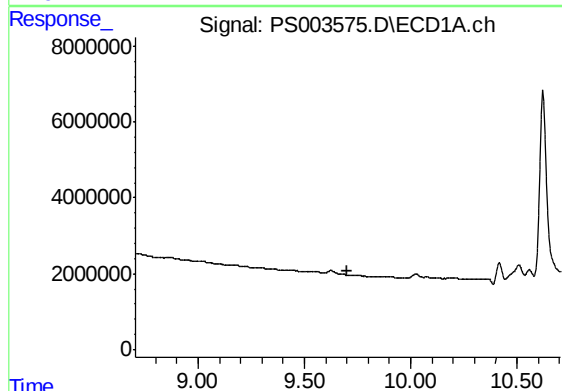


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

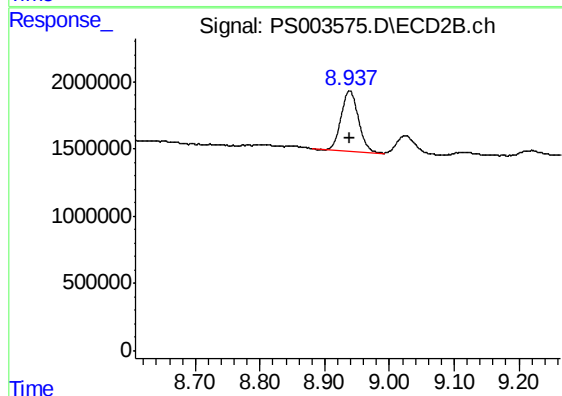

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.939 min
Delta R.T.: 0.000 min
Response: 8236264
Conc: 13.34 ng/ml

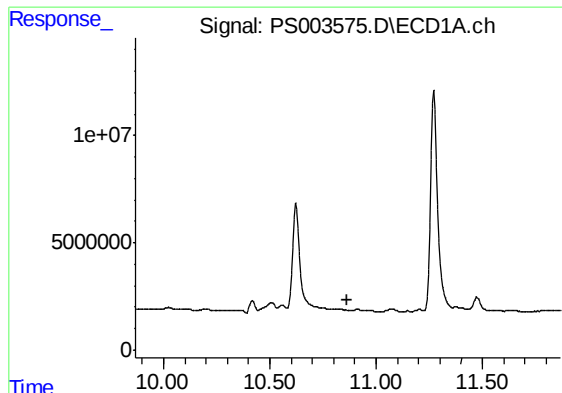

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-B

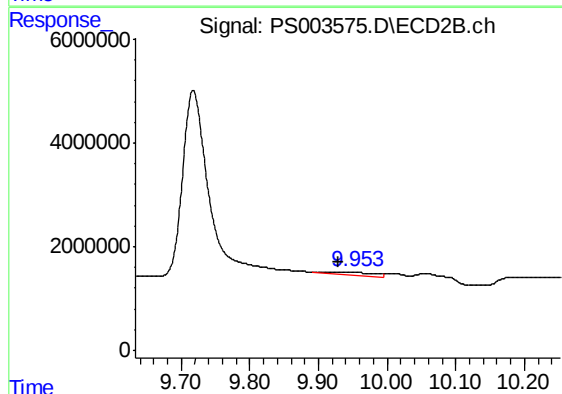


#3 4-Nitrophenol

R.T.: 9.944 min
Delta R.T.: 0.015 min
Response: 2582047
Conc: 11.48 ng/ml

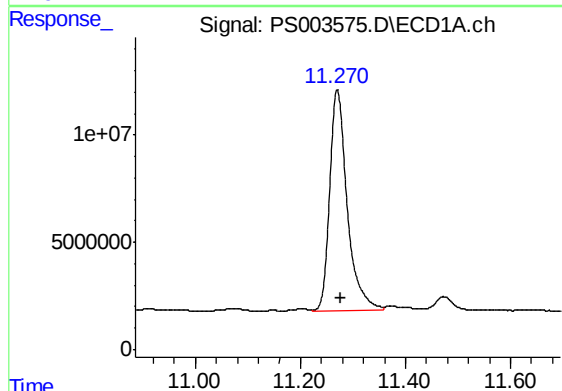


#4 2,4-DCAA

R.T.: 11.270 min
Delta R.T.: -0.007 min
Response: 238386974
Conc: 542.99 ng/ml

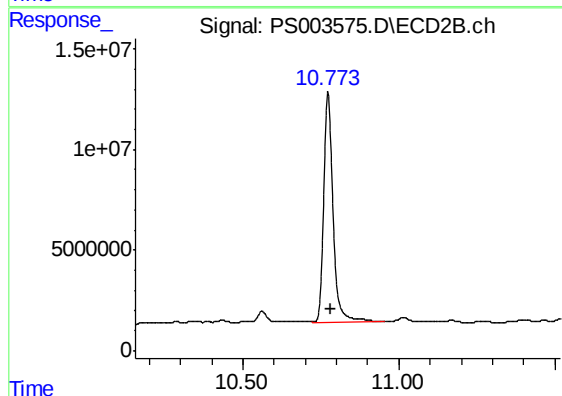

#4 2,4-DCAA


R.T.: 10.773 min
Delta R.T.: -0.007 min
Response: 237308325
Conc: 505.37 ng/ml

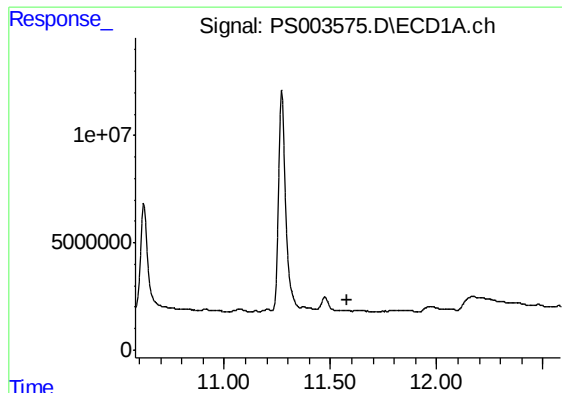

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-B

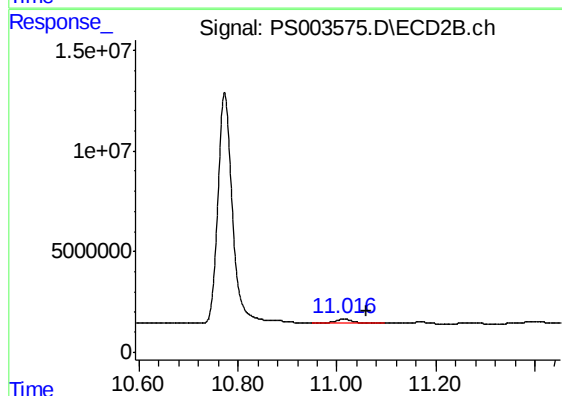


#5 DICAMBA

R.T.: 11.014 min
Delta R.T.: -0.045 min
Response: 6157461
Conc: 3.69 ng/ml

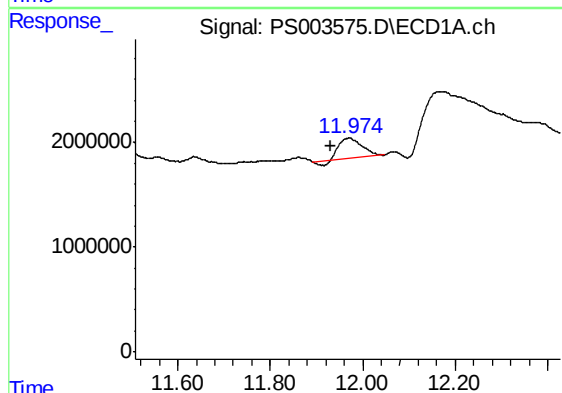


#6 MCPP

R.T.: 11.970 min
Delta R.T.: 0.039 min
Response: 6229876
Conc: 4.75 ug/ml

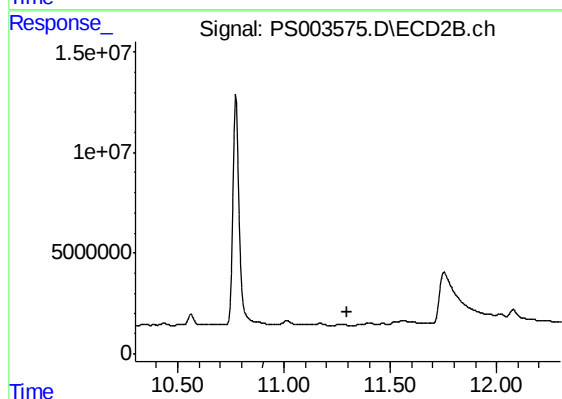

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.300 min
Response: 0
Conc: N.D.

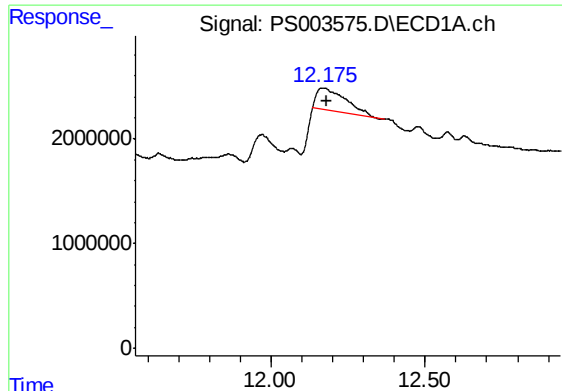

#7 MCPA


R.T.: 12.165 min
Delta R.T.: -0.017 min
Response: 14231186
Conc: 7.17 ug/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-B

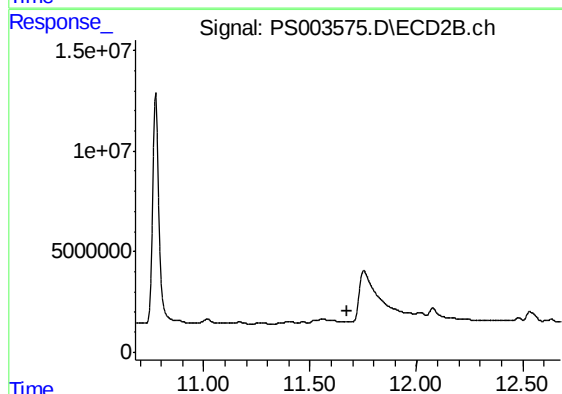


#7 MCPA

R.T.: 11.685 min
Delta R.T.: 0.007 min
Response: -650862
Conc: N.D.

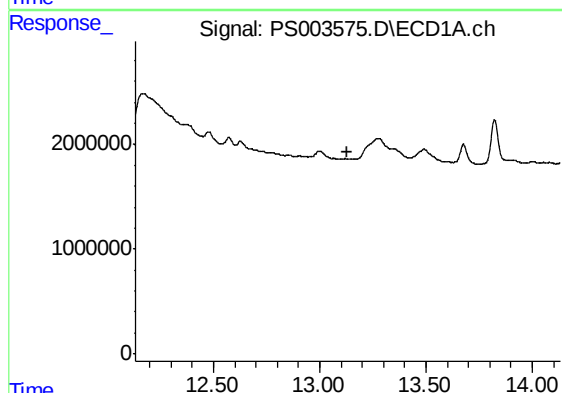


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

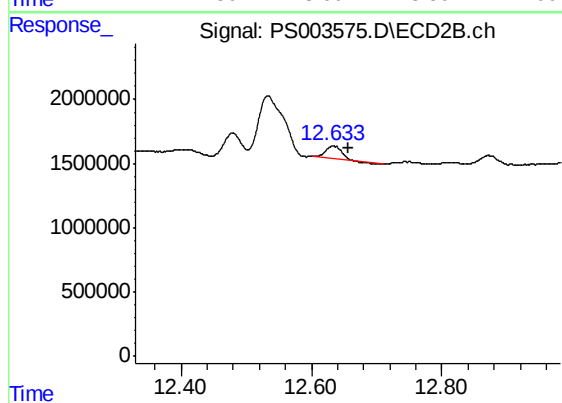

#9 2,4-D


R.T.: 12.634 min
Delta R.T.: -0.023 min
Response: 1551262
Conc: 2.96 ng/ml

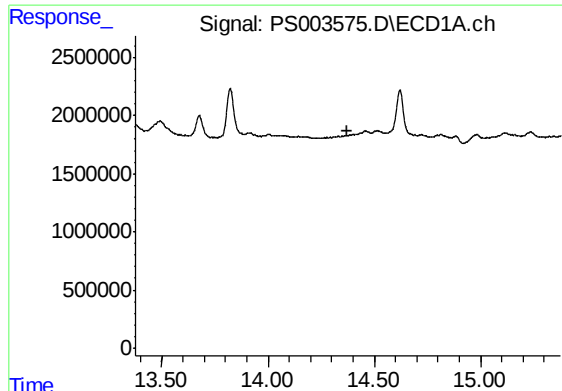

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-B

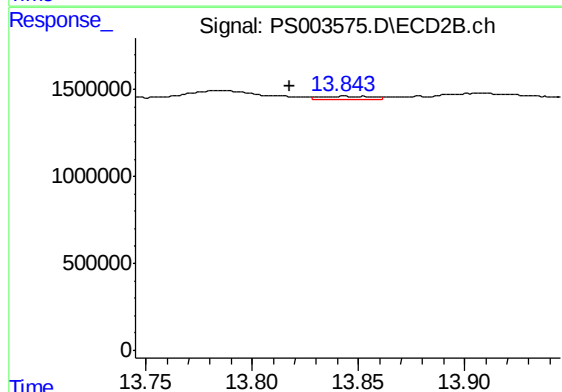


#11 2,4,5-TP (SILVEX)

R.T.: 13.845 min
Delta R.T.: 0.027 min
Response: 308728
Conc: 0.12 ng/ml

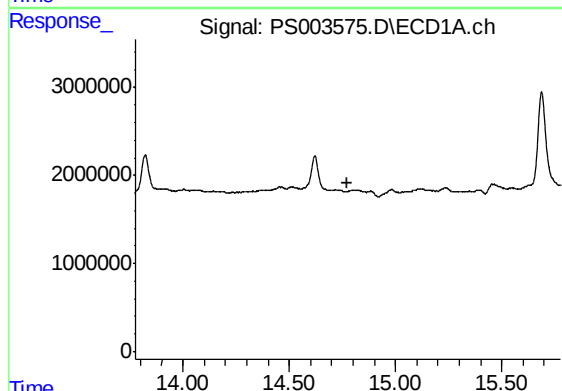


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

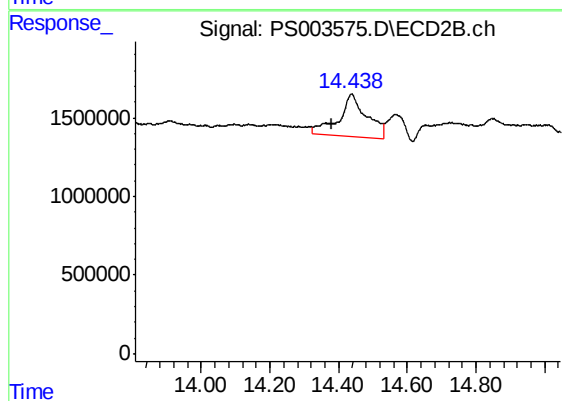

#12 2,4,5-T


R.T.: 14.437 min
Delta R.T.: 0.057 min
Response: 15324505
Conc: 7.60 ng/ml

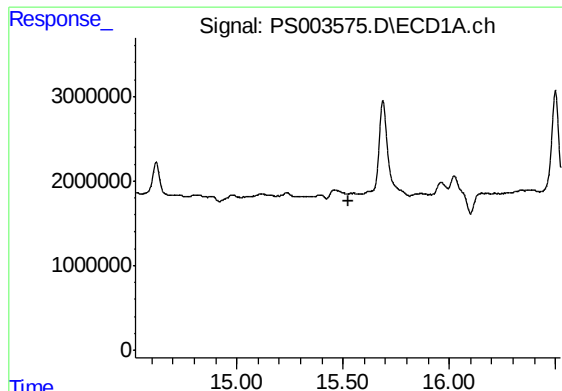

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-B

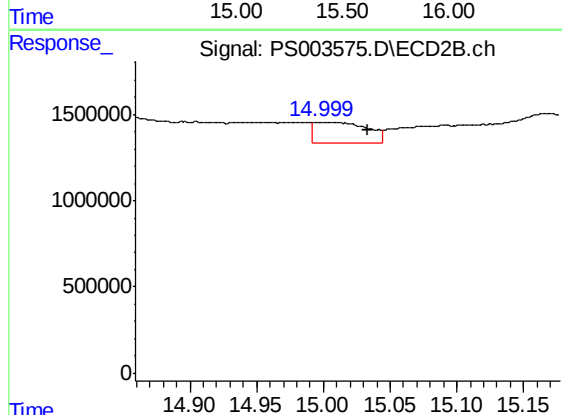


#13 2,4-DB

R.T.: 15.001 min
Delta R.T.: -0.032 min
Response: 3304946
Conc: 12.94 ng/ml

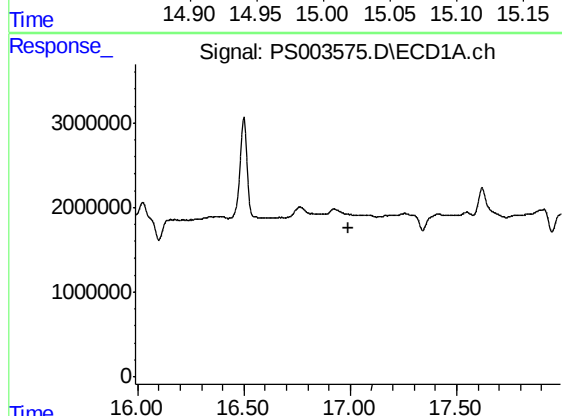


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

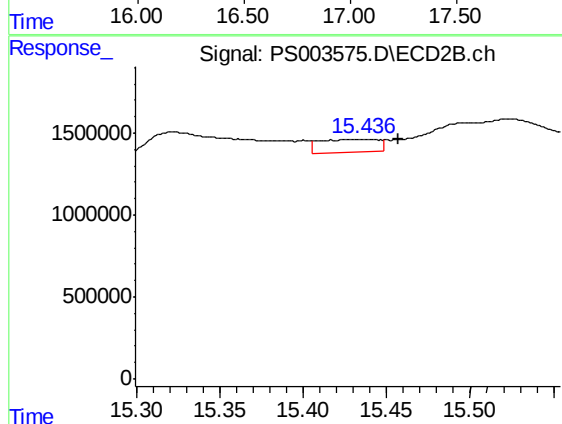

#14 DINOSEB


R.T.: 15.438 min
Delta R.T.: -0.019 min
Response: 1873317
Conc: 1.05 ng/ml

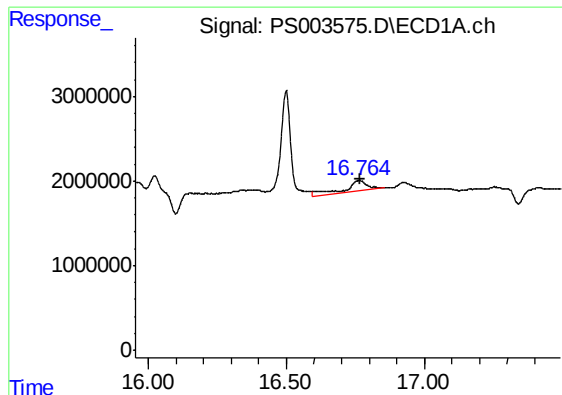

#15 Picloram

R.T.: 16.762 min
Delta R.T.: -0.003 min
Response: 7890526
Conc: 3.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-B

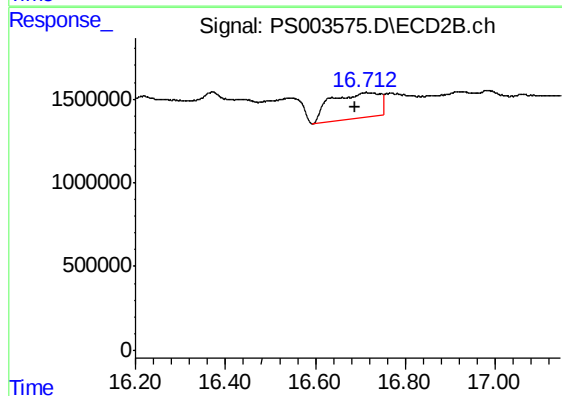

#15 Picloram

R.T.: 16.715 min
Delta R.T.: 0.026 min
Response: 11305690
Conc: 4.45 ng/ml