

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
 Data File : PS003576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2019 14:13
 Operator : EI\SJ
 Sample : K1685-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-05-031419-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 16:37:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.289	10.791	287.0E6	285.5E6	653.694	608.015
Target Compounds							
1) T	Dalapon	2.807	2.297	35925630	73003026	55.275	115.295 #
2) T	3,5-DICHL...	0.000	8.956	0	1058626	N.D.	1.714 #
3) T	4-Nitroph...	0.000	9.966	0	3122796	N.D.	13.890 #
5) T	DICAMBA	0.000	11.033	0	5392873	N.D.	3.228 #
6) T	MCPD	11.972	11.287	251911	1270621	0.192	1.076 #
7) T	MCPA	12.246	11.645	4961266	6951395	2.501	4.030 #
9) T	2,4-D	0.000	12.652	0	1714370	N.D.	3.266 #
11) T	2,4,5-TP ...	0.000	13.803	0	1240749	N.D.	0.487 #
12) T	2,4,5-T	0.000	14.392	0	6719231	N.D.	3.332 #
13) T	2,4-DB	15.492	15.033	-3911147	8016308	N.D.	31.393
14) T	DINOSEB	0.000	15.448	0	2753876	N.D.	1.543 #
15) T	Picloram	16.792	16.660	14981268	9602771	6.087	3.783 #
16) T	DCPA	0.000	16.660	0	9602771	N.D.	3.087 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
Data File : PS003576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2019 14:13
Operator : EI\SJ
Sample : K1685-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 16:37:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

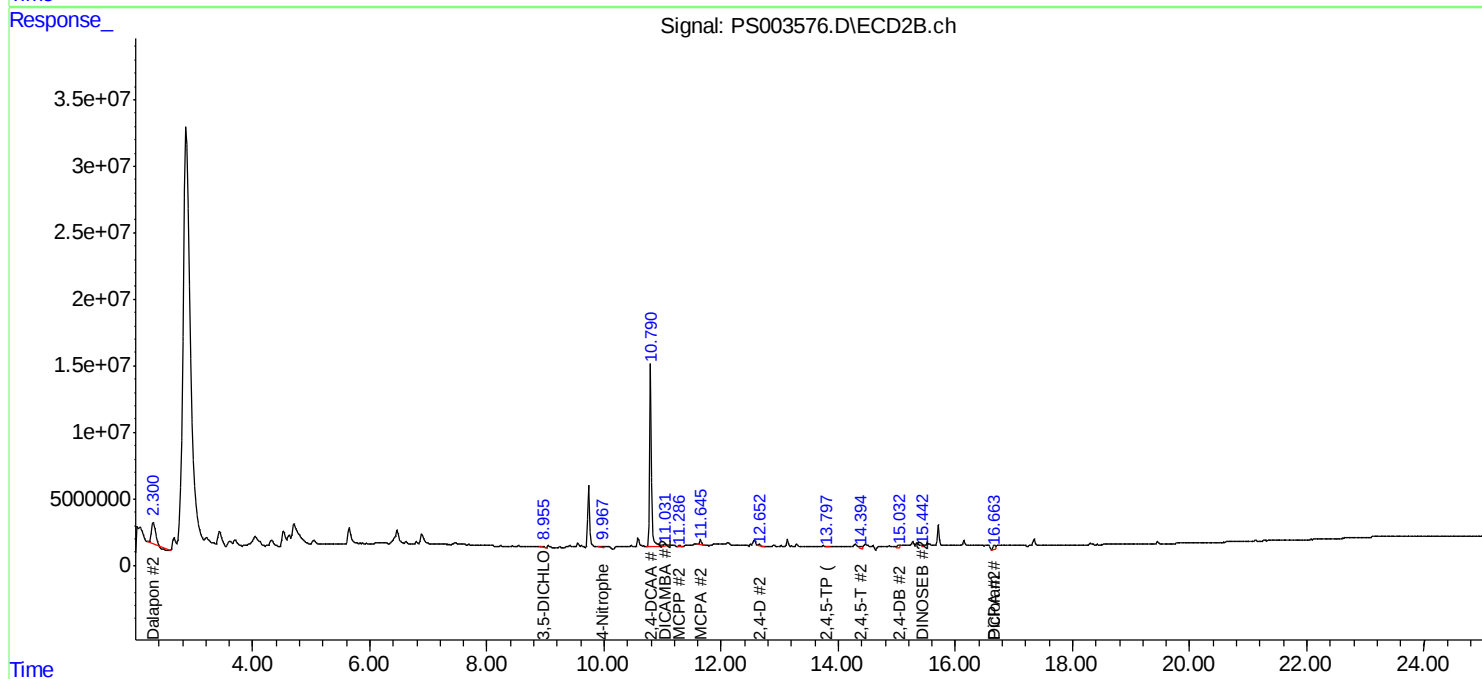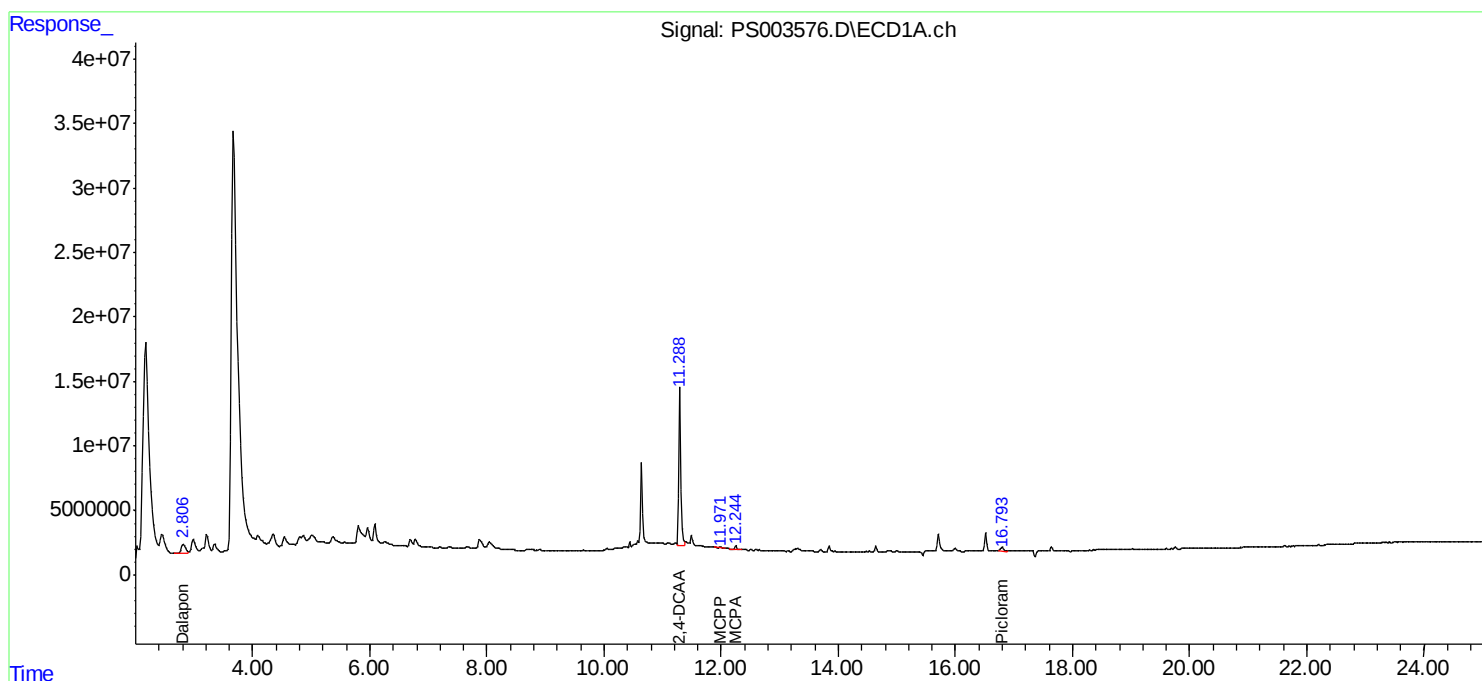


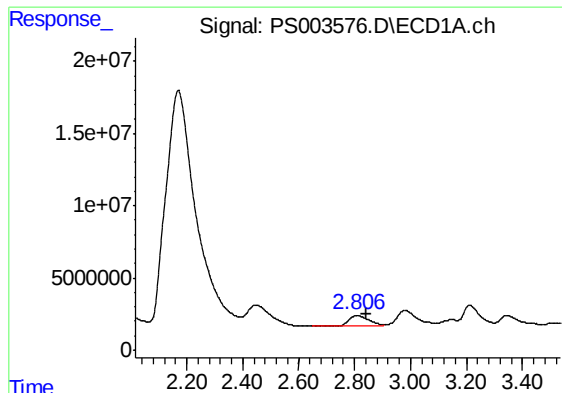

#1 Dalapon


R.T.: 2.807 min
Delta R.T.: -0.037 min
Response: 35925630
Conc: 55.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-C

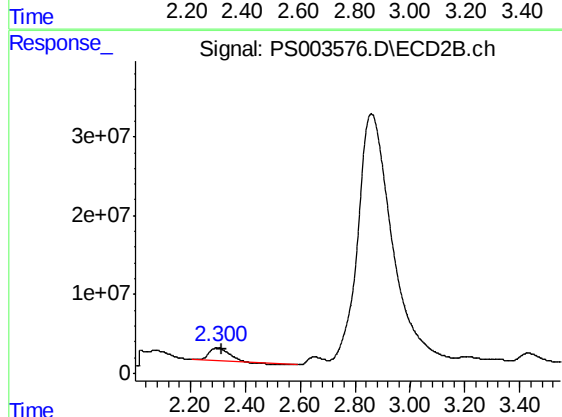


#1 Dalapon

R.T.: 2.297 min
Delta R.T.: -0.019 min
Response: 73003026
Conc: 115.29 ng/ml

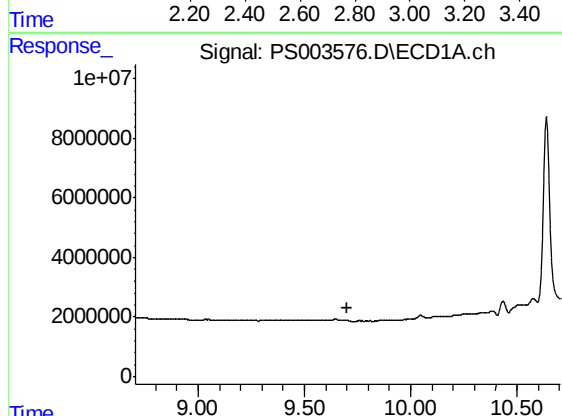


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

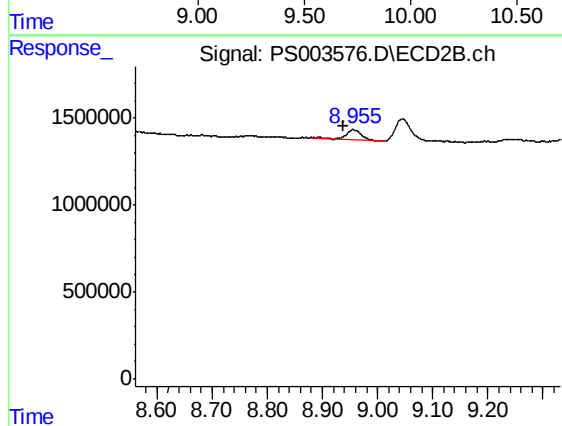

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.956 min
Delta R.T.: 0.017 min
Response: 1058626
Conc: 1.71 ng/ml

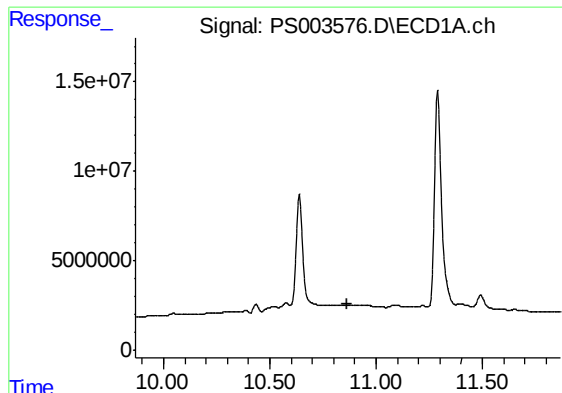

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-C

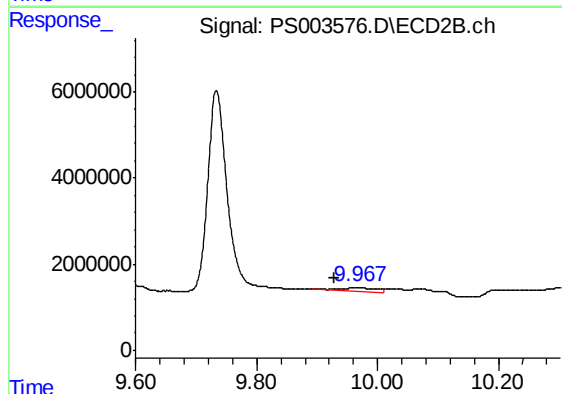


#3 4-Nitrophenol

R.T.: 9.966 min
Delta R.T.: 0.038 min
Response: 3122796
Conc: 13.89 ng/ml

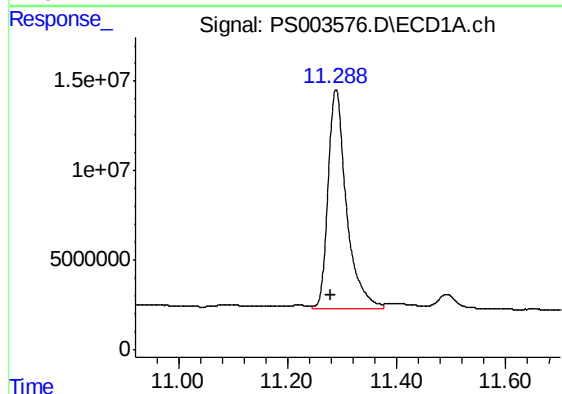


#4 2,4-DCAA

R.T.: 11.289 min
Delta R.T.: 0.011 min
Response: 286987618
Conc: 653.69 ng/ml

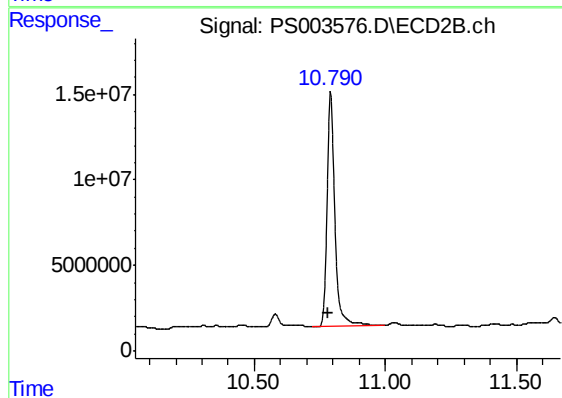

#4 2,4-DCAA


R.T.: 10.791 min
Delta R.T.: 0.011 min
Response: 285505181
Conc: 608.02 ng/ml

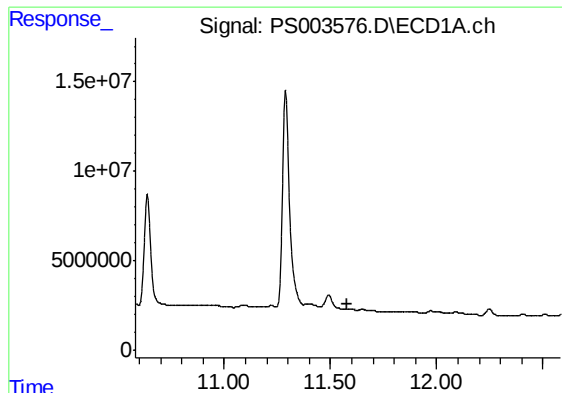

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-C

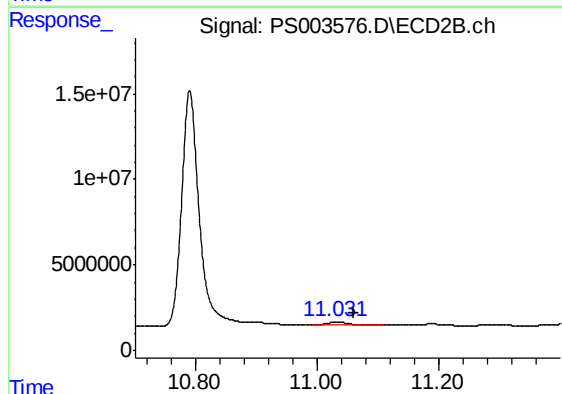


#5 DICAMBA

R.T.: 11.033 min
Delta R.T.: -0.027 min
Response: 5392873
Conc: 3.23 ng/ml

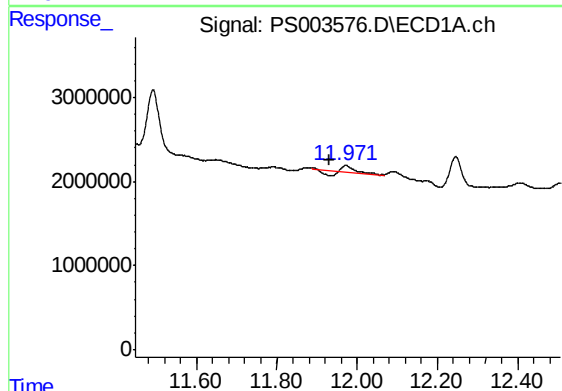


#6 MCPP

R.T.: 11.972 min
Delta R.T.: 0.041 min
Response: 251911
Conc: 0.19 ug/ml

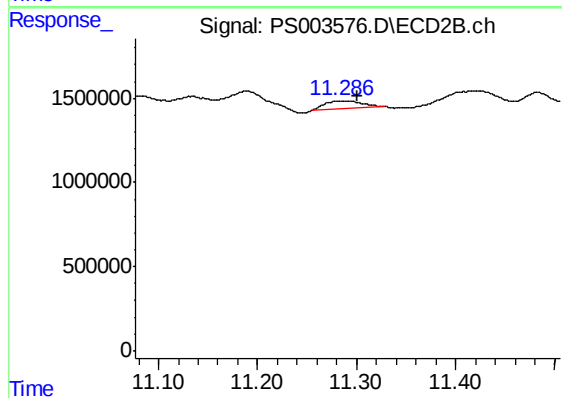

#6 MCPP


R.T.: 11.287 min
Delta R.T.: -0.014 min
Response: 1270621
Conc: 1.08 ug/ml

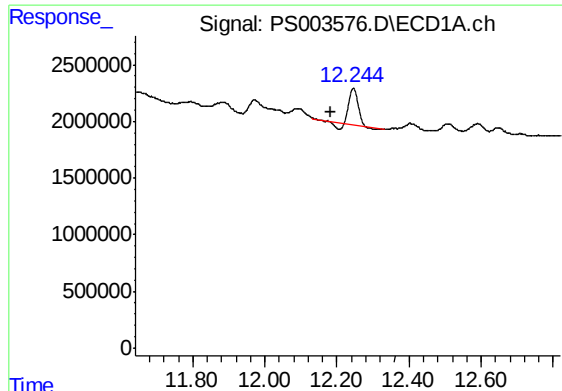

#7 MCPA


R.T.: 12.246 min
Delta R.T.: 0.063 min
Response: 4961266
Conc: 2.50 ug/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-C

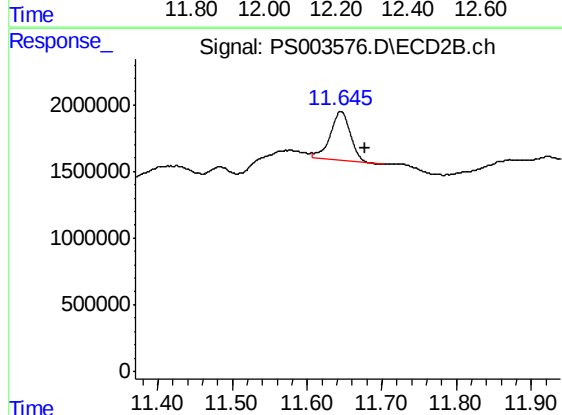


#7 MCPA

R.T.: 11.645 min
Delta R.T.: -0.032 min
Response: 6951395
Conc: 4.03 ug/ml

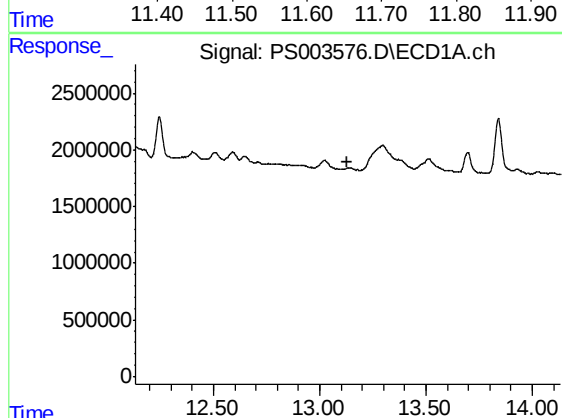


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

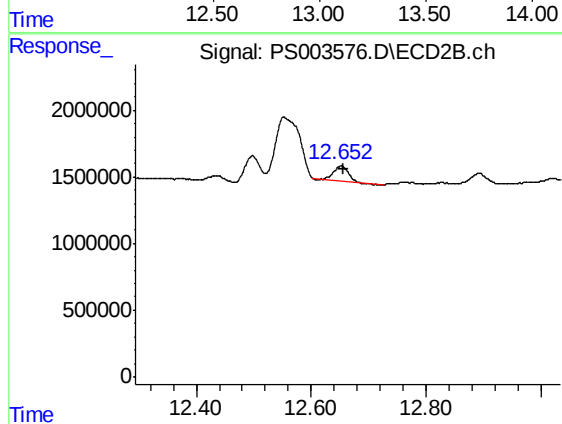

#9 2,4-D


R.T.: 12.652 min
Delta R.T.: -0.005 min
Response: 1714370
Conc: 3.27 ng/ml

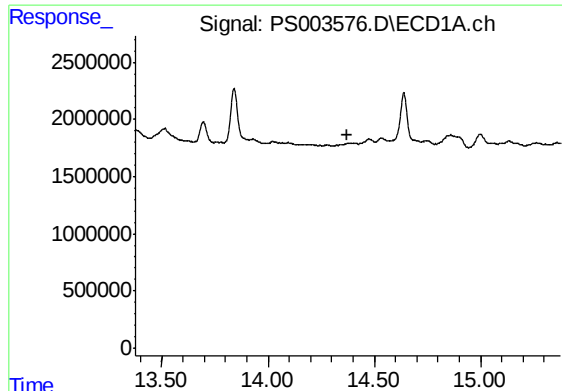

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-C

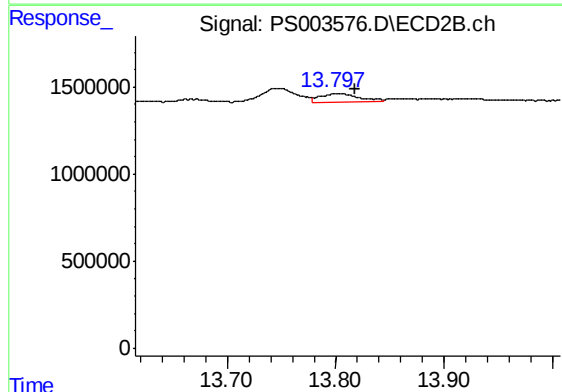


#11 2,4,5-TP (SILVEX)

R.T.: 13.803 min
Delta R.T.: -0.015 min
Response: 1240749
Conc: 0.49 ng/ml

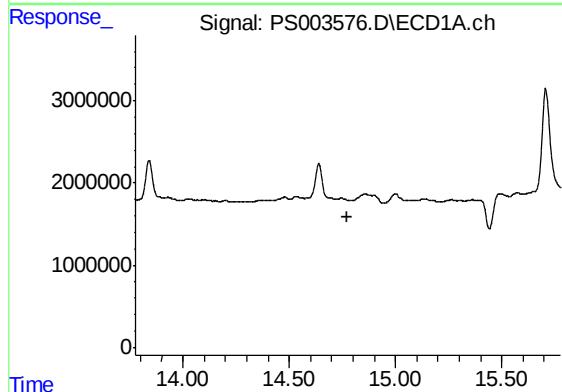


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

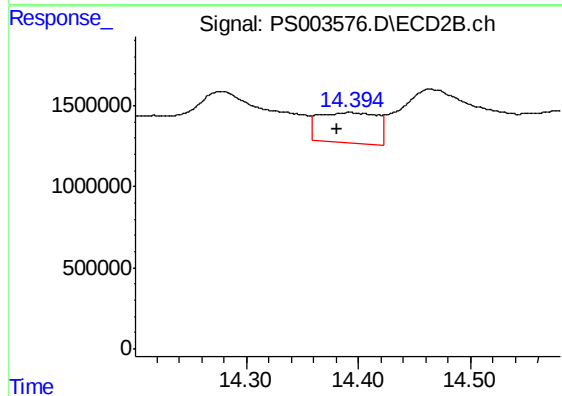

#12 2,4,5-T


R.T.: 14.392 min
Delta R.T.: 0.012 min
Response: 6719231
Conc: 3.33 ng/ml

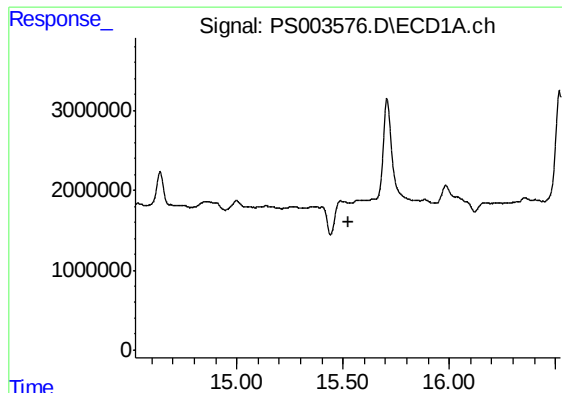

#13 2,4-DB


R.T.: 15.492 min
Delta R.T.: -0.031 min
Response: -3911147
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-C

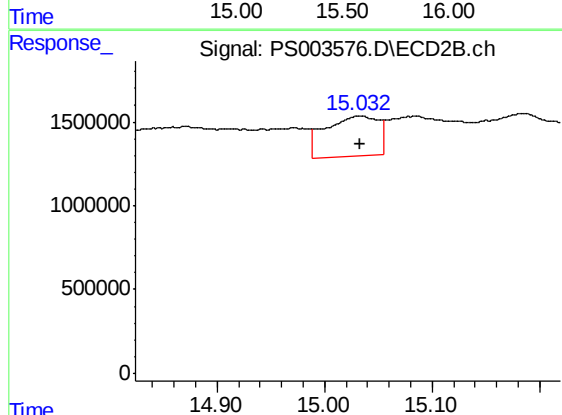


#13 2,4-DB

R.T.: 15.033 min
Delta R.T.: 0.000 min
Response: 8016308
Conc: 31.39 ng/ml

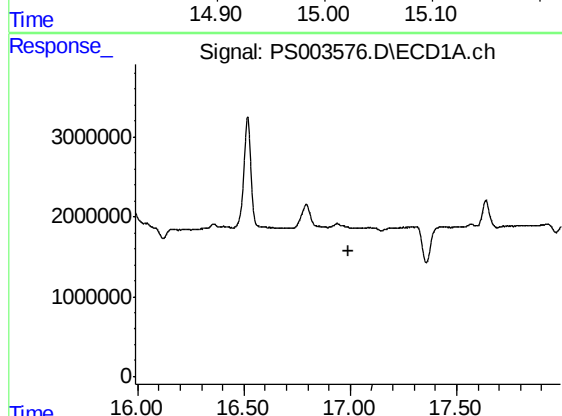


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

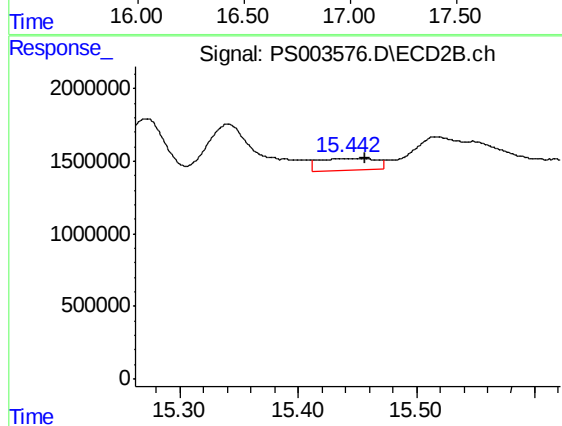

#14 DINOSEB


R.T.: 15.448 min
Delta R.T.: -0.009 min
Response: 2753876
Conc: 1.54 ng/ml

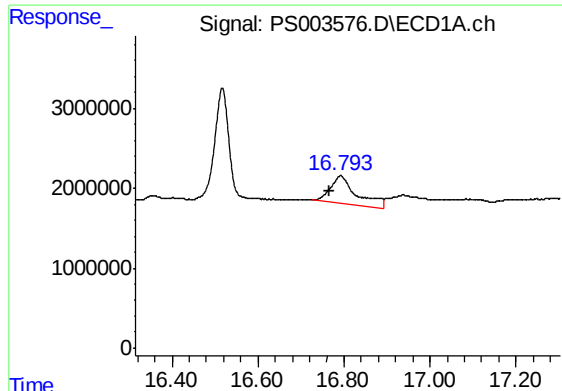

#15 Picloram


R.T.: 16.792 min
Delta R.T.: 0.027 min
Response: 14981268
Conc: 6.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-05-031419-C

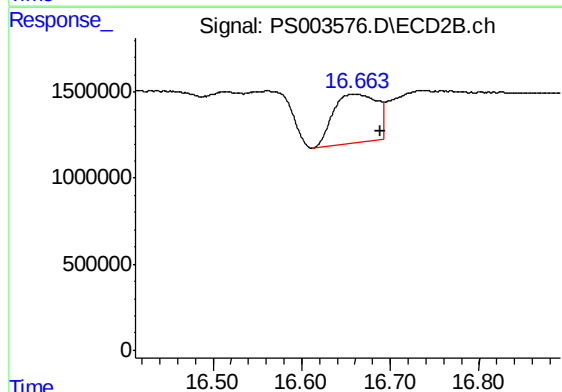


#15 Picloram

R.T.: 16.660 min
Delta R.T.: -0.028 min
Response: 9602771
Conc: 3.78 ng/ml

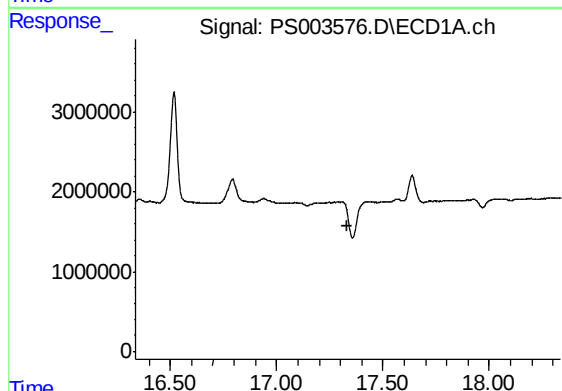

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

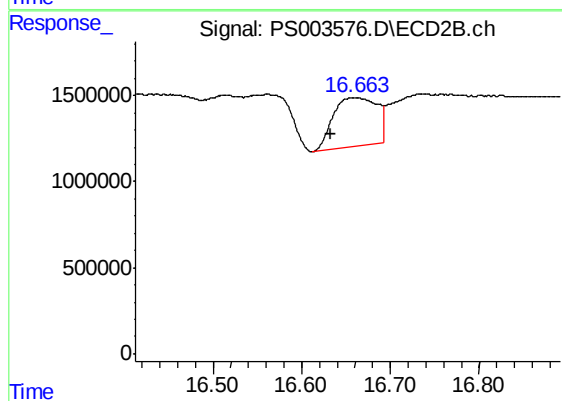

#16 DCPA

R.T.: 16.660 min
Delta R.T.: 0.028 min
Response: 9602771
Conc: 3.09 ng/ml