

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
 Data File : PS003580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2019 21:29
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 07:30:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.795	224.0E6	211.9E6	510.255	451.202
Target Compounds							
3) T	4-Nitroph...	0.000	9.988	0	121228	N.D.	0.539 #
7) T	MCPA	0.000	11.681	0	303841	N.D.	0.176 #
8) T	DICHLORPROP	0.000	12.214	0	174854	N.D.	0.423 #
10) T	Pentachlo...	0.000	13.213	0	535539	N.D.	0.081 #
11) T	2,4,5-TP ...	0.000	13.802	0	51114	N.D.	0.020 #
12) T	2,4,5-T	0.000	14.367	0	115121	N.D.	0.057 #
13) T	2,4-DB	0.000	15.097	0	228516	N.D.	0.895 #
14) T	DINOSEB	0.000	15.455	0	50929	N.D.	0.029 #
15) T	Picloram	0.000	16.649	0	288886	N.D.	0.114 #
16) T	DCPA	0.000	16.649	0	288886	N.D.	0.093 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
Data File : PS003580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2019 21:29
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 07:30:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

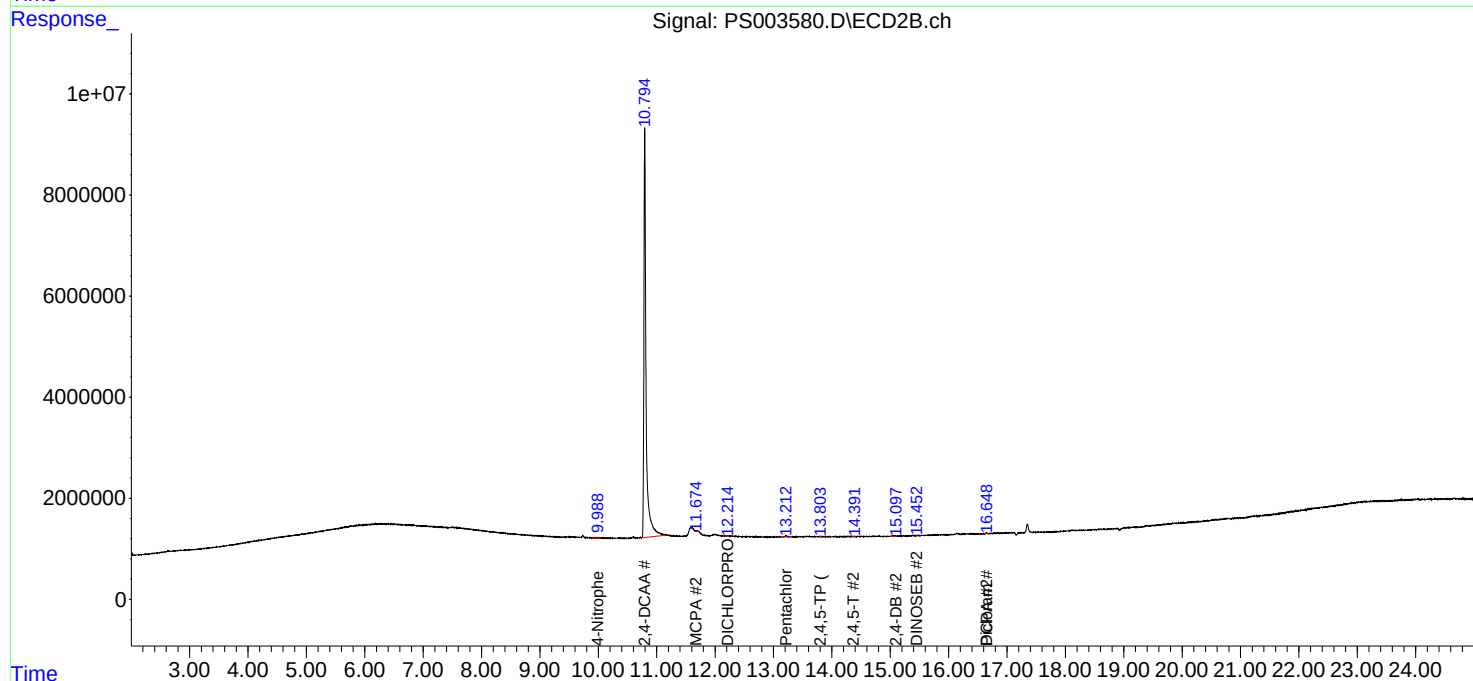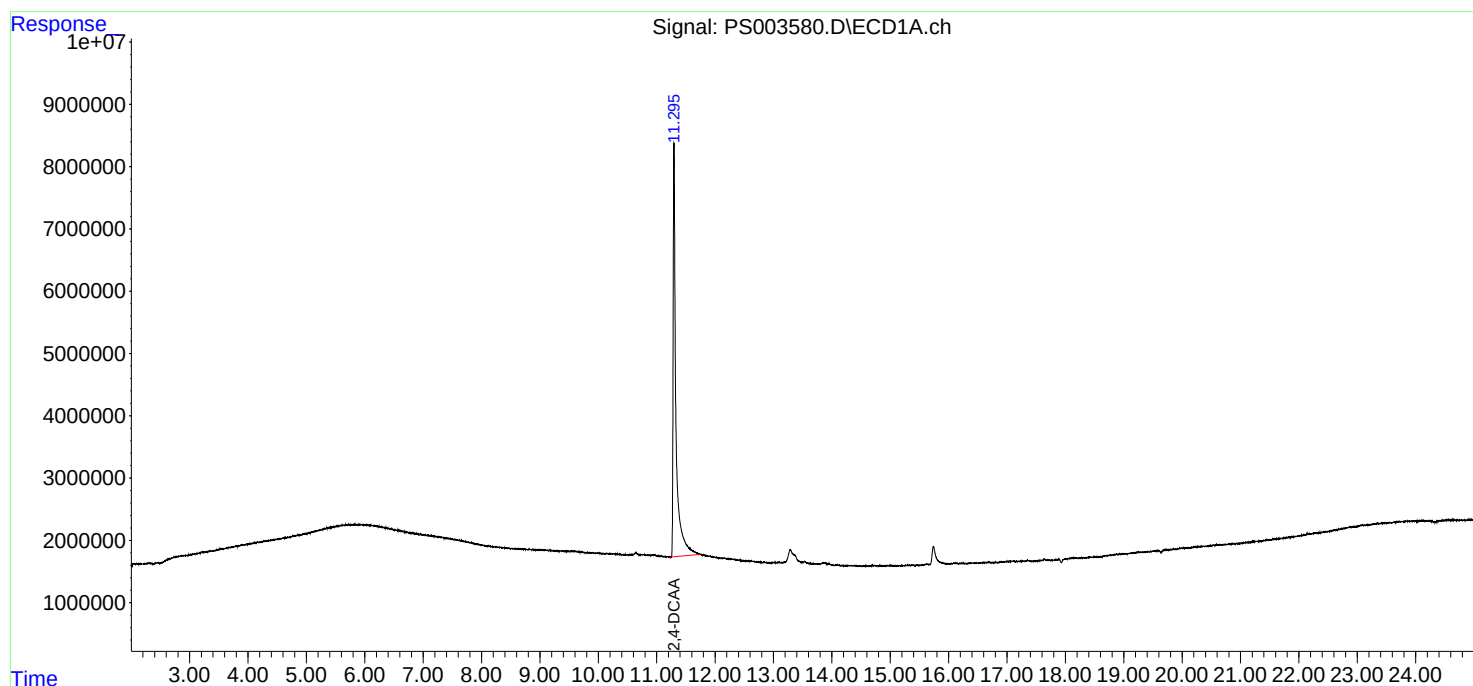


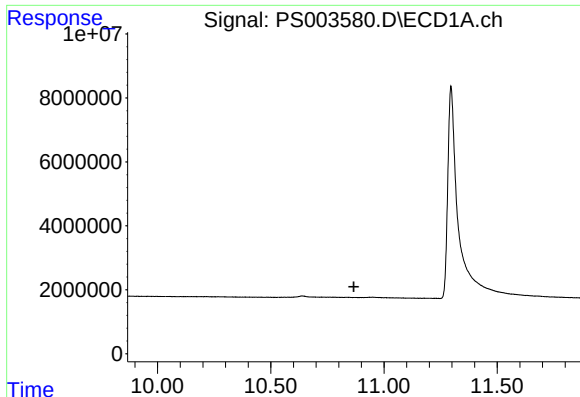

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

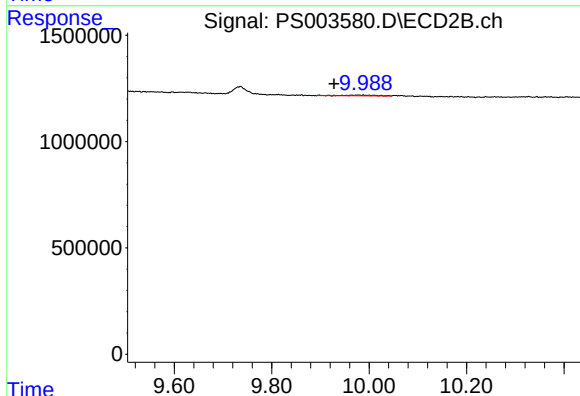


#3 4-Nitrophenol

R.T.: 9.988 min
Delta R.T.: 0.059 min
Response: 121228
Conc: 0.54 ng/ml

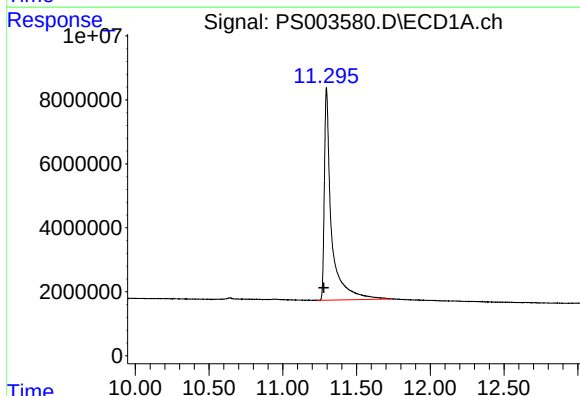


#4 2,4-DCAA

R.T.: 11.296 min
Delta R.T.: 0.018 min
Response: 224014392
Conc: 510.25 ng/ml

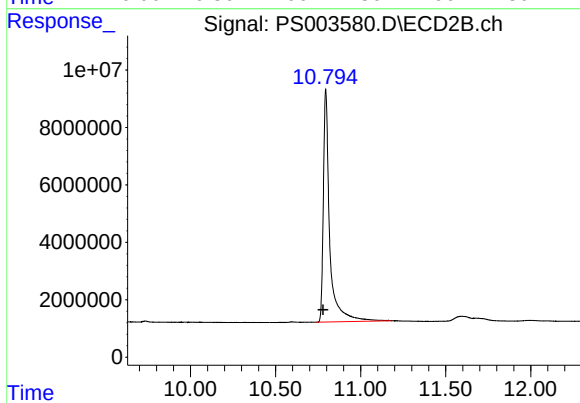

#4 2,4-DCAA


R.T.: 10.795 min
Delta R.T.: 0.015 min
Response: 211870411
Conc: 451.20 ng/ml

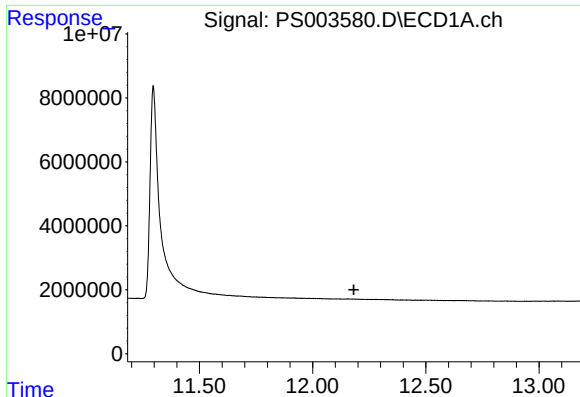

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

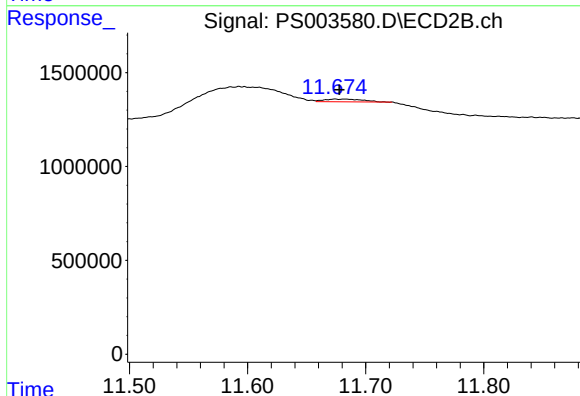


#7 MCPA

R.T.: 11.681 min
Delta R.T.: 0.004 min
Response: 303841
Conc: 0.18 ug/ml

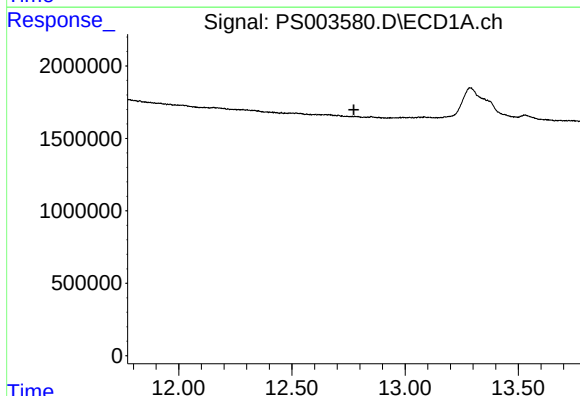


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

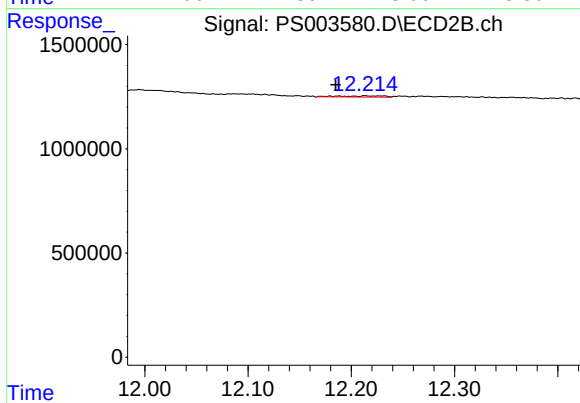

#8 DICHLORPROP


R.T.: 12.214 min
Delta R.T.: 0.029 min
Response: 174854
Conc: 0.42 ng/ml

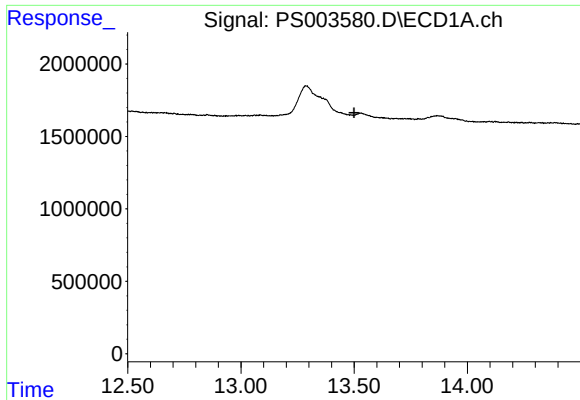

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

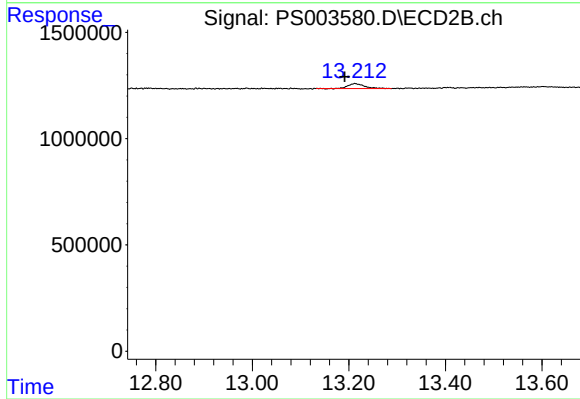


#10 Pentachlorophenol

R.T.: 13.213 min
Delta R.T.: 0.021 min
Response: 535539
Conc: 0.08 ng/ml

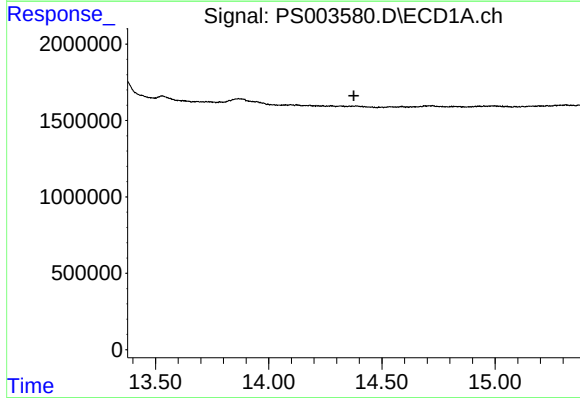


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

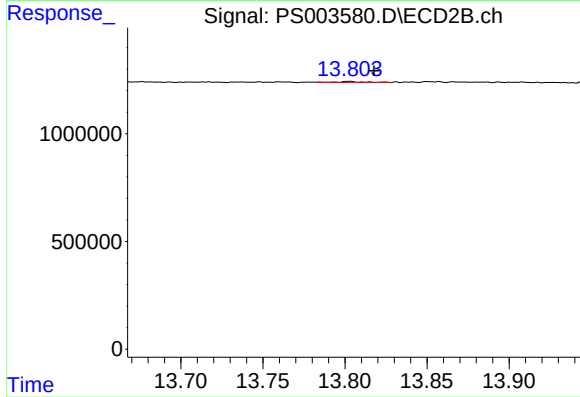

#11 2,4,5-TP (SILVEX)


R.T.: 13.802 min
Delta R.T.: -0.015 min
Response: 51114
Conc: 0.02 ng/ml

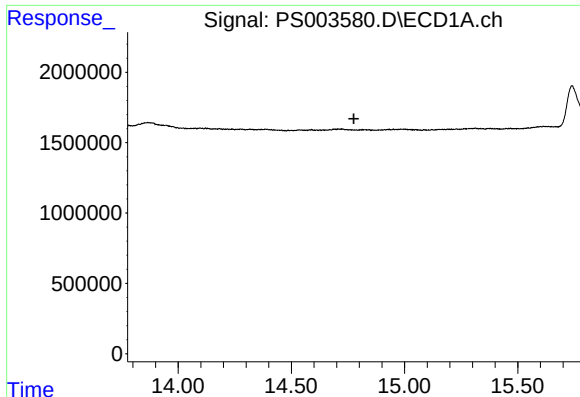

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

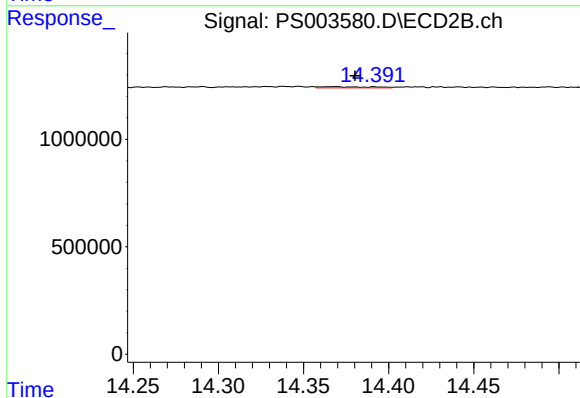


#12 2,4,5-T

R.T.: 14.367 min
Delta R.T.: -0.013 min
Response: 115121
Conc: 0.06 ng/ml

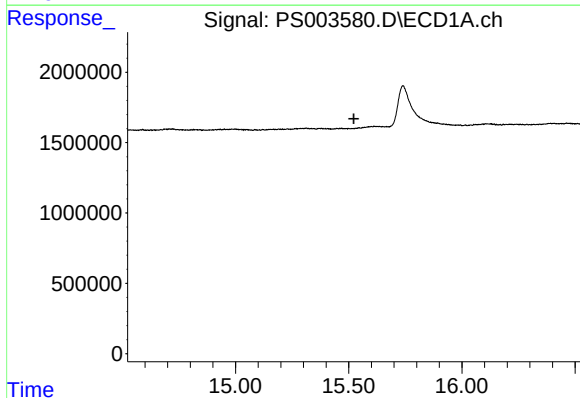


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

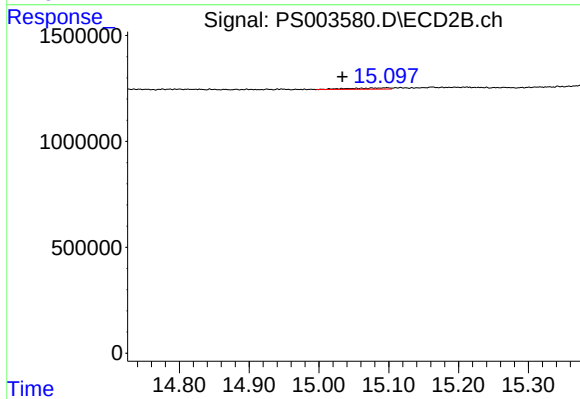

#13 2,4-DB


R.T.: 15.097 min
Delta R.T.: 0.063 min
Response: 228516
Conc: 0.89 ng/ml

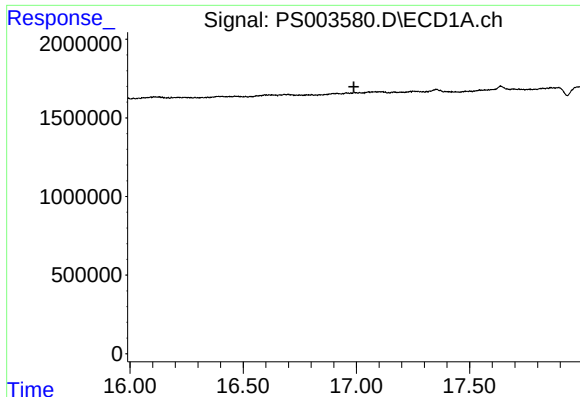

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

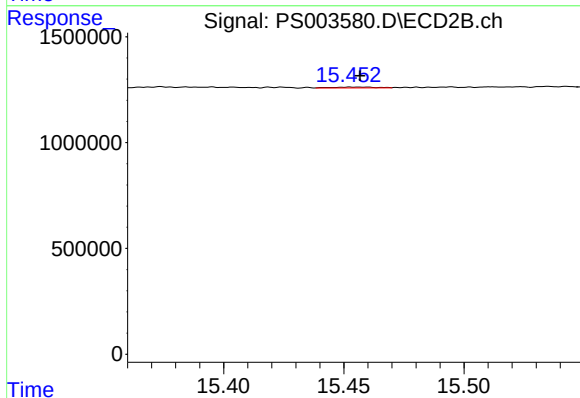


#14 DINOSEB

R.T.: 15.455 min
Delta R.T.: -0.002 min
Response: 50929
Conc: 0.03 ng/ml

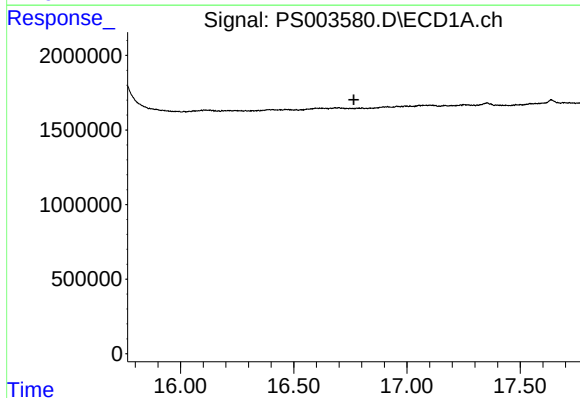


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

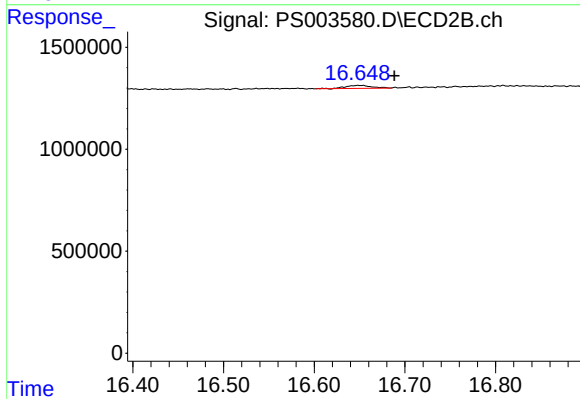

#15 Picloram


R.T.: 16.649 min
Delta R.T.: -0.039 min
Response: 288886
Conc: 0.11 ng/ml

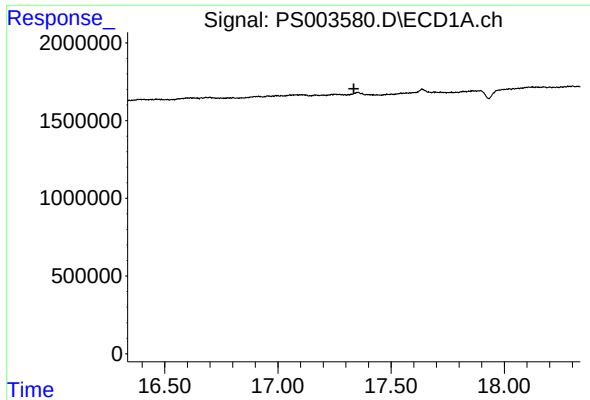

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

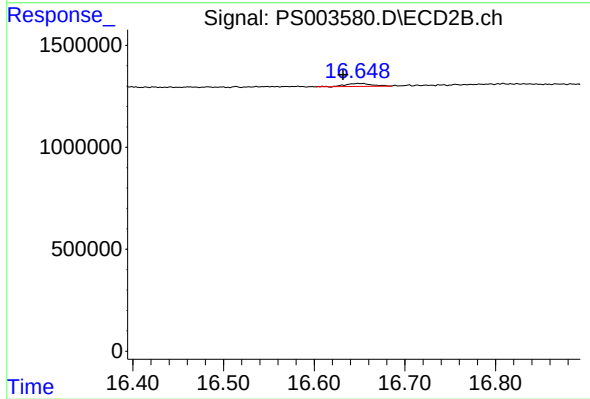

#16 DCPA

R.T.: 16.649 min
Delta R.T.: 0.017 min
Response: 288886
Conc: 0.09 ng/ml