

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
 Data File : PS003585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2019 06:35
 Operator : EI\SJ
 Sample : K1698-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-04-031419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 07:32:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.270	10.773	302.3E6	278.9E6	688.510	593.847
Target Compounds							
1) T	Dalapon	2.793	2.288	42280510	58191516	65.053	91.903 #
2) T	3,5-DICHL...	0.000	8.940	0	12073714	N.D.	19.554 #
3) T	4-Nitroph...	10.818	9.949	908152	990816	4.316	4.407
5) T	DICAMBA	11.636	11.013	2857109	7056524	1.621	4.224 #
6) T	MCPD	11.946	0.000	77834066	0	59.284	N.D. #
7) T	MCPA	12.121	11.674	16327953	-272892	8.232	N.D. #
9) T	2,4-D	0.000	12.635	0	1488923	N.D.	2.837 #
11) T	2,4,5-TP ...	0.000	13.838	0	976416	N.D.	0.383 #
12) T	2,4,5-T	0.000	14.432	0	14173651	N.D.	7.028 #
13) T	2,4-DB	0.000	15.001	0	2937962	N.D.	11.505 #
14) T	DINOSEB	0.000	15.520	0	12371576	N.D.	6.931 #
15) T	Picloram	16.748	16.724	10974110	11599375	4.459	4.570
16) T	DCPA	0.000	16.633	0	3838545	N.D.	1.234 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
Data File : PS003585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2019 06:35
Operator : EI\SJ
Sample : K1698-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TR-04-031419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 07:32:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

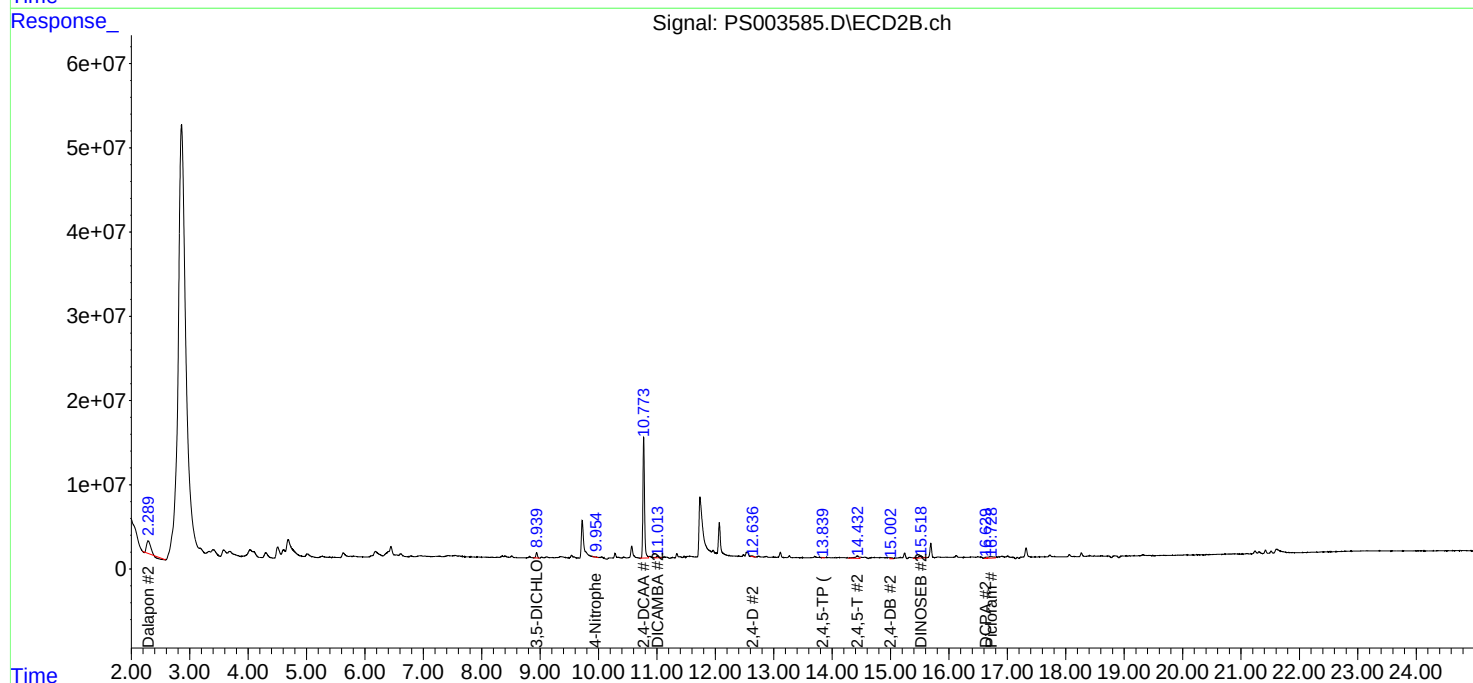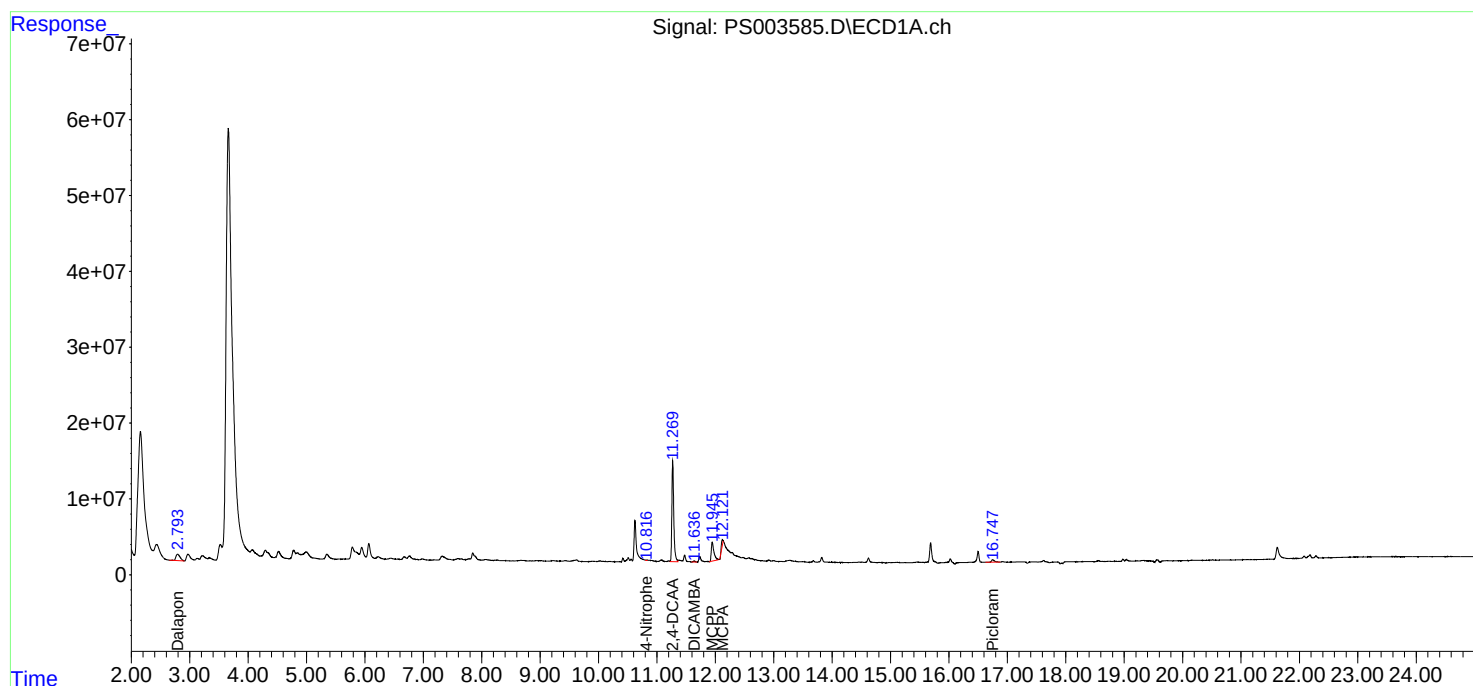


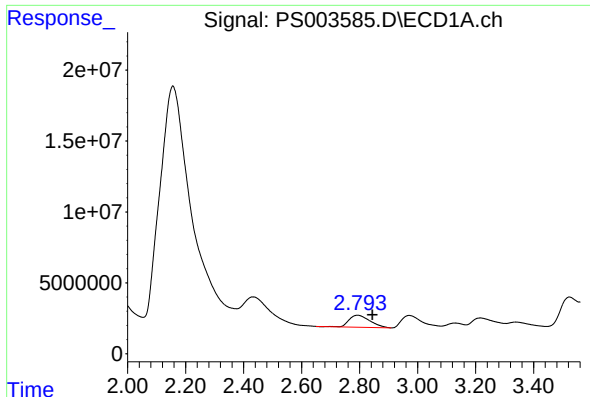

#1 Dalapon


R.T.: 2.793 min
Delta R.T.: -0.051 min
Response: 42280510
Conc: 65.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-031419

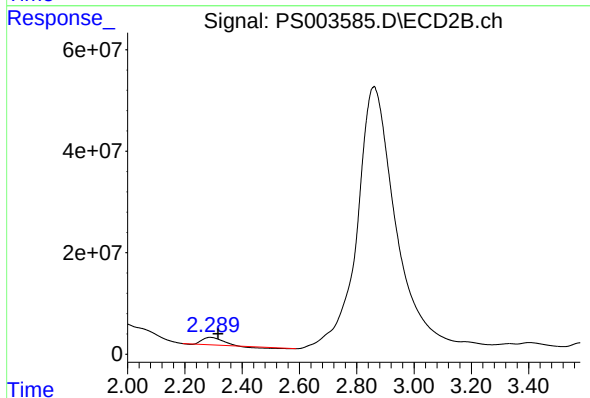


#1 Dalapon

R.T.: 2.288 min
Delta R.T.: -0.029 min
Response: 58191516
Conc: 91.90 ng/ml

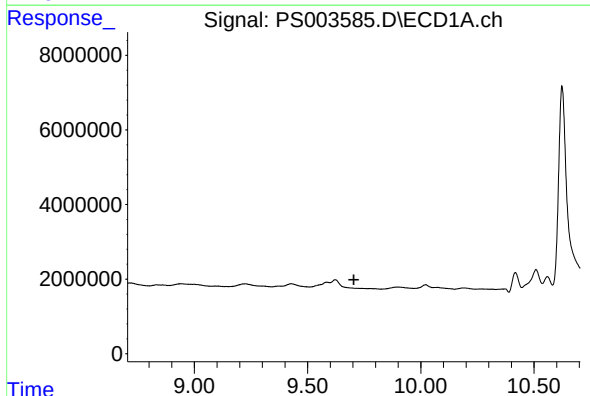


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

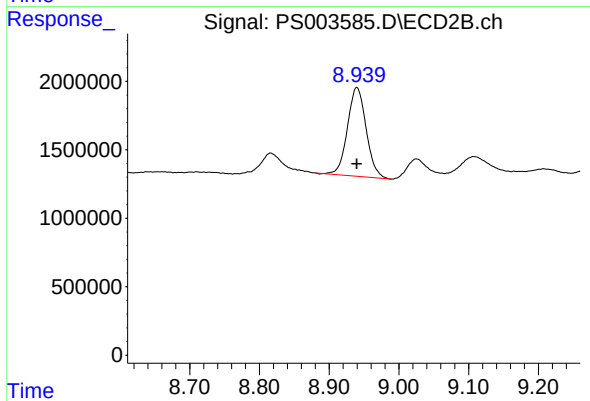

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.940 min
Delta R.T.: 0.000 min
Response: 12073714
Conc: 19.55 ng/ml

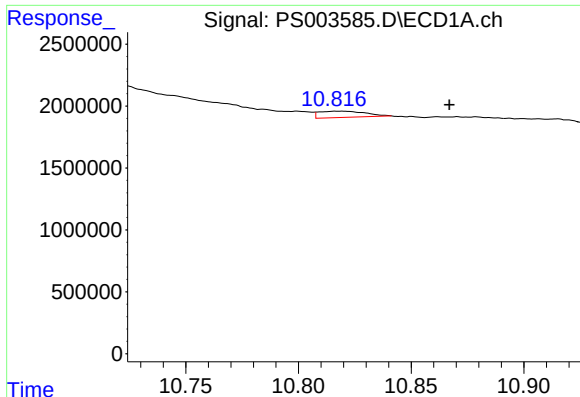

#3 4-Nitrophenol


R.T.: 10.818 min
Delta R.T.: -0.049 min
Response: 908152
Conc: 4.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-031419

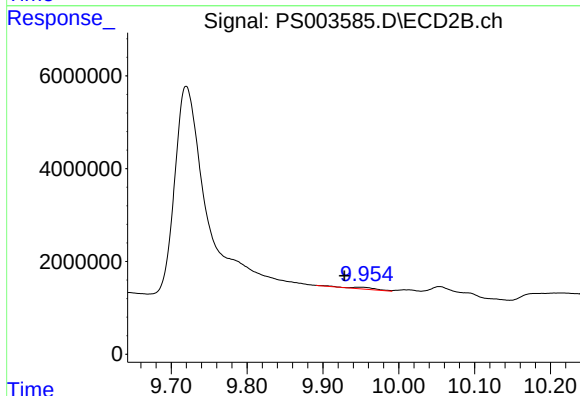


#3 4-Nitrophenol

R.T.: 9.949 min
Delta R.T.: 0.021 min
Response: 990816
Conc: 4.41 ng/ml

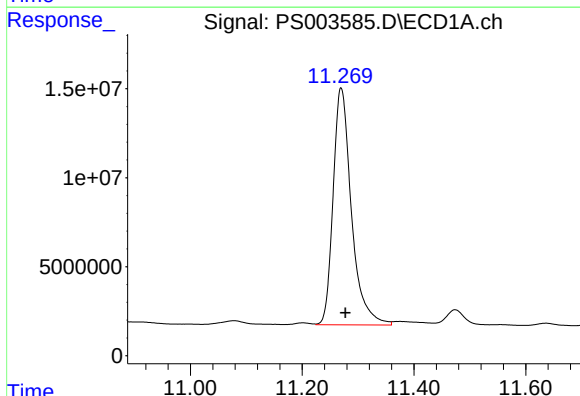


#4 2,4-DCAA

R.T.: 11.270 min
Delta R.T.: -0.008 min
Response: 302272637
Conc: 688.51 ng/ml

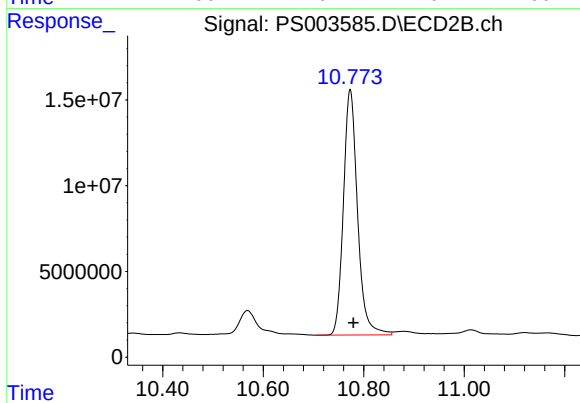

#4 2,4-DCAA


R.T.: 10.773 min
Delta R.T.: -0.007 min
Response: 278852371
Conc: 593.85 ng/ml

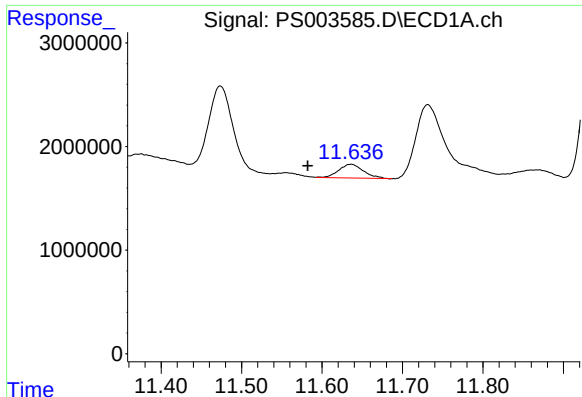

#5 DICAMBA


R.T.: 11.636 min
Delta R.T.: 0.054 min
Response: 2857109
Conc: 1.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-031419

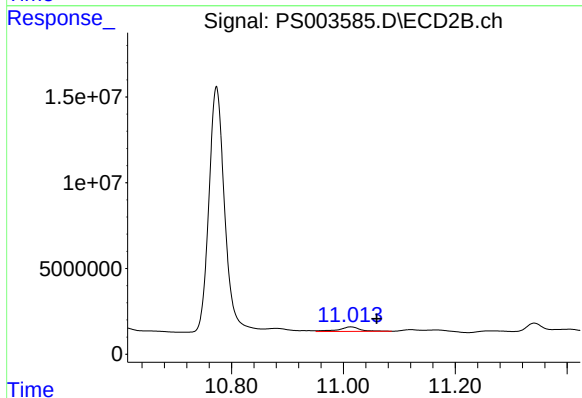


#5 DICAMBA

R.T.: 11.013 min
Delta R.T.: -0.046 min
Response: 7056524
Conc: 4.22 ng/ml

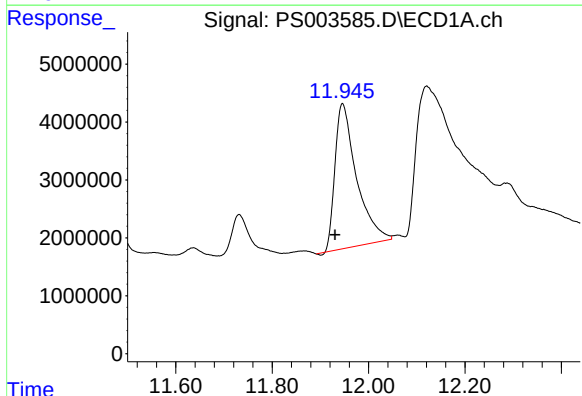


#6 MCP

R.T.: 11.946 min
Delta R.T.: 0.015 min
Response: 77834066
Conc: 59.28 ug/ml

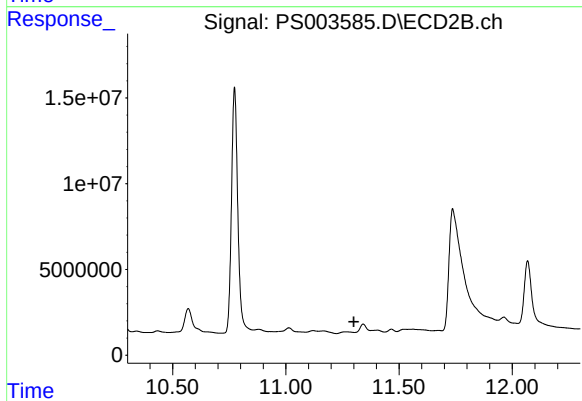

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.300 min
Response: 0
Conc: N.D.

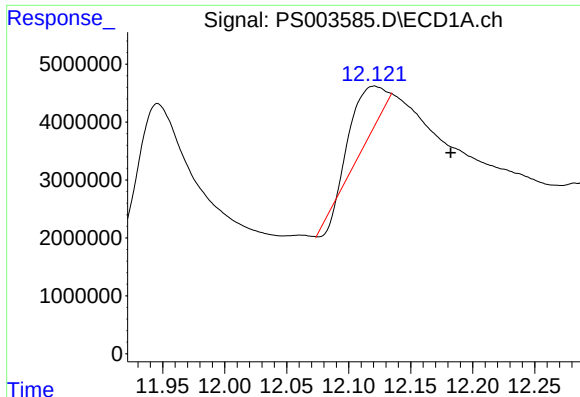

#7 MCPA


R.T.: 12.121 min
Delta R.T.: -0.061 min
Response: 16327953
Conc: 8.23 ug/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-031419

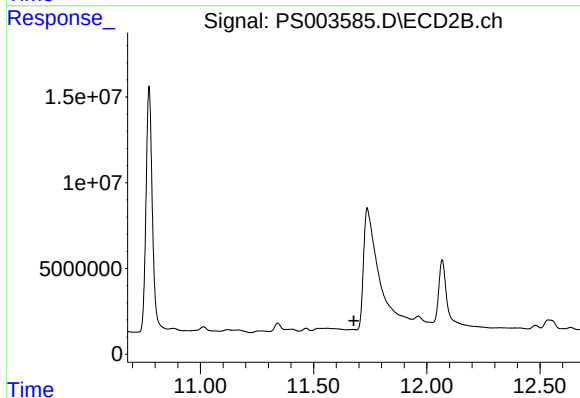


#7 MCPA

R.T.: 11.674 min
Delta R.T.: -0.004 min
Response: -272892
Conc: N.D.

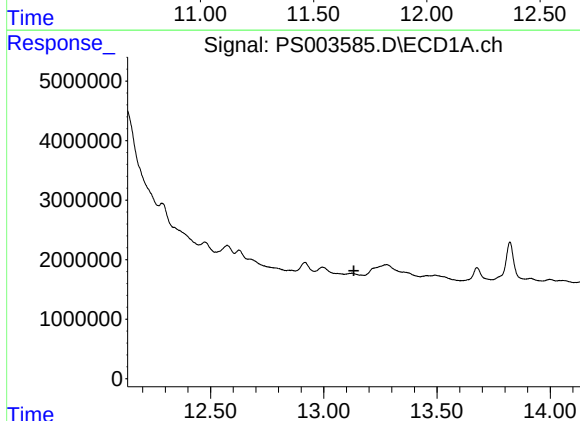


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

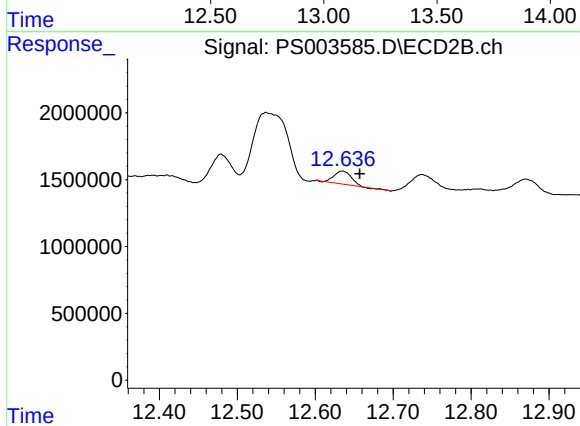

#9 2,4-D


R.T.: 12.635 min
Delta R.T.: -0.022 min
Response: 1488923
Conc: 2.84 ng/ml

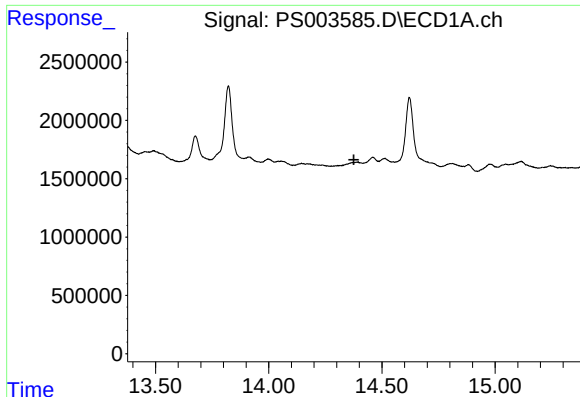

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-031419

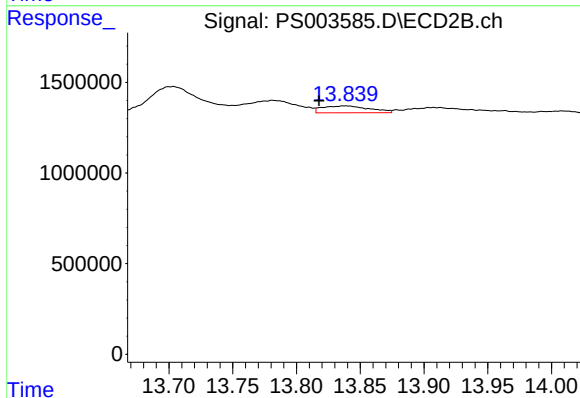


#11 2,4,5-TP (SILVEX)

R.T.: 13.838 min
Delta R.T.: 0.021 min
Response: 976416
Conc: 0.38 ng/ml

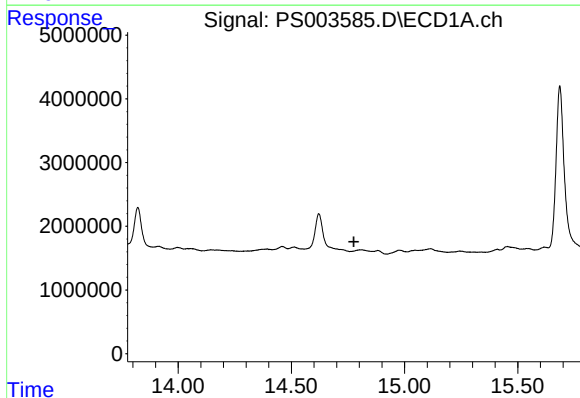


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

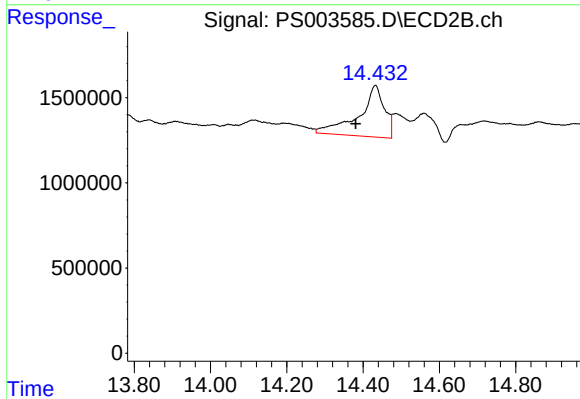

#12 2,4,5-T


R.T.: 14.432 min
Delta R.T.: 0.052 min
Response: 14173651
Conc: 7.03 ng/ml

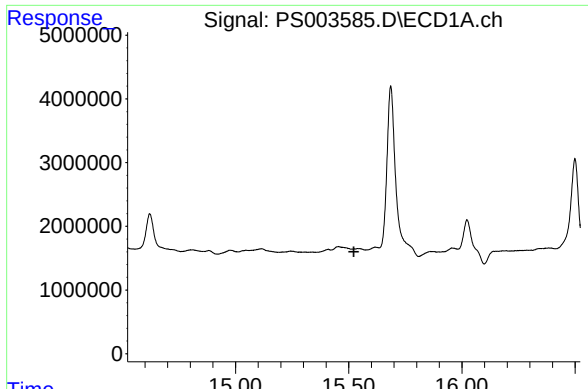

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-031419

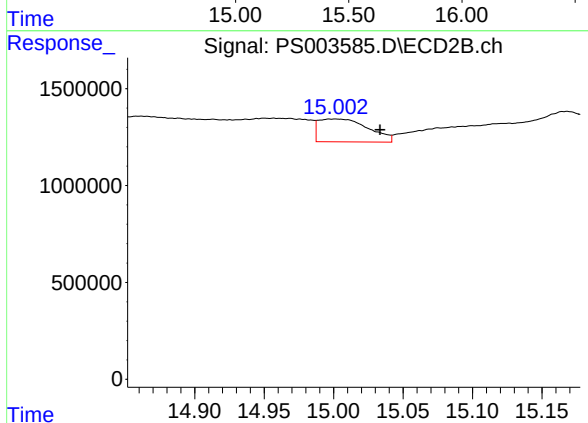


#13 2,4-DB

R.T.: 15.001 min
Delta R.T.: -0.033 min
Response: 2937962
Conc: 11.51 ng/ml

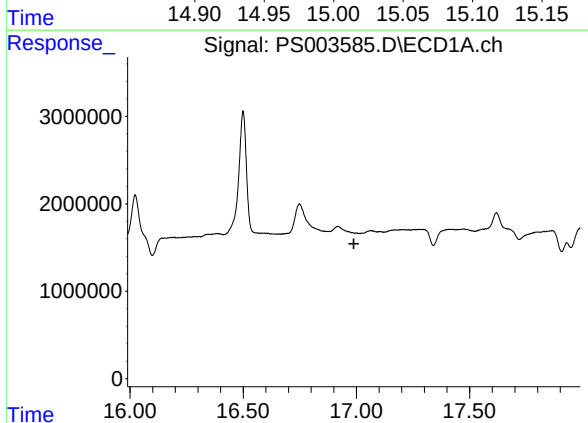


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

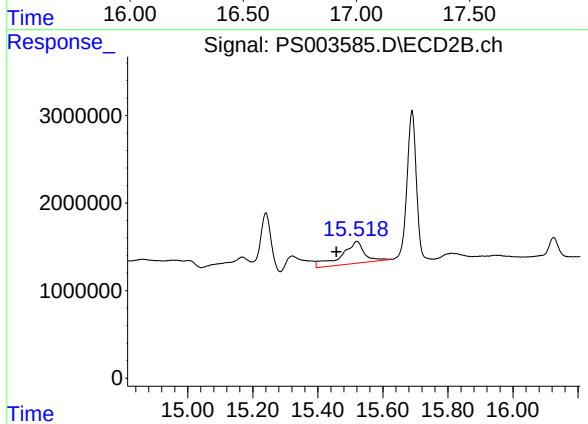

#14 DINOSEB


R.T.: 15.520 min
Delta R.T.: 0.063 min
Response: 12371576
Conc: 6.93 ng/ml

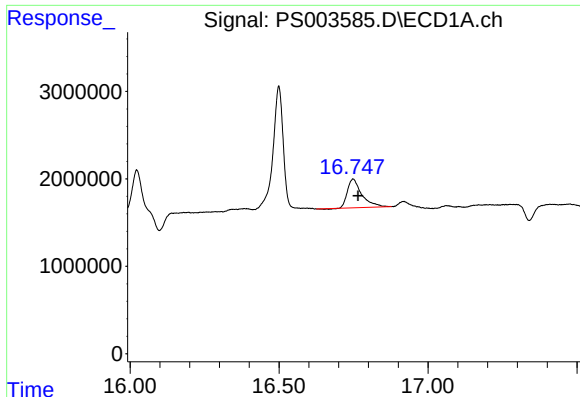

#15 Picloram


R.T.: 16.748 min
Delta R.T.: -0.017 min
Response: 10974110
Conc: 4.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-031419

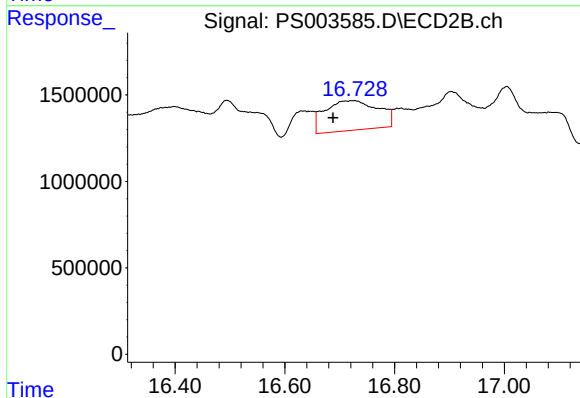


#15 Picloram

R.T.: 16.724 min
Delta R.T.: 0.036 min
Response: 11599375
Conc: 4.57 ng/ml

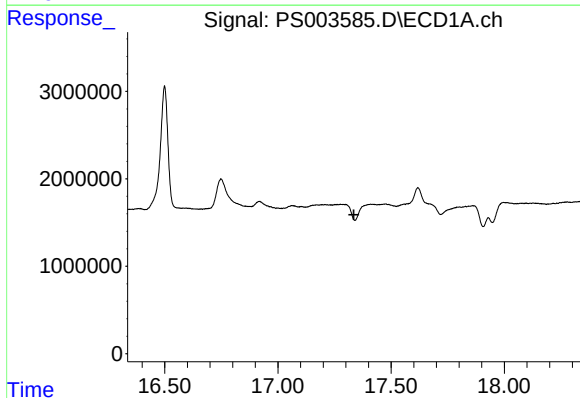

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

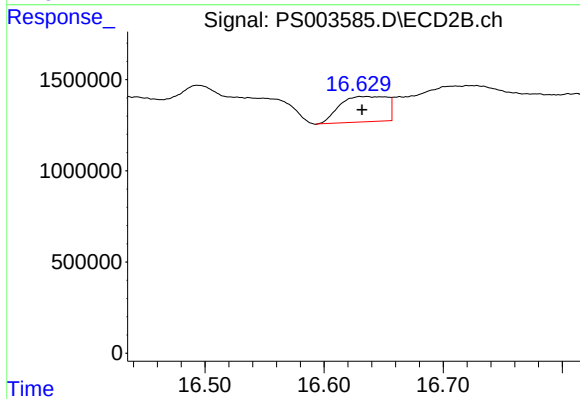

#16 DCPA

R.T.: 16.633 min
Delta R.T.: 0.002 min
Response: 3838545
Conc: 1.23 ng/ml