

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
 Data File : PS003588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2019 08:08
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 15:32:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.284	10.782	233.9E6	216.7E6	532.828	461.586
Target Compounds							
1) T	Dalapon	0.000	2.280	0	25704	N.D.	0.041 #
2) T	3,5-DICHL...	0.000	9.003	0	80494	N.D.	0.130 #
3) T	4-Nitroph...	0.000	9.971	0	57156	N.D.	0.254 #
7) T	MCPA	0.000	11.663	0	314762	N.D.	0.182 #
8) T	DICHLORPROP	0.000	12.203	0	2925157	N.D.	7.079 #
9) T	2,4-D	0.000	12.663	0	65984	N.D.	0.126 #
10) T	Pentachlo...	0.000	13.202	0	1029211	N.D.	0.156 #
11) T	2,4,5-TP ...	0.000	13.798	0	187819	N.D.	0.074 #
12) T	2,4,5-T	0.000	14.375	0	36354	N.D.	0.018 #
13) T	2,4-DB	0.000	15.033	0	80779	N.D.	0.316 #
14) T	DINOSEB	0.000	15.511	0	245729	N.D.	0.138 #
15) T	Picloram	0.000	16.687	0	44705	N.D.	0.018 #
16) T	DCPA	0.000	16.632	0	357122	N.D.	0.115 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
Data File : PS003588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2019 08:08
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 15:32:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

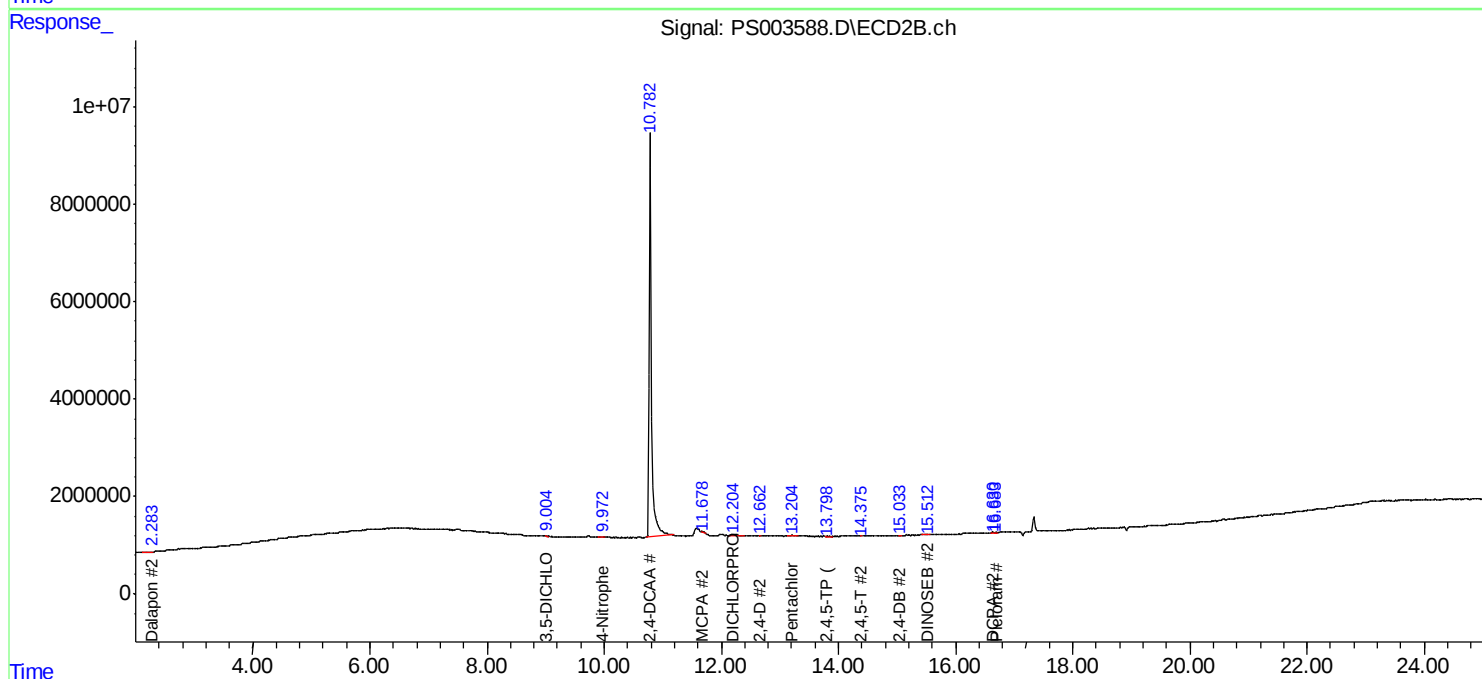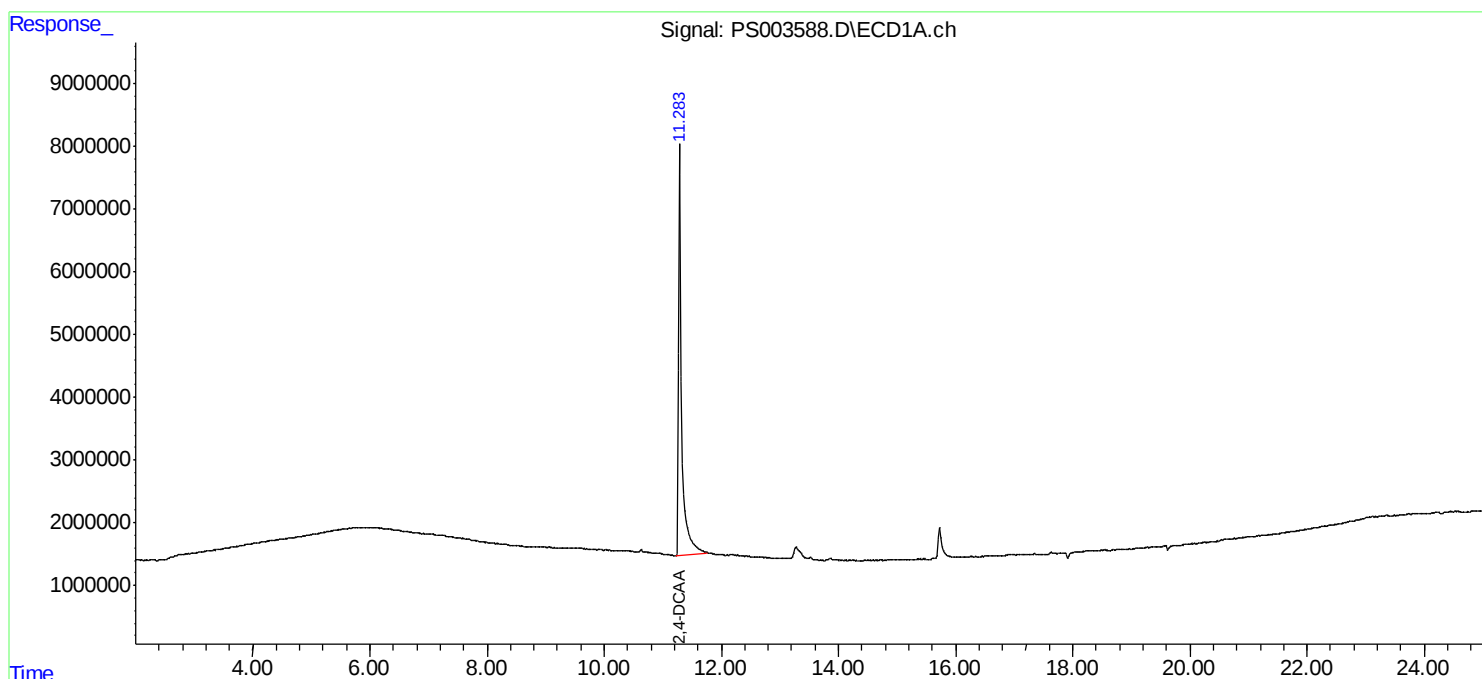


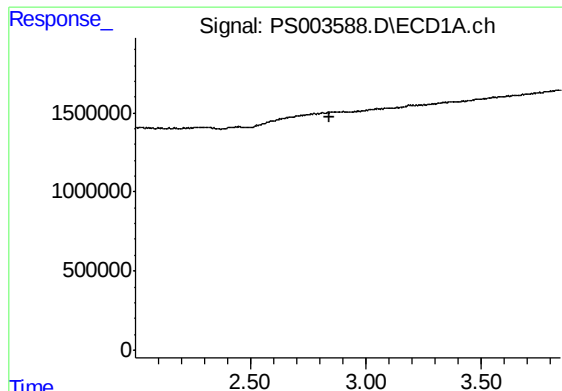

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

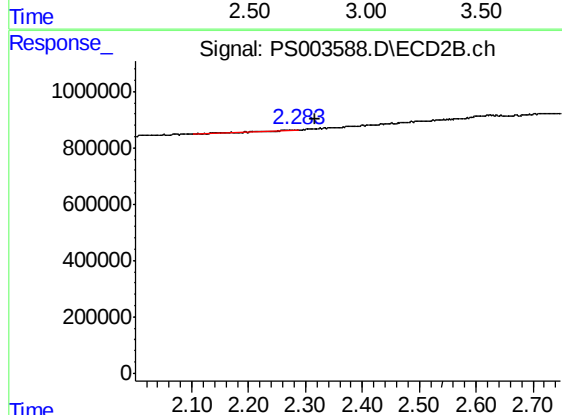


#1 Dalapon

R.T.: 2.280 min
Delta R.T.: -0.036 min
Response: 25704
Conc: 0.04 ng/ml

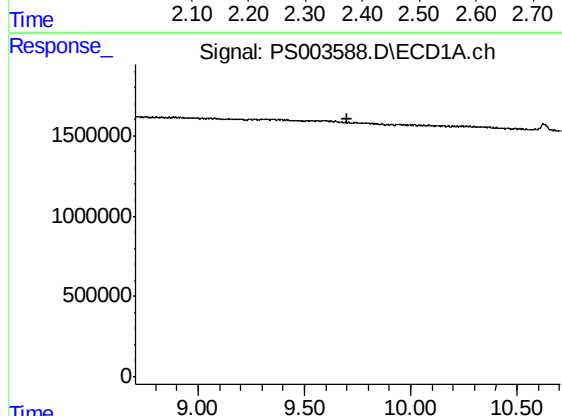


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

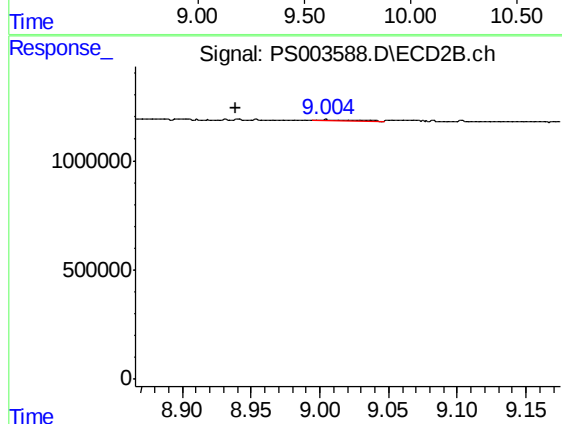

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.003 min
Delta R.T.: 0.064 min
Response: 80494
Conc: 0.13 ng/ml

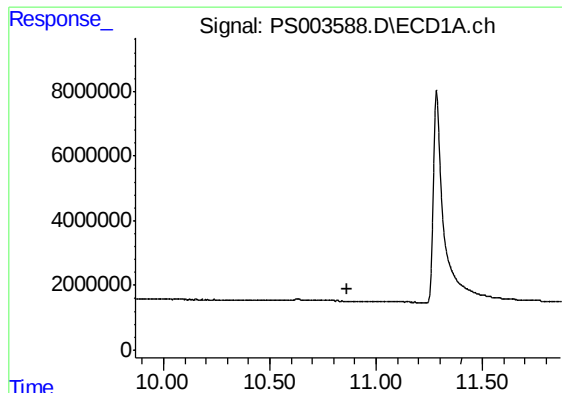

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

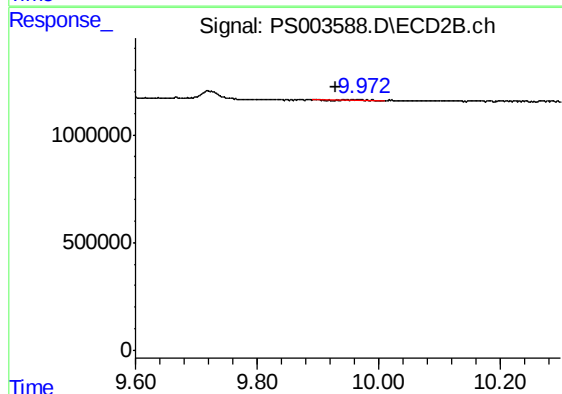


#3 4-Nitrophenol

R.T.: 9.971 min
Delta R.T.: 0.042 min
Response: 57156
Conc: 0.25 ng/ml

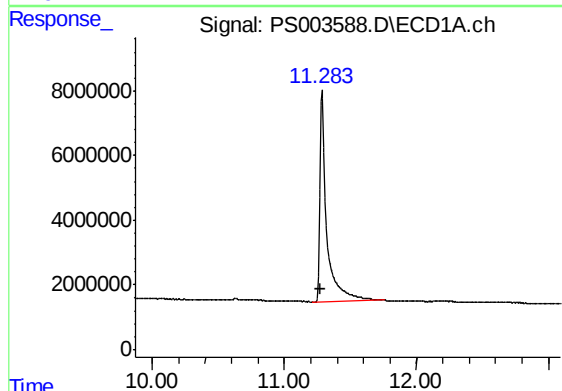


#4 2,4-DCAA

R.T.: 11.284 min
Delta R.T.: 0.006 min
Response: 233924585
Conc: 532.83 ng/ml

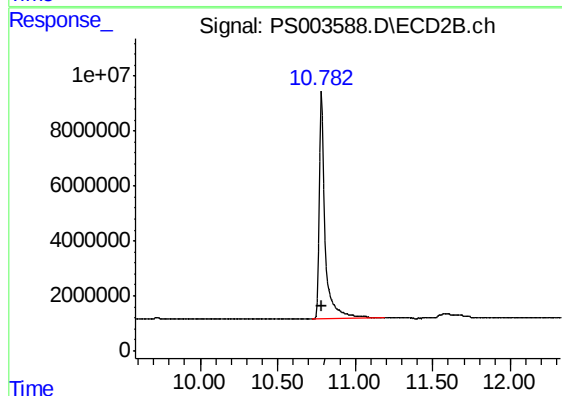

#4 2,4-DCAA


R.T.: 10.782 min
Delta R.T.: 0.002 min
Response: 216746561
Conc: 461.59 ng/ml

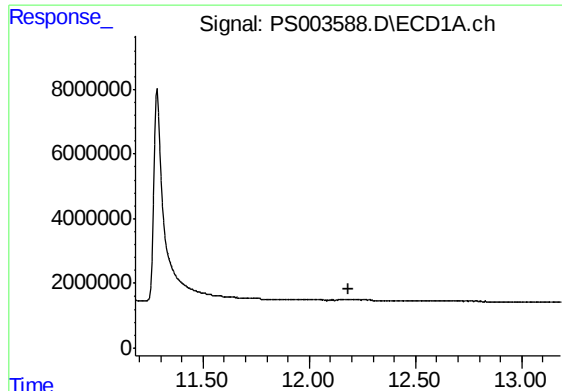

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

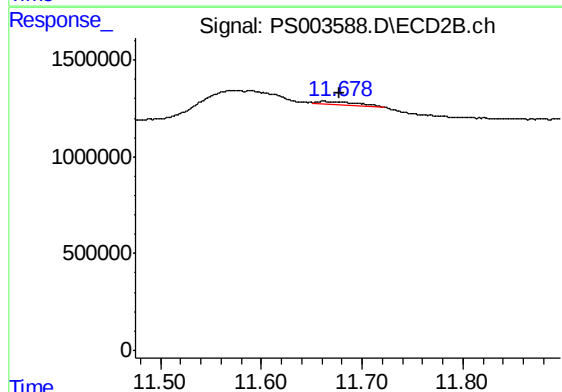


#7 MCPA

R.T.: 11.663 min
Delta R.T.: -0.015 min
Response: 314762
Conc: 0.18 ug/ml

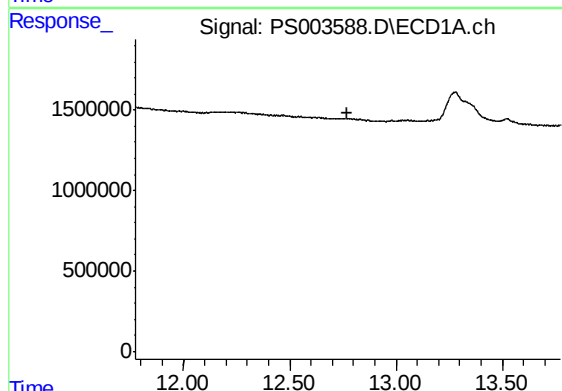


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

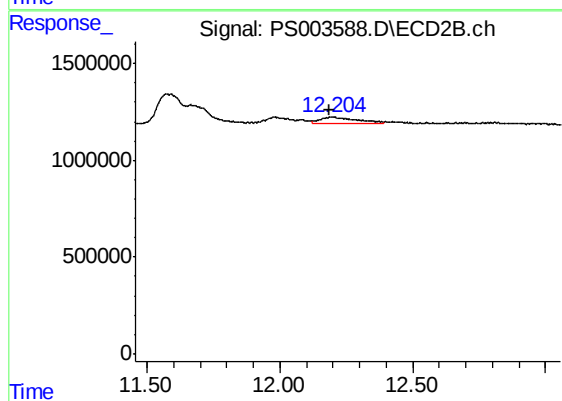

#8 DICHLORPROP


R.T.: 12.203 min
Delta R.T.: 0.018 min
Response: 2925157
Conc: 7.08 ng/ml

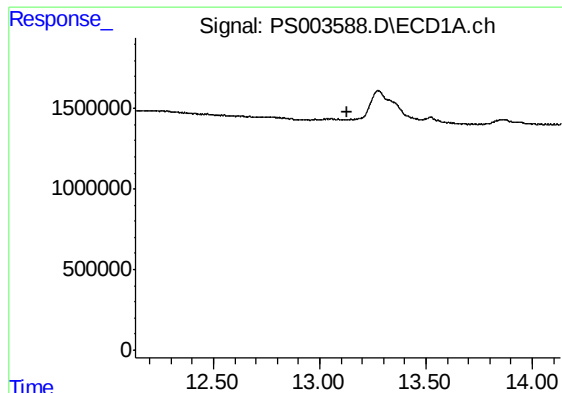

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

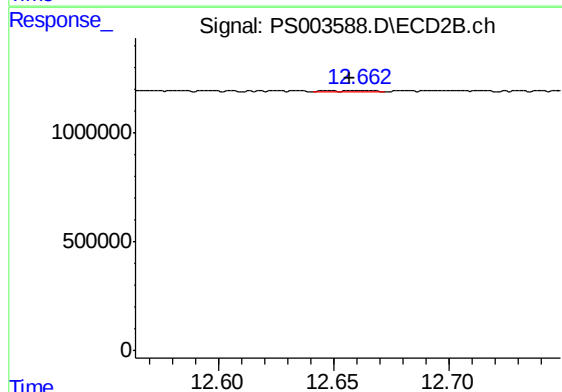


#9 2,4-D

R.T.: 12.663 min
Delta R.T.: 0.006 min
Response: 65984
Conc: 0.13 ng/ml

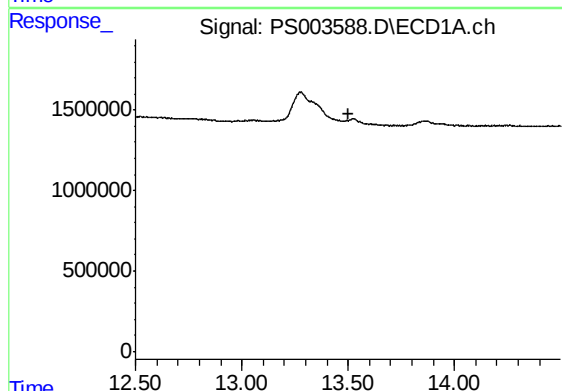


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

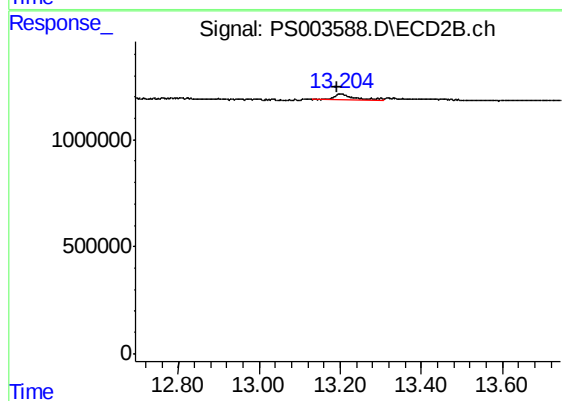

#10 Pentachlorophenol


R.T.: 13.202 min
Delta R.T.: 0.011 min
Response: 1029211
Conc: 0.16 ng/ml

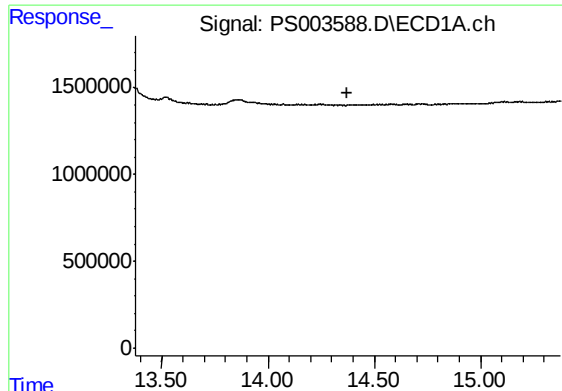

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

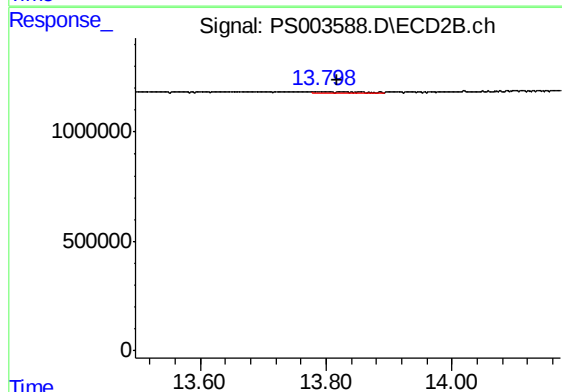


#11 2,4,5-TP (SILVEX)

R.T.: 13.798 min
Delta R.T.: -0.019 min
Response: 187819
Conc: 0.07 ng/ml

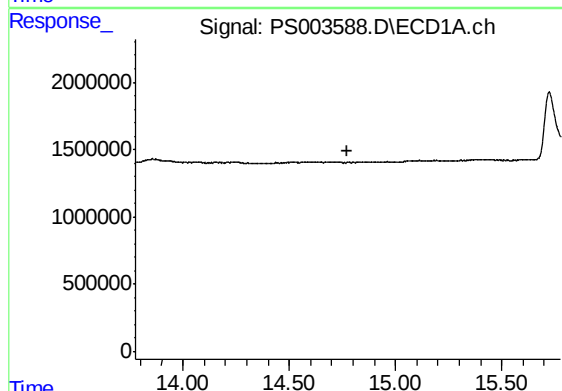


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

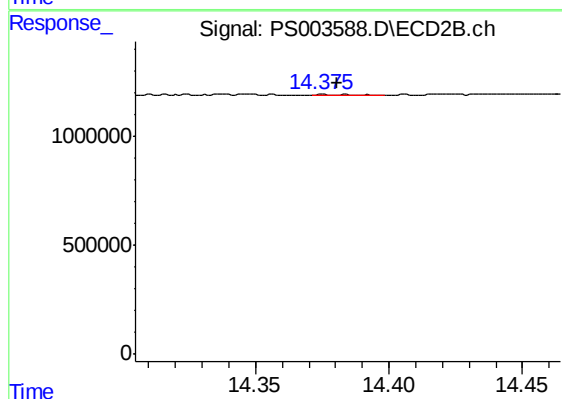

#12 2,4,5-T


R.T.: 14.375 min
Delta R.T.: -0.005 min
Response: 36354
Conc: 0.02 ng/ml

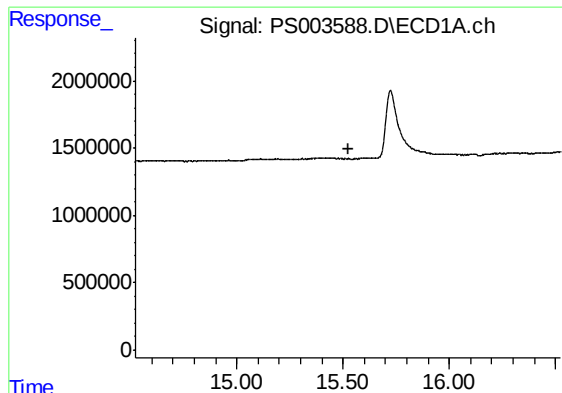

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

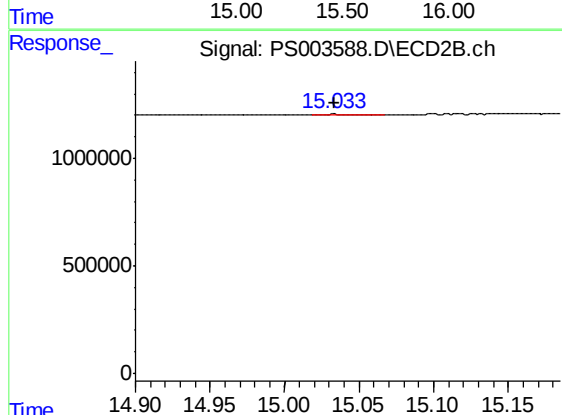


#13 2,4-DB

R.T.: 15.033 min
Delta R.T.: 0.000 min
Response: 80779
Conc: 0.32 ng/ml

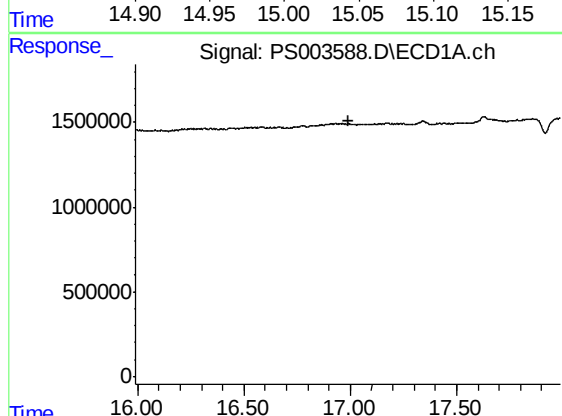


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

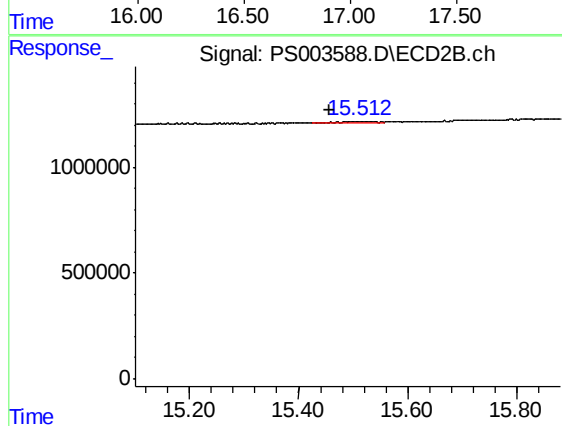

#14 DINOSEB


R.T.: 15.511 min
Delta R.T.: 0.054 min
Response: 245729
Conc: 0.14 ng/ml

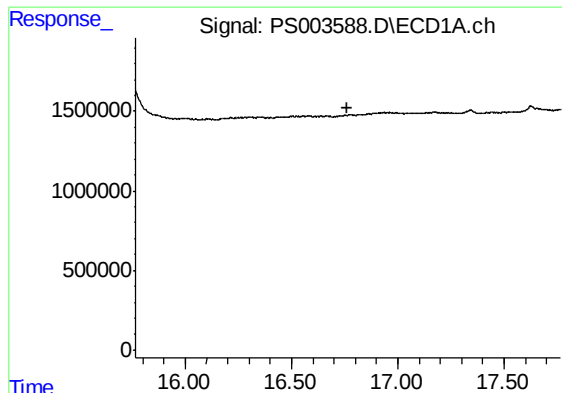

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

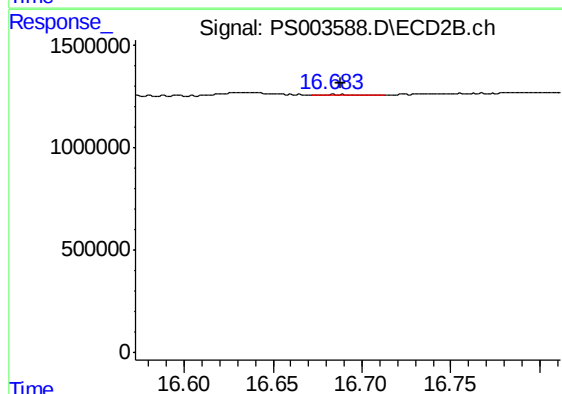


#15 Picloram

R.T.: 16.687 min
Delta R.T.: -0.002 min
Response: 44705
Conc: 0.02 ng/ml

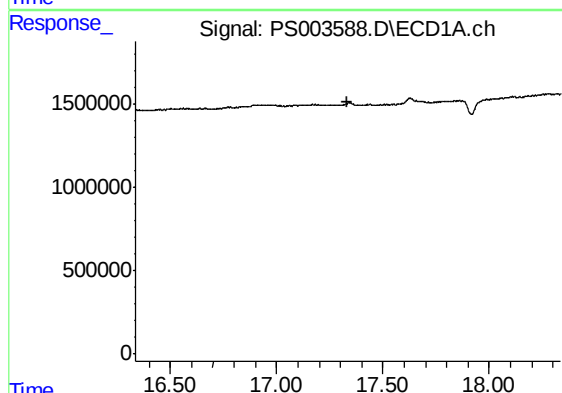

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

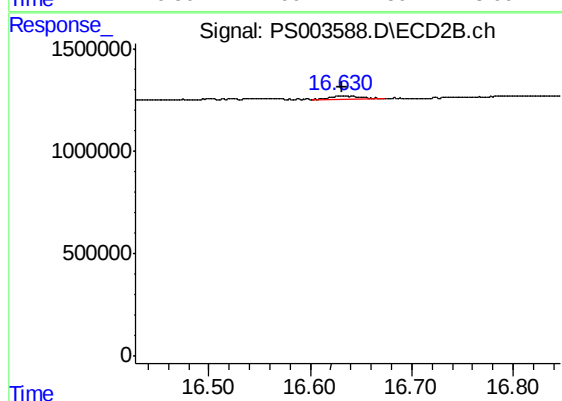

#16 DCPA

R.T.: 16.632 min
Delta R.T.: 0.000 min
Response: 357122
Conc: 0.11 ng/ml