

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
 Data File : PS003592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2019 10:13
 Operator : EI\SJ
 Sample : K1905-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RT-3483

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 15:34:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.301	10.801	105.6E6	104.4E6	240.618	222.230
Target Compounds							
1) T	Dalapon	2.816	2.306	28847381	15200001	44.384	24.006 #
2) T	3,5-DICHL...	0.000	8.964	0	9111002	N.D.	14.756 #
5) T	DICAMBA	0.000	11.039	0	6312347	N.D.	3.778 #
6) T	MCP	11.977	11.288	77507190	629635	59.035	0.533 #
9) T	2,4-D	0.000	12.658	0	448163	N.D.	0.854 #
11) T	2,4,5-TP ...	0.000	13.806	0	1534344	N.D.	0.603 #
13) T	2,4-DB	0.000	15.029	0	3502058	N.D.	13.714 #
14) T	DINOSEB	0.000	15.444	0	2904469	N.D.	1.627 #
15) T	Picloram	16.775	16.718	9738709	7084311	3.957	2.791 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
Data File : PS003592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2019 10:13
Operator : EI\SJ
Sample : K1905-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RT-3483

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 15:34:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

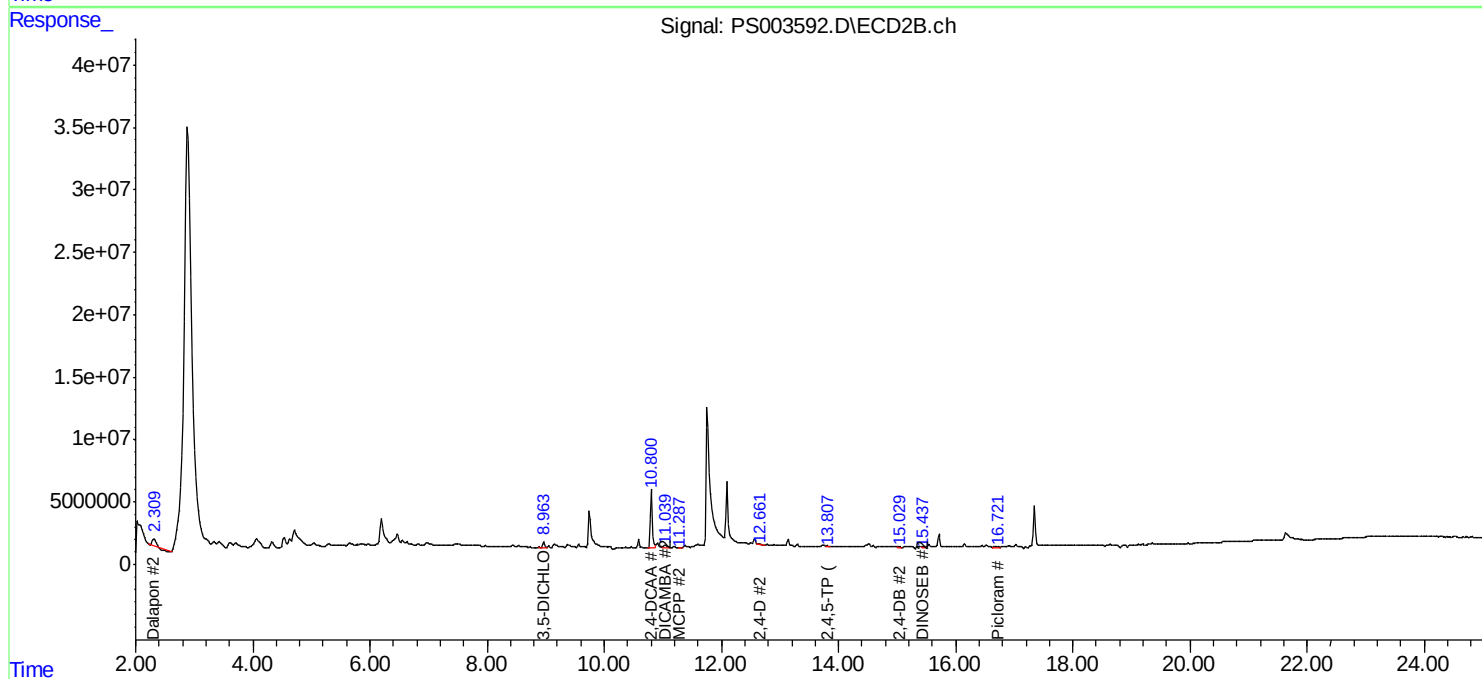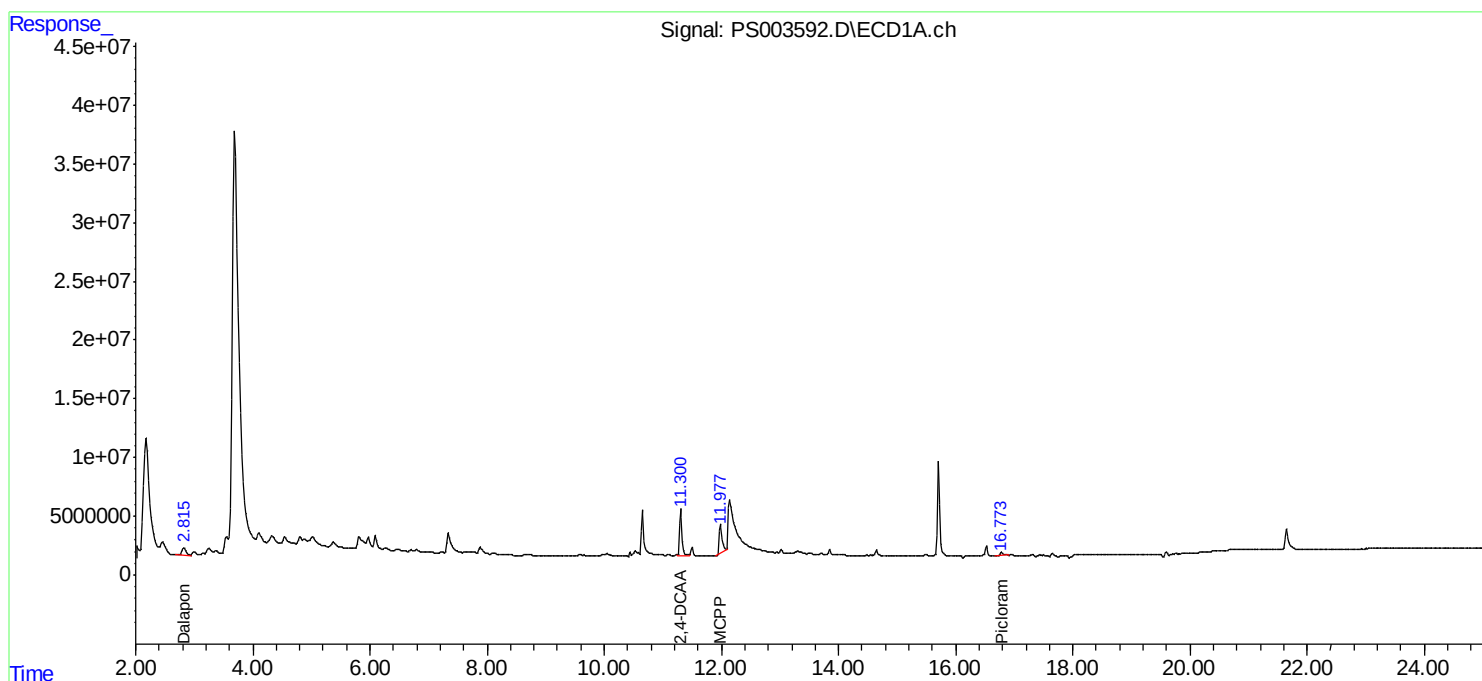


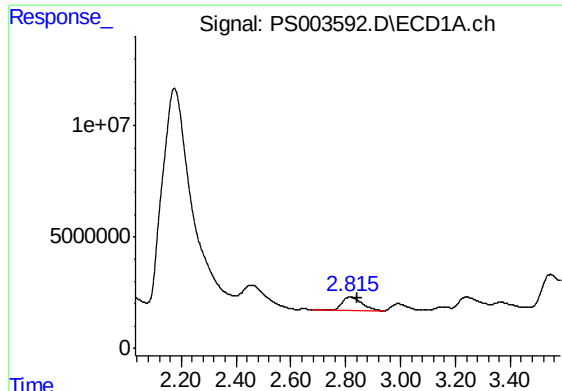

#1 Dalapon


R.T.: 2.816 min
Delta R.T.: -0.028 min
Response: 28847381
Conc: 44.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
RT-3483

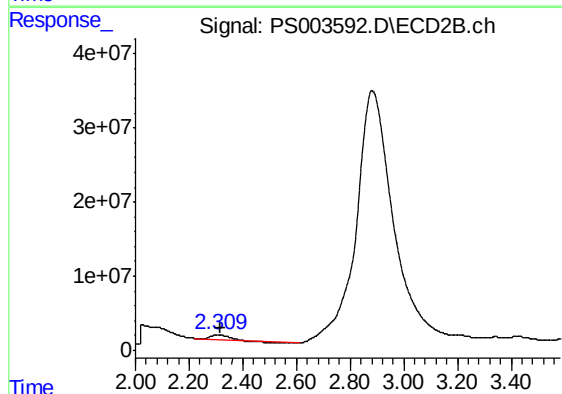


#1 Dalapon

R.T.: 2.306 min
Delta R.T.: -0.011 min
Response: 15200001
Conc: 24.01 ng/ml

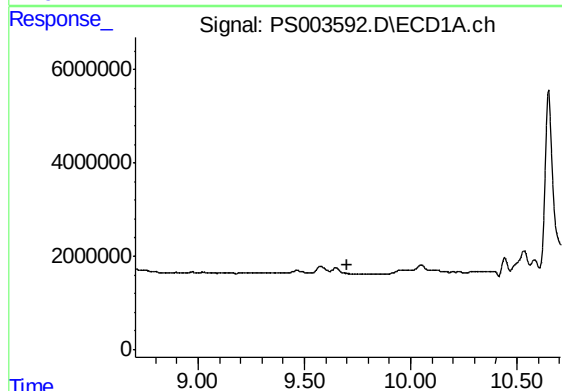


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

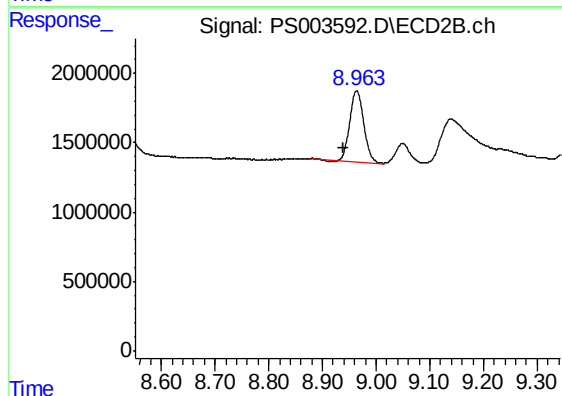

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.964 min
Delta R.T.: 0.024 min
Response: 9111002
Conc: 14.76 ng/ml

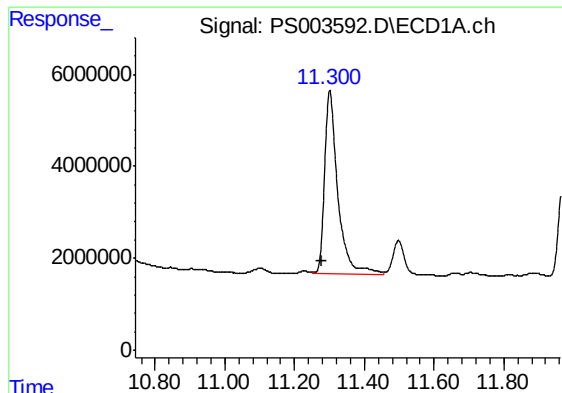

#4 2,4-DCAA


R.T.: 11.301 min
Delta R.T.: 0.023 min
Response: 105637151
Conc: 240.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
RT-3483

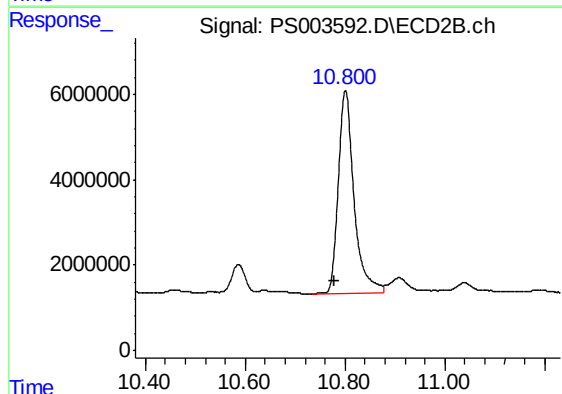


#4 2,4-DCAA

R.T.: 10.801 min
Delta R.T.: 0.021 min
Response: 104352507
Conc: 222.23 ng/ml

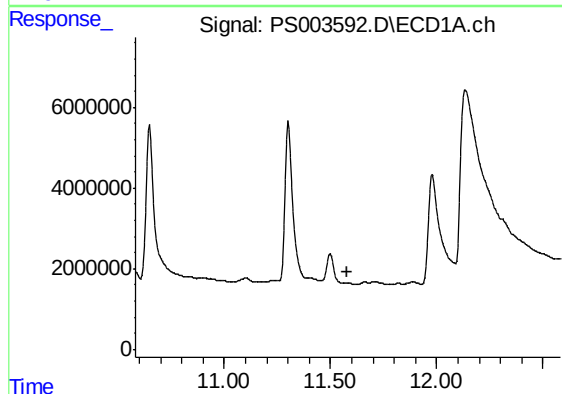


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

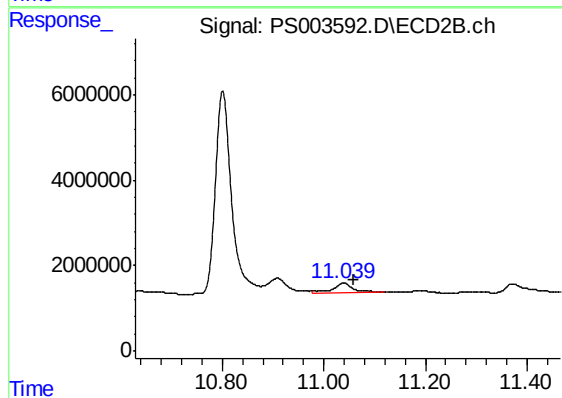

#5 DICAMBA


R.T.: 11.039 min
Delta R.T.: -0.020 min
Response: 6312347
Conc: 3.78 ng/ml

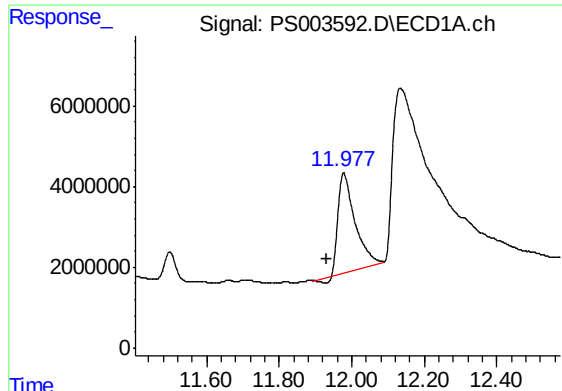

#6 MCPP


R.T.: 11.977 min
Delta R.T.: 0.047 min
Response: 77507190
Conc: 59.03 ug/ml

Instrument :
ECD_S
ClientSampleId :
RT-3483

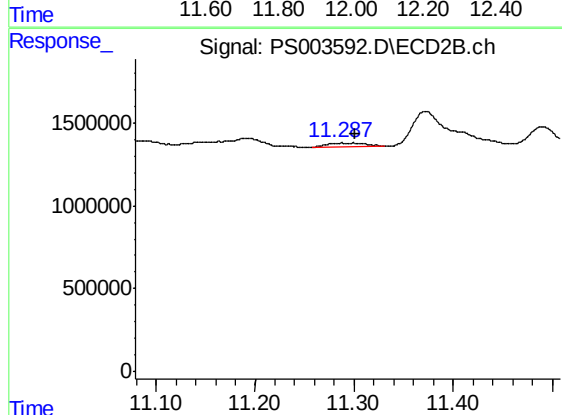


#6 MCPP

R.T.: 11.288 min
Delta R.T.: -0.013 min
Response: 629635
Conc: 0.53 ug/ml

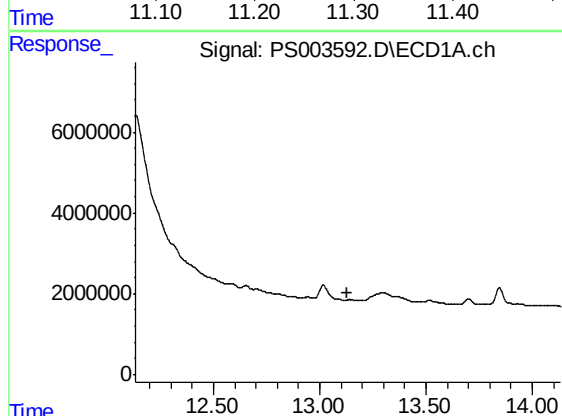


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

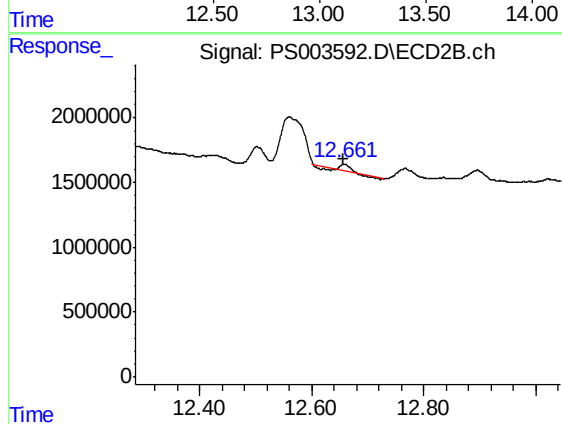

#9 2,4-D


R.T.: 12.658 min
Delta R.T.: 0.001 min
Response: 448163
Conc: 0.85 ng/ml

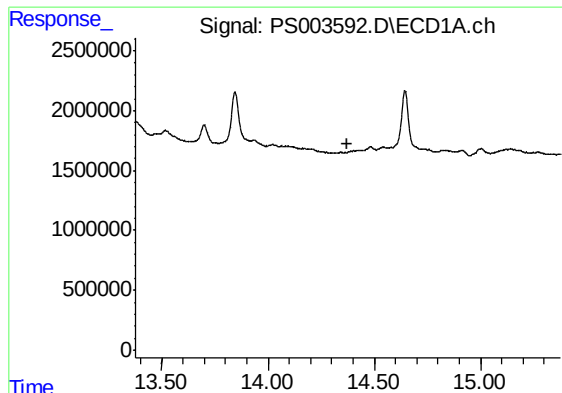

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RT-3483

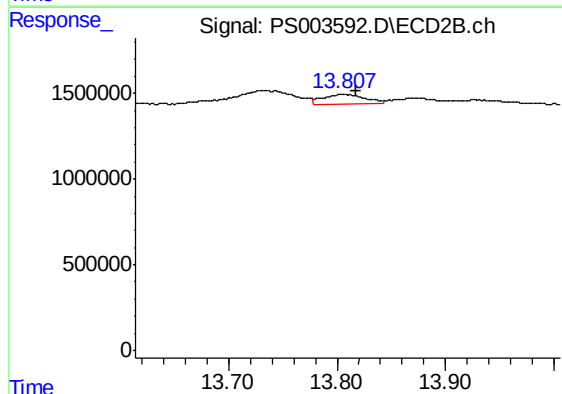


#11 2,4,5-TP (SILVEX)

R.T.: 13.806 min
Delta R.T.: -0.011 min
Response: 1534344
Conc: 0.60 ng/ml

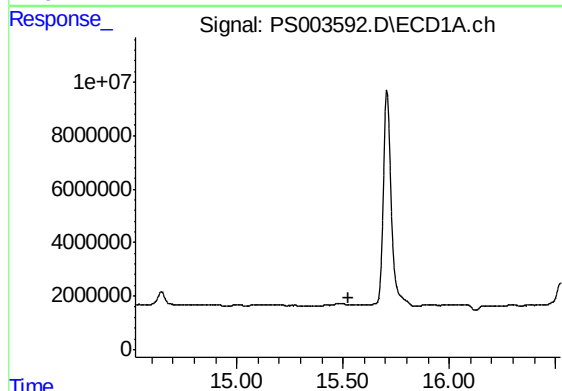


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

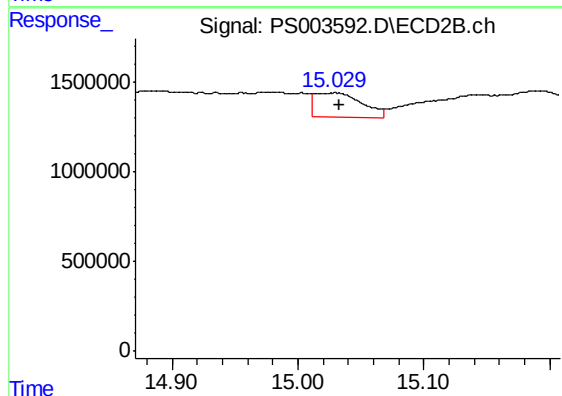

#13 2,4-DB


R.T.: 15.029 min
Delta R.T.: -0.004 min
Response: 3502058
Conc: 13.71 ng/ml

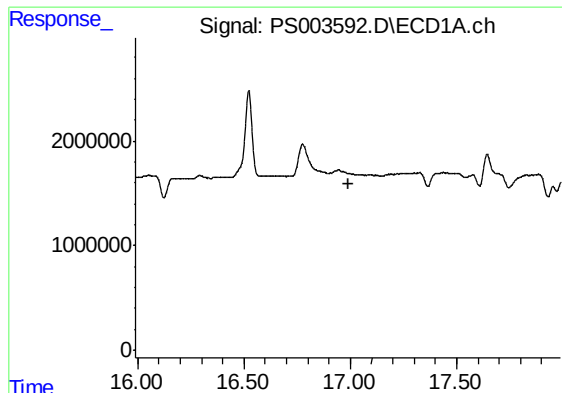

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RT-3483

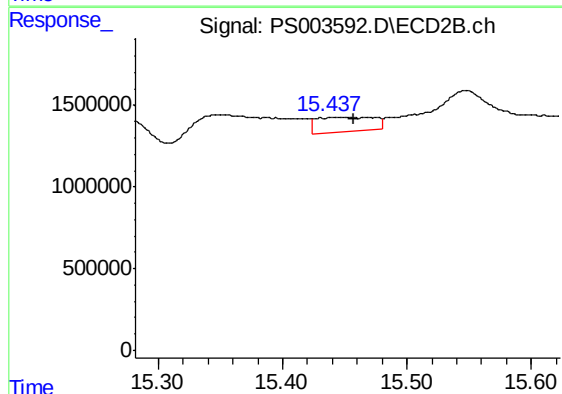


#14 DINOSEB

R.T.: 15.444 min
Delta R.T.: -0.012 min
Response: 2904469
Conc: 1.63 ng/ml

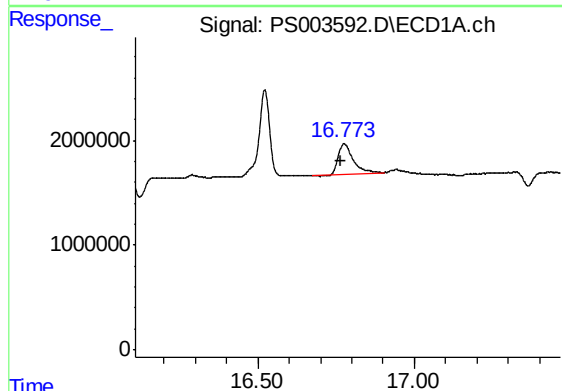

#15 Picloram

R.T.: 16.775 min
Delta R.T.: 0.010 min
Response: 9738709
Conc: 3.96 ng/ml

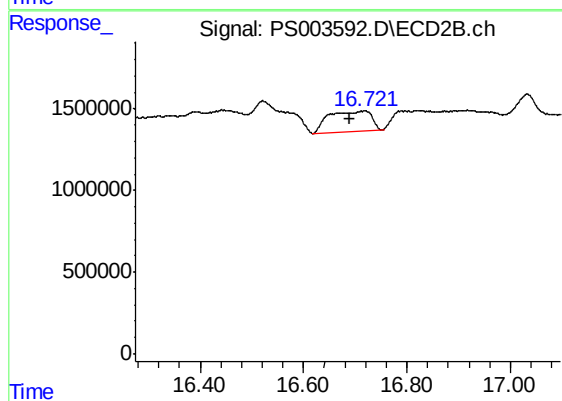

#15 Picloram

R.T.: 16.718 min
Delta R.T.: 0.030 min
Response: 7084311
Conc: 2.79 ng/ml