

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
 Data File : PS003594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2019 11:15
 Operator : EI\SJ
 Sample : K1922-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ORG-031419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 15:34:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.779	61977279	68179961	141.170	145.197
Target Compounds							
1) T	Dalapon	2.791	2.279	20147636	6837122	30.999	10.798 #
2) T	3,5-DICHL...	0.000	8.940	0	8357960	N.D.	13.536 #
5) T	DICAMBA	0.000	11.016	0	4602582	N.D.	2.755 #
6) T	MCPD	11.972	0.000	34773799	0	26.486	N.D. #
7) T	MCPA	0.000	11.741	0	56405845	N.D.	32.701 #
9) T	2,4-D	0.000	12.634	0	1112459	N.D.	2.119 #
11) T	2,4,5-TP ...	0.000	13.847	0	690206	N.D.	0.271 #
12) T	2,4,5-T	0.000	14.362	0	1906060	N.D.	0.945 #
13) T	2,4-DB	0.000	14.972	0	7535052	N.D.	29.508 #
14) T	DINOSEB	0.000	15.412	0	2795013	N.D.	1.566 #
15) T	Picloram	0.000	16.664	0	752161	N.D.	0.296 #
16) T	DCPA	0.000	16.649	0	2863554	N.D.	0.921 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
Data File : PS003594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2019 11:15
Operator : EI\SJ
Sample : K1922-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
ORG-031419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 15:34:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

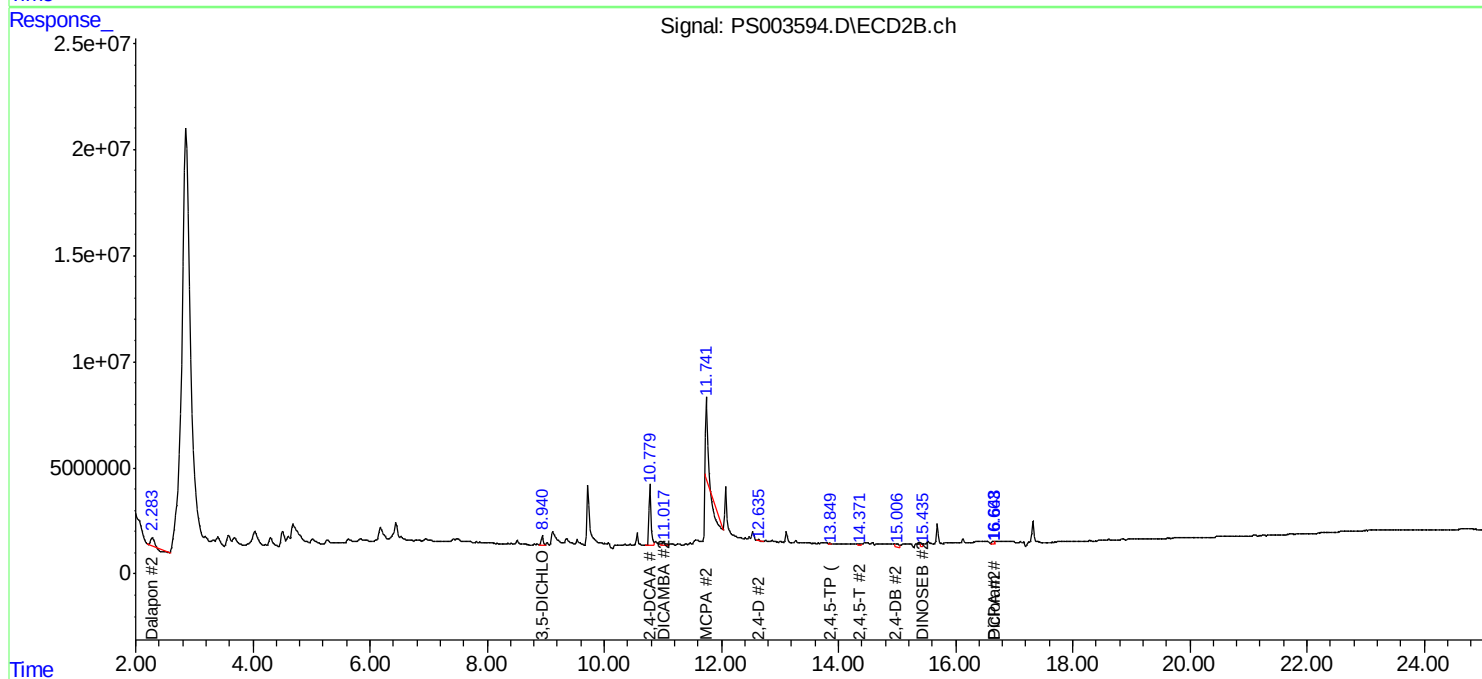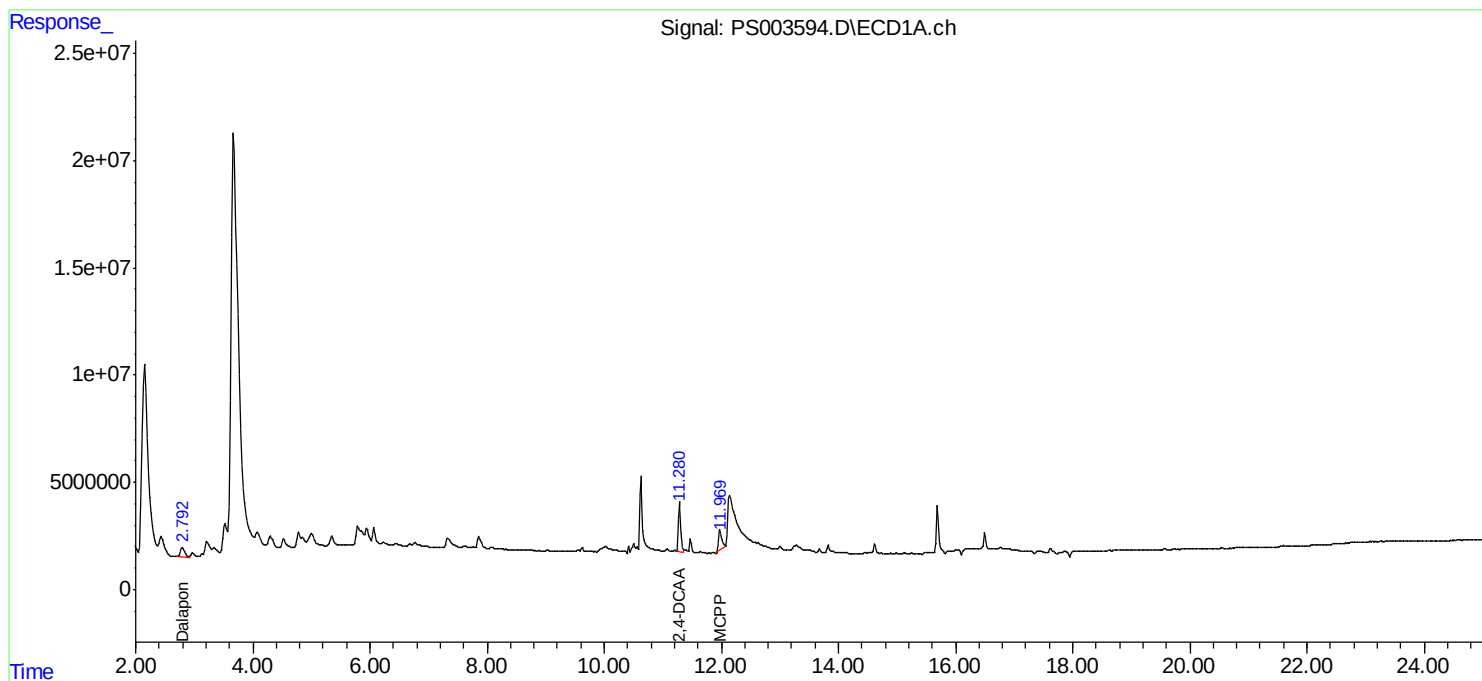


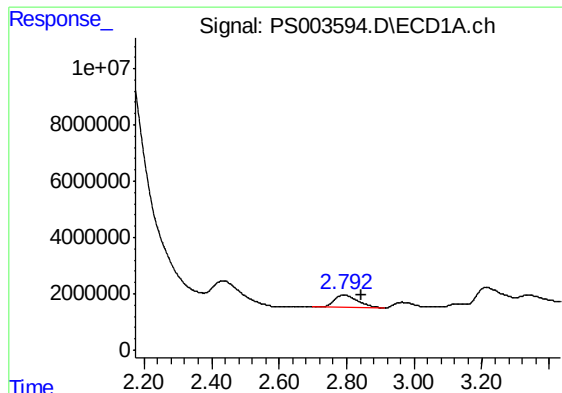

#1 Dalapon


R.T.: 2.791 min
Delta R.T.: -0.053 min
Response: 20147636
Conc: 31.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
ORG-031419

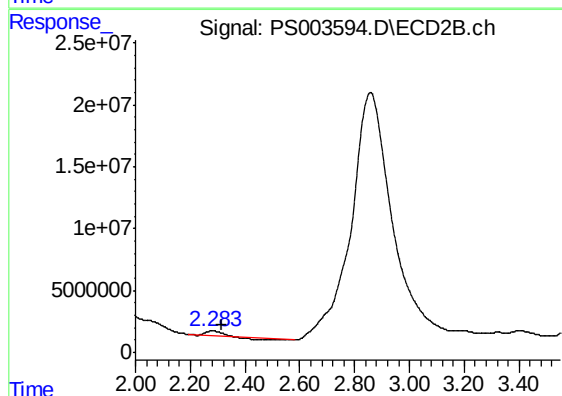


#1 Dalapon

R.T.: 2.279 min
Delta R.T.: -0.037 min
Response: 6837122
Conc: 10.80 ng/ml

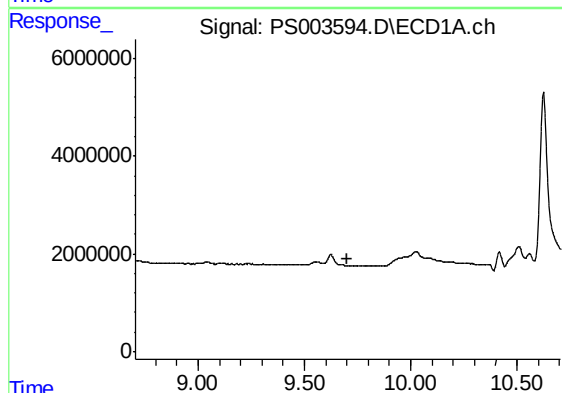


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

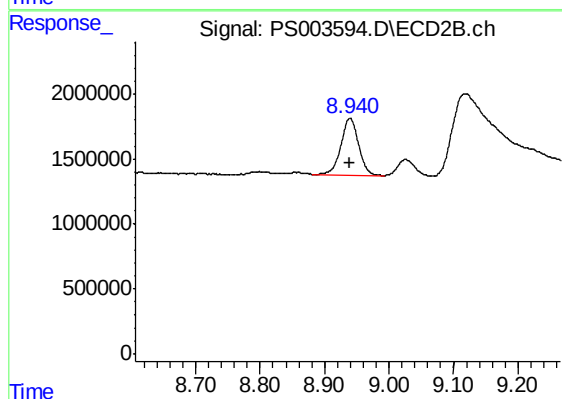

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.940 min
Delta R.T.: 0.000 min
Response: 8357960
Conc: 13.54 ng/ml

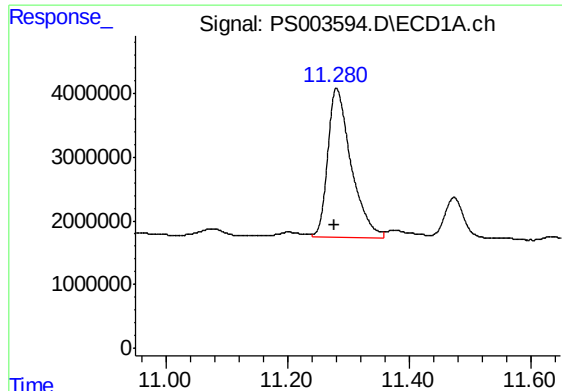

#4 2,4-DCAA


R.T.: 11.282 min
Delta R.T.: 0.004 min
Response: 61977279
Conc: 141.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
ORG-031419

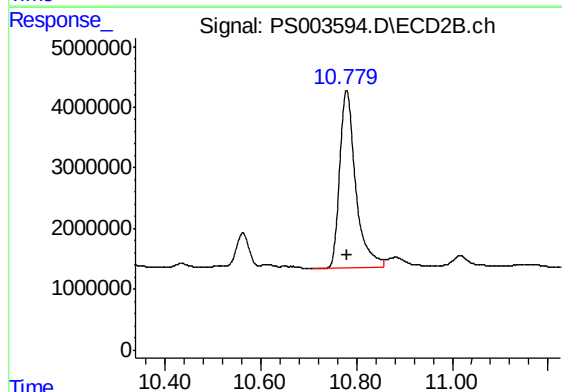


#4 2,4-DCAA

R.T.: 10.779 min
Delta R.T.: 0.000 min
Response: 68179961
Conc: 145.20 ng/ml

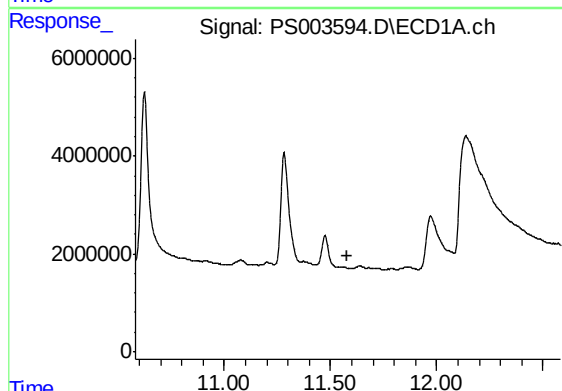


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

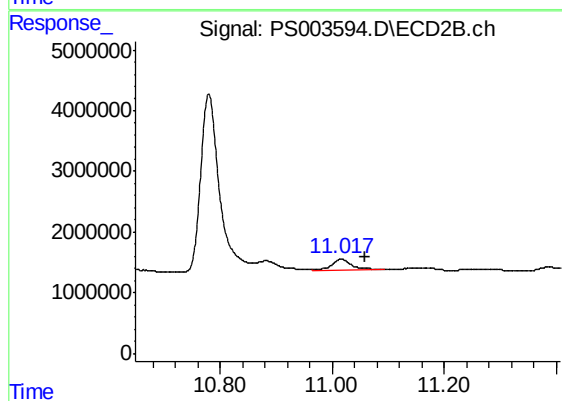

#5 DICAMBA


R.T.: 11.016 min
Delta R.T.: -0.043 min
Response: 4602582
Conc: 2.75 ng/ml

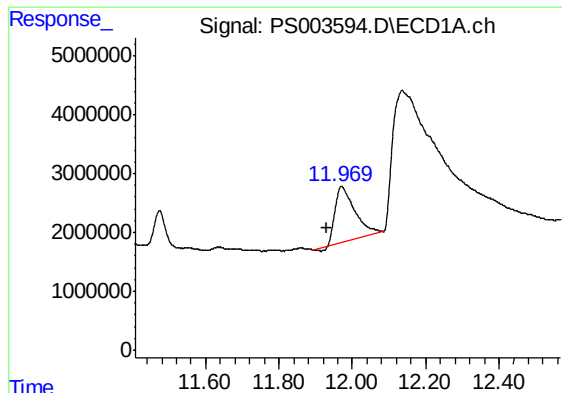

#6 MCPP


R.T.: 11.972 min
Delta R.T.: 0.041 min
Response: 34773799
Conc: 26.49 ug/ml

Instrument :
ECD_S
ClientSampleId :
ORG-031419

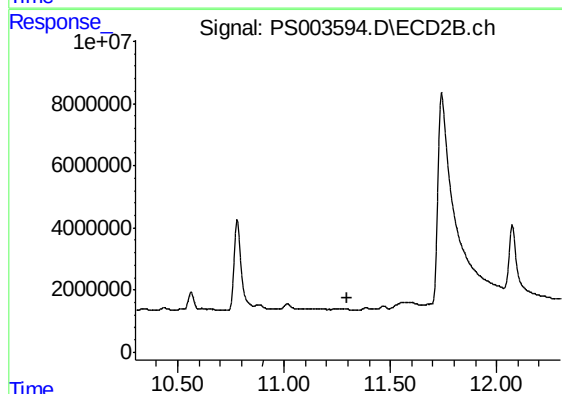


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.300 min
Response: 0
Conc: N.D.

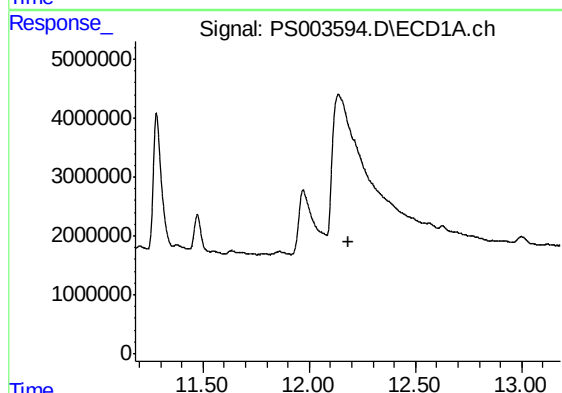


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

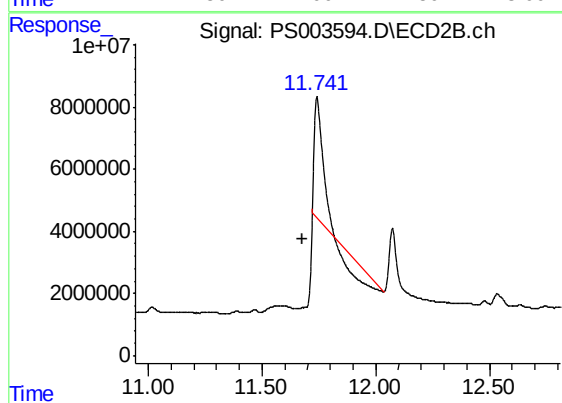

#7 MCPA


R.T.: 11.741 min
Delta R.T.: 0.063 min
Response: 56405845
Conc: 32.70 ug/ml

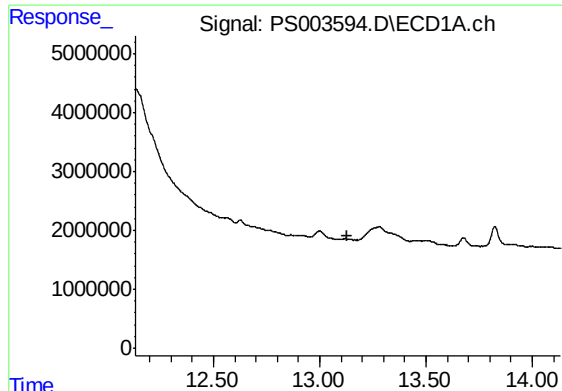

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
ORG-031419

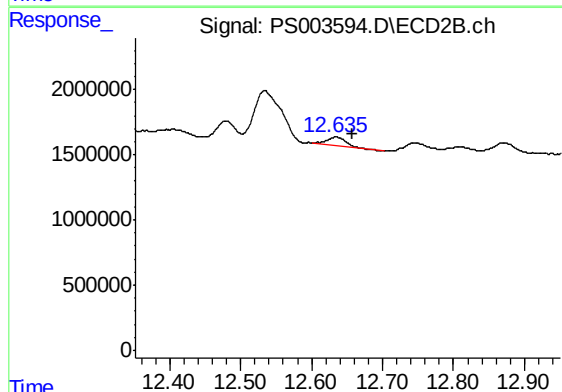


#9 2,4-D

R.T.: 12.634 min
Delta R.T.: -0.023 min
Response: 1112459
Conc: 2.12 ng/ml

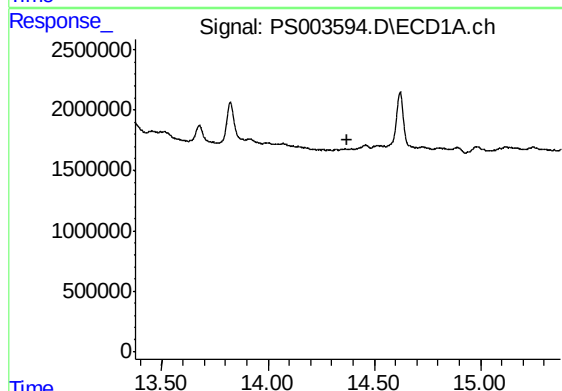


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

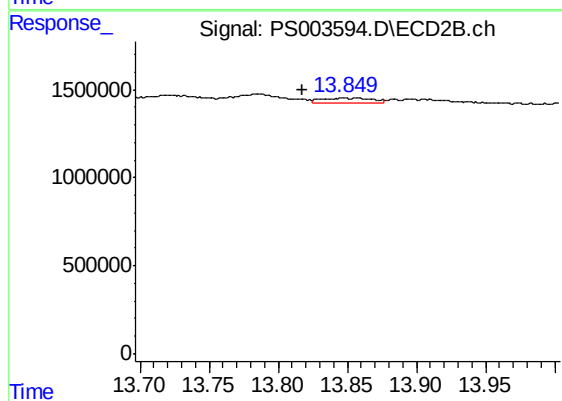

#11 2,4,5-TP (SILVEX)


R.T.: 13.847 min
Delta R.T.: 0.030 min
Response: 690206
Conc: 0.27 ng/ml

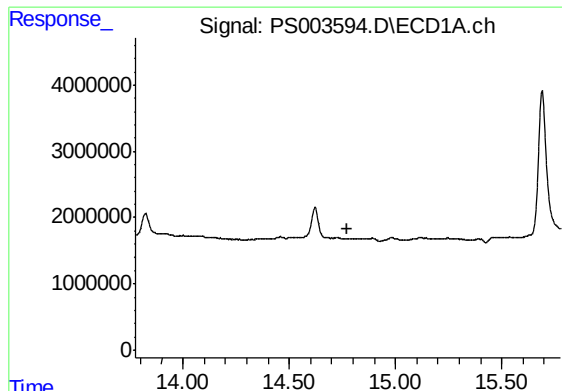

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
ORG-031419

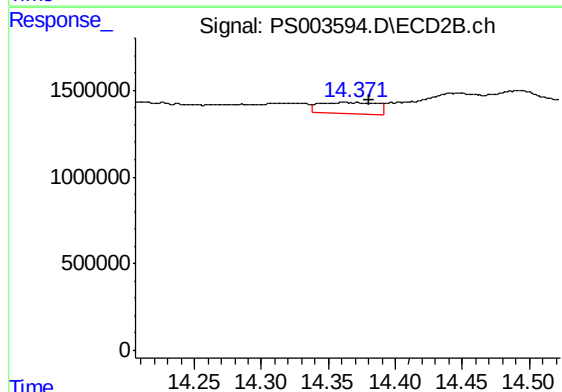


#12 2,4,5-T

R.T.: 14.362 min
Delta R.T.: -0.018 min
Response: 1906060
Conc: 0.95 ng/ml

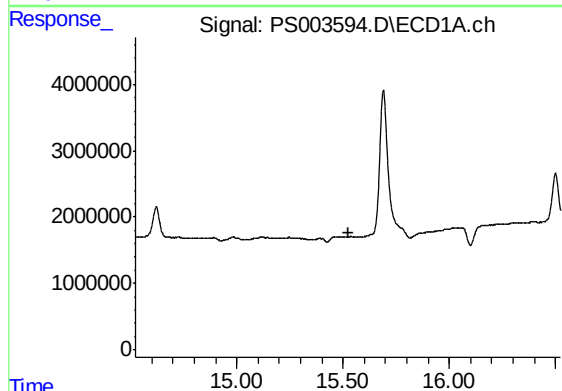


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.523 min
Response: 0
Conc: N.D.

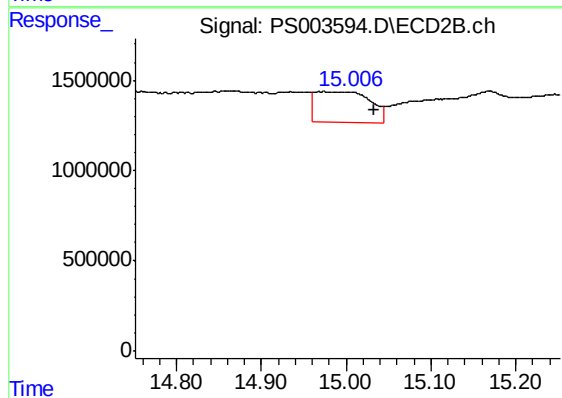

#13 2,4-DB


R.T.: 14.972 min
Delta R.T.: -0.061 min
Response: 7535052
Conc: 29.51 ng/ml

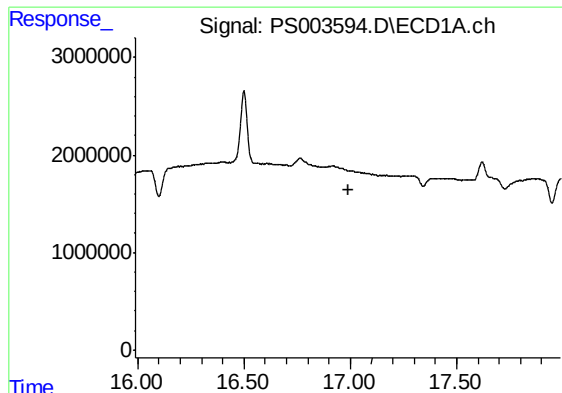

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
ORG-031419

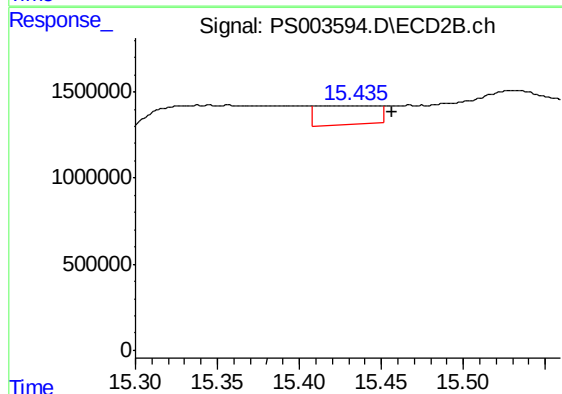


#14 DINOSEB

R.T.: 15.412 min
Delta R.T.: -0.045 min
Response: 2795013
Conc: 1.57 ng/ml

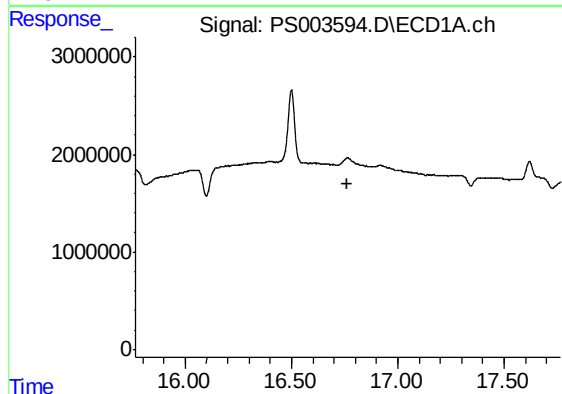


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

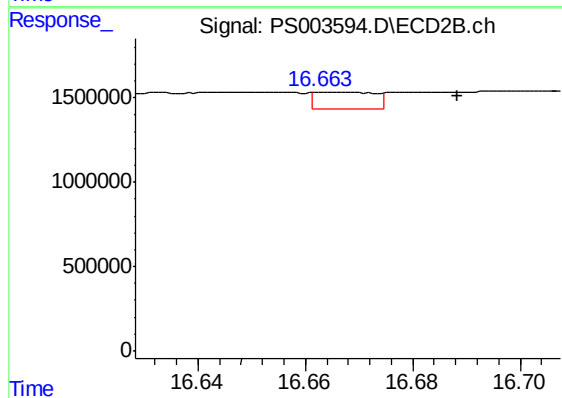

#15 Picloram


R.T.: 16.664 min
Delta R.T.: -0.024 min
Response: 752161
Conc: 0.30 ng/ml

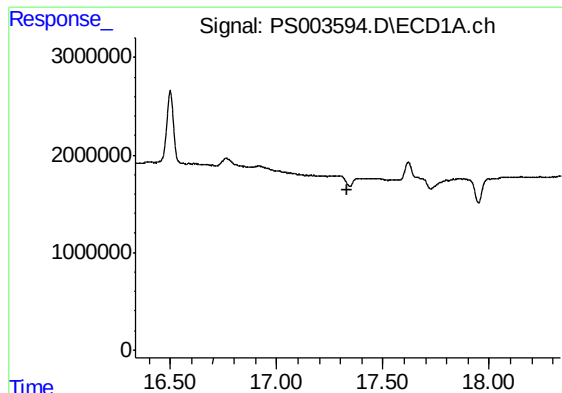

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
ORG-031419

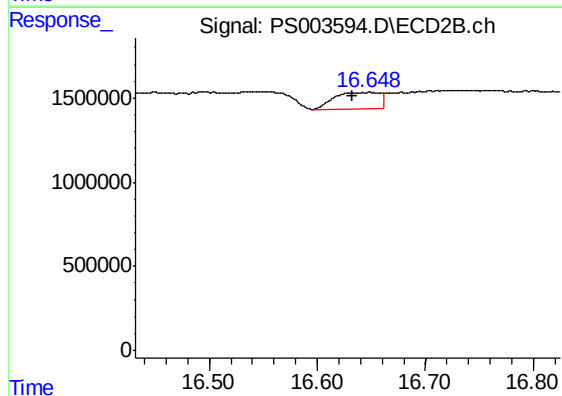

#16 DCPA

R.T.: 16.649 min
Delta R.T.: 0.017 min
Response: 2863554
Conc: 0.92 ng/ml