

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
 Data File : PS003599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2019 13:51
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 15:36:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.284	10.783	231.6E6	219.0E6	527.421	466.302
Target Compounds							
3) T	4-Nitroph...	0.000	9.936	0	139981	N.D.	0.623 #
6) T	MCP	0.000	11.350	0	16106	N.D.	0.014 #
7) T	MCPA	0.000	11.681	0	532921	N.D.	0.309 #
8) T	DICHLORPROP	0.000	12.168	0	3154242	N.D.	7.633 #
9) T	2,4-D	0.000	12.692	0	219408	N.D.	0.418 #
10) T	Pentachlo...	0.000	13.202	0	700706	N.D.	0.106 #
11) T	2,4,5-TP ...	0.000	13.797	0	785988	N.D.	0.309 #
12) T	2,4,5-T	0.000	14.378	0	69335	N.D.	0.034 #
13) T	2,4-DB	0.000	15.065	0	477494	N.D.	1.870 #
14) T	DINOSEB	0.000	15.441	0	69709	N.D.	0.039 #
15) T	Picloram	0.000	16.634	0	561180	N.D.	0.221 #
16) T	DCPA	0.000	16.634	0	561180	N.D.	0.180 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031819\
Data File : PS003599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2019 13:51
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 15:36:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

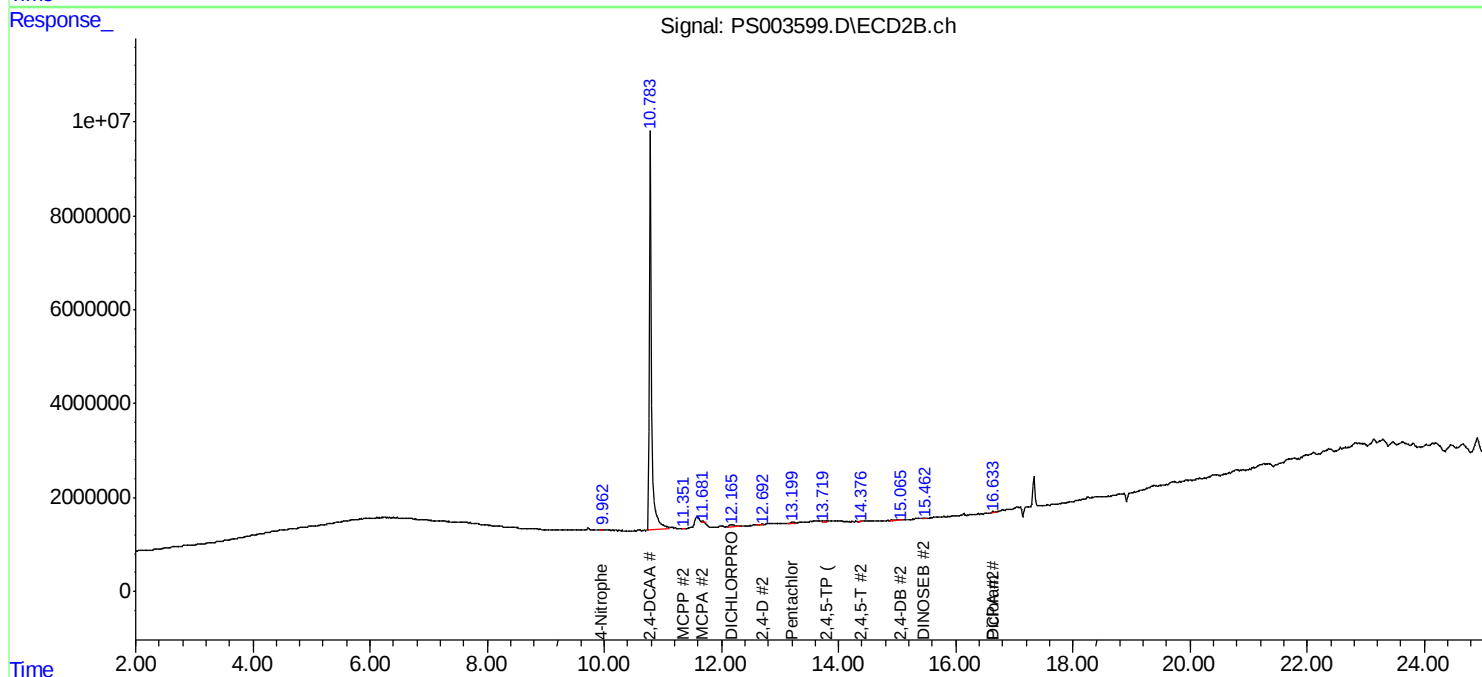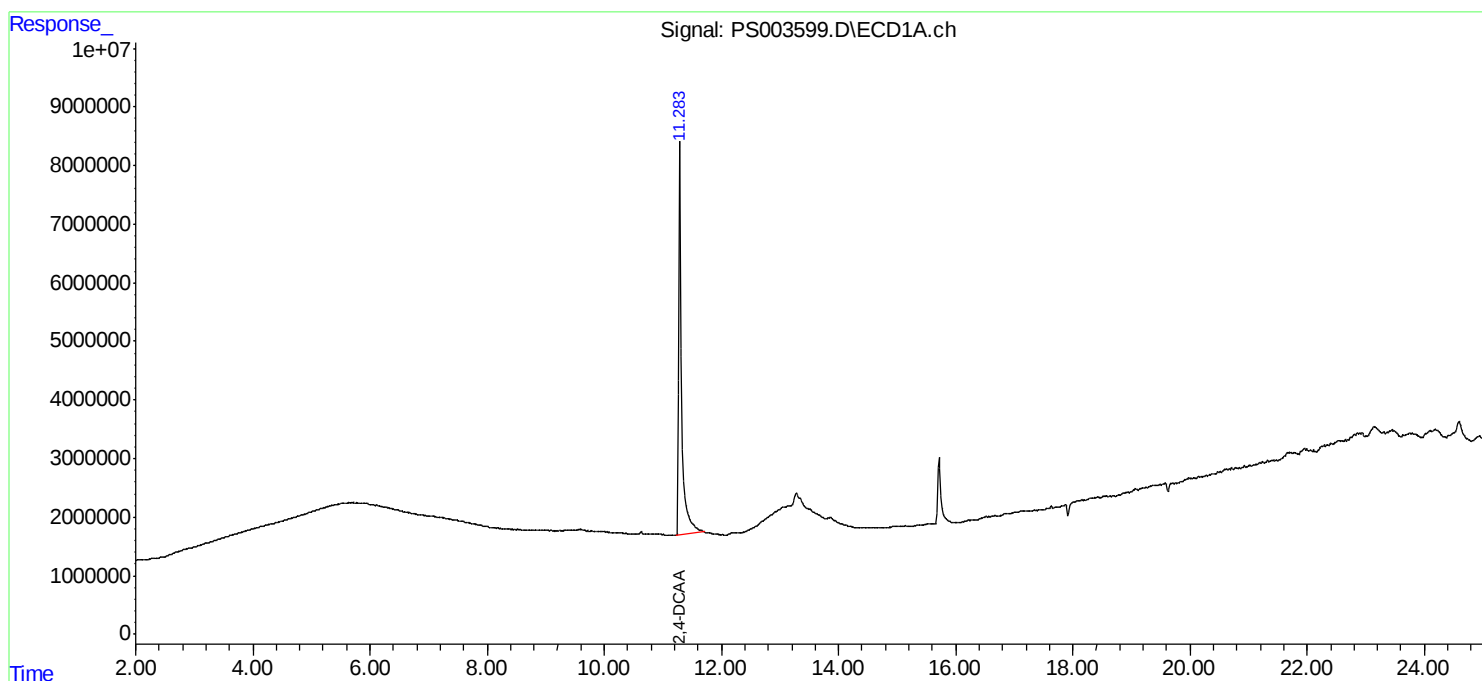


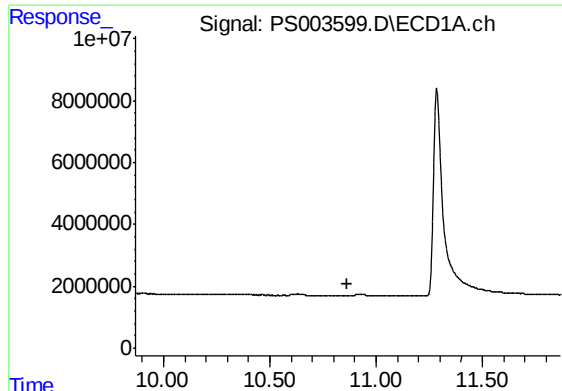

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

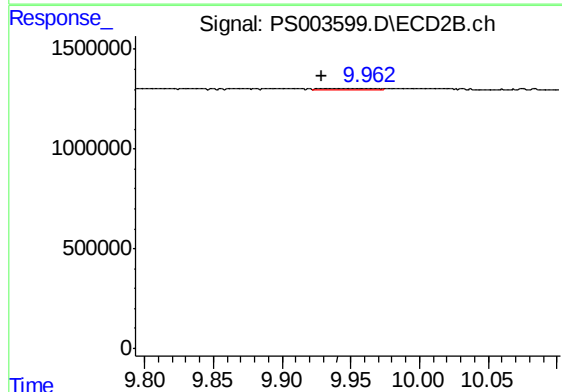


#3 4-Nitrophenol

R.T.: 9.936 min
Delta R.T.: 0.007 min
Response: 139981
Conc: 0.62 ng/ml

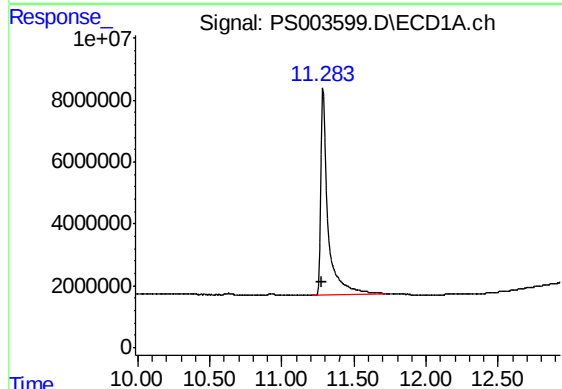


#4 2,4-DCAA

R.T.: 11.284 min
Delta R.T.: 0.007 min
Response: 231550549
Conc: 527.42 ng/ml

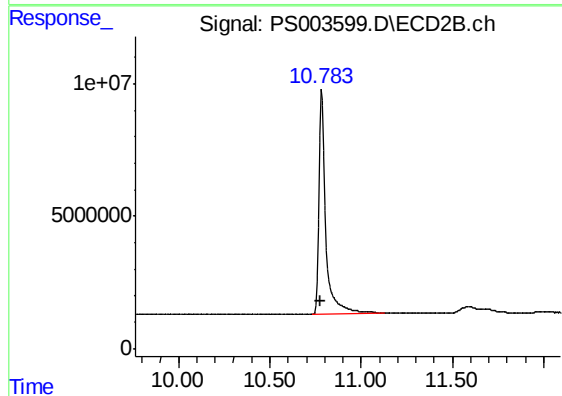

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: 0.004 min
Response: 218960904
Conc: 466.30 ng/ml

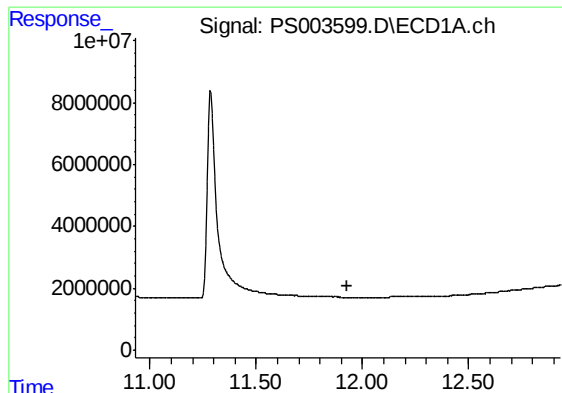

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

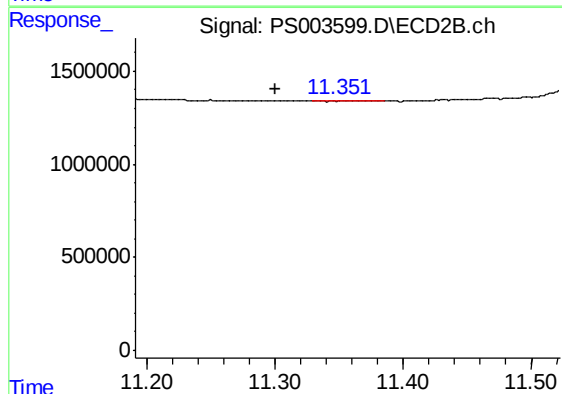


#6 MCPP

R.T.: 11.350 min
Delta R.T.: 0.050 min
Response: 16106
Conc: 0.01 ug/ml

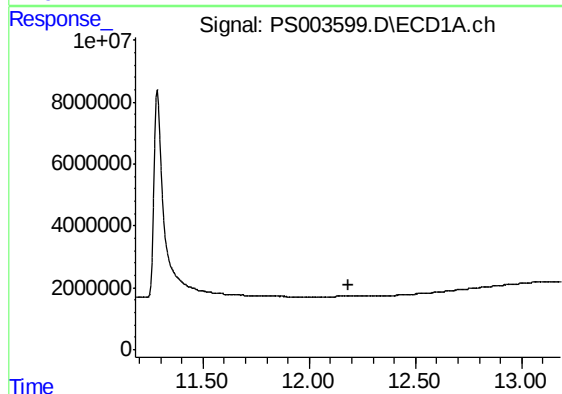


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

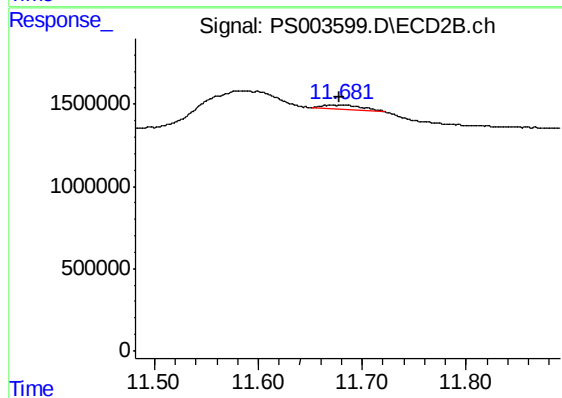

#7 MCPA


R.T.: 11.681 min
Delta R.T.: 0.003 min
Response: 532921
Conc: 0.31 ug/ml

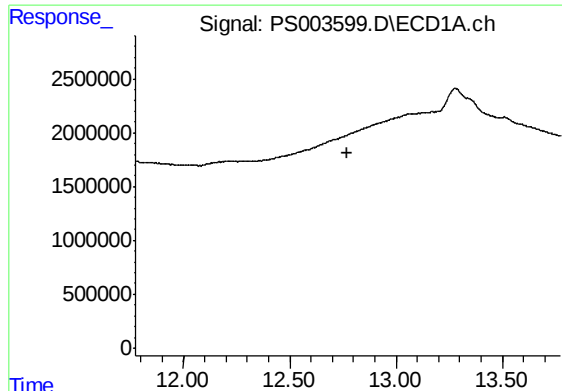

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

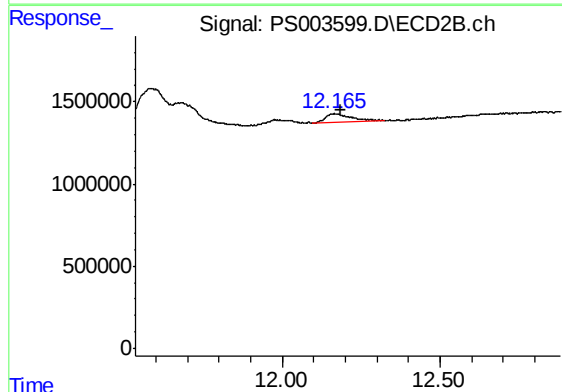


#8 DICHLORPROP

R.T.: 12.168 min
Delta R.T.: -0.017 min
Response: 3154242
Conc: 7.63 ng/ml

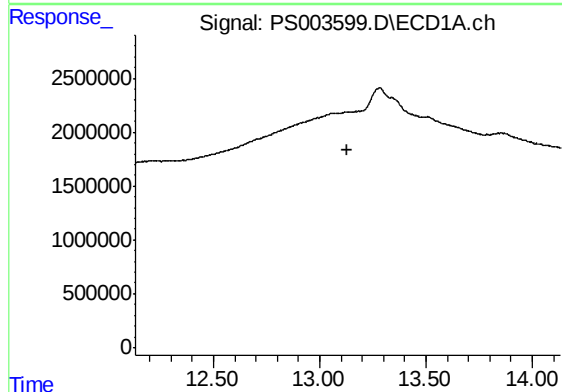


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

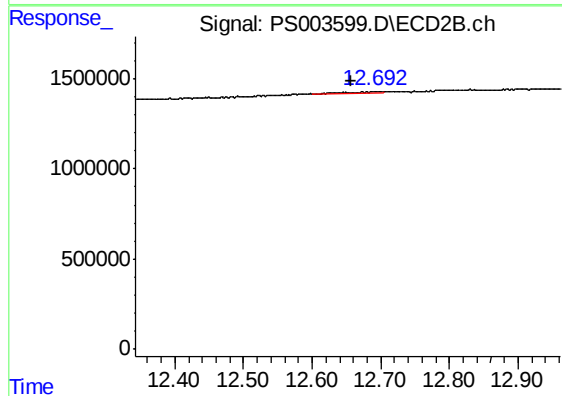

#9 2,4-D


R.T.: 12.692 min
Delta R.T.: 0.035 min
Response: 219408
Conc: 0.42 ng/ml

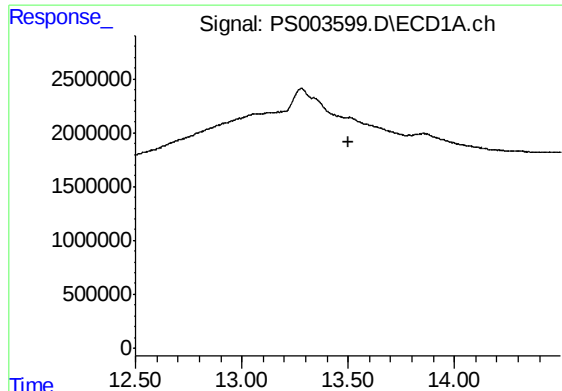

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

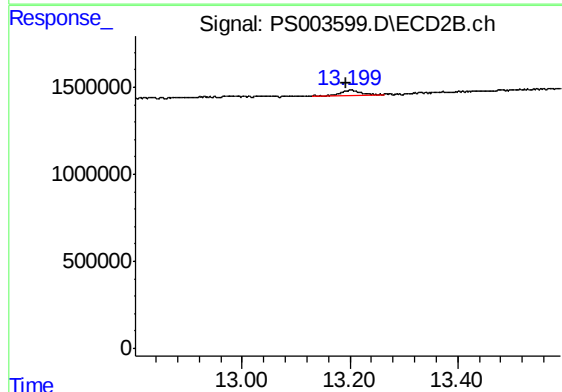


#10 Pentachlorophenol

R.T.: 13.202 min
Delta R.T.: 0.010 min
Response: 700706
Conc: 0.11 ng/ml

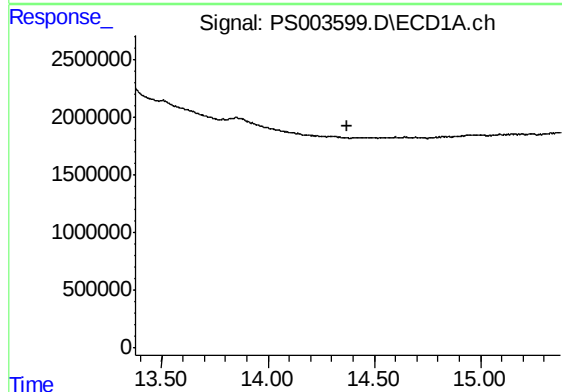


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

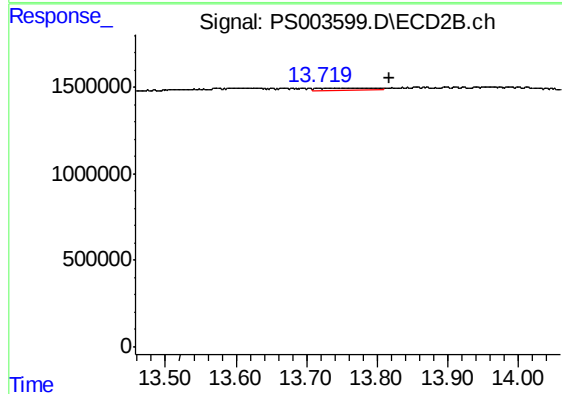

#11 2,4,5-TP (SILVEX)


R.T.: 13.797 min
Delta R.T.: -0.021 min
Response: 785988
Conc: 0.31 ng/ml

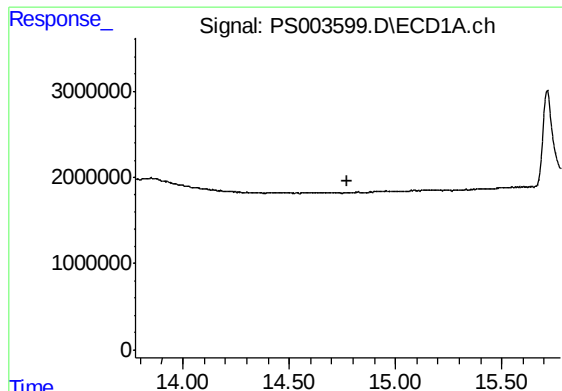

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

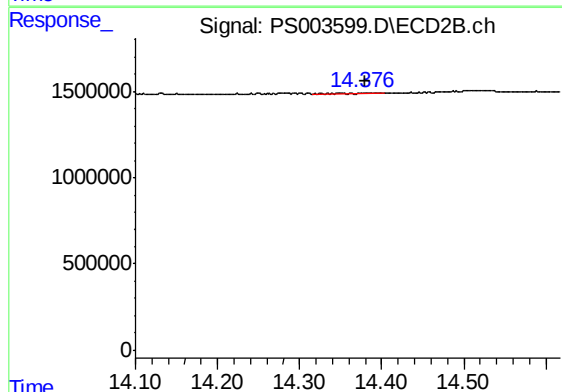


#12 2,4,5-T

R.T.: 14.378 min
Delta R.T.: -0.003 min
Response: 69335
Conc: 0.03 ng/ml

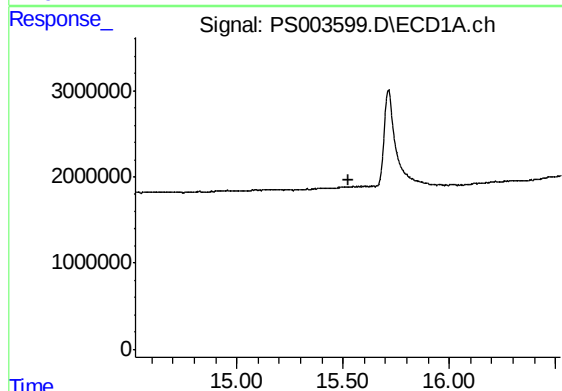


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.523 min
Response: 0
Conc: N.D.

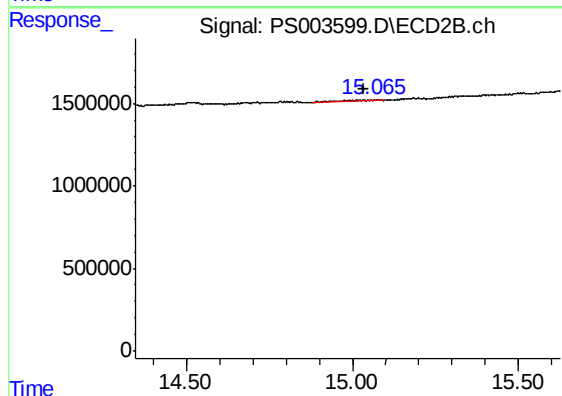

#13 2,4-DB


R.T.: 15.065 min
Delta R.T.: 0.031 min
Response: 477494
Conc: 1.87 ng/ml

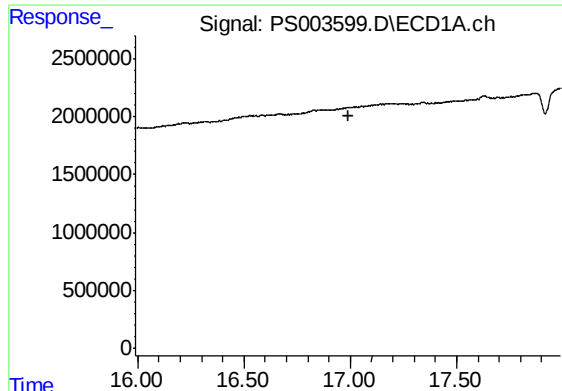

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

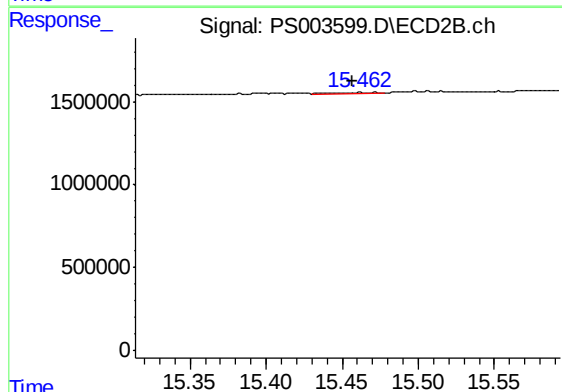


#14 DINOSEB

R.T.: 15.441 min
Delta R.T.: -0.016 min
Response: 69709
Conc: 0.04 ng/ml

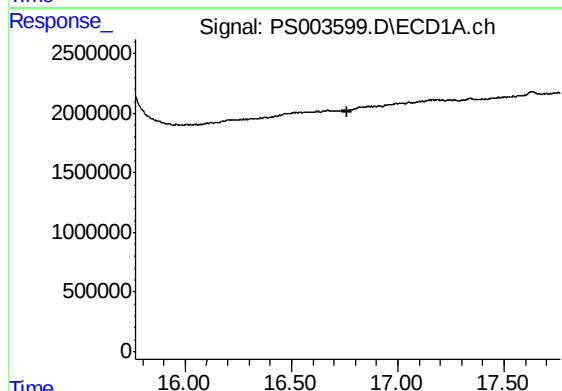


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

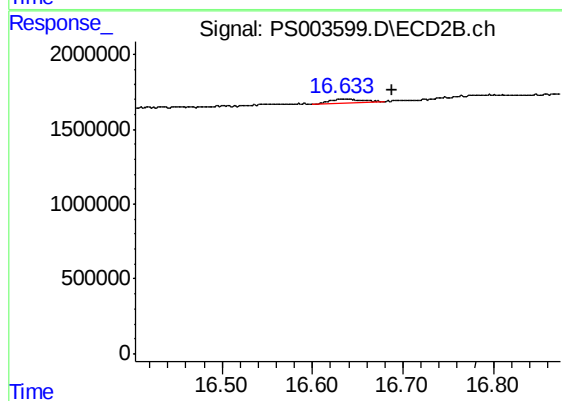

#15 Picloram


R.T.: 16.634 min
Delta R.T.: -0.055 min
Response: 561180
Conc: 0.22 ng/ml

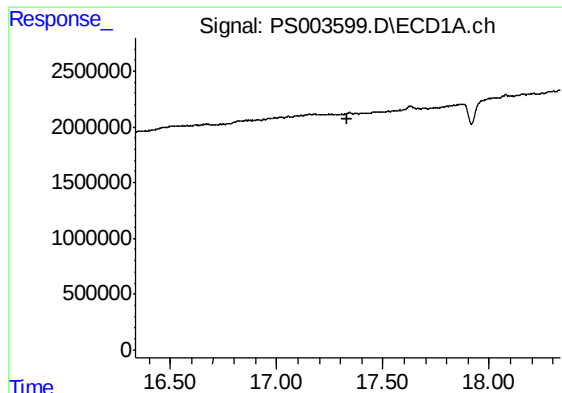

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

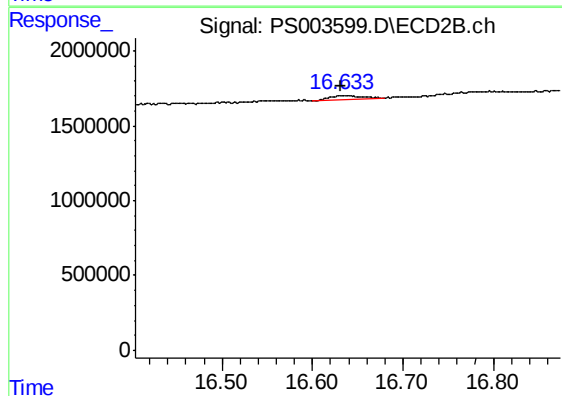

#16 DCPA

R.T.: 16.634 min
Delta R.T.: 0.002 min
Response: 561180
Conc: 0.18 ng/ml