

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031820\
 Data File : PS009351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2020 18:10
 Operator : DD\AJ
 Sample : PB127645BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 19:08:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.933	265.1E6	267.9E6	479.173	487.745
Target Compounds							
1) T	Dalapon	3.007	2.589	22531344	129.8E6	28.892	164.865 #
2) T	3,5-DICHL...	0.000	6.109	0	52734945	N.D.	64.840
5) T	DICAMBA	0.000	7.103	0	8921312	N.D.	3.886
7) T	MCPA	7.792	7.399	70829148	51461654	23.256	19.070
8) T	DICHLORPROP	0.000	7.752	0	37651806	N.D.	67.863
10) T	Pentachlo...	8.669	8.456	10234066	12530797	1.456	1.651
11) T	2,4,5-TP ...	0.000	8.785	0	35397520	N.D.	11.874
12) T	2,4,5-T	9.445	9.198	23600604	9487072	9.278	3.214 #
14) T	DINOSEB	11.187	10.042	17248354	19633198	8.438	8.938
15) T	Picloram	11.036	11.020	117.3E6	184.8E6	38.660	45.388
16) T	DCPA	11.488	10.969	4062131	13560658	1.172	3.501 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031820\
Data File : PS009351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2020 18:10
Operator : DD\AJ
Sample : PB127645BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 19:08:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

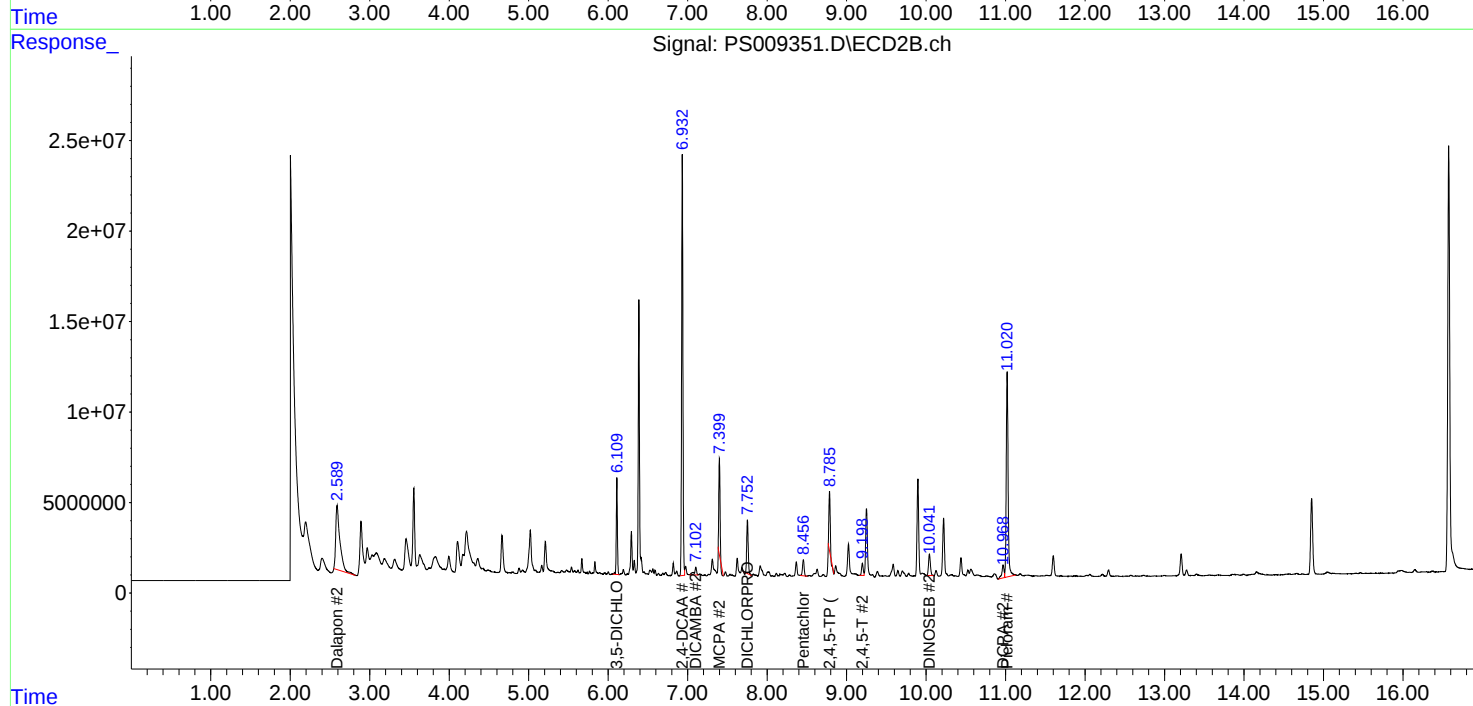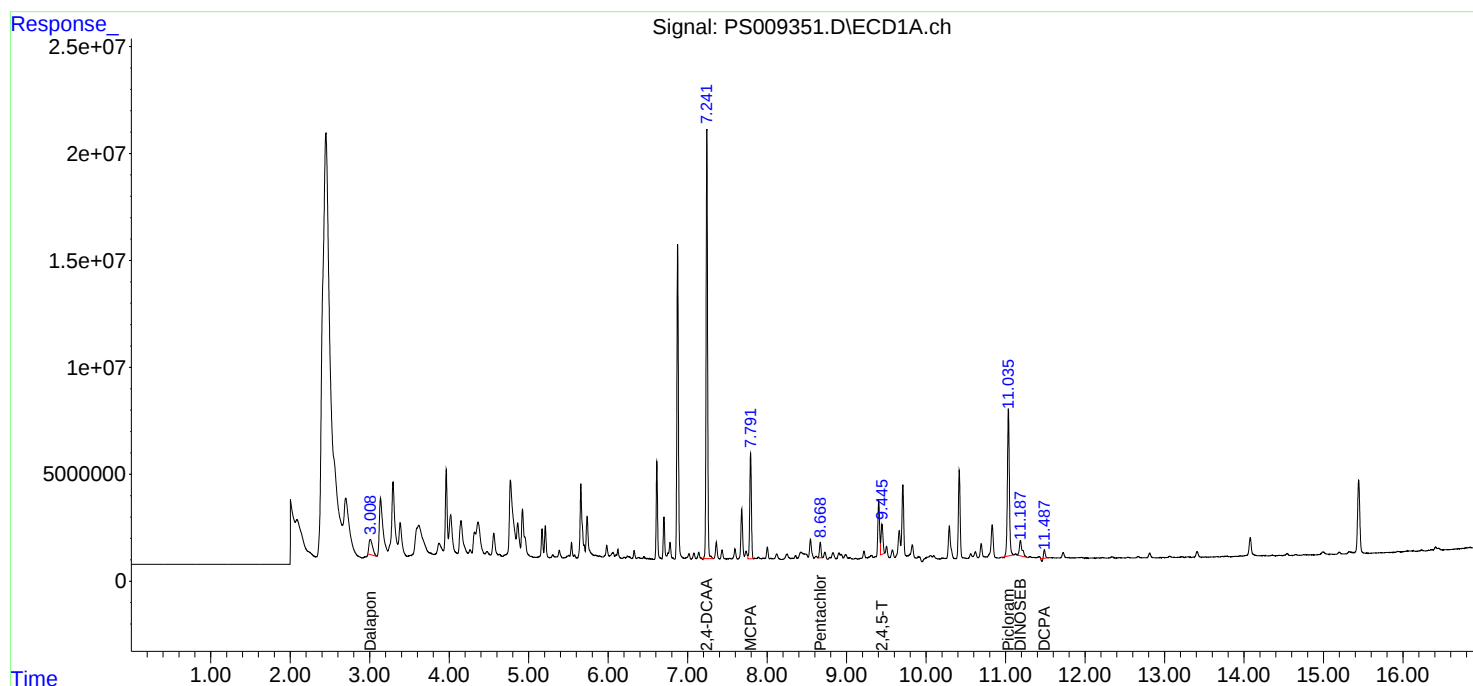


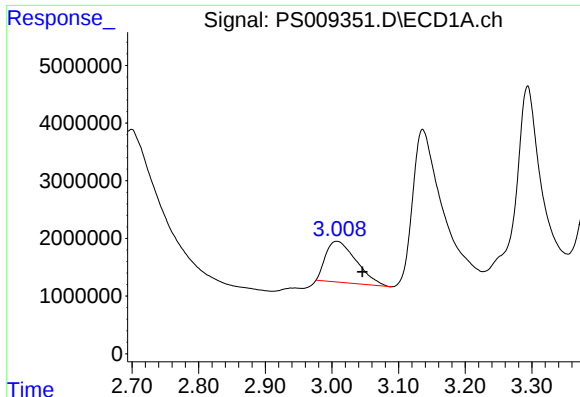

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 22531344
Conc: 28.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

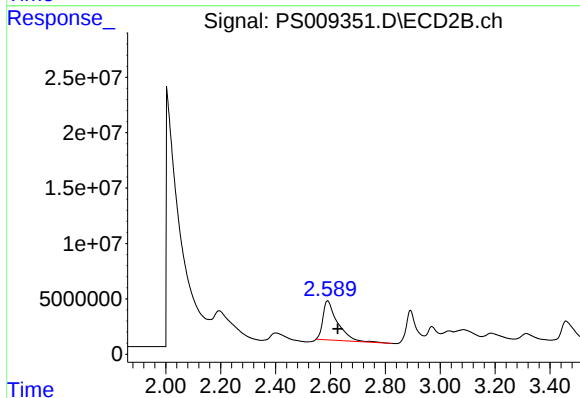


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 129808696
Conc: 164.87 ng/ml

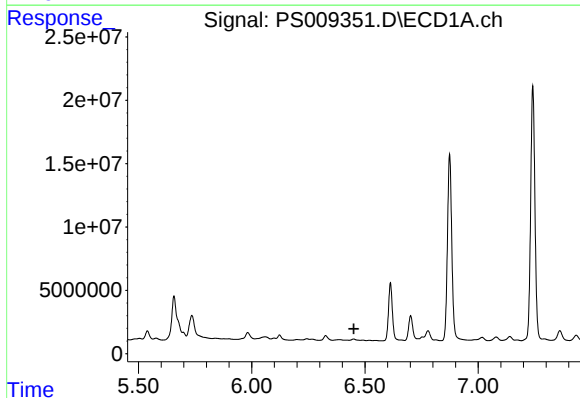


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

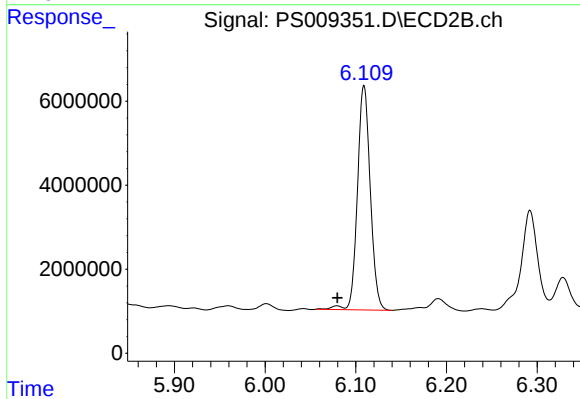

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.029 min
Response: 52734945
Conc: 64.84 ng/ml

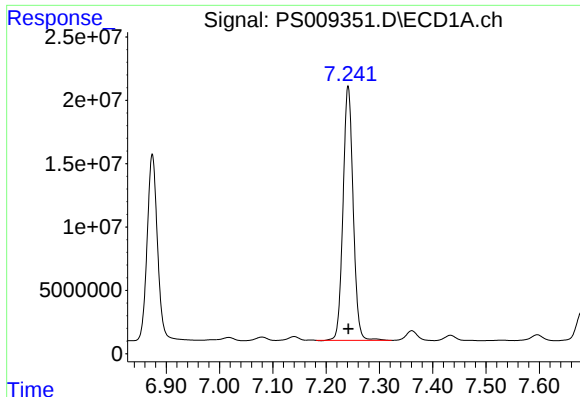

#4 2,4-DCAA


R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 265064109
Conc: 479.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

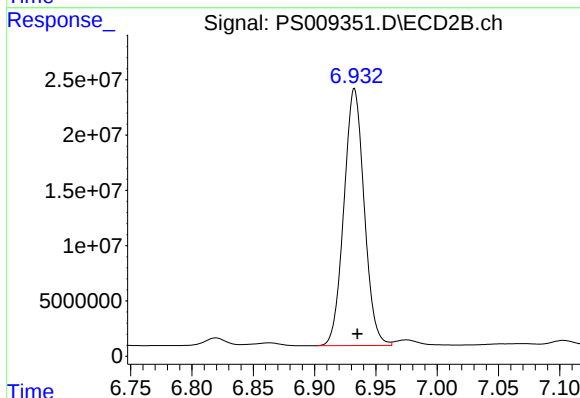


#4 2,4-DCAA

R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 267868395
Conc: 487.74 ng/ml

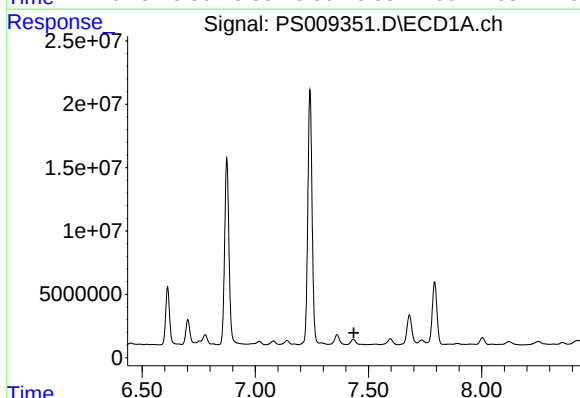


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.435 min
Response: 0
Conc: N.D.

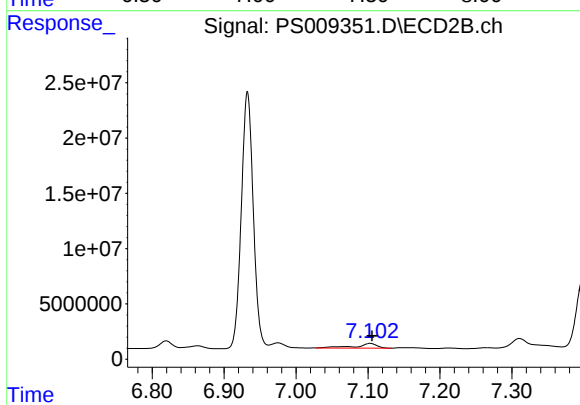

#5 DICAMBA


R.T.: 7.103 min
Delta R.T.: -0.003 min
Response: 8921312
Conc: 3.89 ng/ml

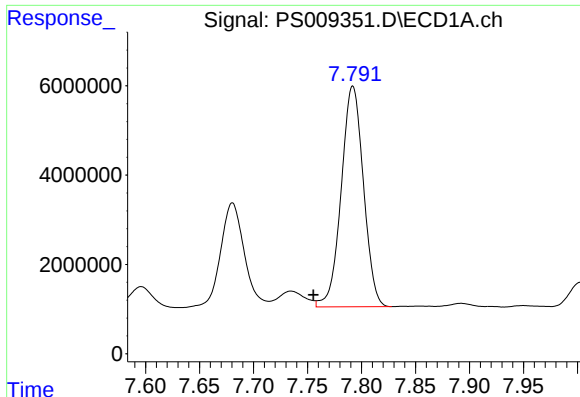

#7 MCPA


R.T.: 7.792 min
Delta R.T.: 0.036 min
Response: 70829148
Conc: 23.26 ug/ml

Instrument :
ECD_S
ClientSampleId :

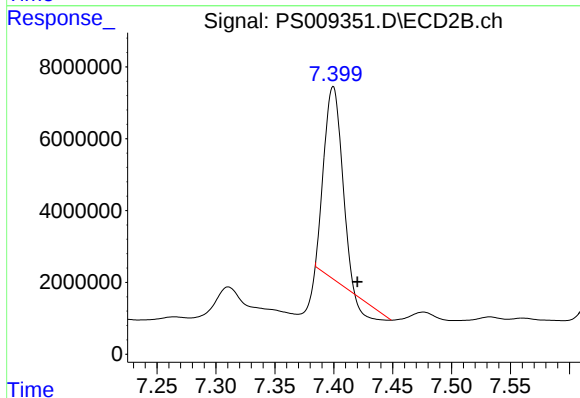


#7 MCPA

R.T.: 7.399 min
Delta R.T.: -0.021 min
Response: 51461654
Conc: 19.07 ug/ml

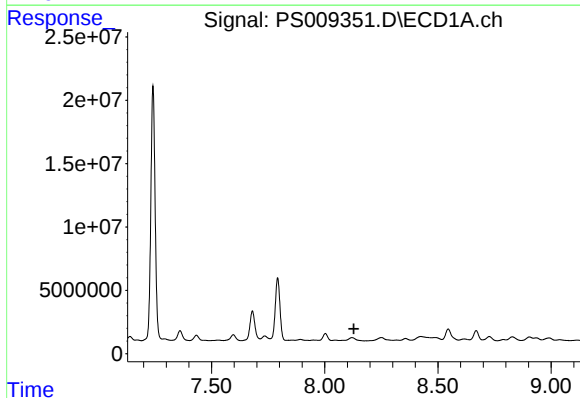


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

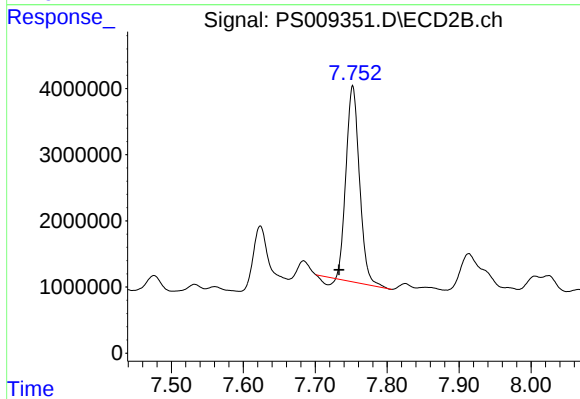

#8 DICHLORPROP


R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 37651806
Conc: 67.86 ng/ml

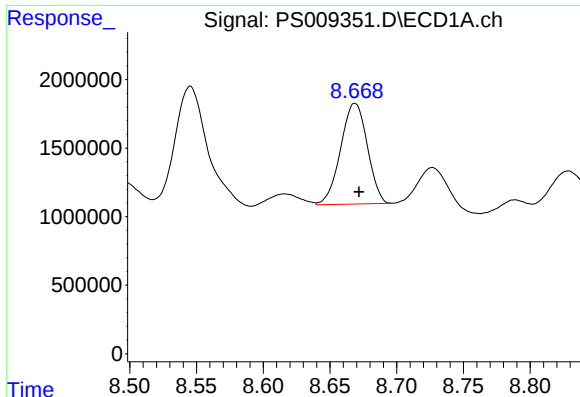

#10 Pentachlorophenol


R.T.: 8.669 min
Delta R.T.: -0.003 min
Response: 10234066
Conc: 1.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

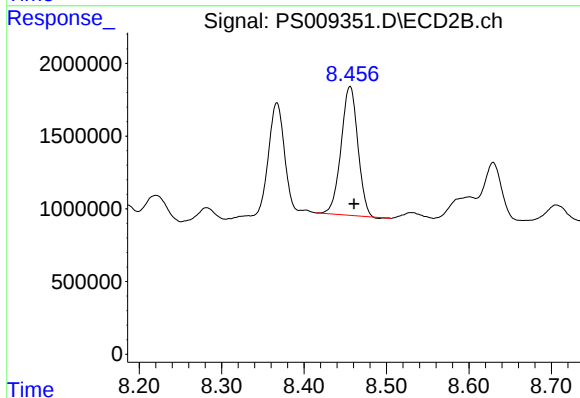


#10 Pentachlorophenol

R.T.: 8.456 min
Delta R.T.: -0.005 min
Response: 12530797
Conc: 1.65 ng/ml

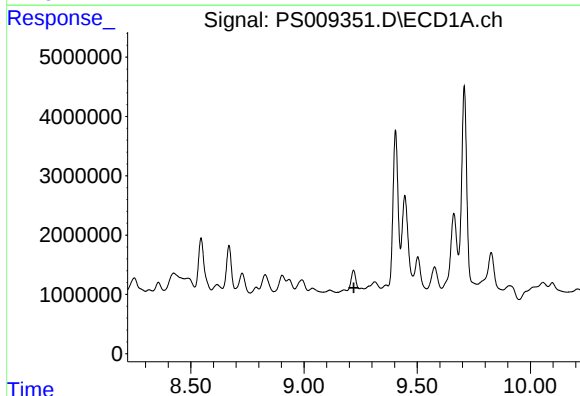


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.221 min
Response: 0
Conc: N.D.

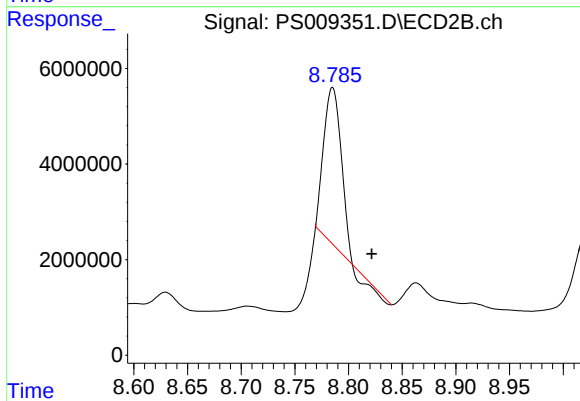

#11 2,4,5-TP (SILVEX)


R.T.: 8.785 min
Delta R.T.: -0.036 min
Response: 35397520
Conc: 11.87 ng/ml

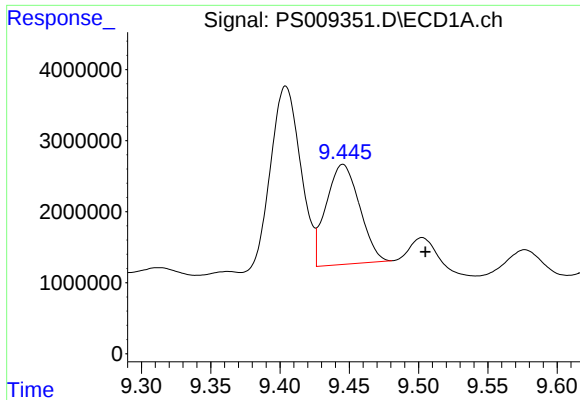

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 23600604
Conc: 9.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

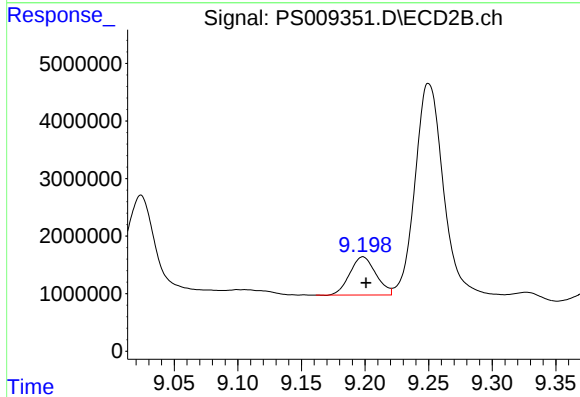


#12 2,4,5-T

R.T.: 9.198 min
Delta R.T.: -0.002 min
Response: 9487072
Conc: 3.21 ng/ml

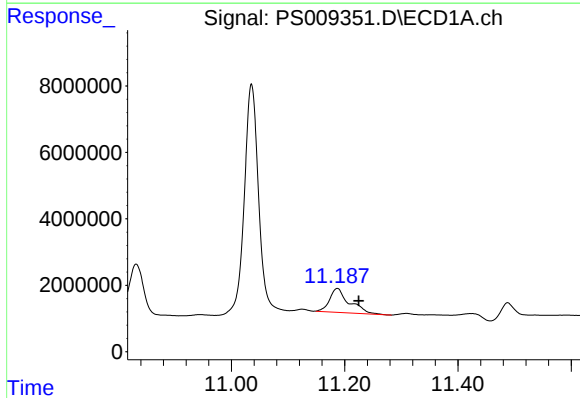


#14 DINOSEB

R.T.: 11.187 min
Delta R.T.: -0.038 min
Response: 17248354
Conc: 8.44 ng/ml

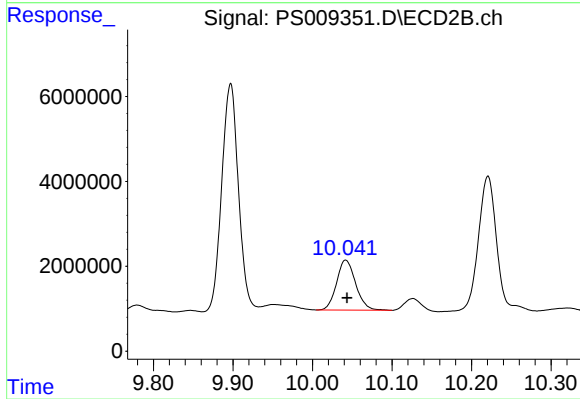

#14 DINOSEB


R.T.: 10.042 min
Delta R.T.: -0.002 min
Response: 19633198
Conc: 8.94 ng/ml

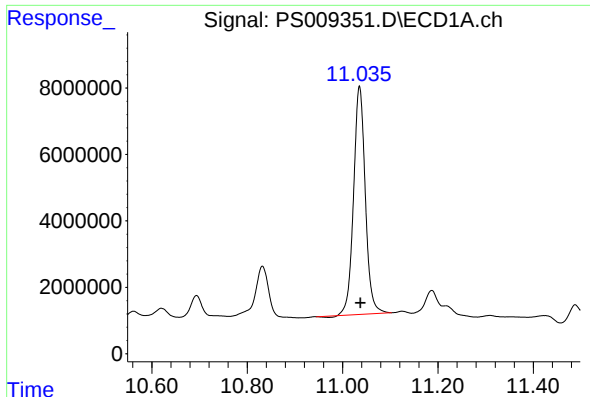

#15 Picloram


R.T.: 11.036 min
Delta R.T.: -0.002 min
Response: 117329427
Conc: 38.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

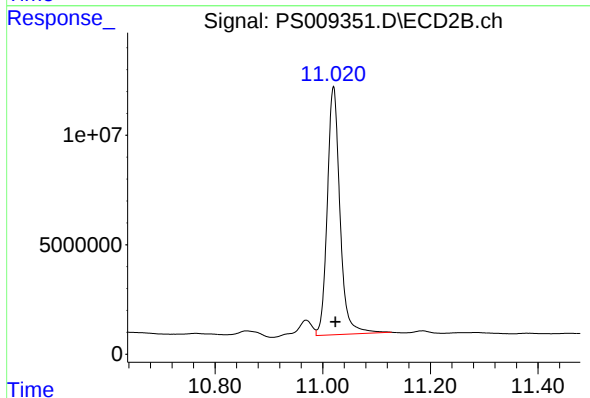


#15 Picloram

R.T.: 11.020 min
Delta R.T.: -0.003 min
Response: 184827145
Conc: 45.39 ng/ml

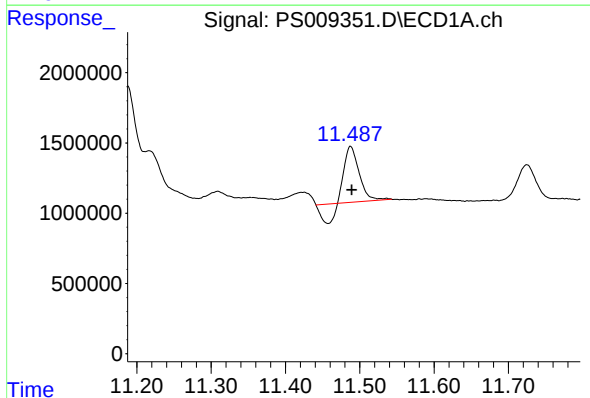

#16 DCPA

R.T.: 11.488 min
Delta R.T.: -0.001 min
Response: 4062131
Conc: 1.17 ng/ml

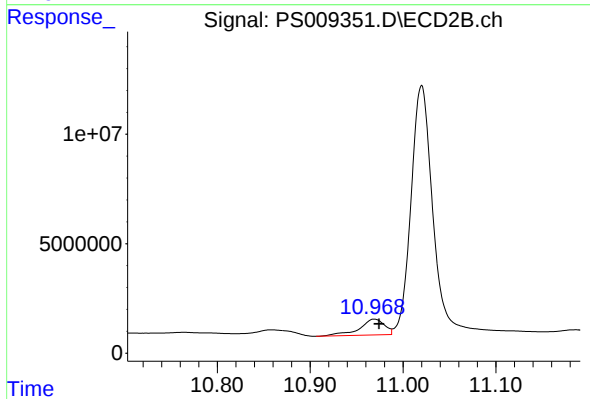

#16 DCPA

R.T.: 10.969 min
Delta R.T.: -0.005 min
Response: 13560658
Conc: 3.50 ng/ml