

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031820\
 Data File : PS009353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2020 18:55
 Operator : DD\AJ
 Sample : PB127645TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:08:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.933	150.3E6	142.1E6	271.722	258.769
Target Compounds							
1) T	Dalapon	3.007	2.591	21936019	115.0E6	28.129	146.073 #
2) T	3,5-DICHL...	0.000	6.109	0	51323618	N.D.	63.105
8) T	DICHLORPROP	0.000	7.752	0	47355032	N.D.	85.352
10) T	Pentachlo...	0.000	8.456	0	7852513	N.D.	1.035
12) T	2,4,5-T	9.444	0.000	57634575	0	22.656	N.D. #
14) T	DINOSEB	11.188	10.086	14841125	35437356	7.260	16.134 #
15) T	Picloram	11.014	11.022	15367243	9283356	5.063	2.280 #
16) T	DCPA	0.000	11.022	0	9283356	N.D.	2.397



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031820\
Data File : PS009353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2020 18:55
Operator : DD\AJ
Sample : PB127645TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:08:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

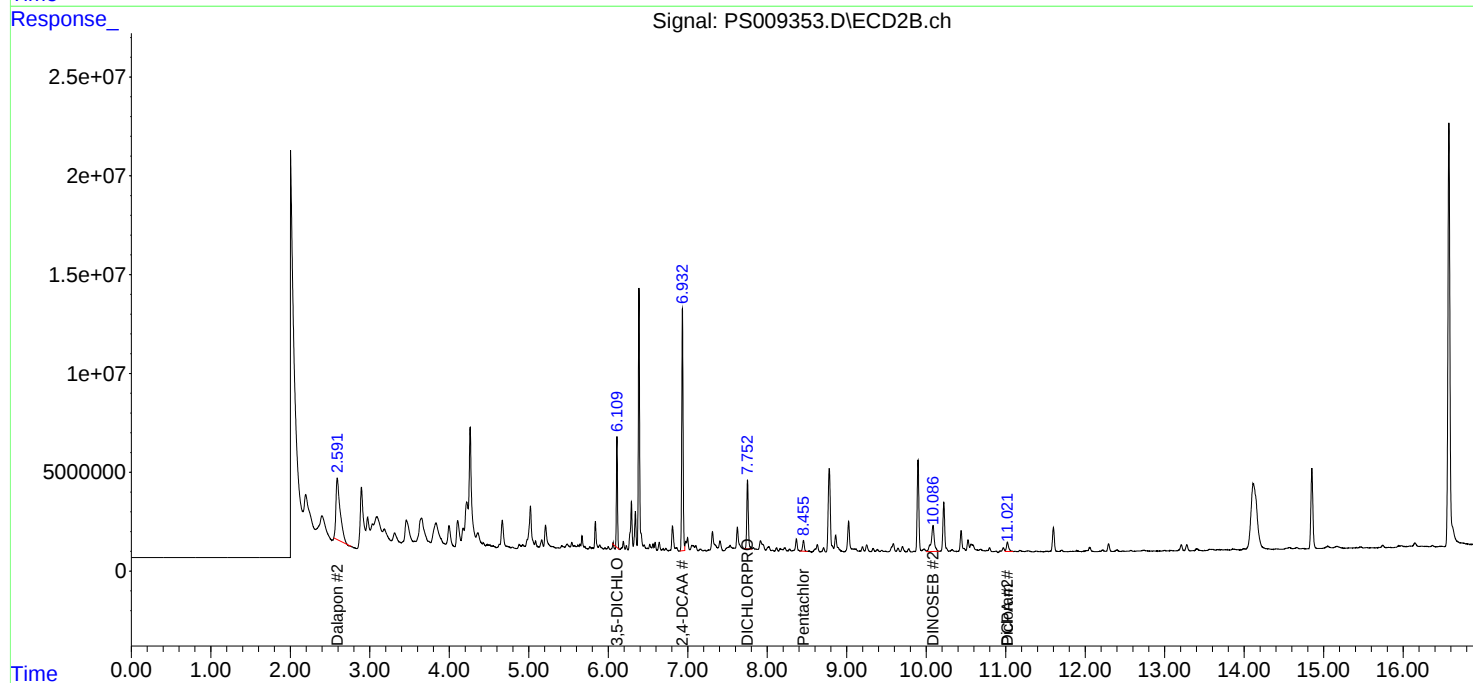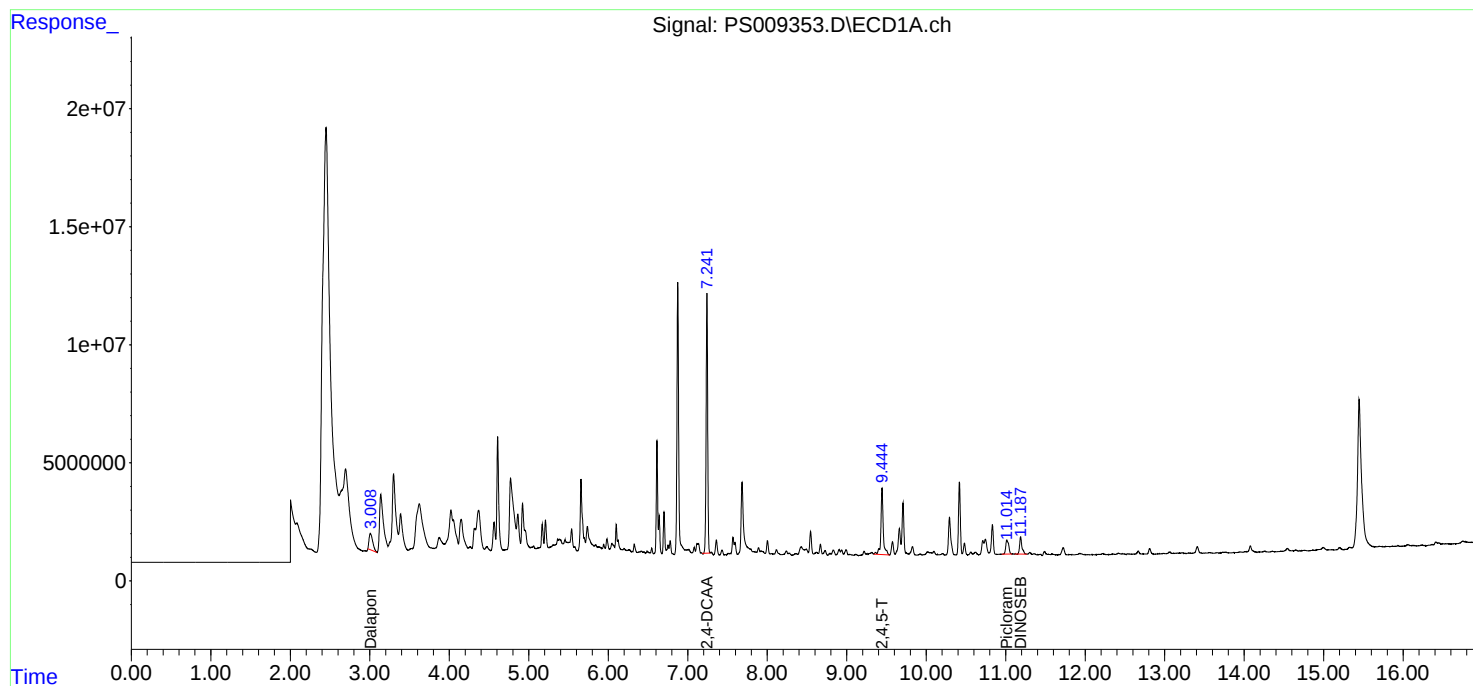


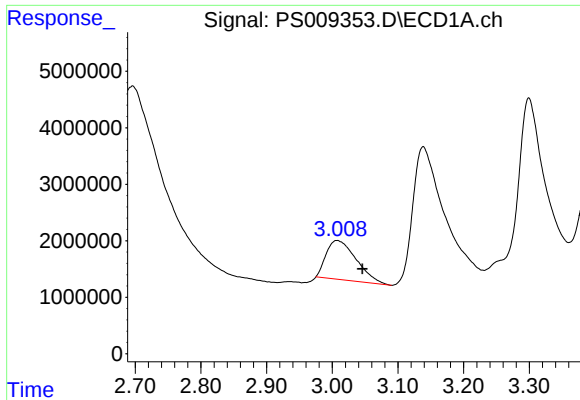

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.038 min
Response: 21936019
Conc: 28.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

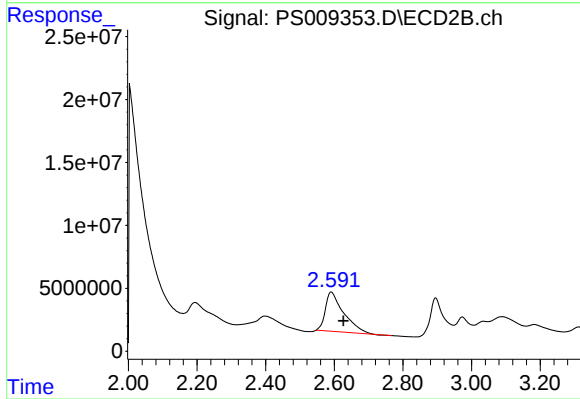


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.036 min
Response: 115012344
Conc: 146.07 ng/ml

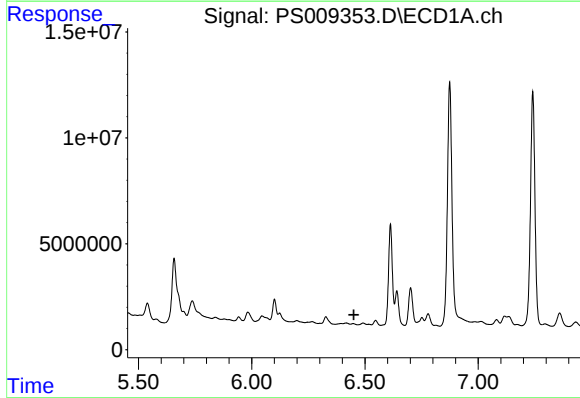


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

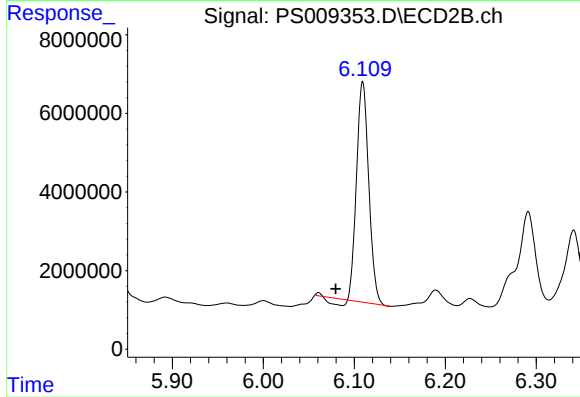

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.030 min
Response: 51323618
Conc: 63.10 ng/ml

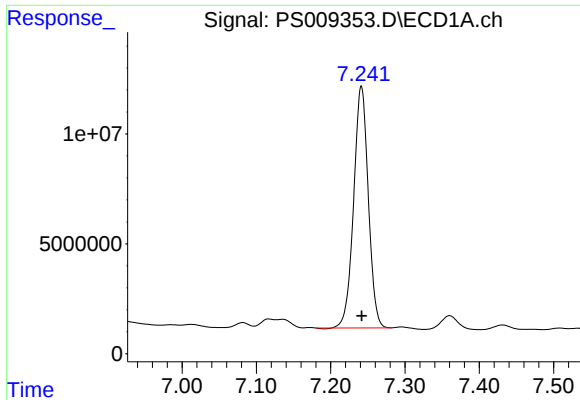

#4 2,4-DCAA


R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 150308478
Conc: 271.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

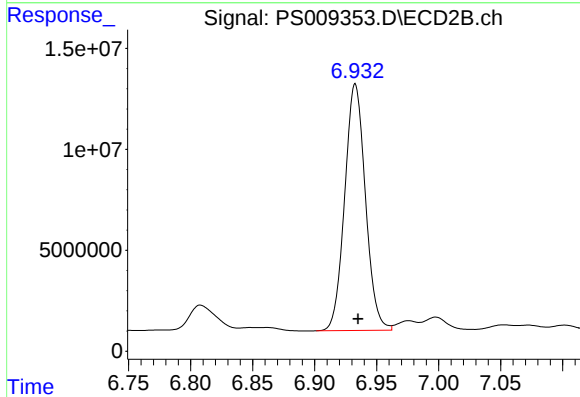


#4 2,4-DCAA

R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 142115260
Conc: 258.77 ng/ml

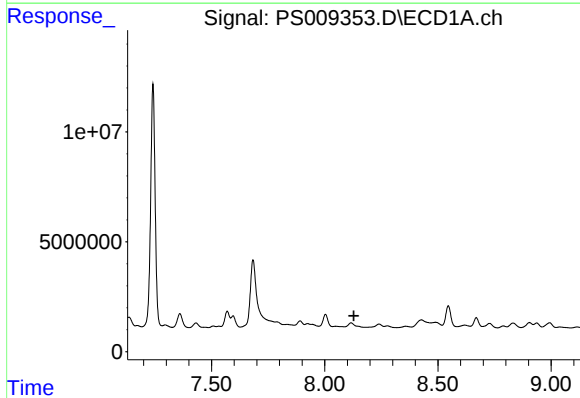


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

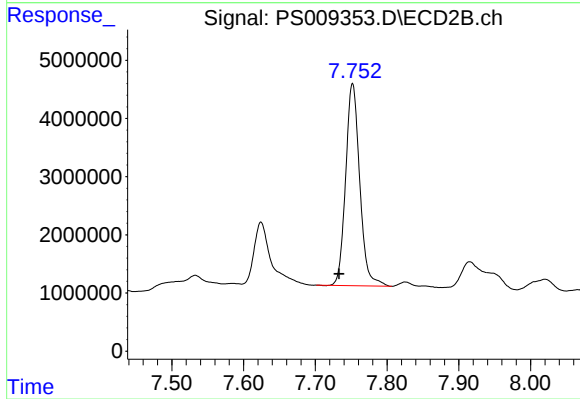

#8 DICHLORPROP


R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 47355032
Conc: 85.35 ng/ml

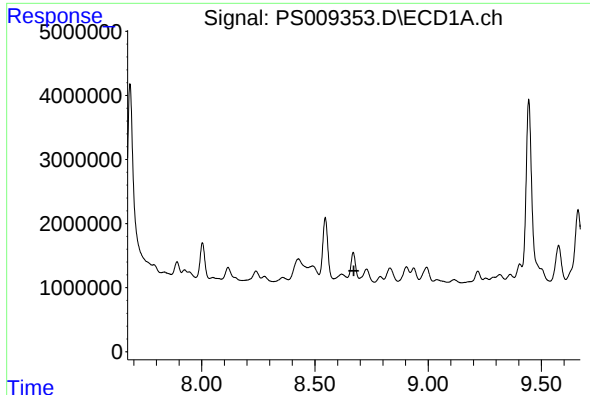

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

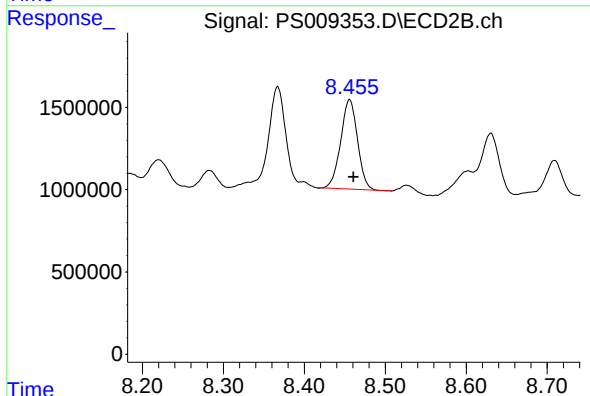


#10 Pentachlorophenol

R.T.: 8.456 min
Delta R.T.: -0.005 min
Response: 7852513
Conc: 1.03 ng/ml

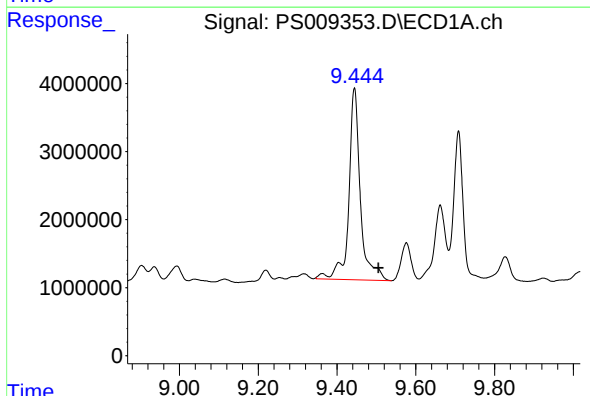


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 57634575
Conc: 22.66 ng/ml

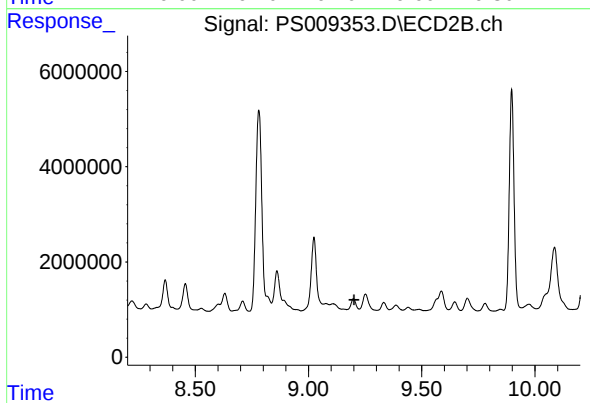

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

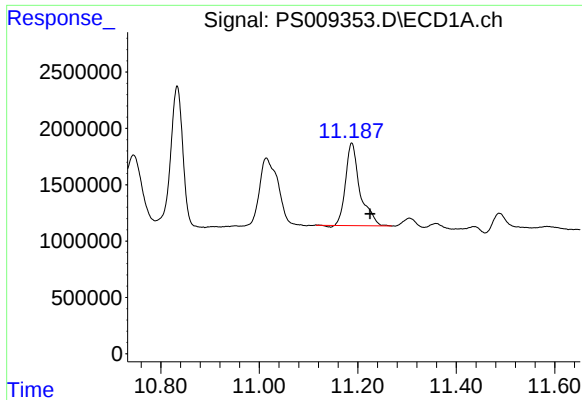

#14 DINOSEB


R.T.: 11.188 min
Delta R.T.: -0.037 min
Response: 14841125
Conc: 7.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

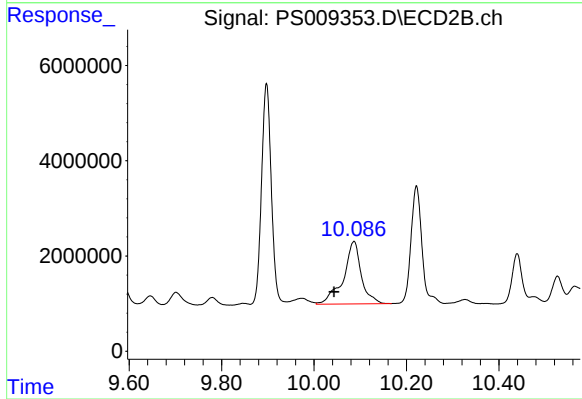


#14 DINOSEB

R.T.: 10.086 min
Delta R.T.: 0.043 min
Response: 35437356
Conc: 16.13 ng/ml

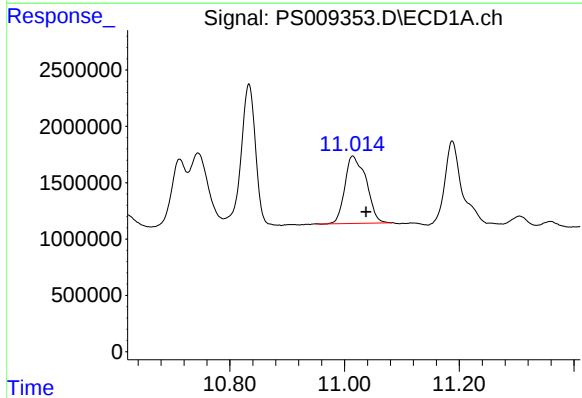


#15 Picloram

R.T.: 11.014 min
Delta R.T.: -0.023 min
Response: 15367243
Conc: 5.06 ng/ml

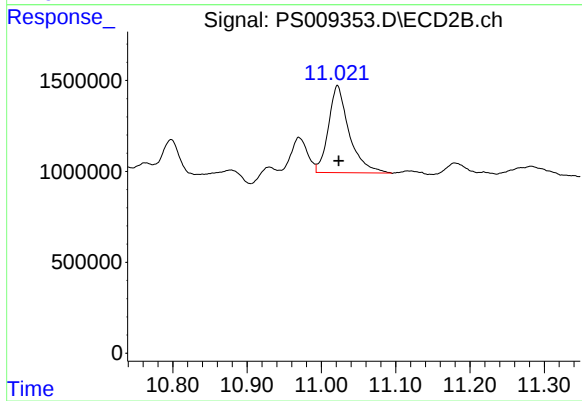

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.002 min
Response: 9283356
Conc: 2.28 ng/ml

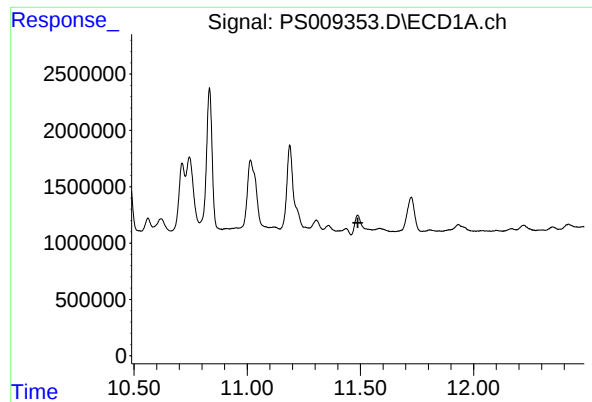

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

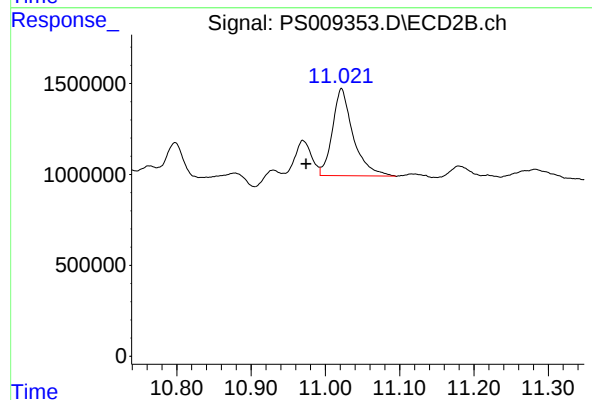

#16 DCPA

R.T.: 11.022 min
Delta R.T.: 0.048 min
Response: 9283356
Conc: 2.40 ng/ml