

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031820\
 Data File : PS009354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2020 19:18
 Operator : DD\AJ
 Sample : L1759-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:09:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.932	237.2E6	221.3E6	428.751	402.958
Target Compounds							
1) T	Dalapon	3.006	2.588	32332091	258.9E6	41.460	328.821 #
2) T	3,5-DICHL...	0.000	6.109	0	59799076	N.D.	73.526
3) T	4-Nitroph...	7.129	6.588	16797140	7750283	70.365	24.357 #
8) T	DICHLORPROP	0.000	7.752	0	45334797	N.D.	81.711
11) T	2,4,5-TP ...	0.000	8.785	0	39875125	N.D.	13.376
12) T	2,4,5-T	9.445	0.000	40784929	0	16.033	N.D. #
14) T	DINOSEB	11.187	10.085	21254555	38997838	10.398	17.755 #
15) T	Picloram	11.011	0.000	15981936	0	5.266	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031820\
Data File : PS009354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2020 19:18
Operator : DD\AJ
Sample : L1759-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:09:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

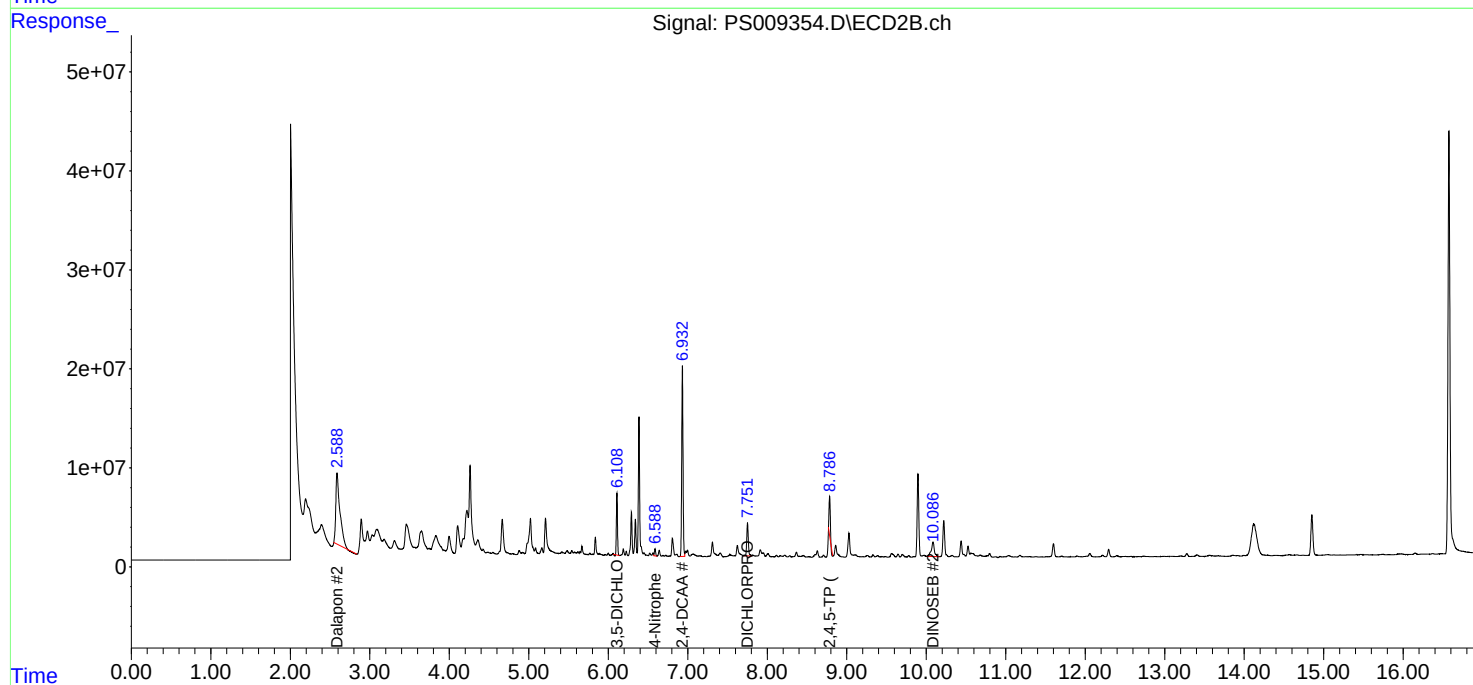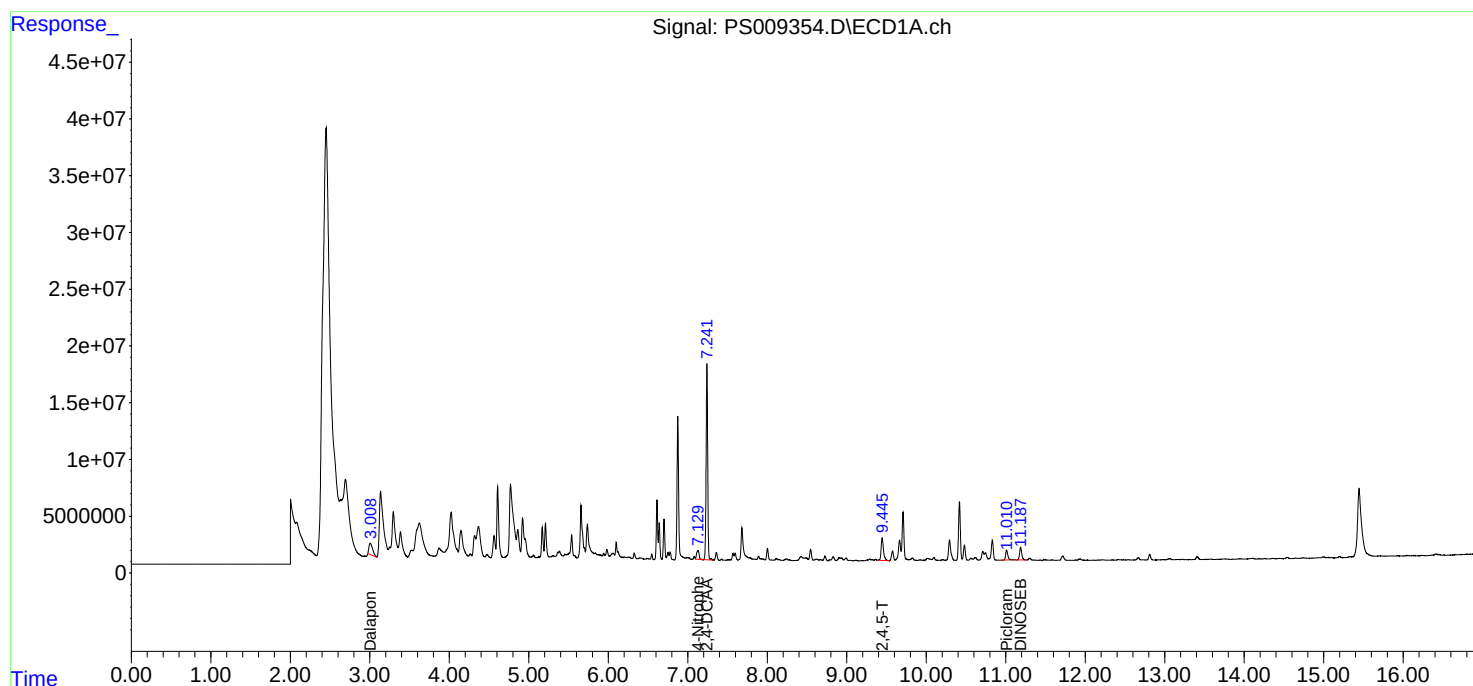


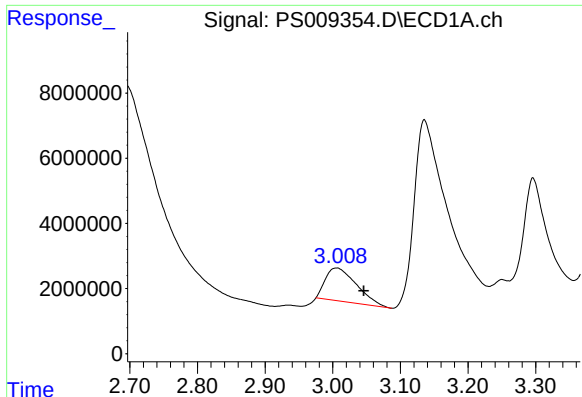

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 32332091
Conc: 41.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

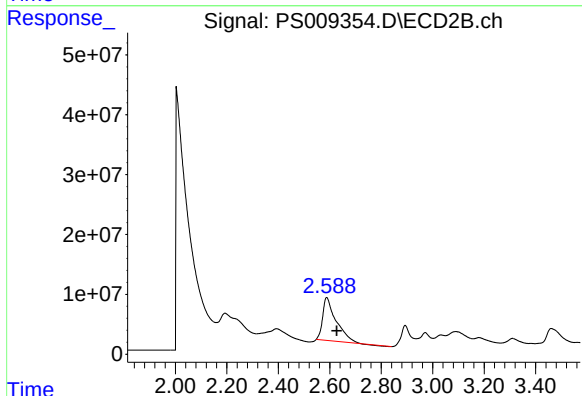


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 258901060
Conc: 328.82 ng/ml

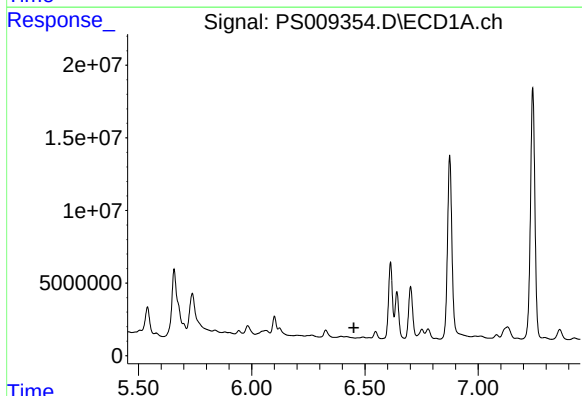


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

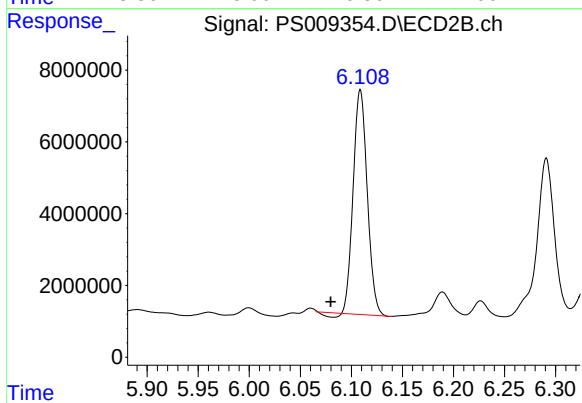

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.029 min
Response: 59799076
Conc: 73.53 ng/ml

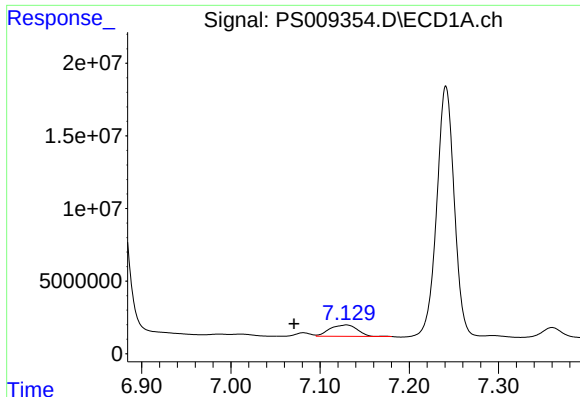

#3 4-Nitrophenol


R.T.: 7.129 min
Delta R.T.: 0.058 min
Response: 16797140
Conc: 70.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

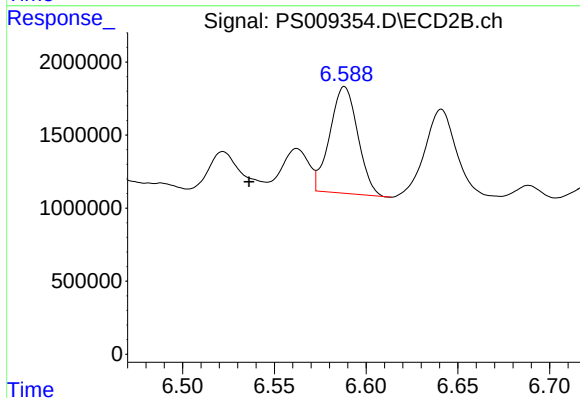


#3 4-Nitrophenol

R.T.: 6.588 min
Delta R.T.: 0.052 min
Response: 7750283
Conc: 24.36 ng/ml

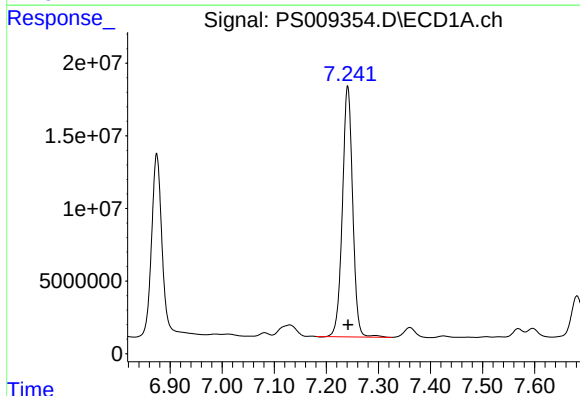


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 237172513
Conc: 428.75 ng/ml

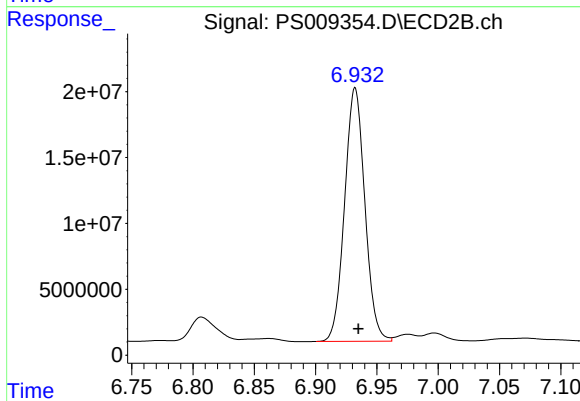

#4 2,4-DCAA


R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 221303714
Conc: 402.96 ng/ml

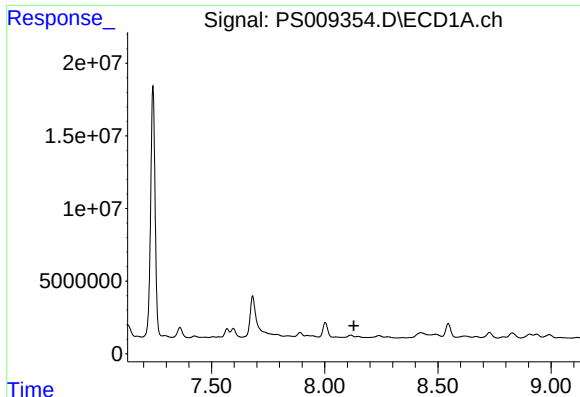

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

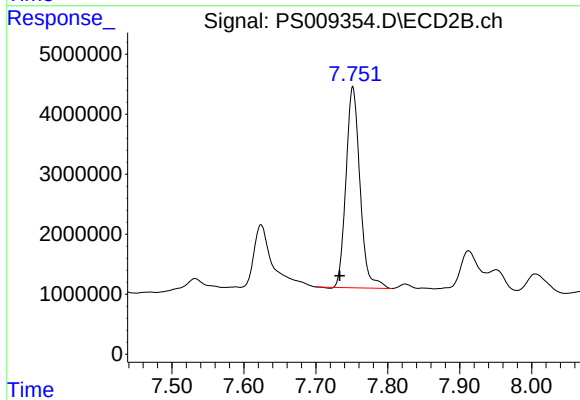


#8 DICHLORPROP

R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 45334797
Conc: 81.71 ng/ml

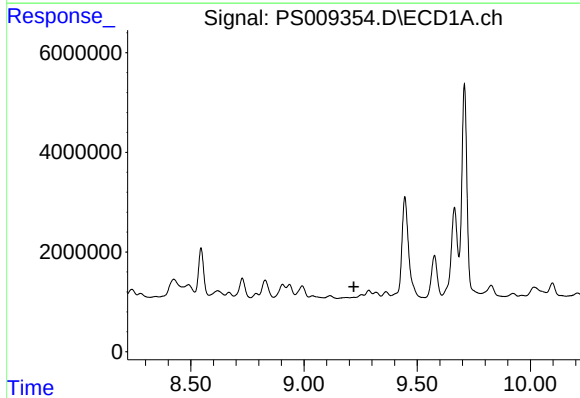


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

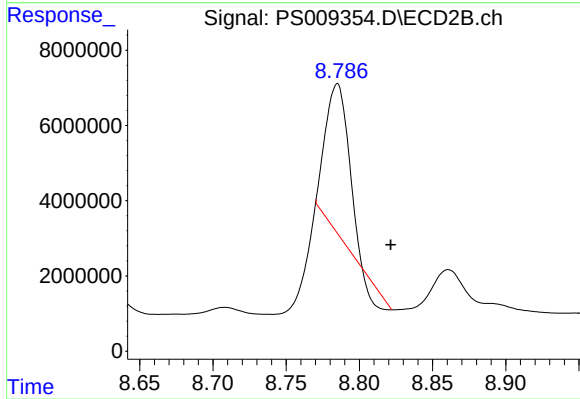

#11 2,4,5-TP (SILVEX)


R.T.: 8.785 min
Delta R.T.: -0.037 min
Response: 39875125
Conc: 13.38 ng/ml

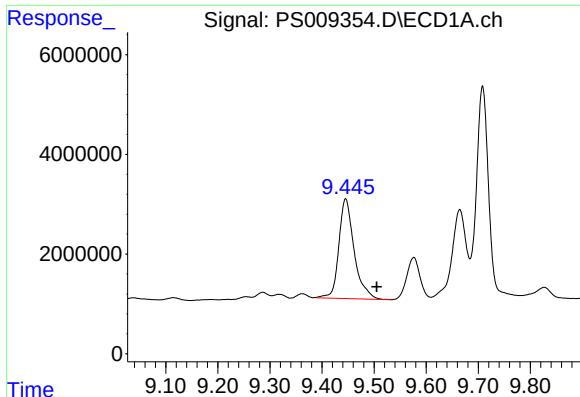

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 40784929
Conc: 16.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

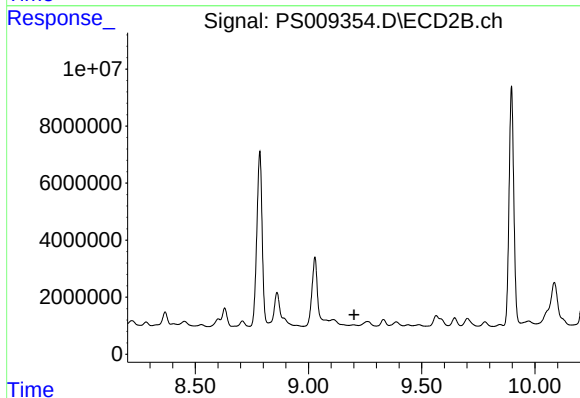


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

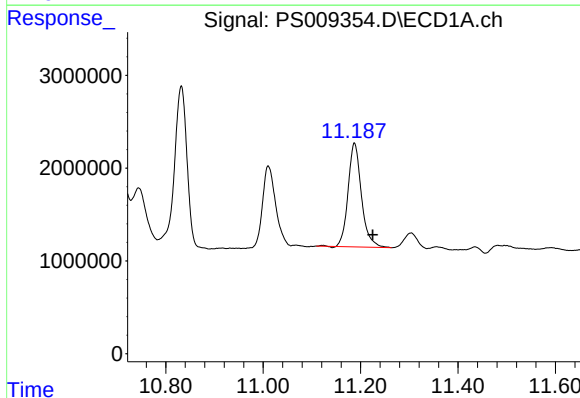


#14 DINOSEB

R.T.: 11.187 min
Delta R.T.: -0.038 min
Response: 21254555
Conc: 10.40 ng/ml

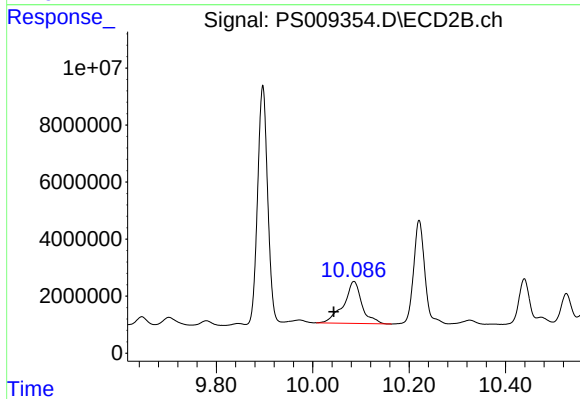

#14 DINOSEB


R.T.: 10.085 min
Delta R.T.: 0.042 min
Response: 38997838
Conc: 17.75 ng/ml

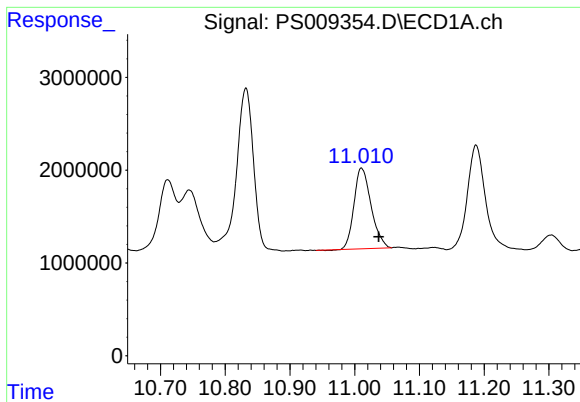

#15 Picloram

R.T.: 11.011 min
Delta R.T.: -0.027 min
Response: 15981936
Conc: 5.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

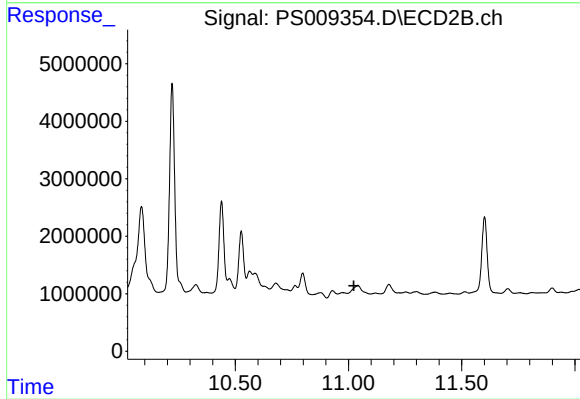

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.