

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031820\
 Data File : PS009357.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2020 20:27
 Operator : DD\AJ
 Sample : L1948-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:10:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	6.932	172.9E6	158.8E6	312.539	289.238
Target Compounds							
1) T	Dalapon	3.008	2.590	21732464	82329128	27.868	104.563 #
2) T	3,5-DICHL...	0.000	6.109	0	48436041	N.D.	59.554
6) T	MCP	7.564	0.000	2262951	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.751	0	37173431	N.D.	67.001
10) T	Pentachlo...	0.000	8.455	0	7777197	N.D.	1.025
12) T	2,4,5-T	9.444	0.000	50409468	0	19.816	N.D. #
14) T	DINOSEB	11.187	10.085	11888440	23288323	5.816	10.603 #
15) T	Picloram	11.013	0.000	12401699	0	4.086	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031820\
Data File : PS009357.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2020 20:27
Operator : DD\AJ
Sample : L1948-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:10:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

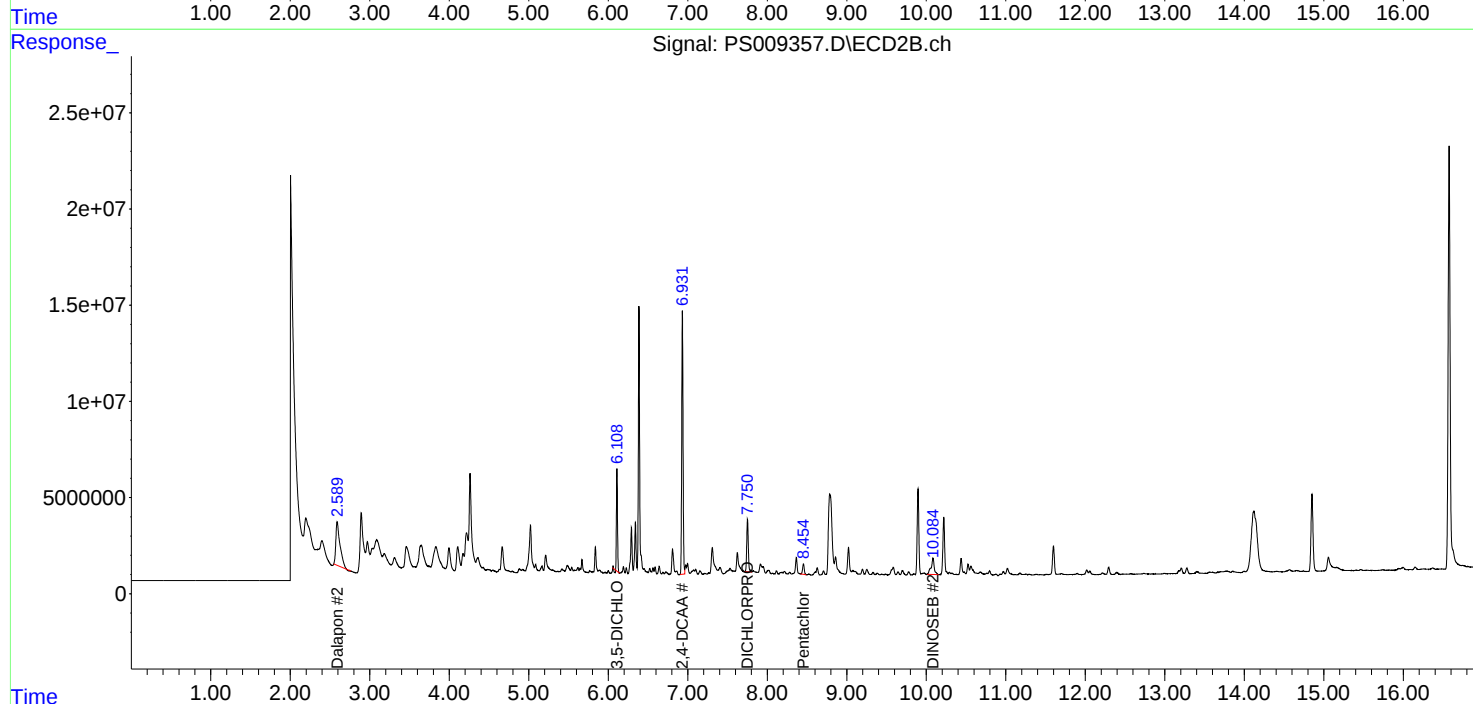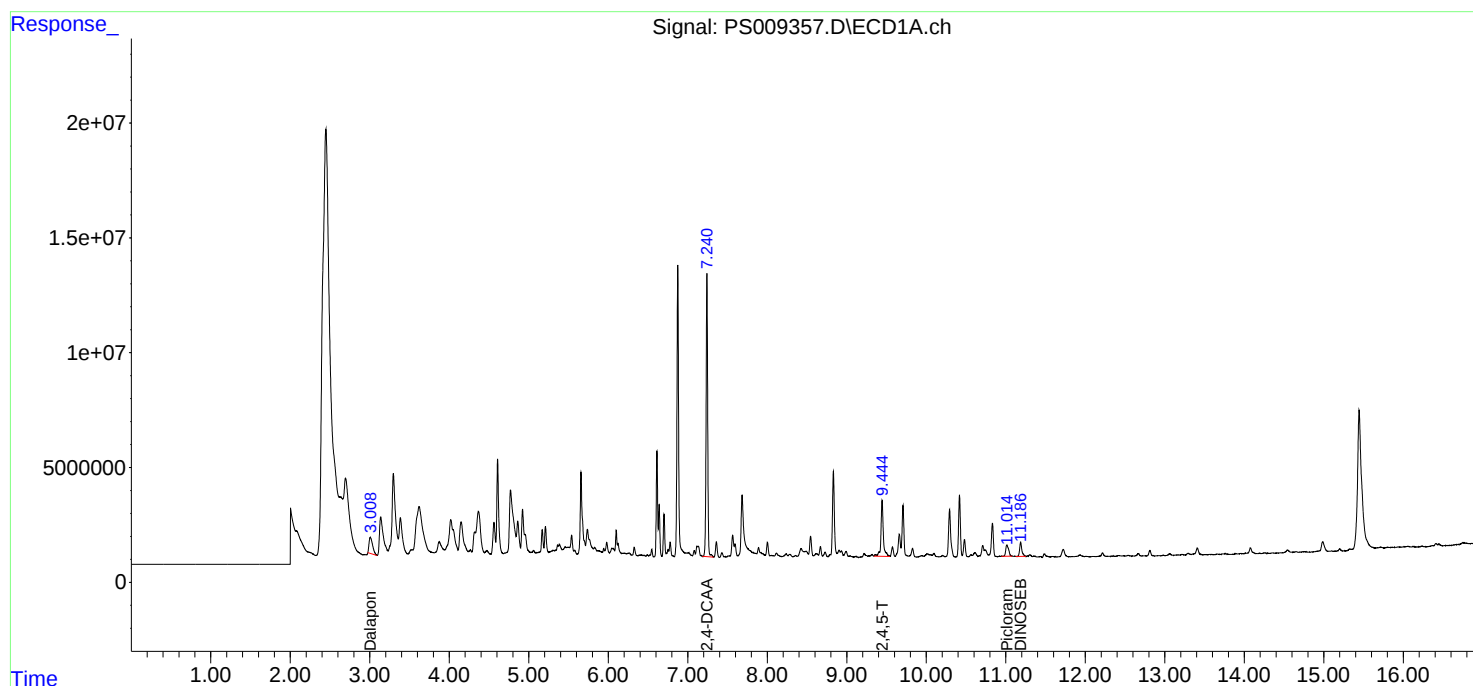


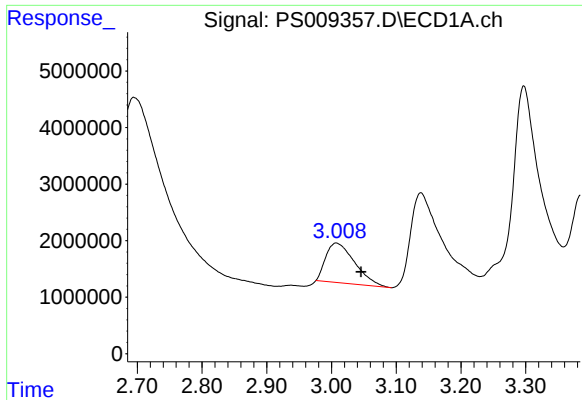

#1 Dalapon


R.T.: 3.008 min
Delta R.T.: -0.038 min
Response: 21732464
Conc: 27.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

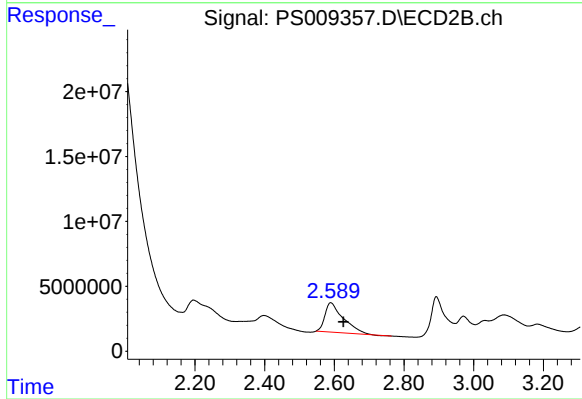


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.036 min
Response: 82329128
Conc: 104.56 ng/ml

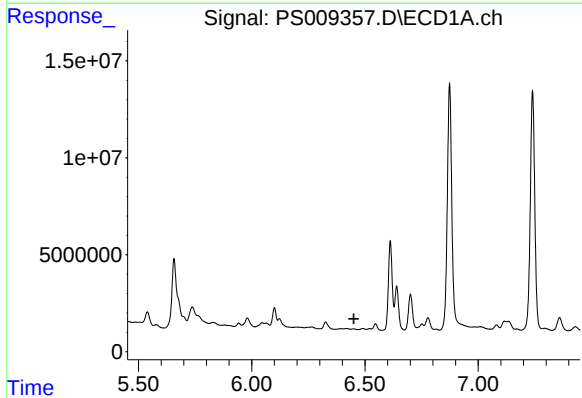


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

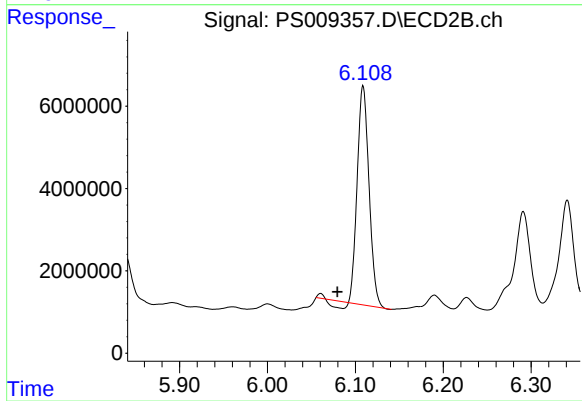

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.029 min
Response: 48436041
Conc: 59.55 ng/ml

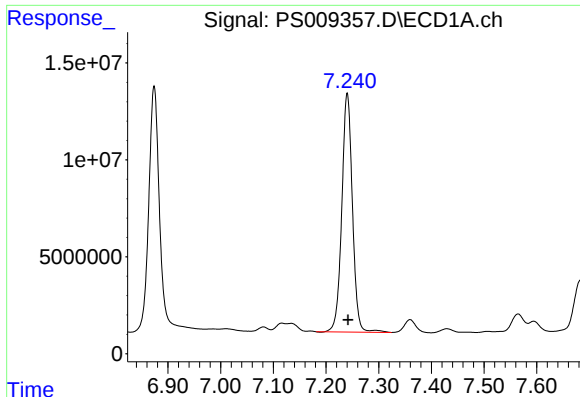

#4 2,4-DCAA


R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 172887301
Conc: 312.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

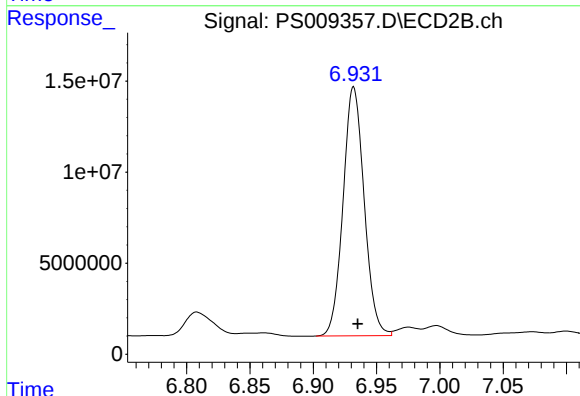


#4 2,4-DCAA

R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 158848890
Conc: 289.24 ng/ml

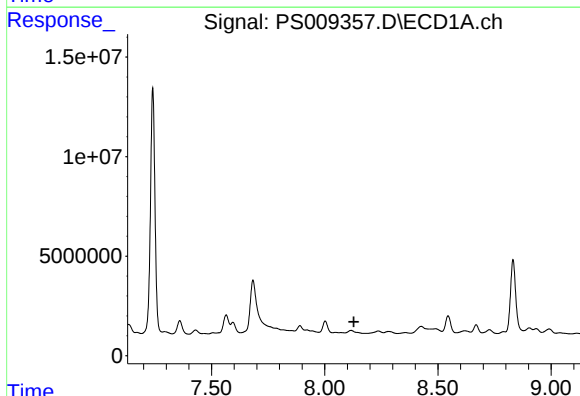


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

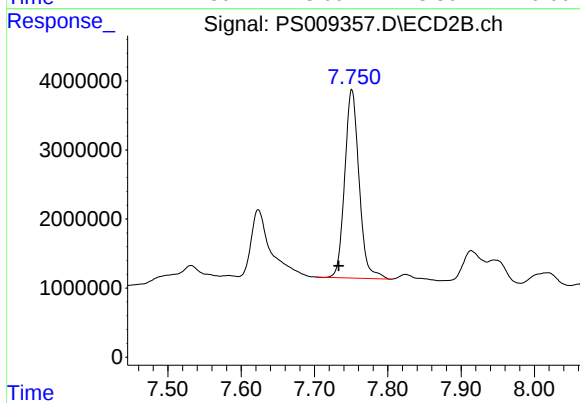

#8 DICHLORPROP


R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 37173431
Conc: 67.00 ng/ml

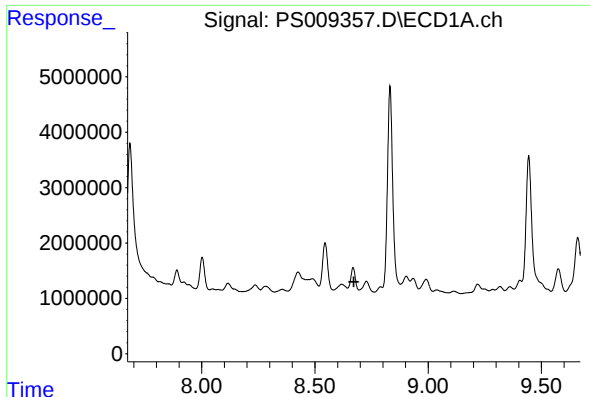

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

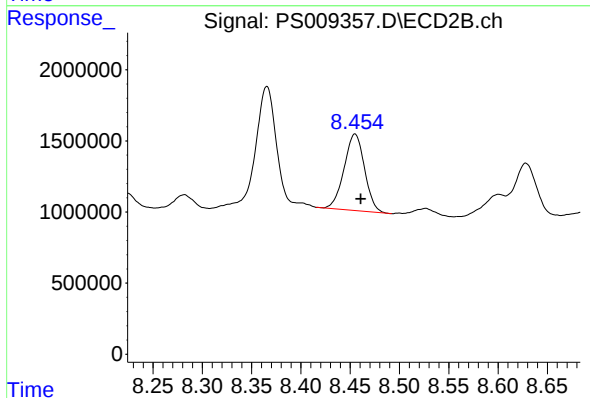


#10 Pentachlorophenol

R.T.: 8.455 min
Delta R.T.: -0.006 min
Response: 7777197
Conc: 1.02 ng/ml

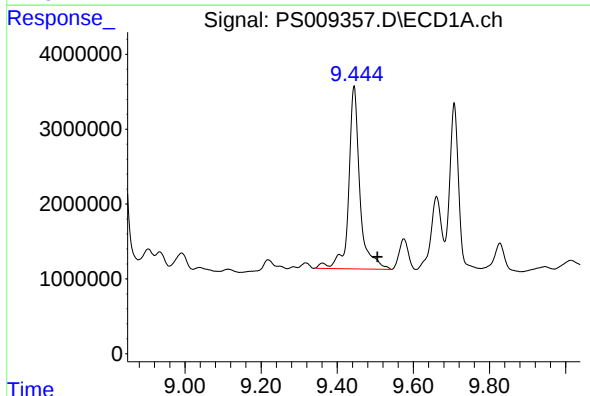


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 50409468
Conc: 19.82 ng/ml

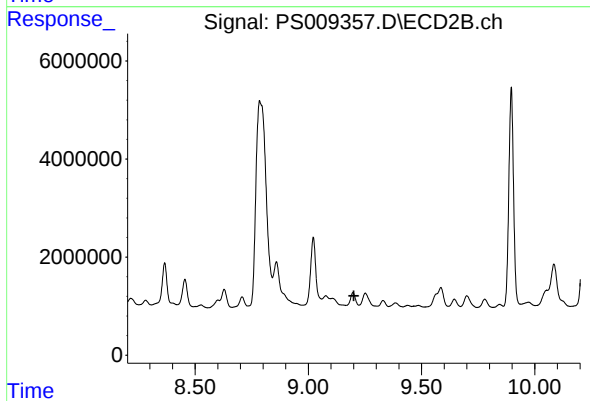

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

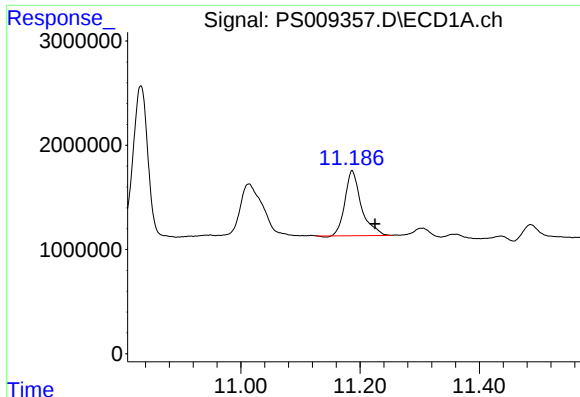

#14 DINOSEB


R.T.: 11.187 min
Delta R.T.: -0.038 min
Response: 11888440
Conc: 5.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

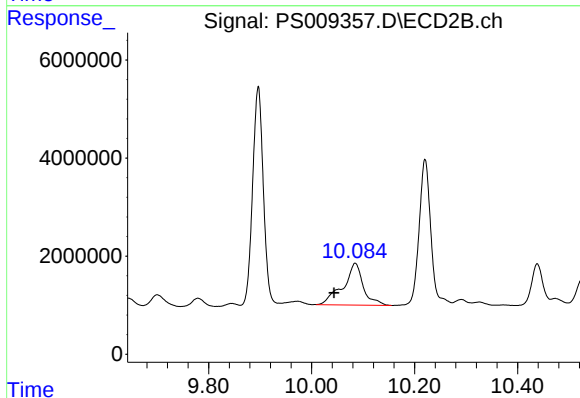


#14 DINOSEB

R.T.: 10.085 min
Delta R.T.: 0.041 min
Response: 23288323
Conc: 10.60 ng/ml

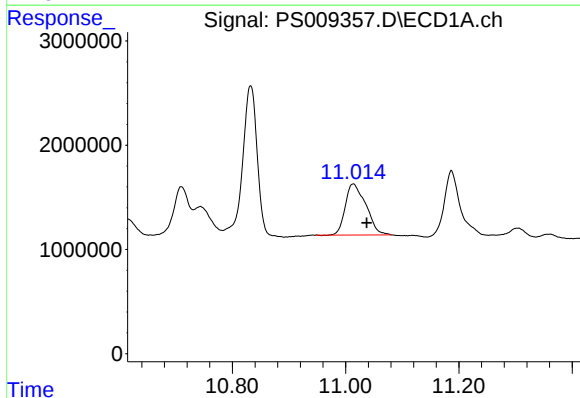

#15 Picloram

R.T.: 11.013 min
Delta R.T.: -0.024 min
Response: 12401699
Conc: 4.09 ng/ml

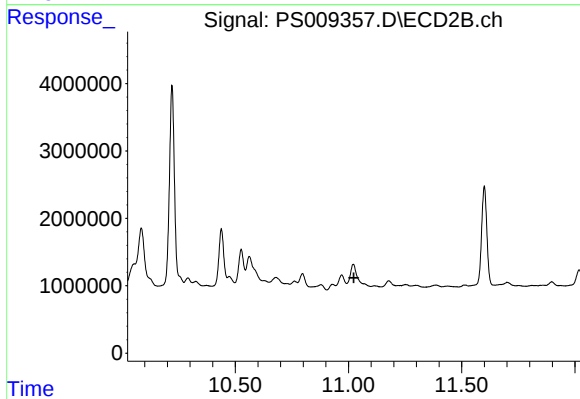

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.