

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031821\
 Data File : PS014294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2021 01:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 05:25:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.168	6.890	639.2E6	259.9E6	447.381	550.897
Target Compounds							
5) T	DICAMBA	0.000	7.124f	0	801528	N.D.	<MDL
6) T	MCPD	0.000	7.124	0	801528	N.D.	<MDL
7) T	MCPA	0.000	7.292f	0	4587522	N.D.	1.883
8) T	DICHLORPROP	0.000	7.741f	0	2548617	N.D.	5.002
12) T	2,4,5-T	0.000	9.168	0	743164	N.D.	<MDL
15) T	Picloram	0.000	10.997	0	1696004	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031821\
Data File : PS014294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2021 01:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 05:25:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

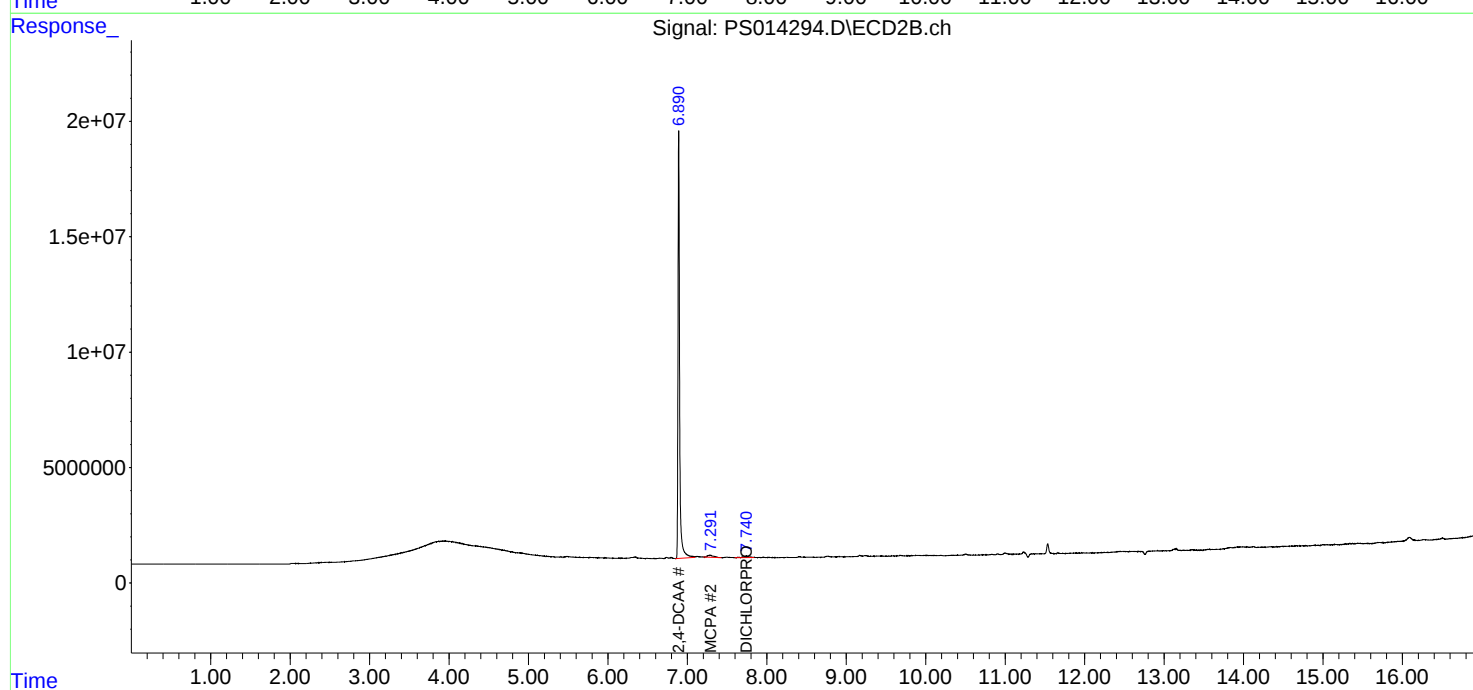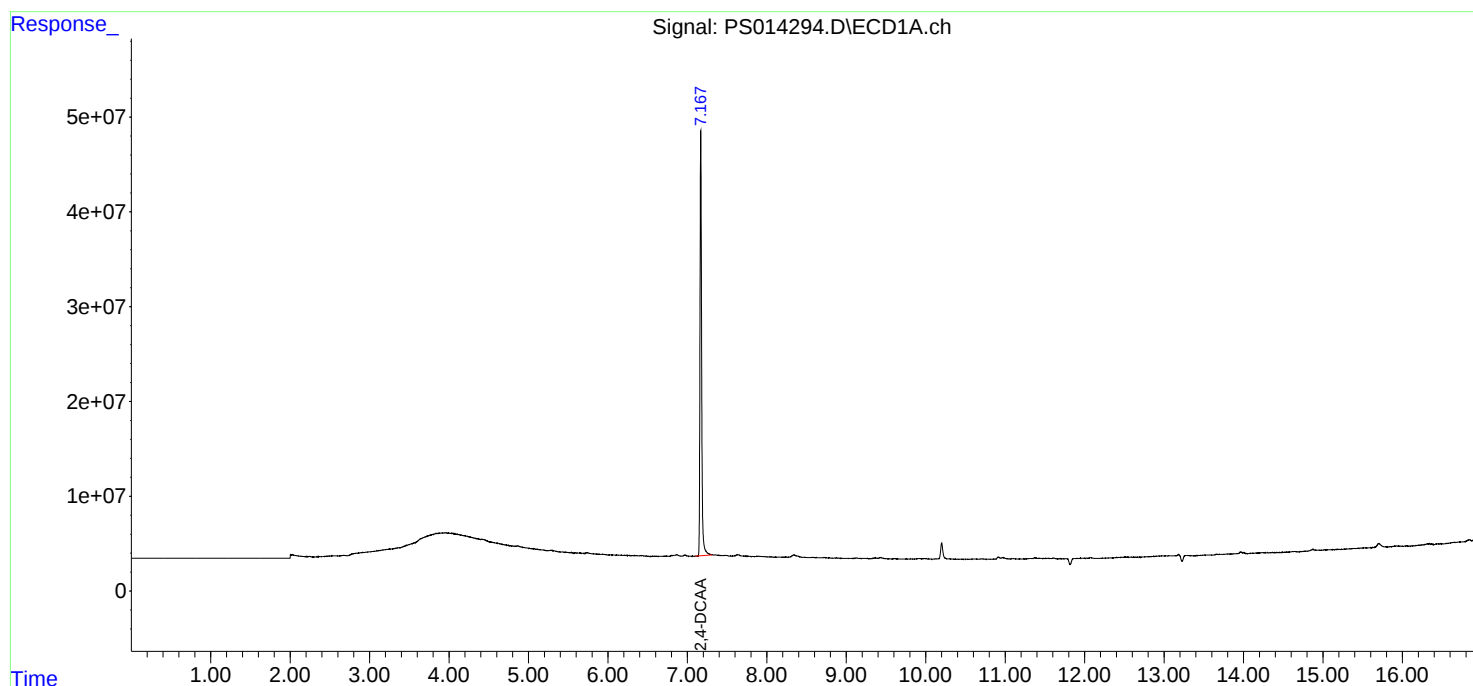


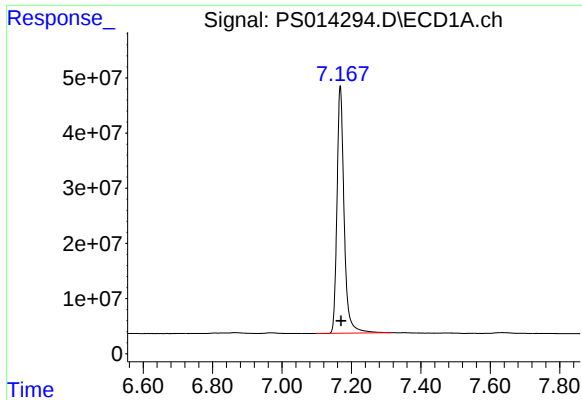

#4 2,4-DCAA


R.T.: 7.168 min
Delta R.T.: -0.002 min
Response: 639236744
Conc: 447.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

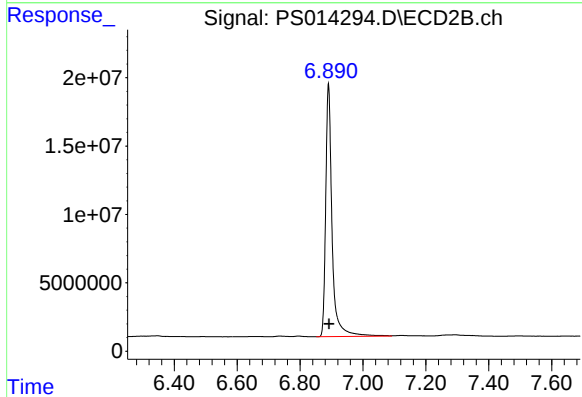


#4 2,4-DCAA

R.T.: 6.890 min
Delta R.T.: -0.002 min
Response: 259896208
Conc: 550.90 ng/ml

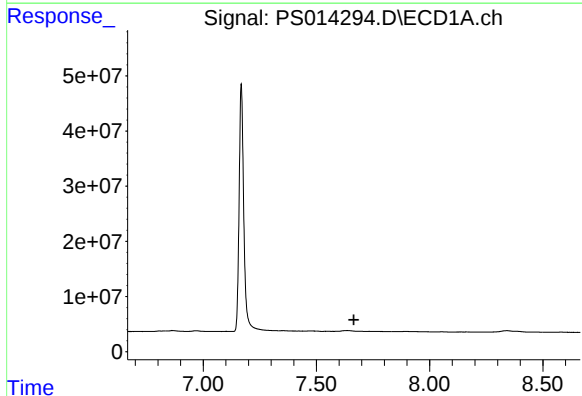


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.666 min
Response: 0
Conc: N.D.

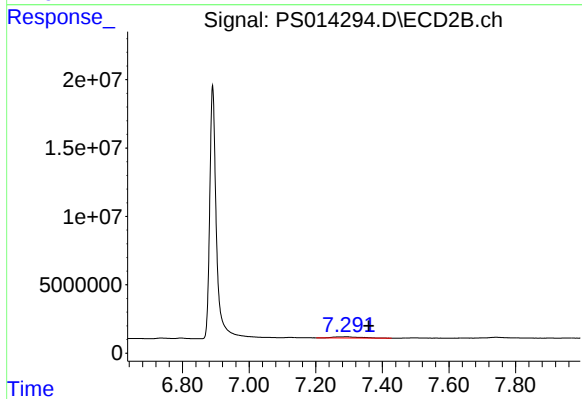

#7 MCPA


R.T.: 7.292 min
Delta R.T.: -0.067 min
Response: 4587522
Conc: 1.88 ug/ml

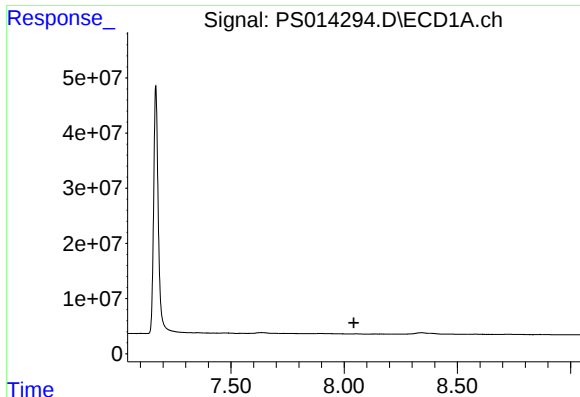

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

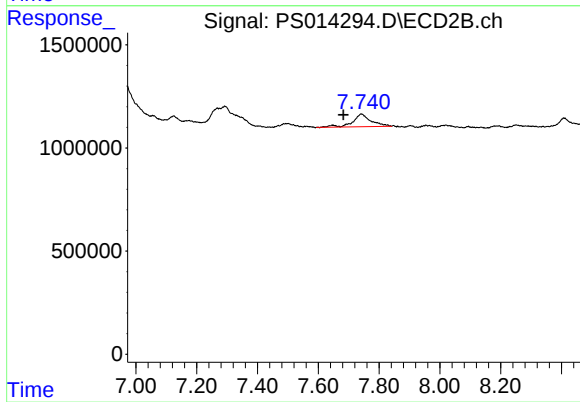

#8 DICHLORPROP

R.T.: 7.741 min
Delta R.T.: 0.058 min
Response: 2548617
Conc: 5.00 ng/ml