

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031821\
 Data File : PS014290.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 23:56
 Operator : DD\AJ
 Sample : M1707-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ELEVATOR-510-EL-167-157

Manual Integrations
 APPROVED

Ankita
 3/19/2021 10:26:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 05:24:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.166	6.888	651.8E6	244.1E6	456.184	517.356m
Target Compounds							
10) T	Pentachlo...	8.576	8.400	2577.9E6	965.6E6	129.512m	141.387m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031821\
Data File : PS014290.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 23:56
Operator : DD\AJ
Sample : M1707-03
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
ELEVATOR-510-EL-167-157


Manual Integrations
APPROVED

Ankita
3/19/2021 10:26:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 05:24:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

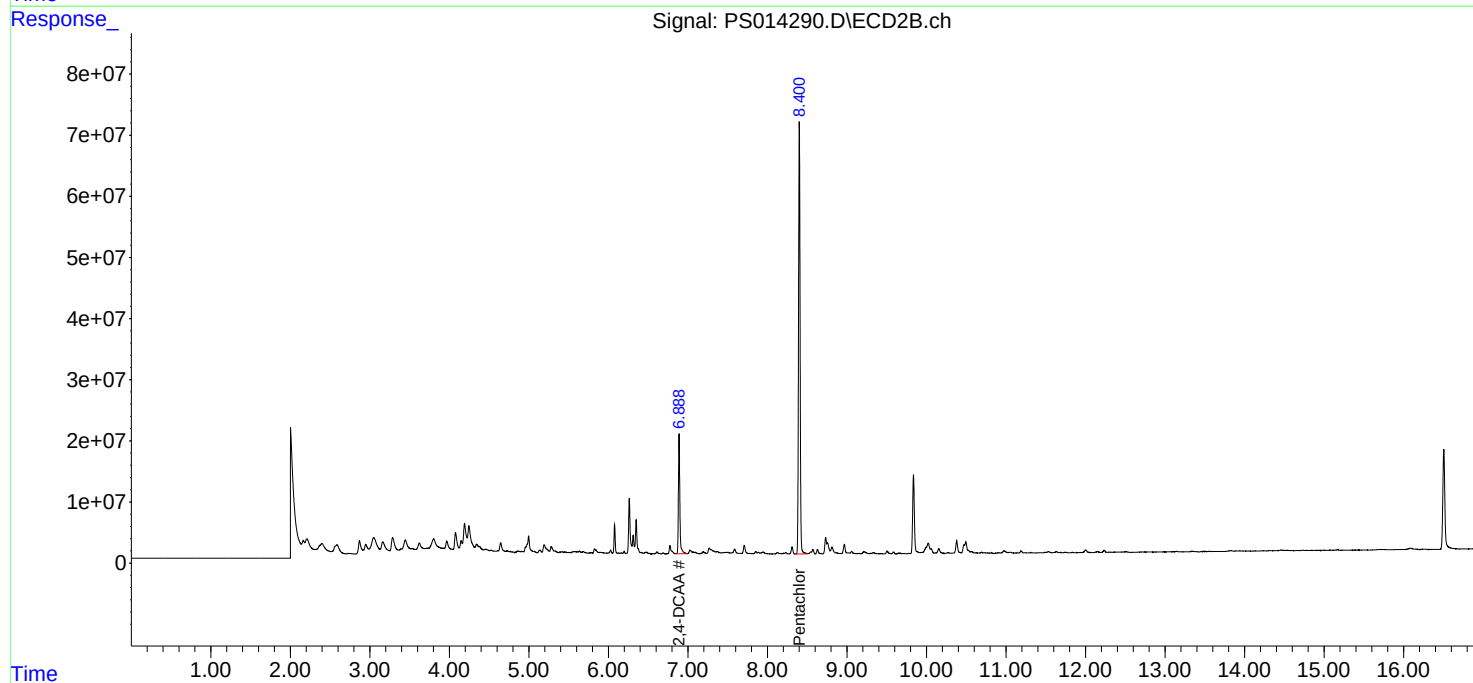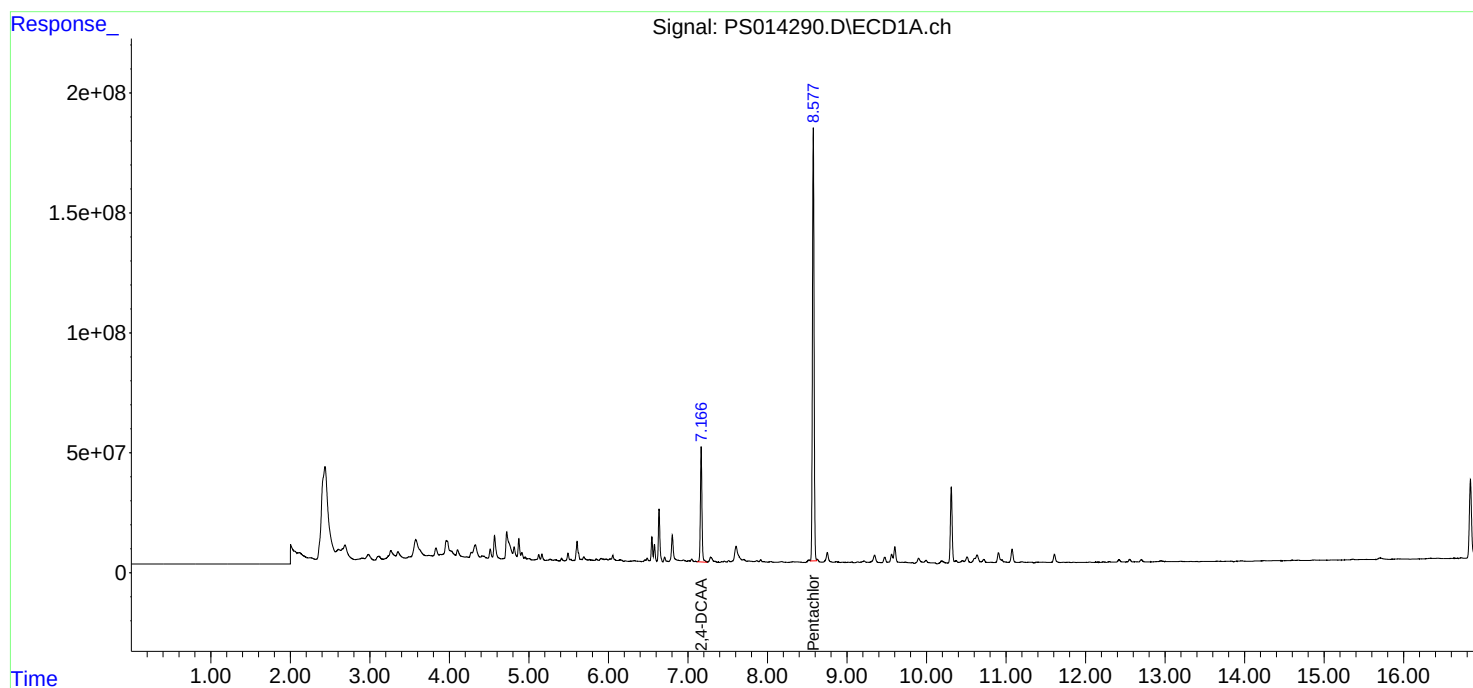

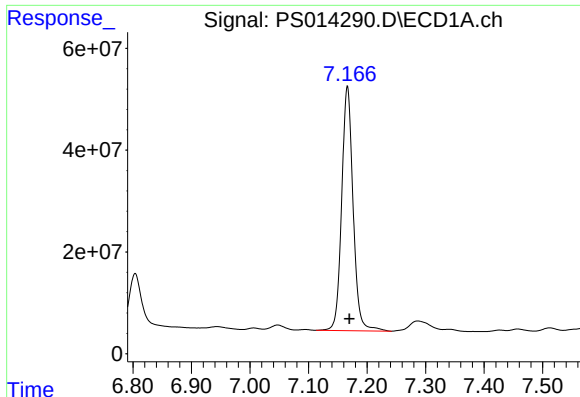


#4 2,4-DCAA

R.T.: 7.166 min
Delta R.T.: -0.004 min
Response: 651814461
Conc: 456.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
ELEVATOR-510-EL-167-157


Manual Integrations
APPROVED

Ankita
3/19/2021 10:26:40 AM

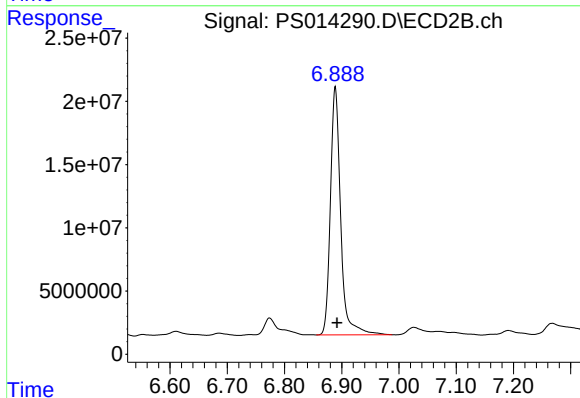


#4 2,4-DCAA

R.T.: 6.888 min
Delta R.T.: -0.004 min
Response: 244072509
Conc: 517.36 ng/ml m

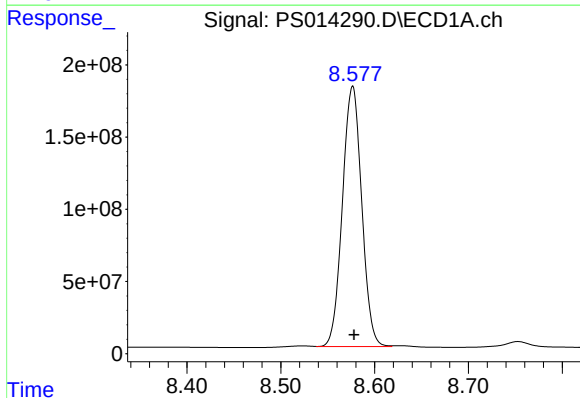

#10 Pentachlorophenol

R.T.: 8.576 min
Delta R.T.: -0.002 min
Response: 2577892942
Conc: 129.51 ng/ml m

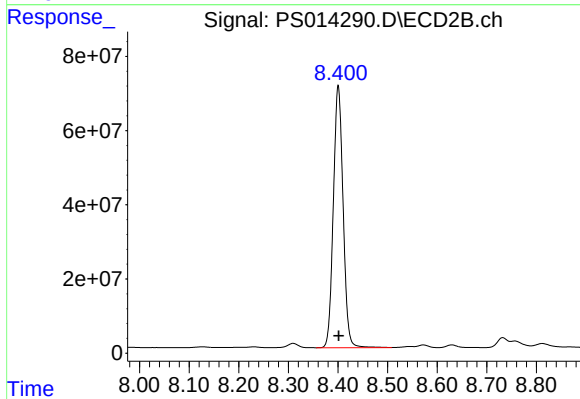

#10 Pentachlorophenol

R.T.: 8.400 min
Delta R.T.: -0.002 min
Response: 965619938
Conc: 141.39 ng/ml m