

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031821\
 Data File : PS014297.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2021 02:37
 Operator : DD\AJ
 Sample : M1712-22
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 NEW-BLOCK-FLOOR-PAT

Manual Integrations
 APPROVED

Ankita
 3/19/2021 10:26:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 05:26:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.166	6.888	738.8E6	252.4E6	517.047	534.981m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031821\
Data File : PS014297.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2021 02:37
Operator : DD\AJ
Sample : M1712-22
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
NEW-BLOCK-FLOOR-PAT


Manual Integrations
APPROVED

Ankita
3/19/2021 10:26:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 05:26:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

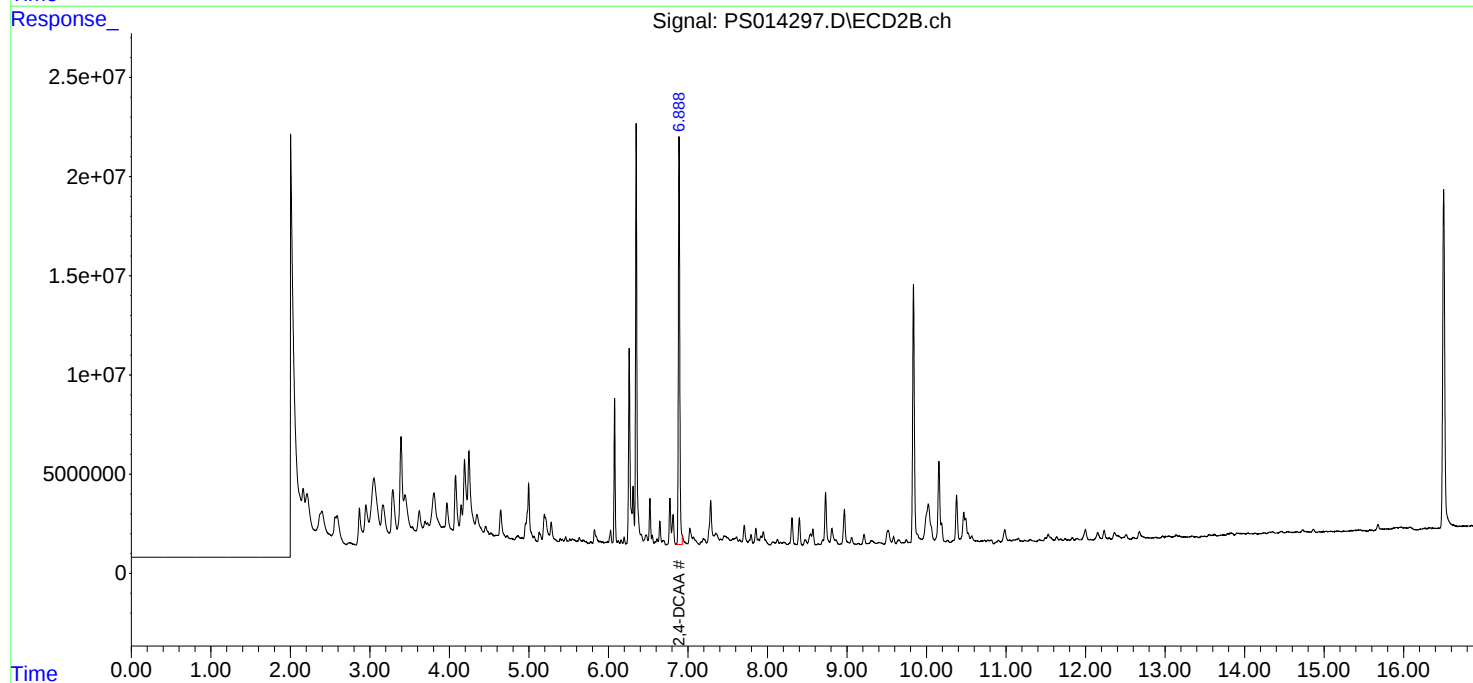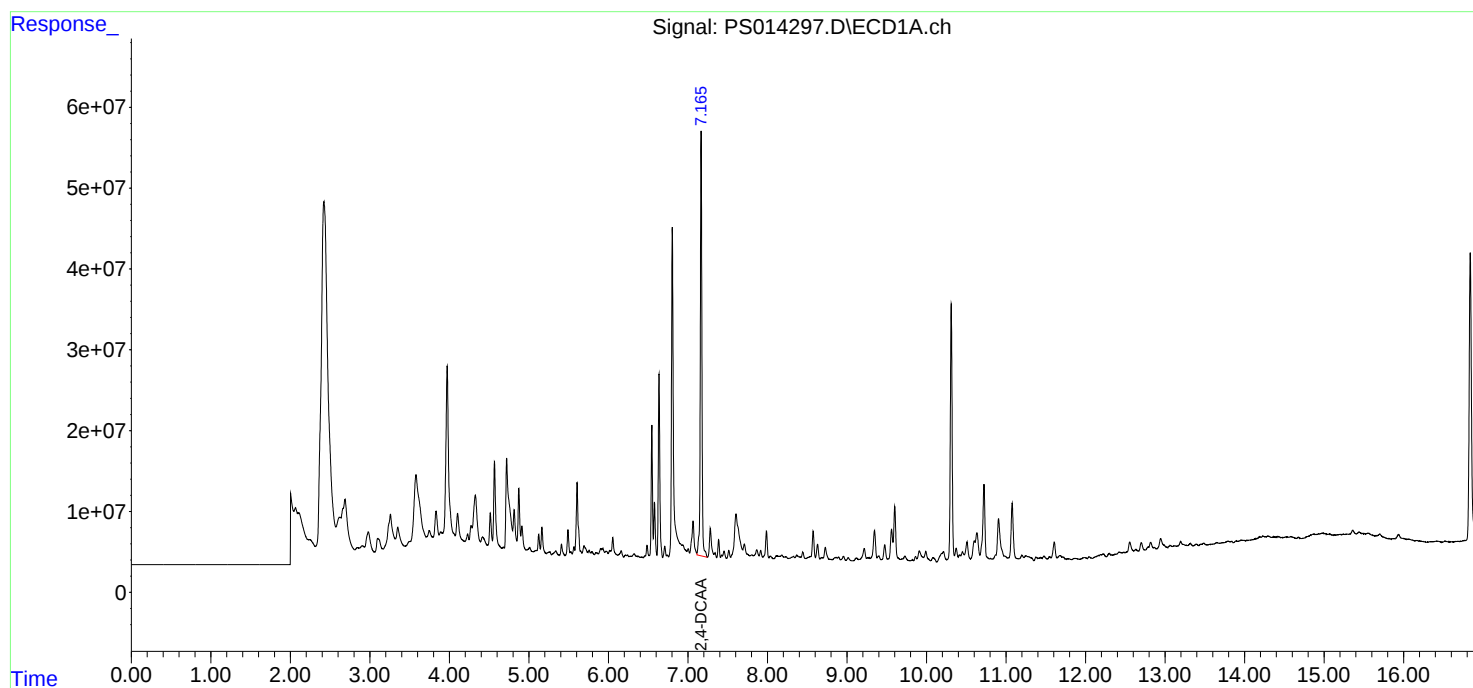

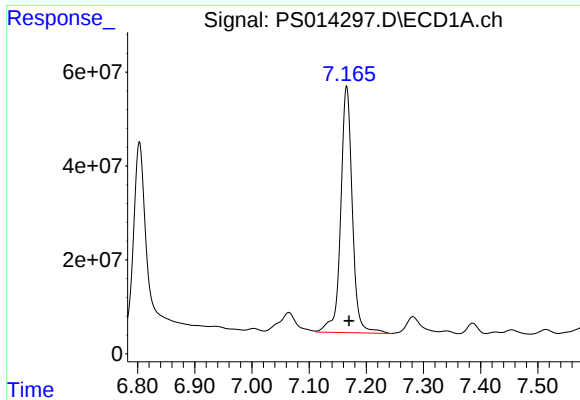


#4 2,4-DCAA

R.T.: 7.166 min
Delta R.T.: -0.004 min
Response: 738779043
Conc: 517.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
NEW-BLOCK-FLOOR-PAT

Manual Integrations
APPROVED

Ankita
3/19/2021 10:26:48 AM

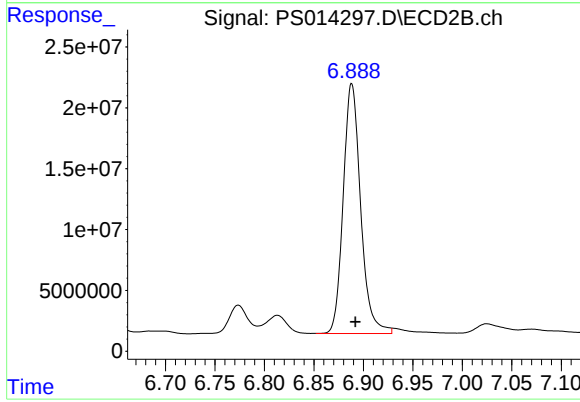

#4 2,4-DCAA

R.T.: 6.888 min
Delta R.T.: -0.004 min
Response: 252387172
Conc: 534.98 ng/ml m