

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031920\
 Data File : PS009363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2020 16:41
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 17:36:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.933	275.1E6	289.4E6	497.329	526.894
Target Compounds							
12) T	2,4,5-T	0.000	9.254	0	7176159	N.D.	2.431
15) T	Picloram	11.038	11.024	13699130	23083002	4.514	5.668 #
16) T	DCPA	0.000	11.024	0	23083002	N.D.	5.960



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS031920\
Data File : PS009363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2020 16:41
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 17:36:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

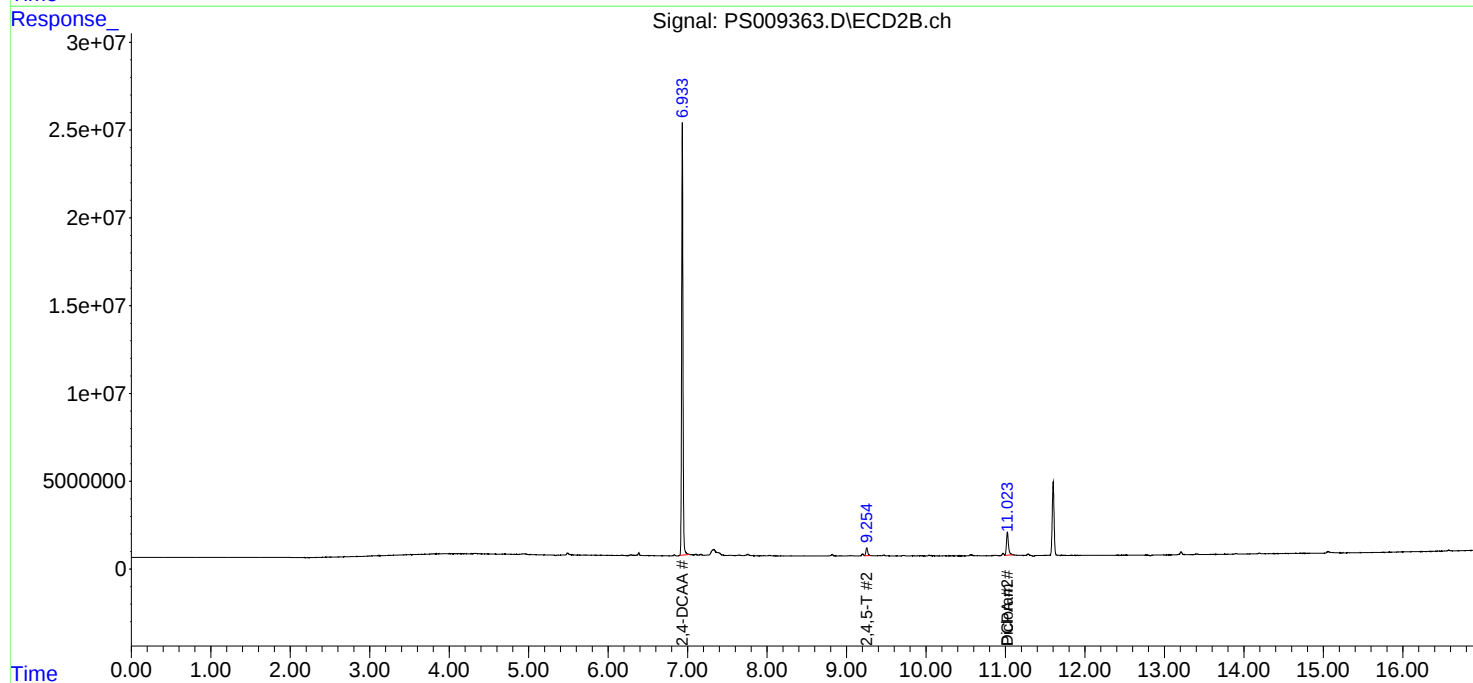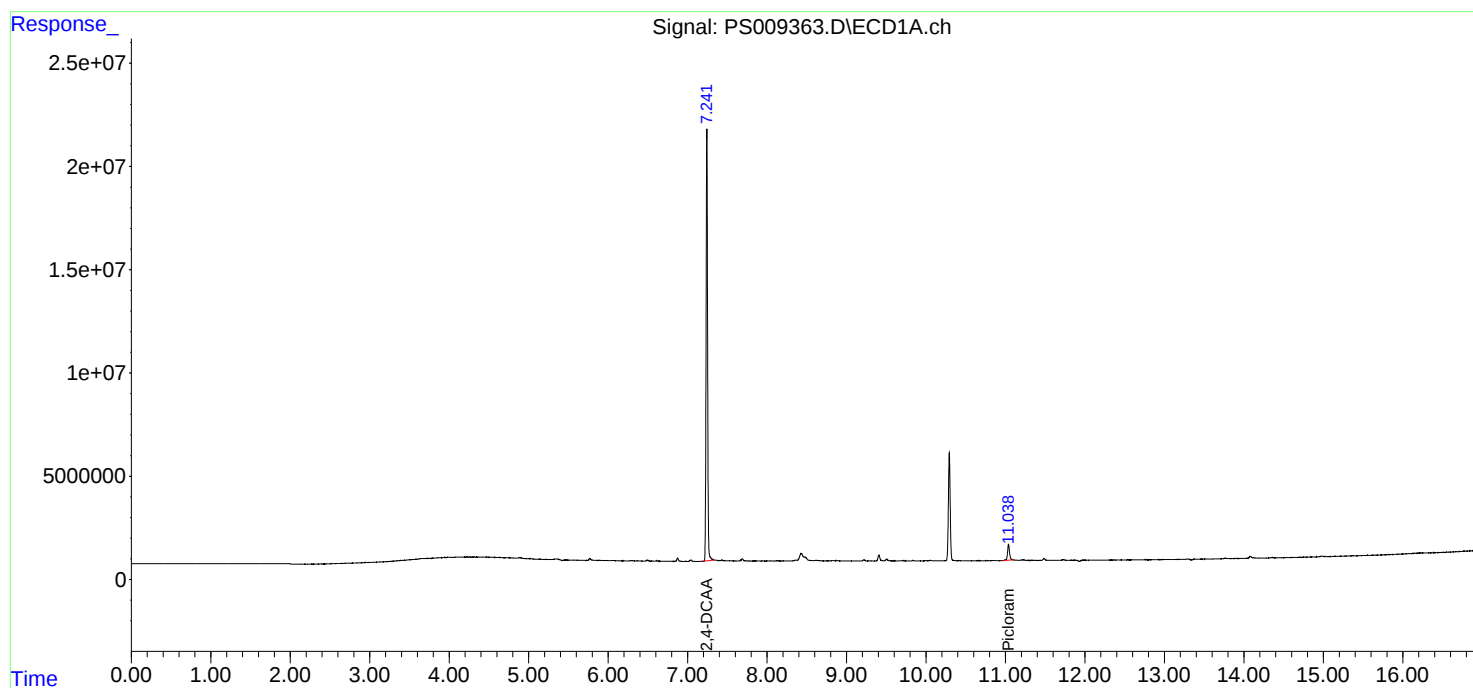


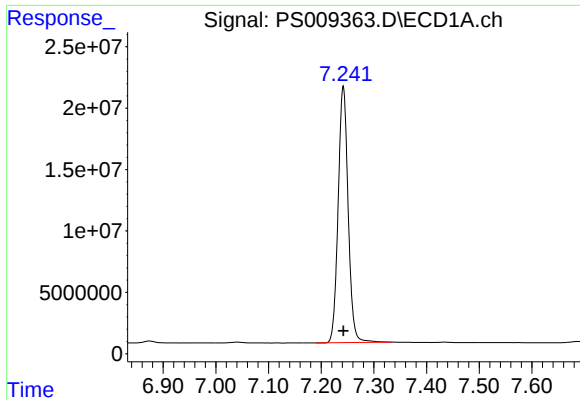

#4 2,4-DCAA


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 275107371
Conc: 497.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

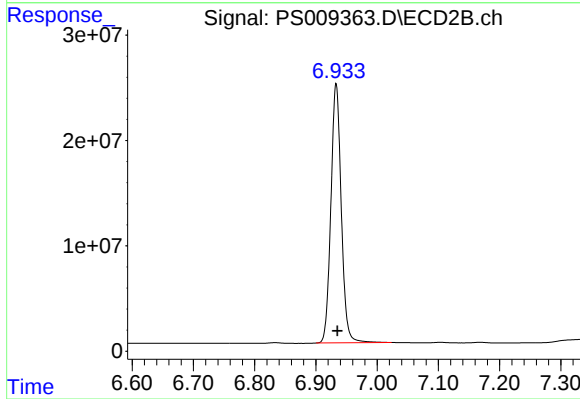


#4 2,4-DCAA

R.T.: 6.933 min
Delta R.T.: -0.002 min
Response: 289368726
Conc: 526.89 ng/ml

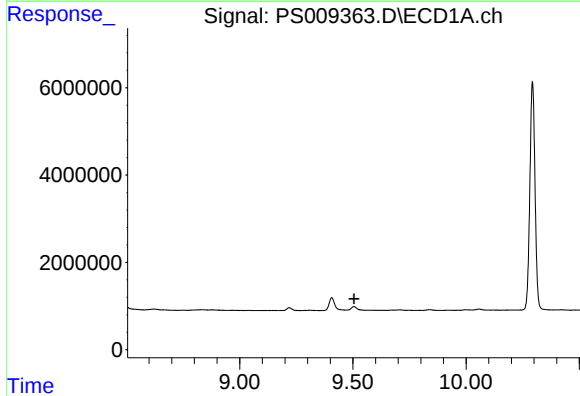


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.505 min
Response: 0
Conc: N.D.

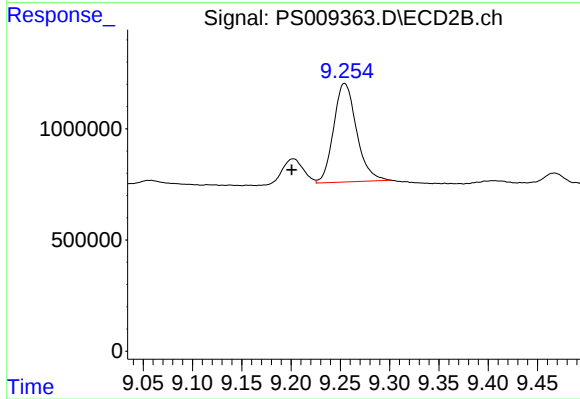

#12 2,4,5-T


R.T.: 9.254 min
Delta R.T.: 0.053 min
Response: 7176159
Conc: 2.43 ng/ml

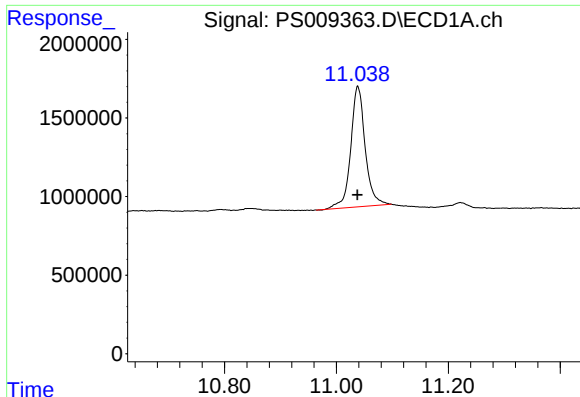

#15 Picloram


R.T.: 11.038 min
Delta R.T.: 0.000 min
Response: 13699130
Conc: 4.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

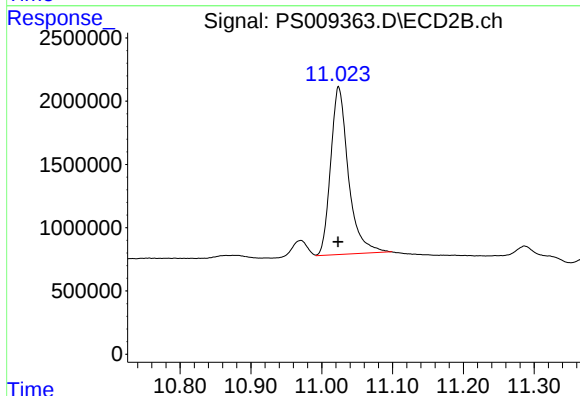


#15 Picloram

R.T.: 11.024 min
Delta R.T.: 0.000 min
Response: 23083002
Conc: 5.67 ng/ml

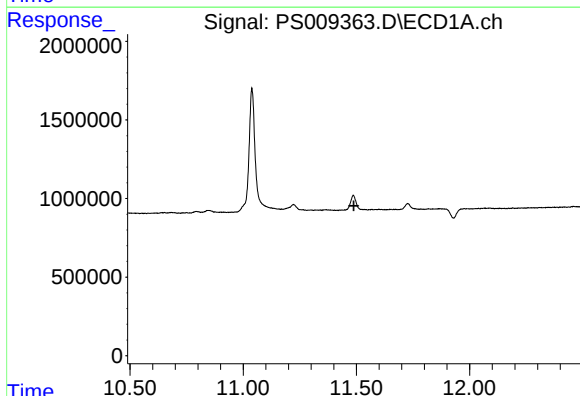

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

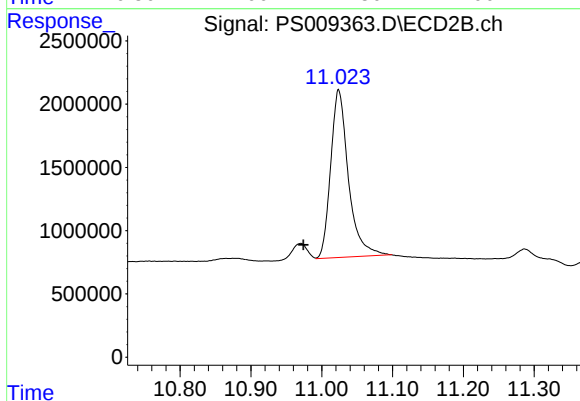

#16 DCPA

R.T.: 11.024 min
Delta R.T.: 0.050 min
Response: 23083002
Conc: 5.96 ng/ml